
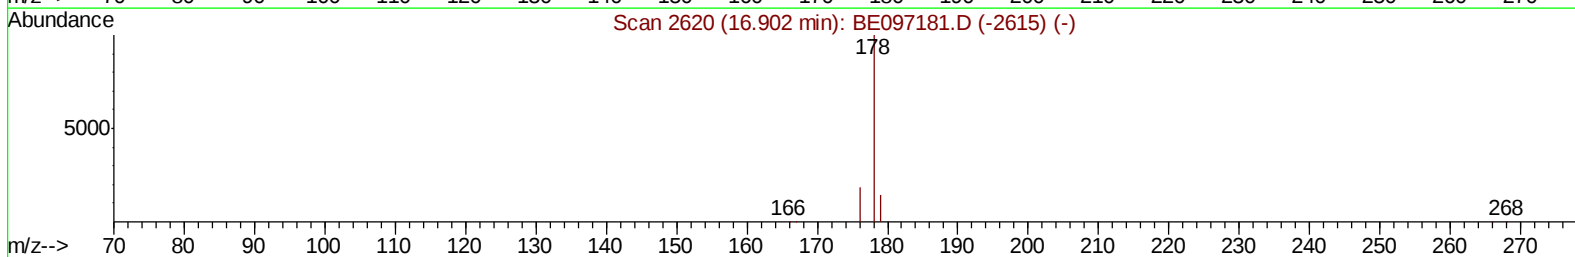
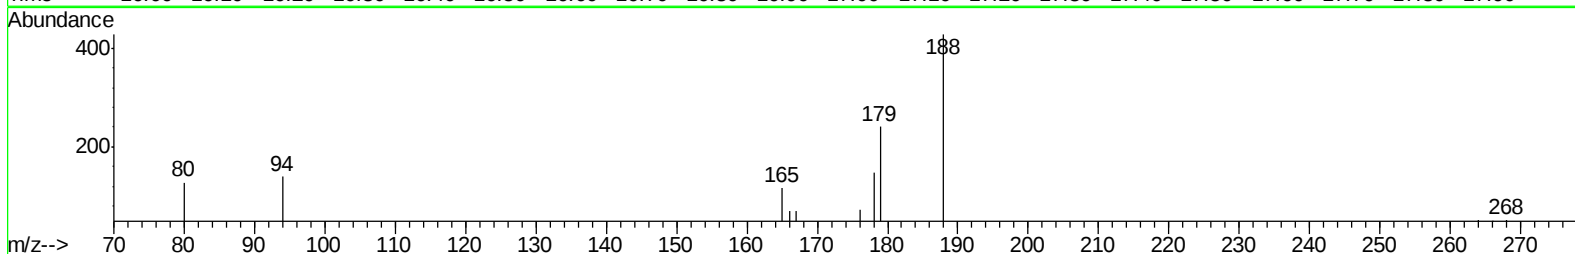


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
Data File : BE097191.D
Acq On : 3 Aug 2018 22:25
Operator : SJ/JU
Sample : J4171-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Aug 04 00:30:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 03 23:39:09 2018
Response via : Initial Calibration

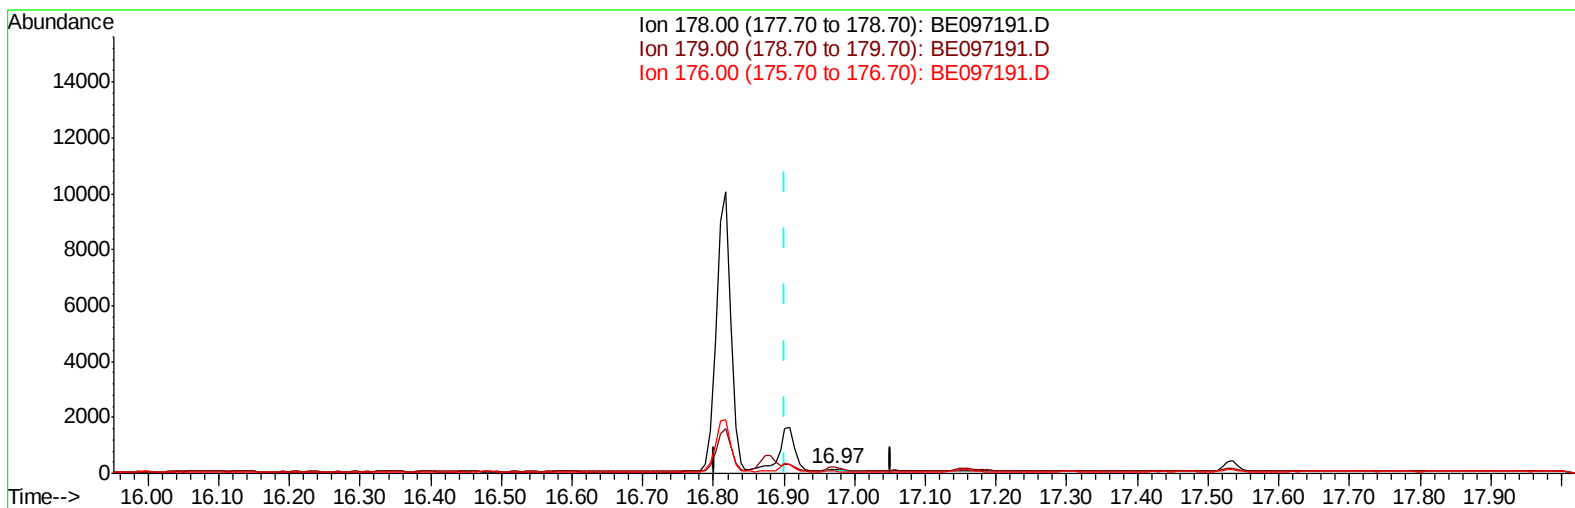

TIC: BE097191.D

(13) Anthracene

16.972min (+0.070) 0.00ng/ul

response 95

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	163.27#
176.00	18.40	49.66#
0.00	0.00	0.00