
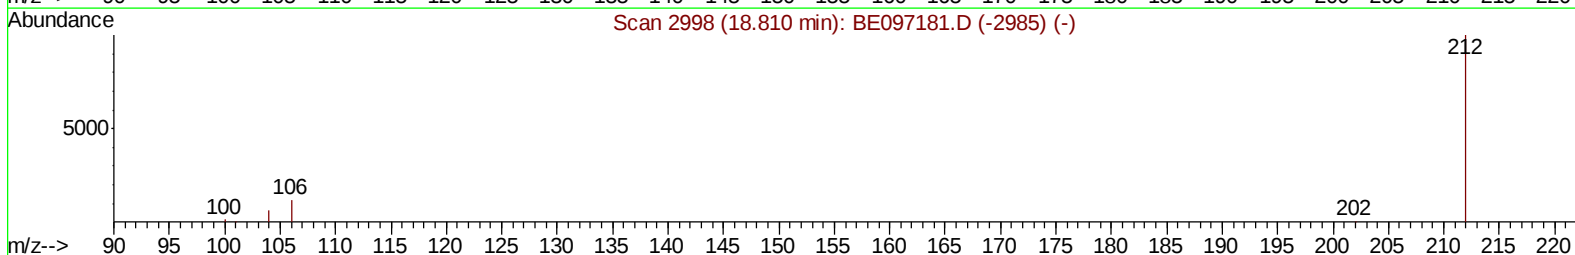
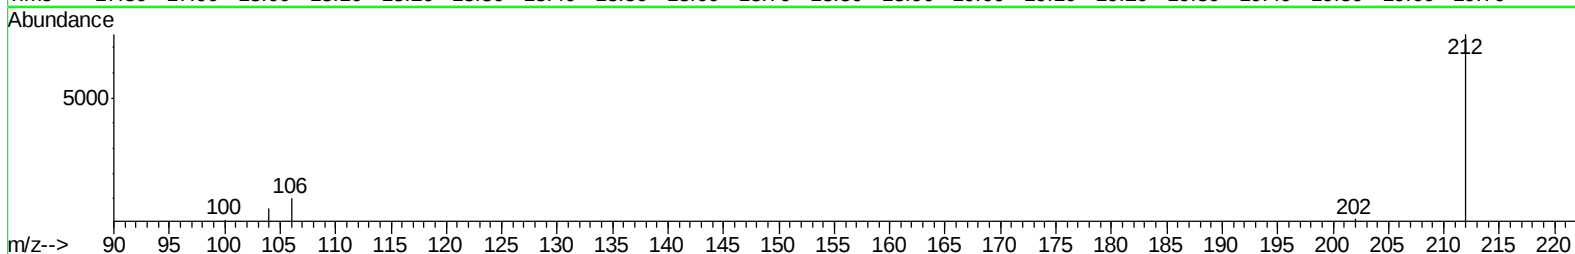


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
Data File : BE097191.D
Acq On : 3 Aug 2018 22:25
Operator : SJ/JU
Sample : J4171-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Aug 04 00:30:33 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 03 23:39:09 2018
Response via : Initial Calibration

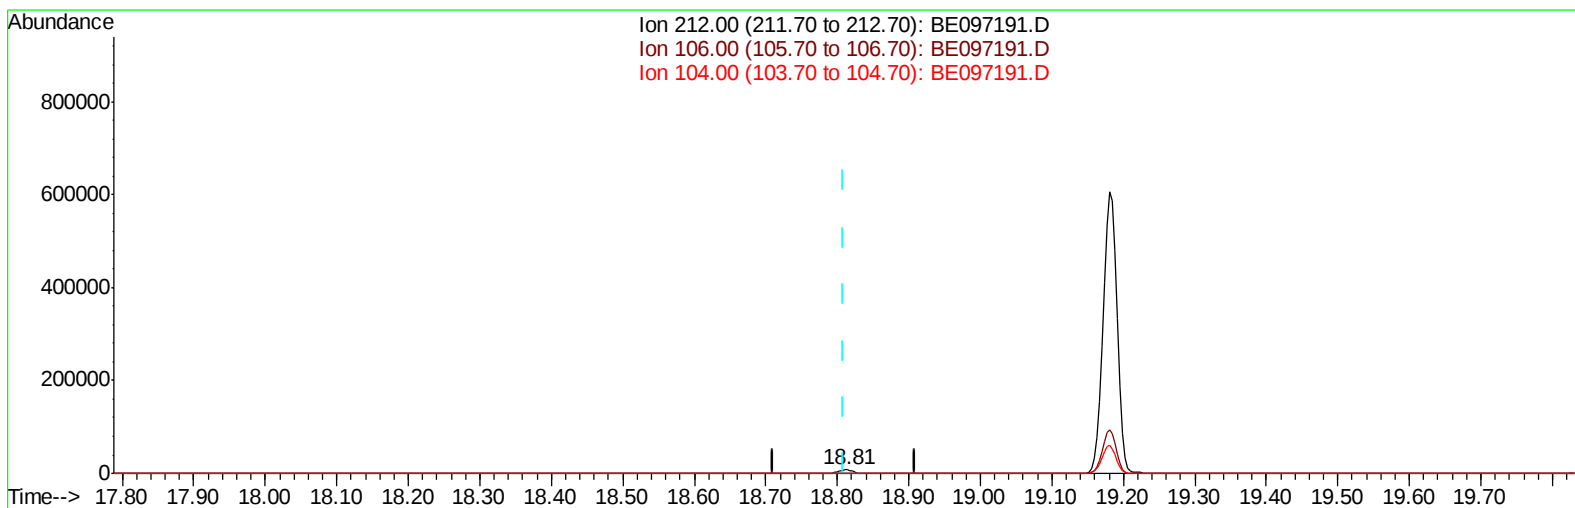

TIC: BE097191.D

(14) Fluoranthene-d10 (SURR)

18.814min (+0.004) 0.27ng/ul m

response 10128

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00