
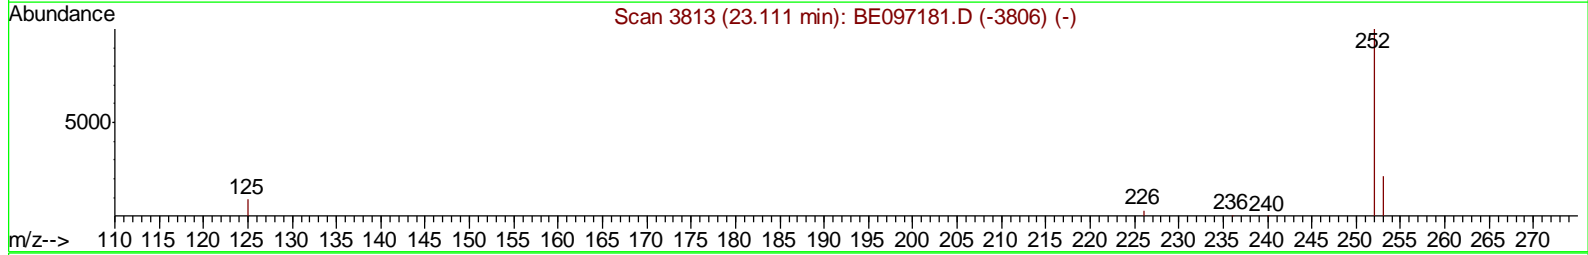
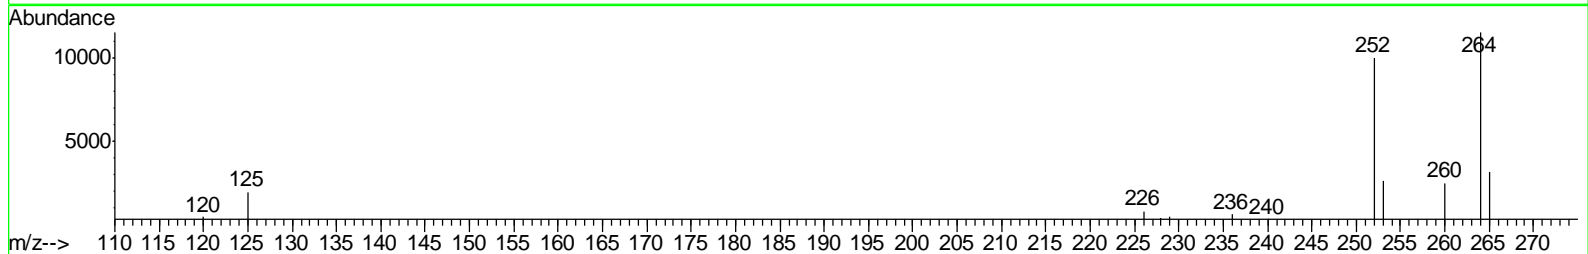


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
 Data File : BE097191.D
 Acq On : 3 Aug 2018 22:25
 Operator : SJ/JU
 Sample : J4171-01
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Quant Time: Aug 04 00:32:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 03 23:39:09 2018
 Response via : Initial Calibration

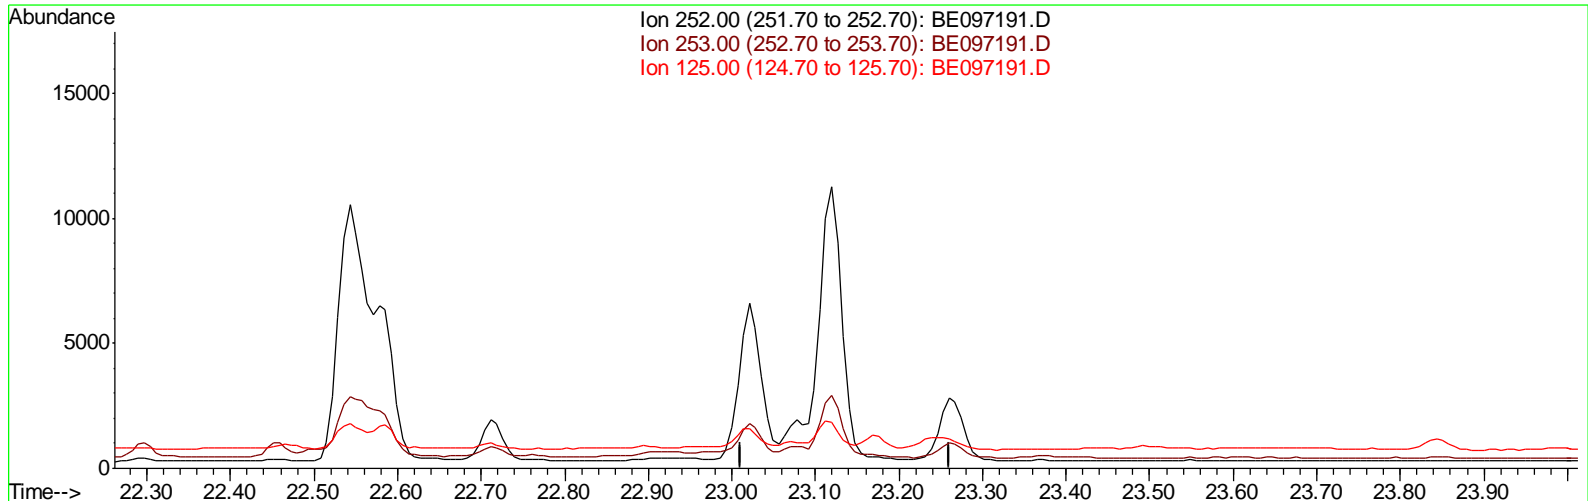

TIC: BE097191.D

(23) Benzo(a)pyrene (C)
 23.111min (-23.111) 0.00ng/ul
 response 0

Ion	Exp%	Act%
252.00	100	0.00
253.00	35.60	0.00#
125.00	22.60	0.00#
0.00	0.00	0.00