
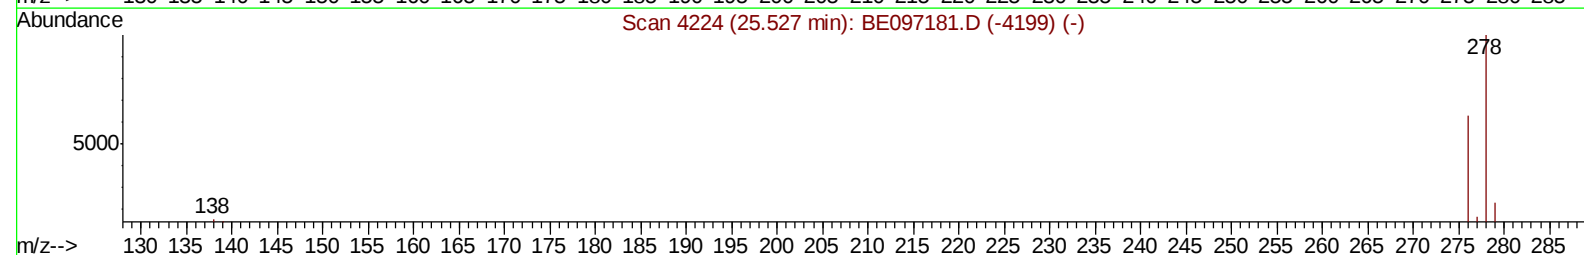
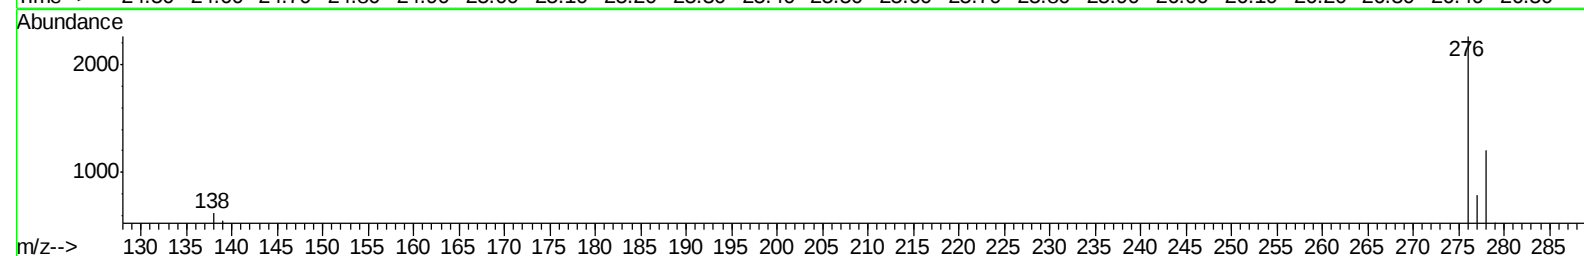


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
Data File : BE097191.D
Acq On : 3 Aug 2018 22:25
Operator : SJ/JU
Sample : J4171-01
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Aug 04 00:32:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 03 23:39:09 2018
Response via : Initial Calibration

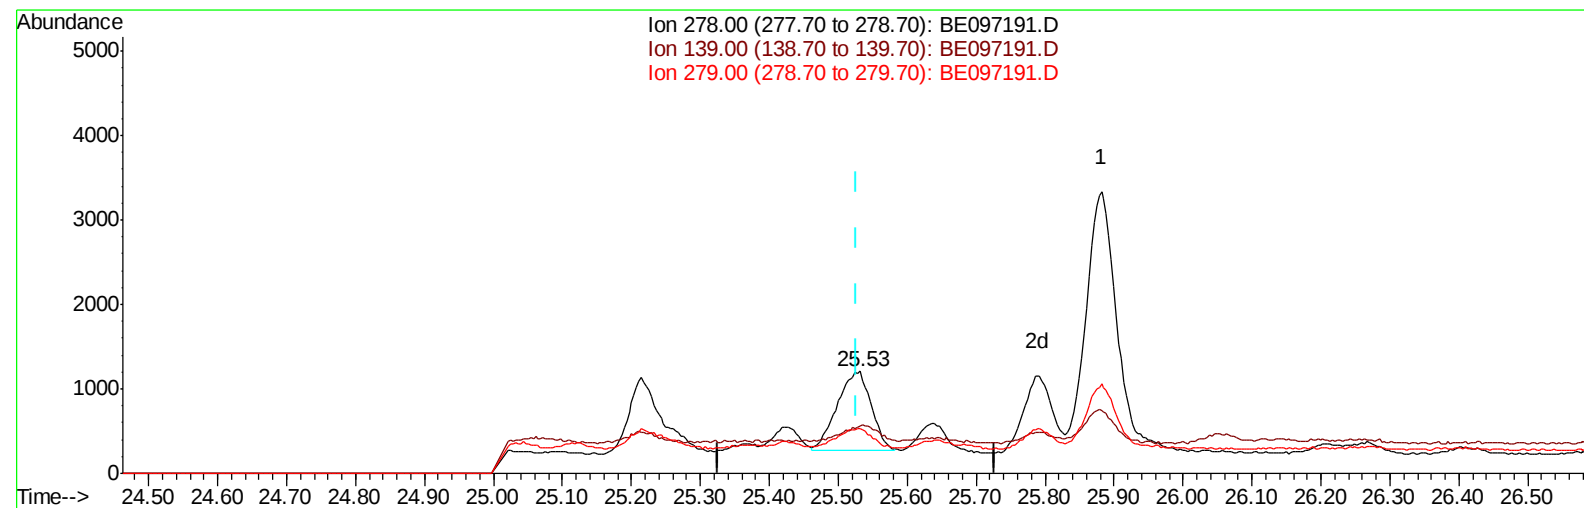

TIC: BE097191.D

(25) Dibenzo(a,h)anthracene

25.532min (+0.005) 0.10ng/ul m

response 3180

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	46.19#
279.00	32.40	44.11#
0.00	0.00	0.00