

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
 Data File : BE097189.D
 Acq On : 3 Aug 2018 21:08
 Operator : SJ/JU
 Sample : J4171-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 03 23:40:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 03 23:39:09 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1530	0.40	ng/ul	0.00
2) Naphthalene-d8	10.14	136	7991	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	5237	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	1061817	0.40	ng/ul	0.10
16) Chrysene-d12	21.08	240	126	0.40	ng/ul	0.10
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-23.21
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	5870	0.46	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds				Ovalue		
17) Pyrene	19.21	202	3221	9.540	ng/ul	92
18) Benzo(a)anthracene	21.08	228	132	0.367	ng/ul#	1
19) Chrysene	21.13	228	196	0.528	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080318\
Data File : BE097189.D
Acq On : 3 Aug 2018 21:08
Operator : SJ/JU
Sample : J4171-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 03 23:40:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 03 23:39:09 2018
Response via : Initial Calibration

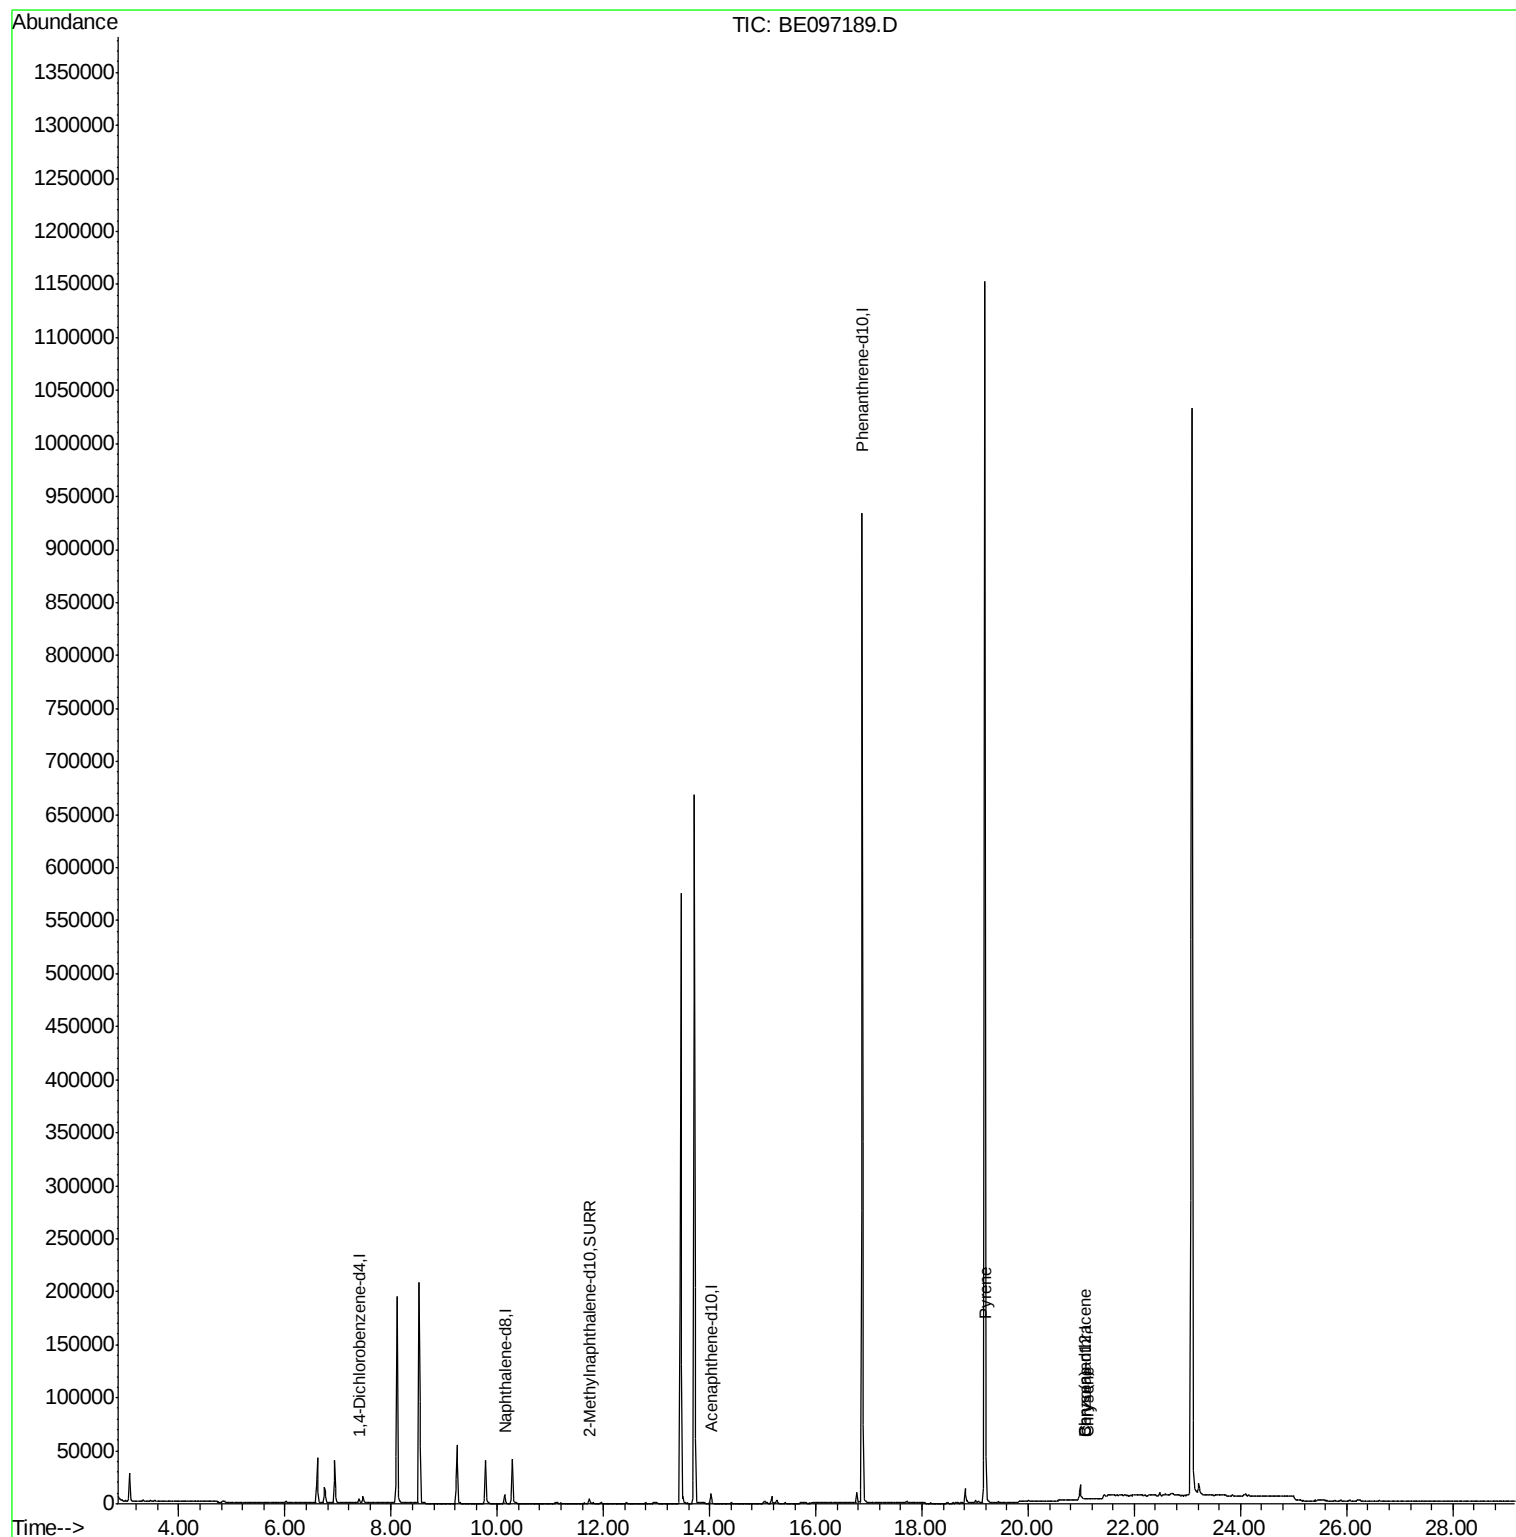


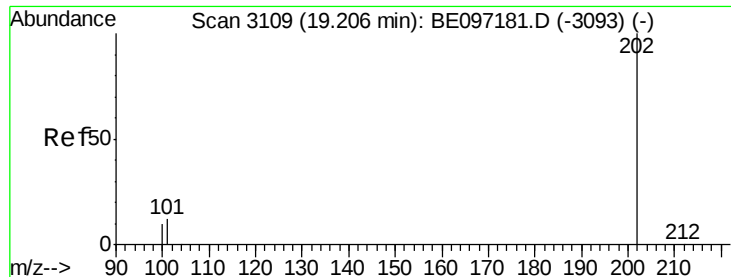




#17
Pvrene
Concen: 9.540 ng/ul
RT: 19.21 min Scan# 3111
Delta R.T. 0.00 min
Lab File: BE097189.D
Acq: 3 Aug 2018 21:08

Instrument :
BNA_E
ClientSampleId :

Tot Ion:202 Resp: 3221
Ion Ratio Lower Upper
202 100
101 18.7 18.2 27.4
100 16.4 15.6 23.4

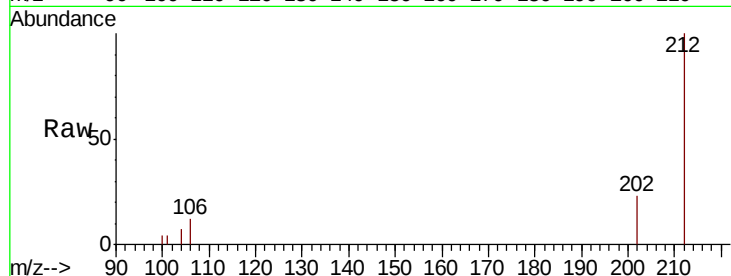


Abundance Ion 202.00 (201.70 to 202.70): E
Ion 101.00 (100.70 to 101.70): E
Ion 100.00 (99.70 to 100.70): E

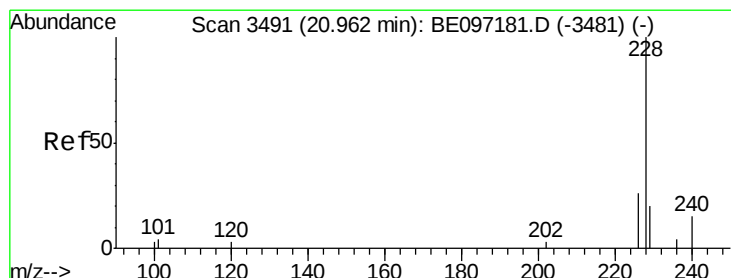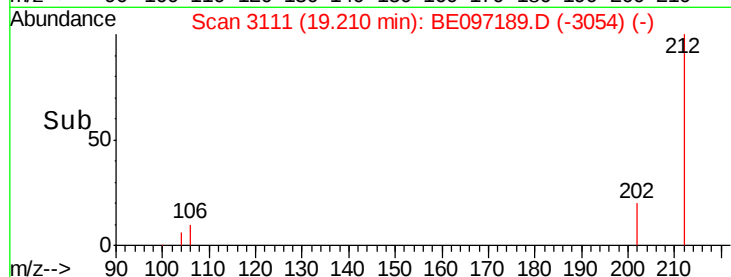
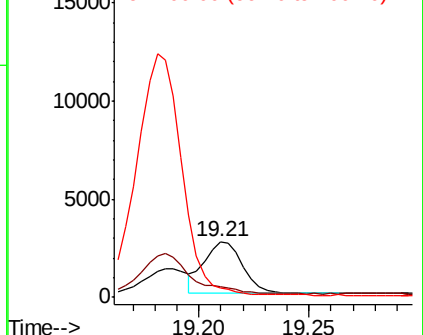



#18
Benzo(a)anthracene
Concen: 0.367 ng/ul
RT: 21.08 min Scan# 3515
Delta R.T. 0.12 min
Lab File: BE097189.D
Acq: 3 Aug 2018 21:08

Tgt Ion:228 Resp: 132
Ion Ratio Lower Upper
228 100
229 155.3 22.8 34.2#
226 107.8 17.0 25.6#

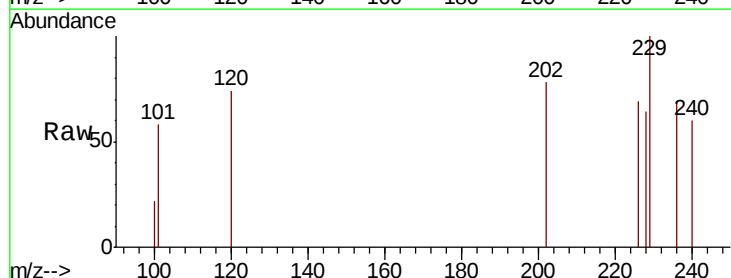

Abundance Ion 228.00 (227.70 to 228.70): E
Ion 229.00 (228.70 to 229.70): E
Ion 226.00 (225.70 to 226.70): E

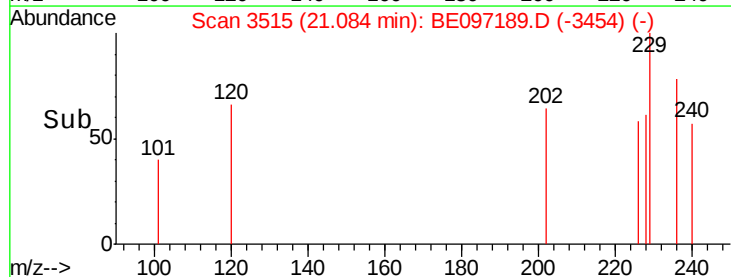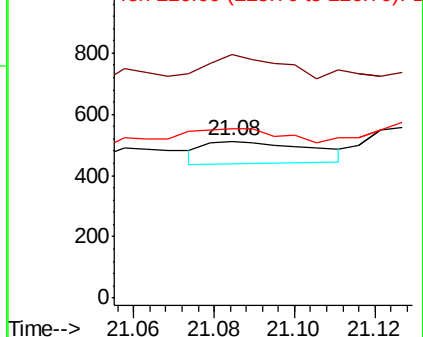

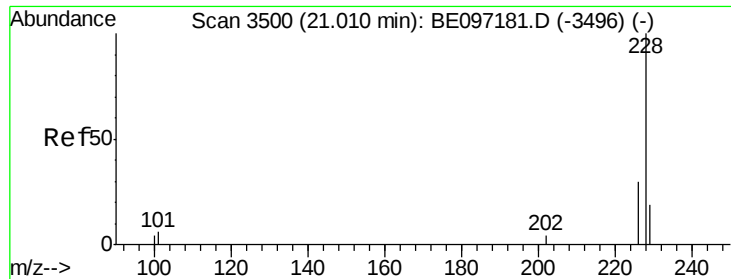

#19

Chrysene

Concen: 0.528 ng/ul

RT: 21.13 min Scan# 3524

Delta R.T. 0.12 min


Lab File: BE097189.D

Acq: 3 Aug 2018 21:08

Instrument :

BNA_E

ClientSampleId :

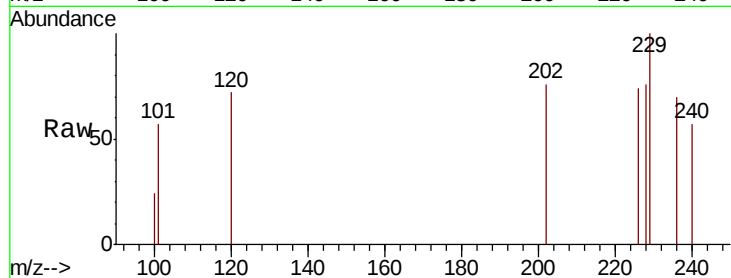

Tot Ion: 228 Resp: 196

Ion Ratio Lower Upper

228 100

226 98.1 23.4 35.0#

229 131.9 17.7 26.5#

