
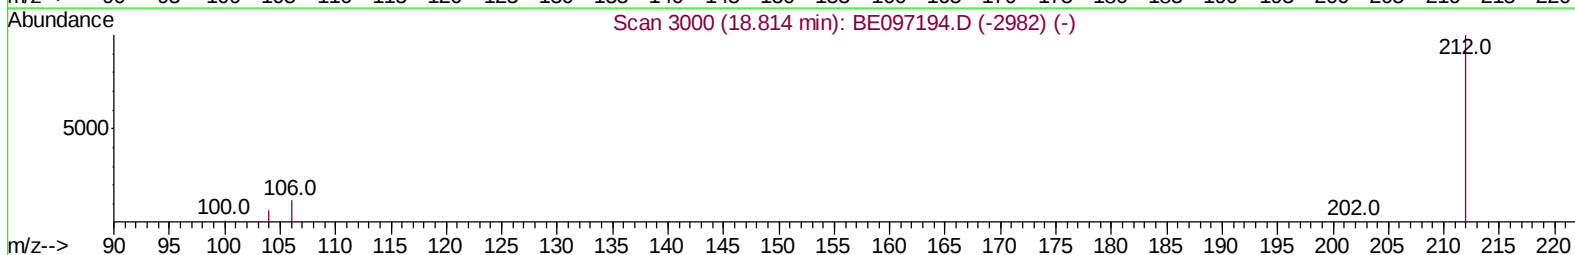
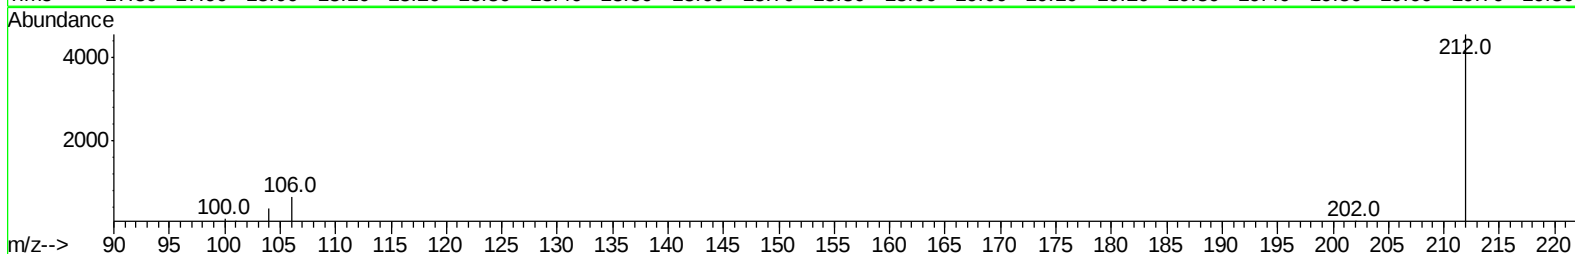


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097195.D
 Acq On : 4 Aug 2018 11:08
 Operator : SJ/JU
 Sample : PB111661BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Quant Time: Aug 06 01:00:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 00:53:27 2018
 Response via : Initial Calibration

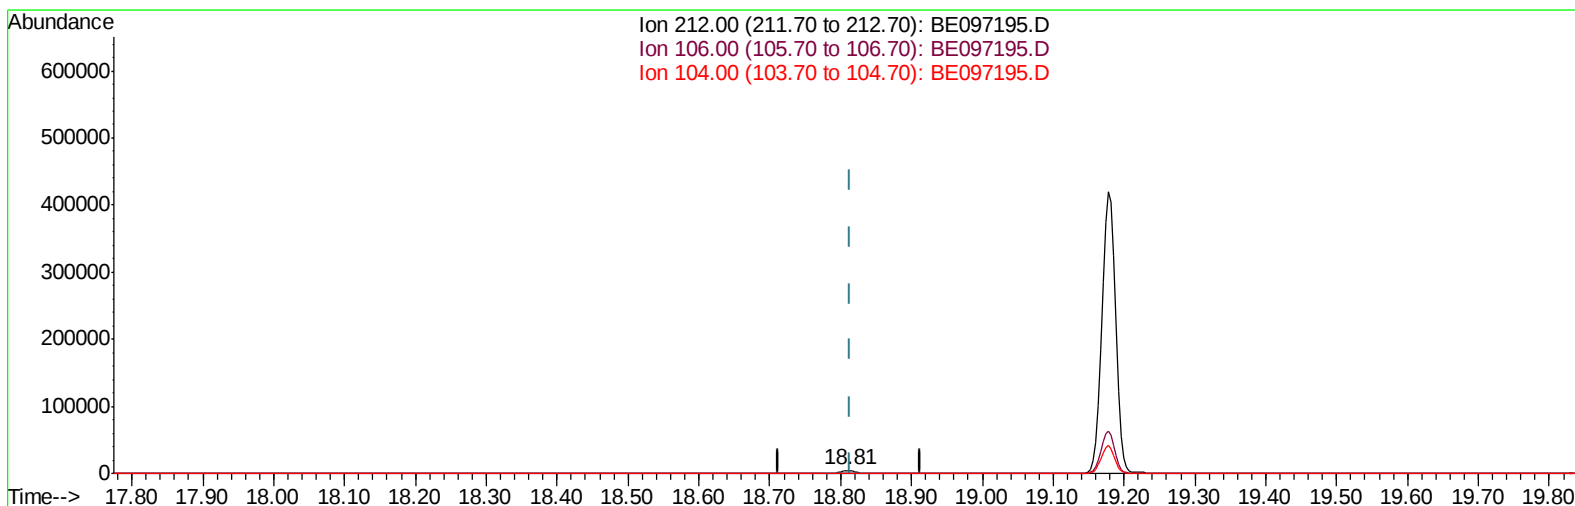

TIC: BE097195.D

(14) Fluoranthene-d10 (SURR)

18.810min (-0.003) 0.18ng/ul m

response 6203

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00