
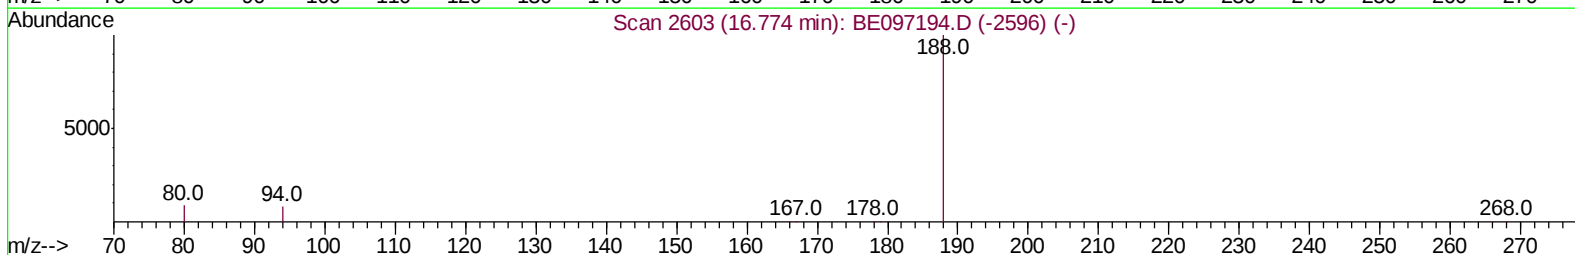
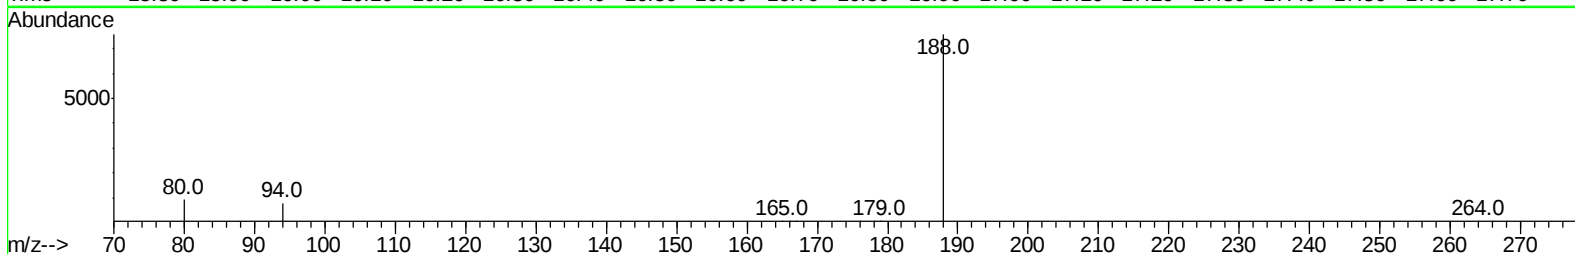


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097200.D
 Acq On : 4 Aug 2018 14:14
 Operator : SJ/JU
 Sample : J4265-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Quant Time: Aug 06 00:55:41 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 00:53:27 2018
 Response via : Initial Calibration

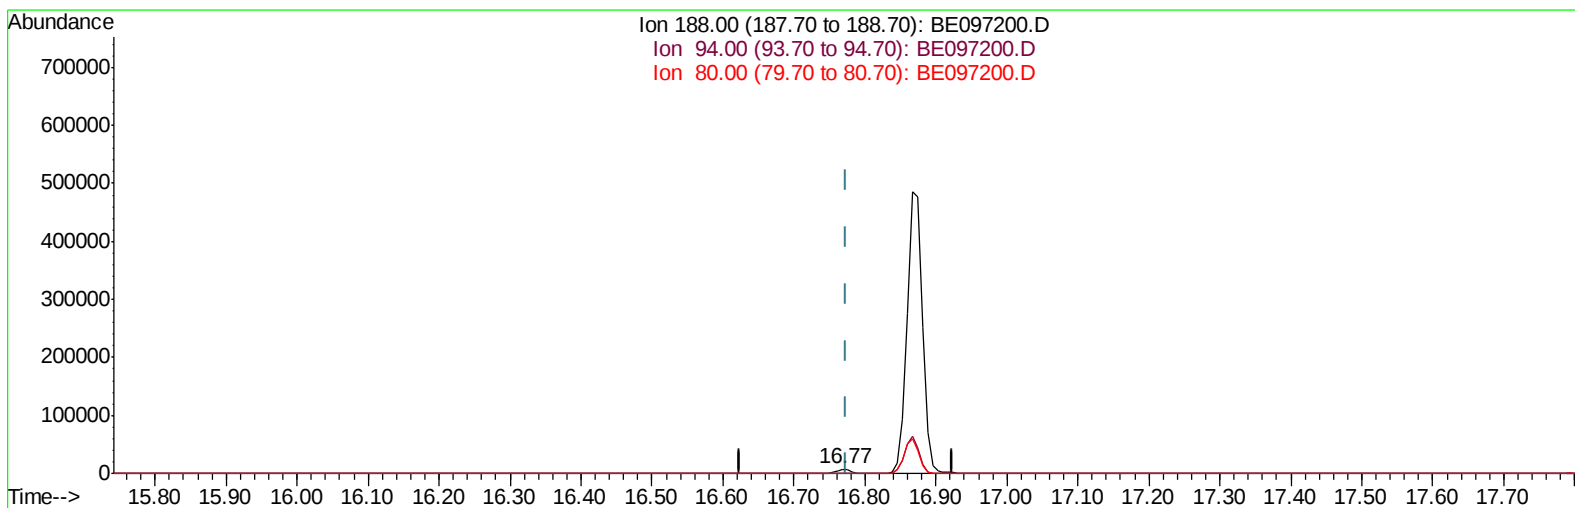

TIC: BE097200.D

(10) Phenanthrene-d10 (I)

16.769min (-0.006) 0.40ng/ul m

response 10650

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.45
80.00	11.80	11.90
0.00	0.00	0.00