
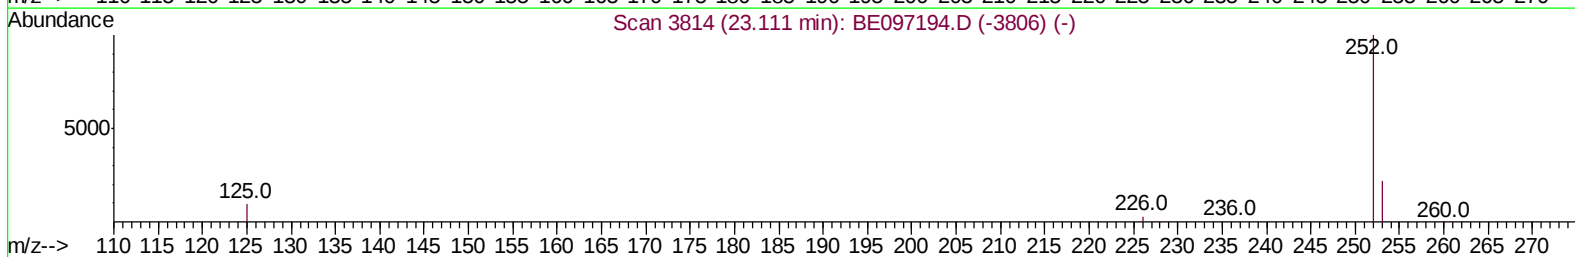
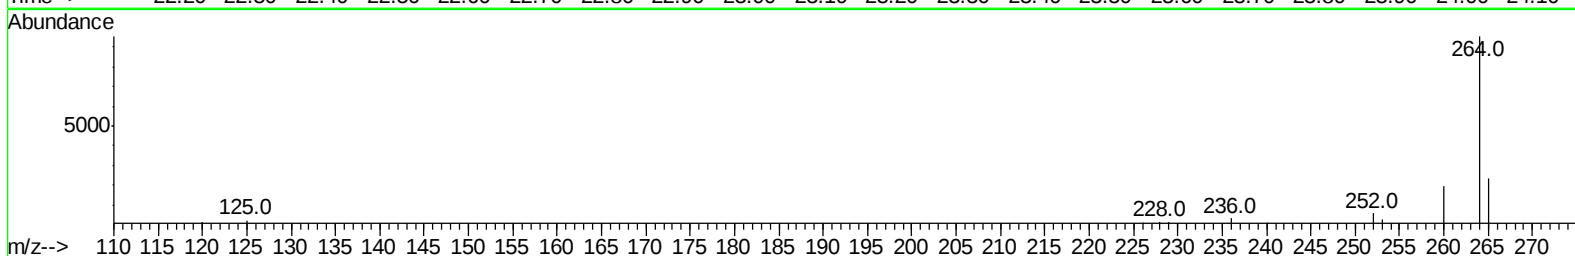


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097200.D
Acq On : 4 Aug 2018 14:14
Operator : SJ/JU
Sample : J4265-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Quant Time: Aug 06 01:30:17 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 00:53:27 2018
Response via : Initial Calibration

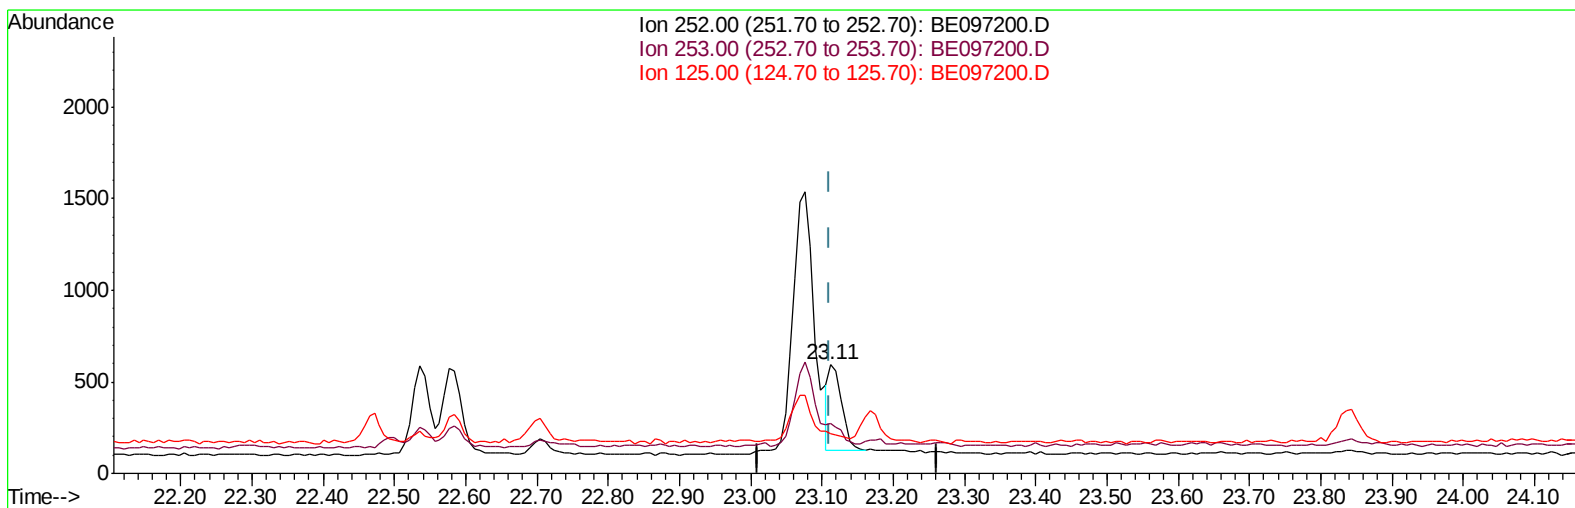

TIC: BE097200.D

(23) Benzo(a)pyrene (C)

23.112min (+0.000) 0.02ng/ul m

response 603

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	46.11#
125.00	22.60	36.99#
0.00	0.00	0.00