
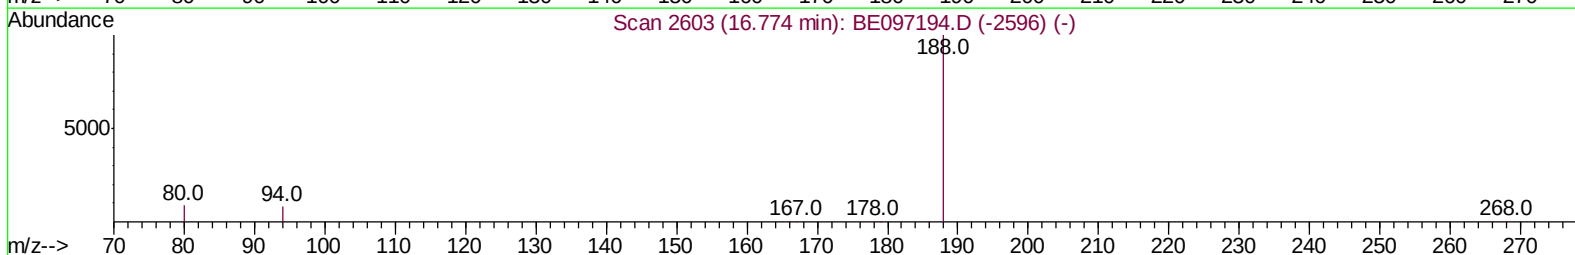
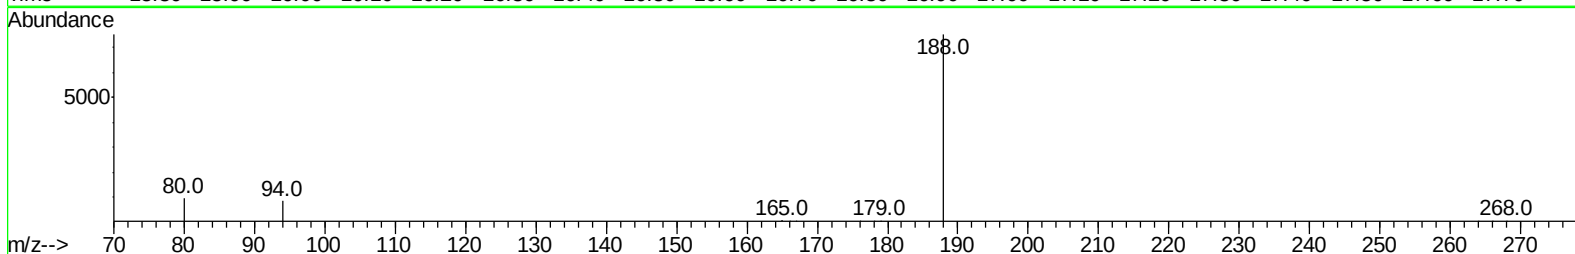


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097201.D
Acq On : 4 Aug 2018 14:50
Operator : SJ/JU
Sample : J4265-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Quant Time: Aug 06 00:55:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 00:53:27 2018
Response via : Initial Calibration

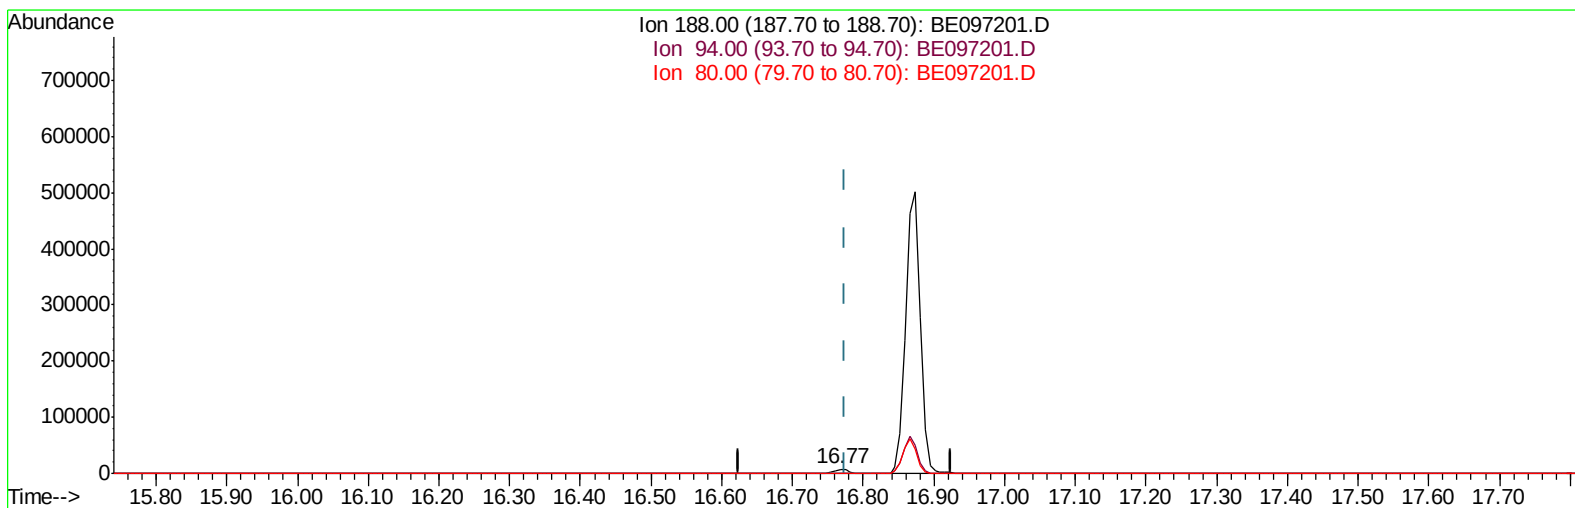

TIC: BE097201.D

(10) Phenanthrene-d10 (I)

16.768min (-0.006) 0.40ng/ul m

response 10661

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.47
80.00	11.80	12.63
0.00	0.00	0.00