
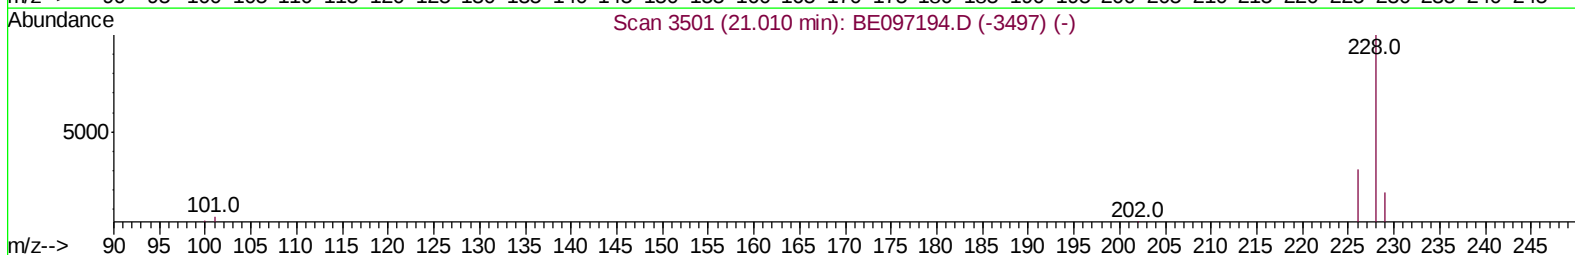
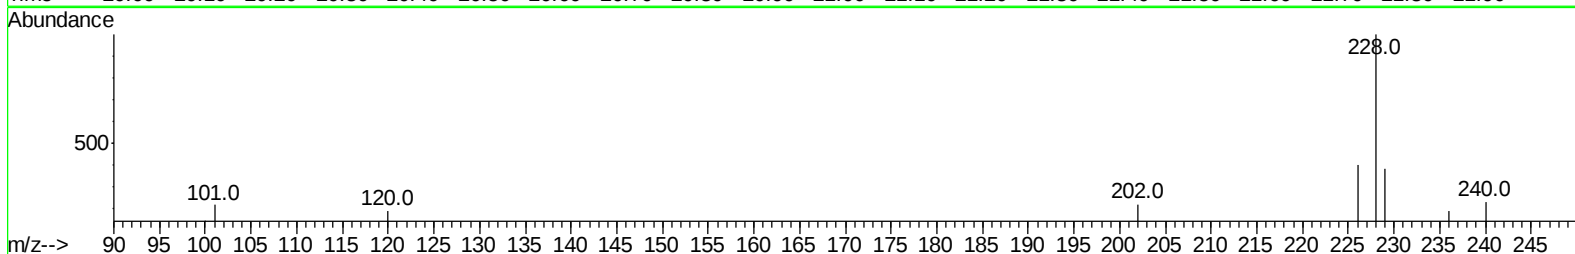


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\  
Data File : BE097204.D  
Acq On : 4 Aug 2018 16:44  
Operator : SJ/JU  
Sample : J4206-01  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Aug 06 01:57:24 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 06 00:53:27 2018  
Response via : Initial Calibration

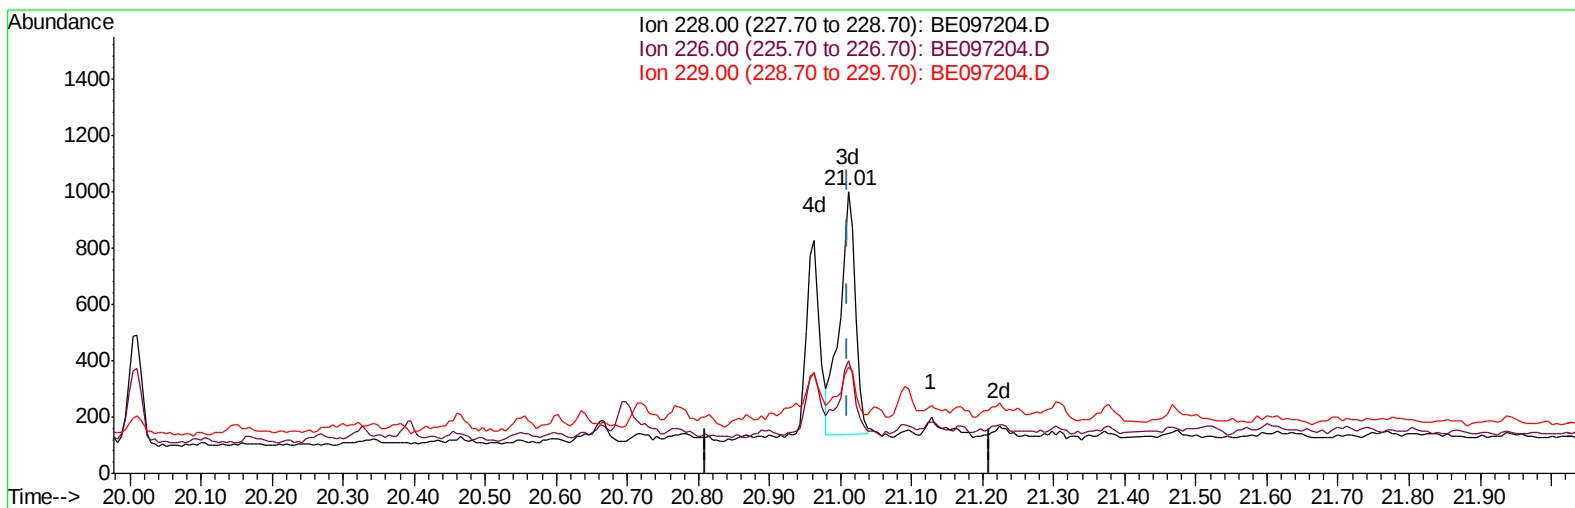

TIC: BE097204.D

(19) Chrysene

21.011min (+0.001) 0.04ng/ul m

response 1293

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 228.00 | 100   | 100    |
| 226.00 | 29.20 | 39.94# |
| 229.00 | 22.10 | 37.94# |
| 0.00   | 0.00  | 0.00   |