
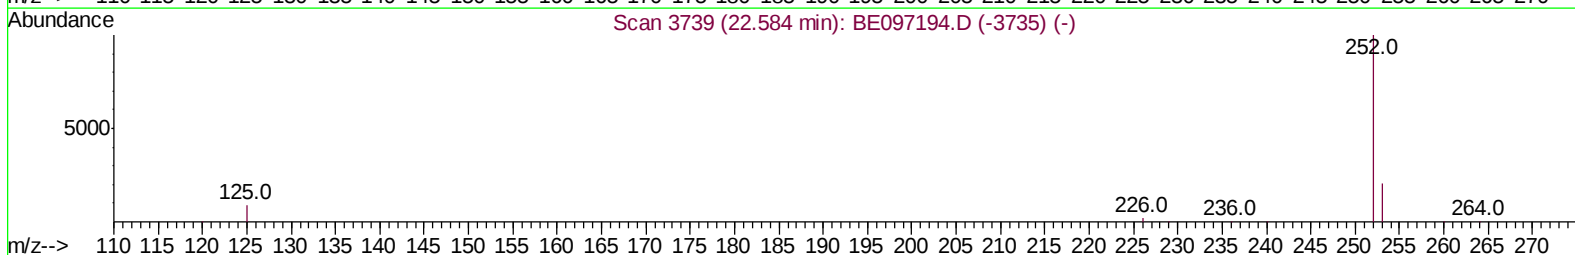
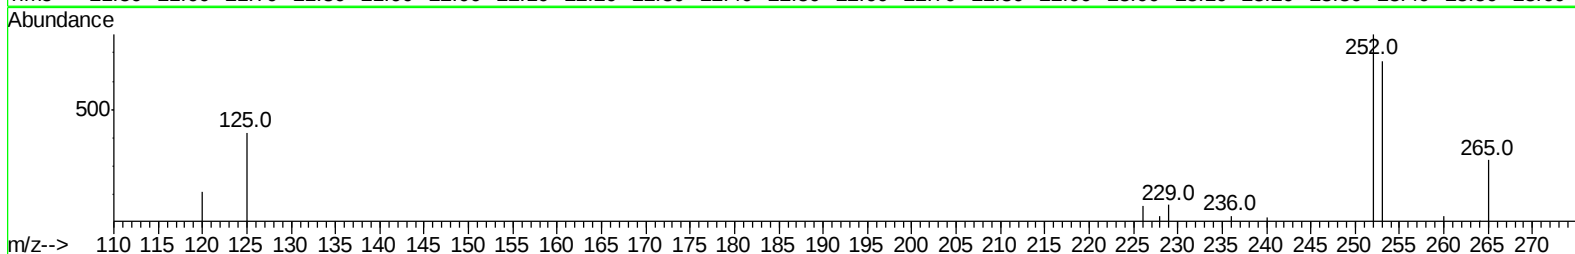


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\  
Data File : BE097204.D  
Acq On : 4 Aug 2018 16:44  
Operator : SJ/JU  
Sample : J4206-01  
Misc :  
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Aug 06 01:59:07 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 06 00:53:27 2018  
Response via : Initial Calibration

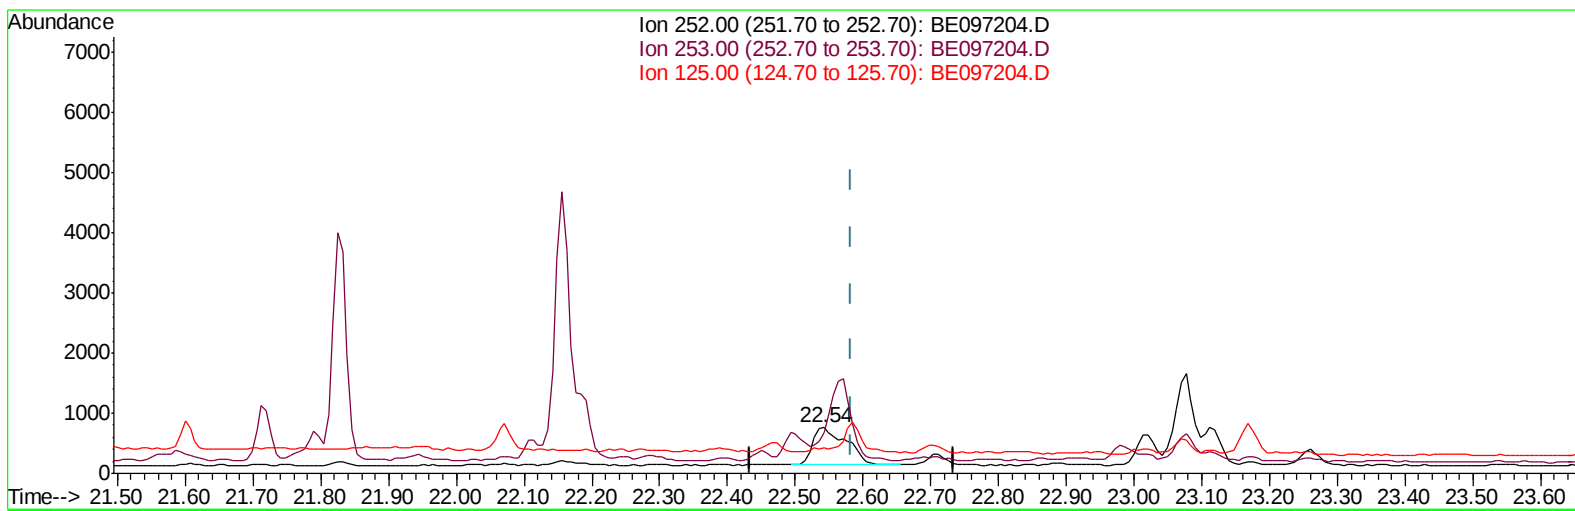

TIC: BE097204.D

(22) Benzo(k)fluoranthene

22.542min (-0.042) 0.08ng/ul

response 2139

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 252.00 | 100   | 100    |
| 253.00 | 30.60 | 87.84# |
| 125.00 | 17.10 | 54.77# |
| 0.00   | 0.00  | 0.00   |