
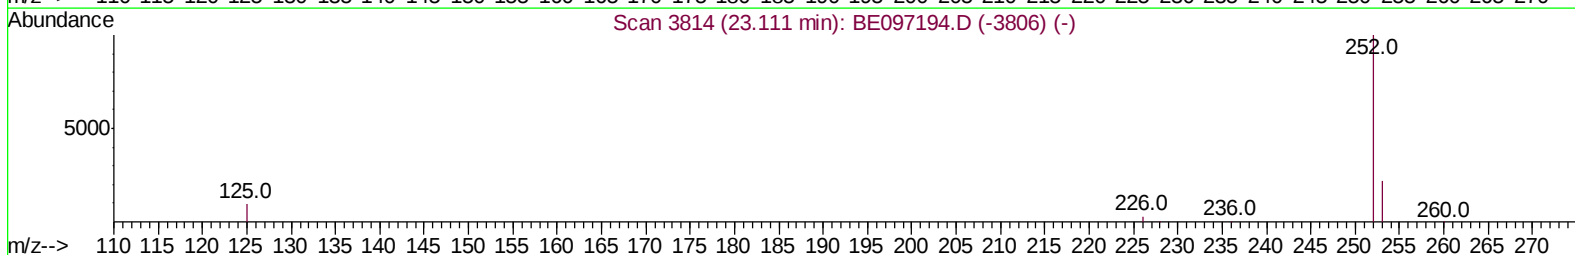
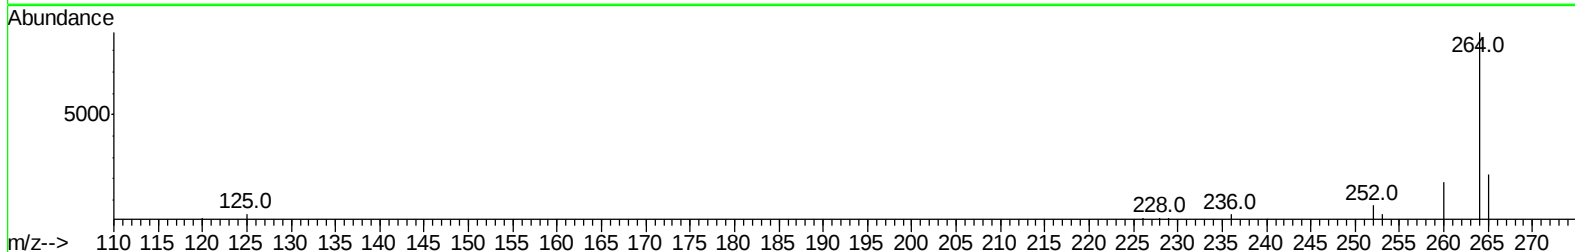


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097204.D
Acq On : 4 Aug 2018 16:44
Operator : SJ/JU
Sample : J4206-01
Misc :
ALS Vial : 12 Sample Multiplier: 1

Quant Time: Aug 06 01:59:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 00:53:27 2018
Response via : Initial Calibration

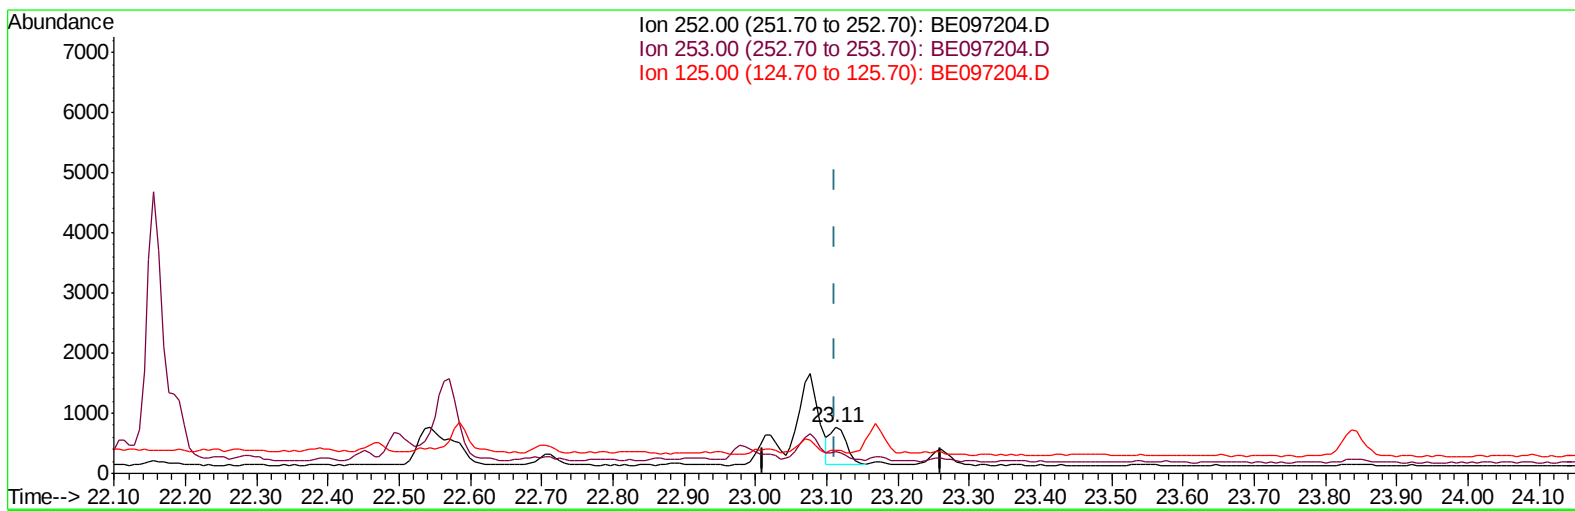

TIC: BE097204.D

(23) Benzo(a)pyrene (C)

23.112min (+0.001) 0.04ng/ul m

response 989

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	46.92#
125.00	22.60	49.28#
0.00	0.00	0.00