
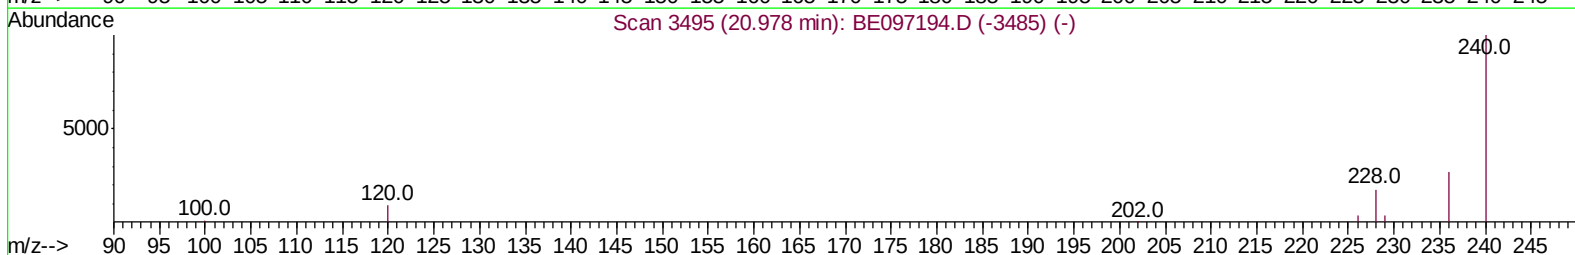
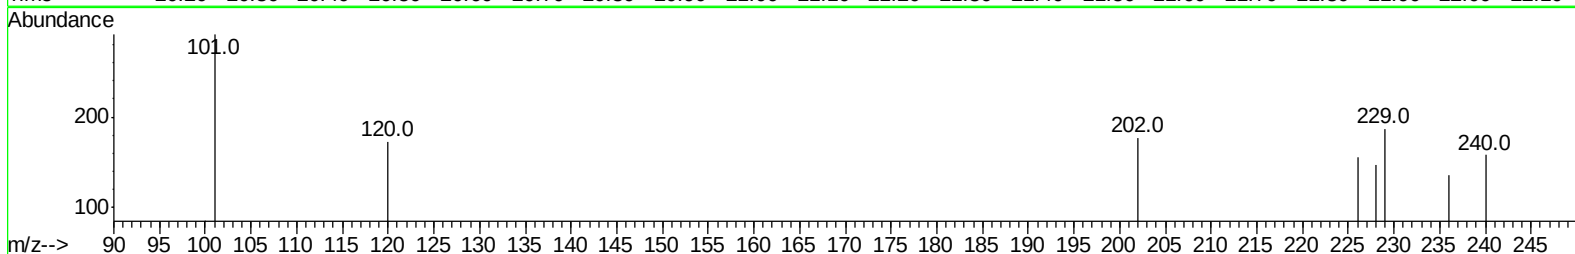


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\  
Data File : BE097205.D  
Acq On : 4 Aug 2018 17:22  
Operator : SJ/JU  
Sample : J4206-03  
Misc :  
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Aug 06 02:02:22 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 06 00:53:27 2018  
Response via : Initial Calibration

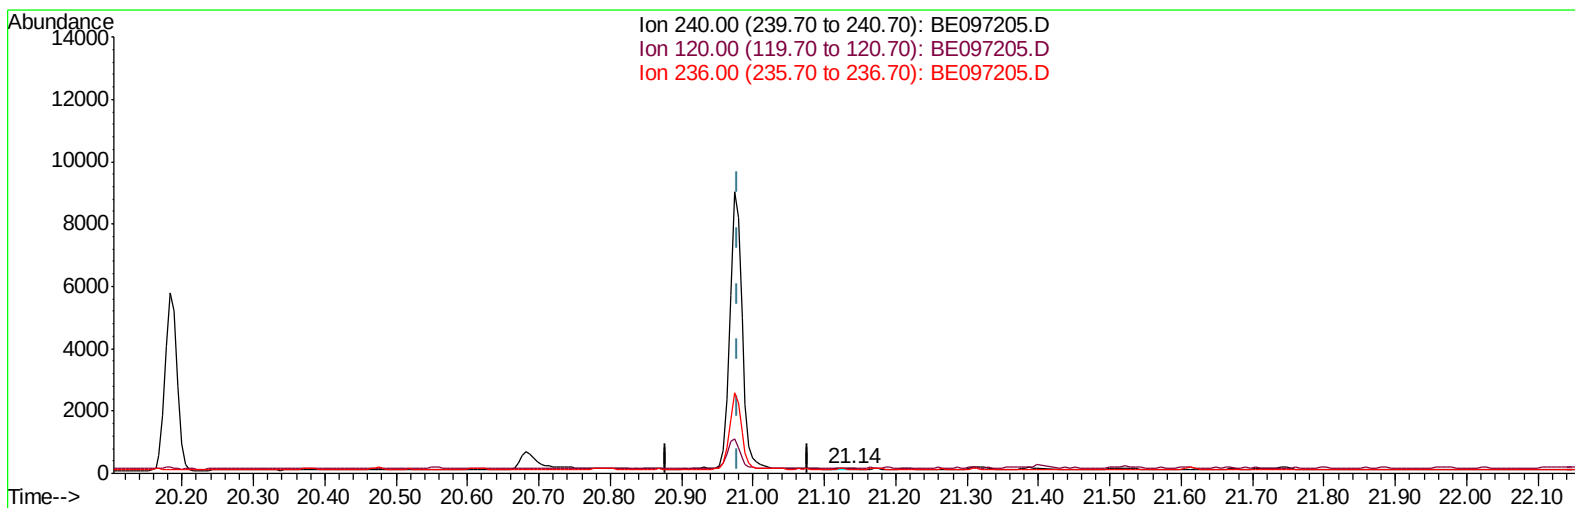

TIC: BE097205.D

(16) Chrysene-d12 (I)

21.138min (+0.160) 0.40ng/ul

response 43

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 240.00 | 100   | 100     |
| 120.00 | 20.60 | 109.49# |
| 236.00 | 34.90 | 86.08#  |
| 0.00   | 0.00  | 0.00    |