
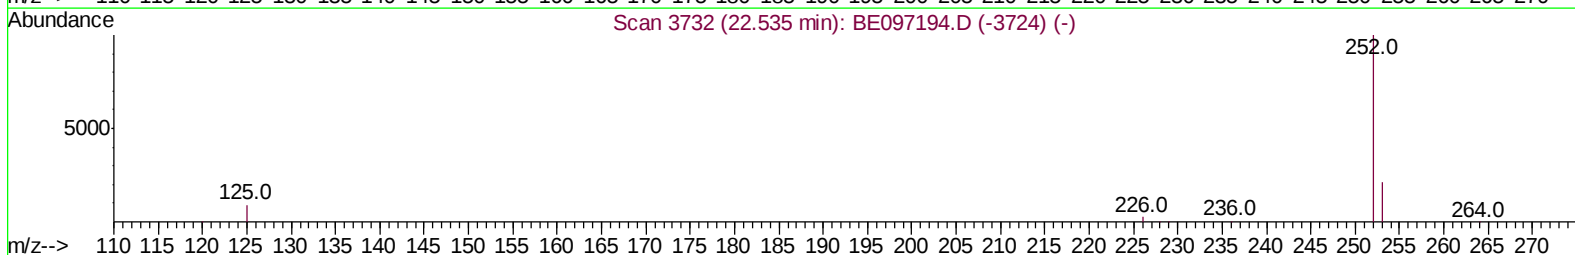
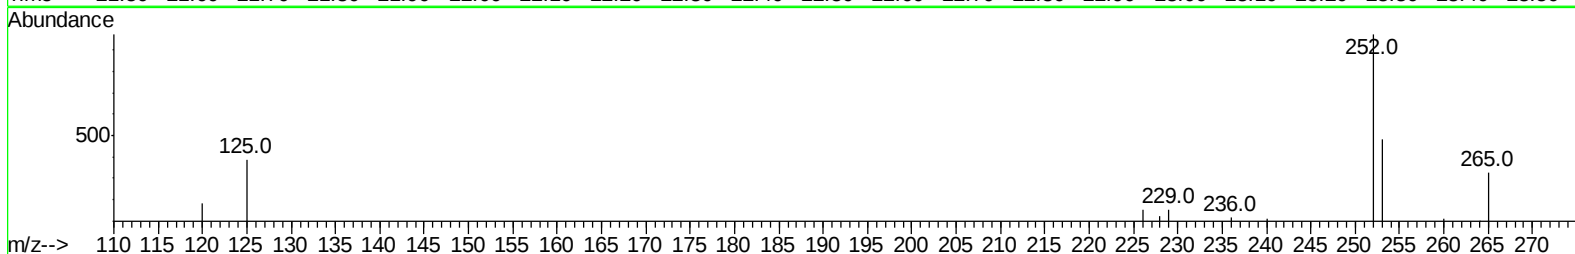


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097205.D
Acq On : 4 Aug 2018 17:22
Operator : SJ/JU
Sample : J4206-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Quant Time: Aug 06 02:06:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 00:53:27 2018
Response via : Initial Calibration

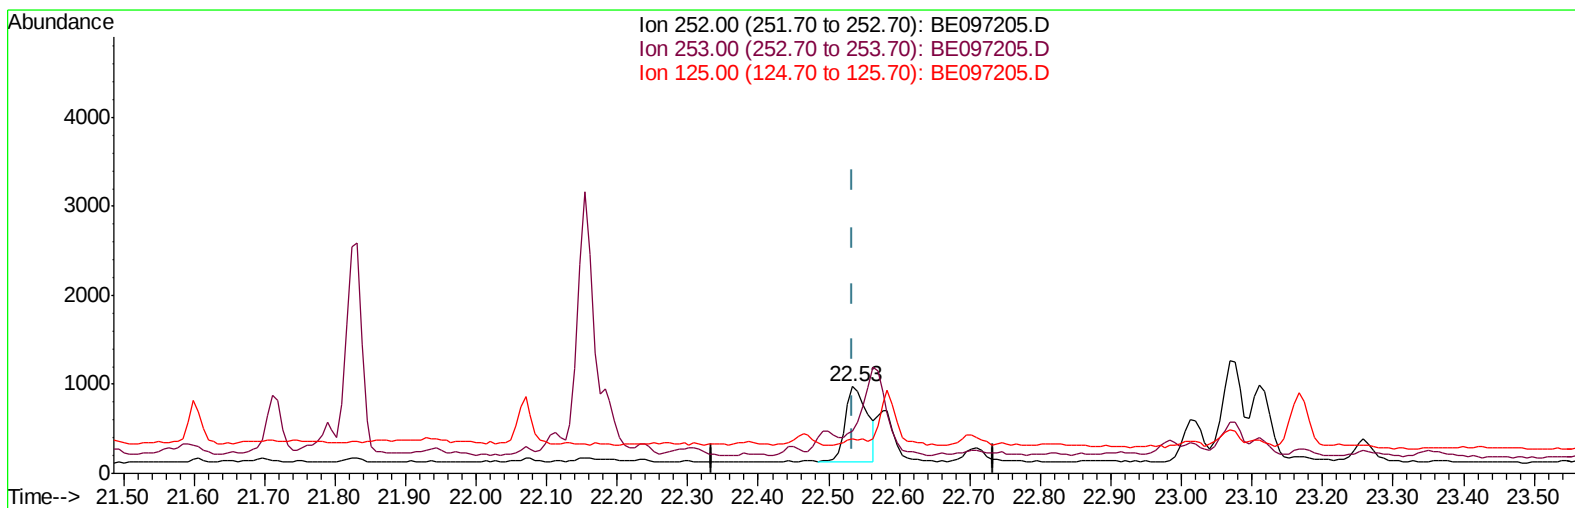

TIC: BE097205.D

(21) Benzo(b)fluoranthene

22.534min (-0.001) 0.07ng/ul m

response 1835

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	49.38
125.00	17.50	39.63#
0.00	0.00	0.00