
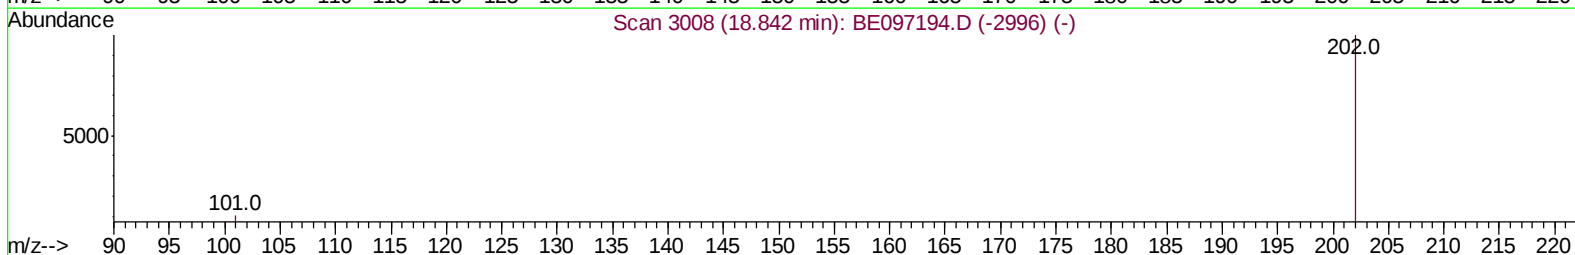
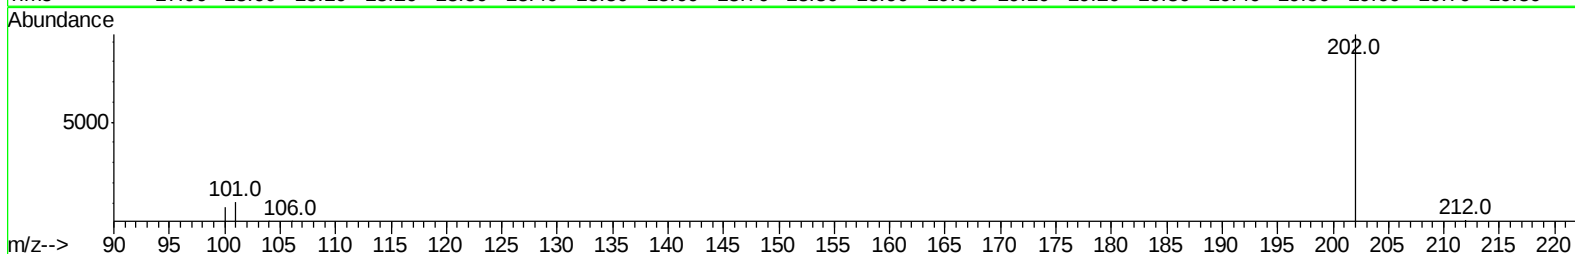


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097206.D
Acq On : 4 Aug 2018 17:58
Operator : SJ/JU
Sample : J4206-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Aug 06 02:09:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 00:53:27 2018
Response via : Initial Calibration

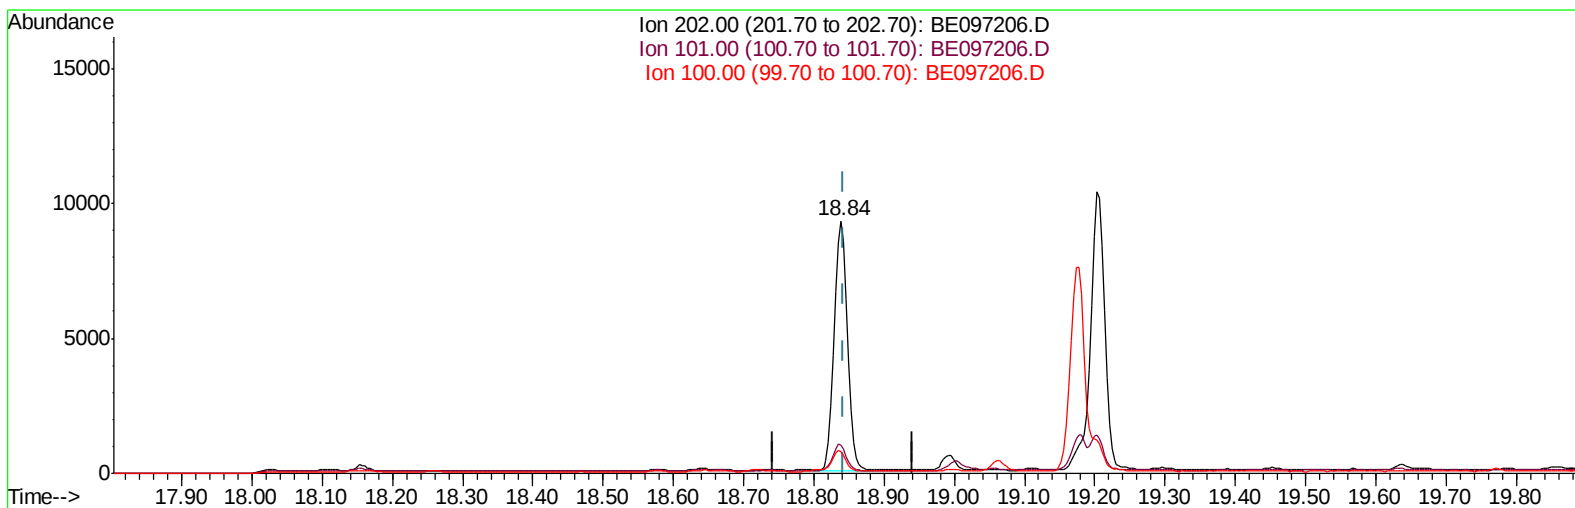

TIC: BE097206.D

(15) Fluoranthene (C)

18.839min (-0.003) 0.33ng/ul m

response 11933

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	11.40
100.00	19.50	8.78
0.00	0.00	0.00