
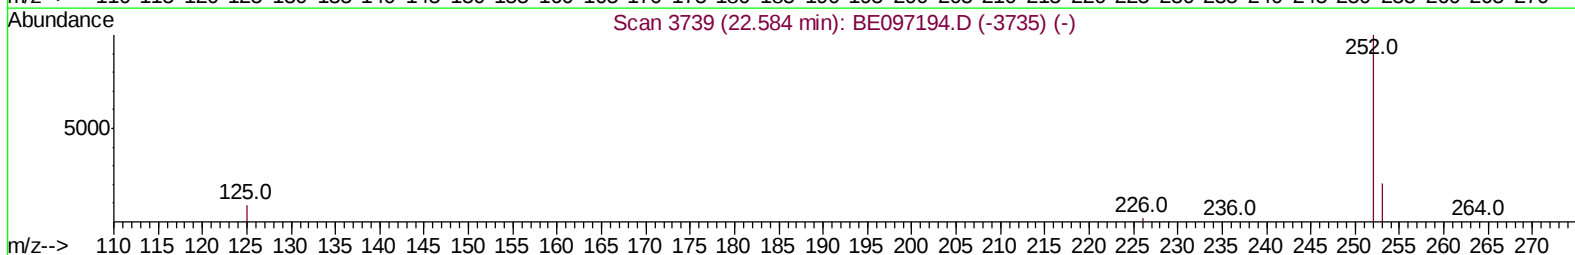
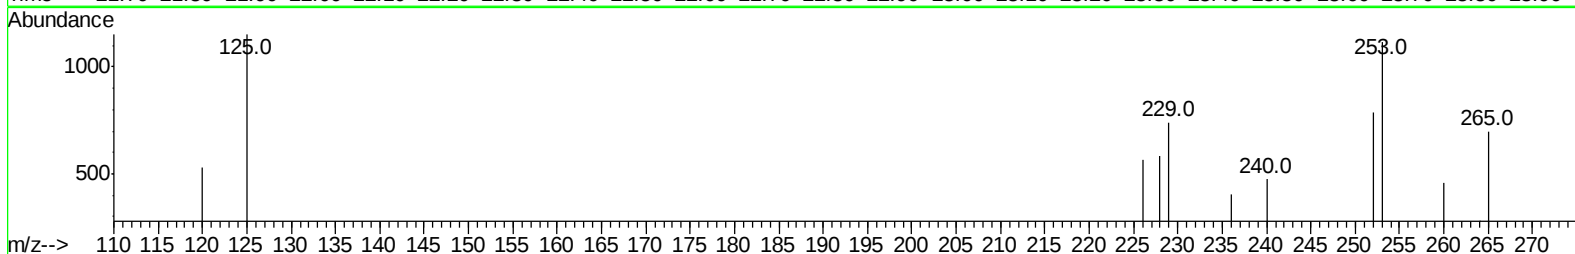


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\  
Data File : BE097207.D  
Acq On : 4 Aug 2018 18:37  
Operator : SJ/JU  
Sample : J4206-02  
Misc :  
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Aug 06 03:05:54 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 06 00:53:27 2018  
Response via : Initial Calibration

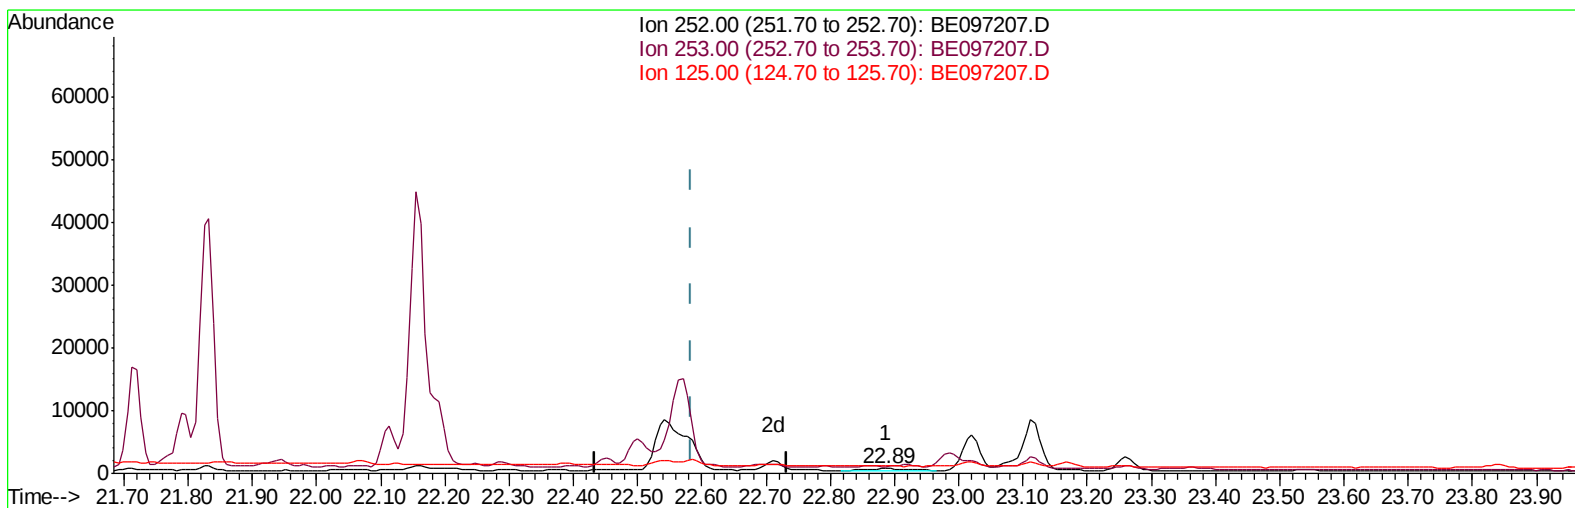

TIC: BE097207.D

(22) Benzo(k)fluoranthene

22.887min (+0.303) 0.03ng/ul

response 946

| Ion    | Exp%  | Act%    |
|--------|-------|---------|
| 252.00 | 100   | 100     |
| 253.00 | 30.60 | 141.70# |
| 125.00 | 17.10 | 146.01# |
| 0.00   | 0.00  | 0.00    |