
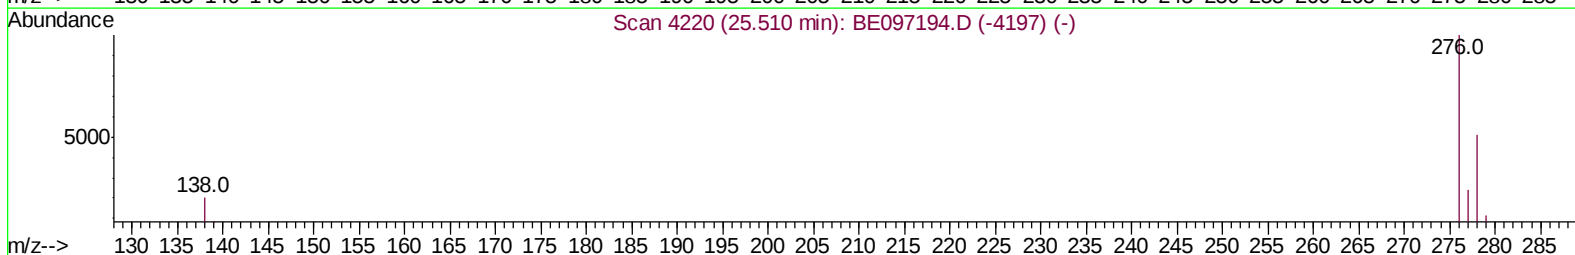
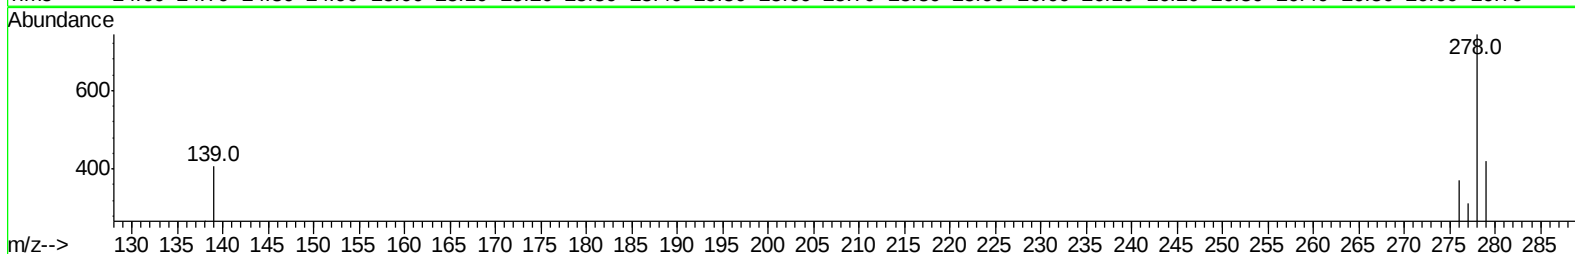


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097207.D
Acq On : 4 Aug 2018 18:37
Operator : SJ/JU
Sample : J4206-02
Misc :
ALS Vial : 15 Sample Multiplier: 1

Quant Time: Aug 06 03:05:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 00:53:27 2018
Response via : Initial Calibration

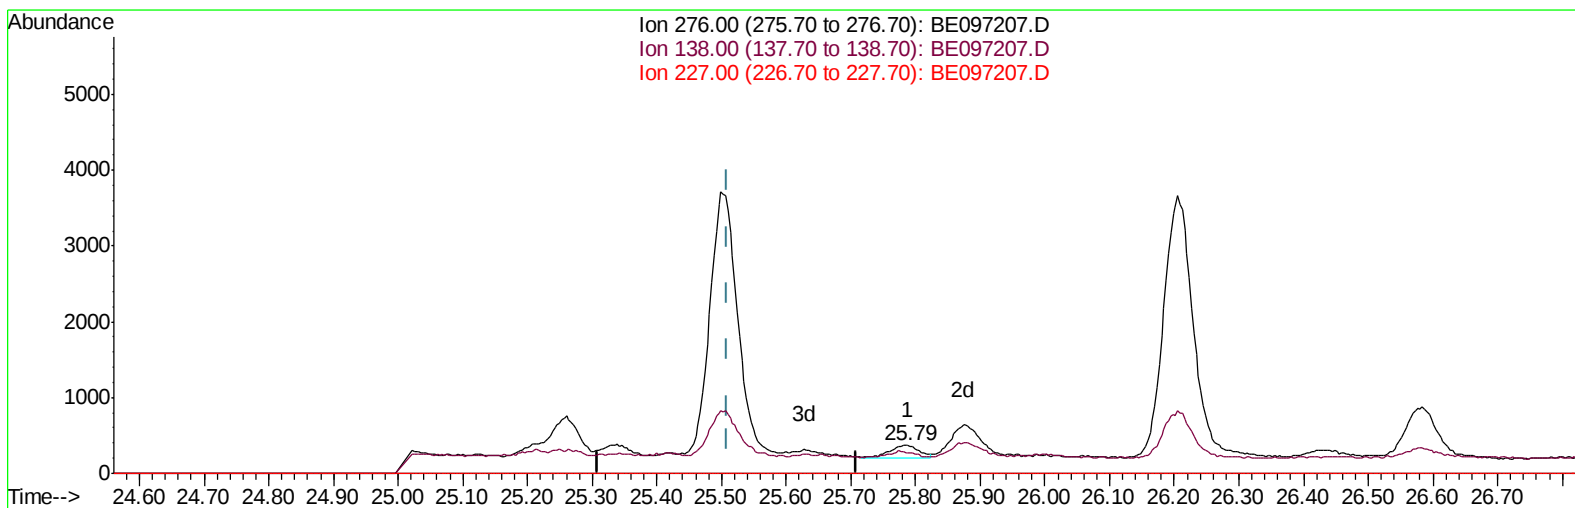

TIC: BE097207.D

(24) Indeno(1,2,3-cd)pyrene

25.788min (+0.278) 0.01ng/ul

response 521

Ion	Exp%	Act%
276.00	100	100
138.00	35.00	47.98#
227.00	10.00	0.00#
0.00	0.00	0.00