
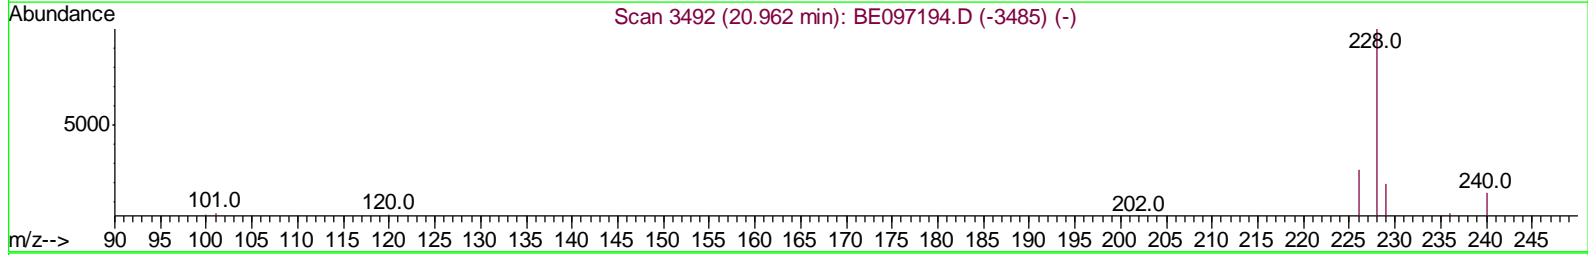
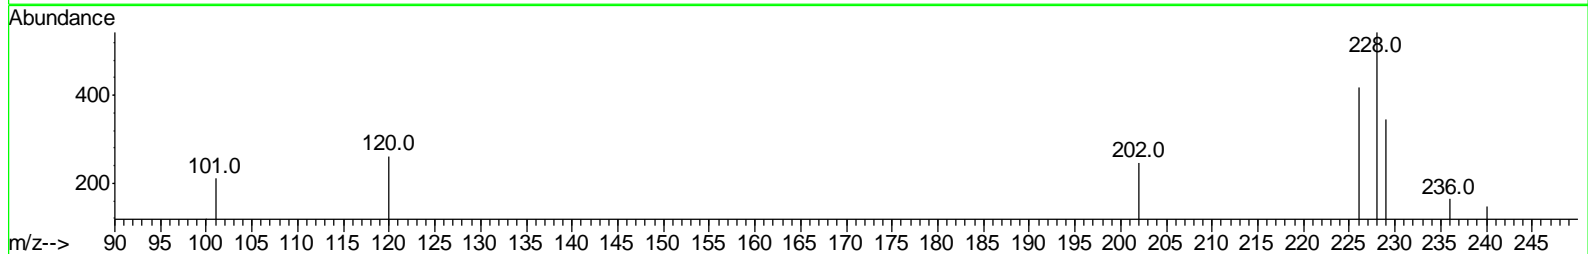


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\  
 Data File : BE097208.D  
 Acq On : 4 Aug 2018 19:13  
 Operator : SJ/JU  
 Sample : J4206-05  
 Misc :  
 ALS Vial : 16 Sample Multiplier: 1

Quant Time: Aug 06 03:24:45 2018  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Mon Aug 06 00:53:27 2018  
 Response via : Initial Calibration

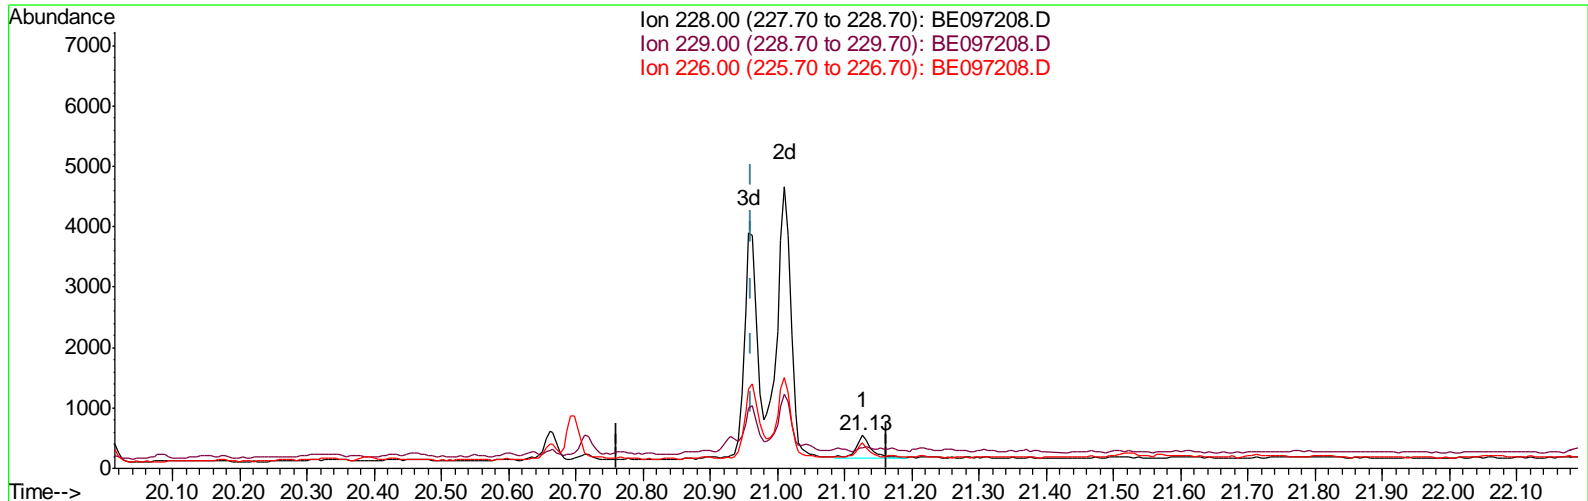

TIC: BE097208.D

(18) Benzo(a)anthracene  
 21.127min (+0.165) 0.02ng/ul  
 response 563

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	63.72#
226.00	21.30	77.16#
0.00	0.00	0.00