
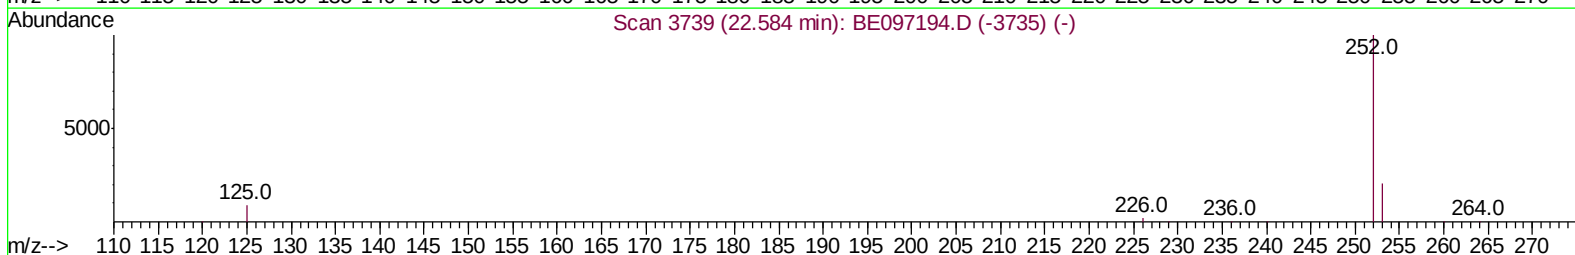
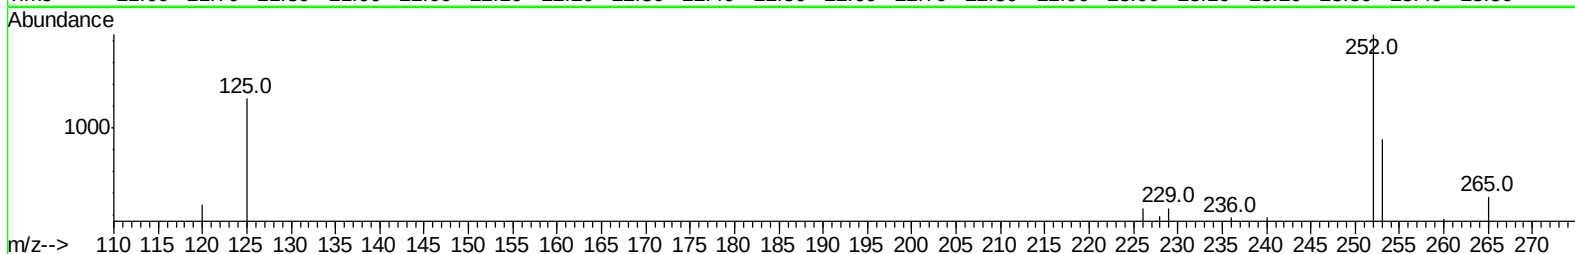


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097208.D
Acq On : 4 Aug 2018 19:13
Operator : SJ/JU
Sample : J4206-05
Misc :
ALS Vial : 16 Sample Multiplier: 1

Quant Time: Aug 06 03:26:58 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 00:53:27 2018
Response via : Initial Calibration

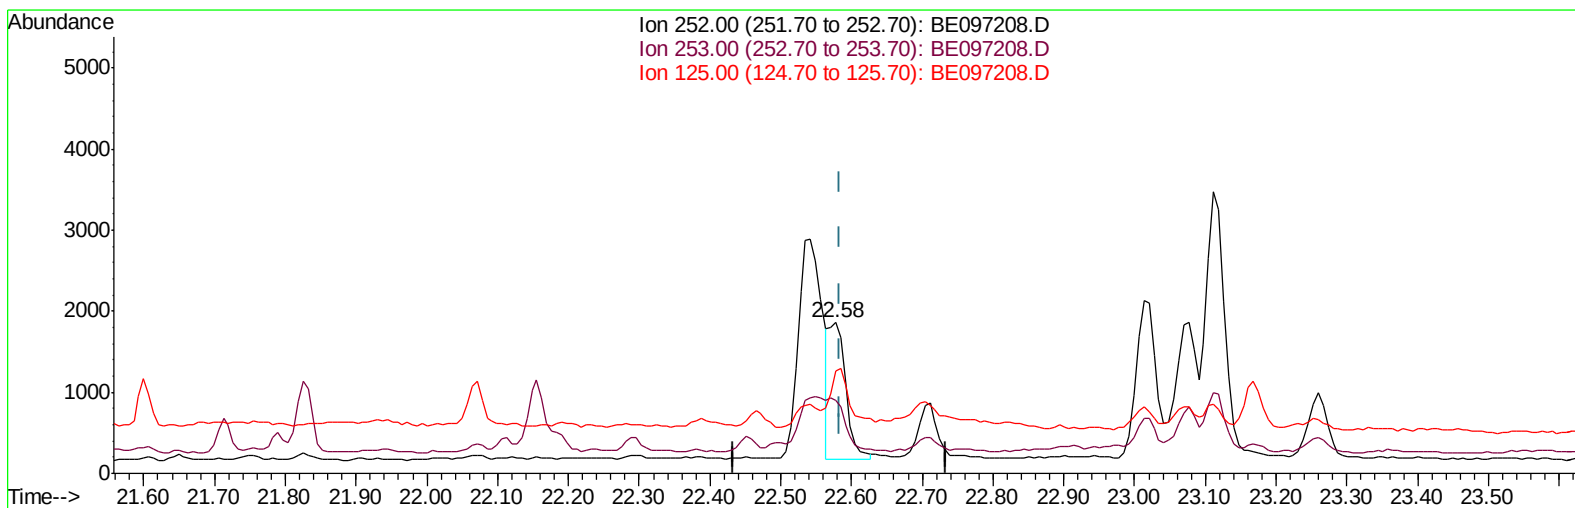

TIC: BE097208.D

(22) Benzo(k)fluoranthene

22.577min (-0.007) 0.09ng/ul m

response 2767

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	48.11#
125.00	17.10	68.27#
0.00	0.00	0.00