
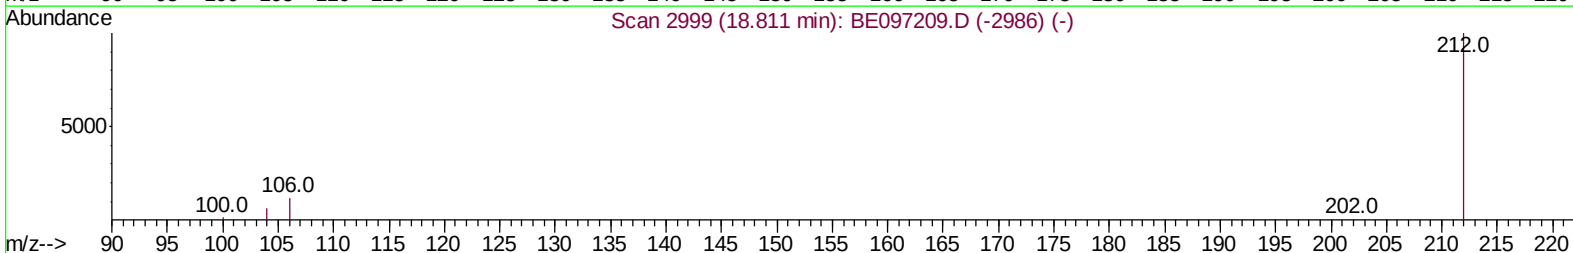
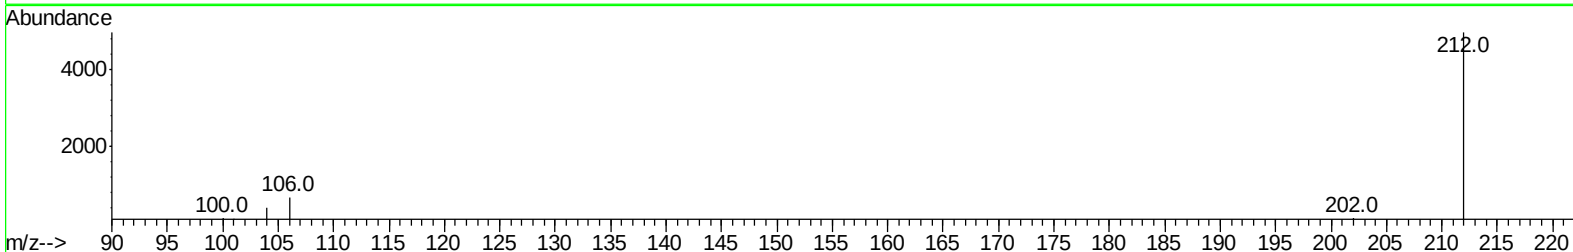


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097210.D
Acq On : 4 Aug 2018 21:06
Operator : SJ/JU
Sample : J4206-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Quant Time: Aug 06 03:54:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

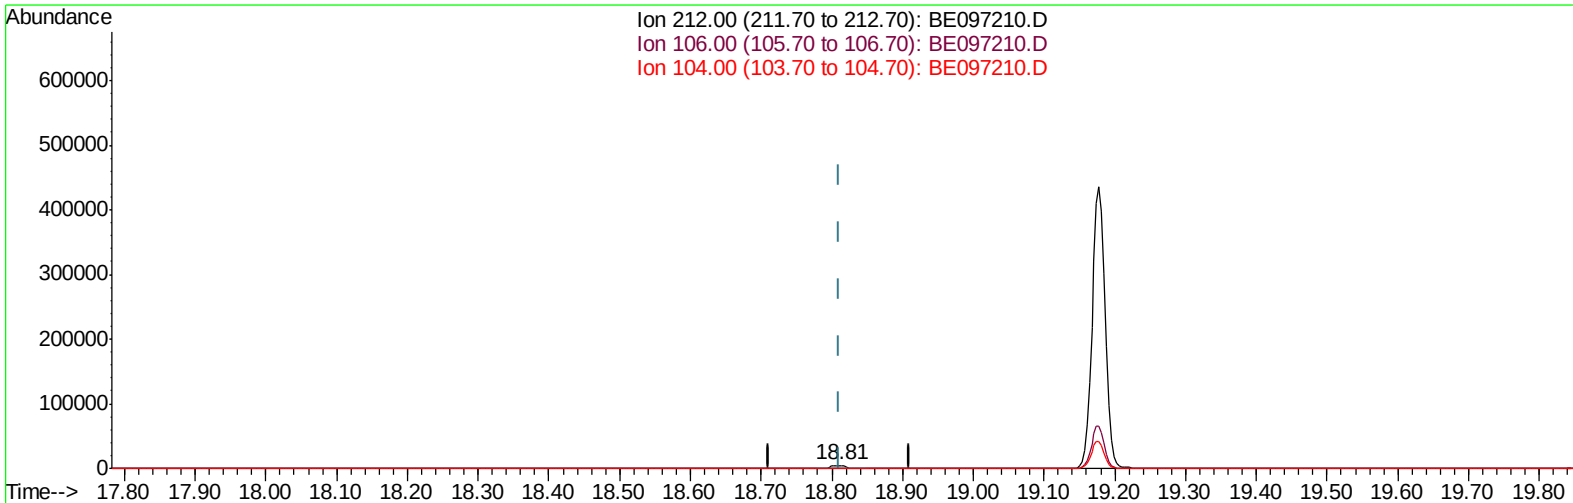

TIC: BE097210.D

(14) Fluoranthene-d10 (SURR)

18.811min (-0.000) 0.20ng/ul m

response 6885

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00