
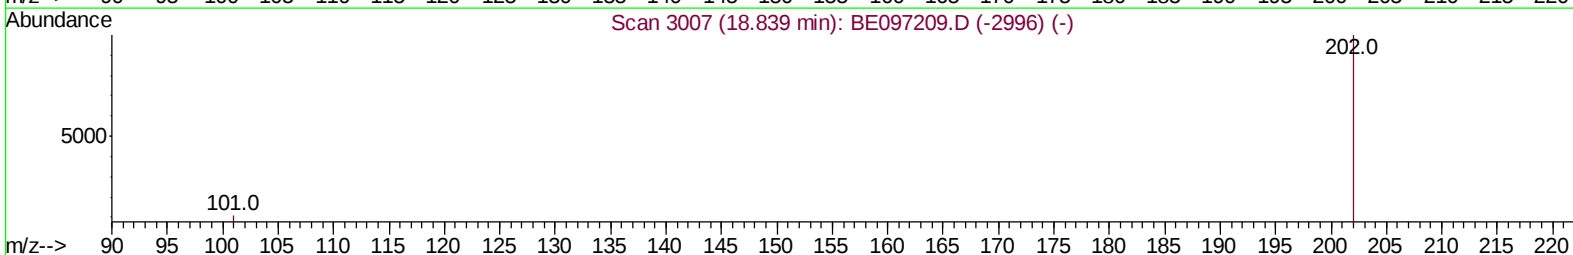
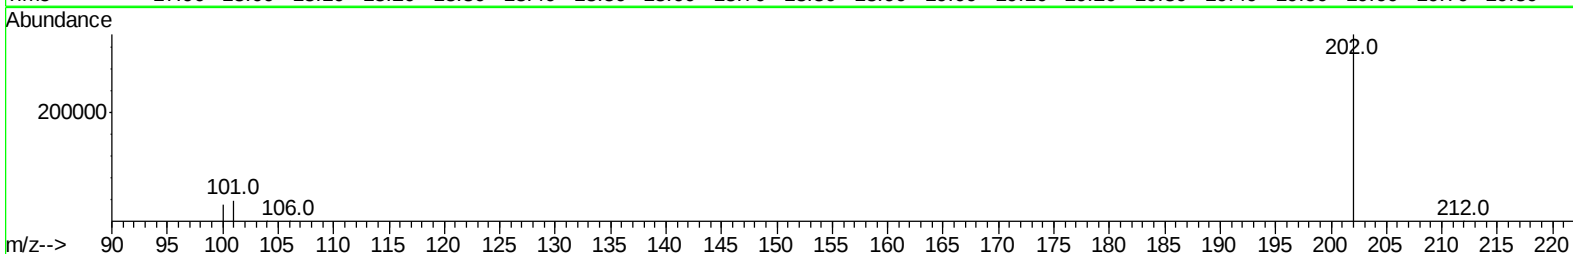


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\  
Data File : BE097212.D  
Acq On : 4 Aug 2018 22:21  
Operator : SJ/JU  
Sample : J4206-06  
Misc :  
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Aug 06 04:15:32 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 06 03:46:27 2018  
Response via : Initial Calibration

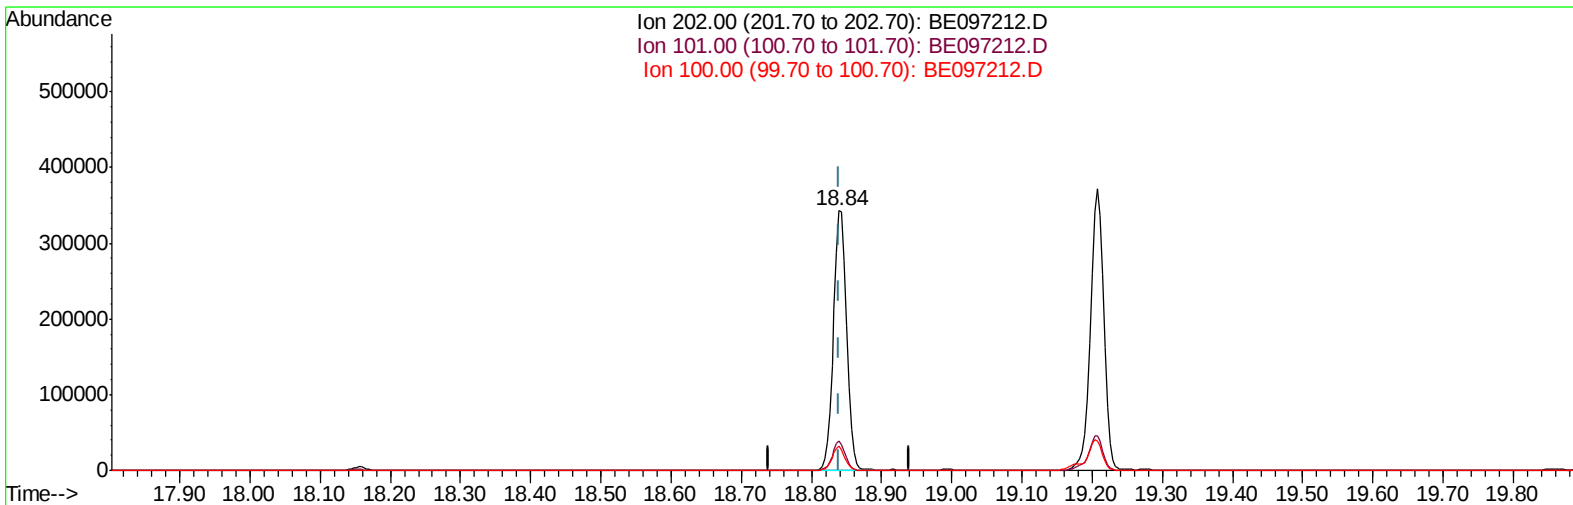

TIC: BE097212.D

(15) Fluoranthene (C)

18.840min (+0.000) 11.90ng/ul m

response 456377

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 202.00 | 100   | 100   |
| 101.00 | 10.30 | 11.32 |
| 100.00 | 19.50 | 9.15  |
| 0.00   | 0.00  | 0.00  |