
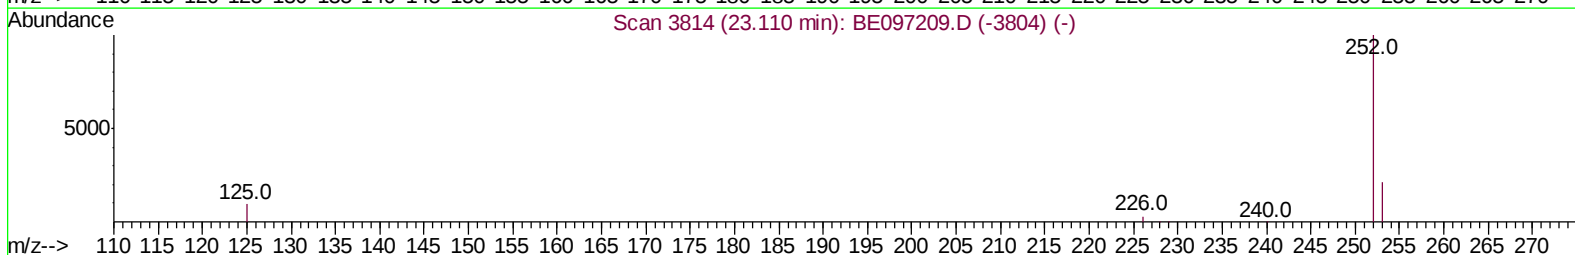
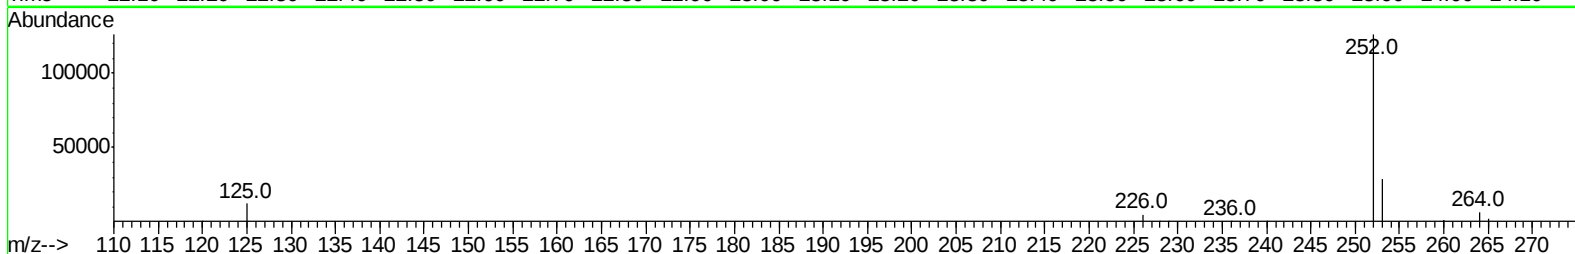


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097212.D
Acq On : 4 Aug 2018 22:21
Operator : SJ/JU
Sample : J4206-06
Misc :
ALS Vial : 19 Sample Multiplier: 1

Quant Time: Aug 06 04:17:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

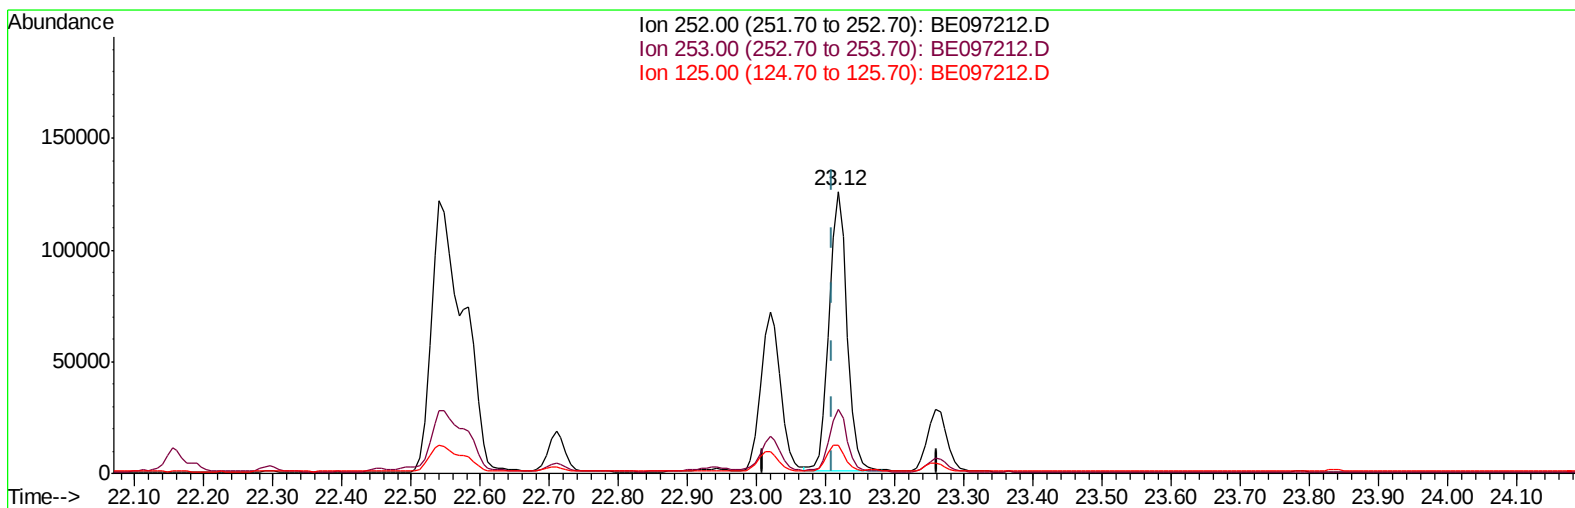

TIC: BE097212.D

(23) Benzo(a)pyrene (C)

23.117min (+0.007) 7.57ng/ul m

response 222878

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	22.65#
125.00	22.60	9.87#
0.00	0.00	0.00