
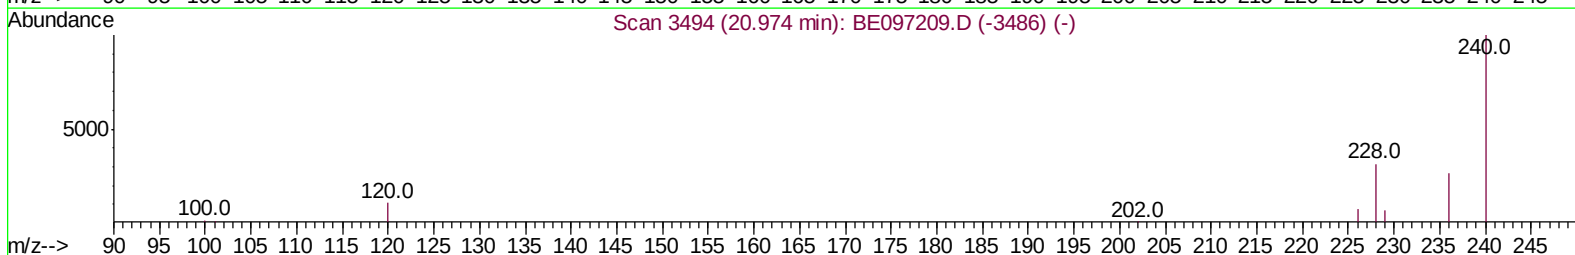
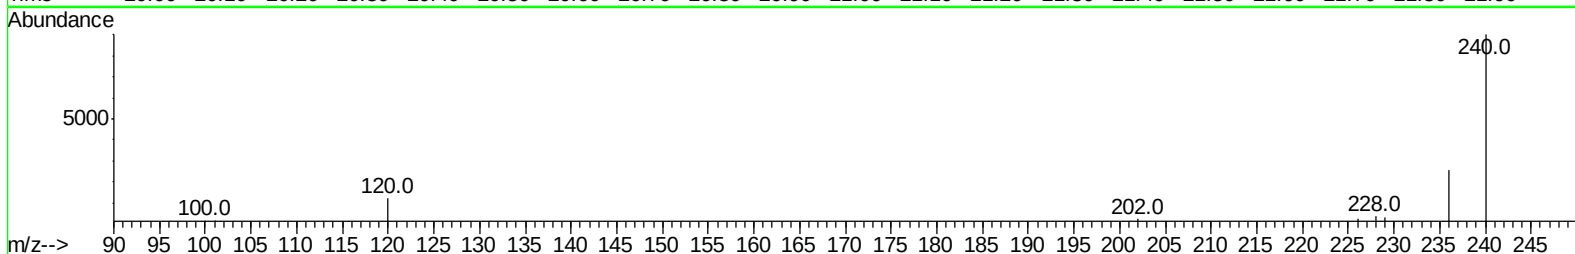


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097213.D
Acq On : 4 Aug 2018 23:00
Operator : SJ/JU
Sample : J4265-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Aug 06 04:22:55 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

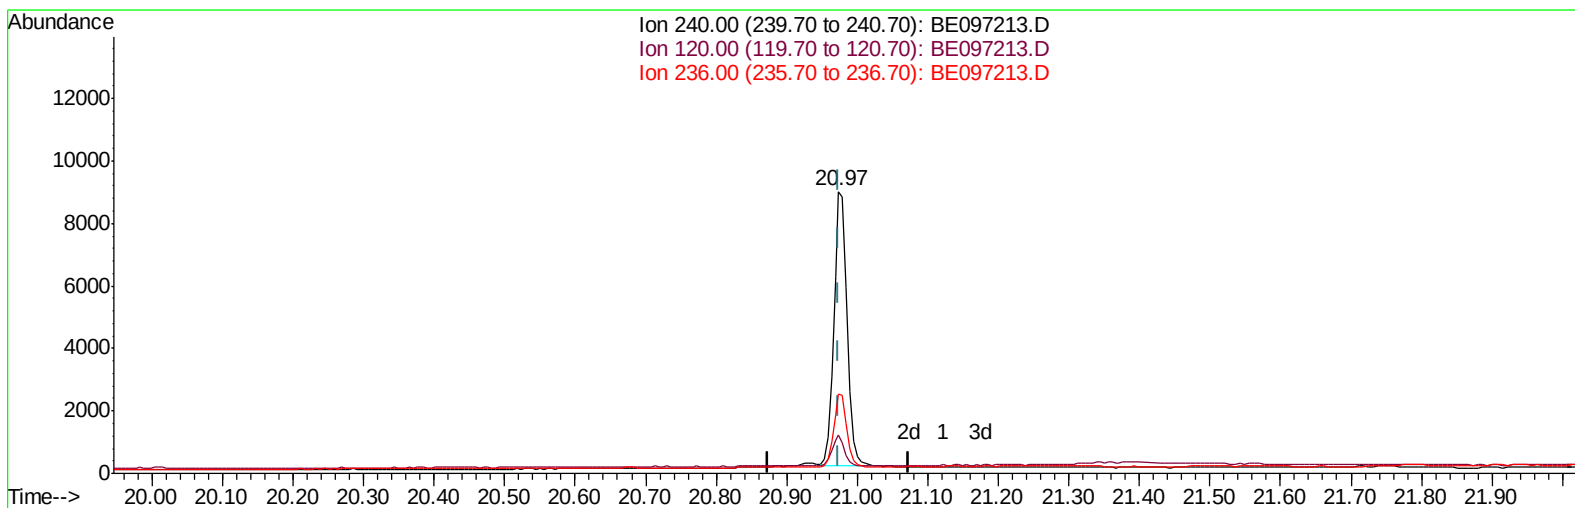

TIC: BE097213.D

(16) Chrysene-d12 (I)

20.974min (-0.000) 0.40ng/ul m

response 11642

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	13.43#
236.00	34.90	28.39
0.00	0.00	0.00