
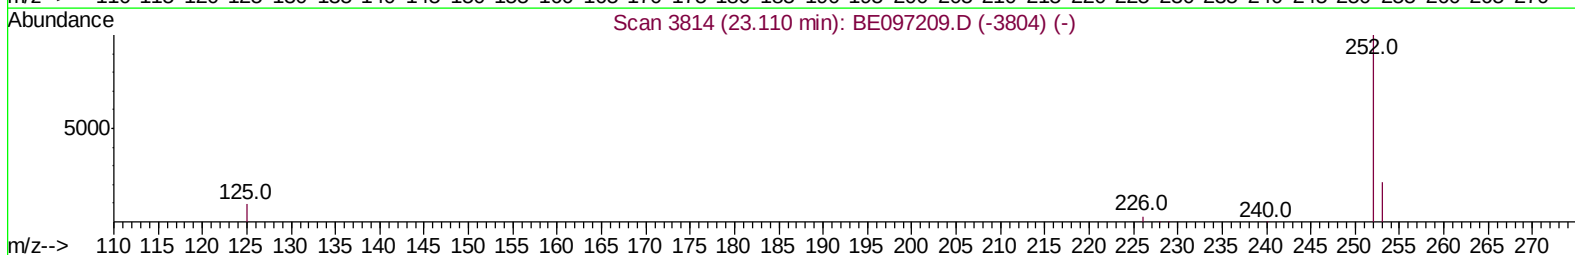
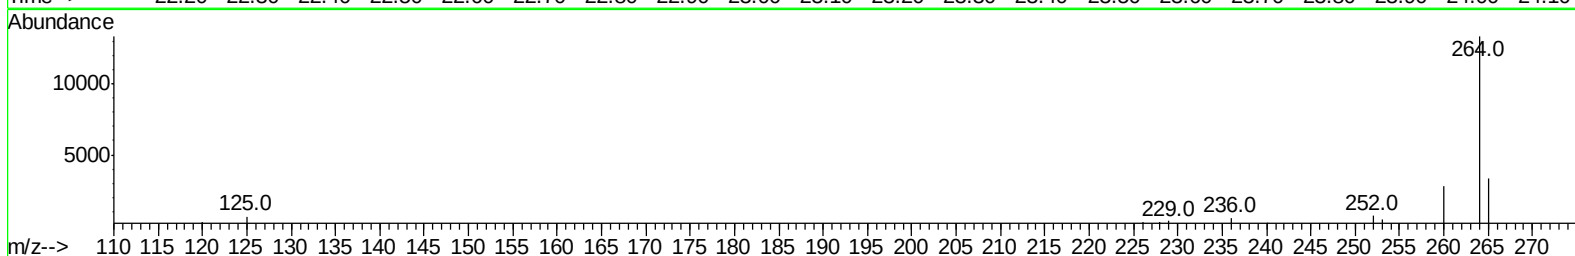


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097213.D
Acq On : 4 Aug 2018 23:00
Operator : SJ/JU
Sample : J4265-07
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Aug 06 04:30:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

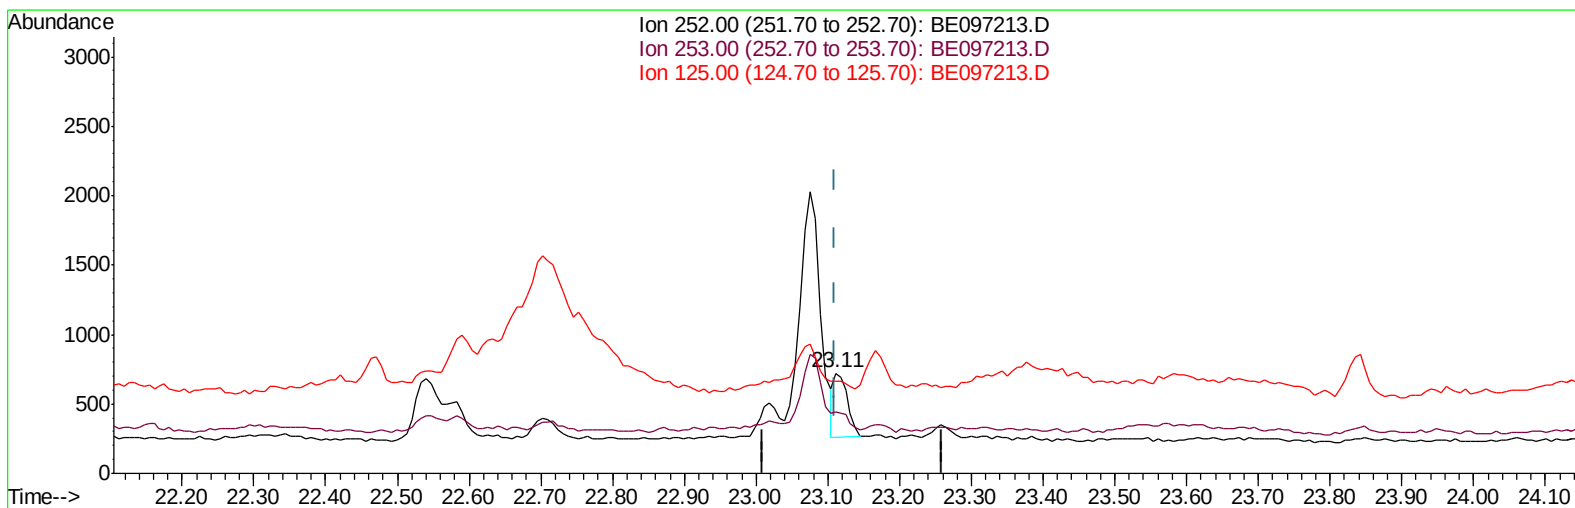

TIC: BE097213.D

(23) Benzo(a)pyrene (C)

23.110min (-0.000) 0.02ng/ul m

response 619

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	61.63#
125.00	22.60	92.52#
0.00	0.00	0.00