
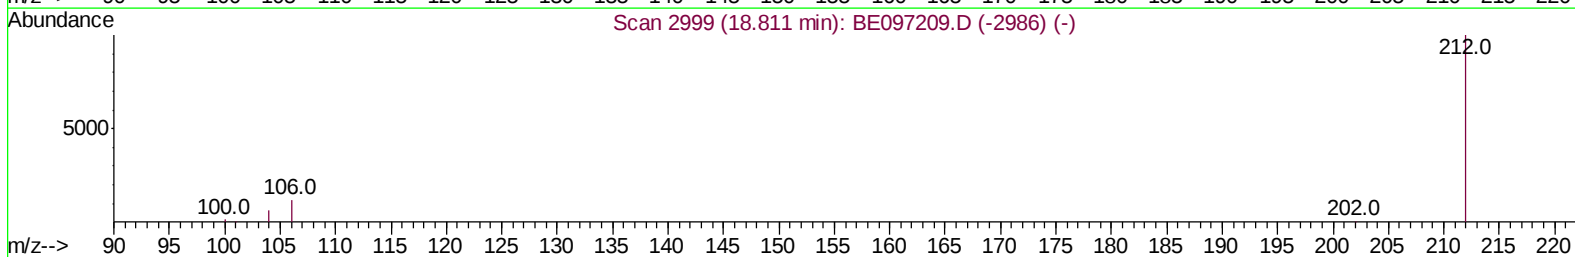
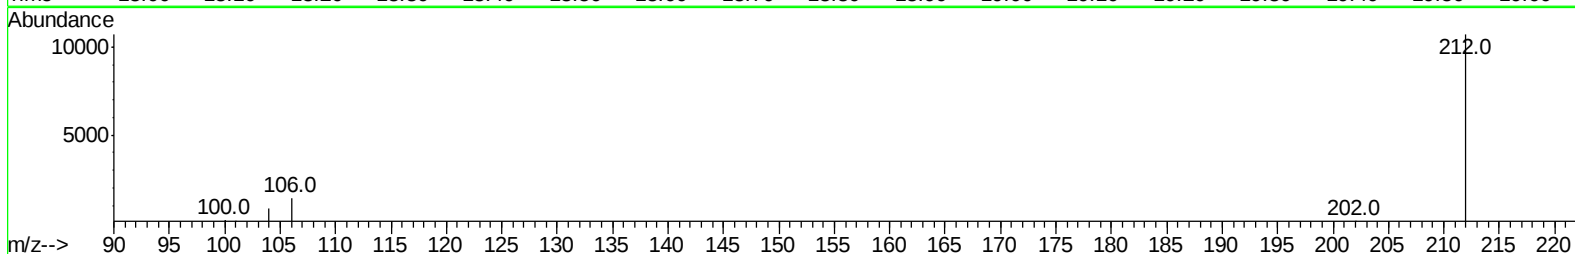


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\  
Data File : BE097214.D  
Acq On : 4 Aug 2018 23:38  
Operator : SJ/JU  
Sample : J4265-10  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Aug 06 04:34:50 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 06 03:46:27 2018  
Response via : Initial Calibration

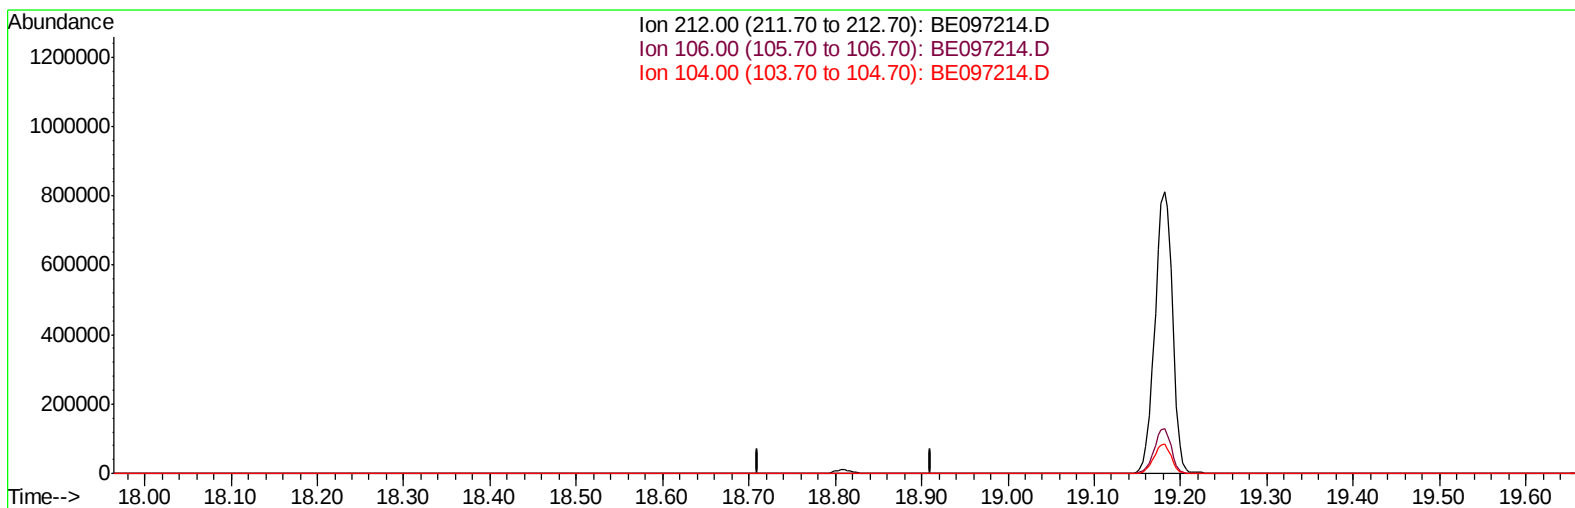

TIC: BE097214.D

(14) Fluoranthene-d10 (SURRE)

18.811min (-18.811) 0.00ng/ul

response 0

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 212.00 | 100   | 0.00  |
| 106.00 | 18.30 | 0.00# |
| 104.00 | 15.60 | 0.00# |
| 0.00   | 0.00  | 0.00  |