
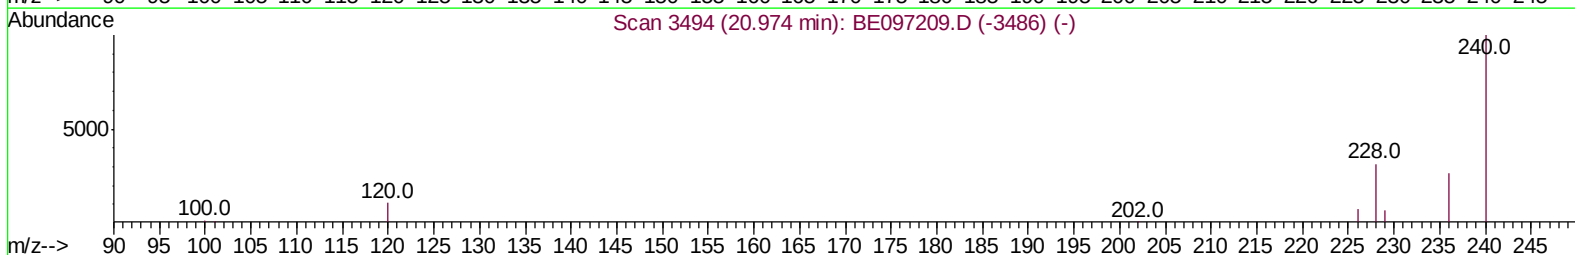
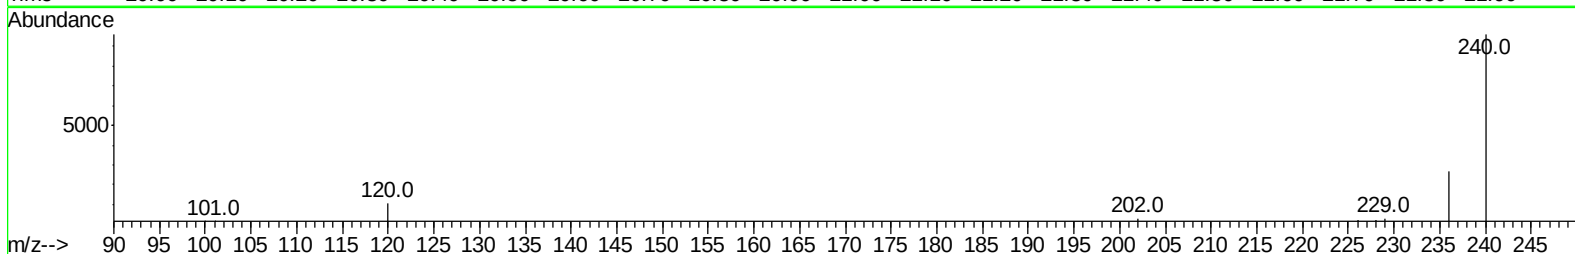


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\  
Data File : BE097214.D  
Acq On : 4 Aug 2018 23:38  
Operator : SJ/JU  
Sample : J4265-10  
Misc :  
ALS Vial : 21 Sample Multiplier: 1

Quant Time: Aug 06 04:34:50 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Aug 06 03:46:27 2018  
Response via : Initial Calibration

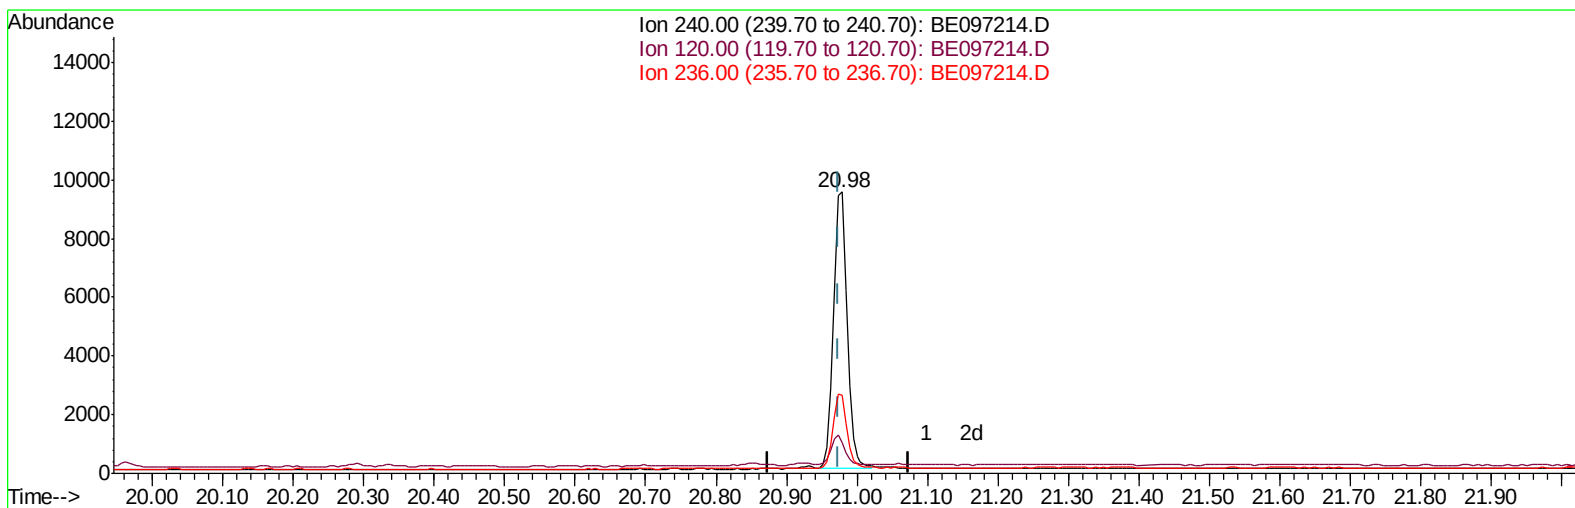

TIC: BE097214.D

(16) Chrysene-d12 (I)

20.979min (+0.005) 0.40ng/ul m

response 12423

| Ion    | Exp%  | Act%   |
|--------|-------|--------|
| 240.00 | 100   | 100    |
| 120.00 | 20.60 | 11.12# |
| 236.00 | 34.90 | 27.75# |
| 0.00   | 0.00  | 0.00   |