
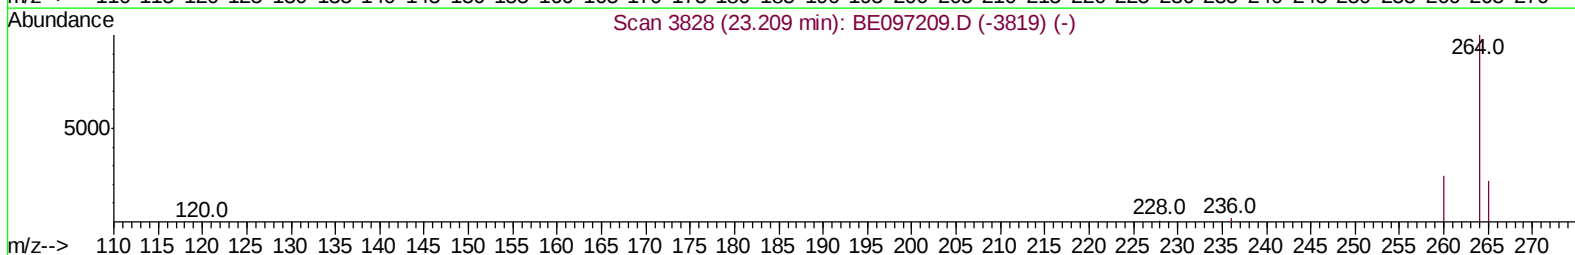
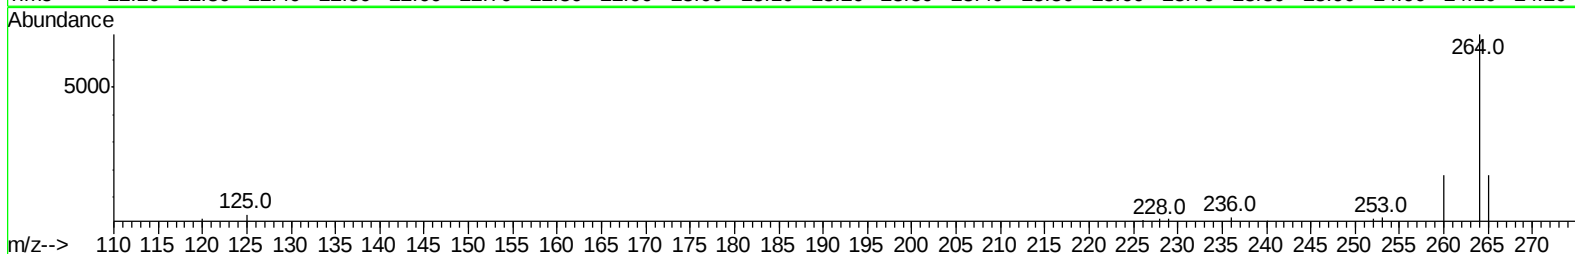


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097215.D
Acq On : 5 Aug 2018 00:17
Operator : SJ/JU
Sample : J4171-16DL 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Aug 06 03:52:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

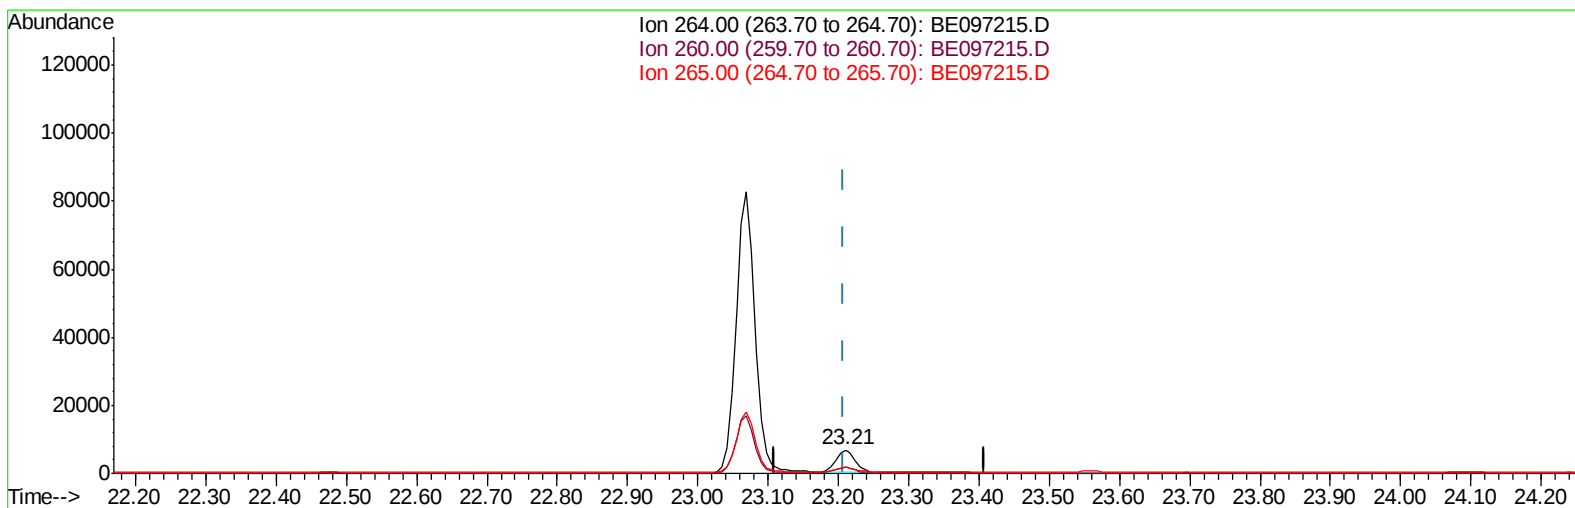

TIC: BE097215.D

(20) Perylene-d12 (I)

23.210min (+0.001) 0.40ng/ul m

response 12357

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.41
265.00	103.50	26.19#
0.00	0.00	0.00