

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097201.D
 Acq On : 4 Aug 2018 14:50
 Operator : SJ/JU
 Sample : J4265-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 06 00:55:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 00:53:27 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1343	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	7285	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	4557	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	699073	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.98
20) Perylene-d12	23.21	264	14257	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	3069	0.26	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.07	252	2689	0.069	ng/ul#	Ovalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097201.D
Acq On : 4 Aug 2018 14:50
Operator : SJ/JU
Sample : J4265-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 06 00:55:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 00:53:27 2018
Response via : Initial Calibration

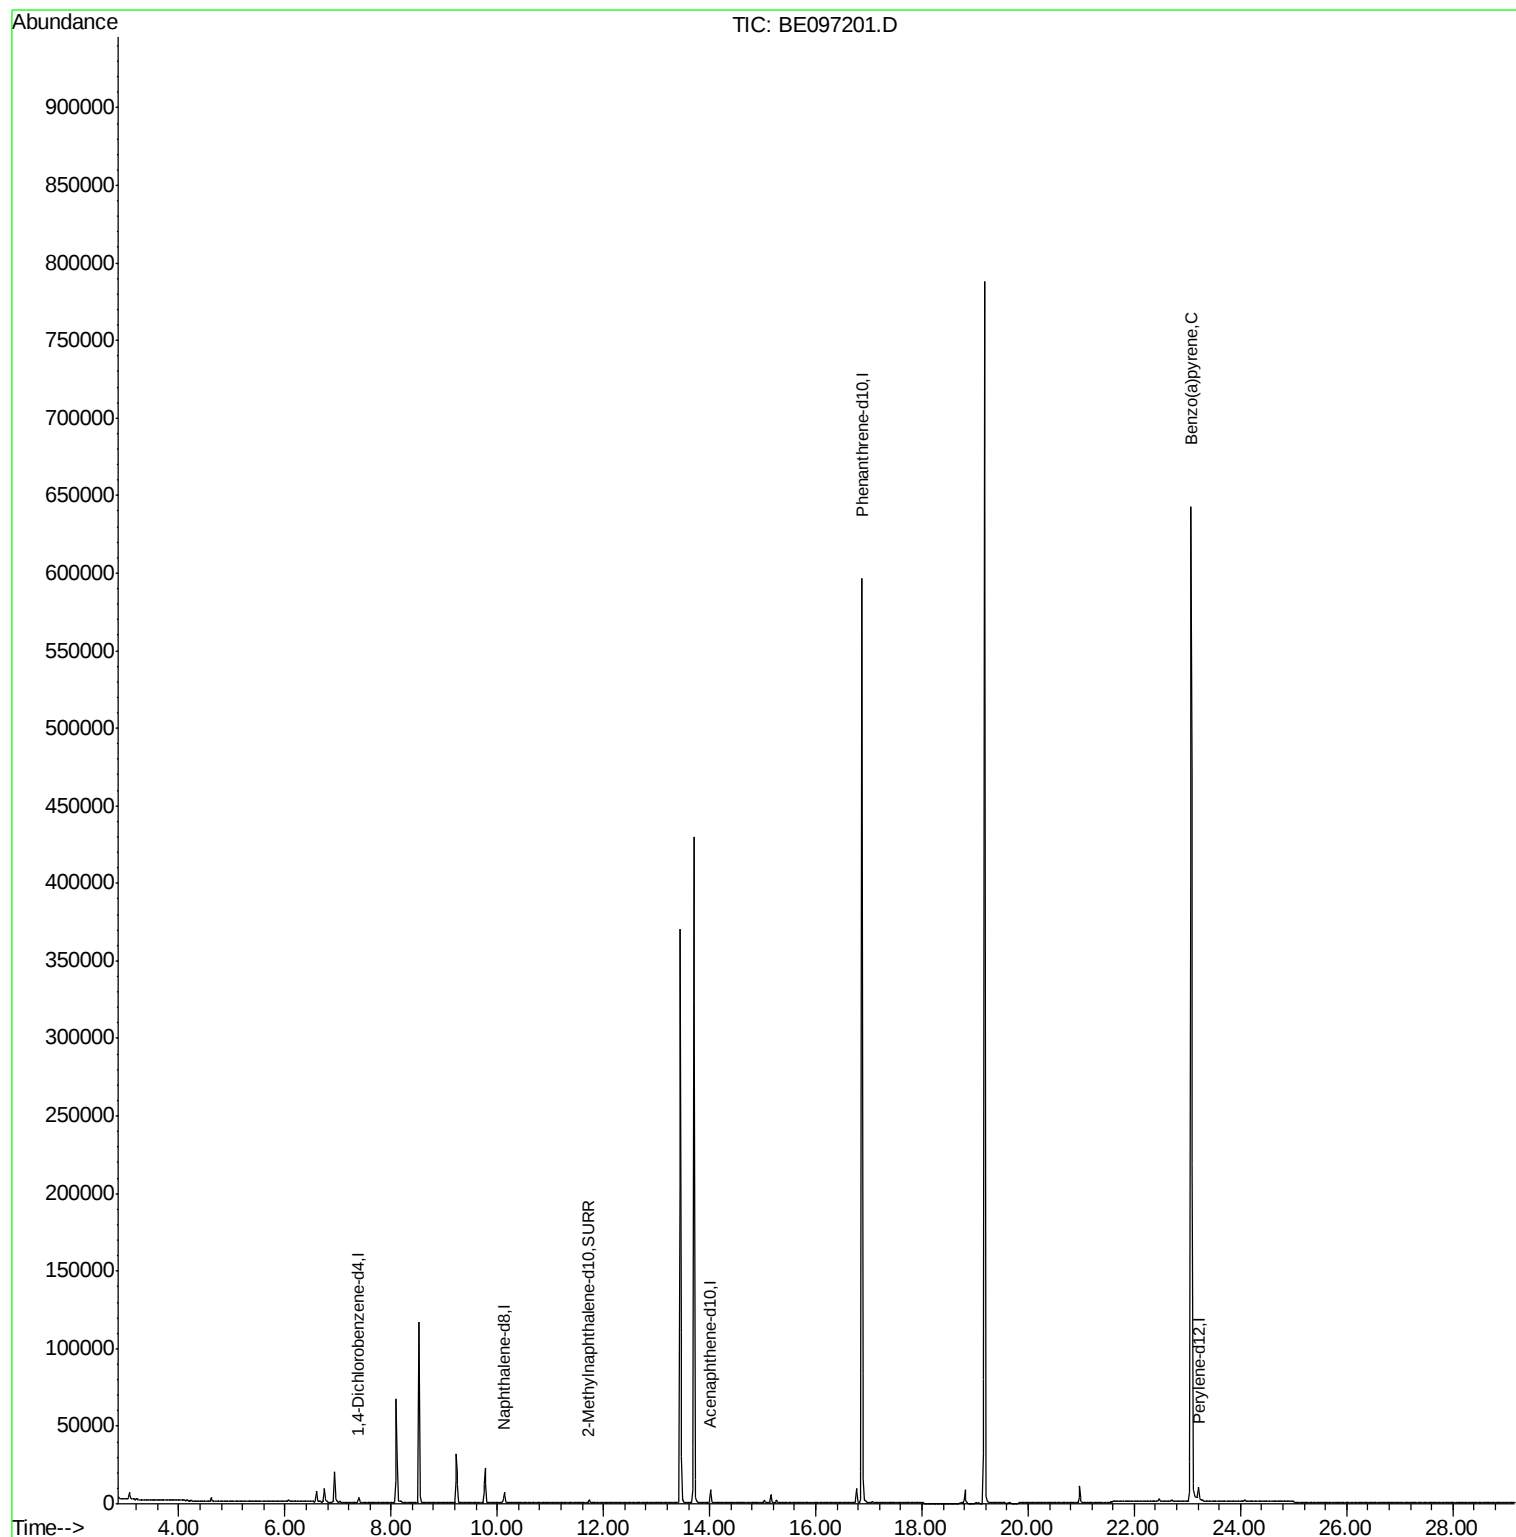

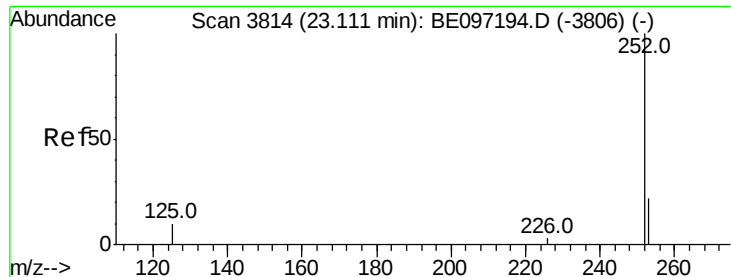

#23

Benzo(a)pyrene

Concen: 0.069 ng/ul

RT: 23.07 min Scan# 3807

Delta R.T. -0.04 min


Lab File: BE097201.D

Acq: 4 Aug 2018 14:50

Instrument :

BNA_E

ClientSampleId :

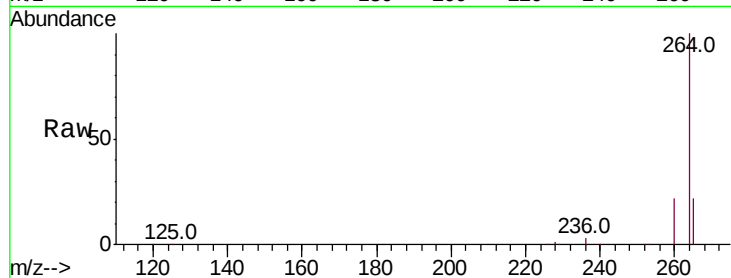


Tot Ion: 252 Resp: 2689

Ion Ratio Lower Upper

252 100

253 36.1 28.5 42.7

125 27.8 18.1 27.1#

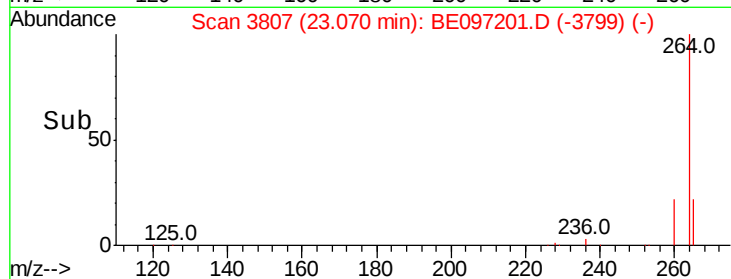

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

