

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097203.D
 Acq On : 4 Aug 2018 16:05
 Operator : SJ/JU
 Sample : J4265-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 06 00:55:53 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 00:53:27 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1311	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	7115	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	4495	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	758397	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.98
20) Perylene-d12	23.21	264	14488	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	3357	0.29	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
					Ovalue	
21) Benzo(b)fluoranthene	22.54	252	1453	0.037	ng/ul	93
22) Benzo(k)fluoranthene	22.58	252	1527	0.036	ng/ul#	75
23) Benzo(a)pyrene	23.11	252	1338	0.034	ng/ul	97
24) Indeno(1,2,3-cd)pyrene	25.51	276	1823	0.037	ng/ul#	82
25) Dibenzo(a,h)anthracene	25.53	278	1650	0.041	ng/ul#	81
26) Benzo(g,h,i)perylene	26.21	276	1564	0.037	ng/ul#	88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097203.D
Acq On : 4 Aug 2018 16:05
Operator : SJ/JU
Sample : J4265-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 06 00:55:53 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 00:53:27 2018
Response via : Initial Calibration

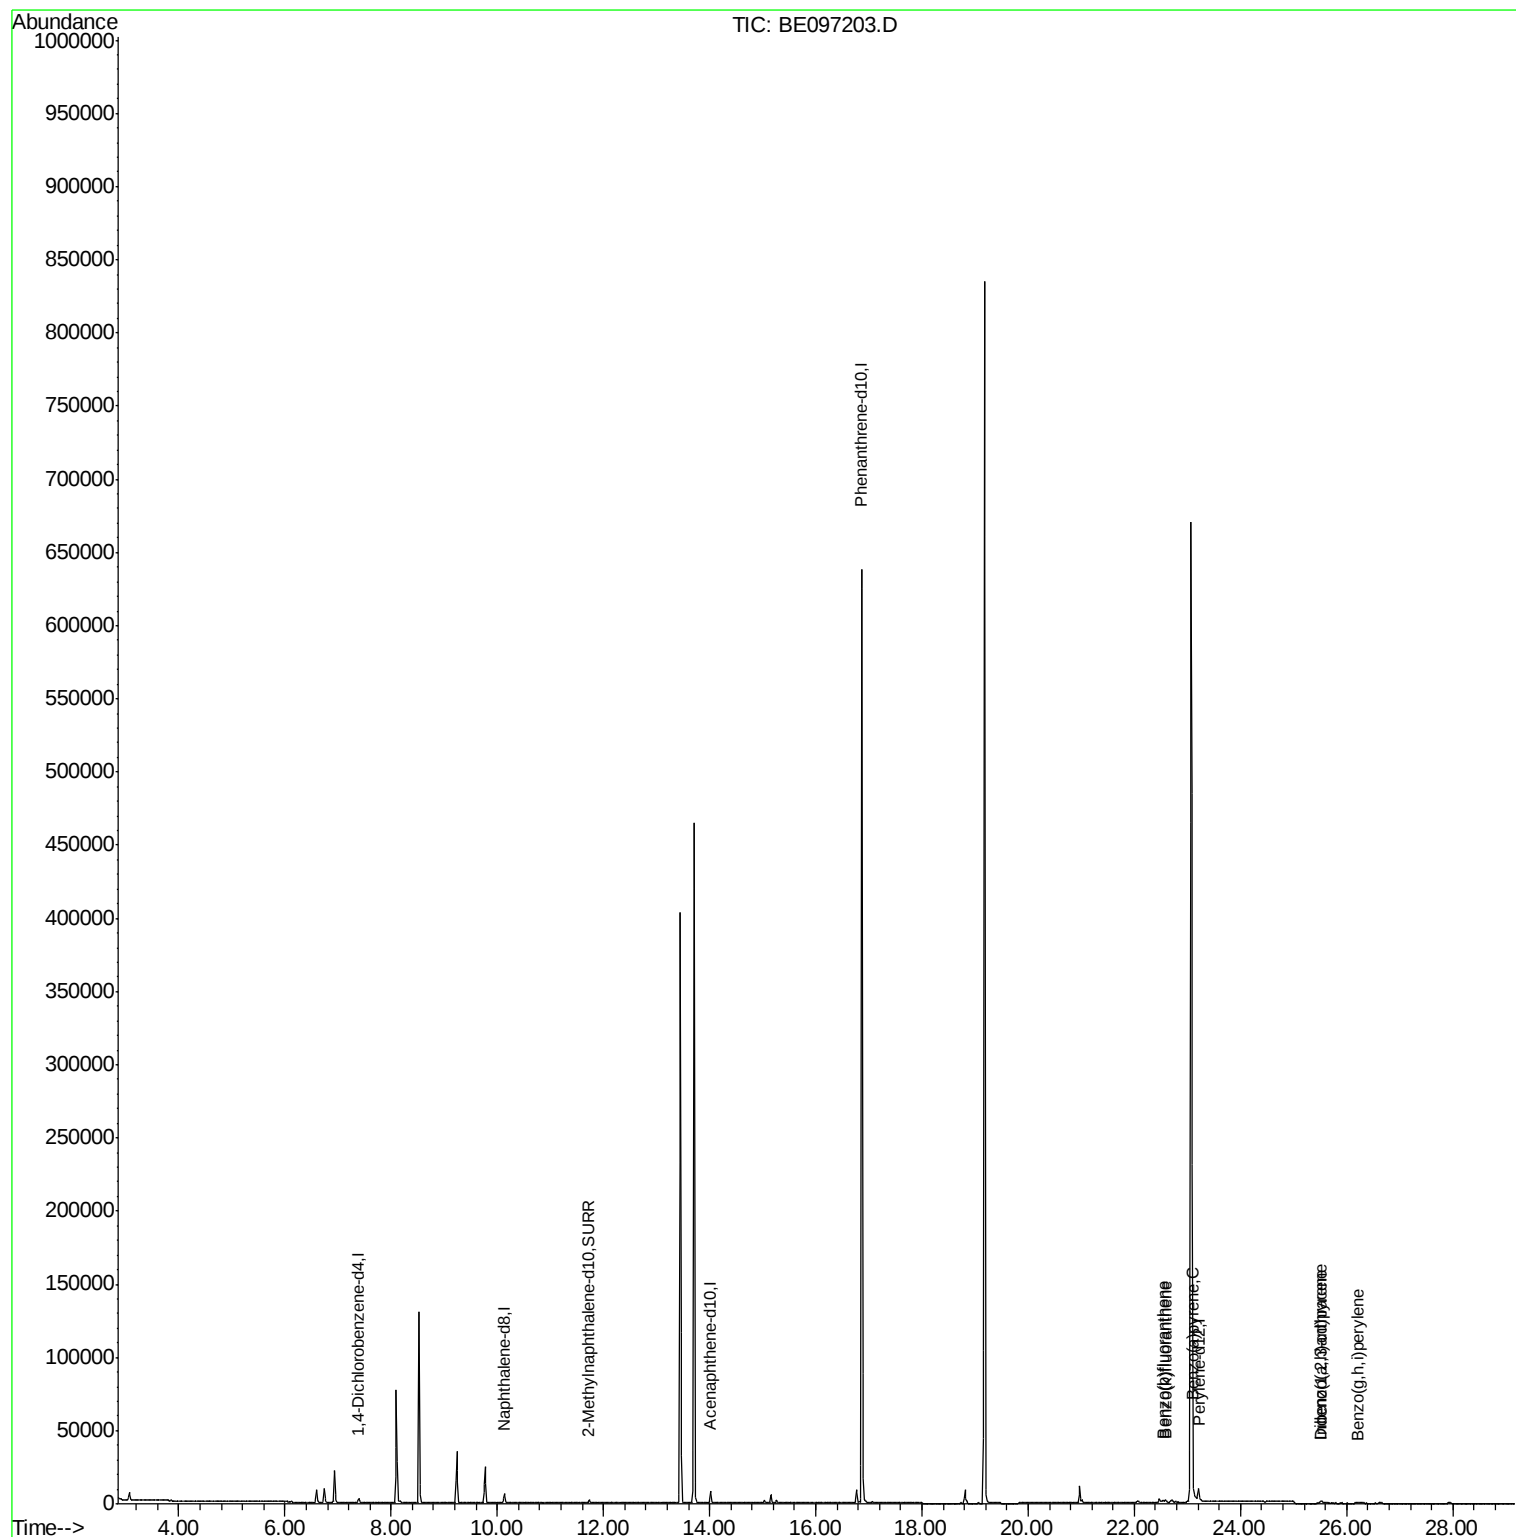

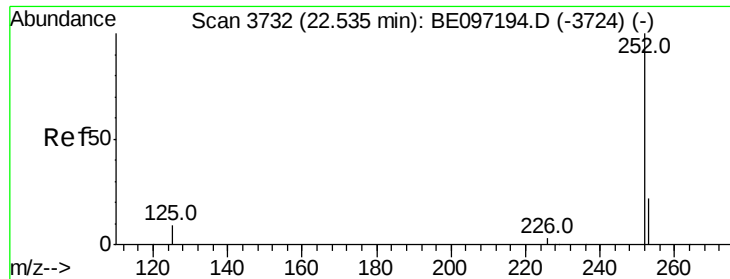

#21

Benzo(b)fluoranthene

Concen: 0.037 ng/ul

RT: 22.54 min Scan# 3732

Delta R.T. 0.00 min

Lab File: BE097203.D

Acq: 4 Aug 2018 16:05

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 1453

Ion Ratio Lower Upper

252 100

253 34.2 0.0 64.2




125 23.0 0.0 35.0

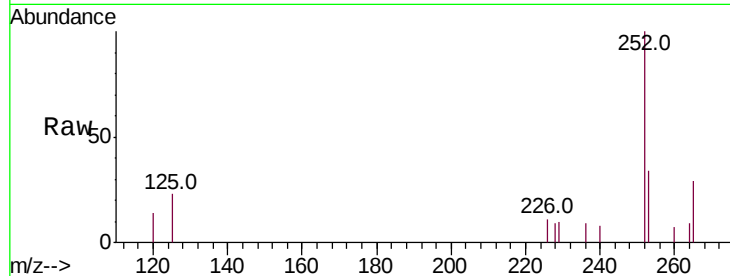

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

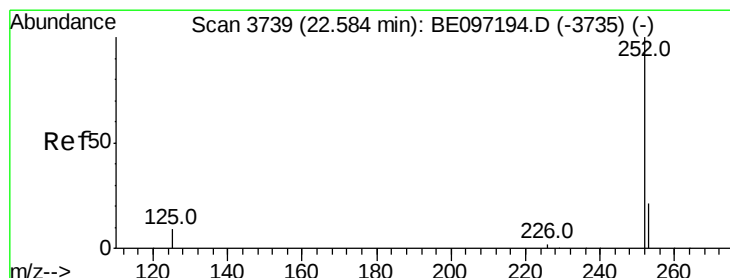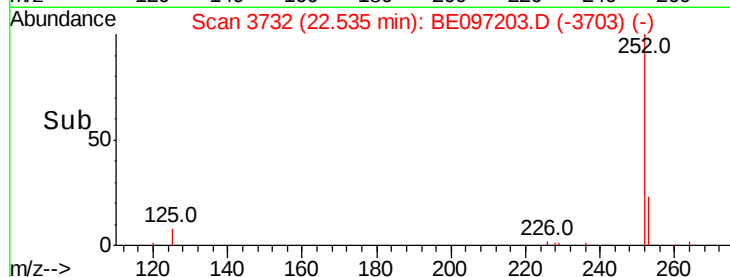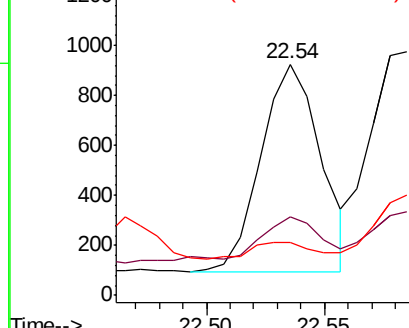

#22

Benzo(k)fluoranthene

Concen: 0.036 ng/ul

RT: 22.58 min Scan# 3739

Delta R.T. 0.00 min

Lab File: BE097203.D

Acq: 4 Aug 2018 16:05


Tgt Ion:252 Resp: 1527

Ion Ratio Lower Upper

252 100

253 34.6 24.5 36.7



125 41.4 13.7 20.5#

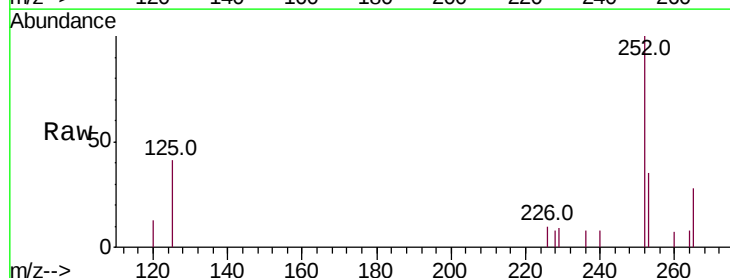


Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

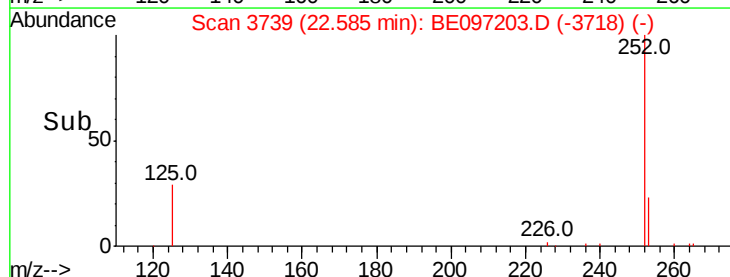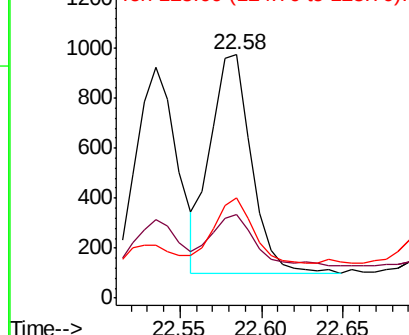

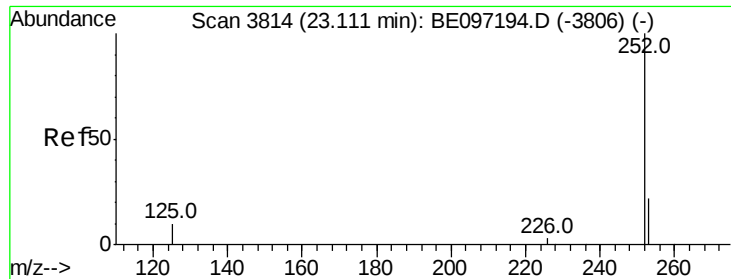

#23

Benzo(a)pyrene

Concen: 0.034 ng/ul

RT: 23.11 min Scan# 3814

Delta R.T. 0.00 min

Lab File: BE097203.D

Acq: 4 Aug 2018 16:05

Instrument :

BNA_E

ClientSampleId :


Tot Ion:252 Resp: 1338

Ion Ratio Lower Upper

252 100

253 33.0 28.5 42.7




125 23.3 18.1 27.1

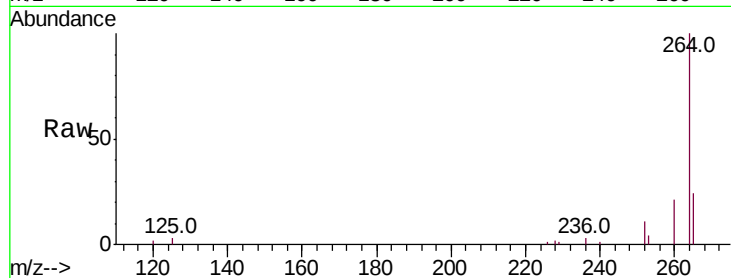

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

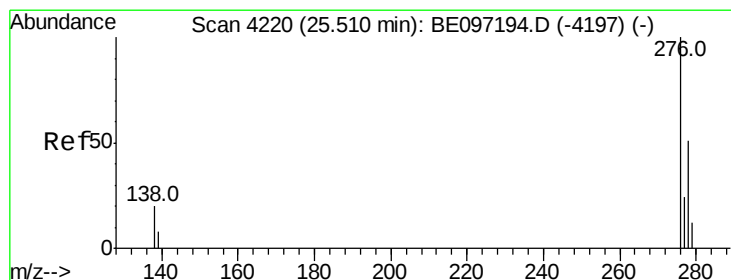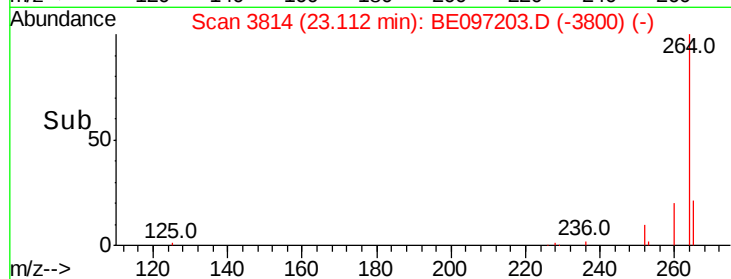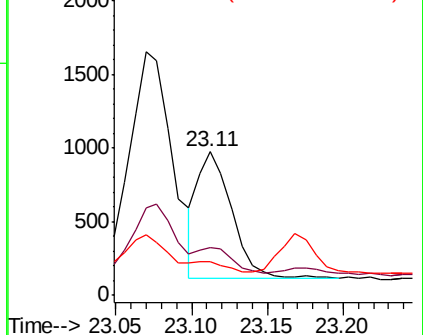

#24

Indeno(1,2,3-cd)pyrene

Concen: 0.037 ng/ul

RT: 25.51 min Scan# 4220

Delta R.T. 0.00 min

Lab File: BE097203.D

Acq: 4 Aug 2018 16:05


Tgt Ion:276 Resp: 1823

Ion Ratio Lower Upper

276 100

138 26.4 28.0 42.0#



227 0.0 8.0 12.0#

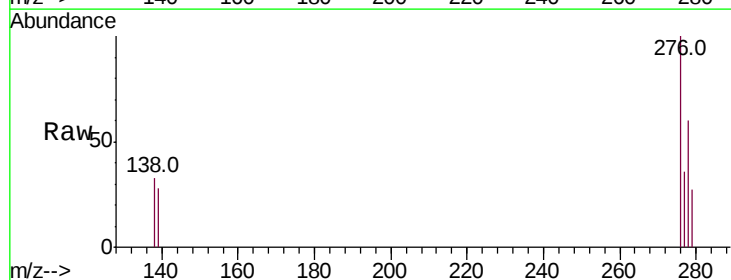


Abundance Ion 276.00 (275.70 to 276.70): E

Ion 138.00 (137.70 to 138.70): E

Ion 227.00 (226.70 to 227.70): E



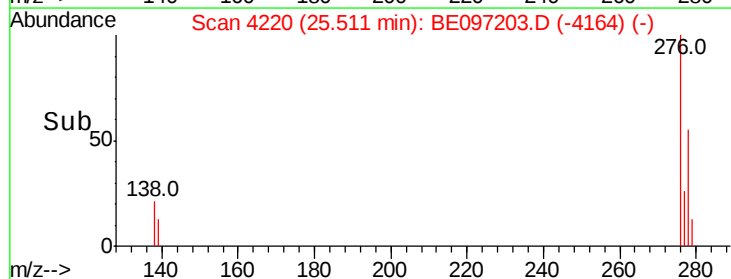
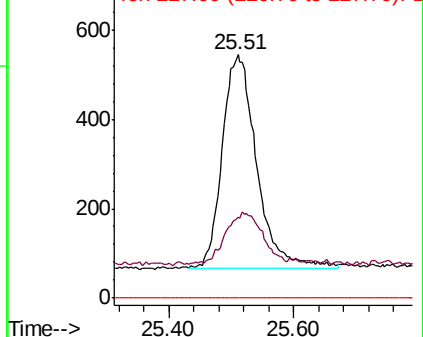


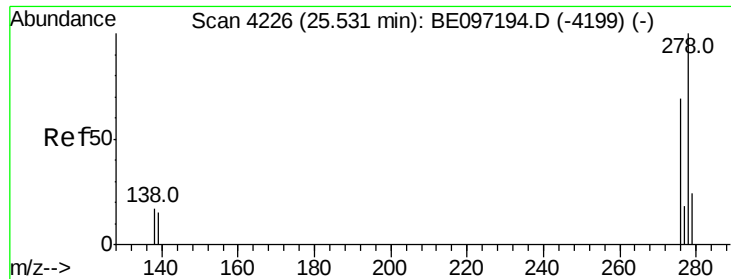

#25
Dibenzo(a,h)anthracene
Concen: 0.041 ng/ul
RT: 25.53 min Scan# 4226
Delta R.T. 0.00 min
Lab File: BE097203.D
Acq: 4 Aug 2018 16:05

Instrument :
BNA_E
ClientSampleId :

Tot Ion:278 Resp: 1650
Ion Ratio Lower Upper
278 100
139 39.3 17.4 26.0#
279 35.8 25.9 38.9

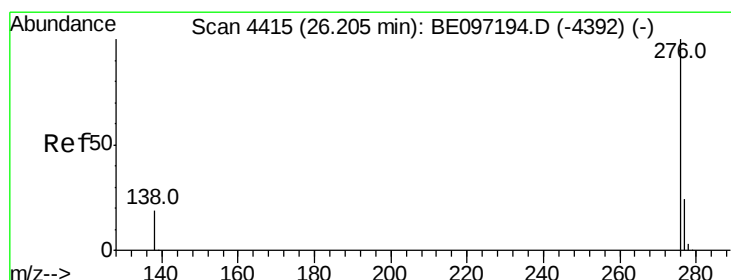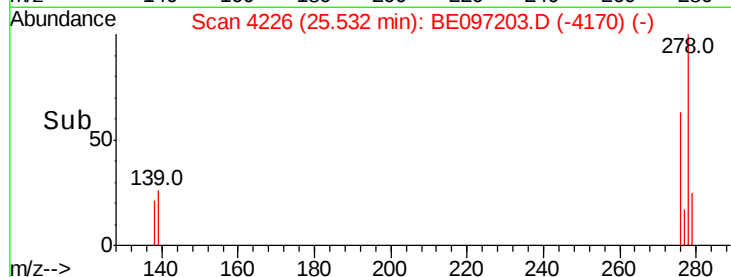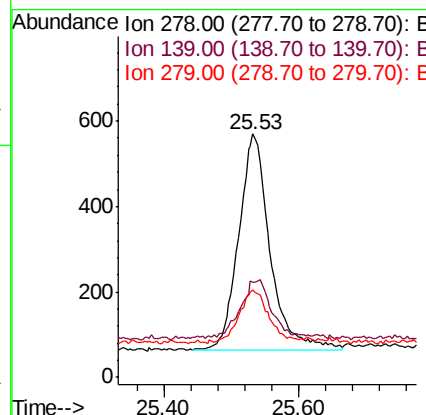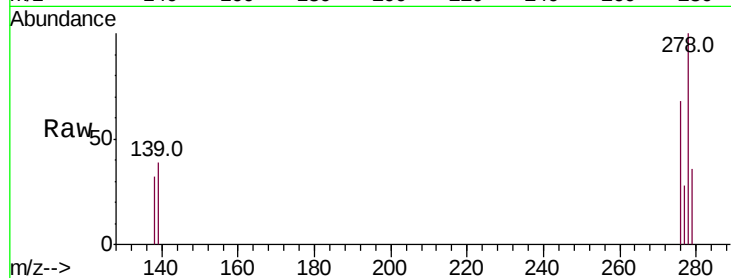

#26
Benzo(g,h,i)perylene
Concen: 0.037 ng/ul
RT: 26.21 min Scan# 4416
Delta R.T. 0.00 min
Lab File: BE097203.D
Acq: 4 Aug 2018 16:05

Tgt Ion:276 Resp: 1564
Ion Ratio Lower Upper
276 100
138 30.3 21.8 32.8
277 35.5 20.5 30.7#

