

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097205.D
 Acq On : 4 Aug 2018 17:22
 Operator : SJ/JU
 Sample : J4206-03
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 06 00:56:01 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 00:53:27 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1326	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	7212	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	4454	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	523323	0.40	ng/ul	0.09
16) Chrysene-d12	21.14	240	43	0.40	ng/ul	0.16
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-23.21
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	2552	0.22	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
					Ovalue	
17) Pyrene	19.30	202	184	1.597	ng/ul#	26
18) Benzo(a)anthracene	21.13	228	147	1.196	ng/ul#	1
19) Chrysene	21.13	228	147	1.161	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097205.D
Acq On : 4 Aug 2018 17:22
Operator : SJ/JU
Sample : J4206-03
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 06 00:56:01 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 00:53:27 2018
Response via : Initial Calibration




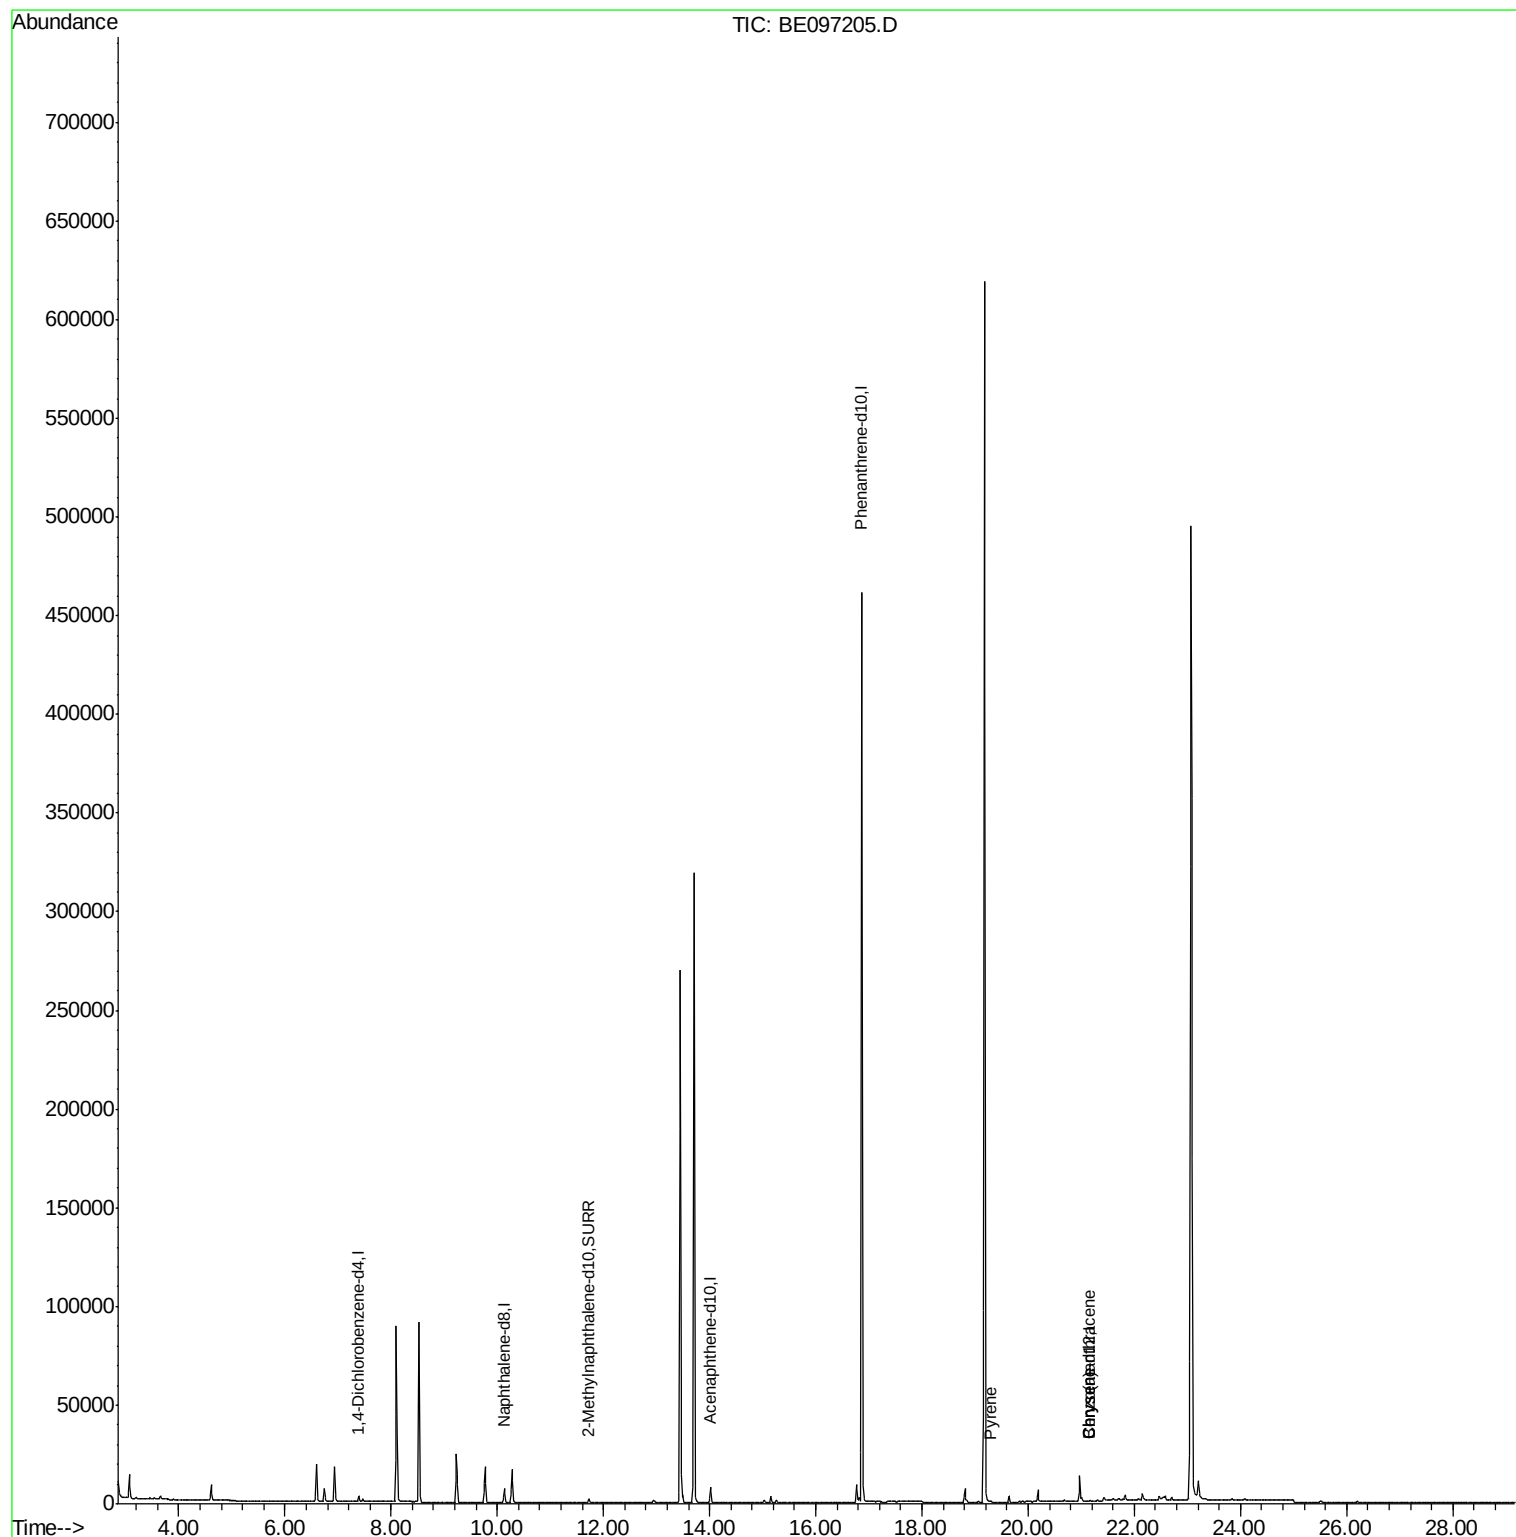


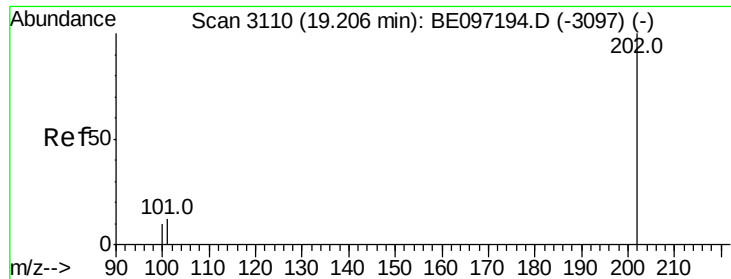

#17
Pvrene
Concen: 1.597 ng/ul
RT: 19.30 min Scan# 3136
Delta R.T. 0.10 min
Lab File: BE097205.D
Acq: 4 Aug 2018 17:22




Instrument :
BNA_E
ClientSampled :




Tot Ion:202 Resp: 184
Ion Ratio Lower Upper
202 100
101 72.6 18.2 27.4#
100 37.6 15.6 23.4#

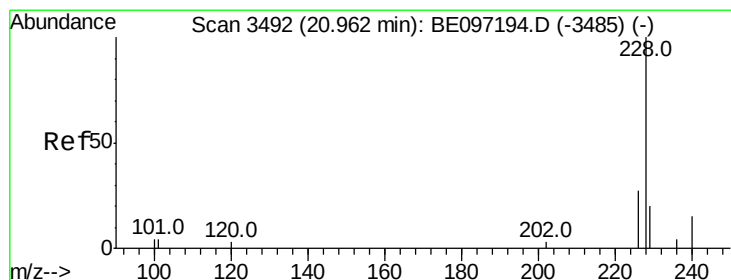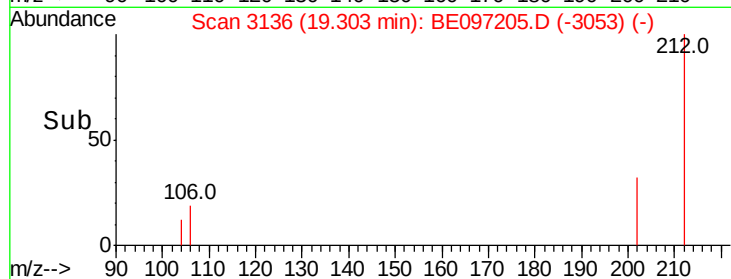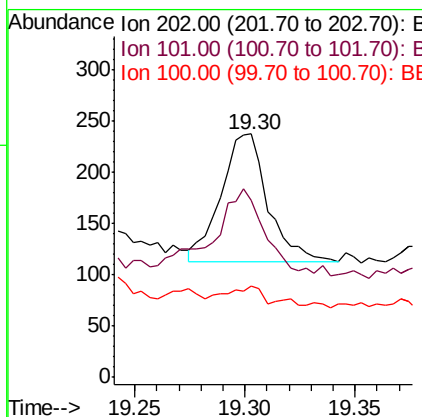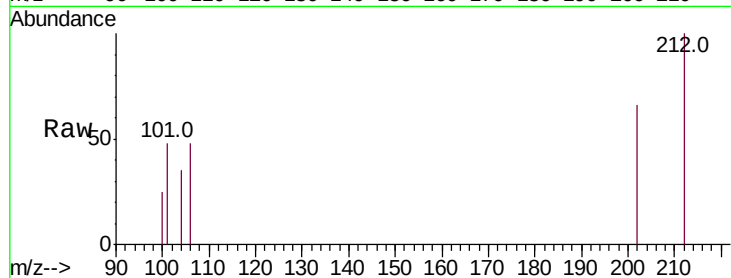

#18
Benzo(a)anthracene
Concen: 1.196 ng/ul
RT: 21.13 min Scan# 3523
Delta R.T. 0.17 min
Lab File: BE097205.D
Acq: 4 Aug 2018 17:22

Tgt Ion:228 Resp: 147
Ion Ratio Lower Upper
228 100
229 120.0 22.8 34.2#
226 93.9 17.0 25.6#

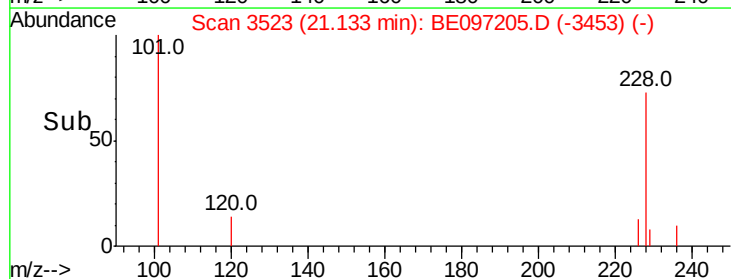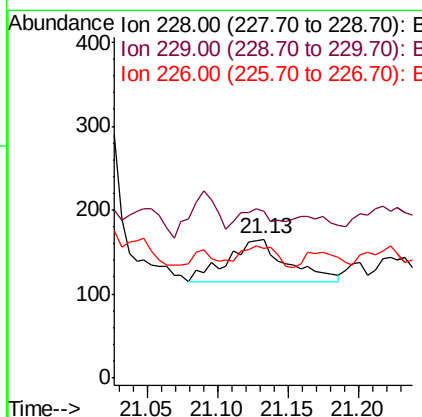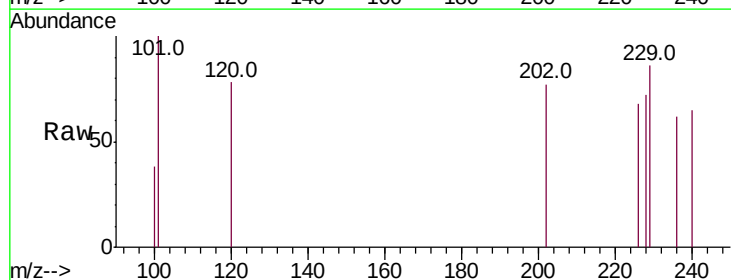

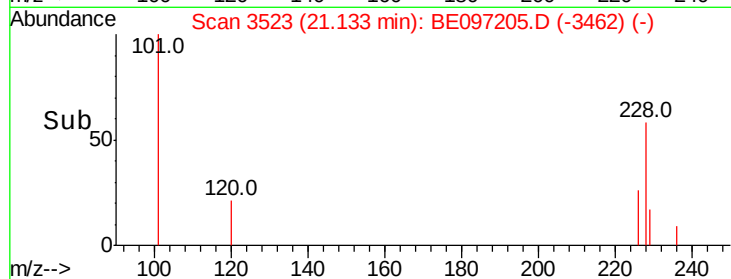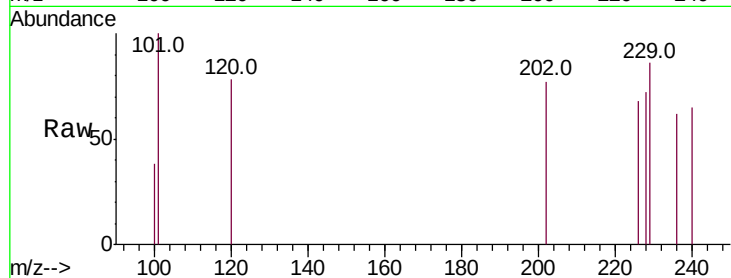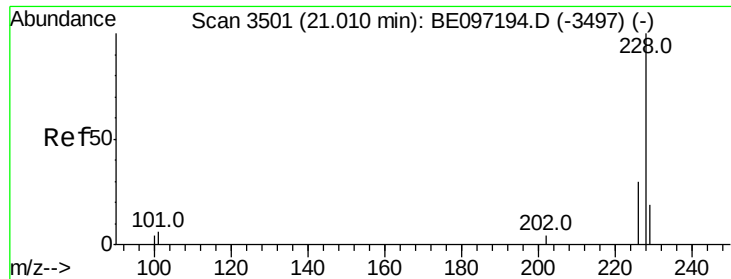

#19

Chrysene

Concen: 1.161 ng/ul

RT: 21.13 min Scan# 3523

Delta R.T. 0.12 min

Lab File: BE097205.D

Acq: 4 Aug 2018 17:22

Instrument :

BNA_E

ClientSampleId :

Tot Ion: 228 Resp: 147

Ion Ratio Lower Upper

228 100

226 93.9 23.4 35.0#

229 120.0 17.7 26.5#

