

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097211.D
 Acq On : 4 Aug 2018 21:45
 Operator : SJ/JU
 Sample : J4265-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 06 03:51:52 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1290	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6981	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	4488	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	858965	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.97
20) Perylene-d12	23.21	264	14892	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	4203	0.37	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.08	252	3488	0.086	ng/ul	Ovalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097211.D
Acq On : 4 Aug 2018 21:45
Operator : SJ/JU
Sample : J4265-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 06 03:51:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

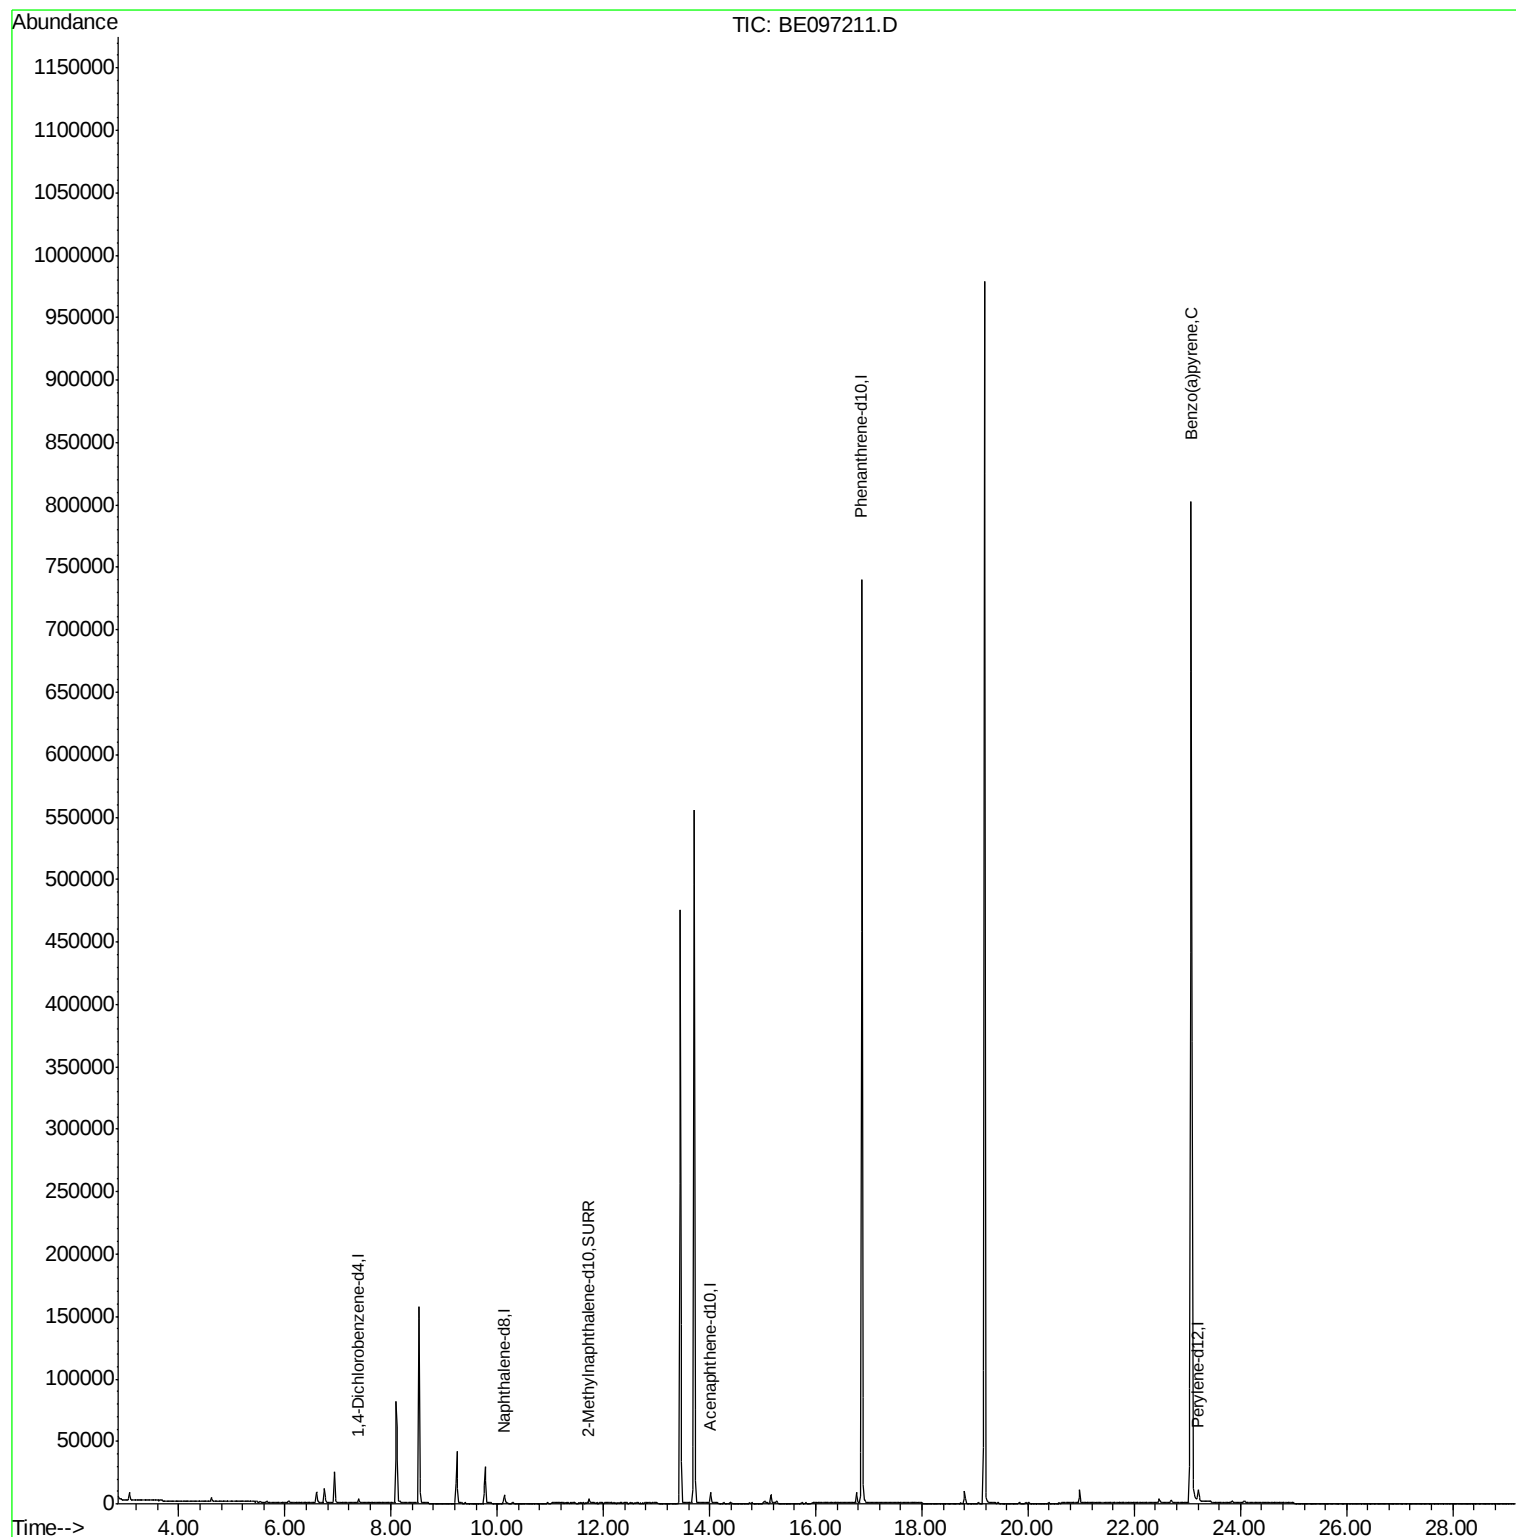

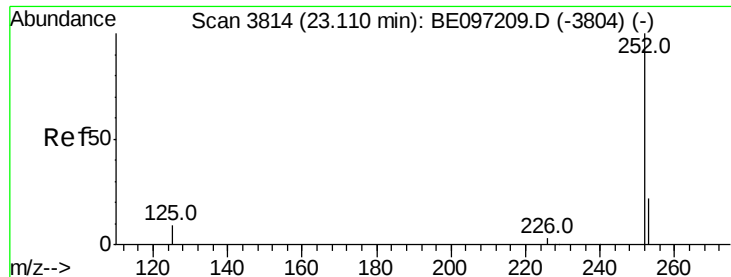

#23

Benzo(a)pyrene

Concen: 0.086 ng/ul

RT: 23.08 min Scan# 3810

Delta R.T. -0.04 min

Lab File: BE097211.D

Acq: 4 Aug 2018 21:45

Instrument :

BNA_E

ClientSampleId :


Tot Ion: 252 Resp: 3488

Ion Ratio Lower Upper

252 100

253 35.7 28.5 42.7

125 23.0 18.1 27.1

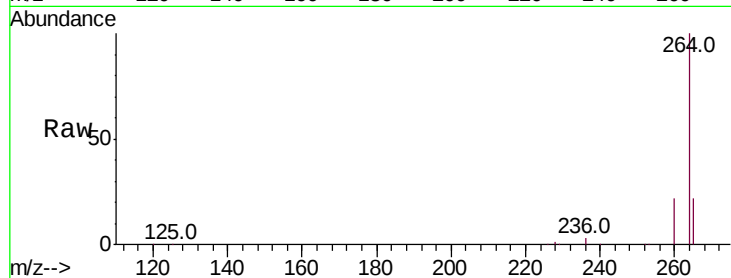

Abundance Ion 252.00 (251.70 to 252.70): E
Ion 253.00 (252.70 to 253.70): E
Ion 125.00 (124.70 to 125.70): E

