

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097214.D
 Acq On : 4 Aug 2018 23:38
 Operator : SJ/JU
 Sample : J4265-10
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 06 03:52:06 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1551	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	8199	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	5368	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	982485	0.40	ng/ul	0.11
16) Chrysene-d12	21.10	240	31	0.40	ng/ul	0.13
20) Perylene-d12	0.00	264	0	0.00	ng/ul	-23.21
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.72	152	4930	0.37	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
					Ovalue	
17) Pyrene	19.44	202	122	1.469	ng/ul#	37
18) Benzo(a)anthracene	21.10	228	22	0.248	ng/ul#	1
19) Chrysene	21.13	228	15	0.164	ng/ul#	1


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097214.D
Acq On : 4 Aug 2018 23:38
Operator : SJ/JU
Sample : J4265-10
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 06 03:52:06 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration




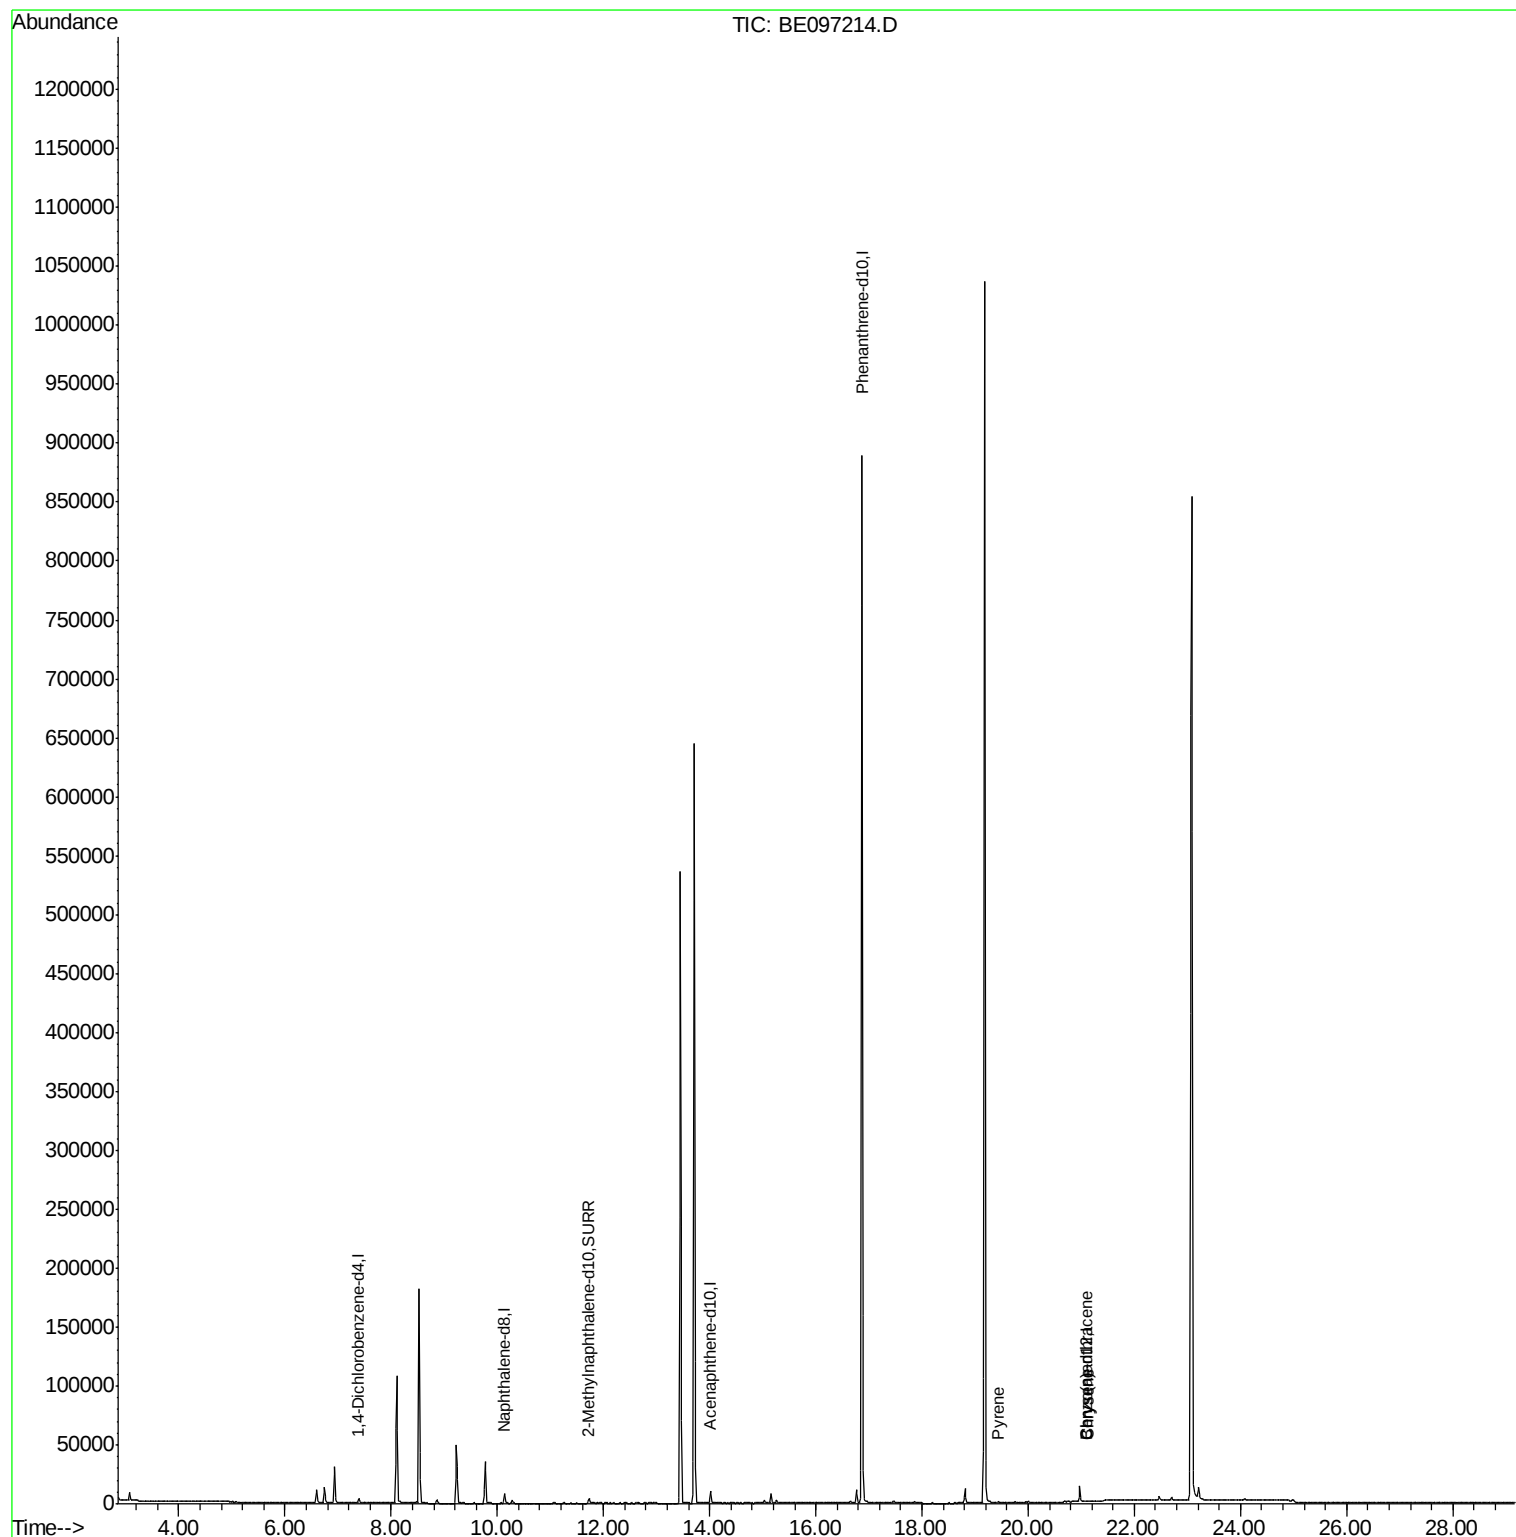


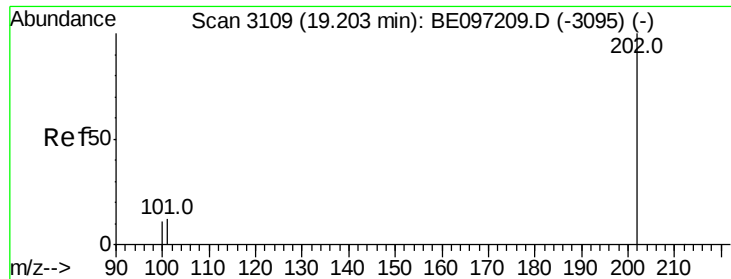

#17
Pvrene
Concen: 1.469 ng/ul
RT: 19.44 min Scan# 3175
Delta R.T. 0.23 min
Lab File: BE097214.D
Acq: 4 Aug 2018 23:38




Instrument :
BNA_E
ClientSampled :


Tot Ion:202 Resp: 122
Ion Ratio Lower Upper
202 100
101 58.5 18.2 27.4#
100 42.4 15.6 23.4#

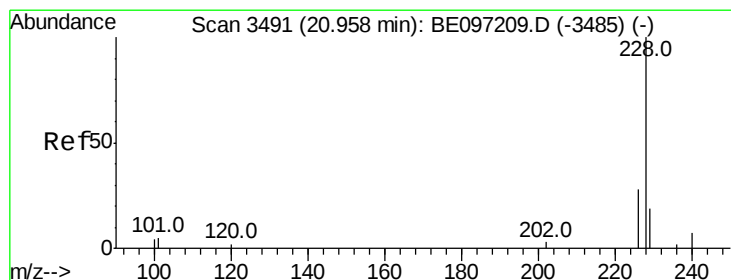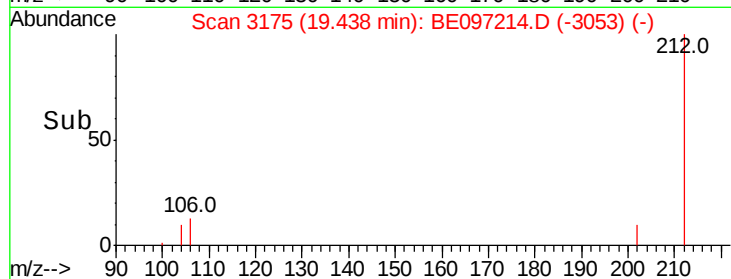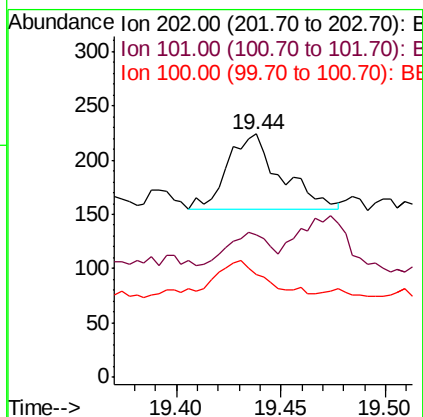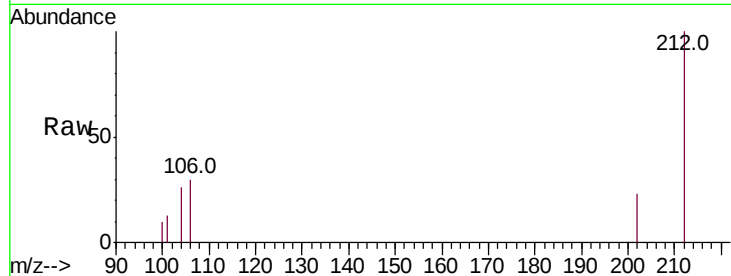

#18
Benzo(a)anthracene
Concen: 0.248 ng/ul
RT: 21.10 min Scan# 3518
Delta R.T. 0.14 min
Lab File: BE097214.D
Acq: 4 Aug 2018 23:38

Tgt Ion:228 Resp: 22
Ion Ratio Lower Upper
228 100
229 136.8 22.8 34.2#
226 100.9 17.0 25.6#

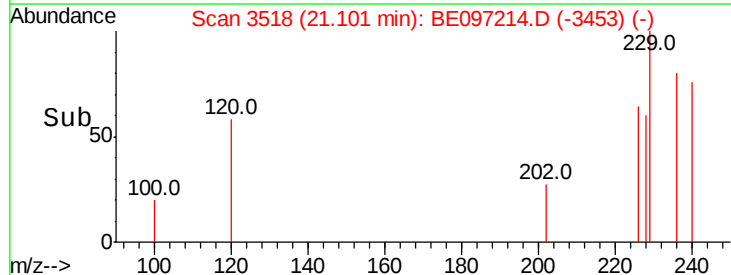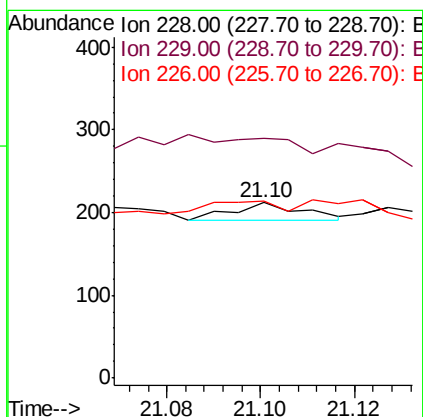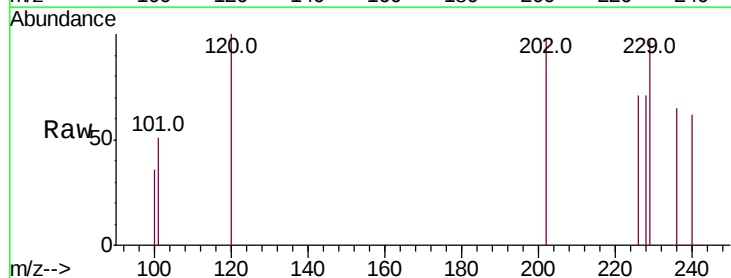

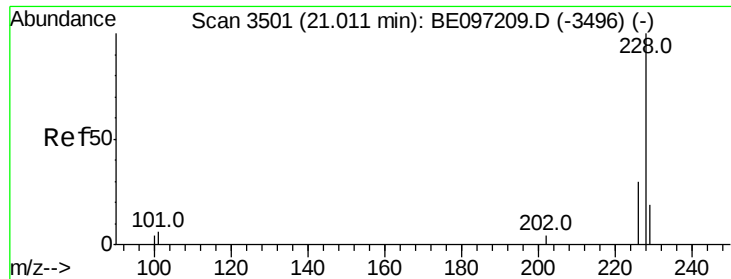

#19

Chrysene

Concen: 0.164 ng/ul

RT: 21.13 min Scan# 3523

Delta R.T. 0.12 min


Lab File: BE097214.D

Acq: 4 Aug 2018 23:38

Instrument :

BNA_E

ClientSampleId :

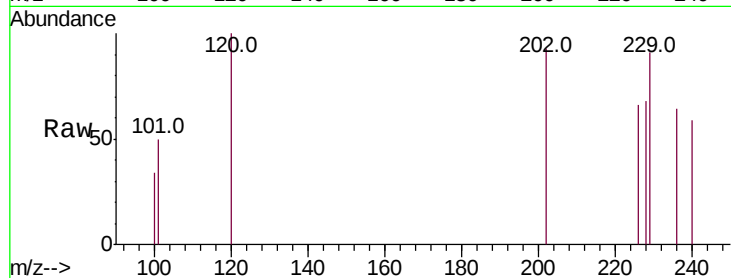

Tot Ion:	228	Resp:	15
Ion	Ratio	Lower	Upper
228	100		
226	97.1	23.4	35.0#
229	133.0	17.7	26.5#

