

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097210.D
 Acq On : 4 Aug 2018 21:06
 Operator : SJ/JU
 Sample : J4206-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L0

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:50:57 PM

Quant Time: Aug 06 03:59:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

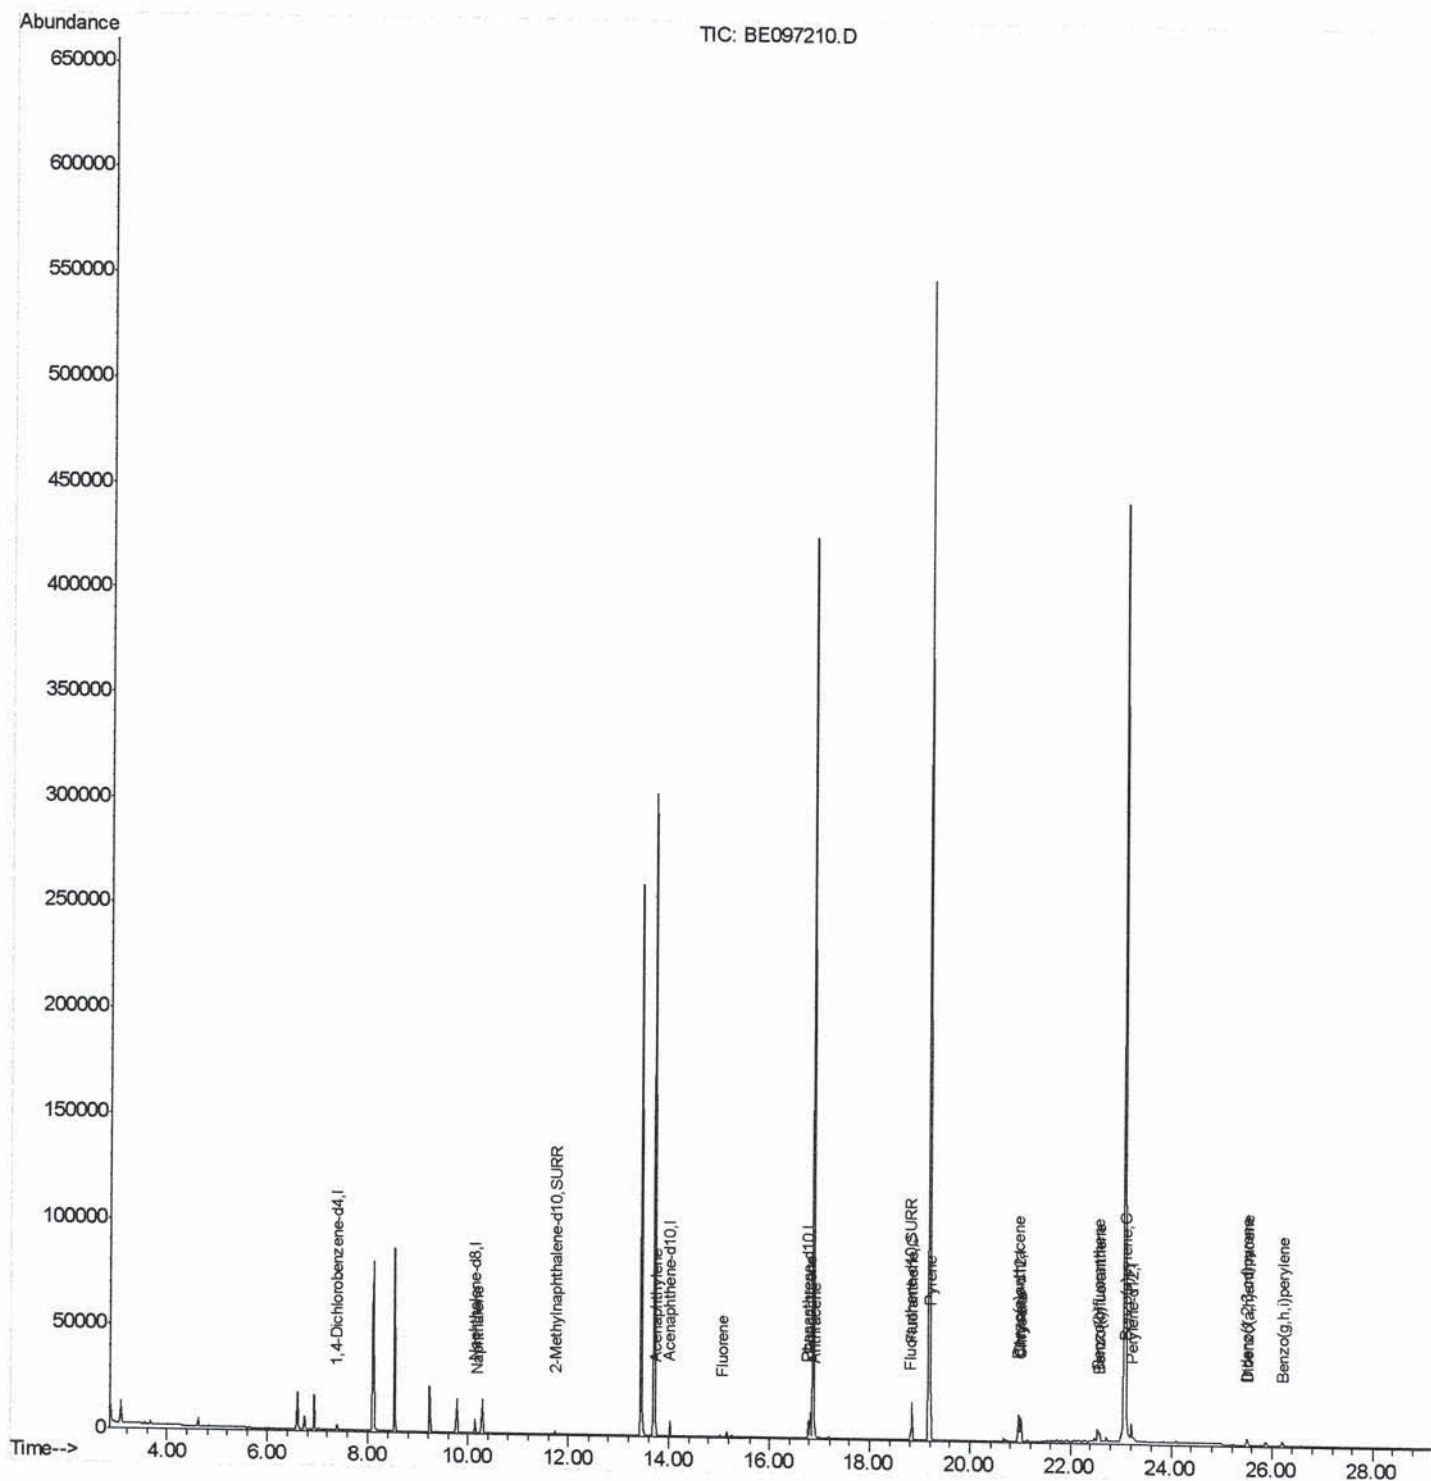

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097210.D
 Acq On : 4 Aug 2018 21:06
 Operator : SJ/JU
 Sample : J4206-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L0

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:50:57 PM

Quant Time: Aug 06 03:46:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

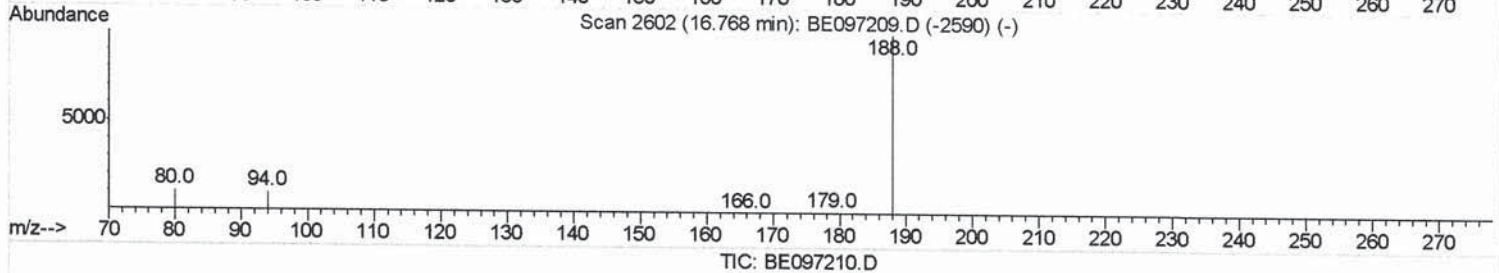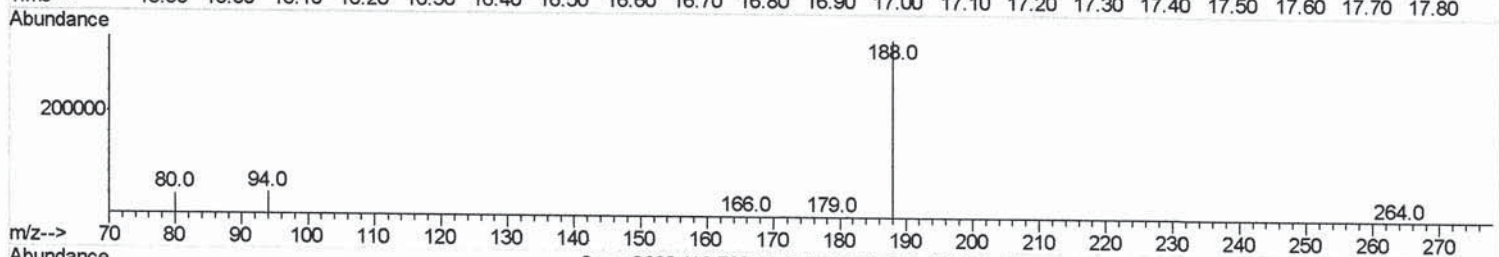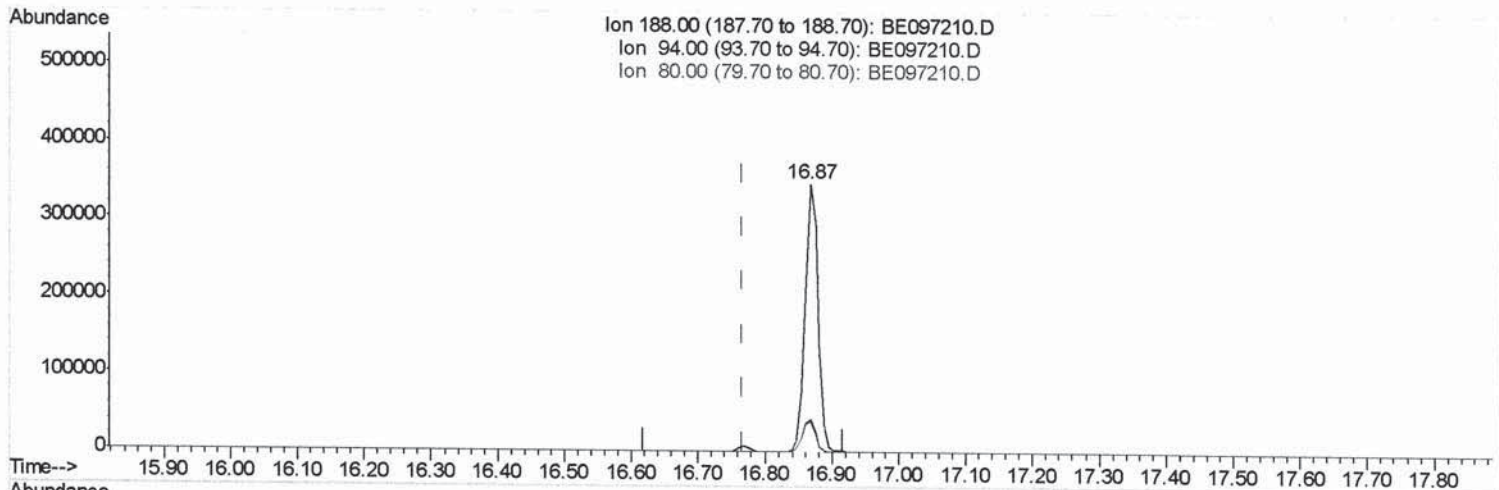

TIC: BE097210.D

(10) Phenanthrene-d10 (I)
 16.867min (+0.099) 0.40ng/ul
 response 469258

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	12.13
80.00	11.80	11.23
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097210.D
Acq On : 4 Aug 2018 21:06
Operator : SJ/JU
Sample : J4206-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1L0

Manual Integrations
APPROVED

Sohil
8/6/2018 12:50:57 PM

Quant Time: Aug 06 03:46:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

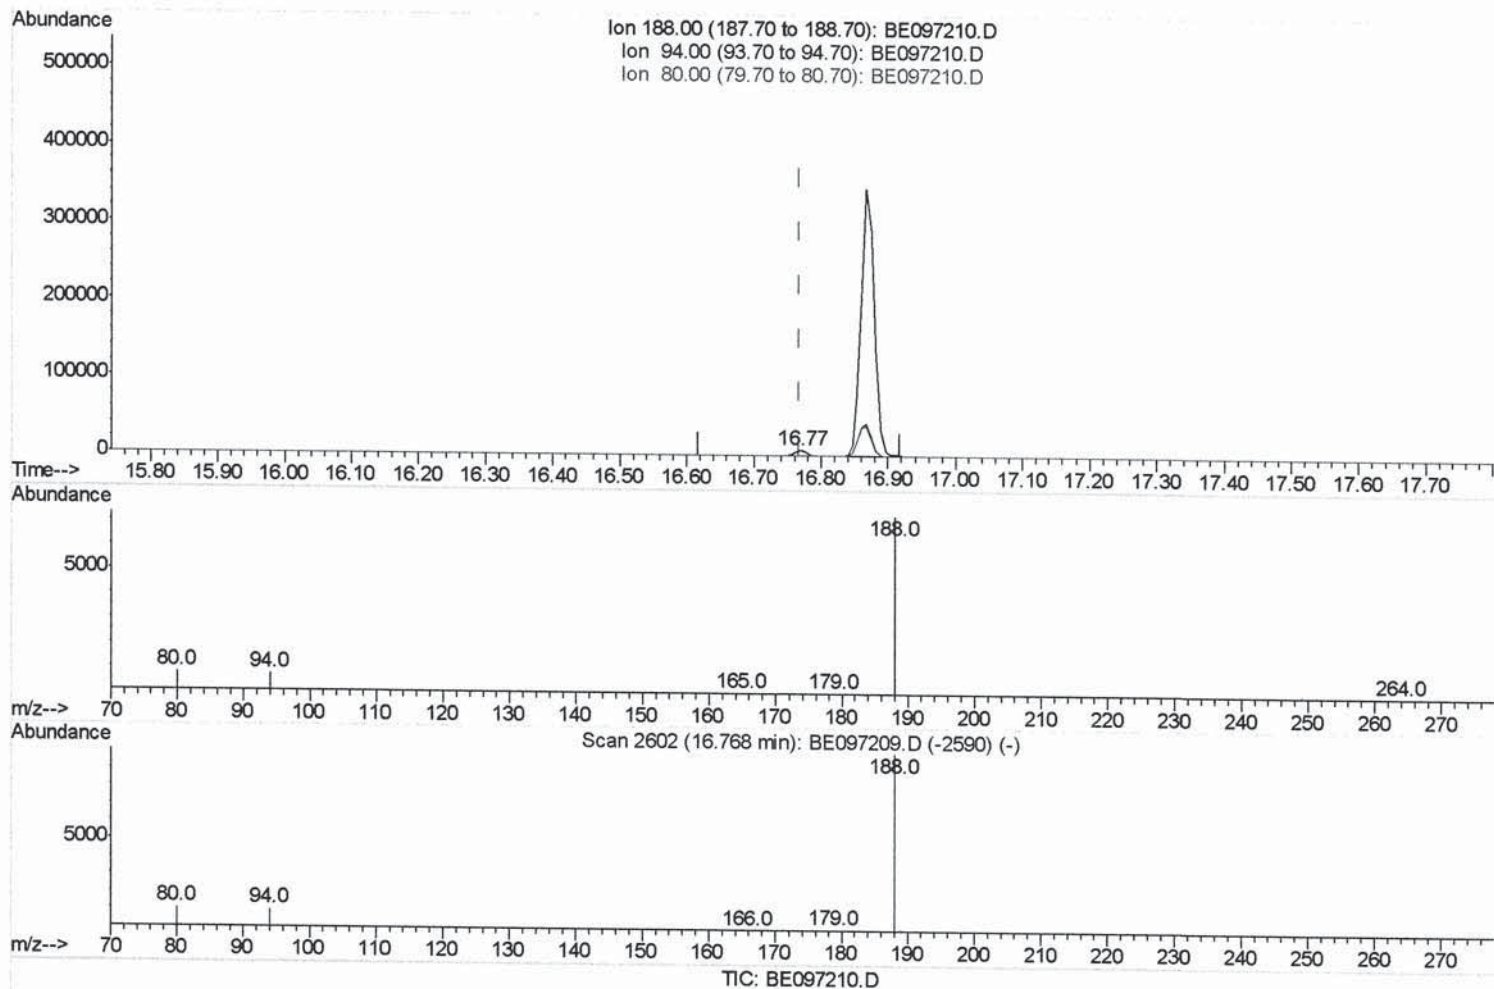

(10) Phenanthrene-d10 (I)

16.769min (+0.001) 0.40ng/ul m

SJ 8/7/18

response 9861

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.94
80.00	11.80	10.73
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097210.D
Acq On : 4 Aug 2018 21:06
Operator : SJ/JU
Sample : J4206-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1LO

Manual Integrations
APPROVED

Sohil
8/6/2018 12:50:57 PM

Quant Time: Aug 06 03:54:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

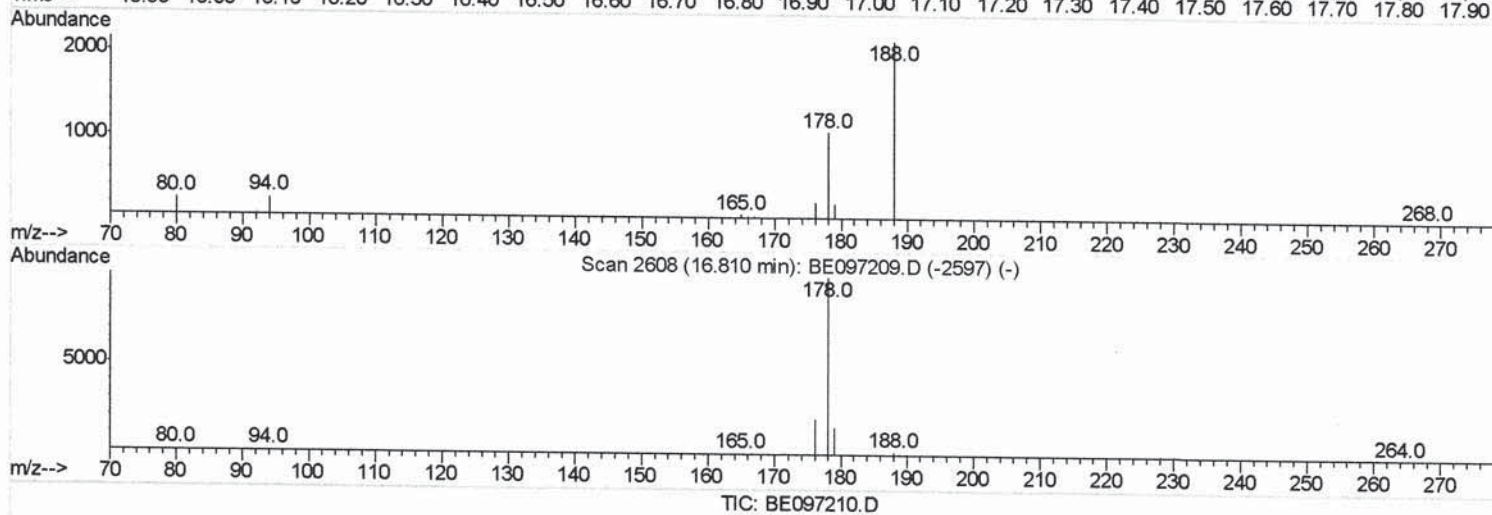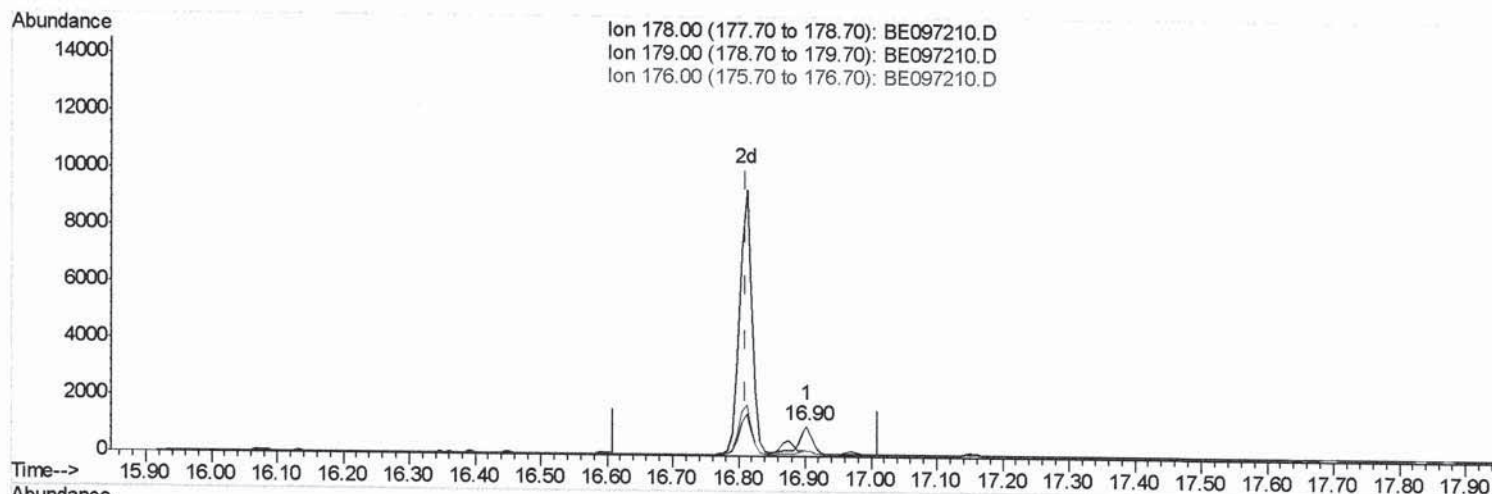

(12) Phenanthrene

16.903min (+0.092) 0.06ng/ul

response 1582

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	20.71
176.00	17.00	21.37#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097210.D
 Acq On : 4 Aug 2018 21:06
 Operator : SJ/JU
 Sample : J4206-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L0

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:50:57 PM

Quant Time: Aug 06 03:54:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

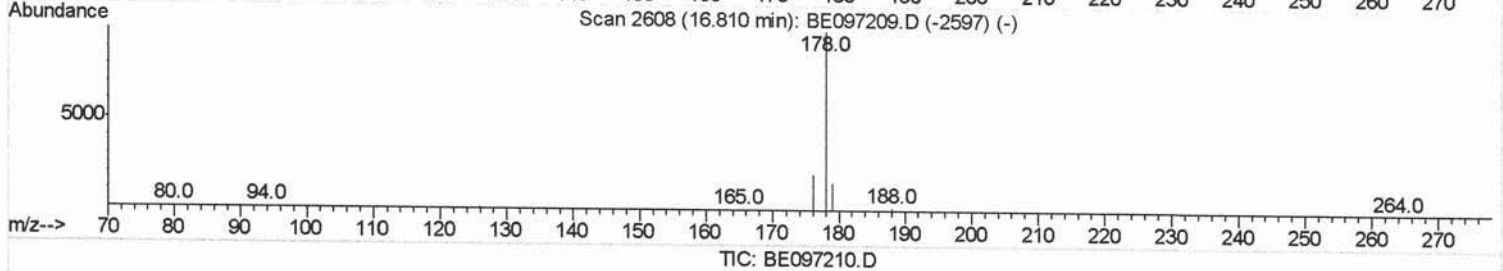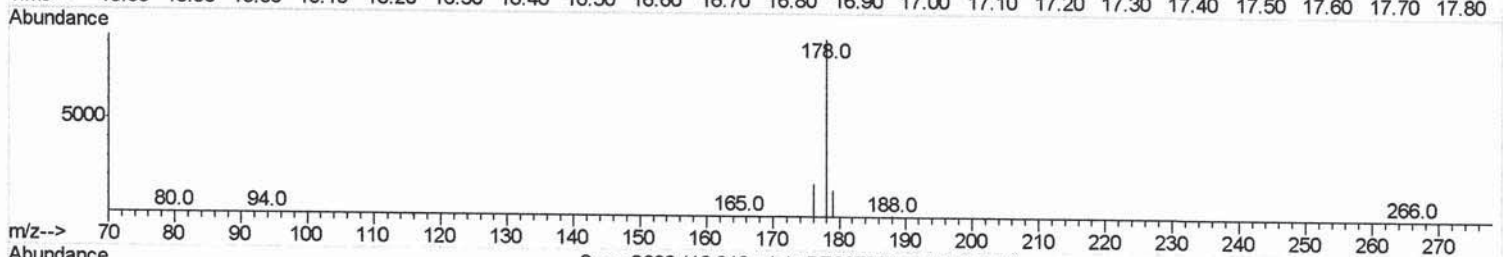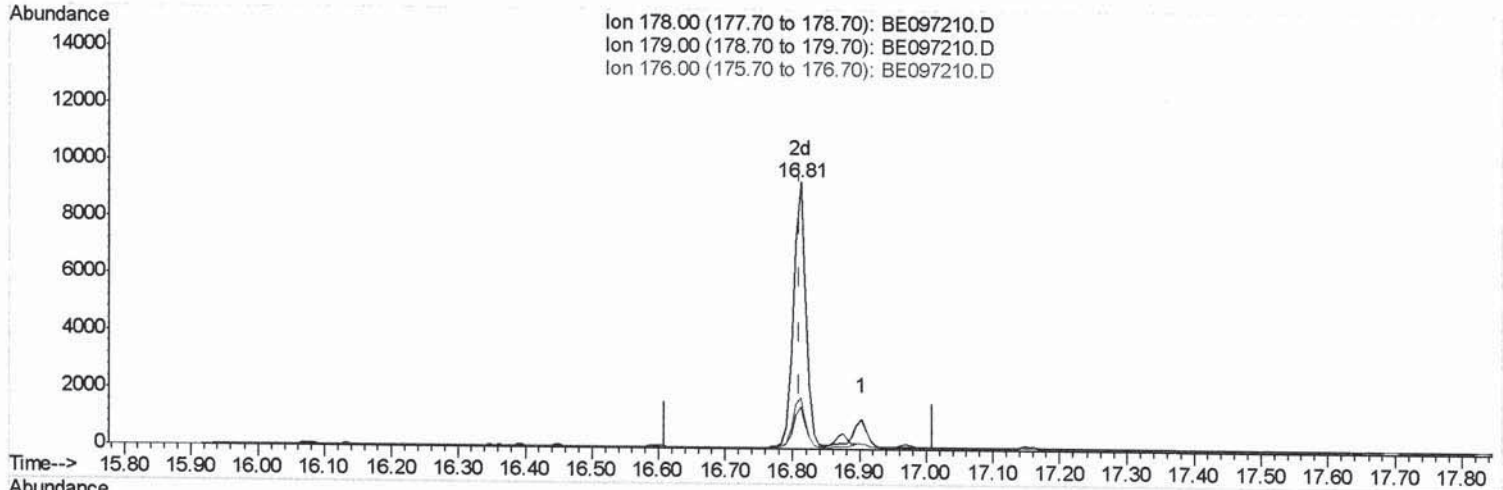

(12) Phenanthrene

16.811min (+0.001) 0.49ng/ul m

SJ 8/7/18

response 12416

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	15.71#
176.00	17.00	19.19
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097210.D
 Acq On : 4 Aug 2018 21:06
 Operator : SJ/JU
 Sample : J4206-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L0

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:50:57 PM

Quant Time: Aug 06 03:54:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

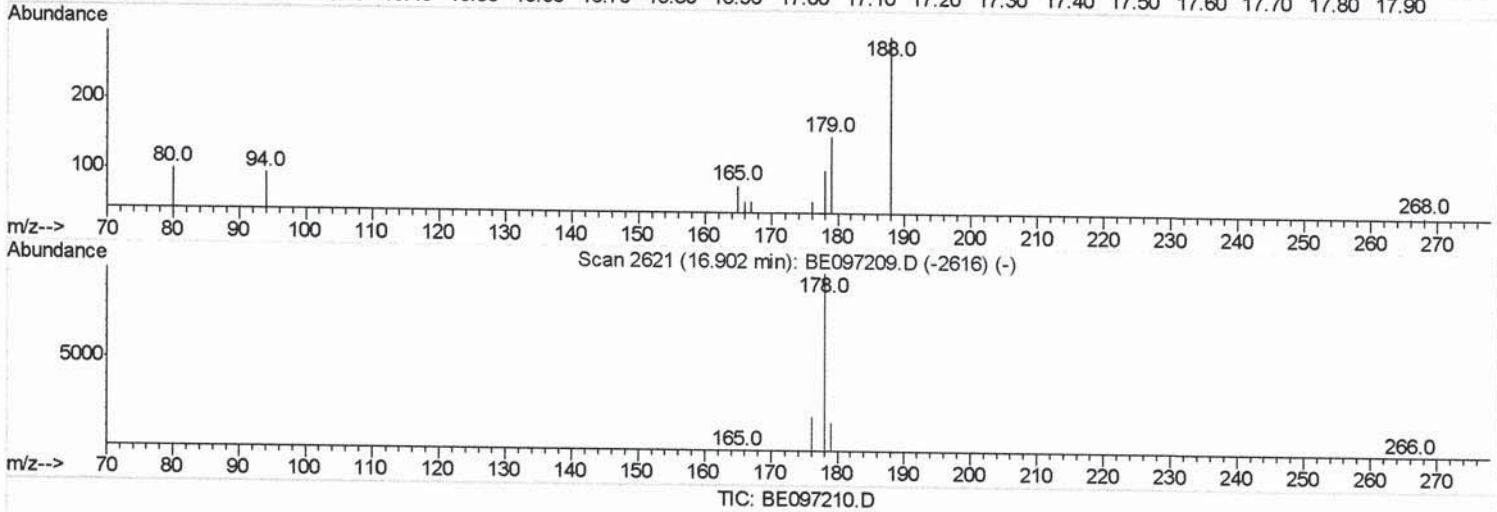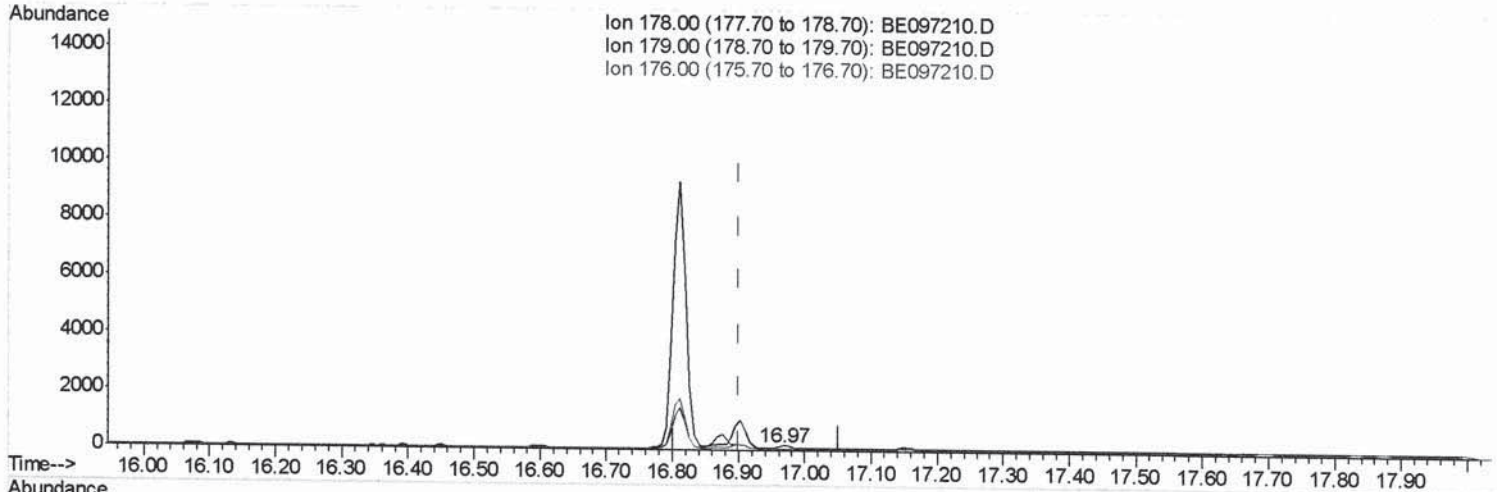

(13) Anthracene

16.966min (+0.064) 0.00ng/ul

response 59

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	146.15#
176.00	18.40	56.73#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097210.D
Acq On : 4 Aug 2018 21:06
Operator : SJ/JU
Sample : J4206-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1LO

Manual Integrations
APPROVED

Sohil
8/6/2018 12:50:57 PM

Quant Time: Aug 06 03:54:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

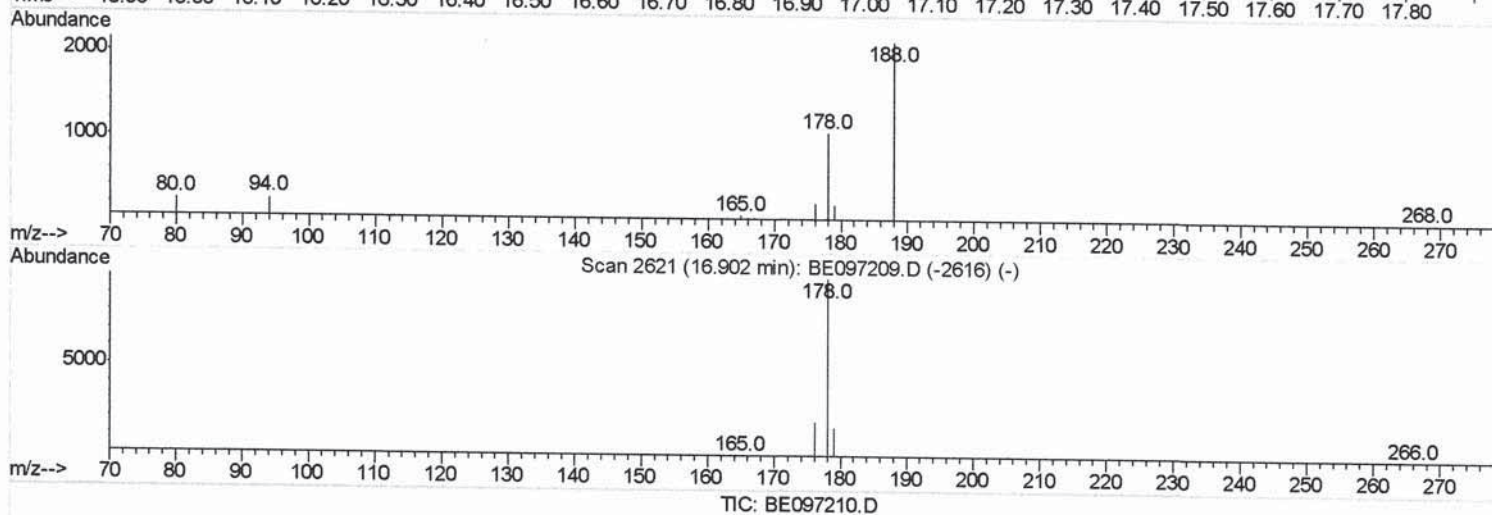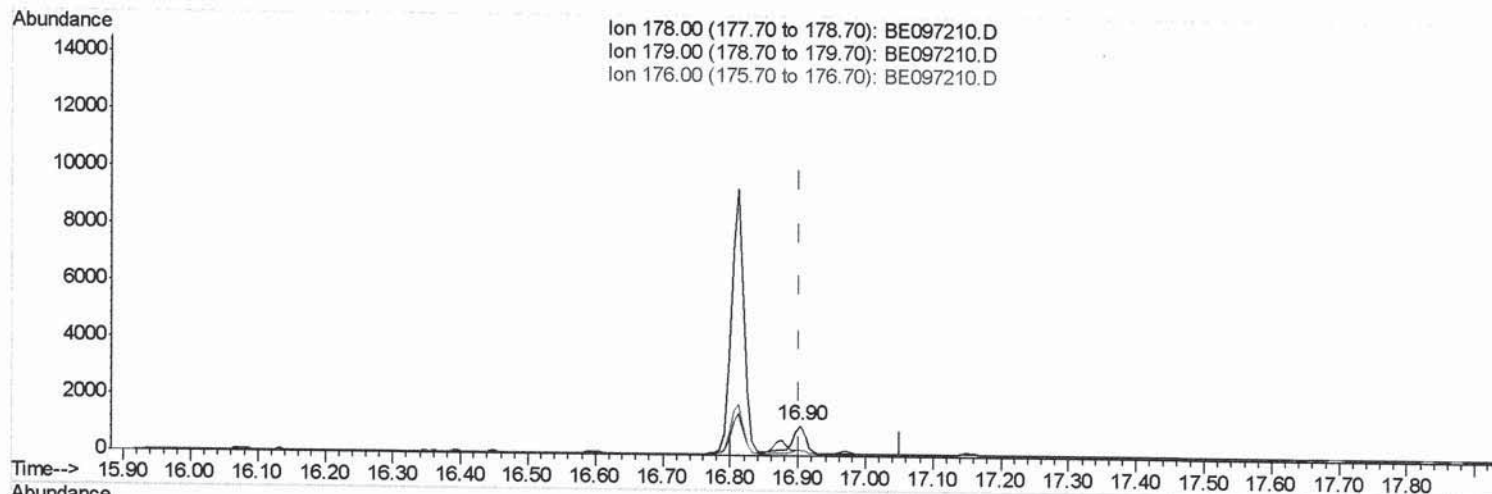

(13) Anthracene

16.903min (+0.001) 0.05ng/ul m

response 1266

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	20.71
176.00	18.40	21.37
0.00	0.00	0.00

SJ 8/7/18

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097210.D
 Acq On : 4 Aug 2018 21:06
 Operator : SJ/JU
 Sample : J4206-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L0

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:50:57 PM

Quant Time: Aug 06 03:54:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

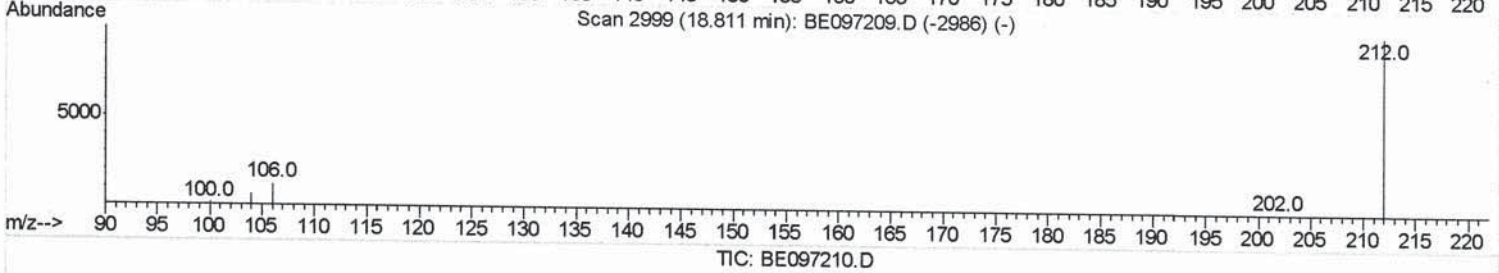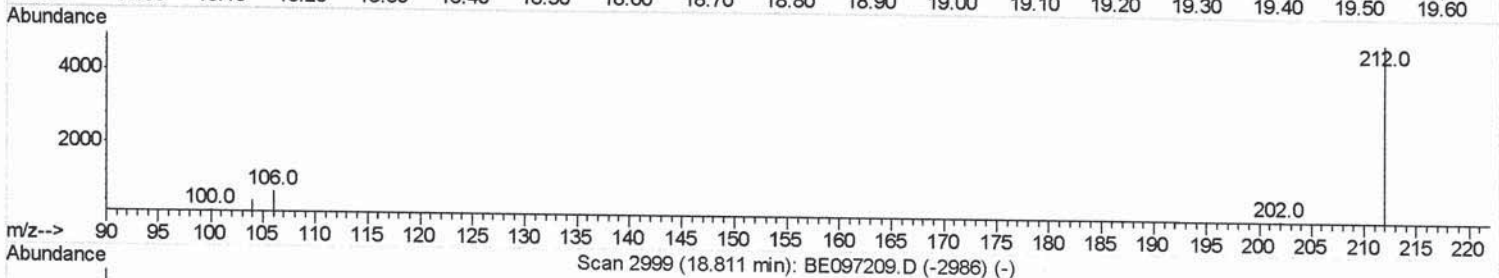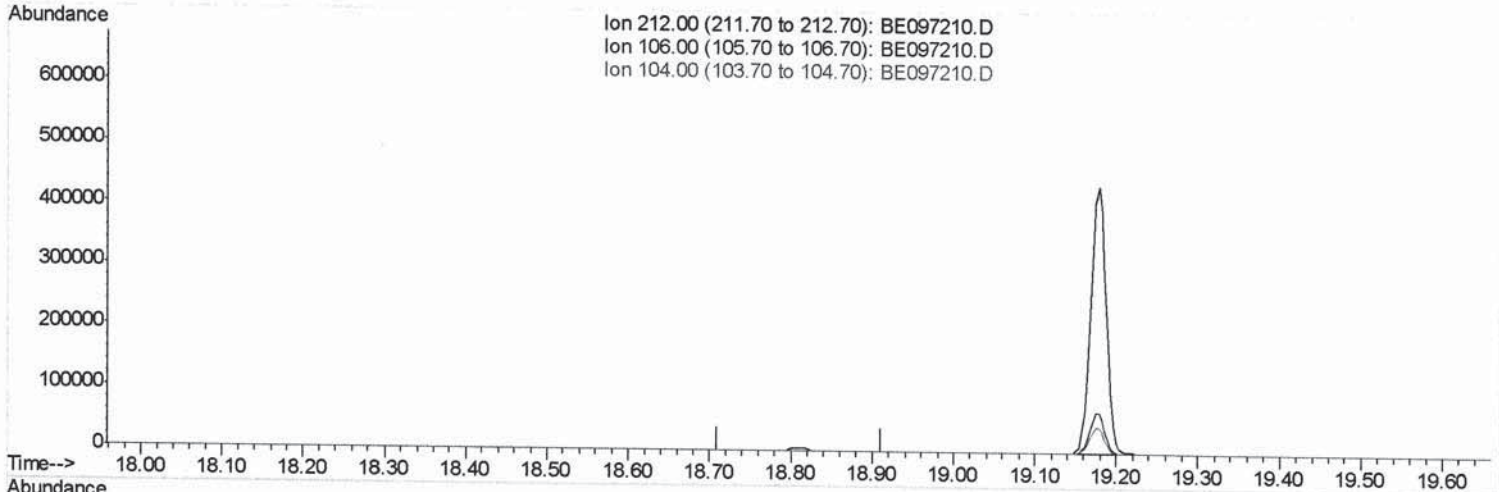

(14) Fluoranthene-d10 (SURR)

18.811min (-18.811) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097210.D
 Acq On : 4 Aug 2018 21:06
 Operator : SJ/JU
 Sample : J4206-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L0

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:50:57 PM

Quant Time: Aug 06 03:54:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

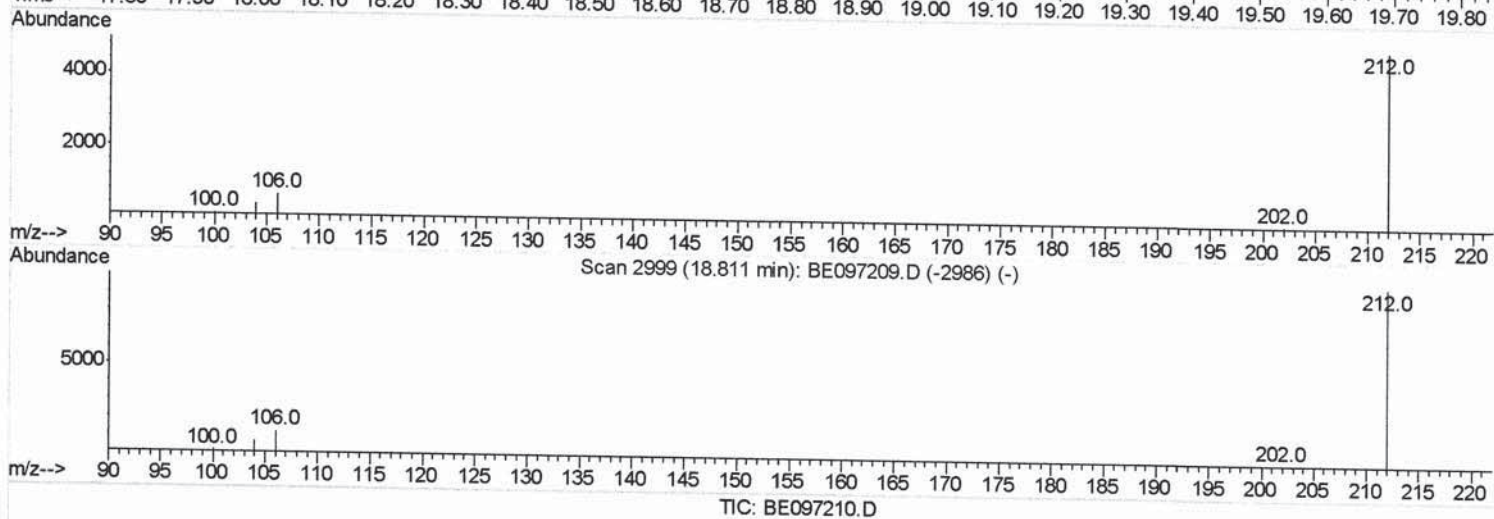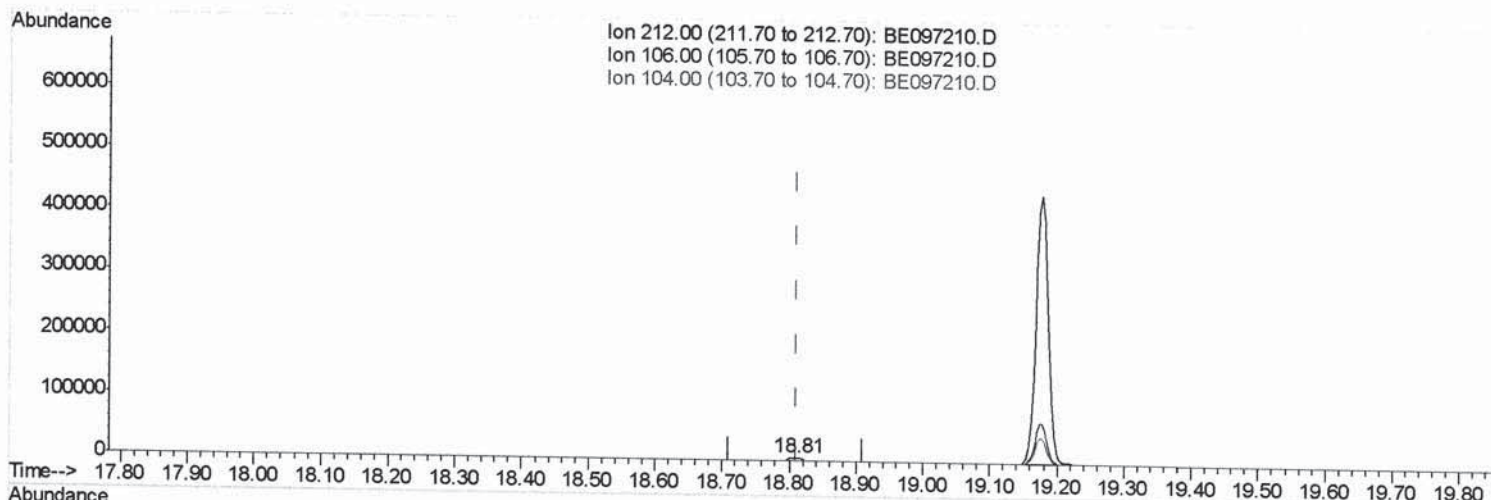

(14) Fluoranthene-d10 (SURR)

18.811min (-0.000) 0.20ng/ul m

response 6885

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

SJ 8/7/18

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097210.D
 Acq On : 4 Aug 2018 21:06
 Operator : SJ/JU
 Sample : J4206-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L0

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:50:57 PM

Quant Time: Aug 06 03:54:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

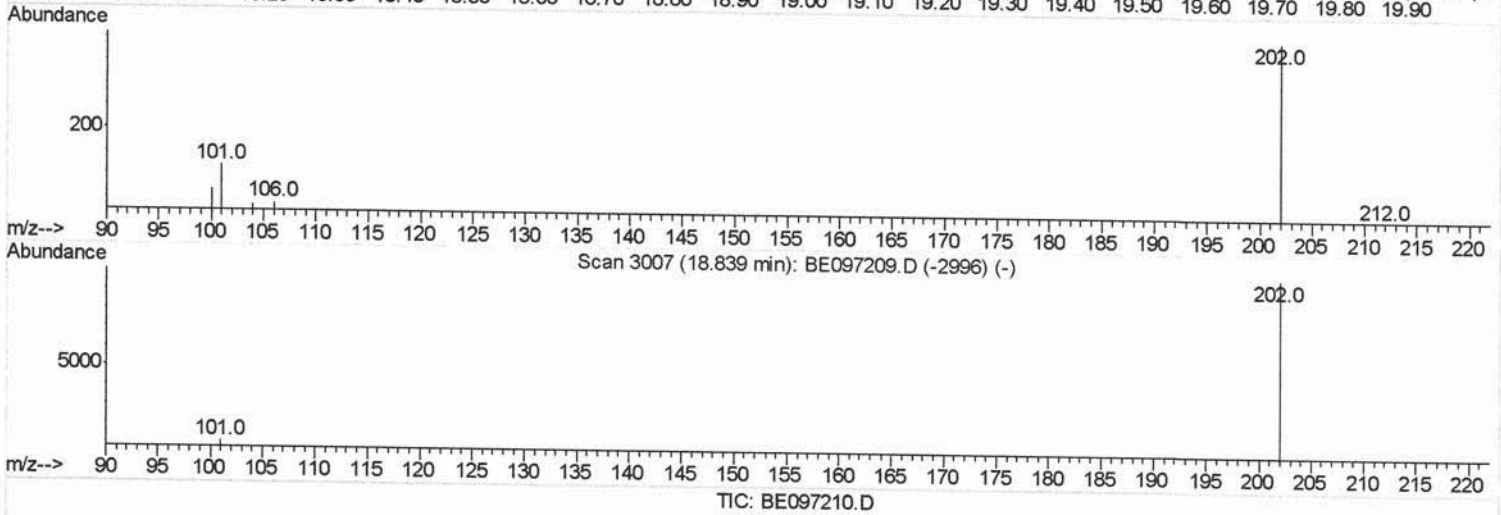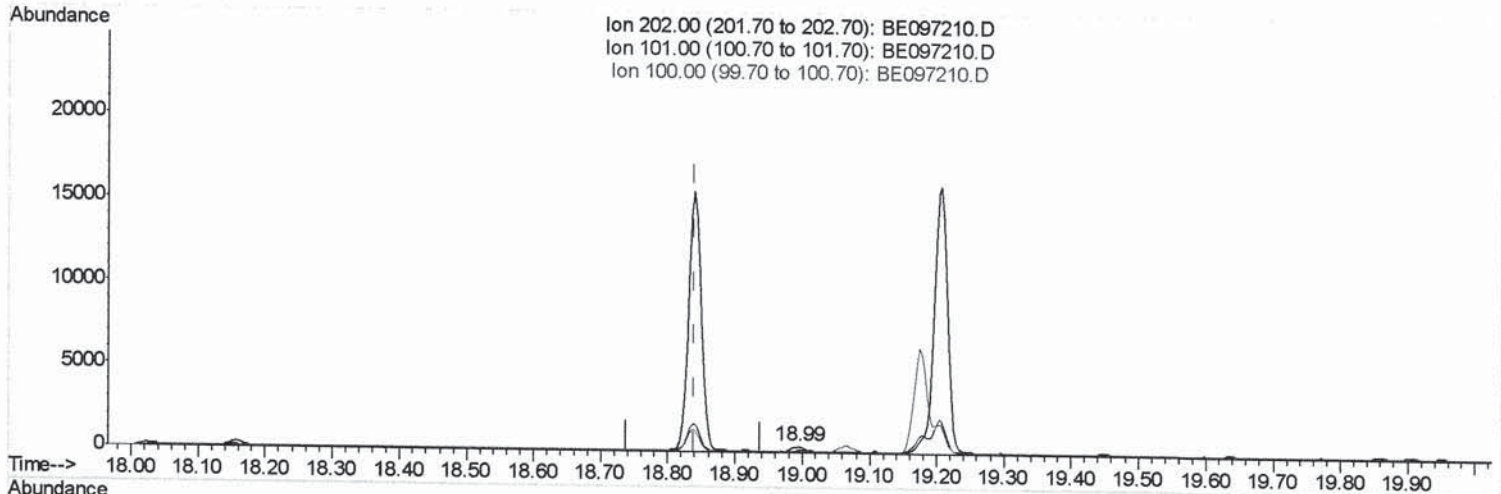

(15) Fluoranthene (C)

18.993min (+0.153) 0.01ng/ul

response 354

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	36.59#
100.00	19.50	25.20
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097210.D
 Acq On : 4 Aug 2018 21:06
 Operator : SJ/JU
 Sample : J4206-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L0

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:50:57 PM

Quant Time: Aug 06 03:54:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

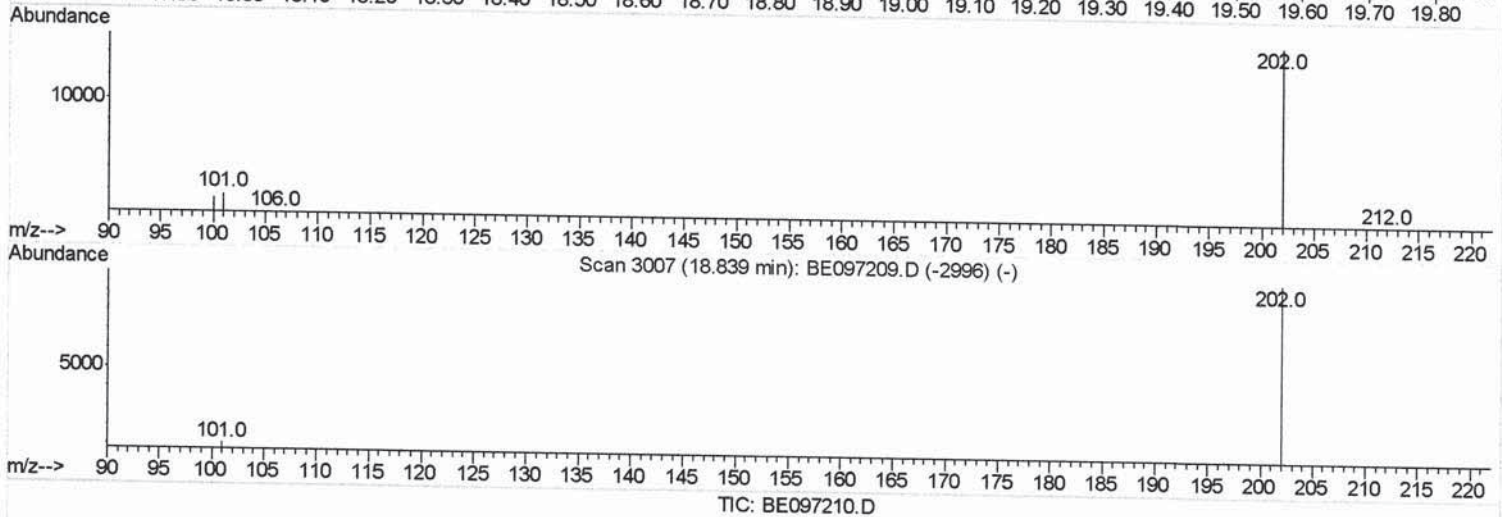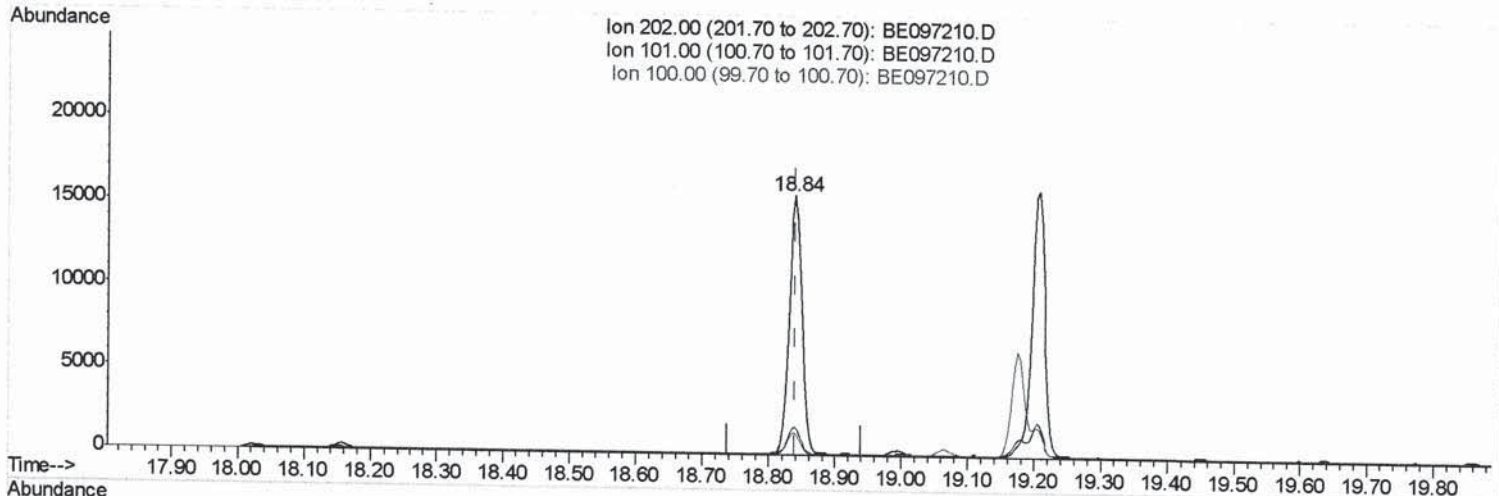

(15) Fluoranthene (C)

18.839min (-0.000) 0.61ng/ul m

SJ 8/7/18

response 20114

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	10.94
100.00	19.50	8.58
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097210.D
 Acq On : 4 Aug 2018 21:06
 Operator : SJ/JU
 Sample : J4206-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L0

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:50:57 PM

Quant Time: Aug 06 03:54:32 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

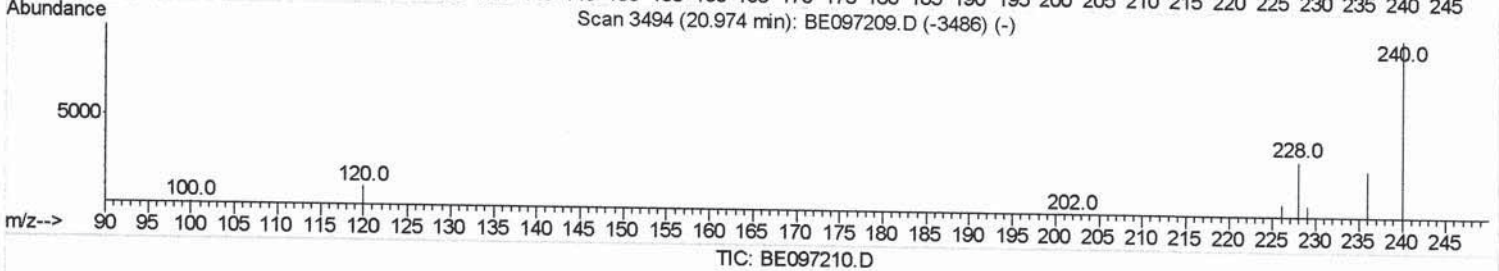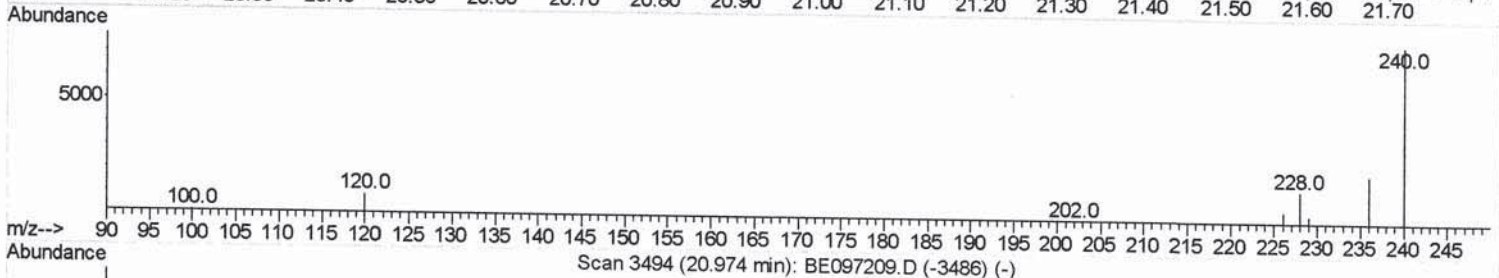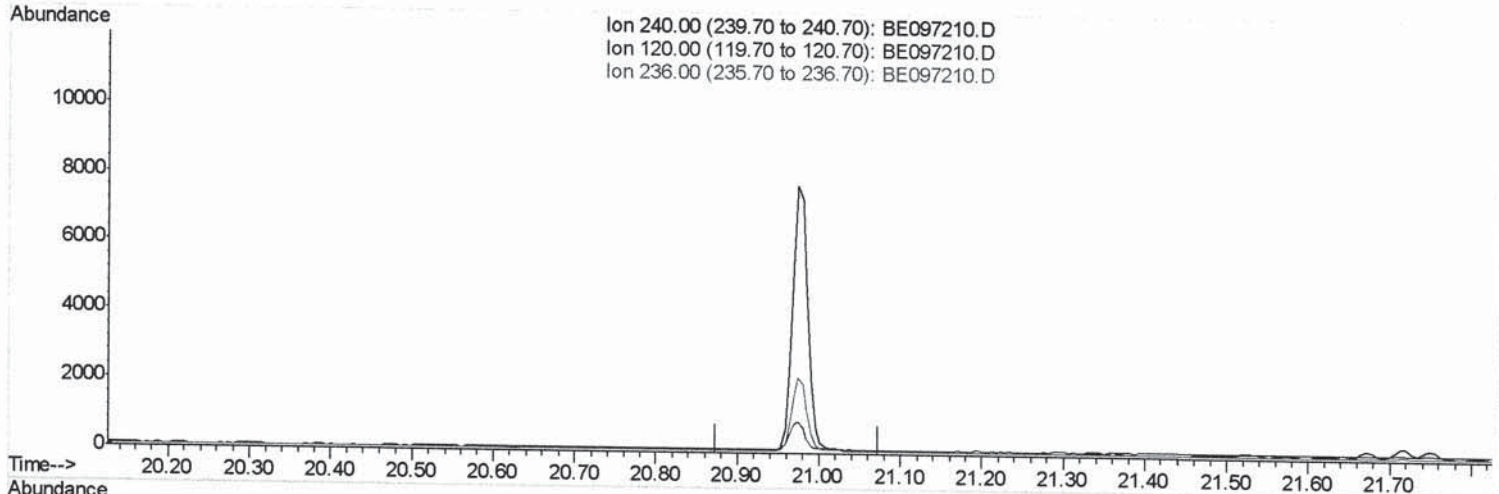

(16) Chrysene-d12 (I)

20.974min (-20.974) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.60	0.00#
236.00	34.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097210.D
Acq On : 4 Aug 2018 21:06
Operator : SJ/JU
Sample : J4206-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1L0

Manual Integrations
APPROVED

Sohil
8/6/2018 12:50:57 PM

Quant Time: Aug 06 03:54:32 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

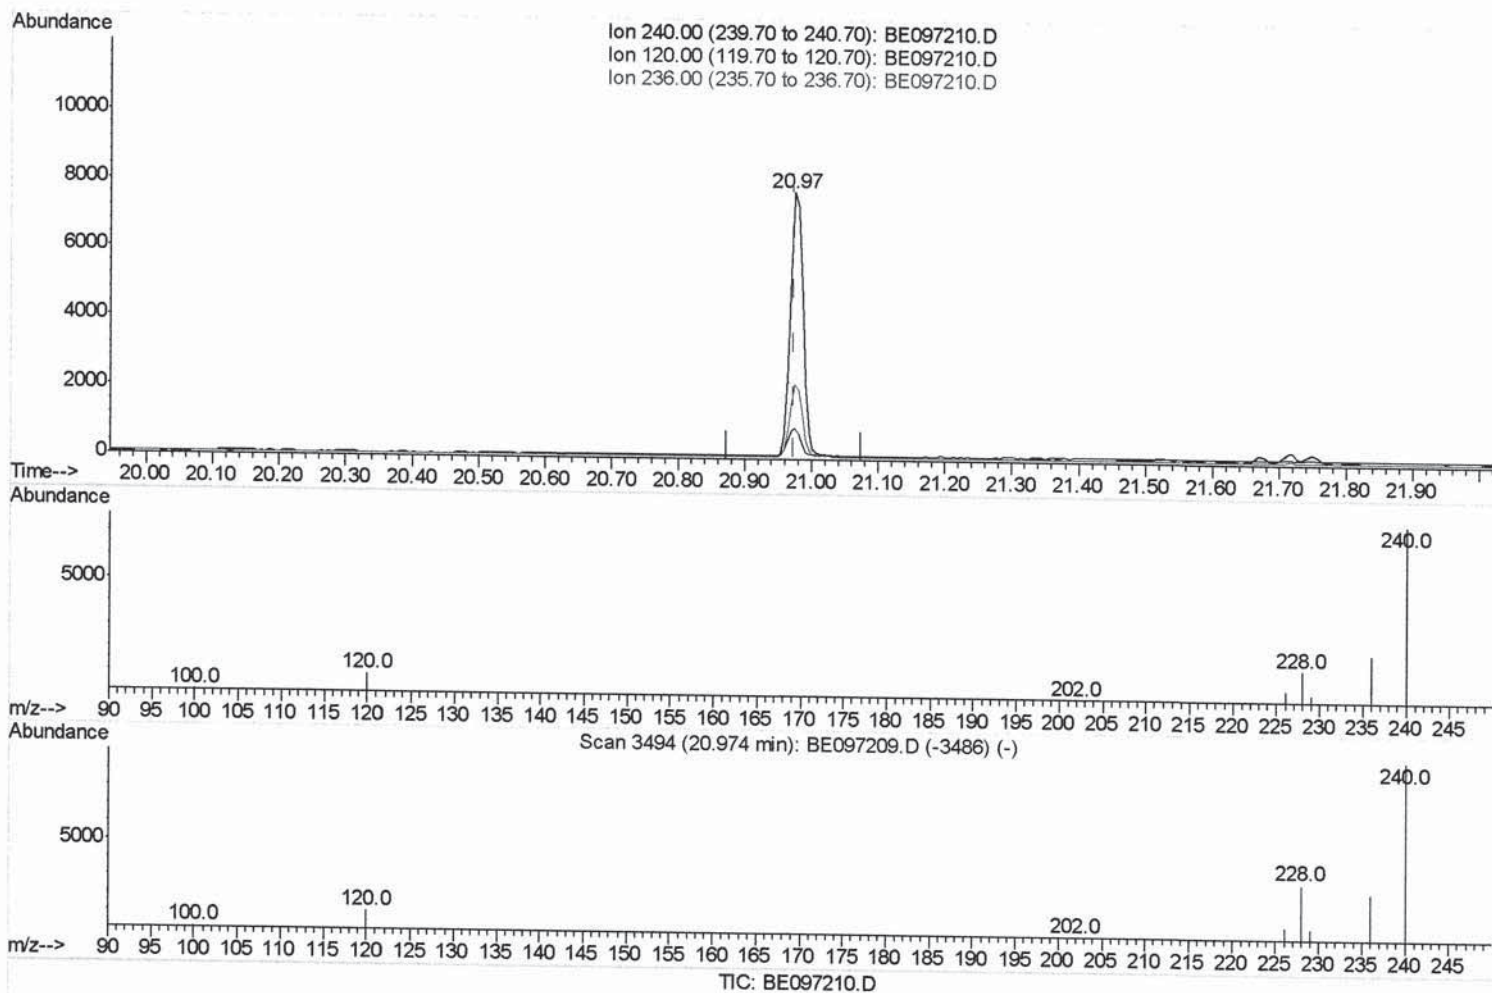

(16) Chrysene-d12 (I)

20.974min (-0.000) 0.40ng/ul m

response 10060

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	11.83#
236.00	34.90	28.36
0.00	0.00	0.00

SJ 8/7/18

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097210.D
 Acq On : 4 Aug 2018 21:06
 Operator : SJ/JU
 Sample : J4206-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L0

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:50:57 PM

Quant Time: Aug 06 03:57:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

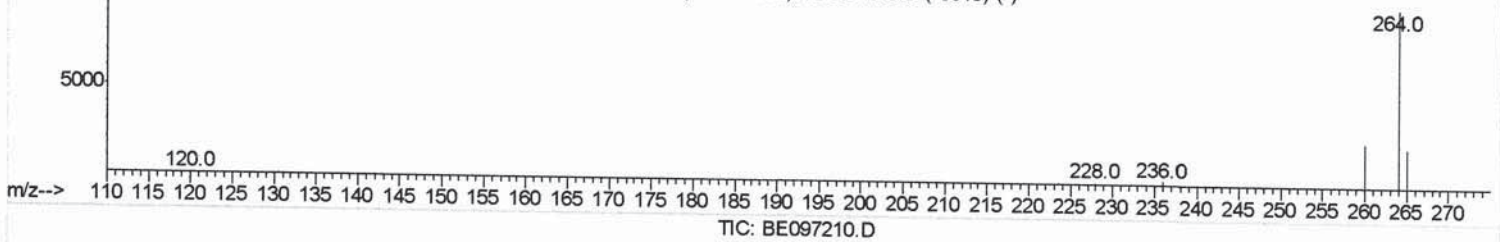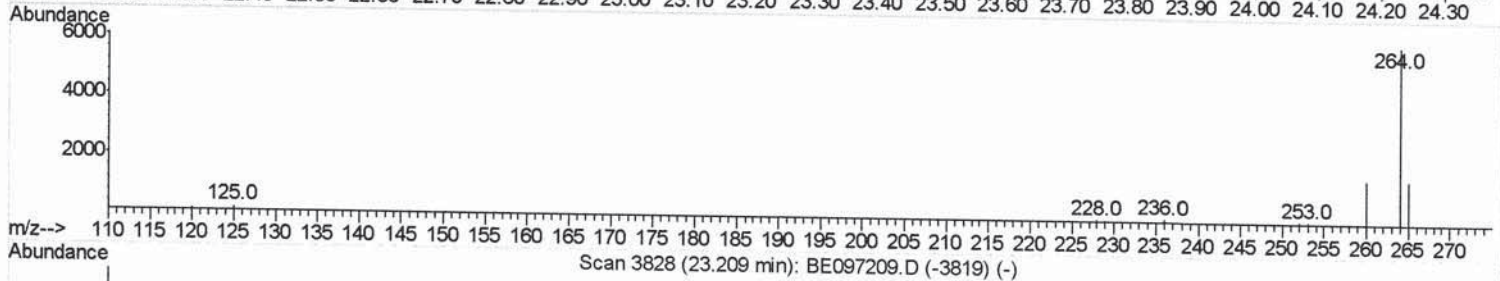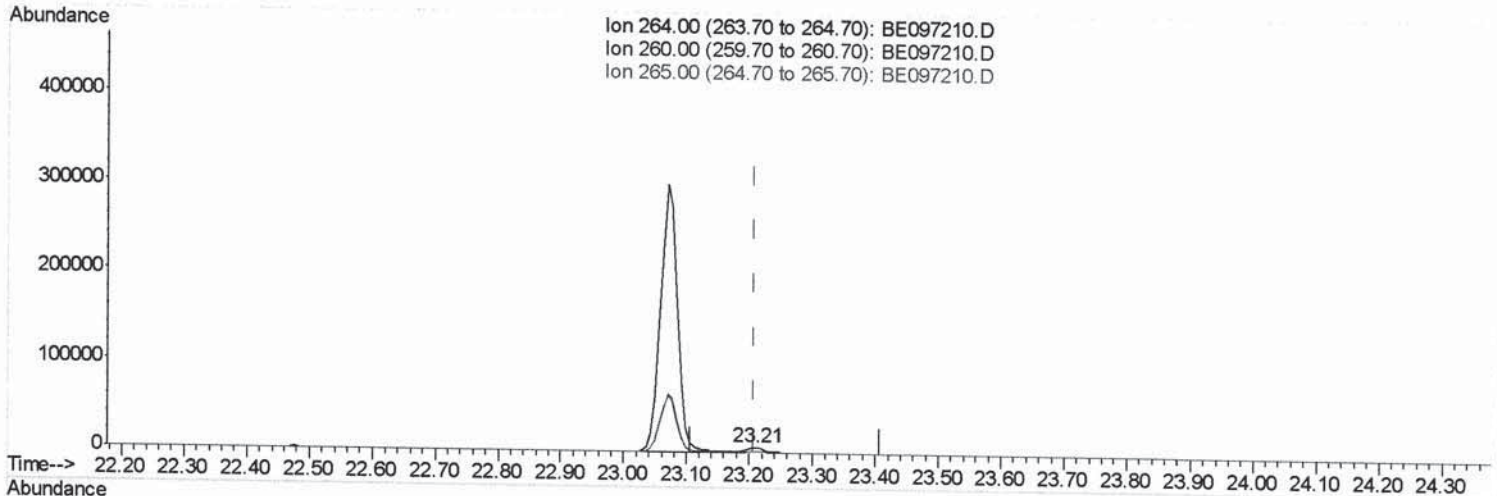

(20) Perylene-d12 (I)

23.211min (+0.002) 0.40ng/ul

response 13107

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.62
265.00	103.50	25.88#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097210.D
Acq On : 4 Aug 2018 21:06
Operator : SJ/JU
Sample : J4206-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1L0

Manual Integrations
APPROVED

Sohil
8/6/2018 12:50:57 PM



Quant Time: Aug 06 03:57:50 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Aug 06 03:46:27 2018

Response via : Initial Calibration

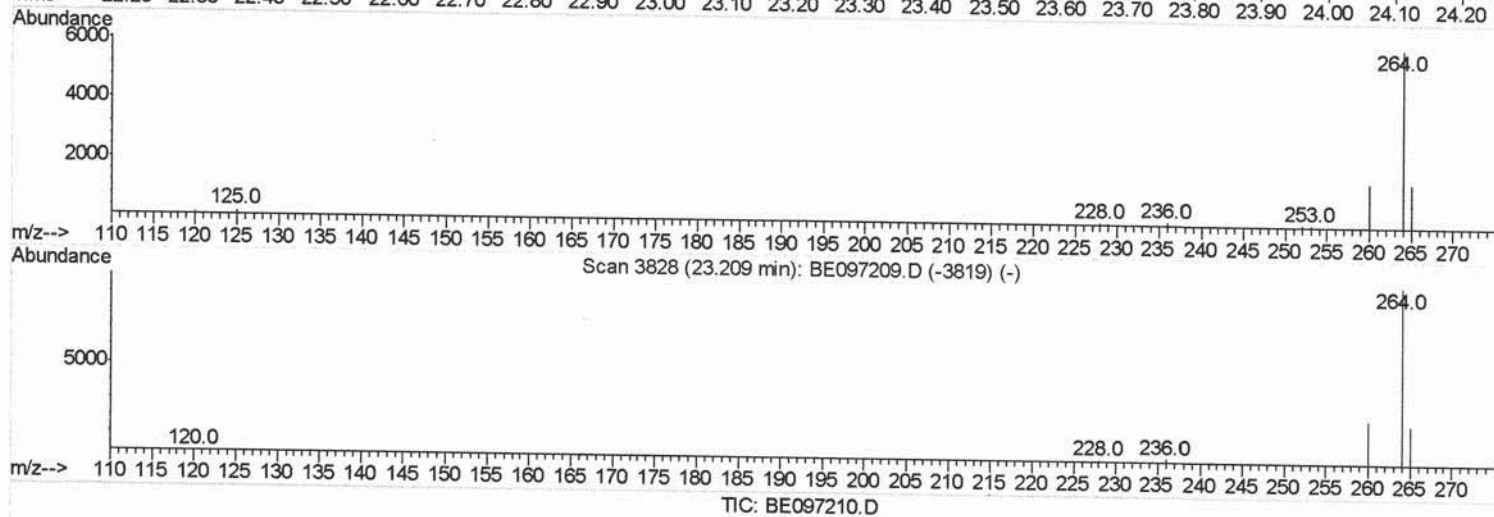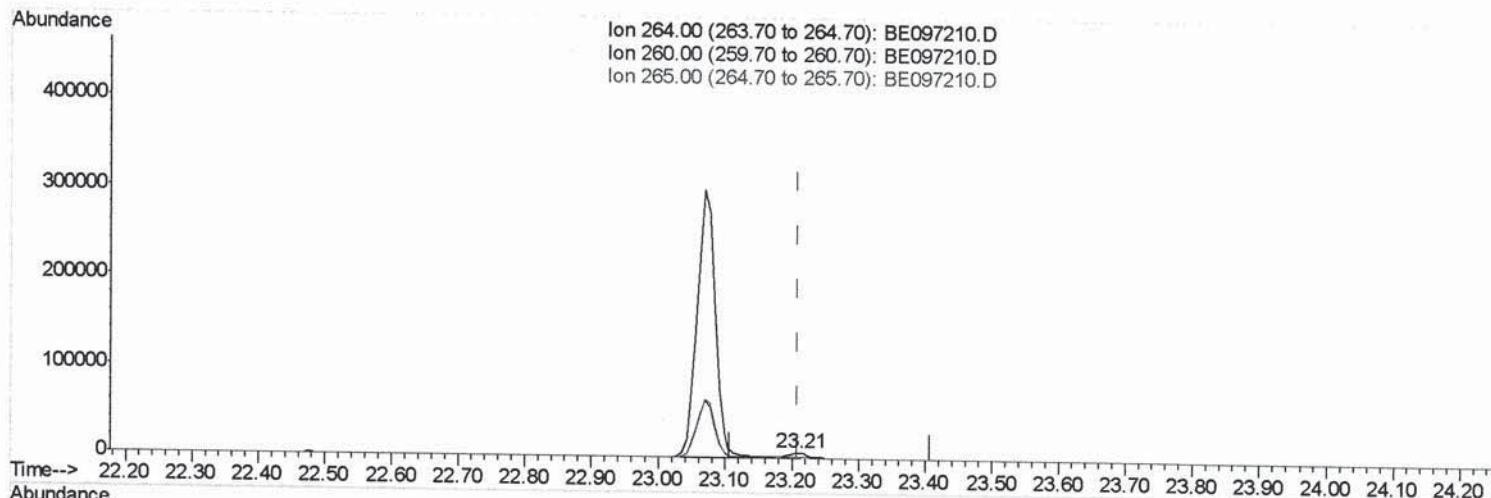

(20) Perylene-d12 (I)

23.211min (+0.002) 0.40ng/ul m

SJ 8/7/18

response 9703

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.62
265.00	103.50	25.88#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097210.D
Acq On : 4 Aug 2018 21:06
Operator : SJ/JU
Sample : J4206-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
JJ1L0

Manual Integrations
APPROVED

Sohil
8/6/2018 12:50:57 PM



Quant Time: Aug 06 03:57:50 2018

Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Mon Aug 06 03:46:27 2018

Response via : Initial Calibration

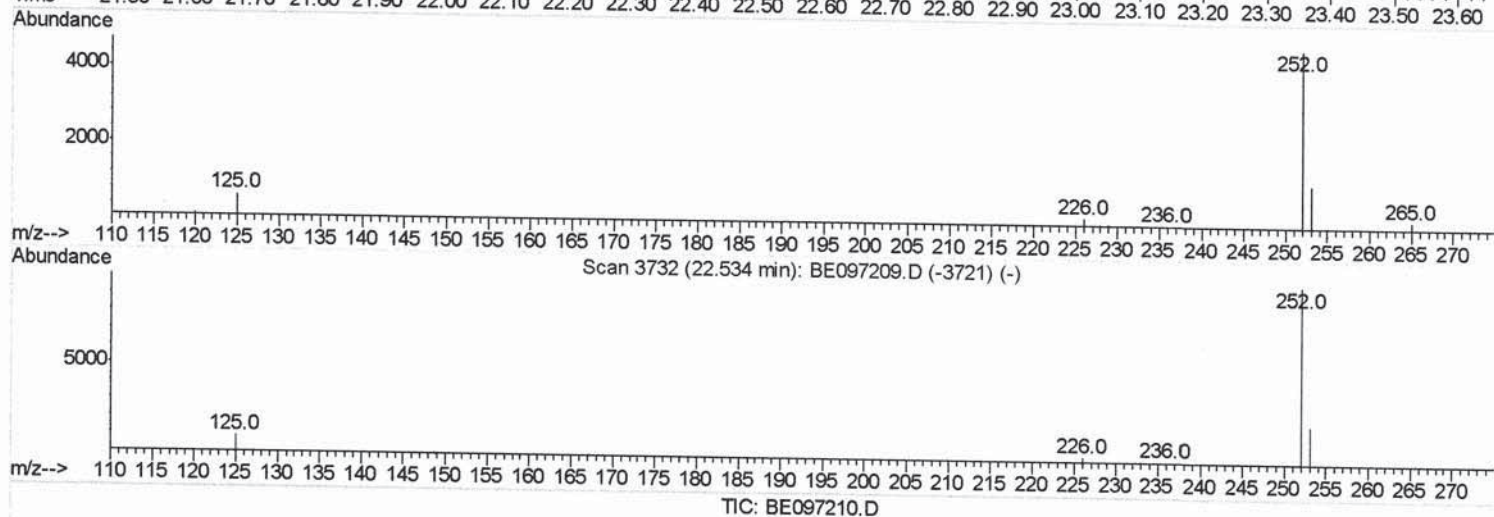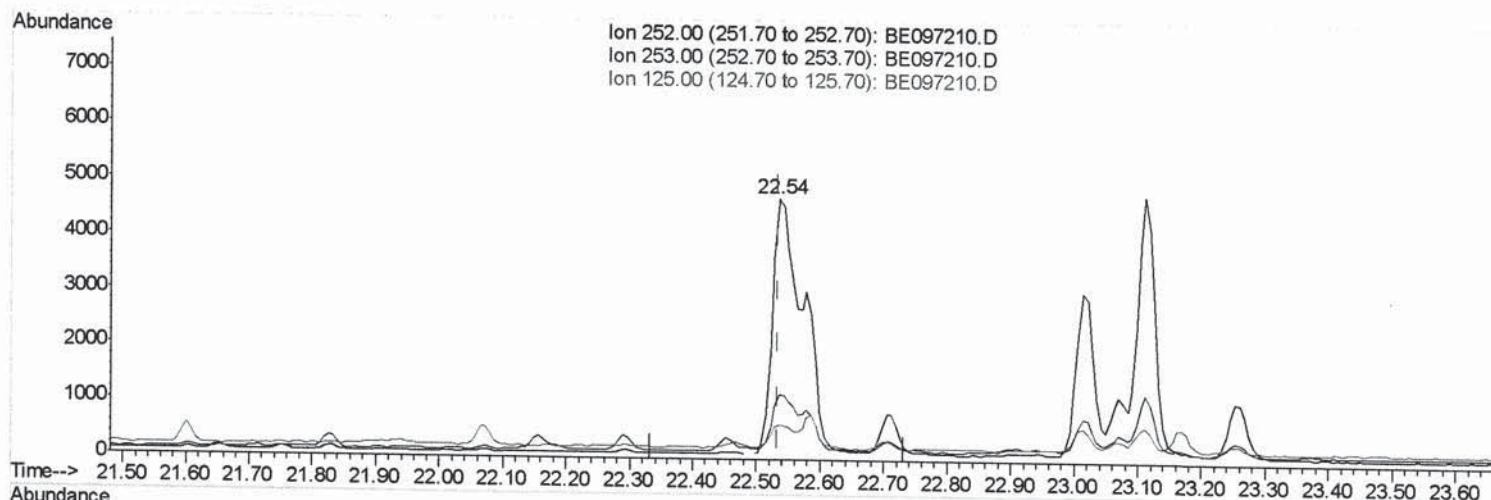

(21) Benzo(b)fluoranthene

22.536min (+0.002) 0.58ng/ul

response 15290

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	25.22
125.00	17.50	13.26
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097210.D
 Acq On : 4 Aug 2018 21:06
 Operator : SJ/JU
 Sample : J4206-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L0

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:50:57 PM

Quant Time: Aug 06 03:57:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

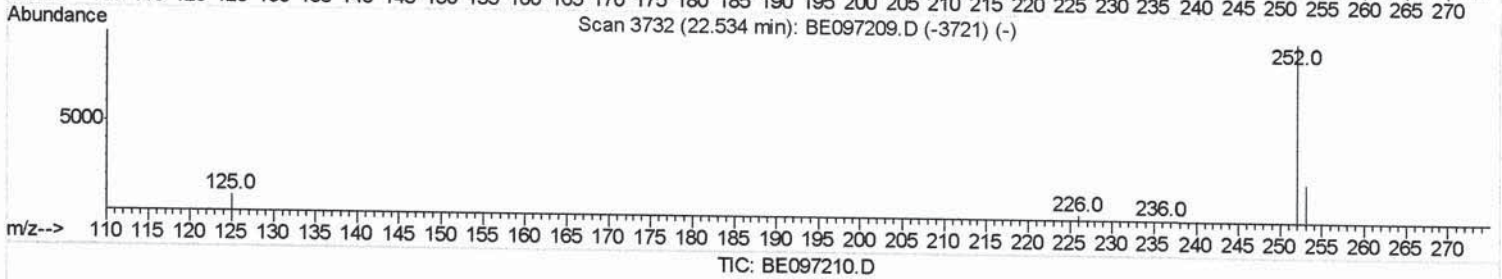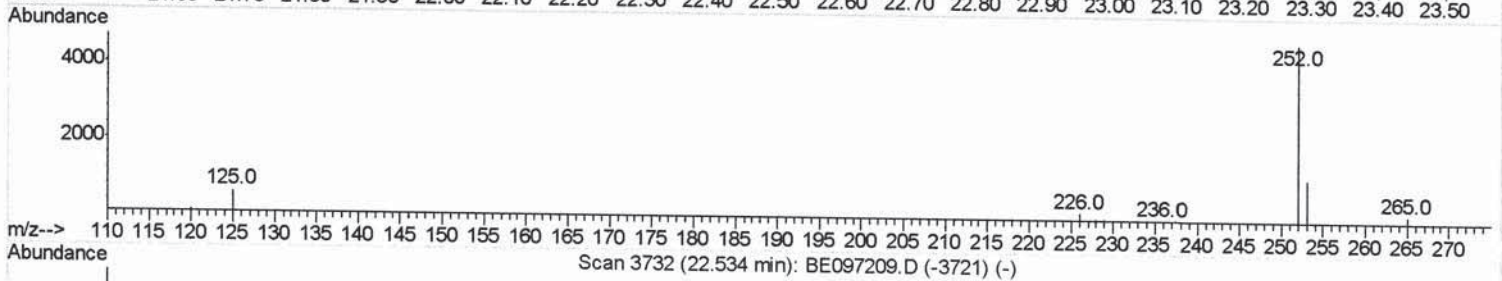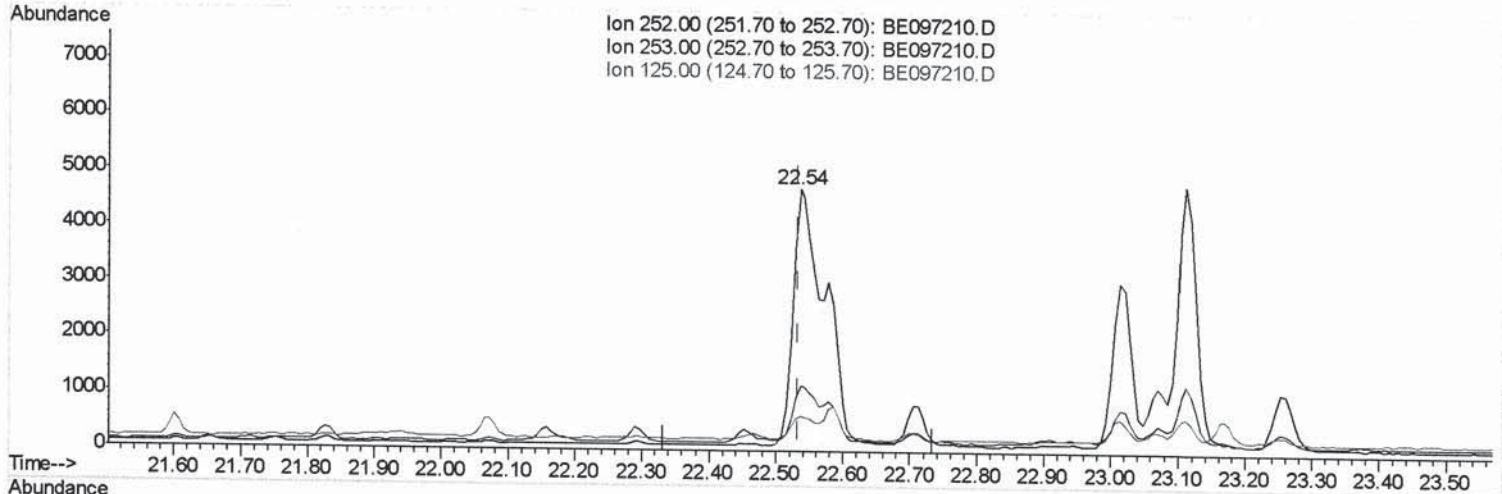

(21) Benzo(b)fluoranthene

22.536min (+0.002) 0.44ng/ul m

response 11609

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	25.22
125.00	17.50	13.26
0.00	0.00	0.00

SJ 8/7/18

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097210.D
Acq On : 4 Aug 2018 21:06
Operator : SJ/JU
Sample : J4206-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1L0

Manual Integrations
APPROVED

Sohil
8/6/2018 12:50:57 PM

Quant Time: Aug 06 03:57:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

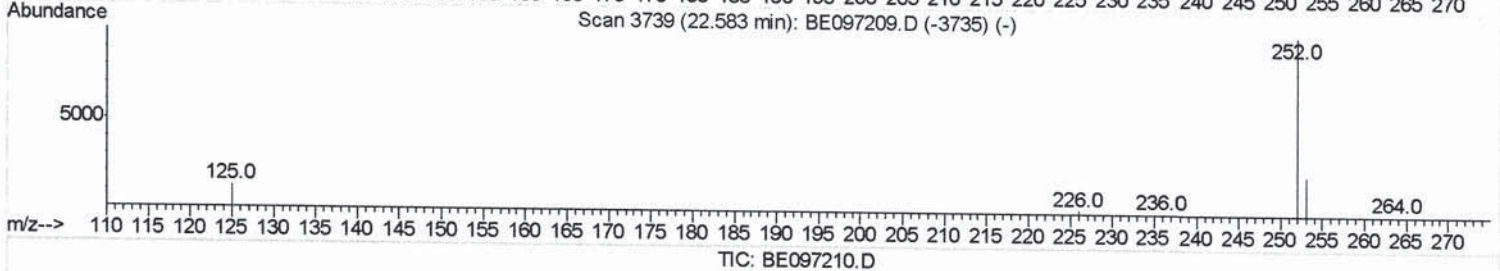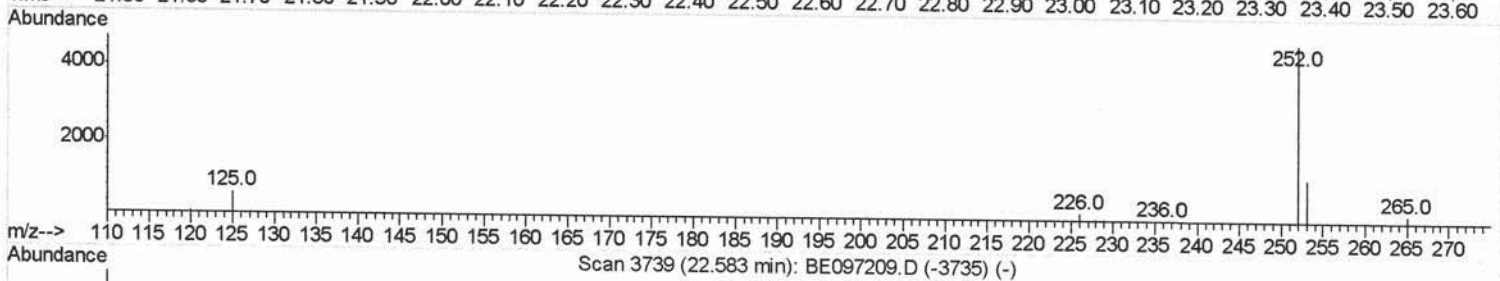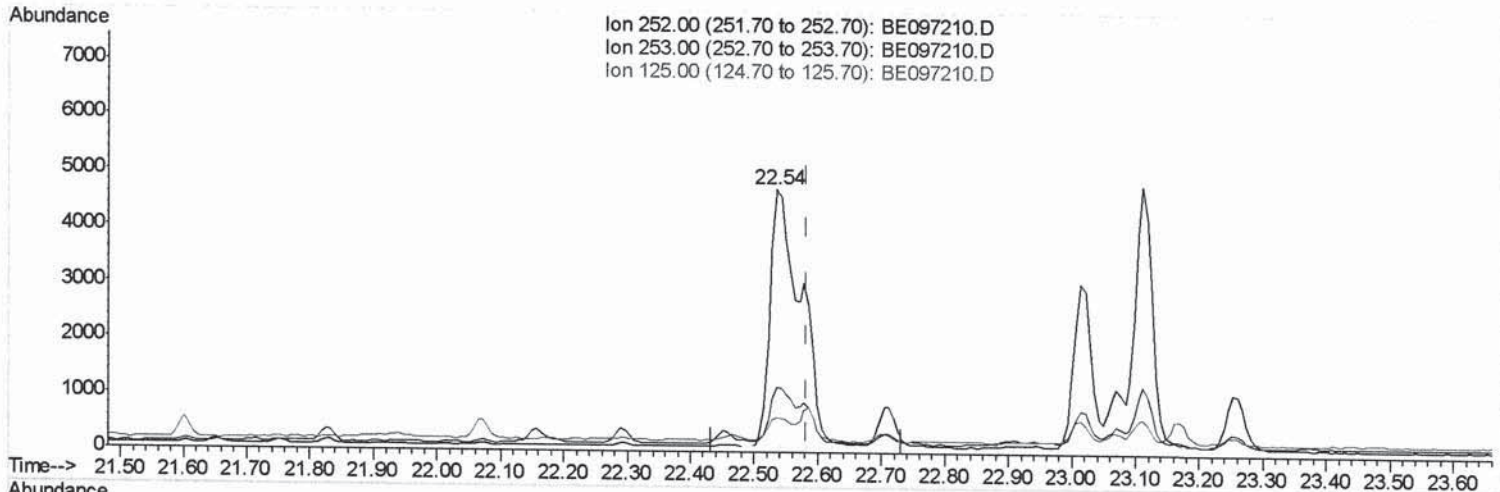

(22) Benzo(k)fluoranthene

22.536min (-0.047) 0.54ng/ui

response 15290

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	25.22
125.00	17.10	13.26#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097210.D
Acq On : 4 Aug 2018 21:06
Operator : SJ/JU
Sample : J4206-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1L0

Manual Integrations
APPROVED

Sohil
8/6/2018 12:50:57 PM

Quant Time: Aug 06 03:57:50 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

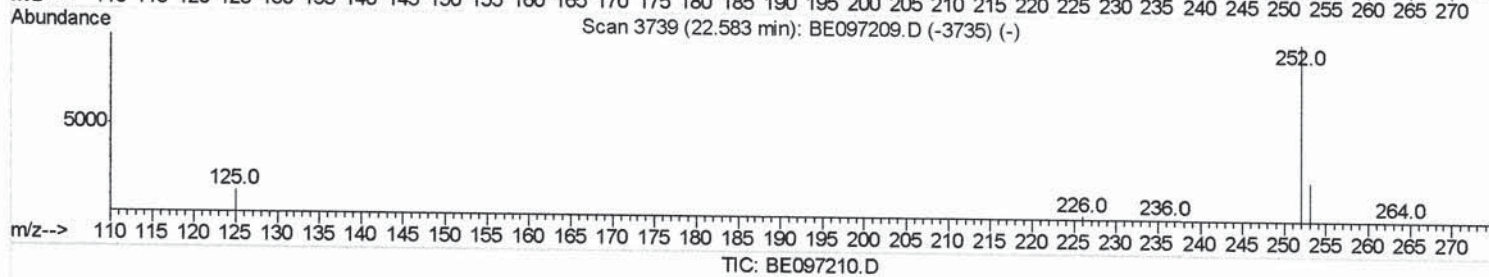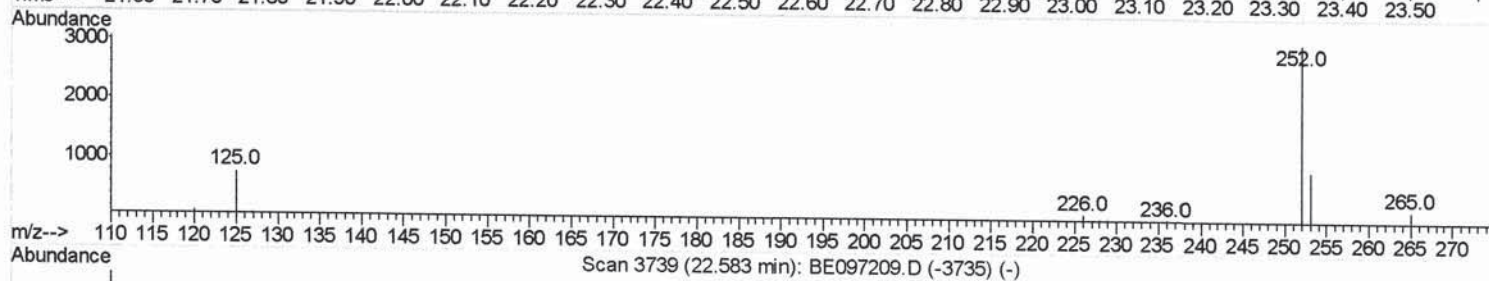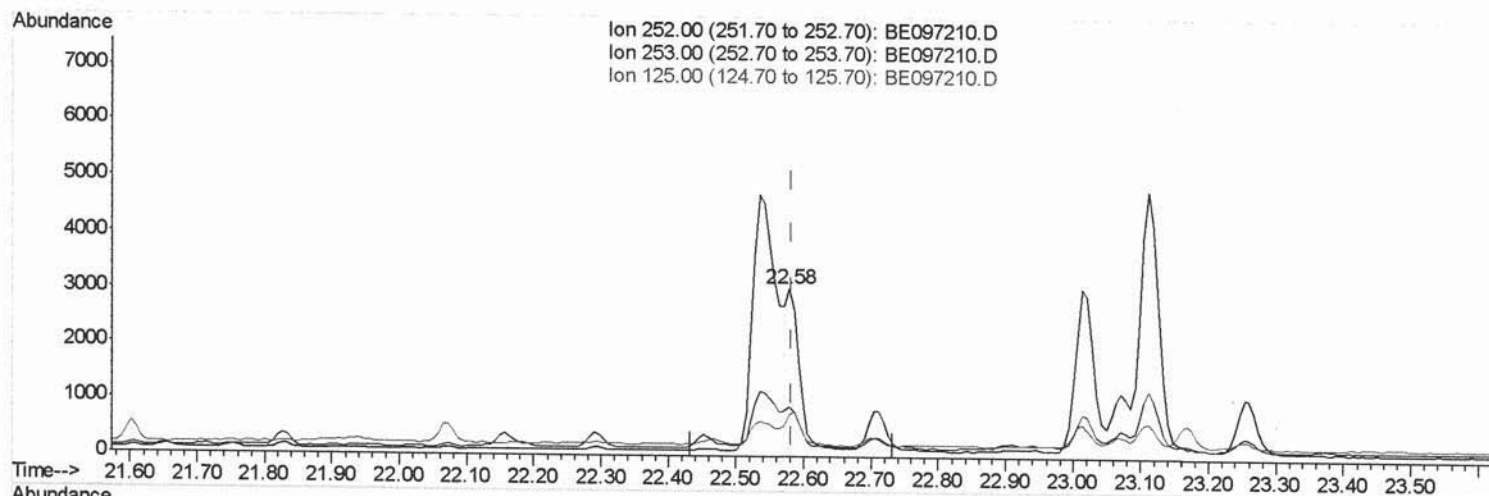

(22) Benzo(k)fluoranthene

22.578min (-0.005) 0.12ng/ul m

SJ 8/7/18

response 3397

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	29.81
125.00	17.10	25.46#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097210.D
 Acq On : 4 Aug 2018 21:06
 Operator : SJ/JU
 Sample : J4206-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L0

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:50:57 PM

Quant Time: Aug 06 03:59:14 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1261	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6839	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	4203	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.77	188	9861m	0.40	ng/ul	0.00
16) Chrysene-d12	20.97	240	10060m	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	9703m	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.73	152	2382	0.22	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	6885m	0.20	ng/ul	0.00

Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
3) Naphthalene	10.18	128	1069	0.065	ng/ul#	87
7) Acenaphthylene	13.74	152	542	0.030	ng/ul#	73
9) Fluorene	15.08	166	446	0.030	ng/ul#	92
12) Phenanthrene	16.81	178	12416m	0.494	ng/ul	
13) Anthracene	16.90	178	1266m	0.054	ng/ul	
15) Fluoranthene	18.84	202	20114m	0.605	ng/ul	
17) Pyrene	19.21	202	22227	0.825	ng/ul#	79
18) Benzo(a)anthracene	20.96	228	6806	0.237	ng/ul#	85
19) Chrysene	21.01	228	10146	0.343	ng/ul	97
21) Benzo(b)fluoranthene	22.54	252	11609m	0.439	ng/ul	
22) Benzo(k)fluoranthene	22.58	252	3397m	0.119	ng/ul	
23) Benzo(a)pyrene	23.11	252	8769	0.331	ng/ul#	82
24) Indeno(1,2,3-cd)pyrene	25.50	276	6462	0.195	ng/ul#	71
25) Dibenzo(a,h)anthracene	25.52	278	1311	0.048	ng/ul#	77
26) Benzo(a,h,i)perylene	26.21	276	6402	0.224	ng/ul	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed