

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097217.D
 Acq On : 5 Aug 2018 1:32
 Operator : SJ/JU
 Sample : J4171-21DL 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L4DL

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:51:05 PM

Quant Time: Aug 06 04:51:04 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

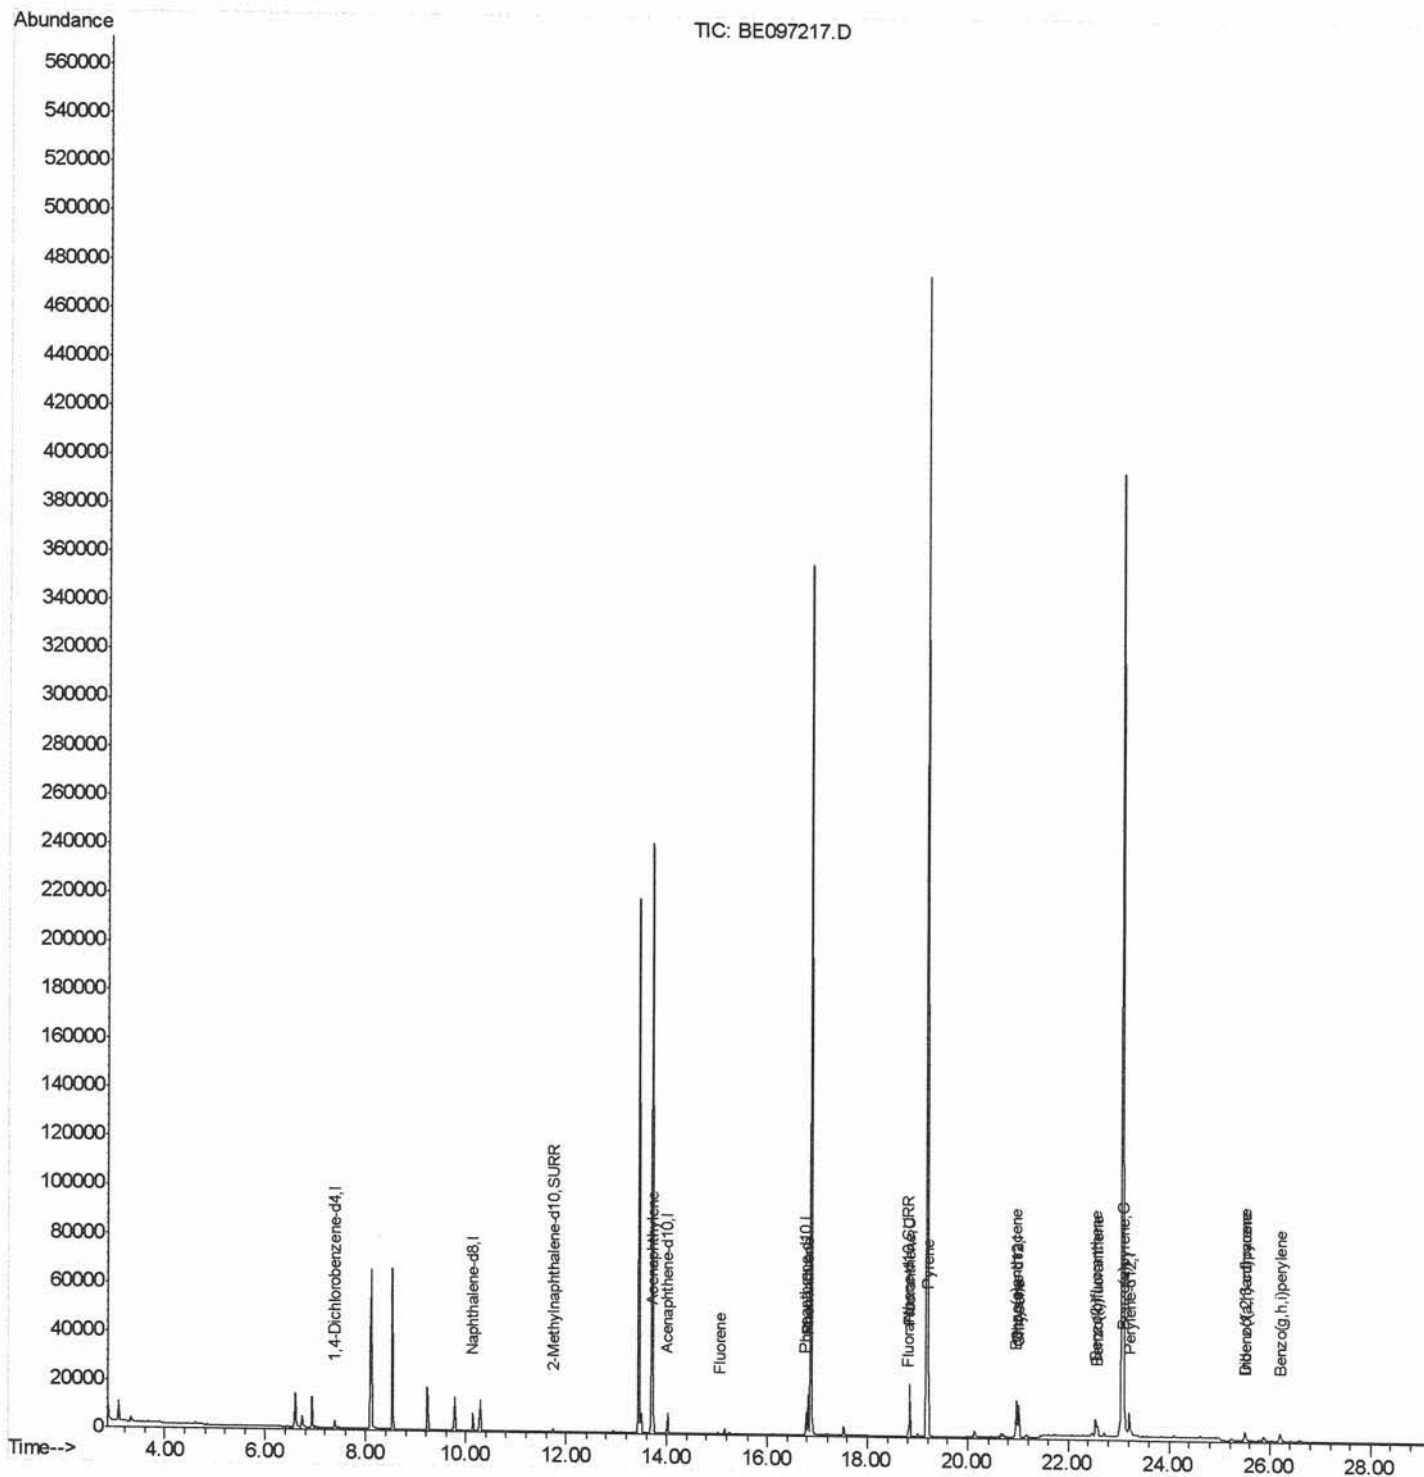

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097217.D
Acq On : 5 Aug 2018 1:32
Operator : SJ/JU
Sample : J4171-21DL 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1L4DL

Manual Integrations
APPROVED

Sohil
8/6/2018 12:51:05 PM

Quant Time: Aug 06 03:52:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

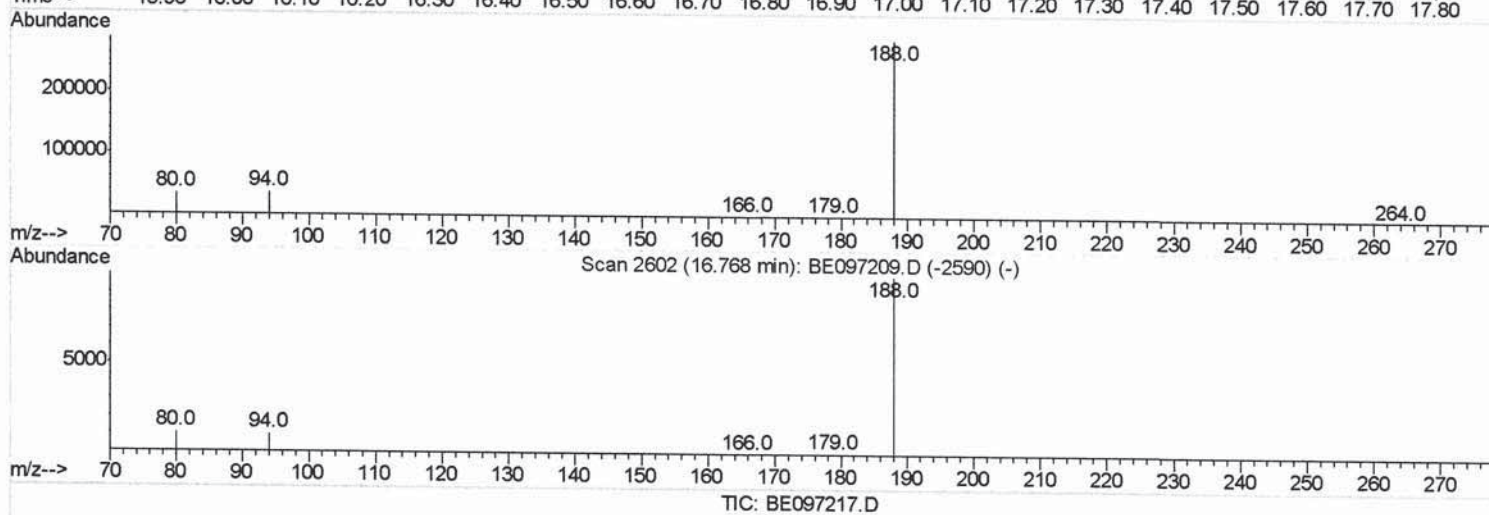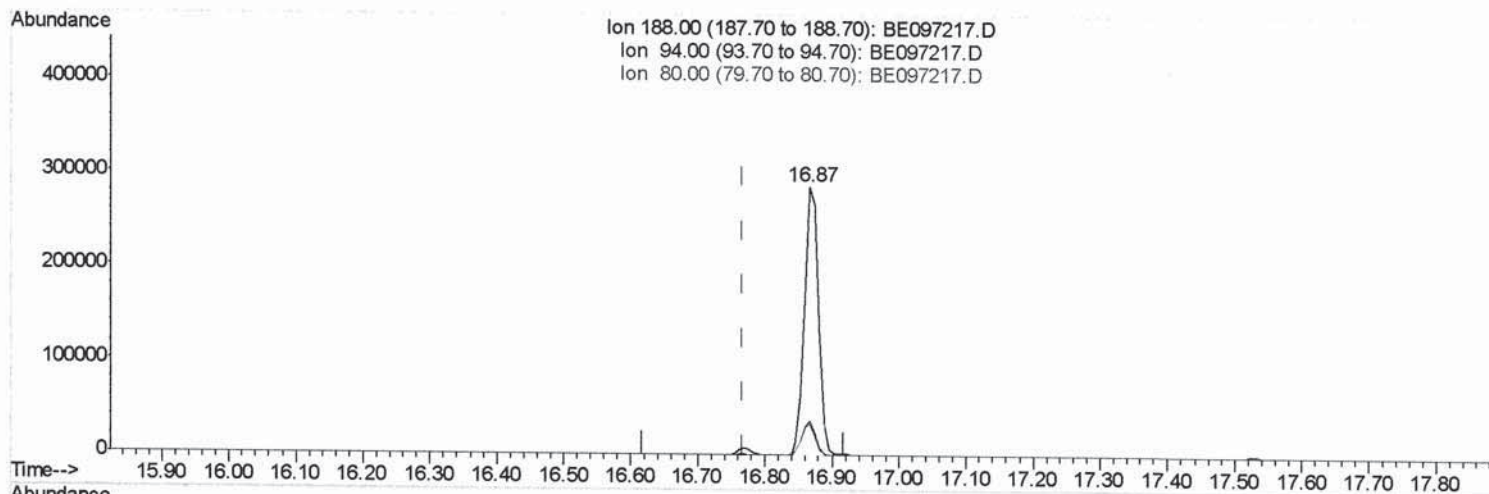

(10) Phenanthrene-d10 (I)

16.867min (+0.099) 0.40ng/ul

response 407237

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	12.71
80.00	11.80	11.83
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097217.D
Acq On : 5 Aug 2018 1:32
Operator : SJ/JU
Sample : J4171-21DL 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1L4DL

Manual Integrations
APPROVED

Sohil
8/6/2018 12:51:05 PM

Quant Time: Aug 06 03:52:21 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

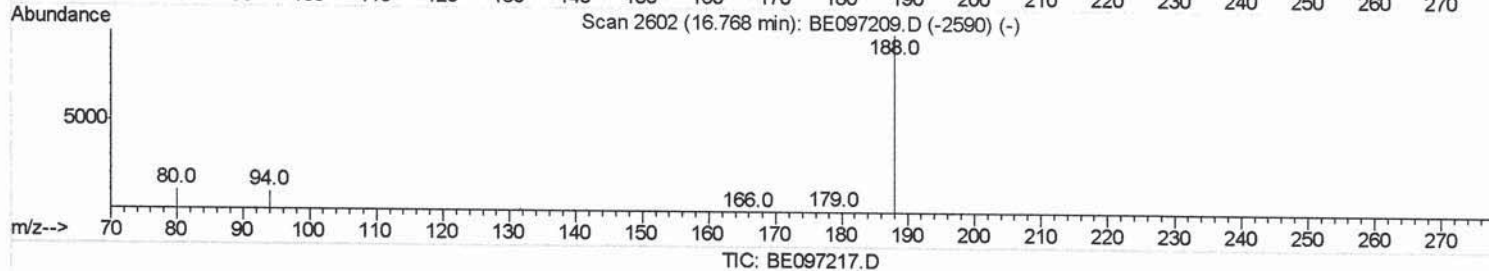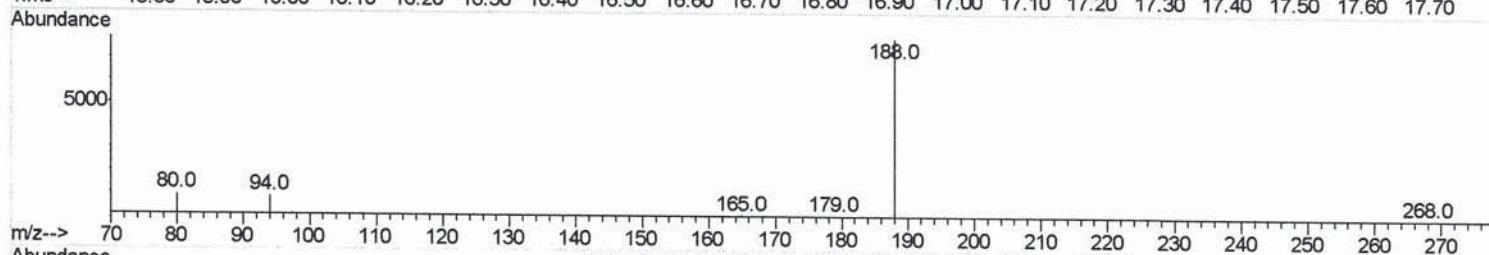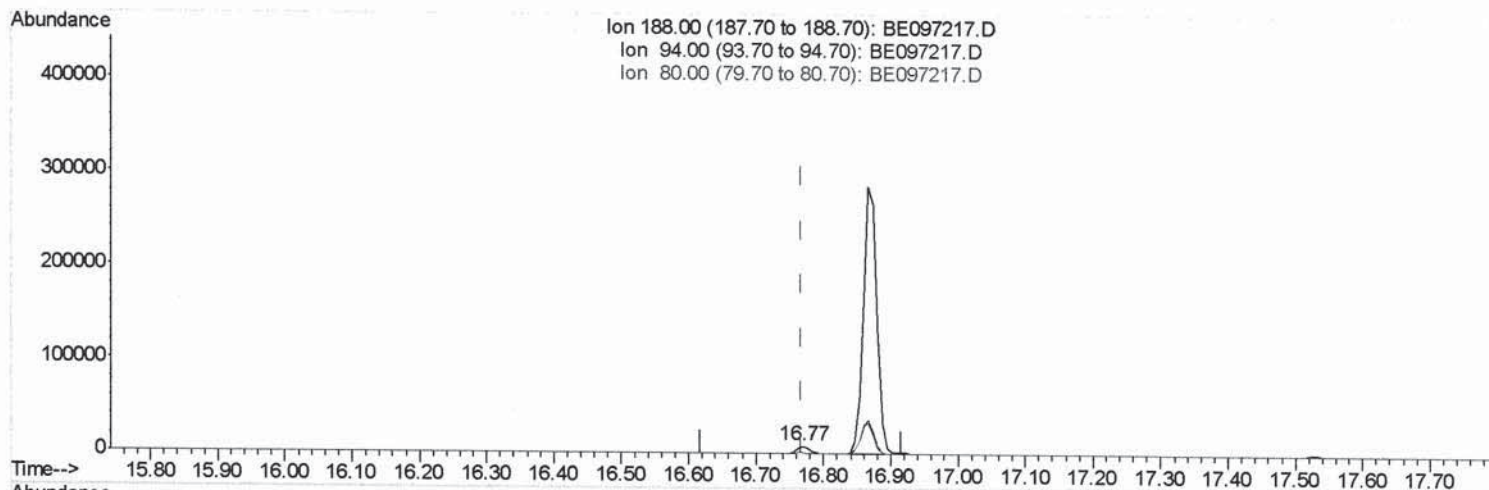

(10) Phenanthrene-d10 (I)

16.768min (+0.000) 0.40ng/ul m

SJ 8/7/18

response 10935

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.59
80.00	11.80	11.70
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097217.D
Acq On : 5 Aug 2018 1:32
Operator : SJ/JU
Sample : J4171-21DL 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1L4DL

Manual Integrations
APPROVED

Sohil
8/6/2018 12:51:05 PM

Quant Time: Aug 06 04:44:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

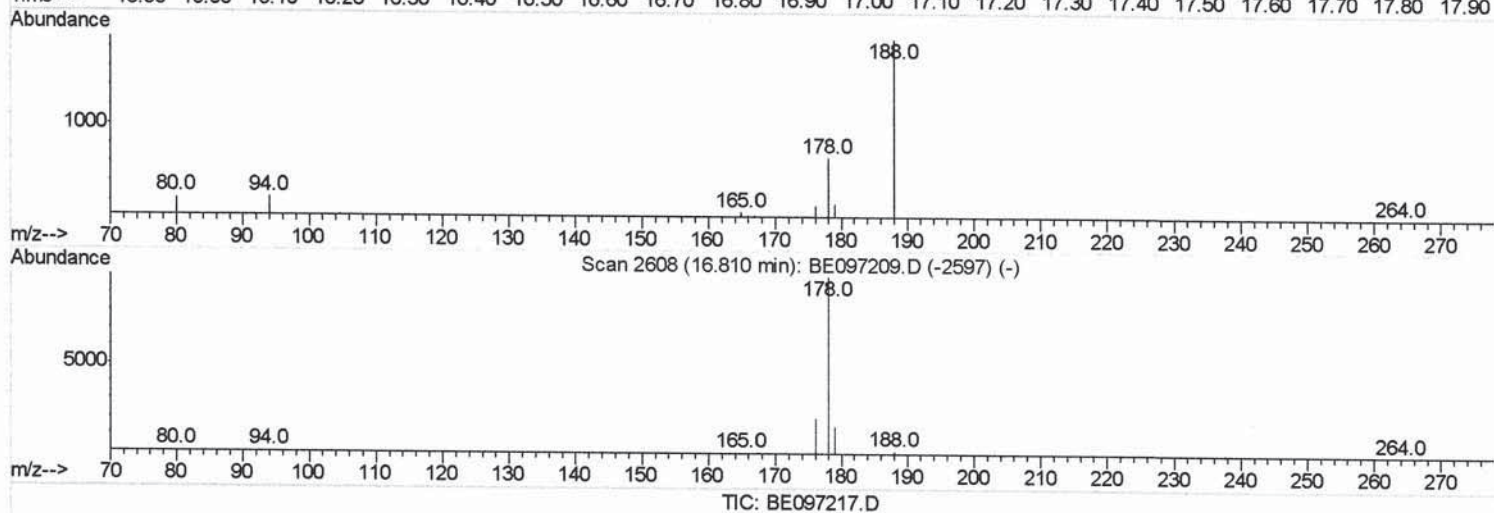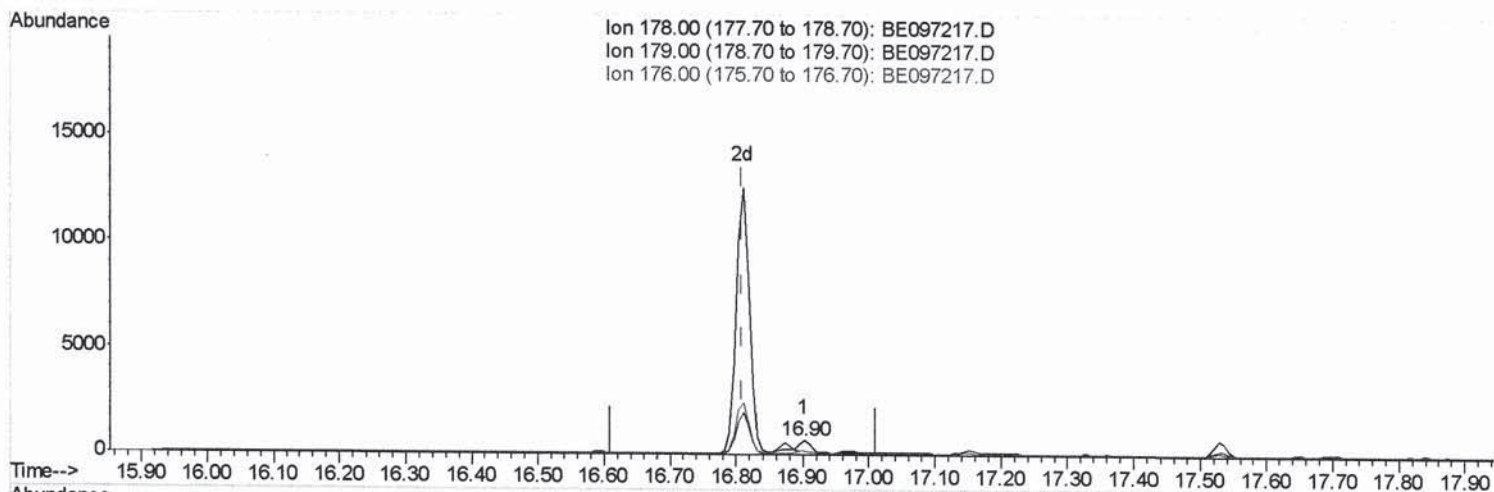

(12) Phenanthrene

16.902min (+0.092) 0.04ng/ul

response 1026

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	27.15
176.00	17.00	25.04#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097217.D
 Acq On : 5 Aug 2018 1:32
 Operator : SJ/JU
 Sample : J4171-21DL 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L4DL

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:51:05 PM

Quant Time: Aug 06 04:44:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

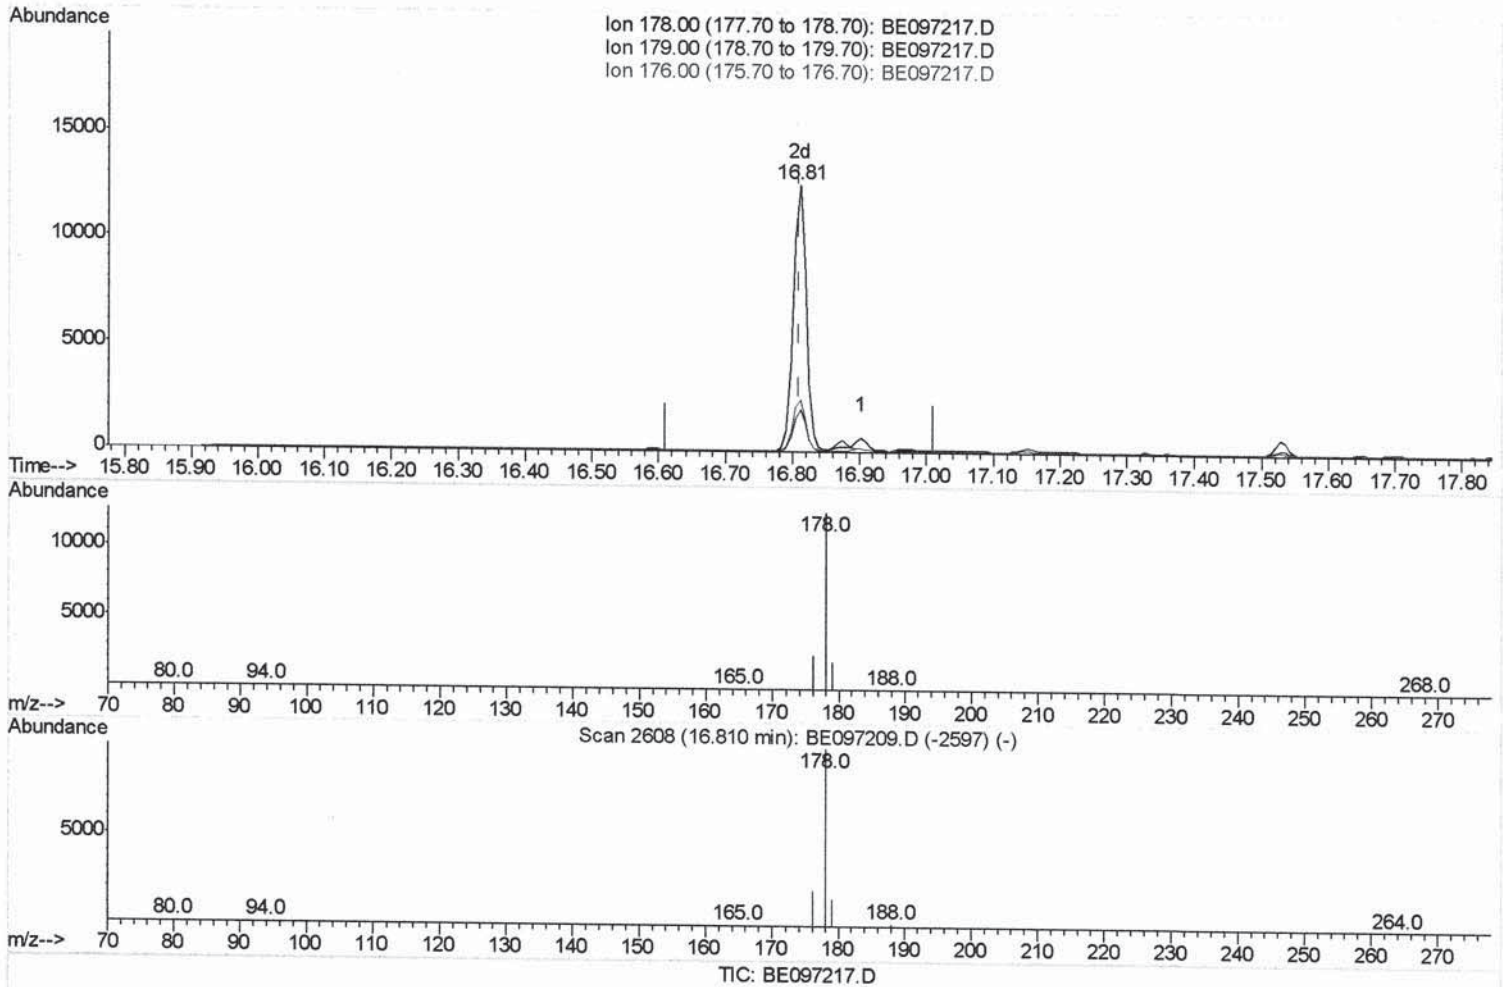

(12) Phenanthrene

16.810min (+0.000) 0.61ng/ul m

SJ 8/7/18

response 16967

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	15.99#
176.00	17.00	19.50
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097217.D
 Acq On : 5 Aug 2018 1:32
 Operator : SJ/JU
 Sample : J4171-21DL 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L4DL

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:51:05 PM

Quant Time: Aug 06 04:44:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

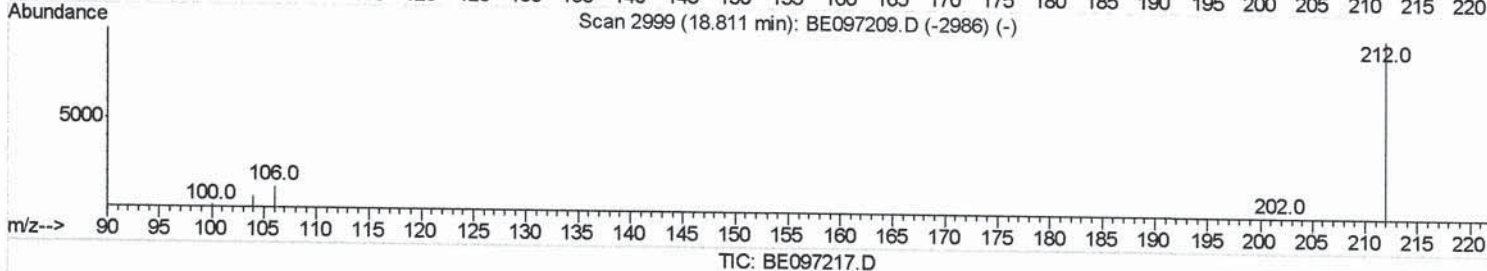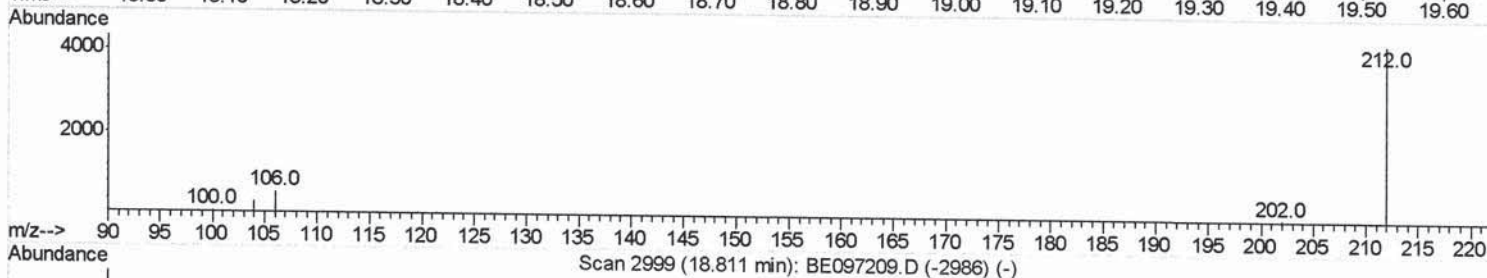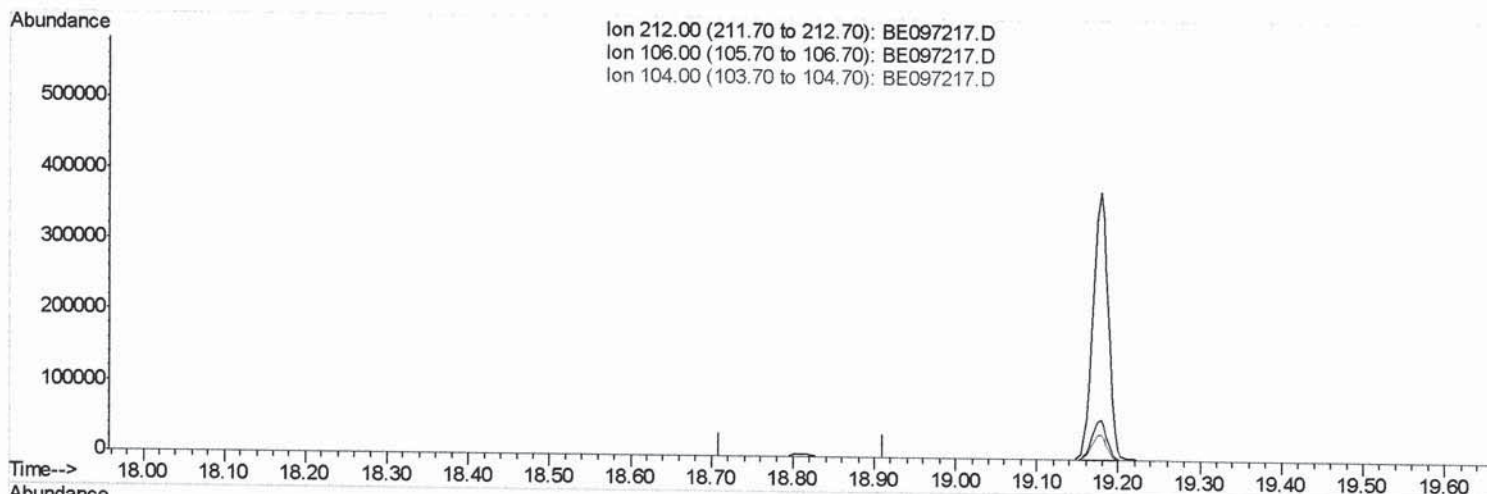

(14) Fluoranthene-d10 (SURR)

18.811min (-18.811) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097217.D
 Acq On : 5 Aug 2018 1:32
 Operator : SJ/JU
 Sample : J4171-21DL 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L4DL

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:51:05 PM

Quant Time: Aug 06 04:44:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

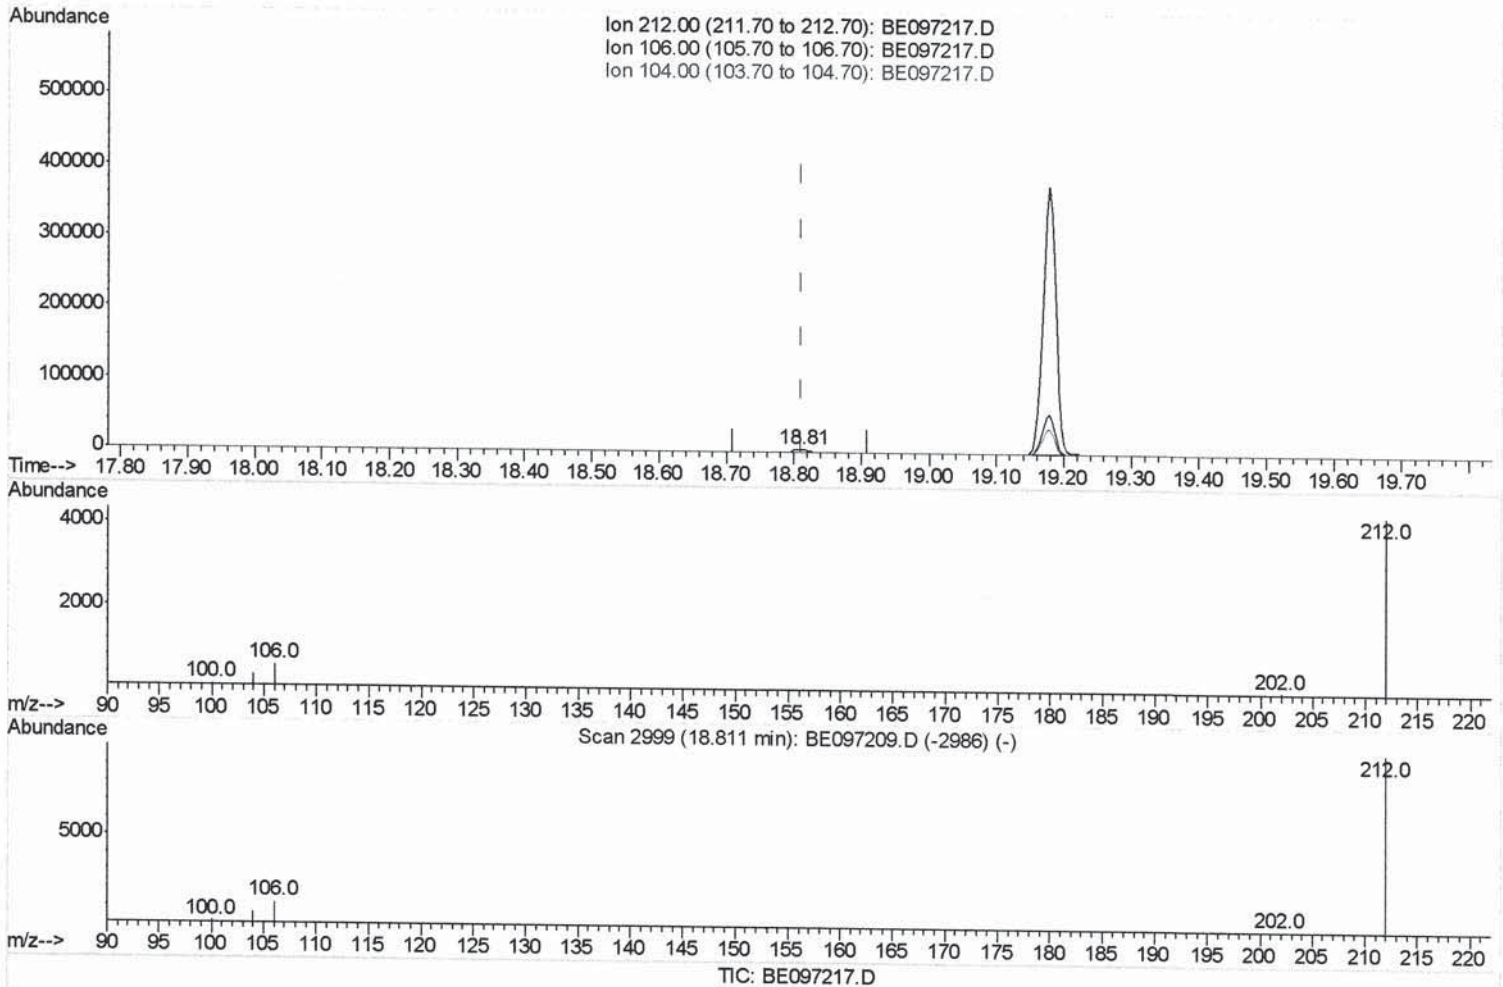

(14) Fluoranthene-d10 (SURR)

18.811min (-0.000) 0.16ng/ul m

response 6029

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

SJ 8/7/18

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097217.D
 Acq On : 5 Aug 2018 1:32
 Operator : SJ/JU
 Sample : J4171-21DL 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L4DL

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:51:05 PM

Quant Time: Aug 06 04:44:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

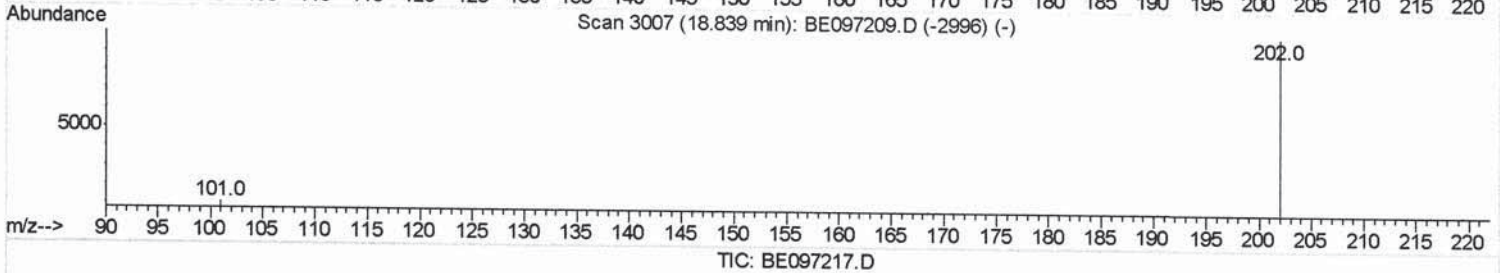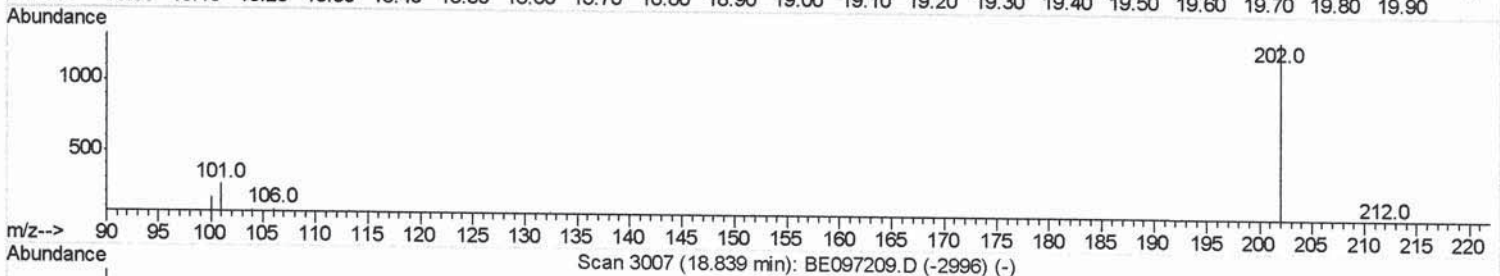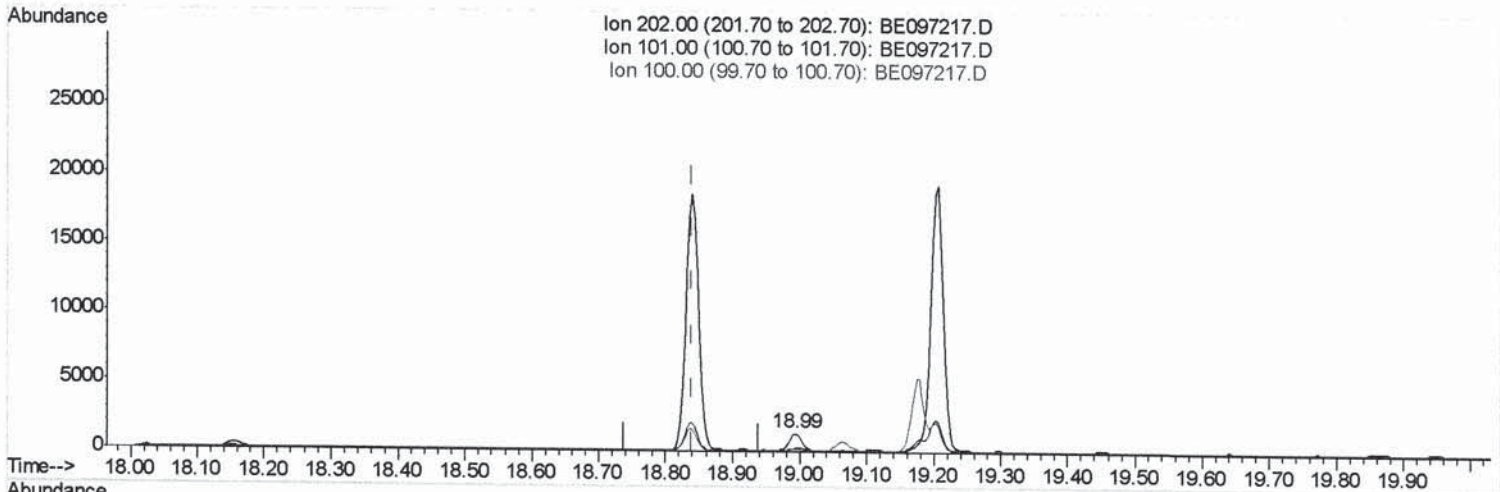

(15) Fluoranthene (C)
 18.993min (+0.153) 0.04ng/ul
 response 1563

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	19.65
100.00	19.50	12.93
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097217.D
 Acq On : 5 Aug 2018 1:32
 Operator : SJ/JU
 Sample : J4171-21DL 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L4DL

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:51:05 PM

Quant Time: Aug 06 04:44:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

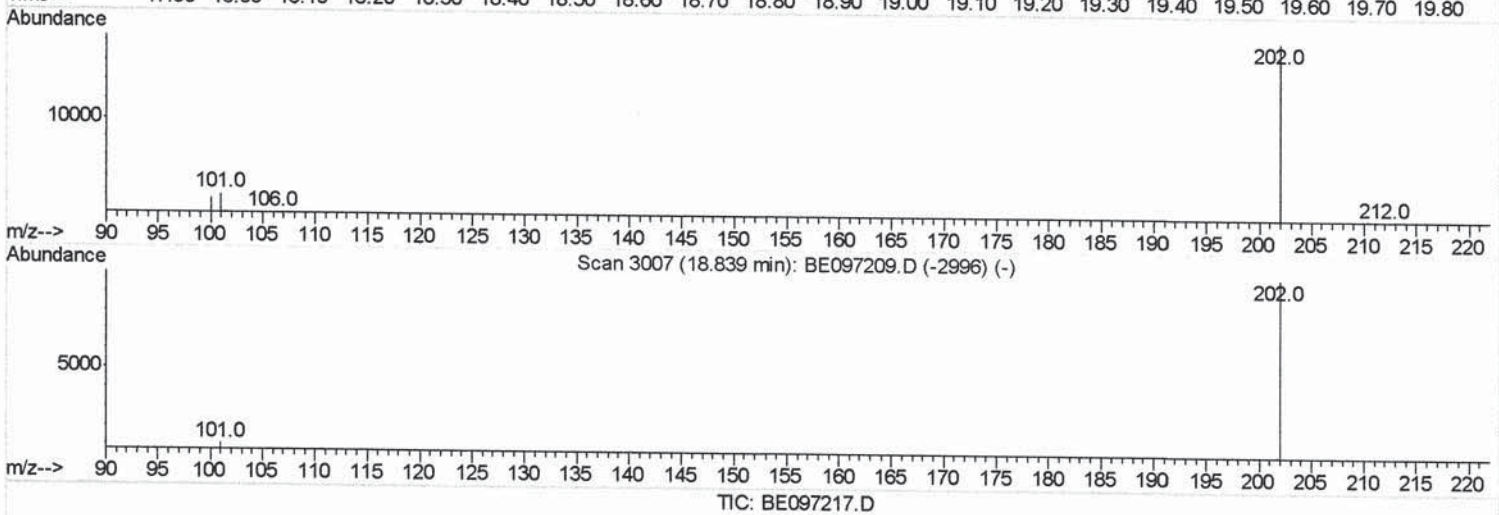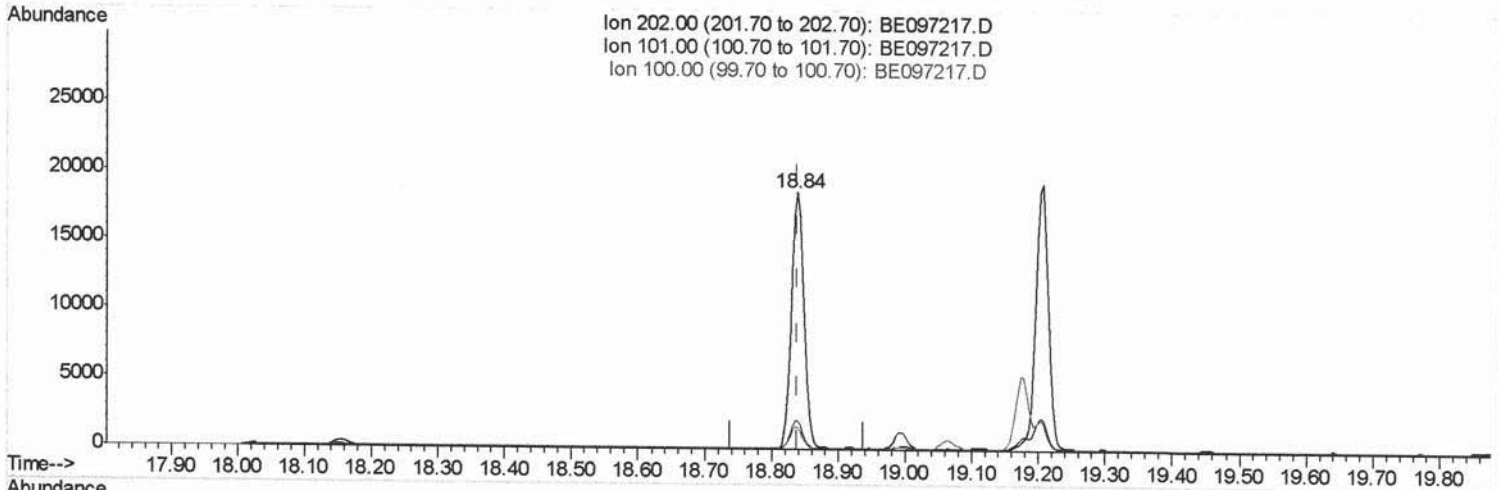

(15) Fluoranthene (C)

18.839min (-0.000) 0.65ng/ul m

SJ 8/7/18

response 23913

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	10.69
100.00	19.50	8.55
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097217.D
 Acq On : 5 Aug 2018 1:32
 Operator : SJ/JU
 Sample : J4171-21DL 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L4DL

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:51:05 PM

Quant Time: Aug 06 04:44:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

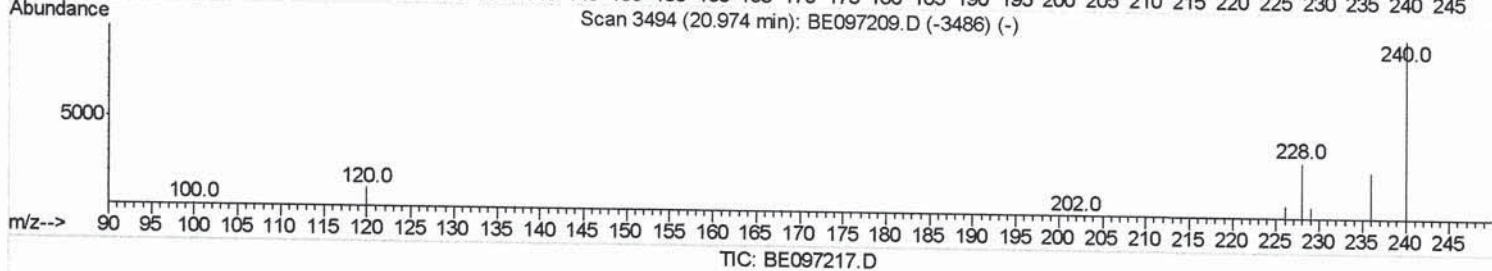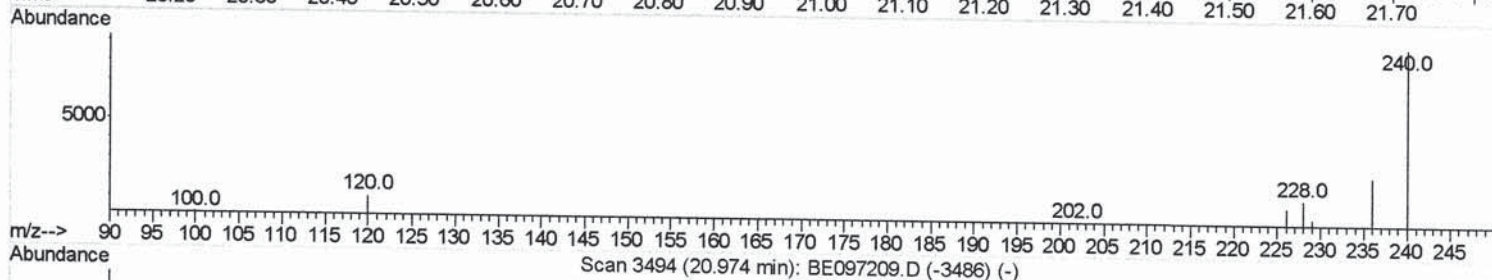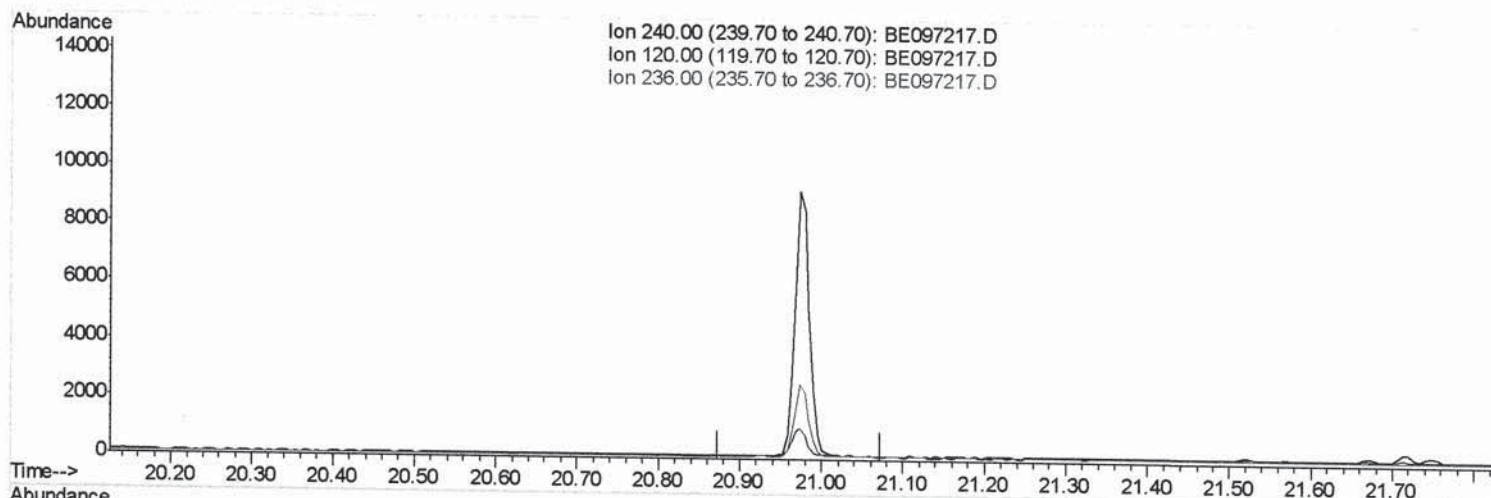

(16) Chrysene-d12 (I)

20.974min (-20.974) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.60	0.00#
236.00	34.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097217.D
 Acq On : 5 Aug 2018 1:32
 Operator : SJ/JU
 Sample : J4171-21DL 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L4DL

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:51:05 PM

Quant Time: Aug 06 04:44:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

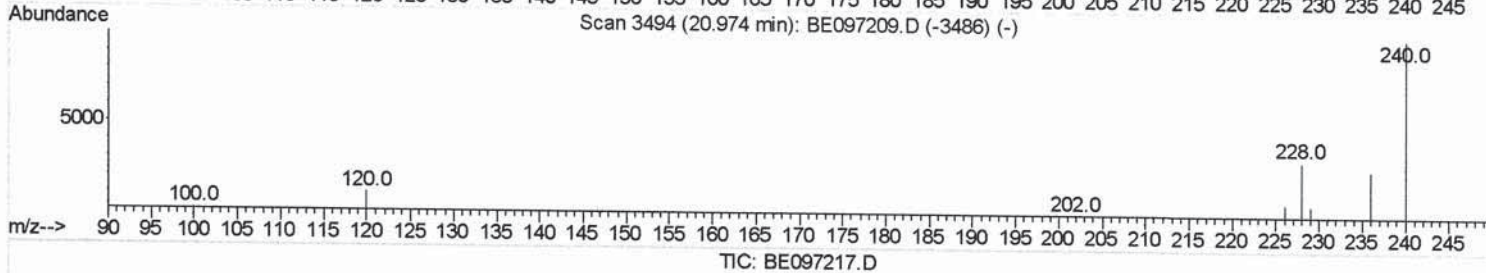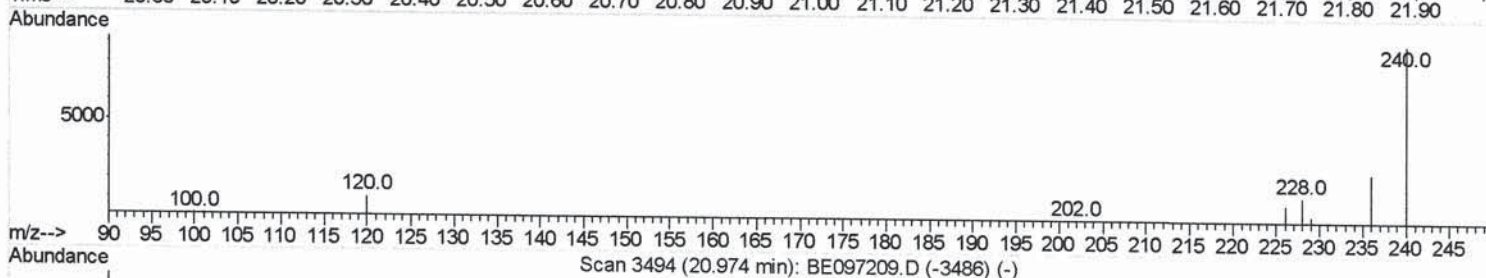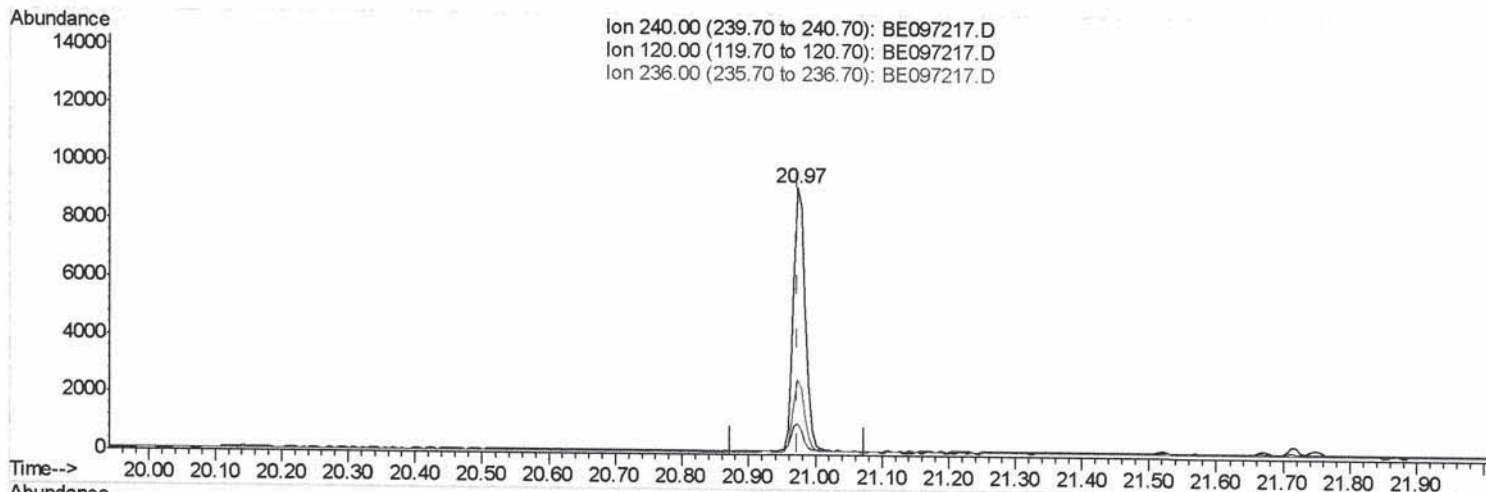

(16) Chrysene-d12 (I)

20.973min (-0.001) 0.40ng/ul m

SJ 8/7/18

response 11323

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	11.92#
236.00	34.90	28.40
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097217.D
Acq On : 5 Aug 2018 1:32
Operator : SJ/JU
Sample : J4171-21DL 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1L4DL

Manual Integrations
APPROVED

Sohil
8/6/2018 12:51:05 PM

Quant Time: Aug 06 04:46:29 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

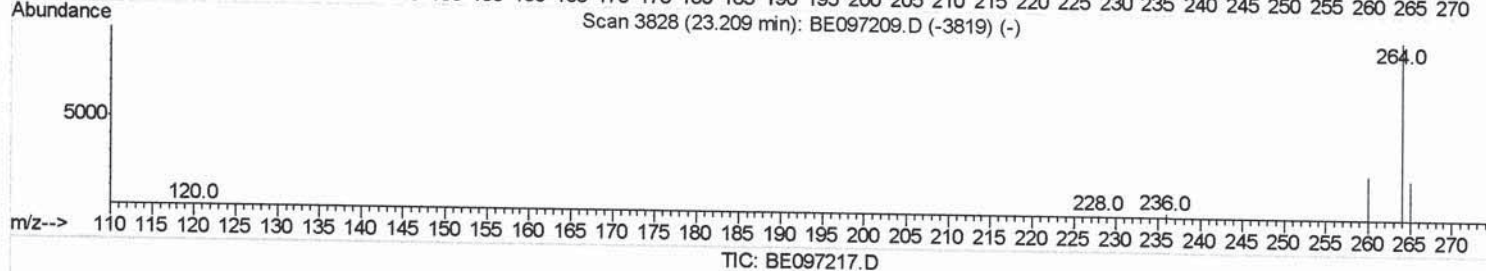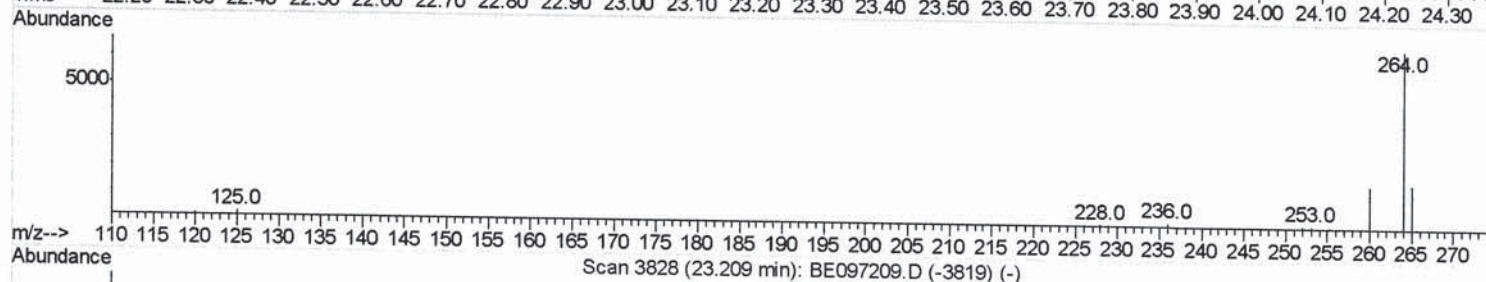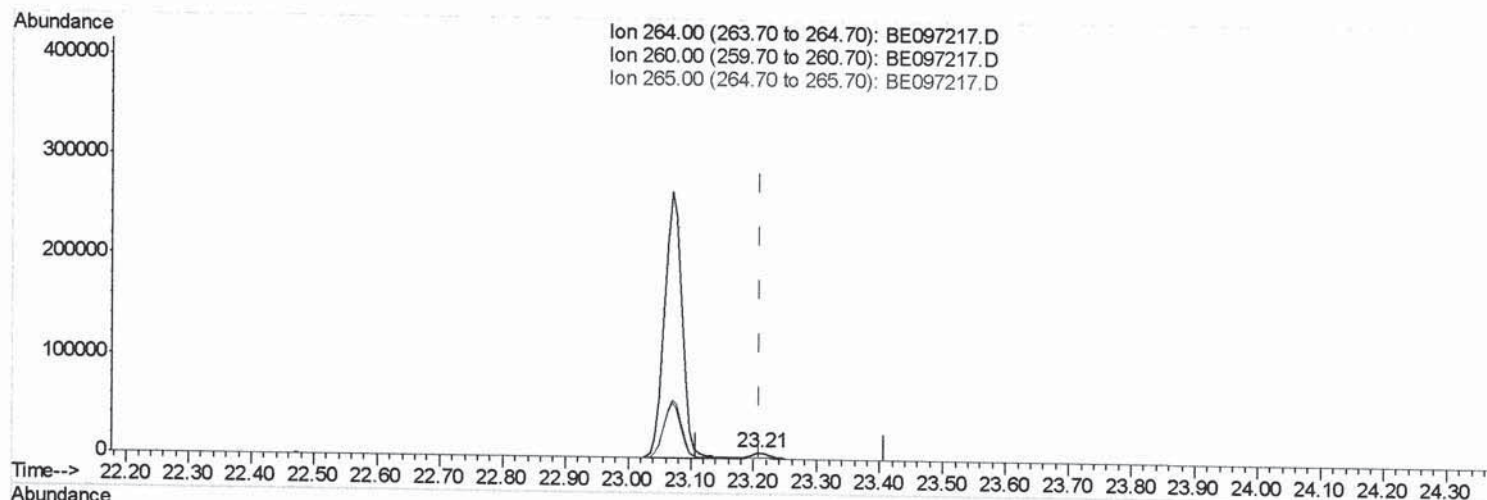

(20) Perylene-d12 (I)

23.210min (+0.001) 0.40ng/ul

response 13810

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.07
265.00	103.50	26.24#
0.00	0.00	0.00

Quantitation Report (Qedit)

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE080418\
 Data File : BE097217.D
 Acq On : 5 Aug 2018 1:32
 Operator : SJ/JU
 Sample : J4171-21DL 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Quant Time: Aug 06 04:51:04 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

Instrument :

BNA_E




Client Sampled :

JJ1L4DL

Manual Integrations
 APPROVED

Sohil

8/6/2018 12:51:05 PM

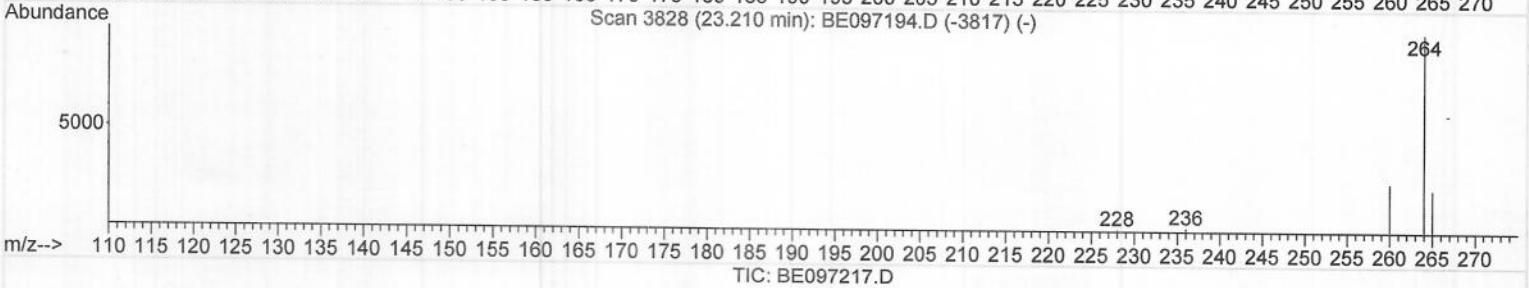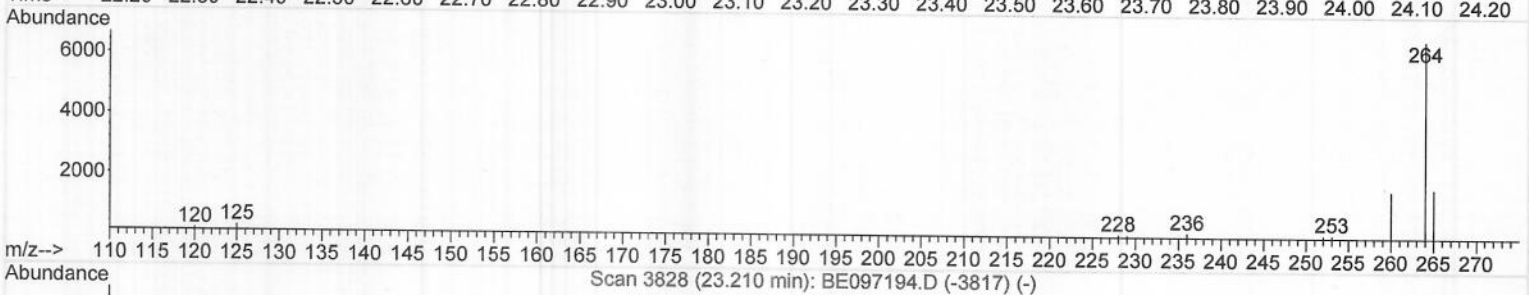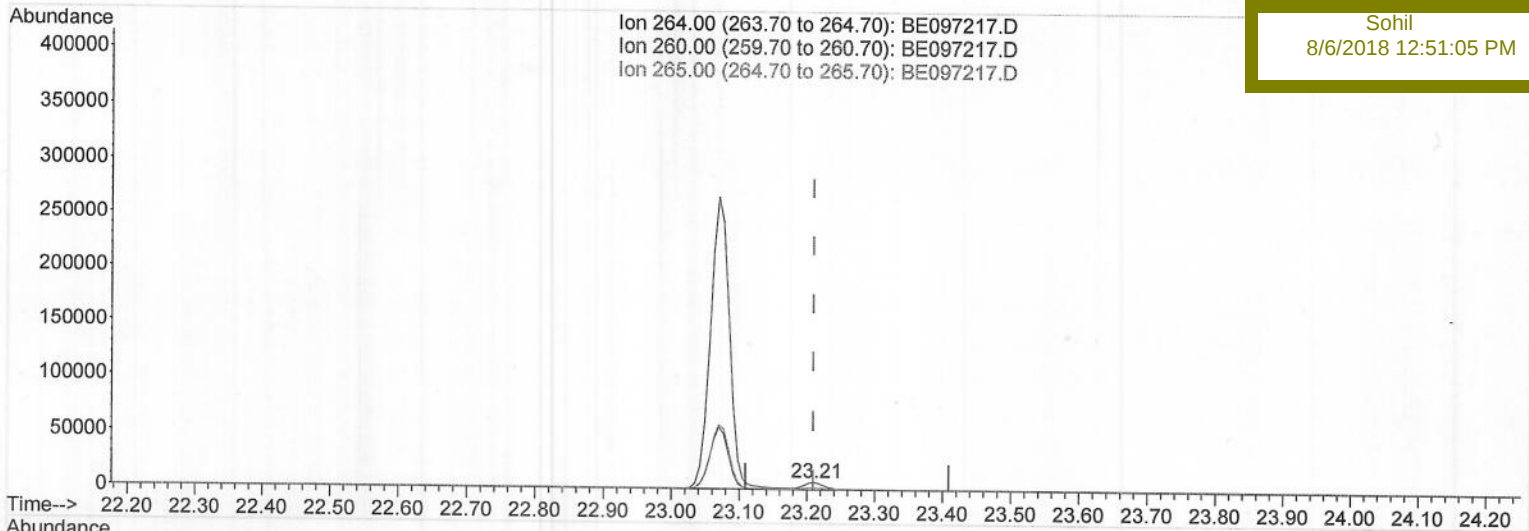

(20) Perylene-d12 (I)

23.210min (+0.001) 0.40ng/ul m

response 10673

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.07
265.00	103.50	26.24#
0.00	0.00	0.00

S-J
 08/14/2018

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097217.D
Acq On : 5 Aug 2018 1:32
Operator : SJ/JU
Sample : J4171-21DL 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1L4DL

Manual Integrations
APPROVED

Sohil
8/6/2018 12:51:05 PM

Quant Time: Aug 06 04:47:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

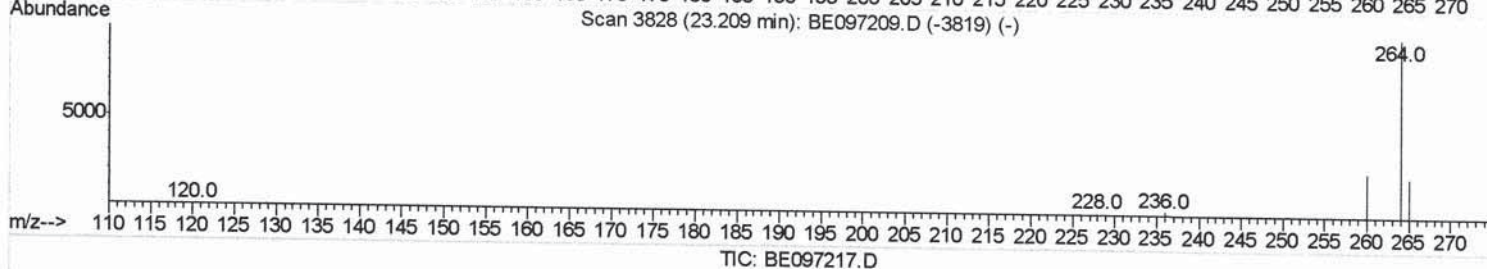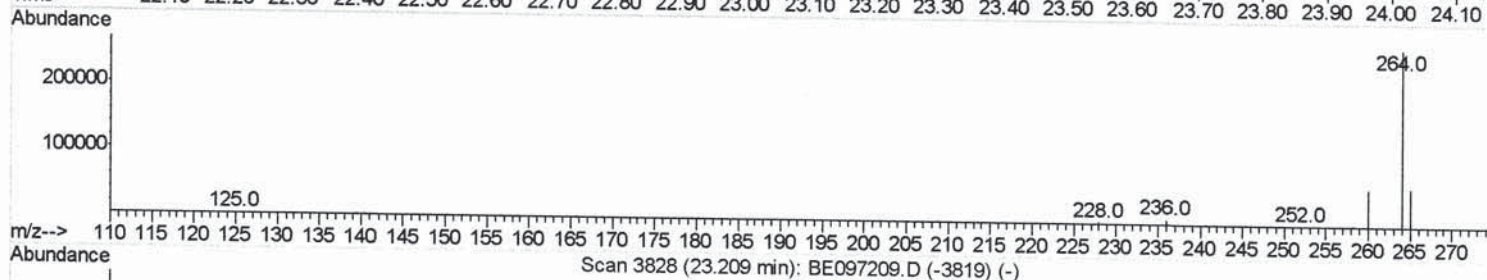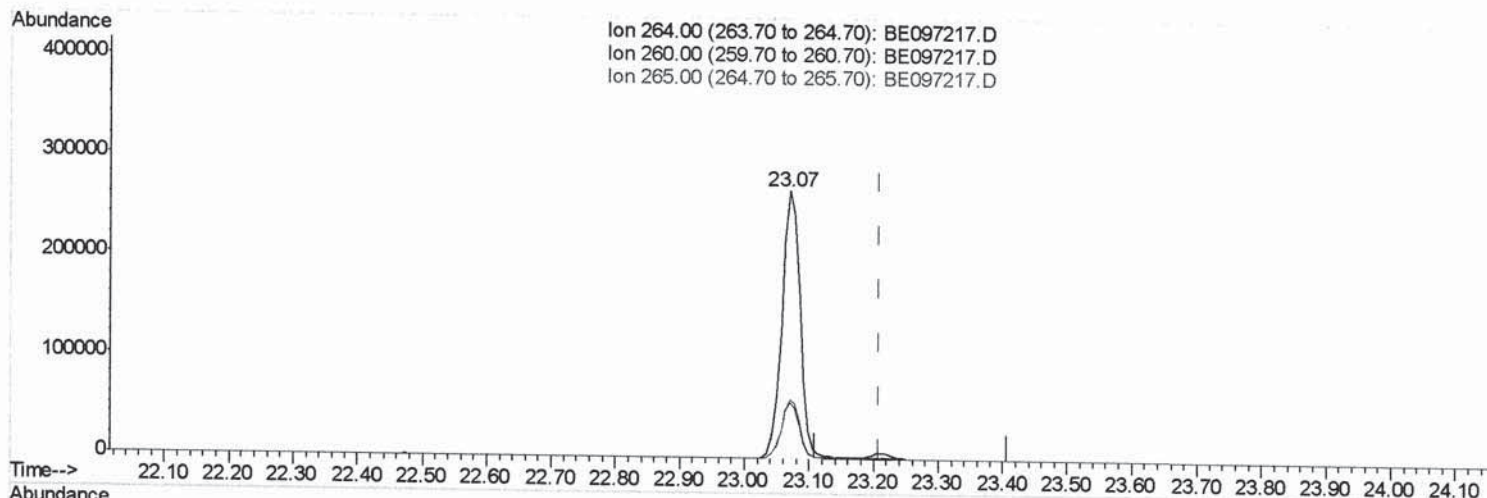

(20) Perylene-d12 (I)

23.070min (-0.139) 0.40ng/ul m

response 519904

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	20.99#
265.00	103.50	21.84#
0.00	0.00	0.00

SJ 8/7/18

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097217.D
 Acq On : 5 Aug 2018 1:32
 Operator : SJ/JU
 Sample : J4171-21DL 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L4DL

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:51:05 PM

Quant Time: Aug 06 04:47:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

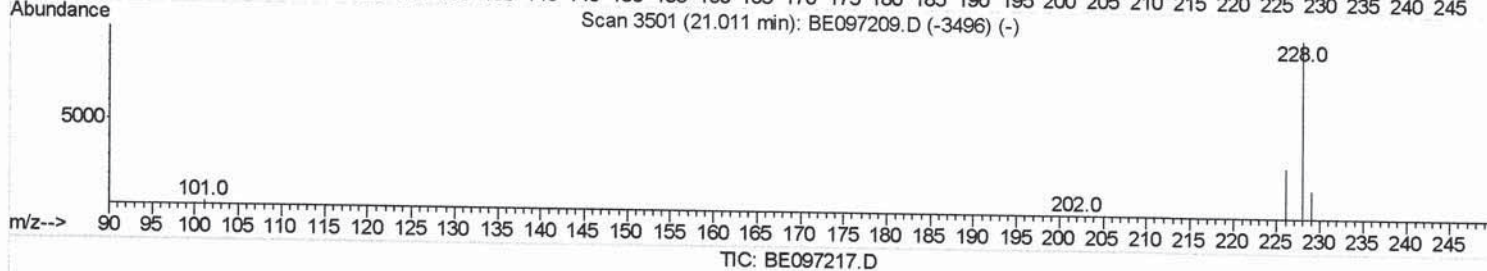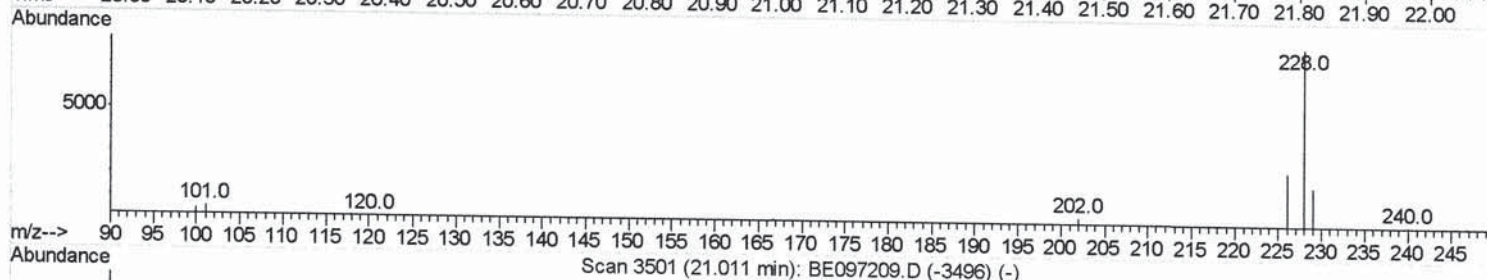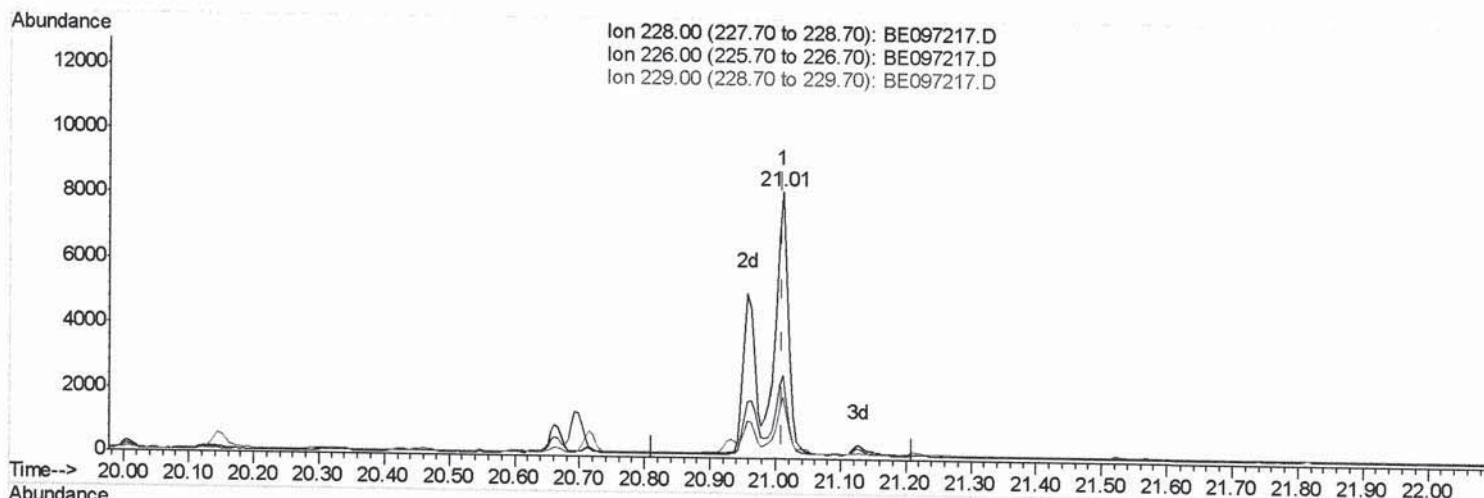

(19) Chrysene

21.010min (-0.001) 0.34ng/ul

response 11312

Ion	Exp%	Act%
228.00	100	100
226.00	29.20	31.30
229.00	22.10	23.00
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097217.D
Acq On : 5 Aug 2018 1:32
Operator : SJ/JU
Sample : J4171-21DL 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1L4DL

Manual Integrations
APPROVED

Sohil
8/6/2018 12:51:05 PM

Quant Time: Aug 06 04:47:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

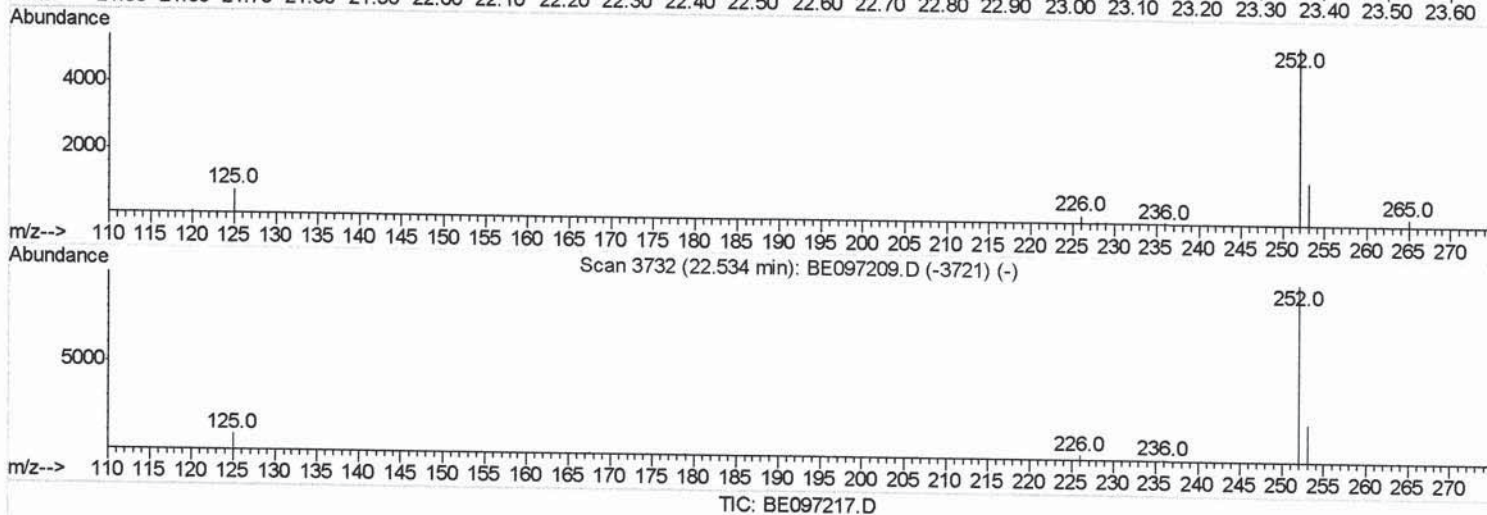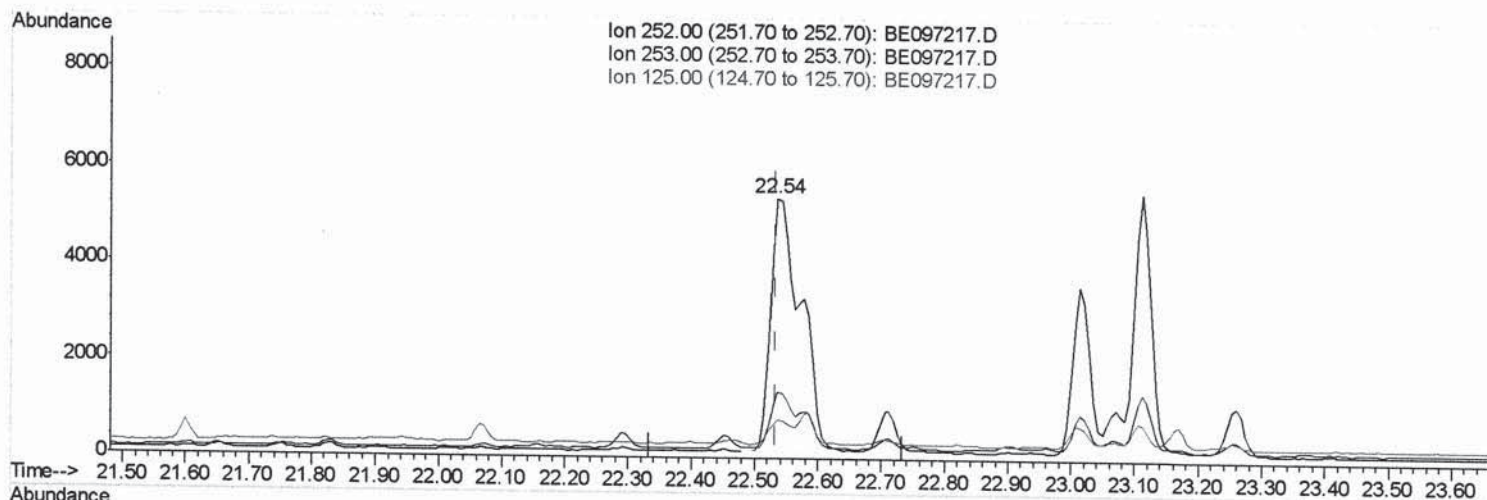

(21) Benzo(b)fluoranthene

22.535min (+0.001) 0.60ng/ul

response 17322

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	25.47
125.00	17.50	14.79
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097217.D
 Acq On : 5 Aug 2018 1:32
 Operator : SJ/JU
 Sample : J4171-21DL 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L4DL

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:51:05 PM

Quant Time: Aug 06 04:47:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

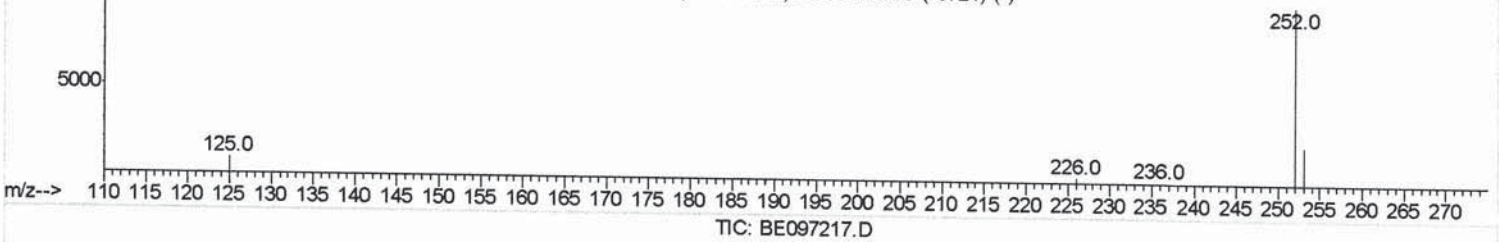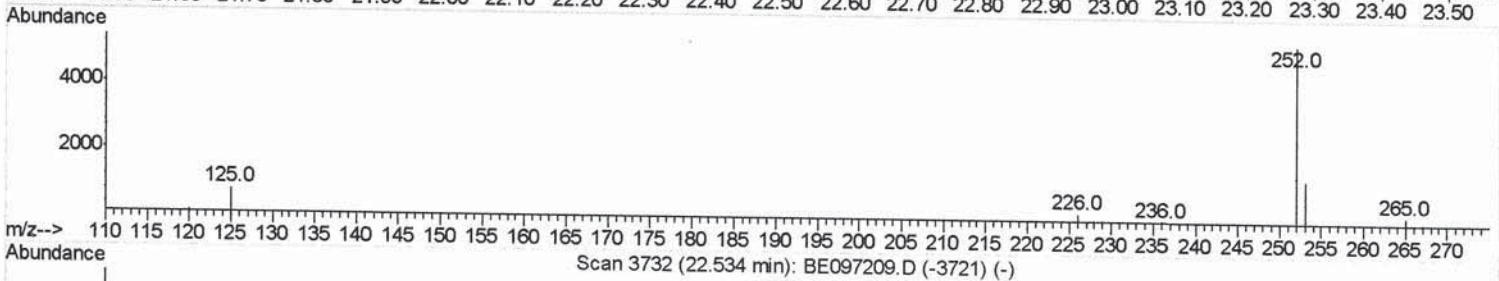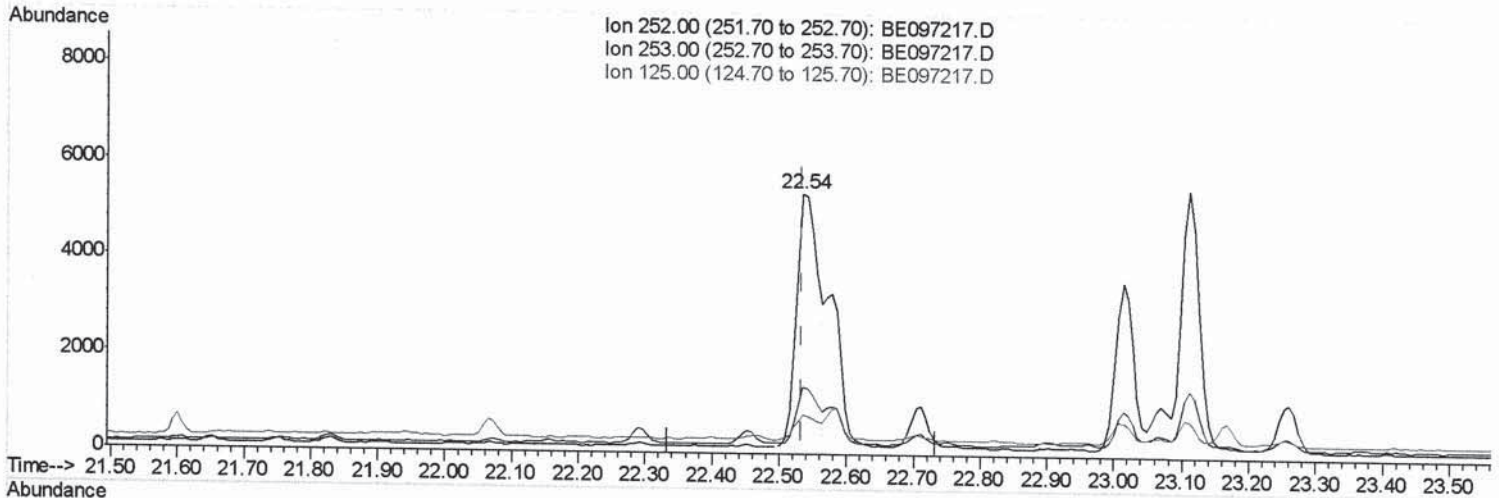

(21) Benzo(b)fluoranthene

22.535min (+0.001) 0.41ng/ul m

SJ 8/7/18

response 11943

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	25.47
125.00	17.50	14.79
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097217.D
 Acq On : 5 Aug 2018 1:32
 Operator : SJ/JU
 Sample : J4171-21DL 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L4DL

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:51:05 PM

Quant Time: Aug 06 04:47:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

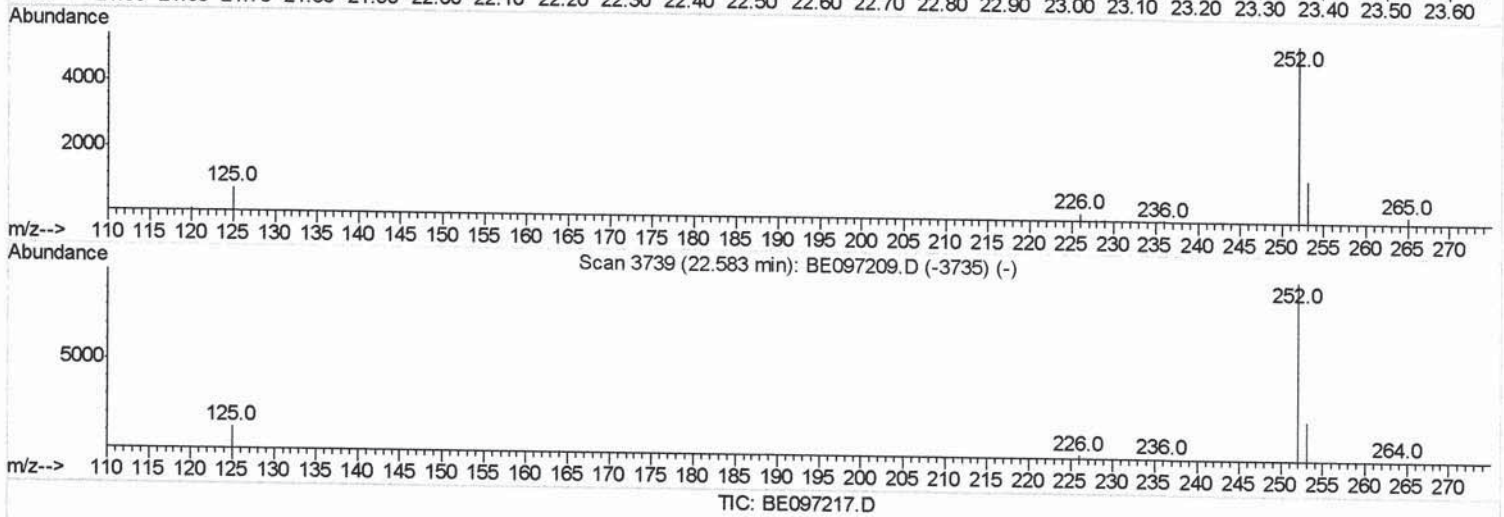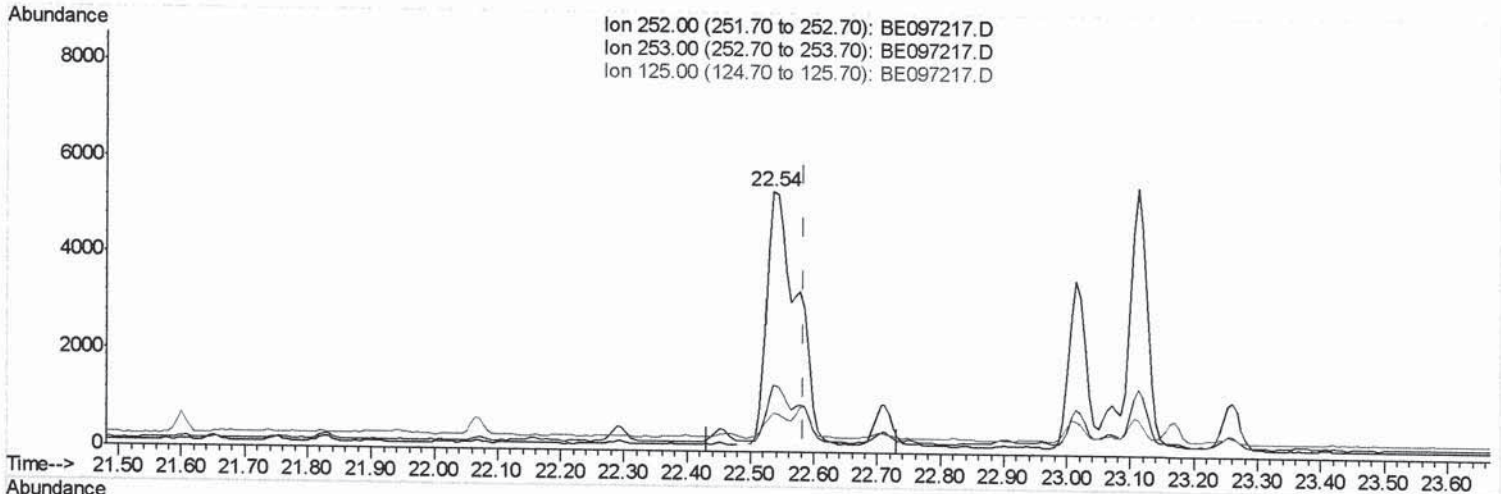

(22) Benzo(k)fluoranthene
 22.535min (-0.048) 0.55ng/ul
 response 17322

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	25.47
125.00	17.10	14.79
0.00	0.00	0.00

Quantitation Report (Qedit)



Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
Data File : BE097217.D
Acq On : 5 Aug 2018 1:32
Operator : SJ/JU
Sample : J4171-21DL 2X
Misc :
ALS Vial : 24 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
JJ1L4DL

Manual Integrations
APPROVED

Sohil
8/6/2018 12:51:05 PM

Quant Time: Aug 06 04:47:13 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 03:46:27 2018
Response via : Initial Calibration

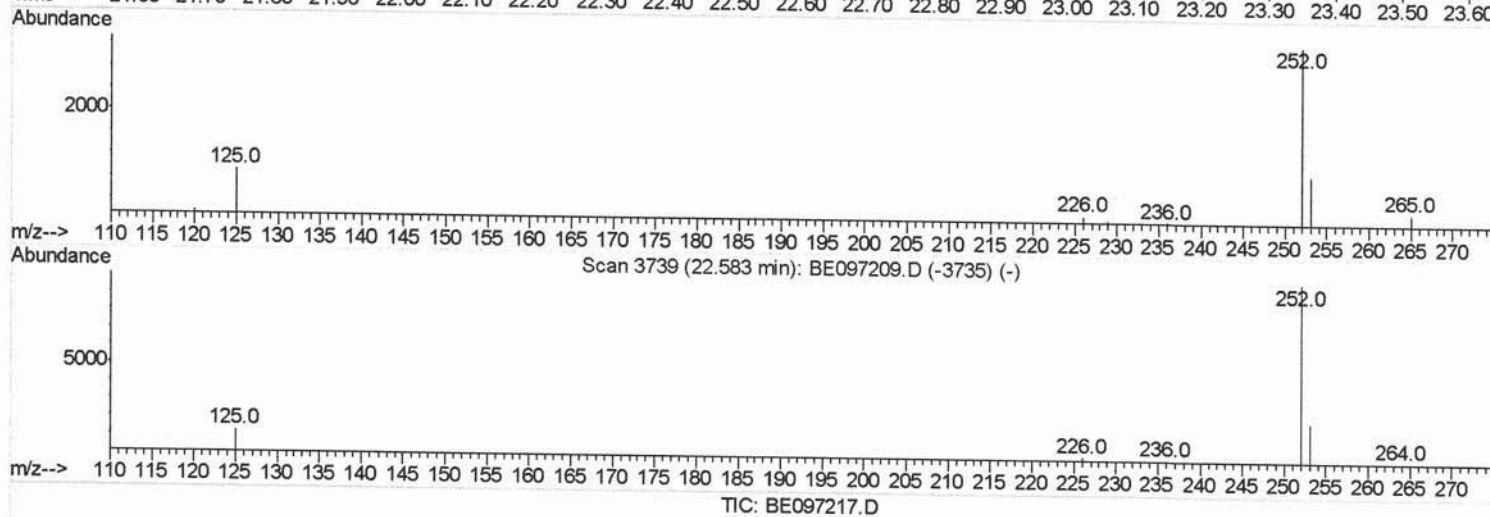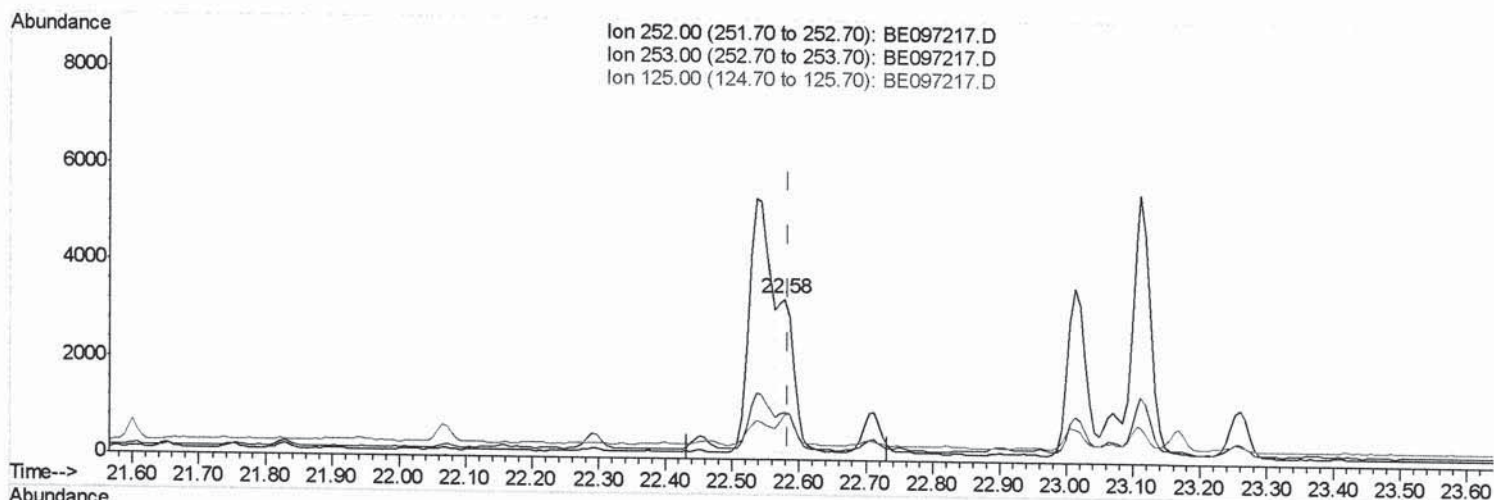

(22) Benzo(k)fluoranthene

22.577min (-0.006) 0.16ng/ul m

SJ 8/7/18

response 5103

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	29.67
125.00	17.10	27.74#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097217.D
 Acq On : 5 Aug 2018 1:32
 Operator : SJ/JU
 Sample : J4171-21DL 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L4DL

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:51:05 PM

Quant Time: Aug 06 04:47:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

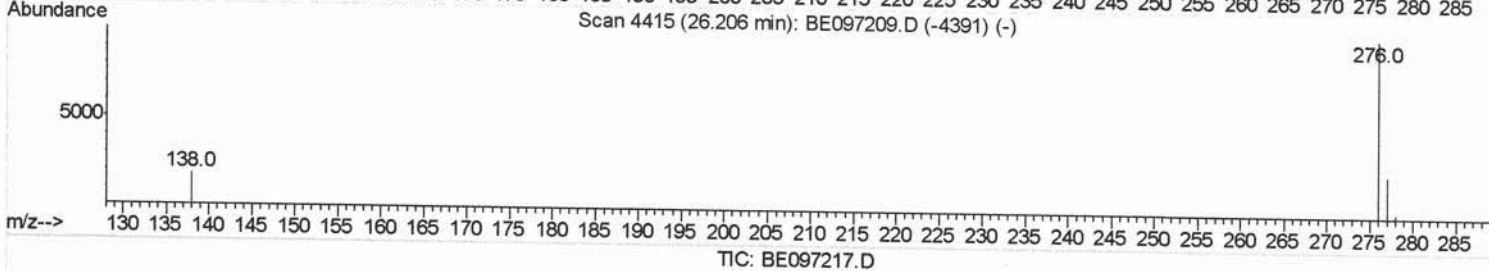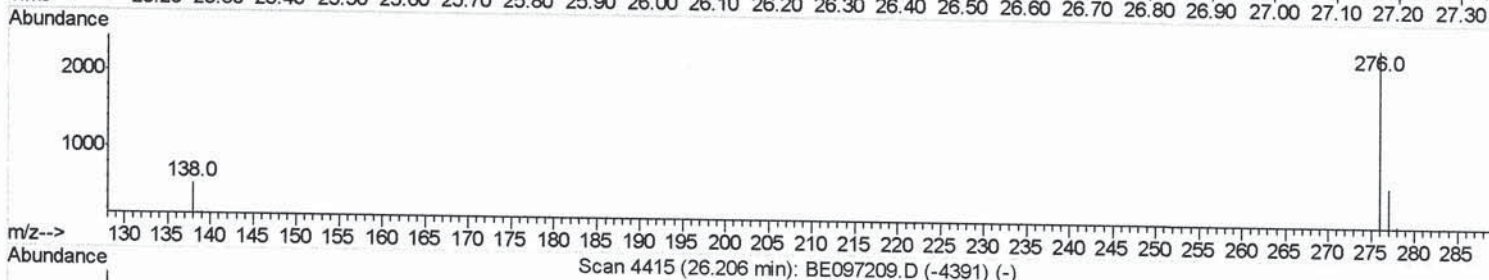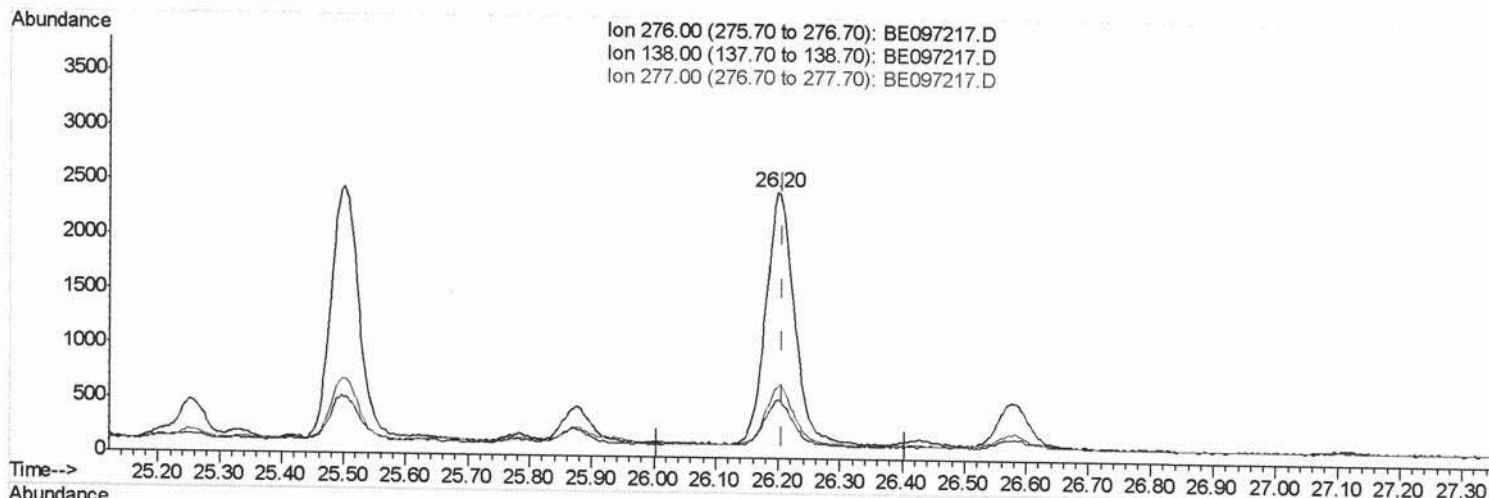

(26) Benzo(g,h,i)perylene
 26.198min (-0.008) 0.24ng/ul
 response 7438

Ion	Exp%	Act%
276.00	100	100
138.00	27.30	21.94
277.00	25.60	26.61
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080418\
 Data File : BE097217.D
 Acq On : 5 Aug 2018 1:32
 Operator : SJ/JU
 Sample : J4171-21DL 2X
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 JJ1L4DL

Manual Integrations
 APPROVED

Sohil
 8/6/2018 12:51:05 PM

Quant Time: Aug 06 04:51:04 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 03:46:27 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1467	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	7666	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	4648	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.77	188	10935m	0.40	ng/ul	0.00
16) Chrysene-d12	20.97	240	11323m	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	10673m	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.72	152	2007	0.16	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	6029m	0.16	ng/ul	0.00

Target Compounds

					Ovalue	
7) Acenaphthylene	13.73	152	1174	0.058	ng/ul#	89
9) Fluorene	15.08	166	437	0.026	ng/ul#	87
12) Phenanthrene	16.81	178	16967m	0.609	ng/ul	> SJ 8/7/18
15) Fluoranthene	18.84	202	23913m	0.649	ng/ul	
17) Pyrene	19.21	202	25012	0.824	ng/ul#	78
18) Benzo(a)anthracene	20.96	228	6368	0.197	ng/ul#	82
19) Chrysene	21.01	228	11312	0.339	ng/ul	97
21) Benzo(b)fluoranthene	22.54	252	11943m	0.411	ng/ul	> SJ 8/7/18
22) Benzo(k)fluoranthene	22.58	252	5103m	0.163	ng/ul	
23) Benzo(a)pyrene	23.11	252	9676	0.332	ng/ul#	82
24) Indeno(1,2,3-cd)pyrene	25.50	276	7276	0.200	ng/ul#	72
25) Dibenzo(a,h)anthracene	25.52	278	1540	0.052	ng/ul#	68
26) Benzo(a,h,i)perylene	26.20	276	7438	0.236	ng/ul	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed