

Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE080618\
 Data File : BE097223.D
 Acq On : 6 Aug 2018 13:00
 Operator : SJ/JU
 Sample : J4265-13DL 2X
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB5DL

Manual Integrations
 APPROVED

Sohil
 8/7/2018 6:58:29 PM

Quant Time: Aug 06 17:34:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Aug 06 17:09:49 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1169	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6268	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	3948	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.77	188	9261m	0.40	ng/ul	0.00
16) Chrysene-d12	20.97	240	9255m	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	8383m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.73	152	2040	0.20	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	5810m	0.18	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.18	128	19236	1.267	ng/ul#	Qvalue 91

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE080618\
Data File : BE097223.D
Acq On : 6 Aug 2018 13:00
Operator : SJ/JU
Sample : J4265-13DL 2X
Misc :
ALS Vial : 5 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
C0AB5DL

Manual Integrations
APPROVED

Sohil
8/7/2018 6:58:29 PM

Quant Time: Aug 06 17:34:10 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Aug 06 17:09:49 2018
Response via : Initial Calibration

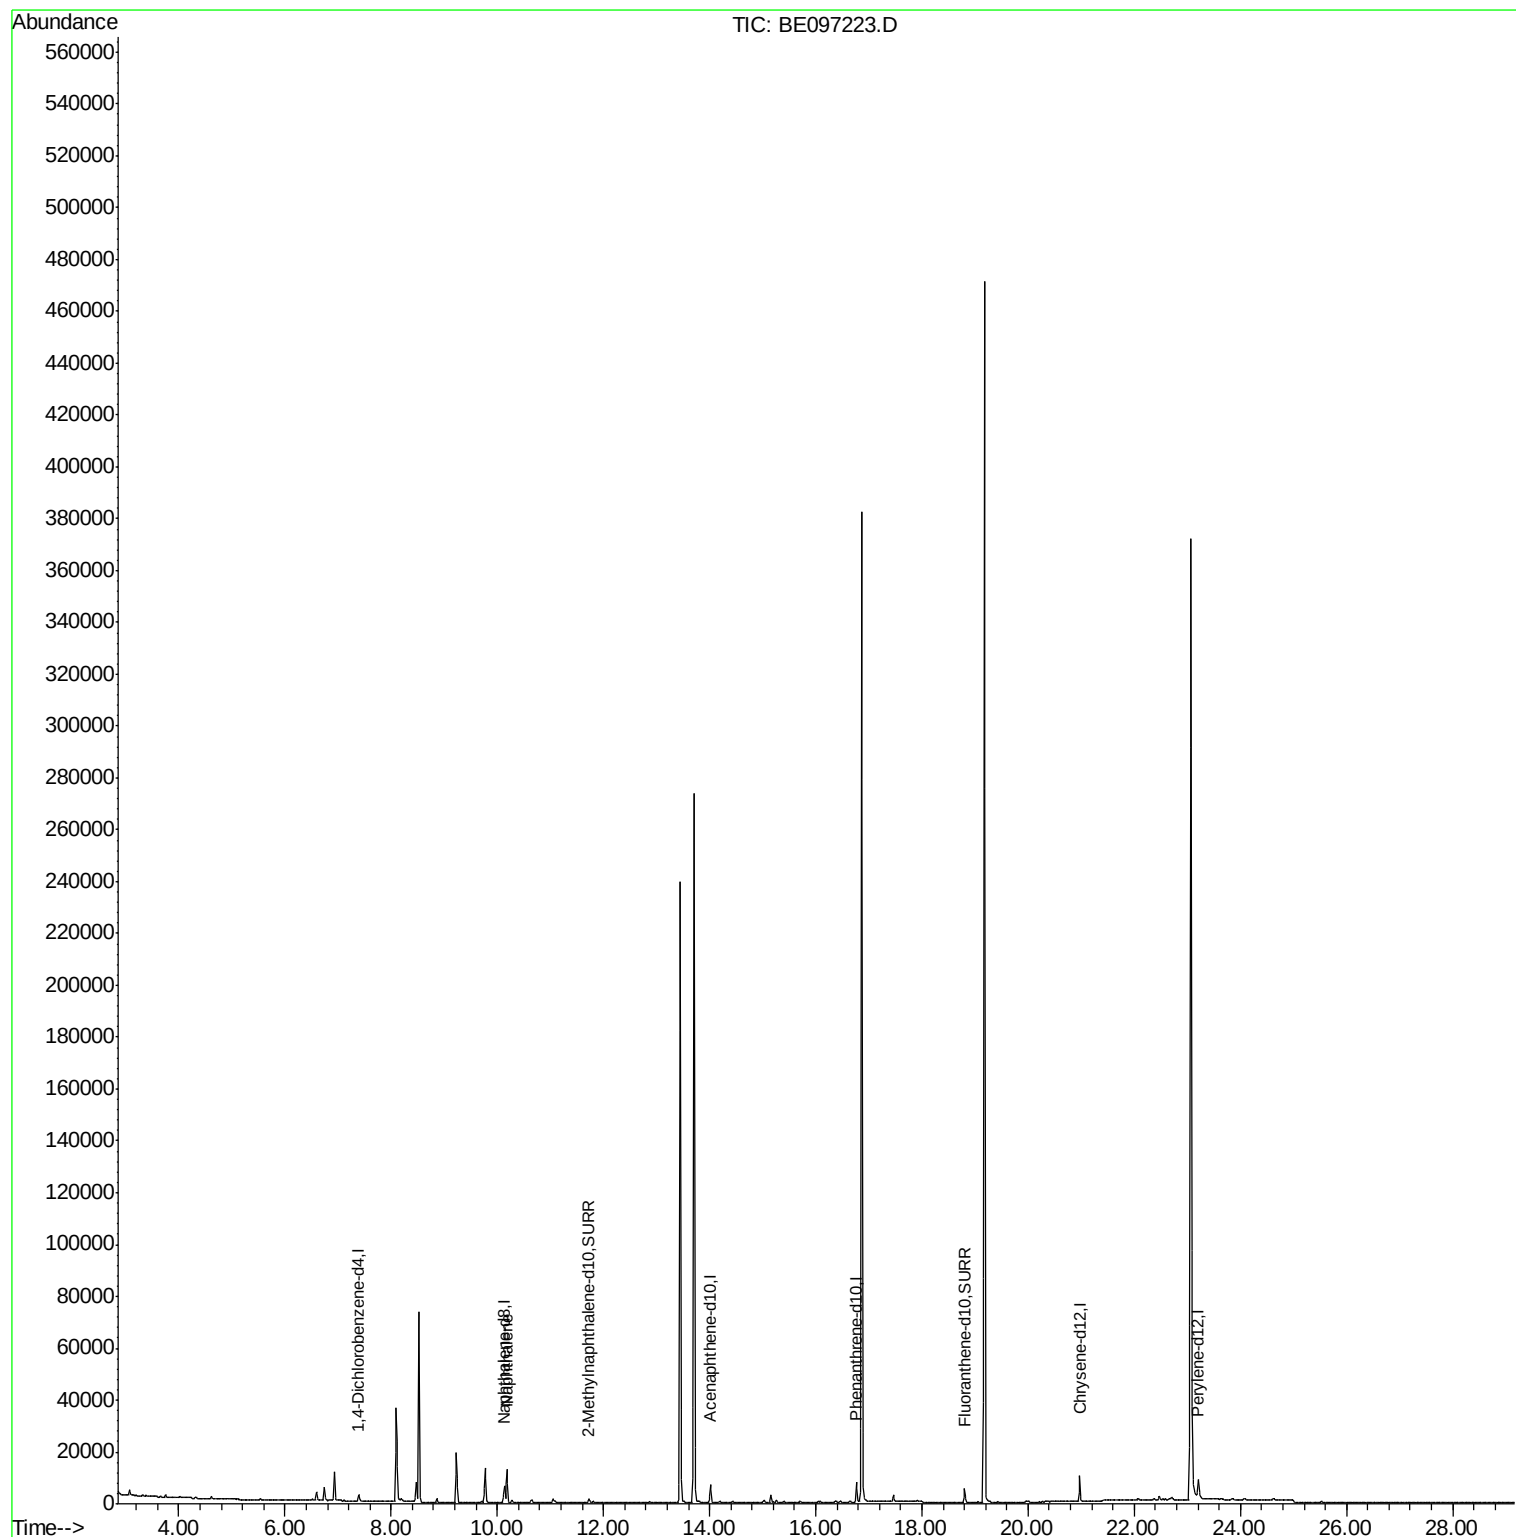

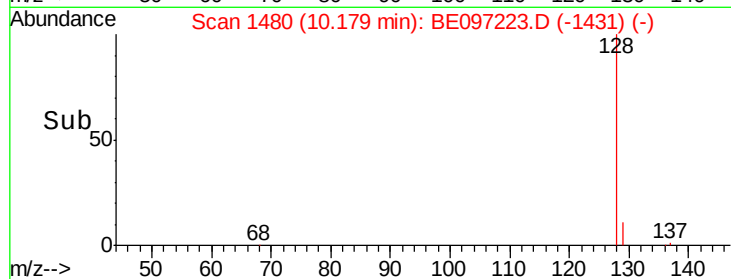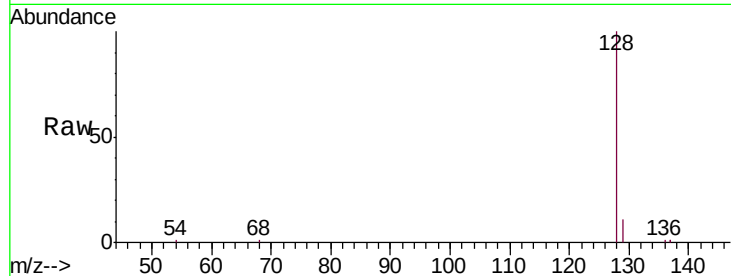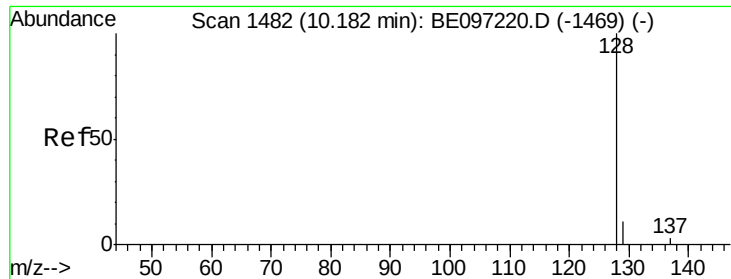

#3

Naphthalene

Concen: 1.267 ng/ul

RT: 10.18 min Scan# 1480

Delta R.T. -0.00 min

Lab File: BE097223.D

Acq: 6 Aug 2018 13:00

Instrument :

BNA_E

ClientSampleId :

C0AB5DL

Tgt Ion:	128	Resp:	19236
Ion Ratio	Lower	Upper	
128	100		
129	11.4	11.3	16.9
127	0.0	4.0	6.0

Manual Integrations
APPROVED

Sohil
8/7/2018 6:58:29 PM

