

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097227.D
 Acq On : 8 Aug 2018 10:03
 Operator : SJ/JU
 Sample : PB111793BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 08 23:26:16 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1154	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6302	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	3947	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	767608	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.97
20) Perylene-d12	23.21	264	14729	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.72	152	3606	0.36	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.02	166	1165	0.082	ng/ul#	21
23) Benzo(a)pyrene	23.08	252	2919	0.073	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097227.D
Acq On : 8 Aug 2018 10:03
Operator : SJ/JU
Sample : PB111793BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 08 23:26:16 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

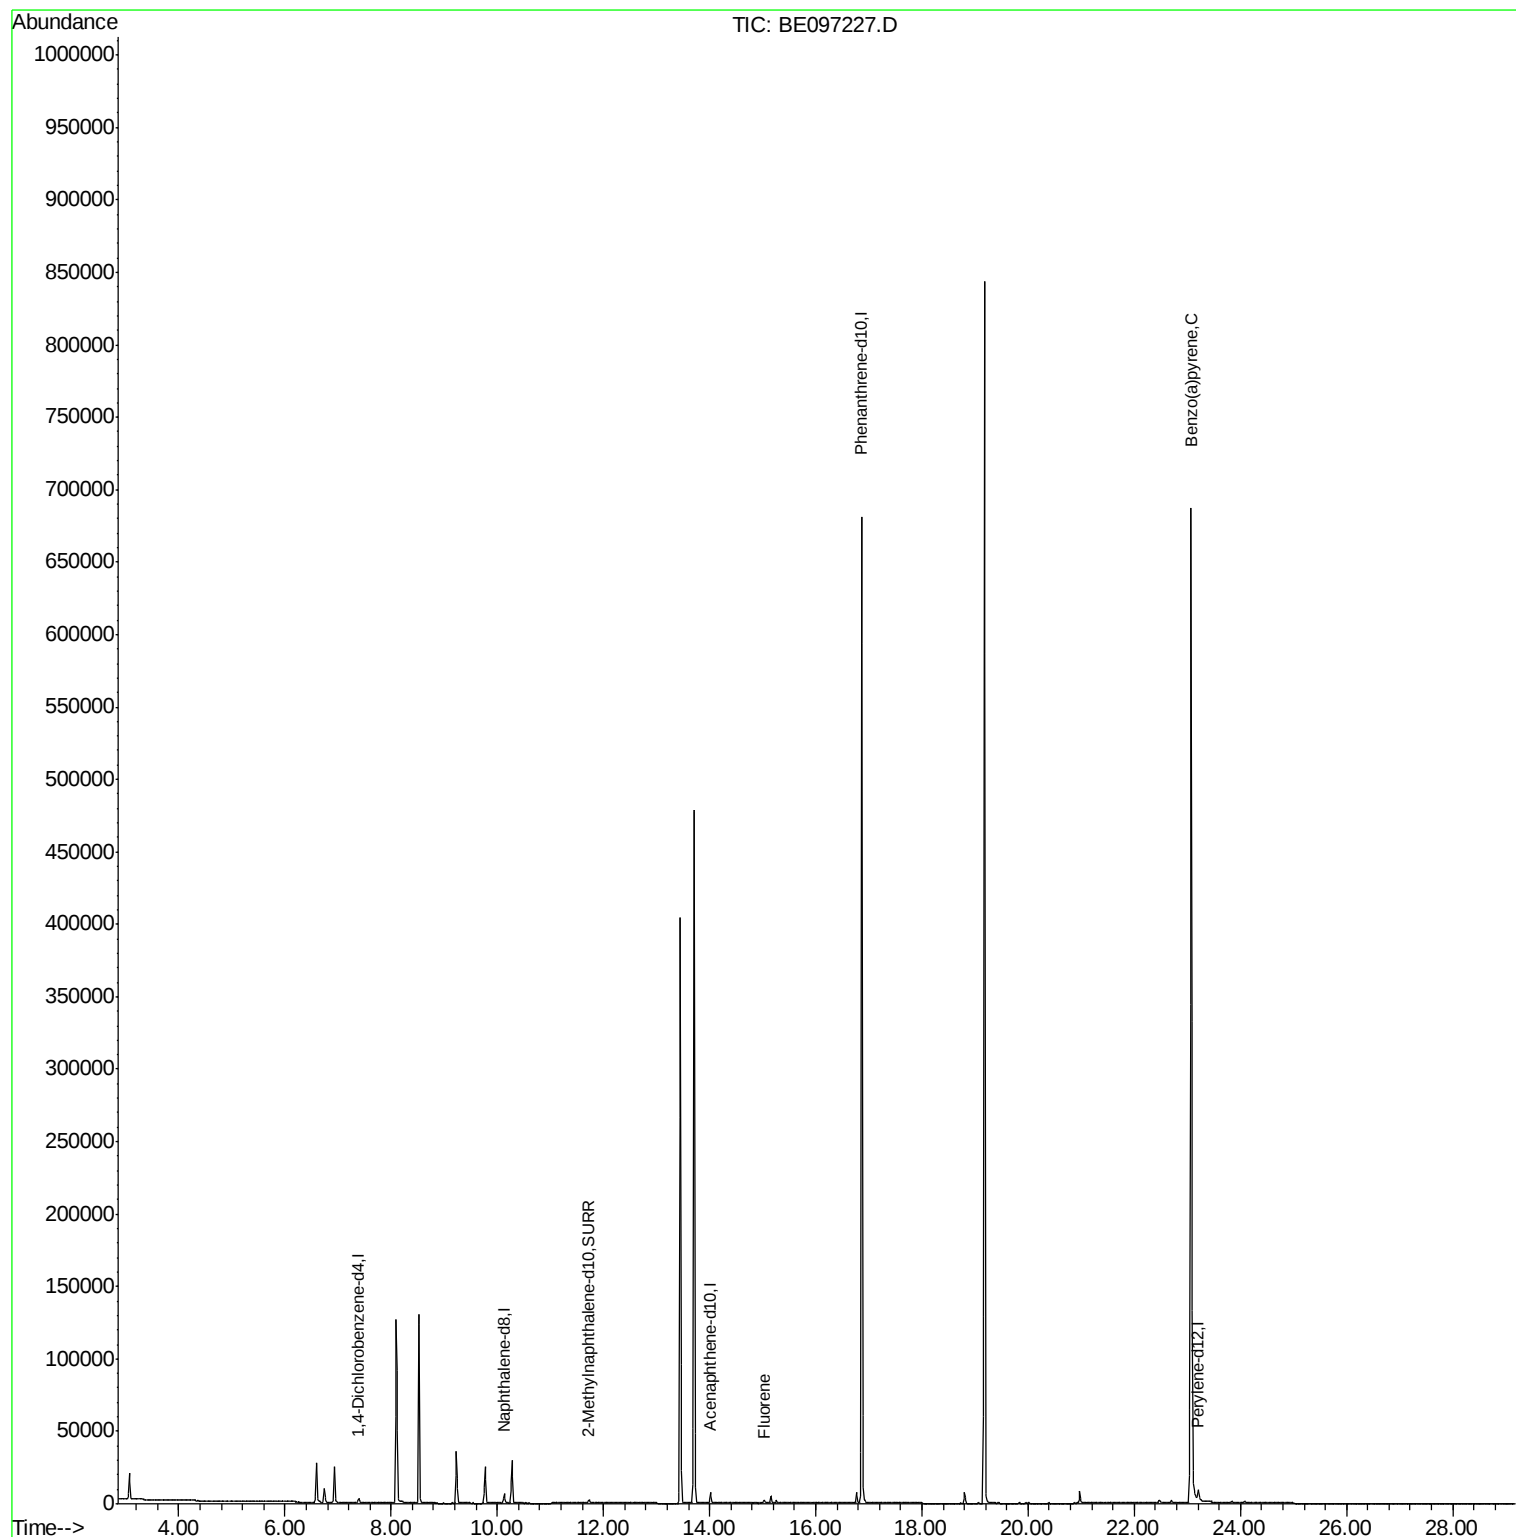

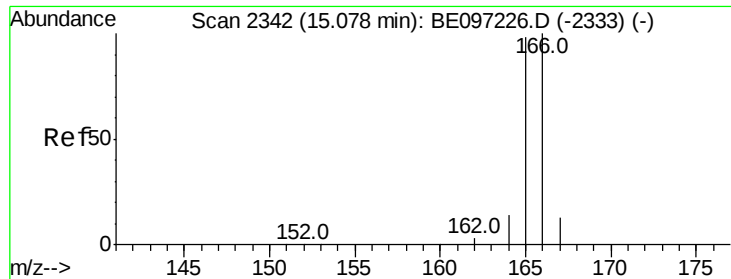

#9

Fluorene

Concen: 0.082 ng/ul

RT: 15.02 min Scan# 2333

Delta R.T. -0.05 min

Lab File: BE097227.D

Acq: 8 Aug 2018 10:03

Instrument :

BNA_E

ClientSampleId :





Tot Ion:166 Resp: 1165

Ion Ratio Lower Upper

166 100

165 9.1 73.4 110.2#

167 36.6 14.6 22.0#

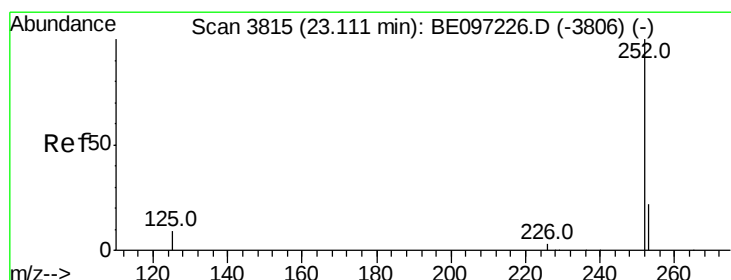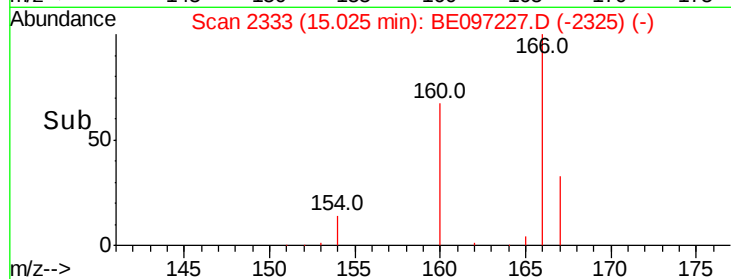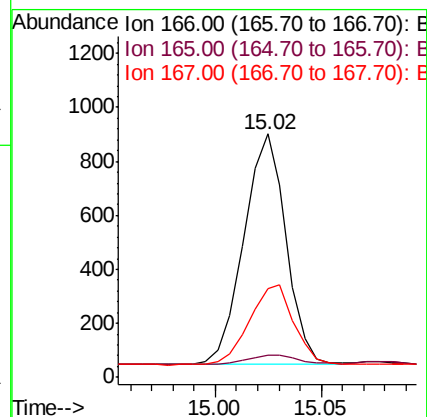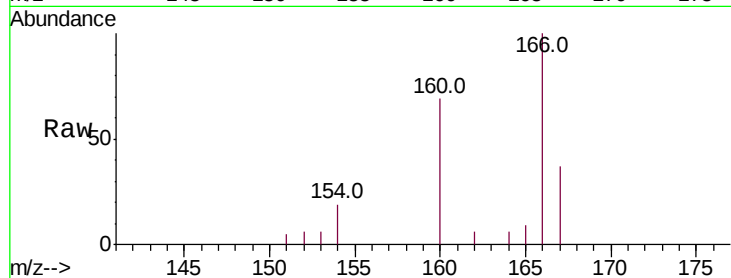

#23

Benzo(a)pyrene

Concen: 0.073 ng/ul

RT: 23.08 min Scan# 3809

Delta R.T. -0.04 min

Lab File: BE097227.D

Acq: 8 Aug 2018 10:03

Tgt Ion:252 Resp: 2919

Ion Ratio Lower Upper

252 100

253 36.5 28.5 42.7

125 22.0 18.1 27.1

