

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097230.D
 Acq On : 8 Aug 2018 11:57
 Operator : SJ/JU
 Sample : PB111788BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 08 23:26:28 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1206	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6517	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	4357	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.87	188	1393731	0.40	ng/ul	0.11
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.97
20) Perylene-d12	23.21	264	16612	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.72	152	5417	0.52	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
23) Benzo(a)pyrene	23.08	252	5991	0.132	ng/ul	Ovalue 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097230.D
Acq On : 8 Aug 2018 11:57
Operator : SJ/JU
Sample : PB111788BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 08 23:26:28 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

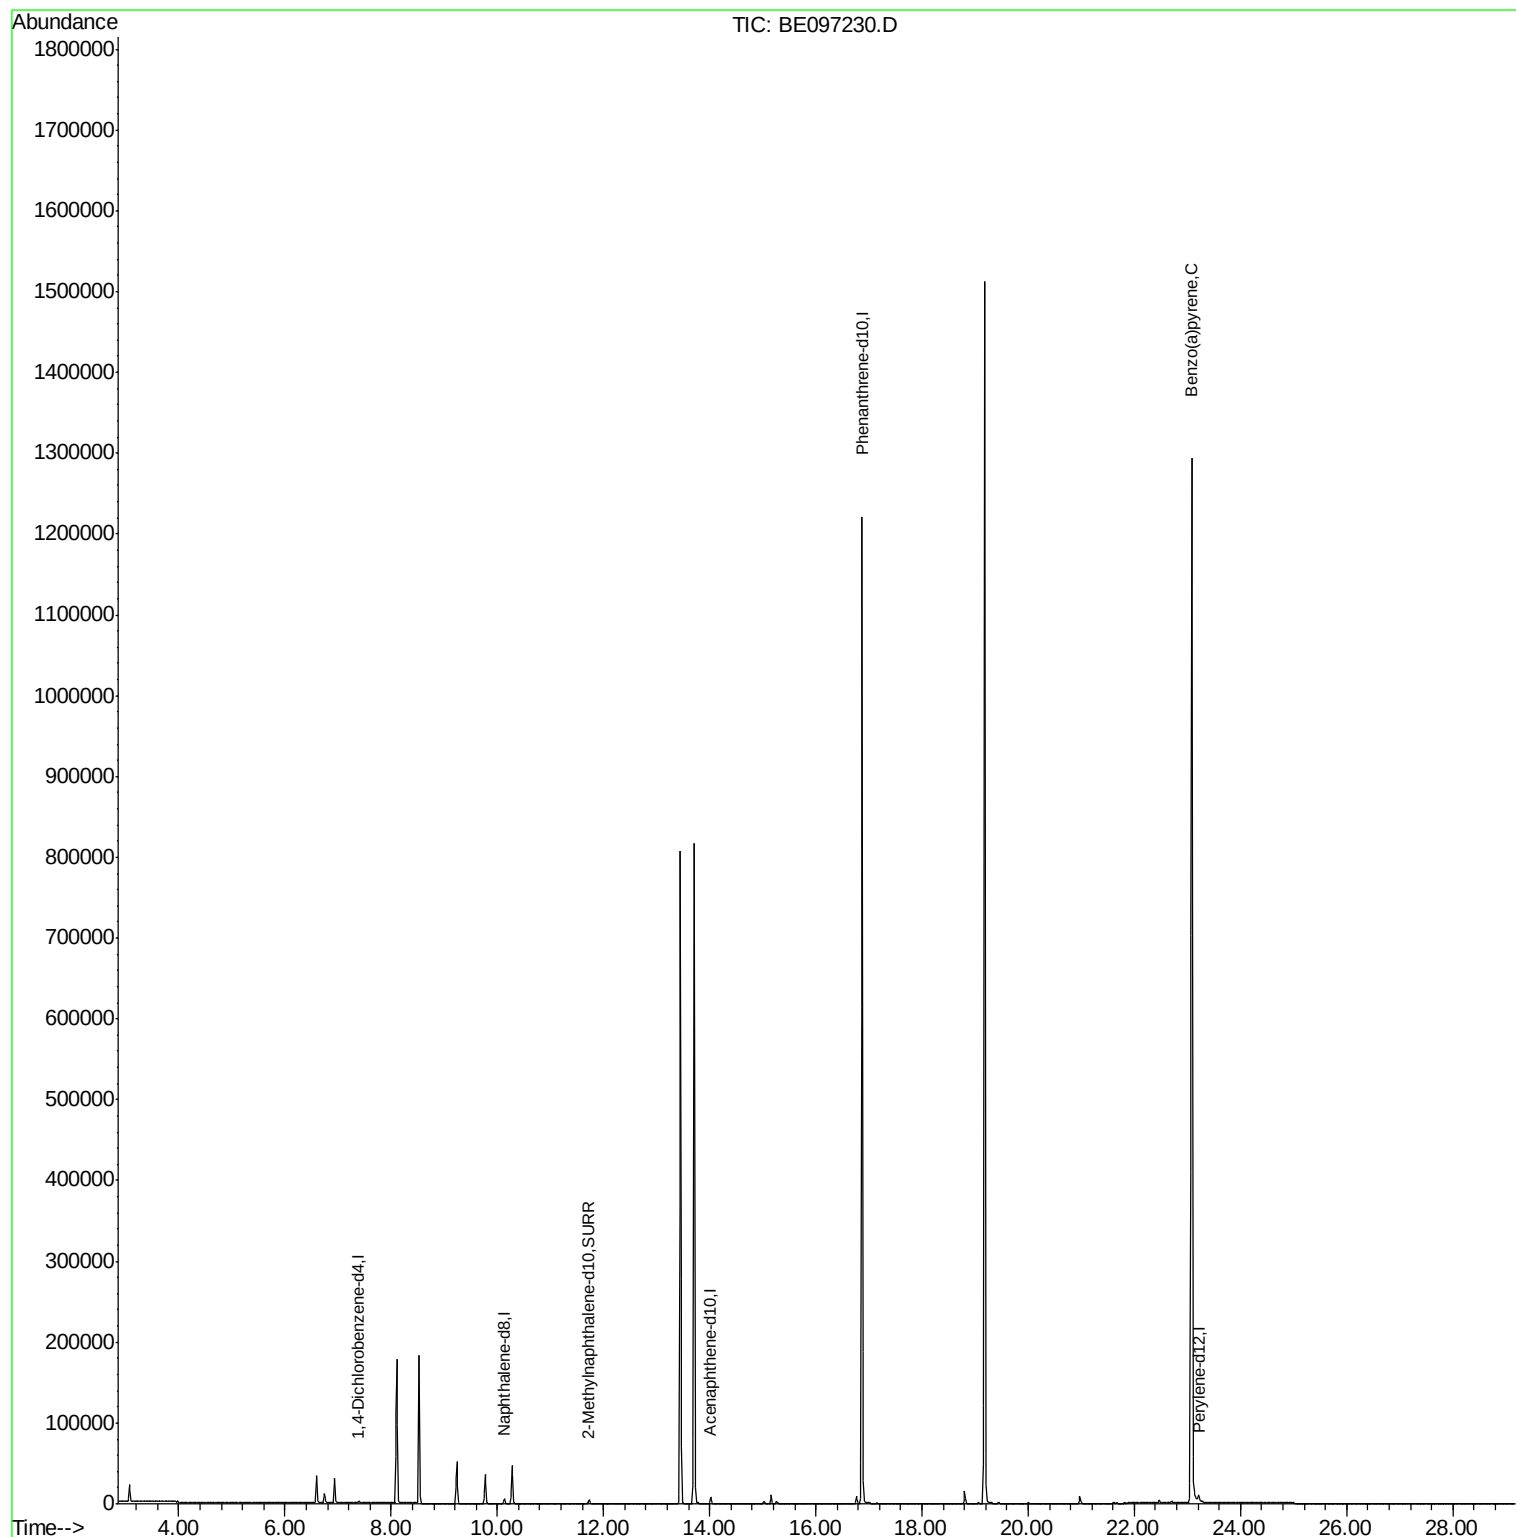

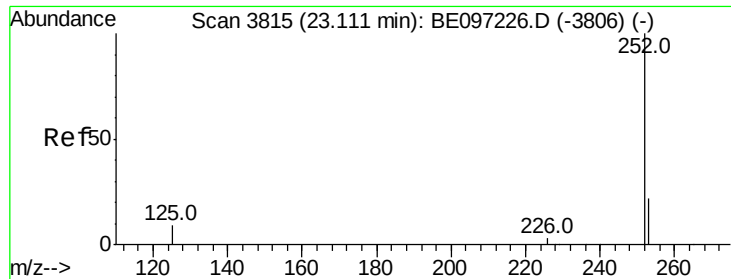

#23

Benzo(a)pyrene

Concen: 0.132 ng/ul

RT: 23.08 min Scan# 3811

Delta R.T. -0.03 min


Lab File: BE097230.D

Acq: 8 Aug 2018 11:57

Instrument :

BNA_E

ClientSampleId :

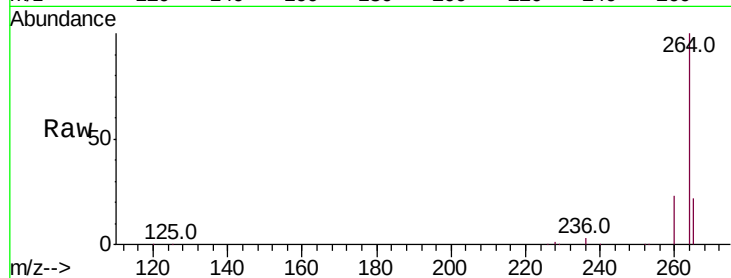

Tot Ion: 252 Resp: 5991

Ion Ratio Lower Upper

252 100

253 34.7 28.5 42.7

125 19.2 18.1 27.1

