

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097234.D
 Acq On : 8 Aug 2018 14:26
 Operator : SJ/JU
 Sample : J4268-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:39:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

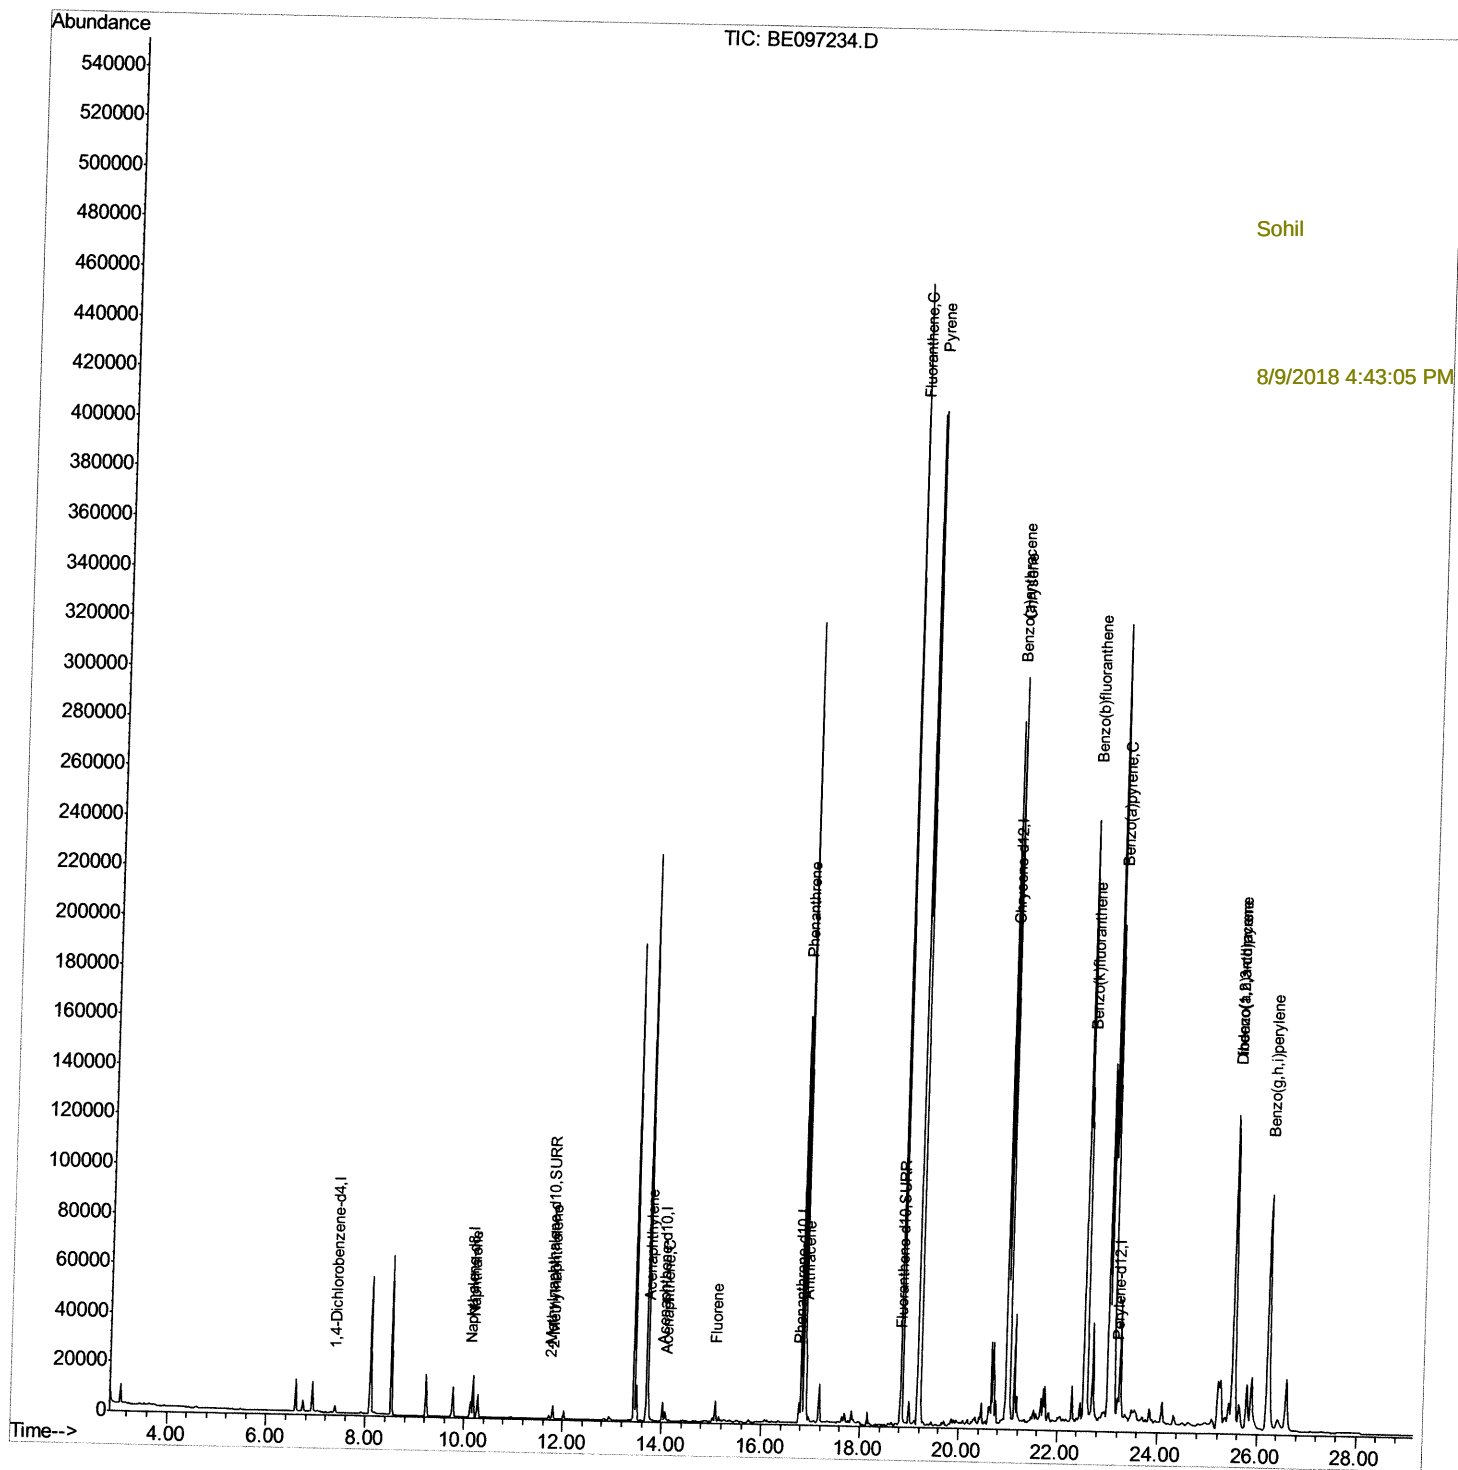

Sohil

8/9/2018 4:43:05 PM

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097234.D
Acq On : 8 Aug 2018 14:26
Operator : SJ/JU
Sample : J4268-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AC6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:05 PM

Quant Time: Aug 08 23:26:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

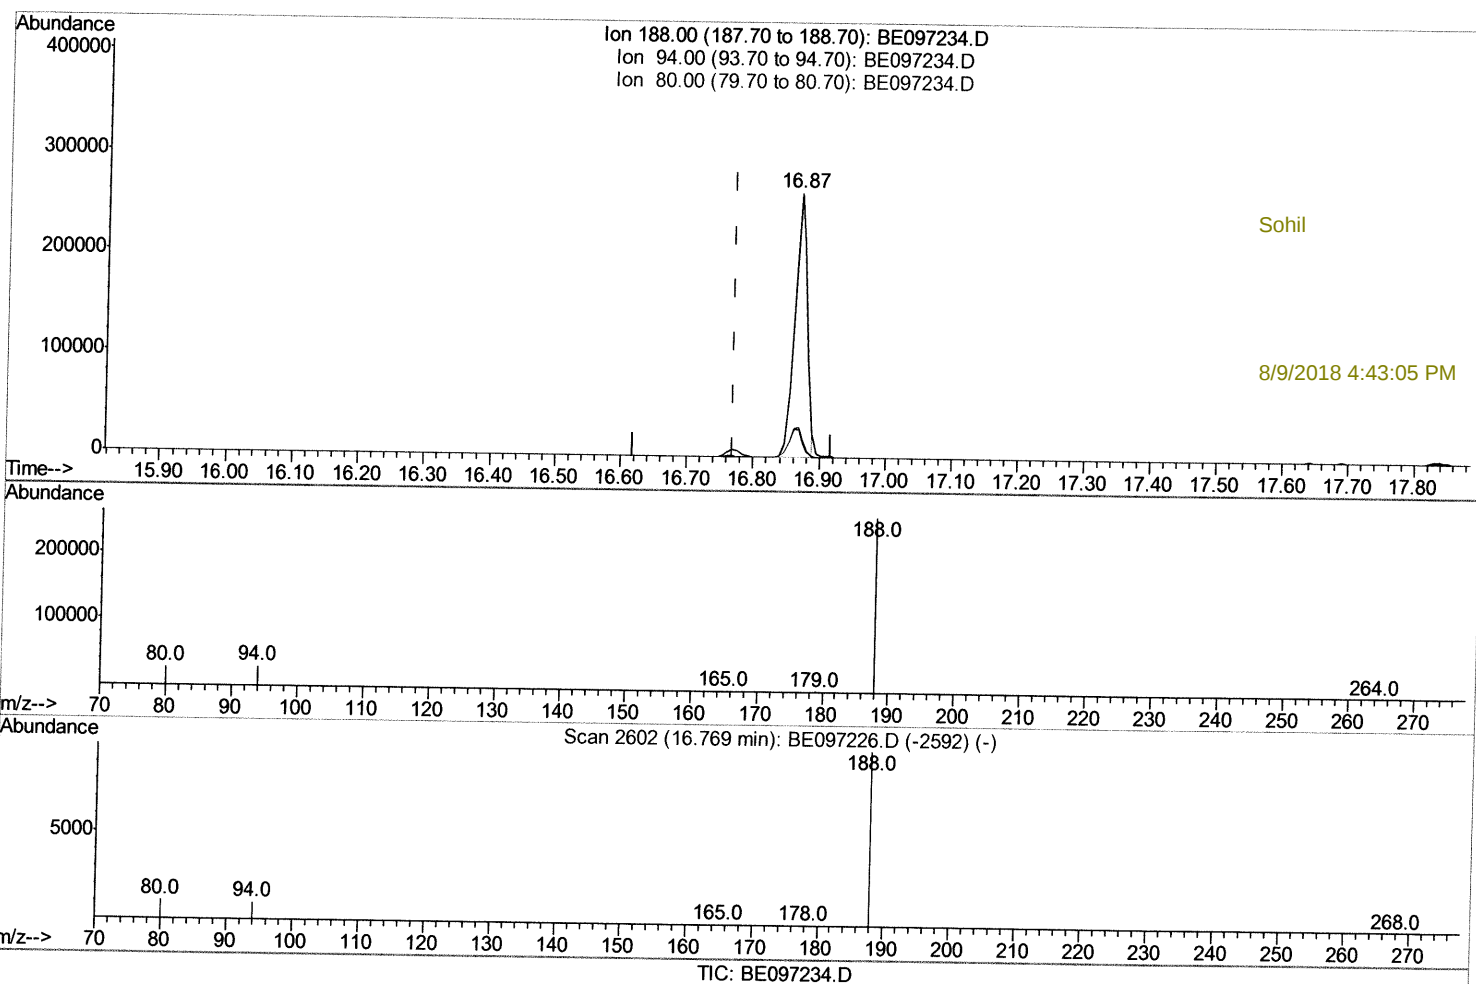

(10) Phenanthrene-d10 (I)

16.867min (+0.099) 0.40ng/ul

response 355226

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.29
80.00	11.80	10.47
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097234.D
Acq On : 8 Aug 2018 14:26
Operator : SJ/JU
Sample : J4268-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AC6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:05 PM

Quant Time: Aug 08 23:26:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

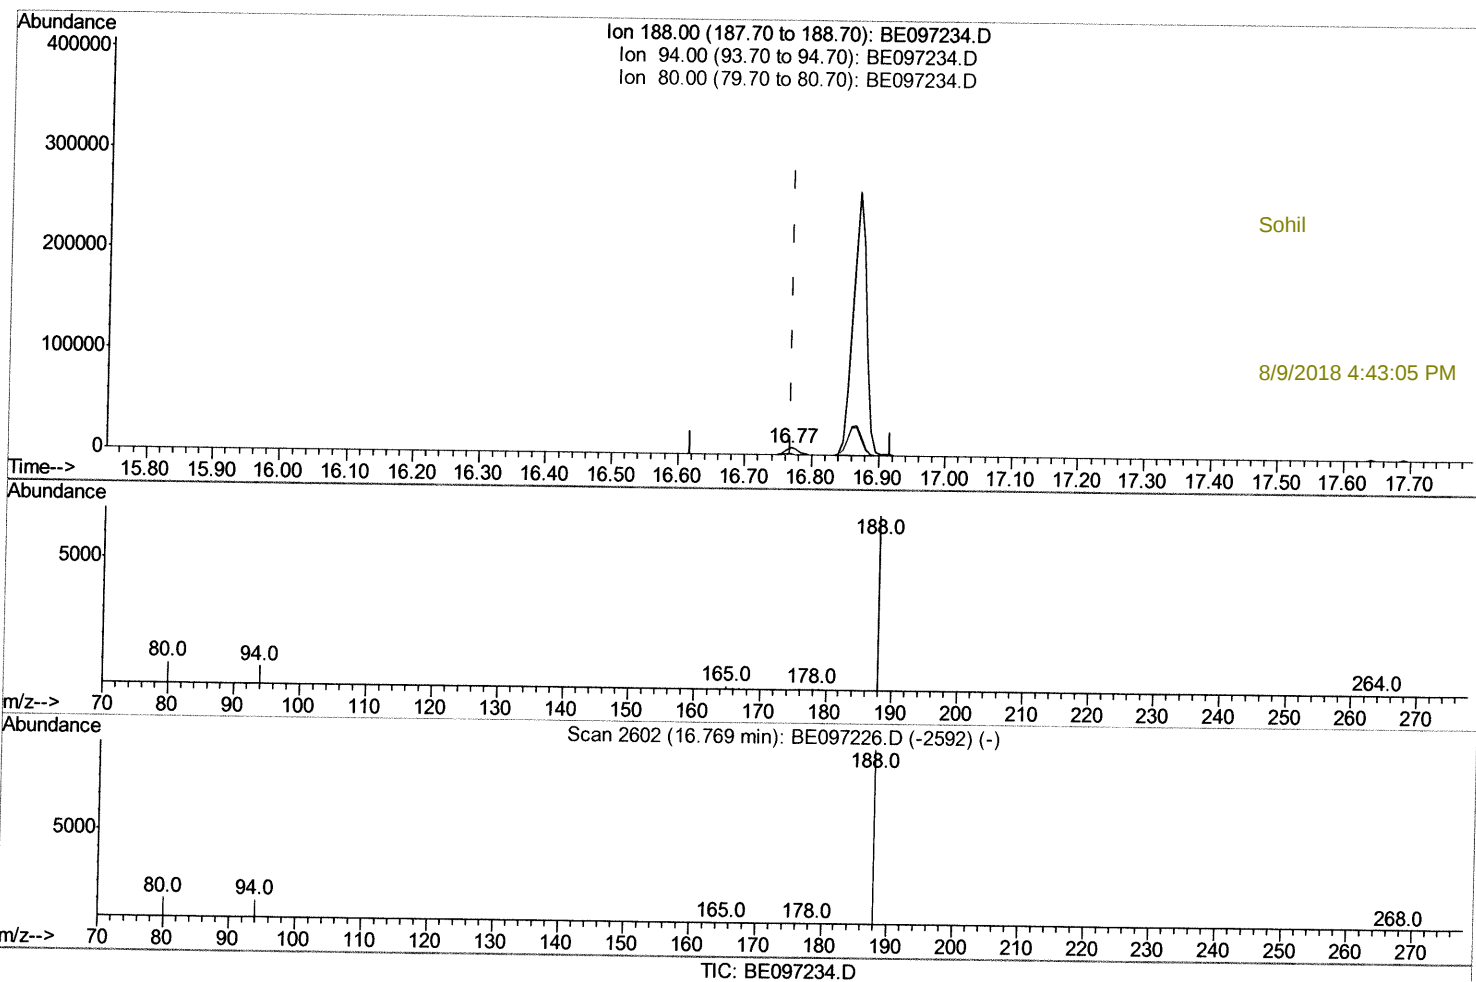

(10) Phenanthrene-d10 (I)

16.769min (0.000) 0.40ng/ul m> SJ 8/10/18

response 9545

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.73
80.00	11.80	12.34
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097234.D
 Acq On : 8 Aug 2018 14:26
 Operator : SJ/JU
 Sample : J4268-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC6

Manual Integrations
 APPROVED



Sohil
 8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:31:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

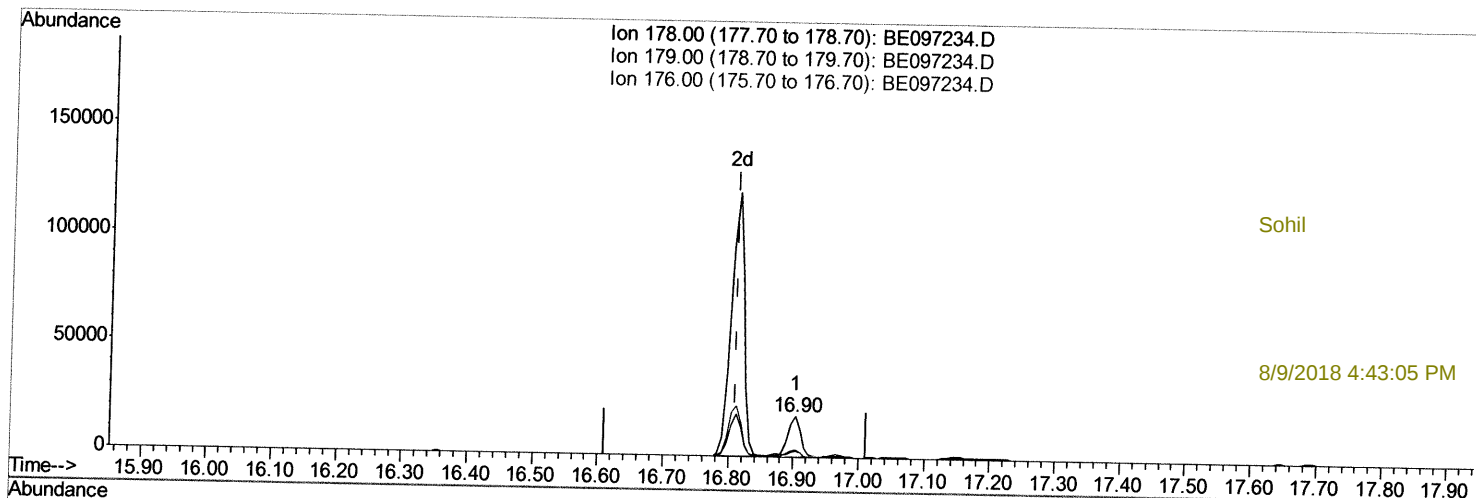

Sohil

8/9/2018 4:43:05 PM

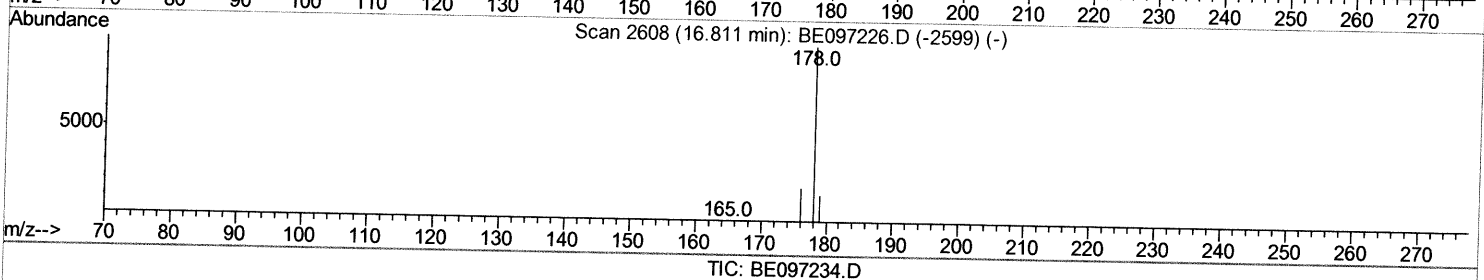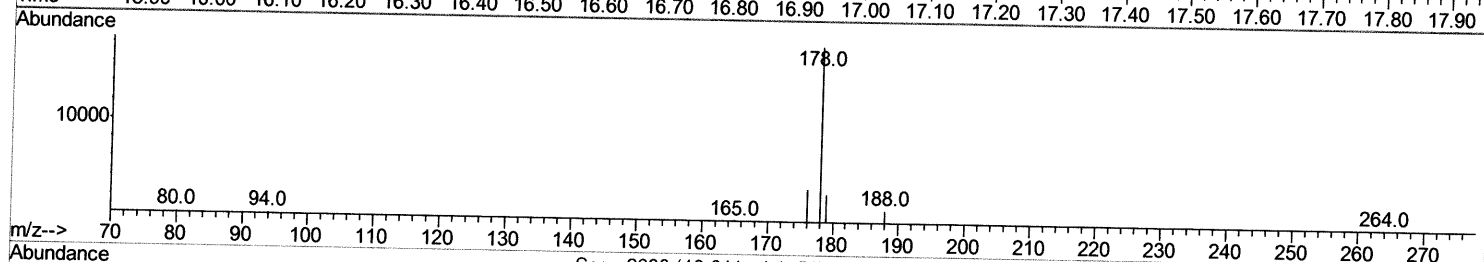

TIC: BE097234.D

(12) Phenanthrene

16.902min (+0.091) 1.02ng/ul

response 24837

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	15.98#
176.00	17.00	19.02
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097234.D
Acq On : 8 Aug 2018 14:26
Operator : SJ/JU
Sample : J4268-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AC6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:31:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

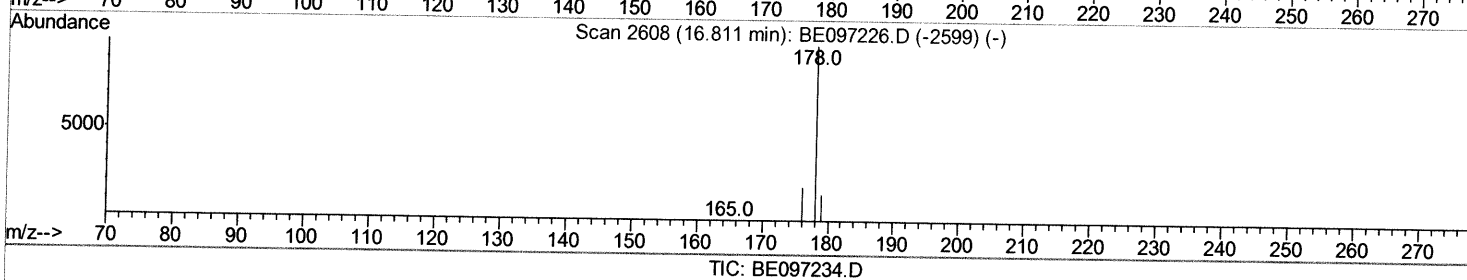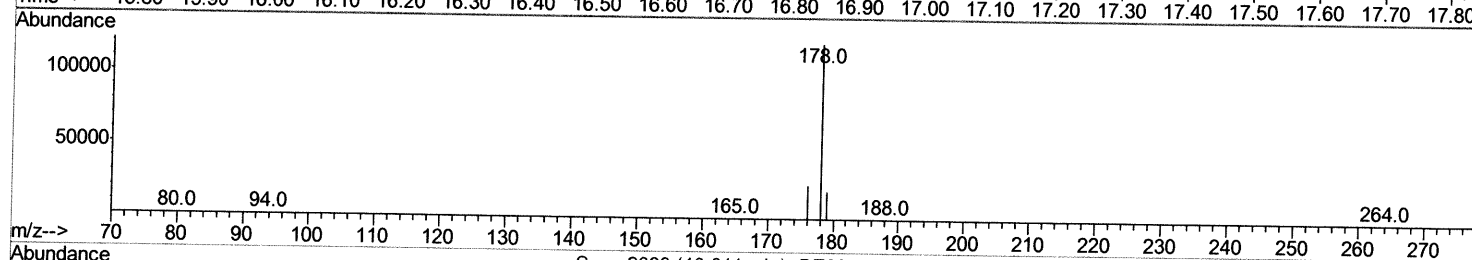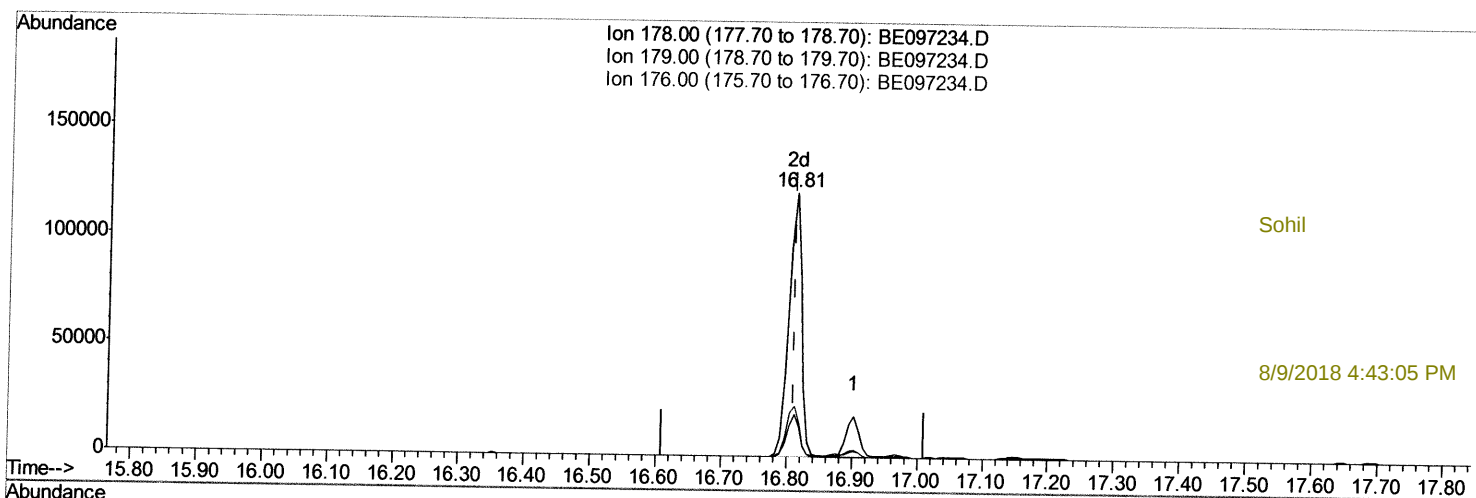

(12) Phenanthrene

16.811min (0.000) 6.71ng/ul m> SJ 8/10/18

response 163384

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	15.81#
176.00	17.00	19.28
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097234.D
 Acq On : 8 Aug 2018 14:26
 Operator : SJ/JU
 Sample : J4268-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC6

Manual Integrations
 APPROVED



Sohil
 8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:31:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

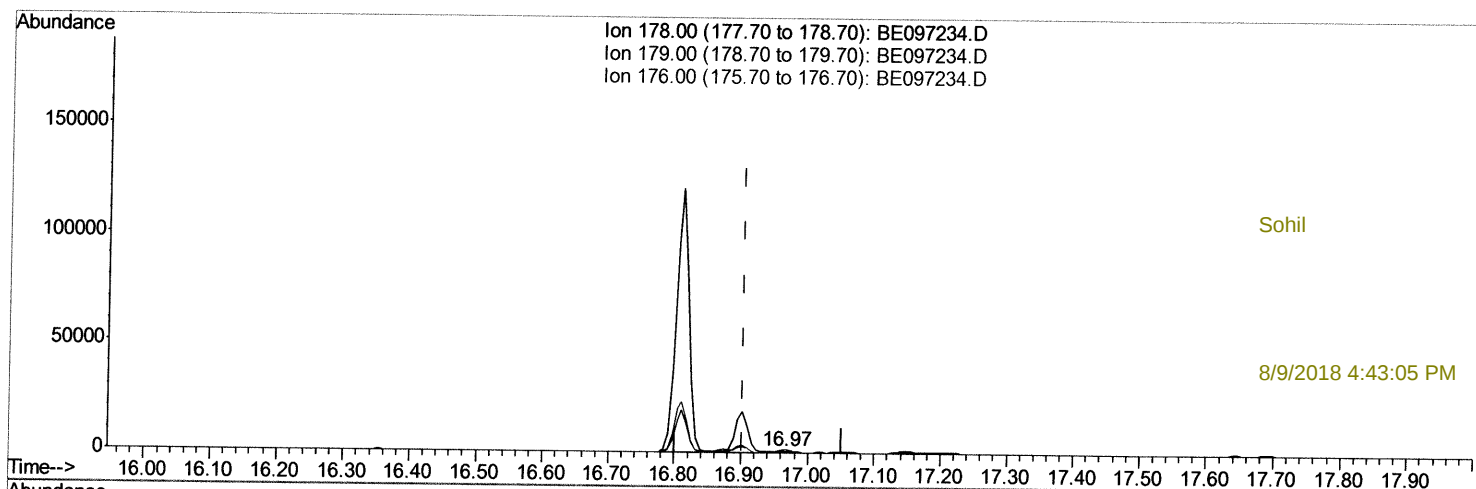

Sohil

8/9/2018 4:43:05 PM

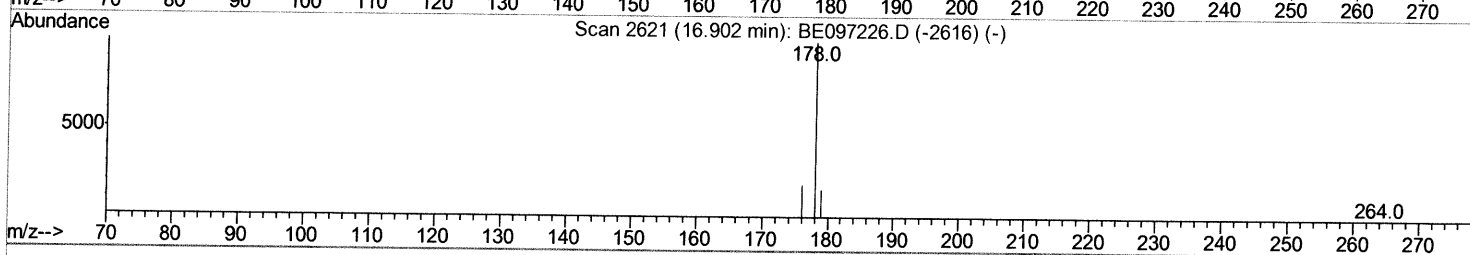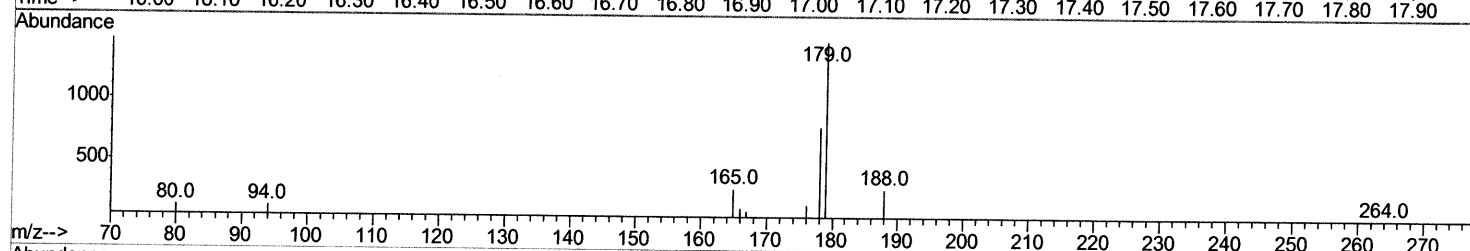

TIC: BE097234.D

(13) Anthracene

16.966min (+0.063) 0.04ng/ul

response 887

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	189.23#
176.00	18.40	18.46
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097234.D
 Acq On : 8 Aug 2018 14:26
 Operator : SJ/JU
 Sample : J4268-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AC6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:31:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

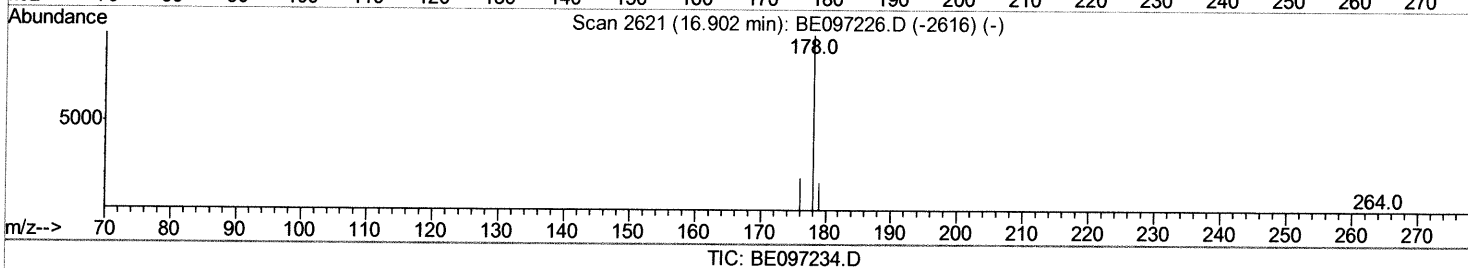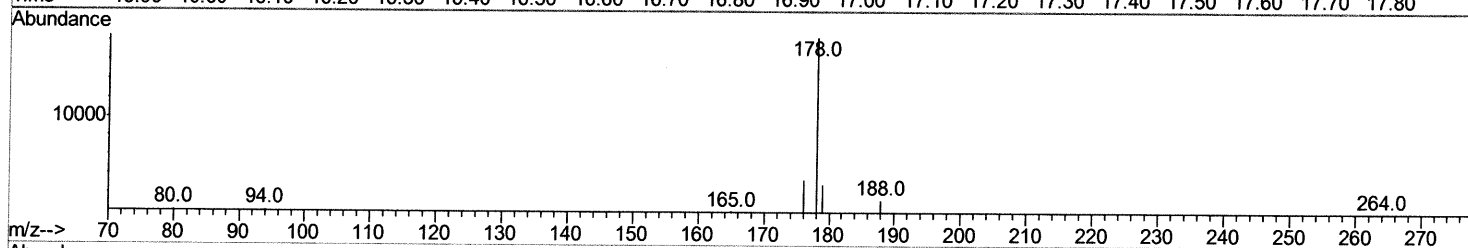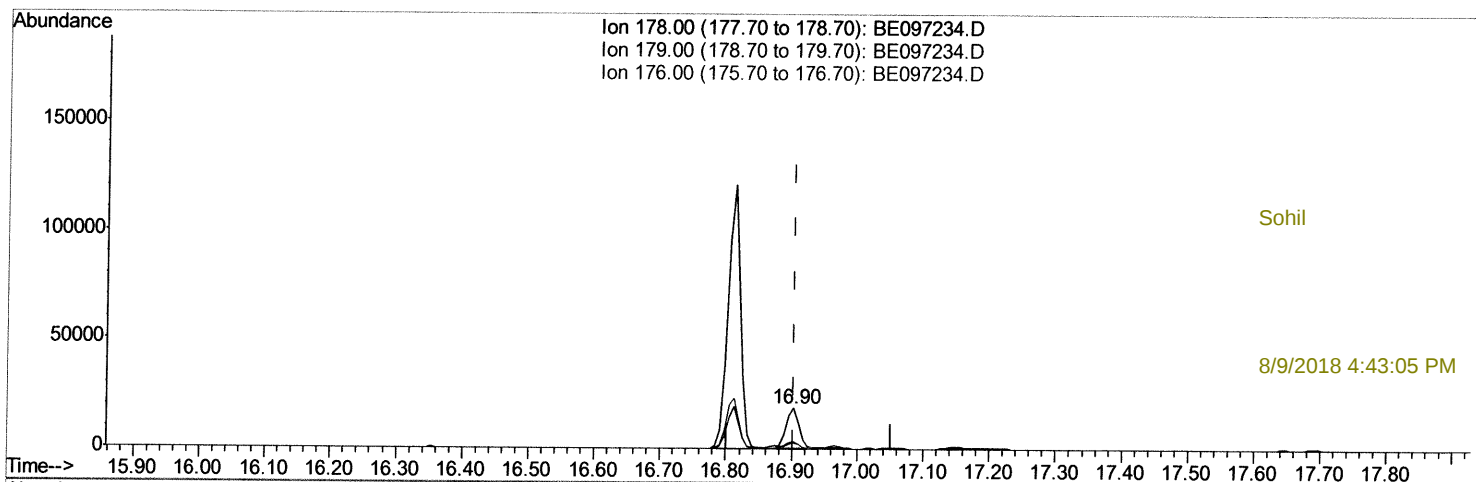

(13) Anthracene

16.902min (0.000) 1.07ng/ul m > SJ 8/10/18

response 24192

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	15.98#
176.00	18.40	19.02
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097234.D
 Acq On : 8 Aug 2018 14:26
 Operator : SJ/JU
 Sample : J4268-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:31:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

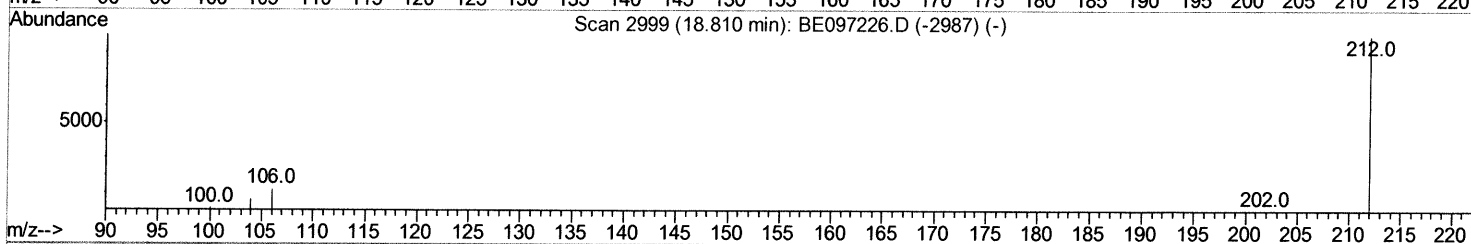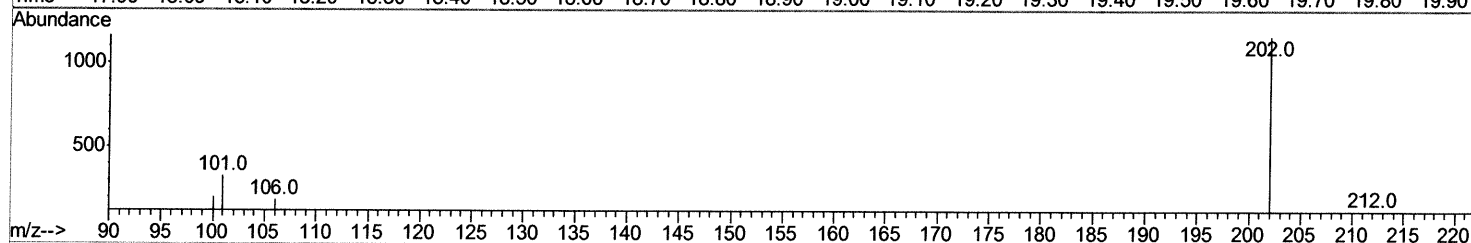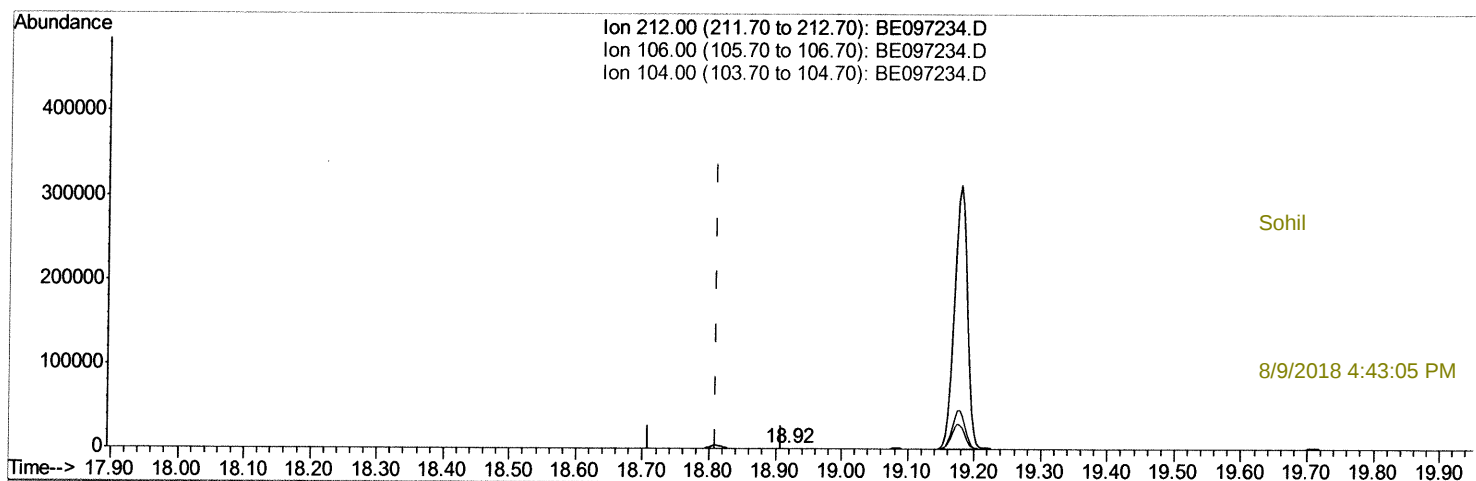

TIC: BE097234.D

(14) Fluoranthene-d10 (SURR)

18.917min (+0.107) 0.00ng/ul

response 64

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	143.75#
104.00	15.60	107.81#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097234.D
Acq On : 8 Aug 2018 14:26
Operator : SJ/JU
Sample : J4268-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AC6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:31:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

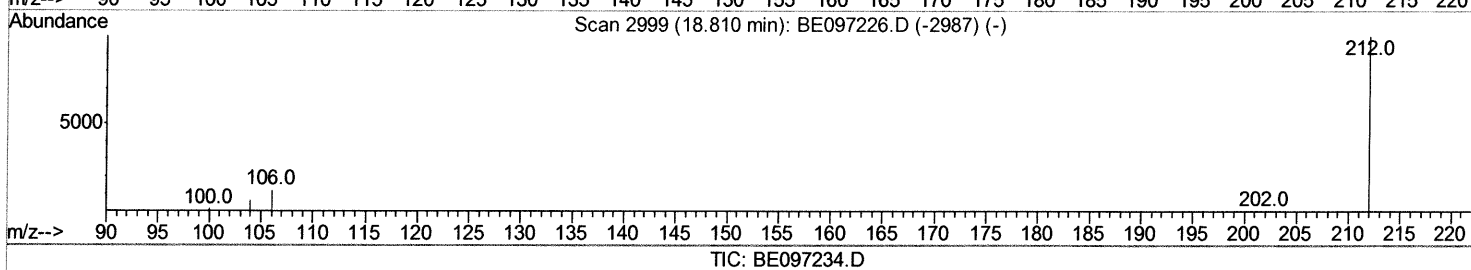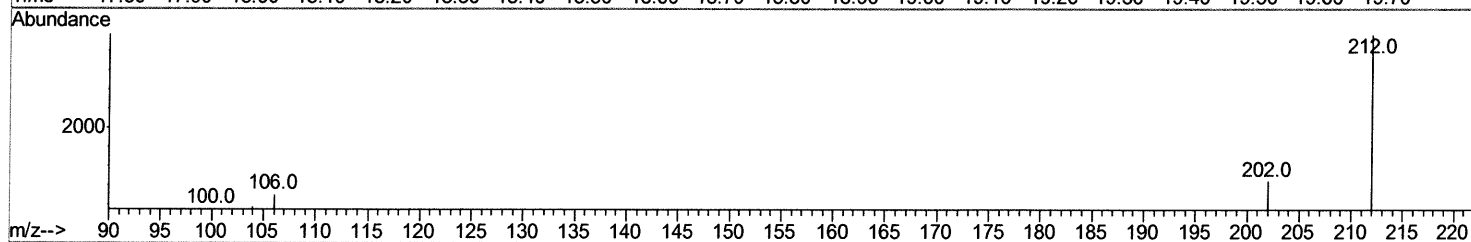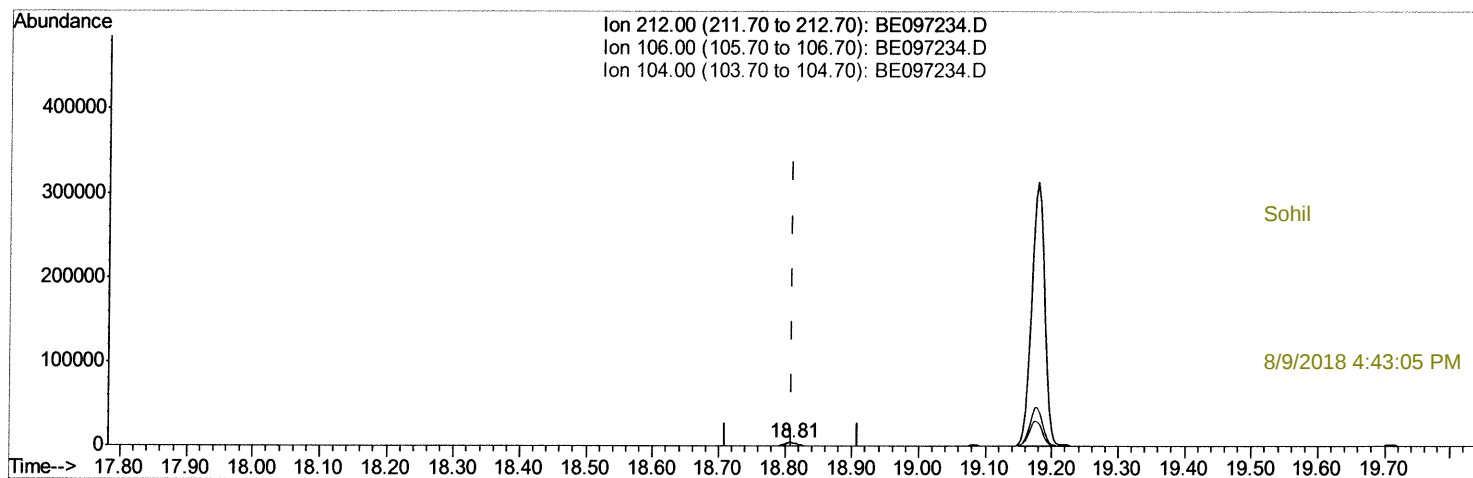

(14) Fluoranthene-d10 (SURR)

18.810min (+0.000) 0.16ng/ul m> SJ 8/10/18

response 5371

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	1.71#
104.00	15.60	1.28#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097234.D
 Acq On : 8 Aug 2018 14:26
 Operator : SJ/JU
 Sample : J4268-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:31:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

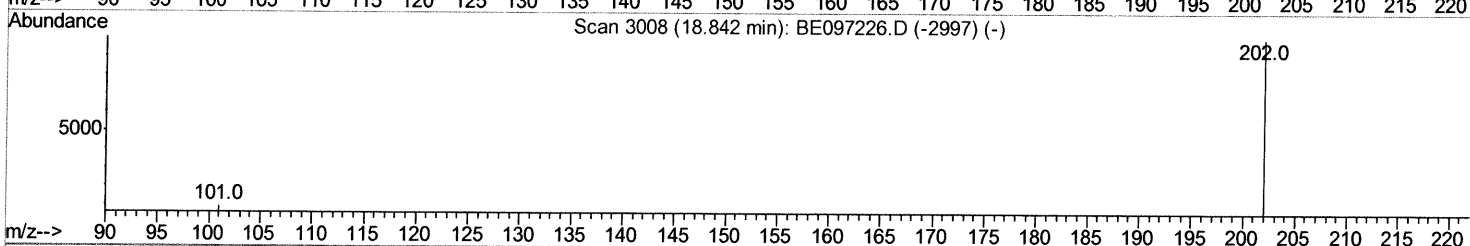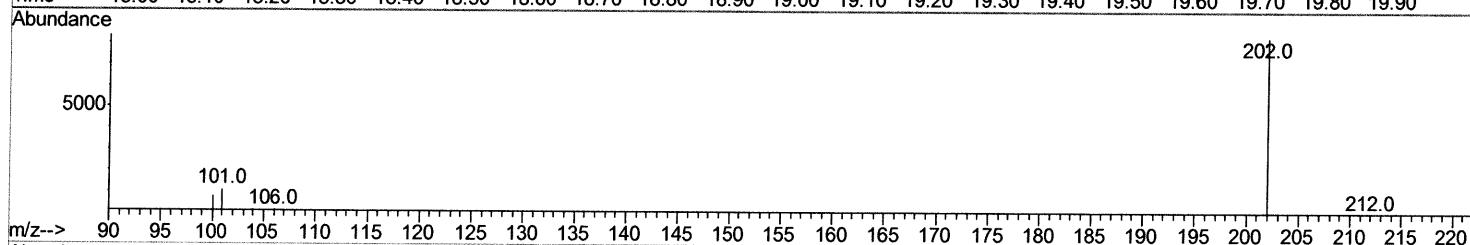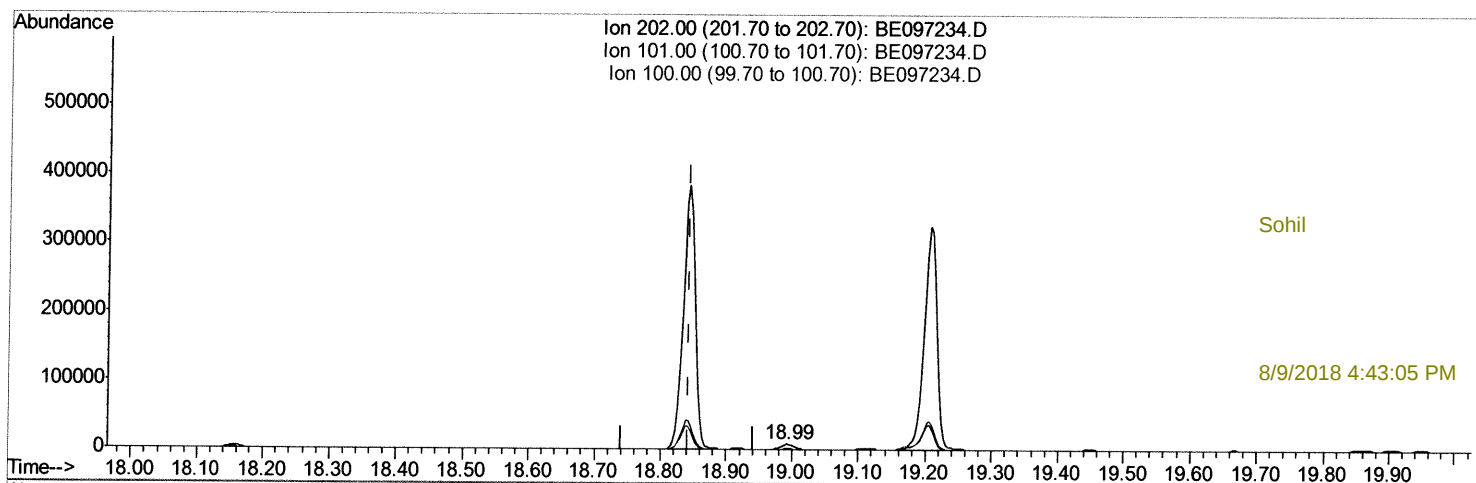

TIC: BE097234.D

(15) Fluoranthene (C)

18.992min (+0.150) 0.31ng/ul

response 10064

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	12.89
100.00	19.50	9.57
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097234.D
 Acq On : 8 Aug 2018 14:26
 Operator : SJ/JU
 Sample : J4268-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AC6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:31:12 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

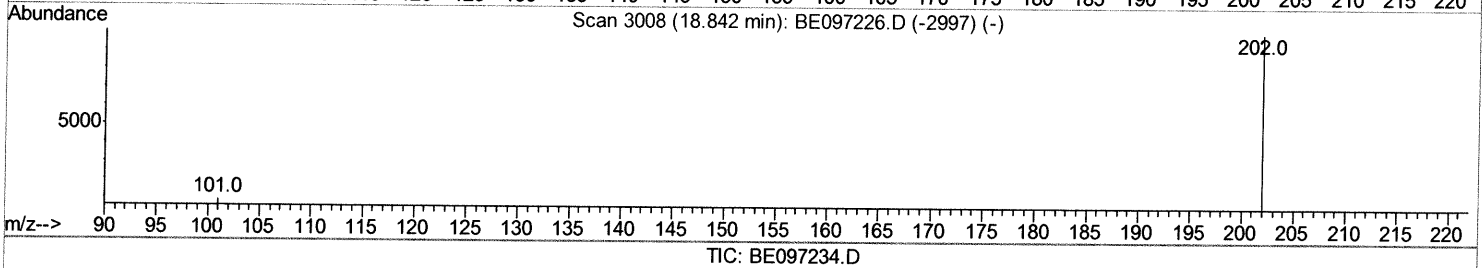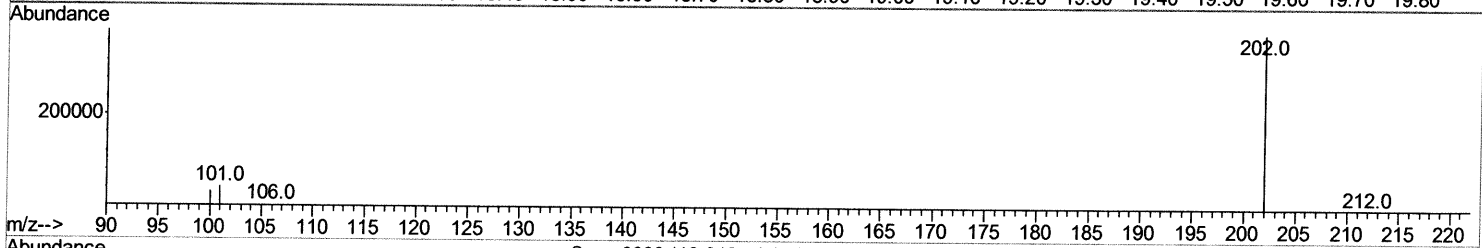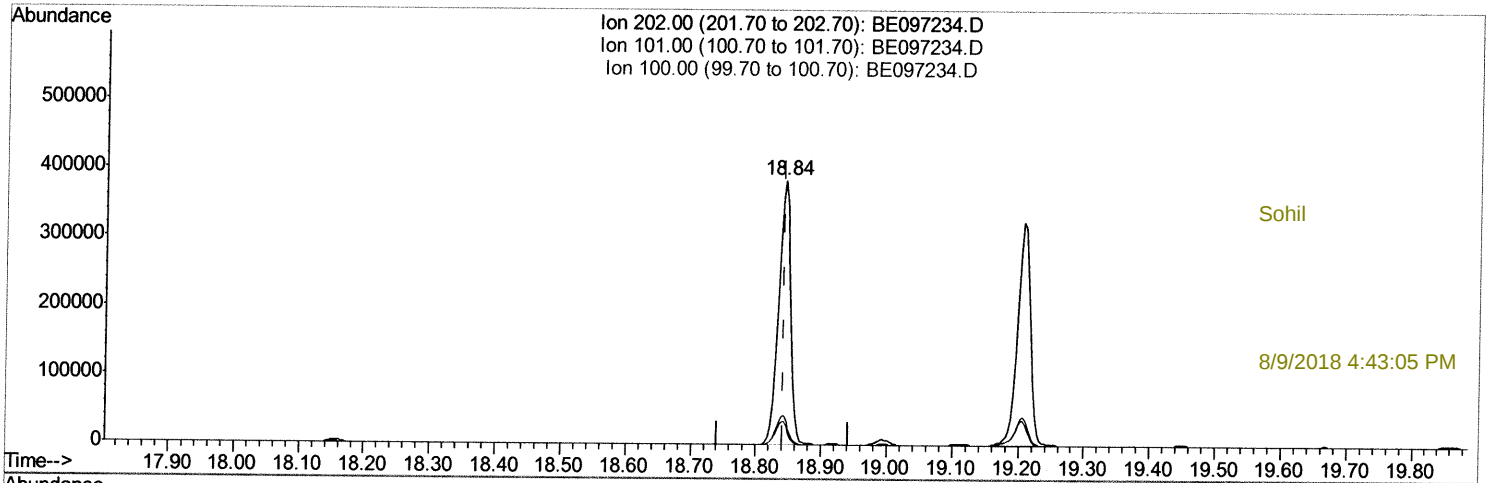

(15) Fluoranthene (C)

18.842min (+0.000) 15.89ng/ul m> SJ 8/10/18

response 510986

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	10.73
100.00	19.50	8.49
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097234.D
Acq On : 8 Aug 2018 14:26
Operator : SJ/JU
Sample : J4268-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AC6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:31:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

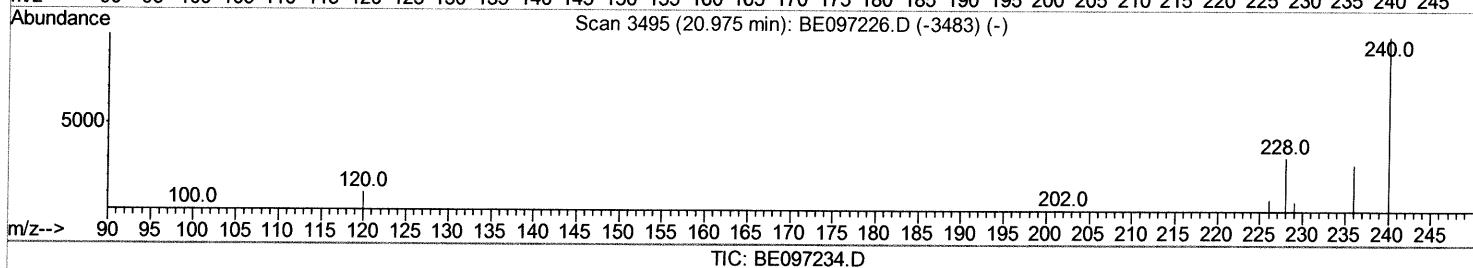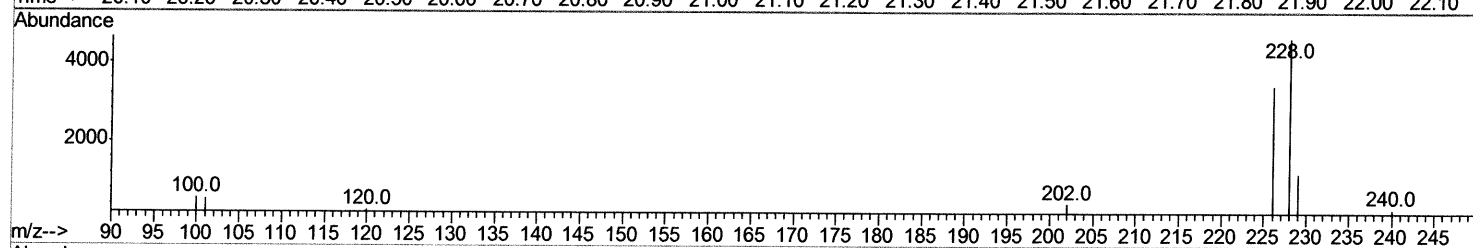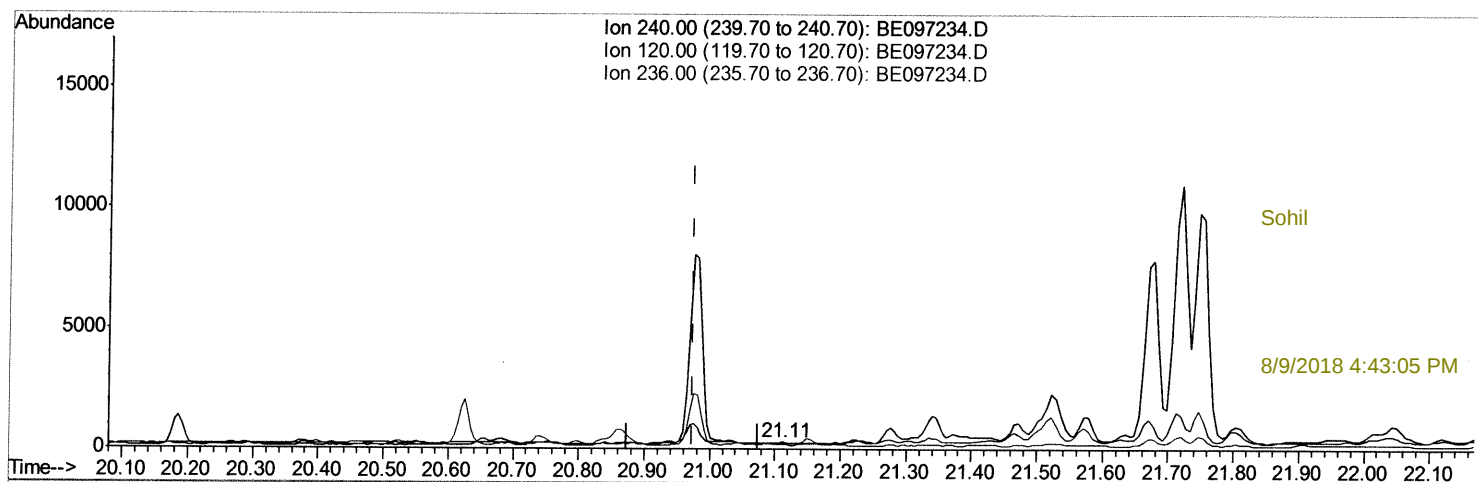

(16) Chrysene-d12 (I)

21.113min (+0.138) 0.40ng/ul

response 174

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	85.71#
236.00	34.90	65.36#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097234.D
Acq On : 8 Aug 2018 14:26
Operator : SJ/JU
Sample : J4268-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AC6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:31:12 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

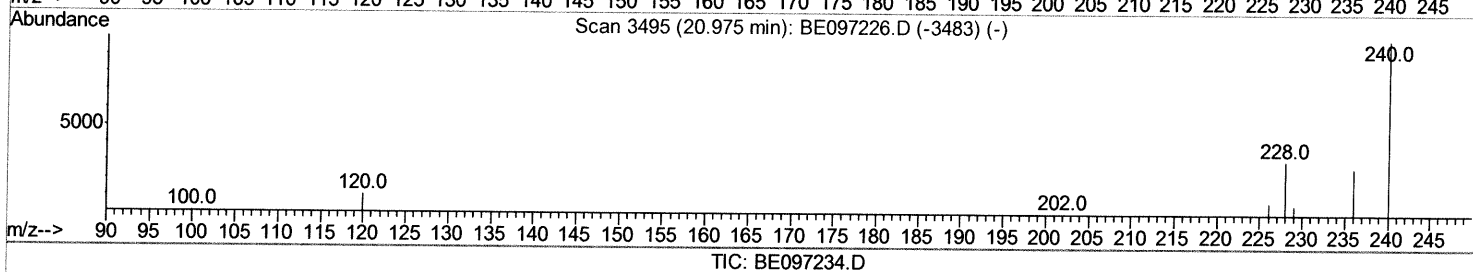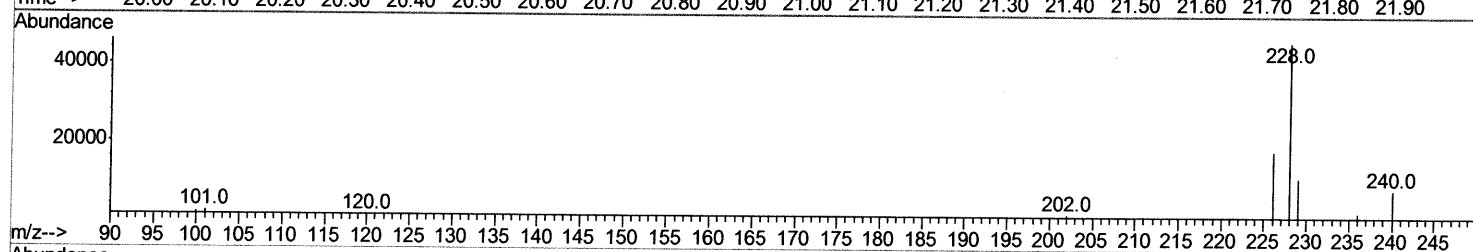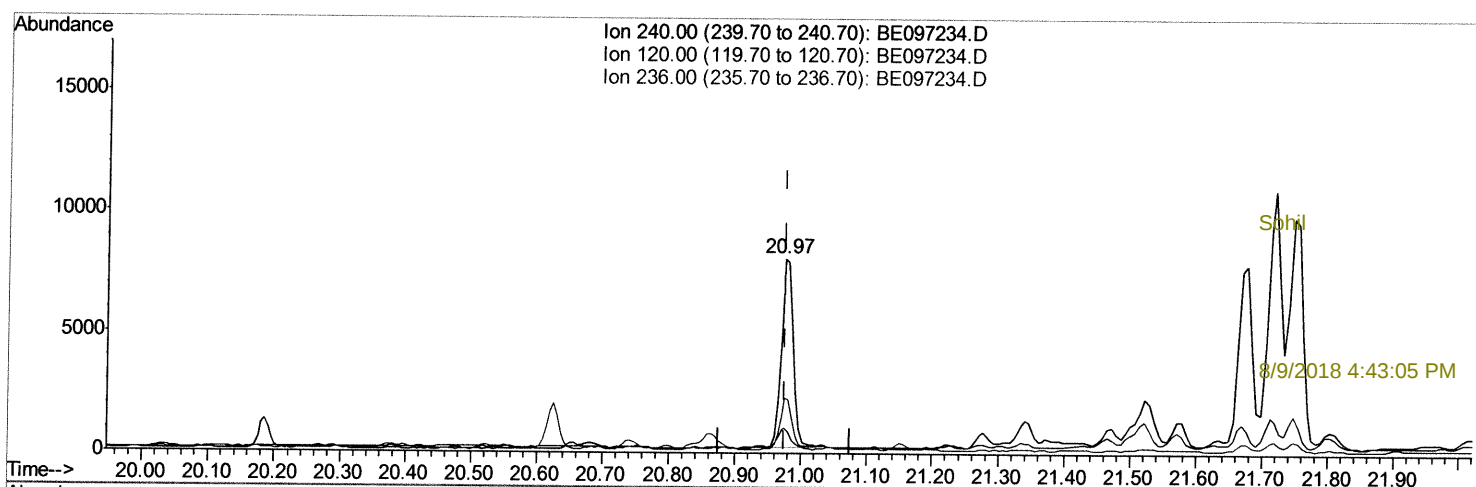

(16) Chrysene-d12 (I)

20.975min (+0.000) 0.40ng/ul m> 52 8/10/18

response 10026

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	13.28#
236.00	34.90	28.56
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097234.D
 Acq On : 8 Aug 2018 14:26
 Operator : SJ/JU
 Sample : J4268-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC6

Manual Integrations
 APPROVED



Sohil
 8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:33:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

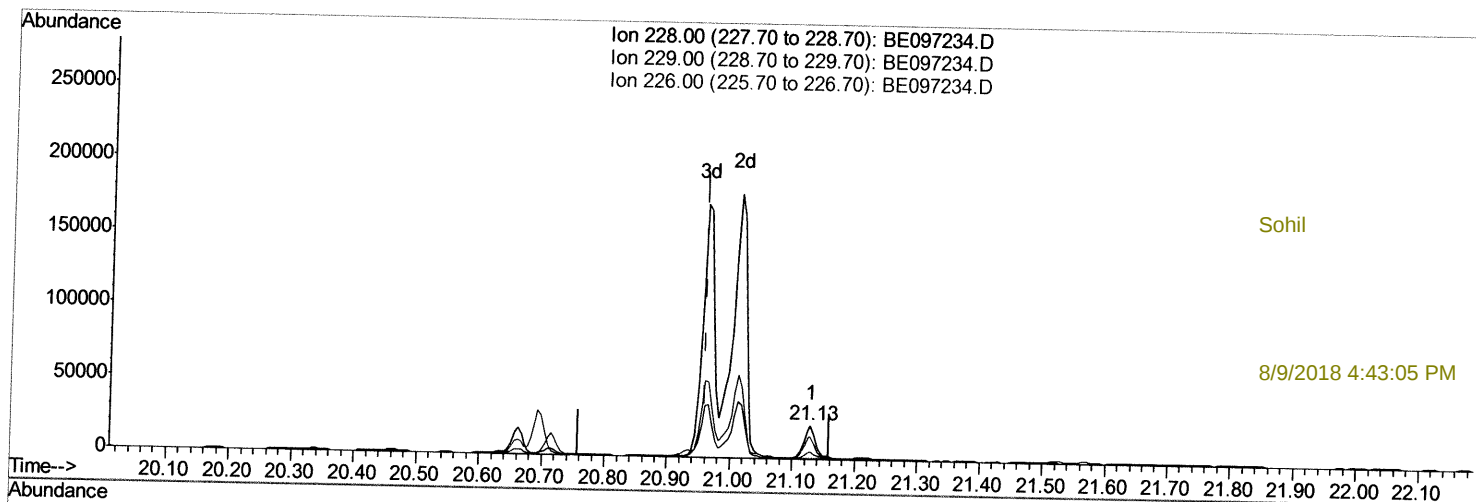

Sohil

8/9/2018 4:43:05 PM

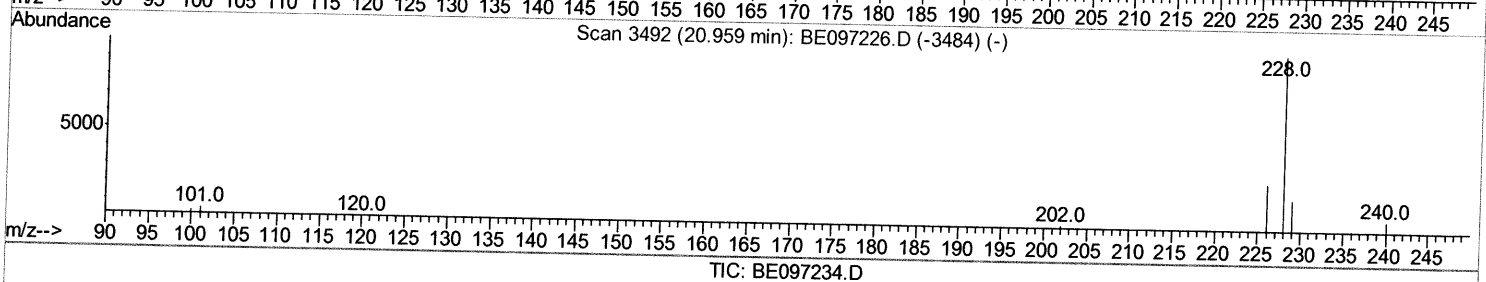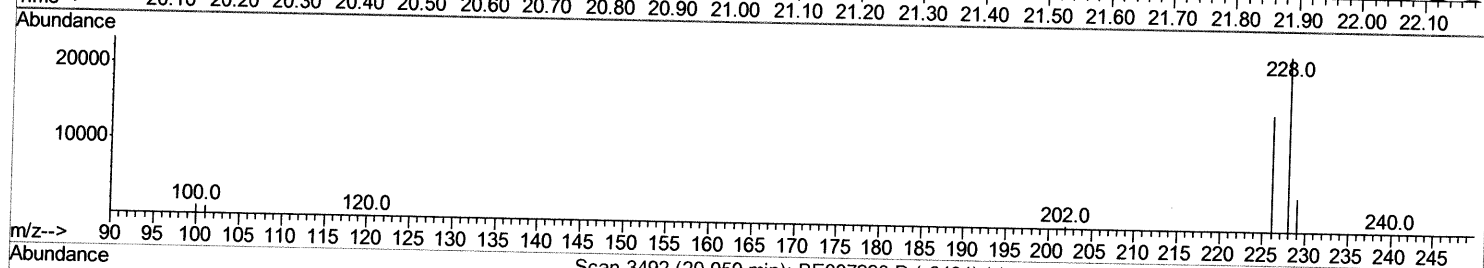

(18) Benzo(a)anthracene

21.129min (+0.170) 0.99ng/ul

response 28474

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	19.88#
226.00	21.30	66.50#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097234.D
 Acq On : 8 Aug 2018 14:26
 Operator : SJ/JU
 Sample : J4268-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AC6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:33:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

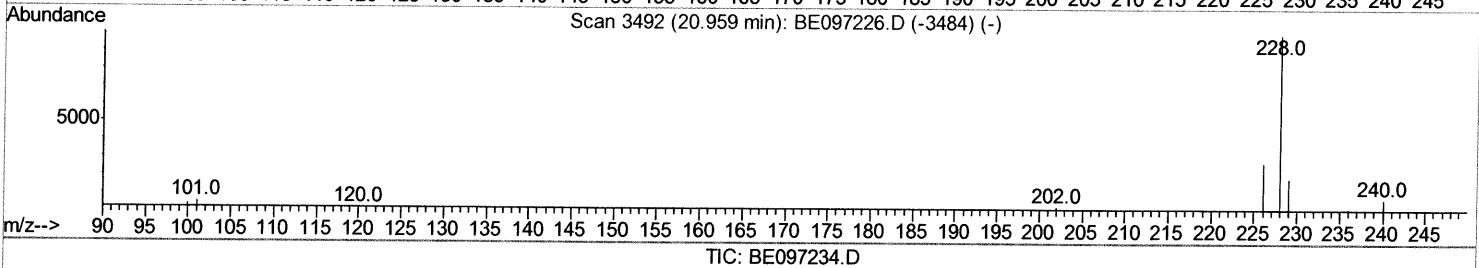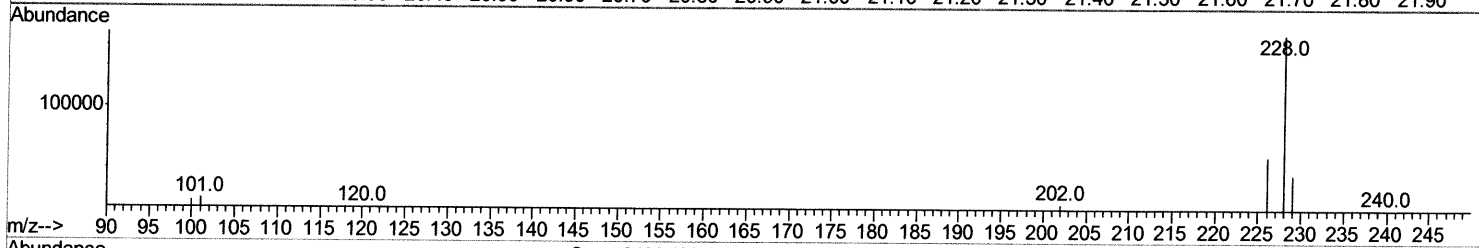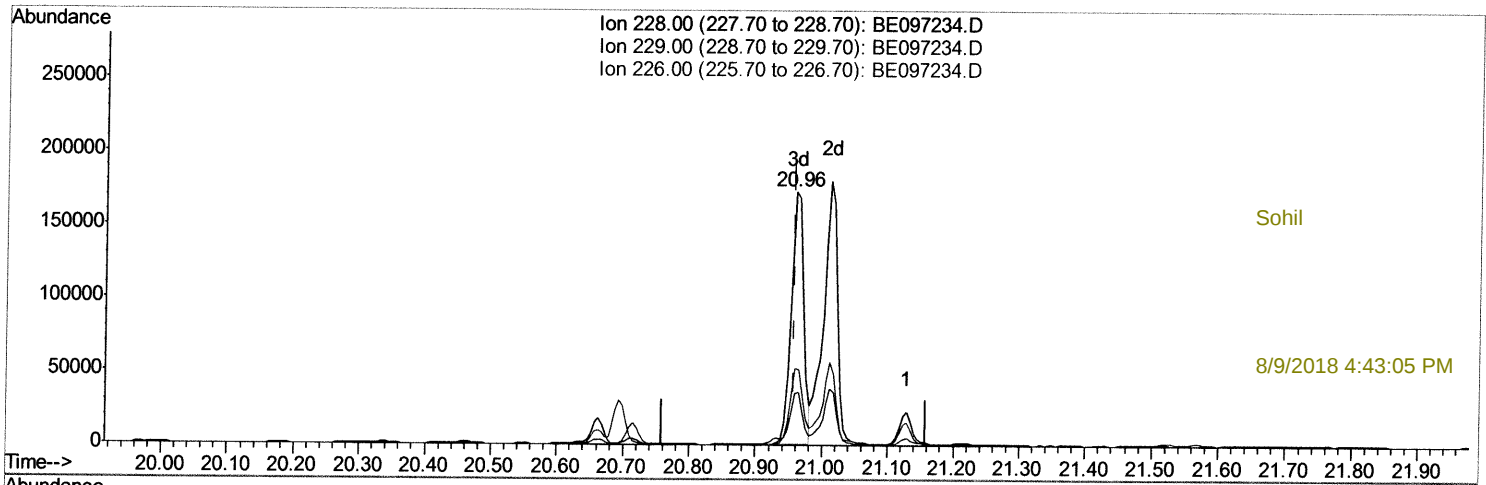

(18) Benzo(a)anthracene

20.959min (+0.000) 7.68ng/ul m> SJ 8/10/18

response 219888

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	20.31#
226.00	21.30	30.22#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097234.D
 Acq On : 8 Aug 2018 14:26
 Operator : SJ/JU
 Sample : J4268-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:33:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

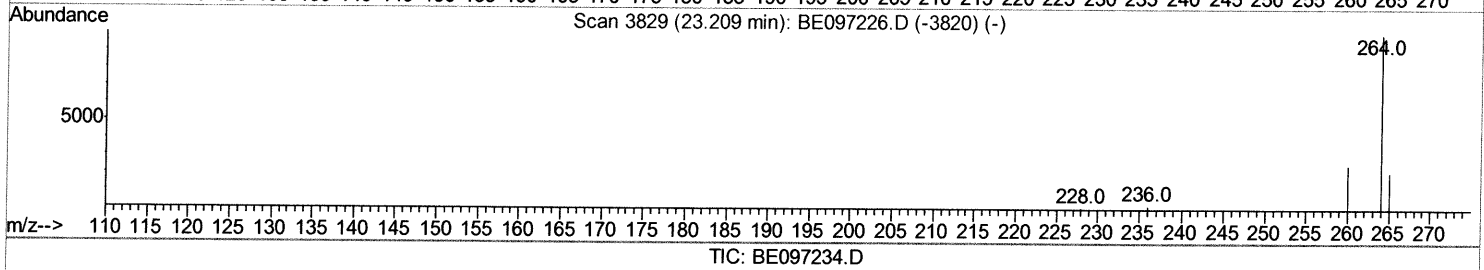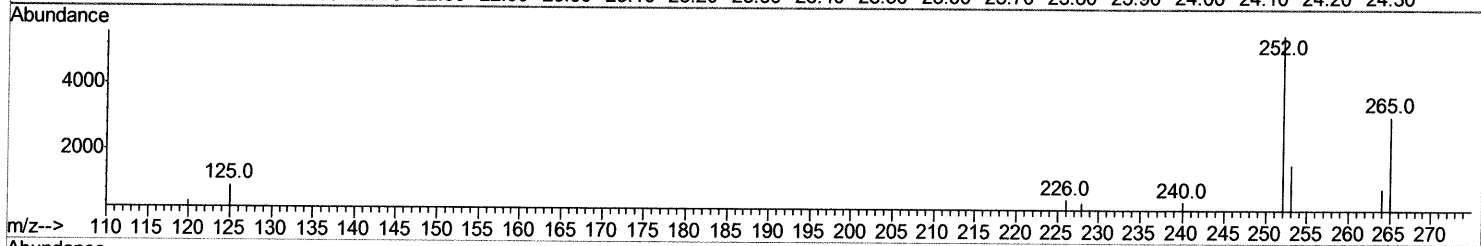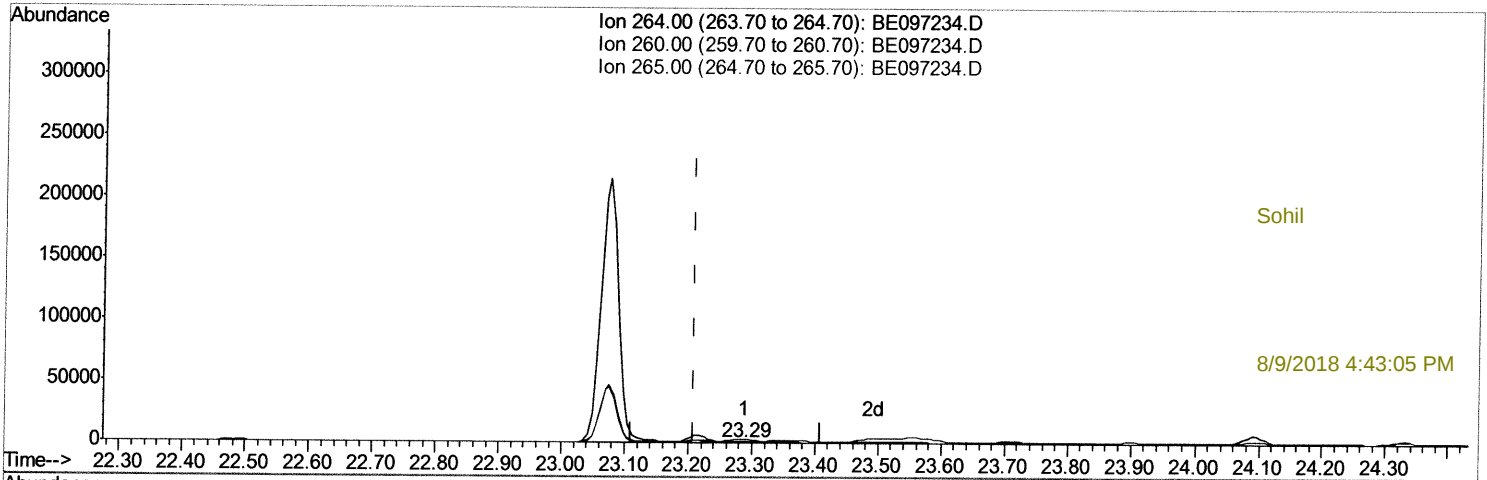

(20) Perylene-d12 (I)
 23.287min (+0.078) 0.40ng/ul
 response 2357

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	27.62
265.00	103.50	341.77#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097234.D
 Acq On : 8 Aug 2018 14:26
 Operator : SJ/JU
 Sample : J4268-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AC6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:33:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

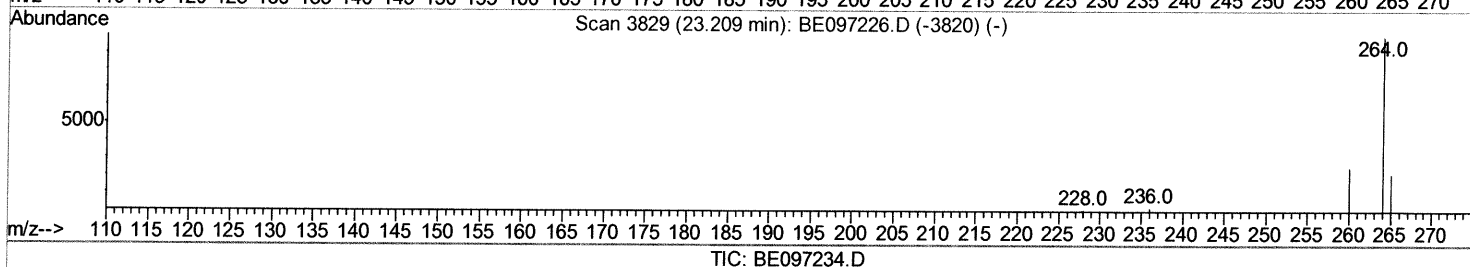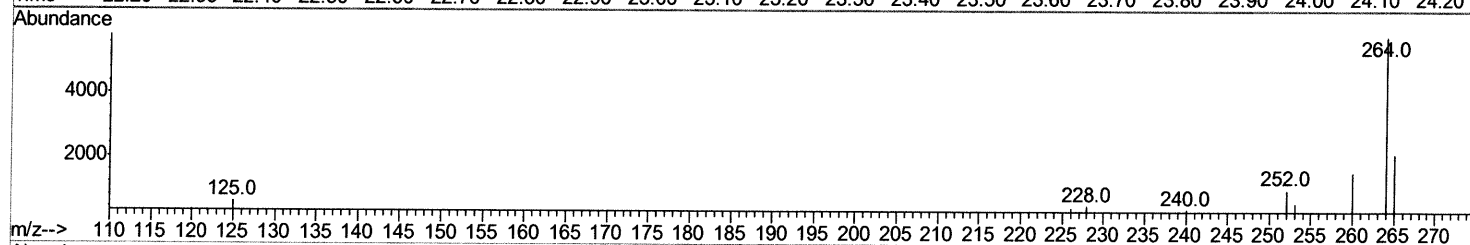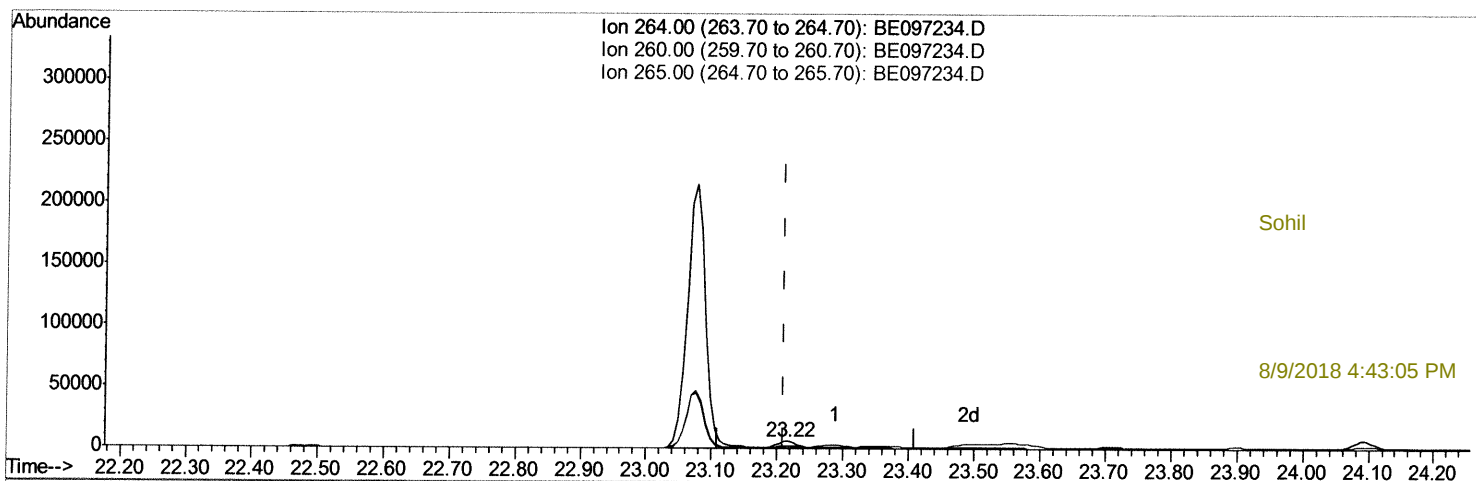

(20) Perylene-d12 (I)

23.217min (+0.007) 0.40ng/ul m > SJ 8/10/18

response 9711

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	26.64
265.00	103.50	36.37#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097234.D
 Acq On : 8 Aug 2018 14:26
 Operator : SJ/JU
 Sample : J4268-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:33:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

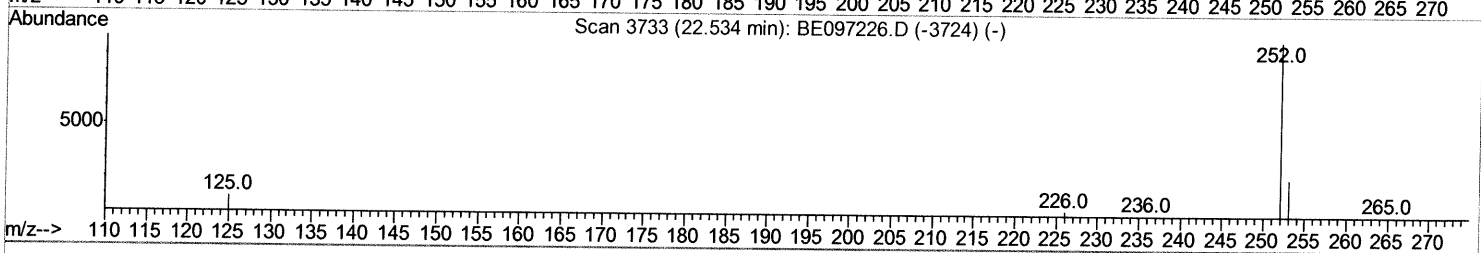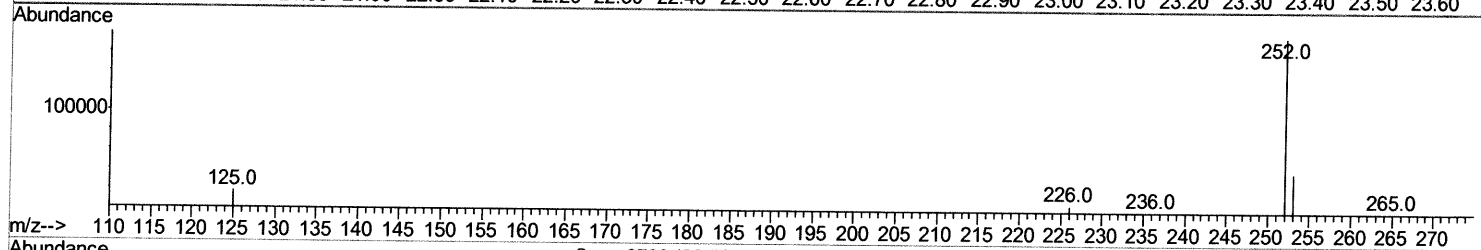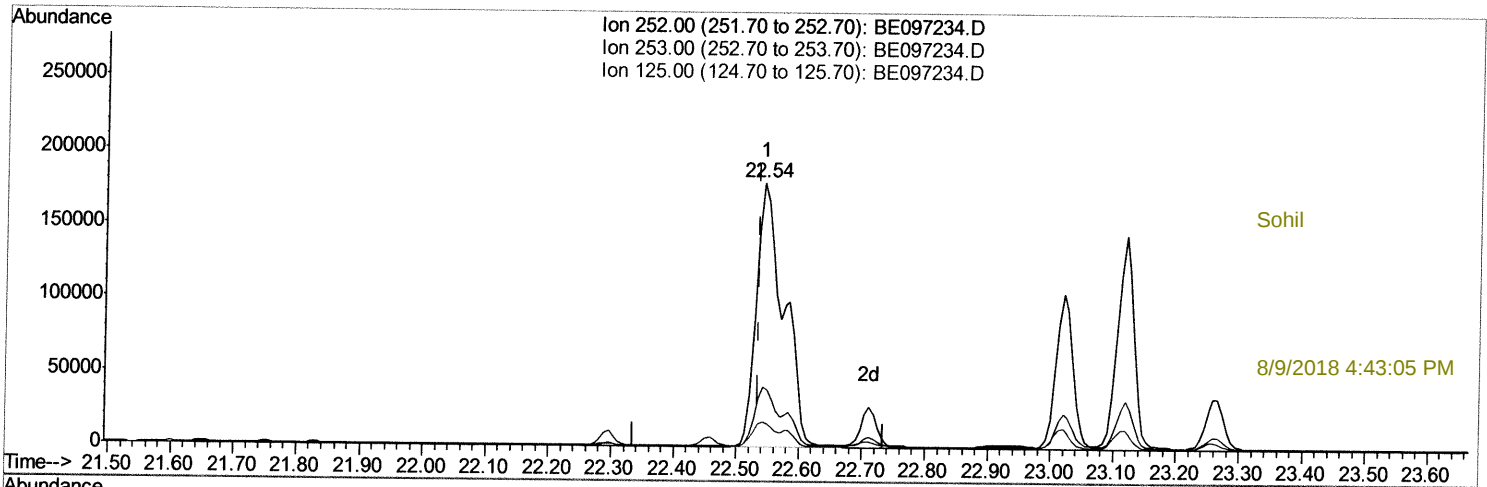

TIC: BE097234.D

(21) Benzo(b)fluoranthene

22.542min (+0.007) 20.49ng/ui

response 542300

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	22.67
125.00	17.50	9.56
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097234.D
Acq On : 8 Aug 2018 14:26
Operator : SJ/JU
Sample : J4268-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AC6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:33:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

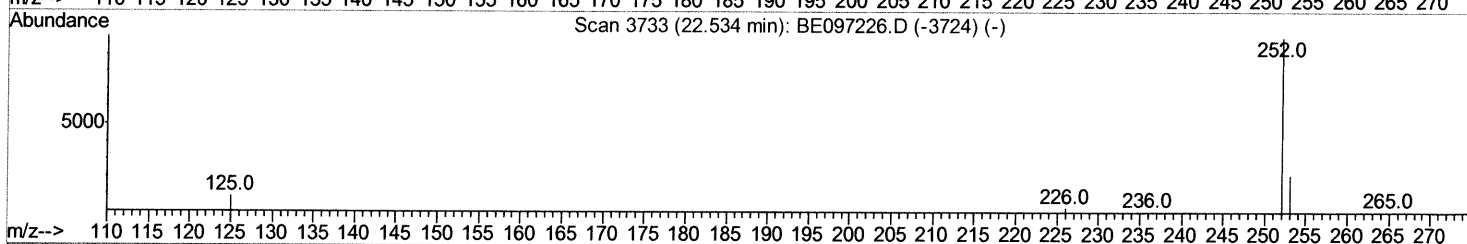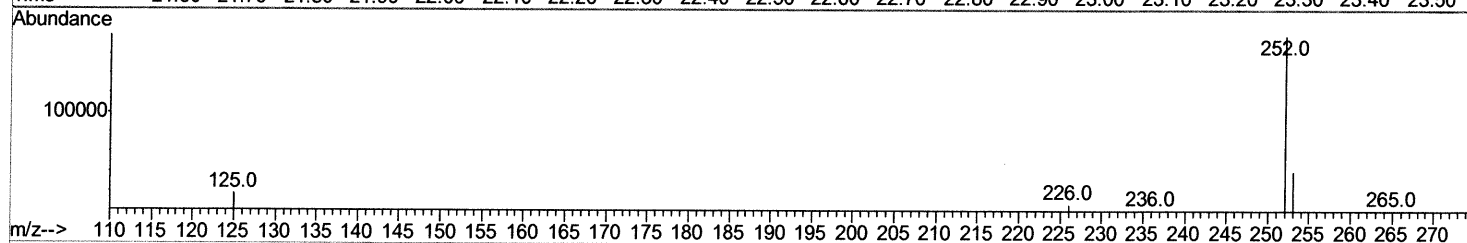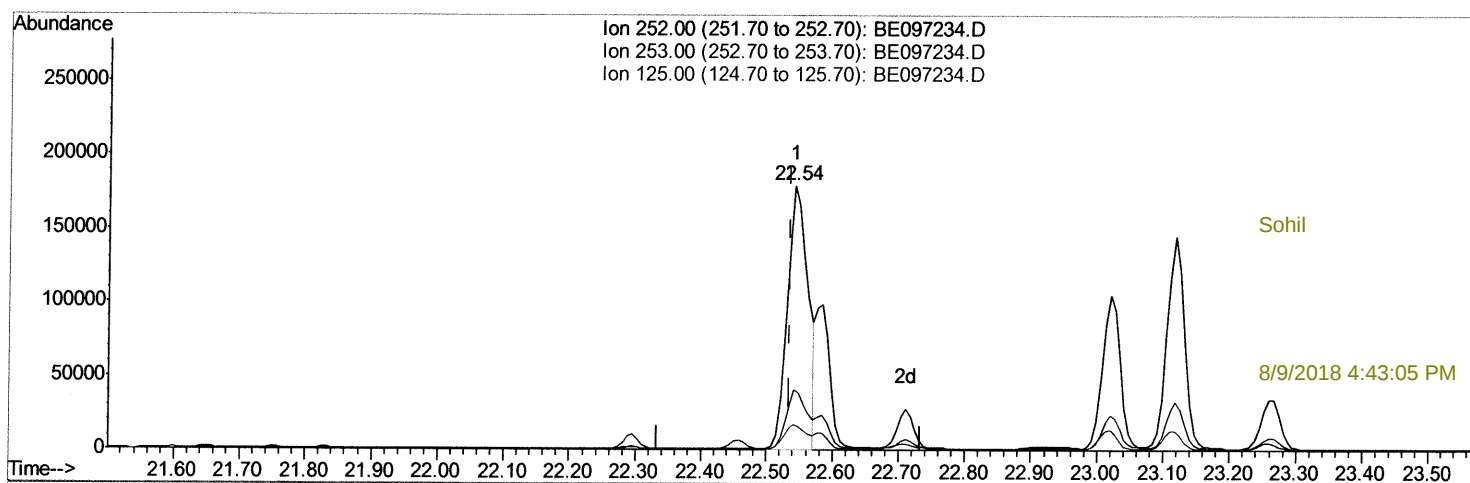

TIC: BE097234.D

(21) Benzo(b)fluoranthene

22.542min (+0.007) 15.03ng/ul m

response 397762

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	22.67
125.00	17.50	9.56
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097234.D
Acq On : 8 Aug 2018 14:26
Operator : SJ/JU
Sample : J4268-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AC6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:33:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

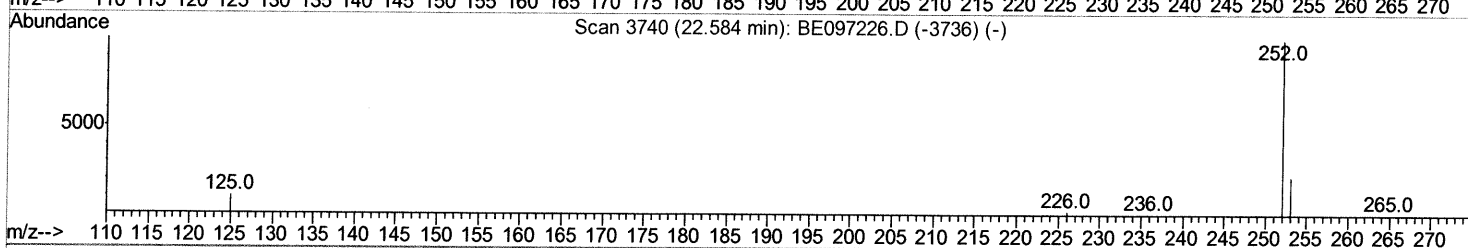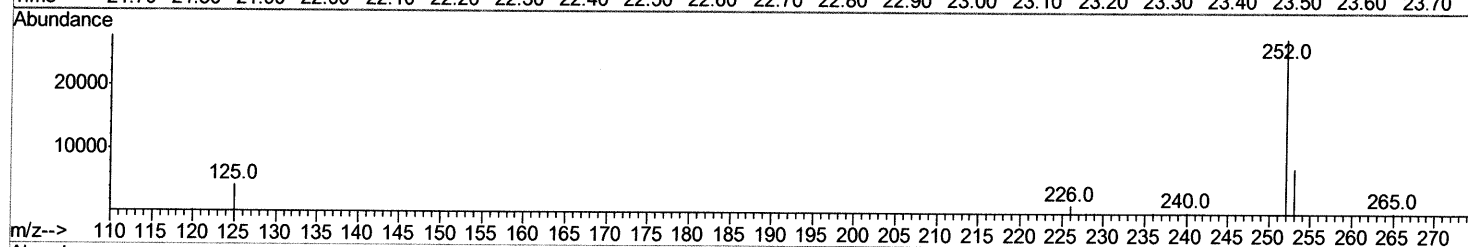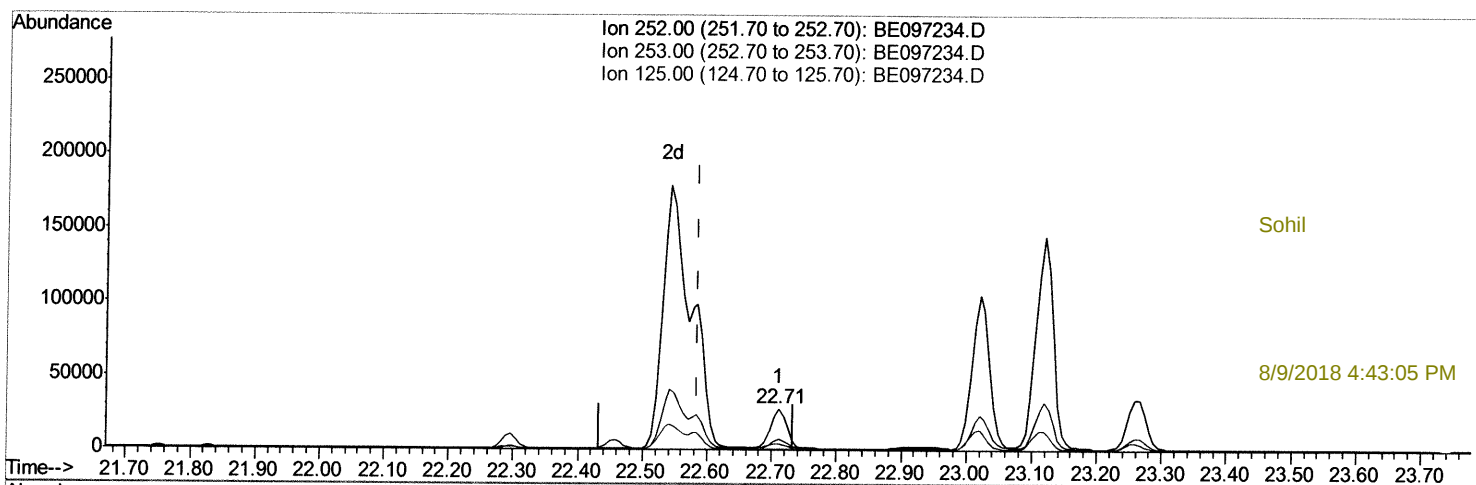

TIC: BE097234.D

(22) Benzo(k)fluoranthene

22.711min (+0.127) 1.59ng/ul

response 45380

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	26.44
125.00	17.10	15.60
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097234.D
 Acq On : 8 Aug 2018 14:26
 Operator : SJ/JU
 Sample : J4268-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:33:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

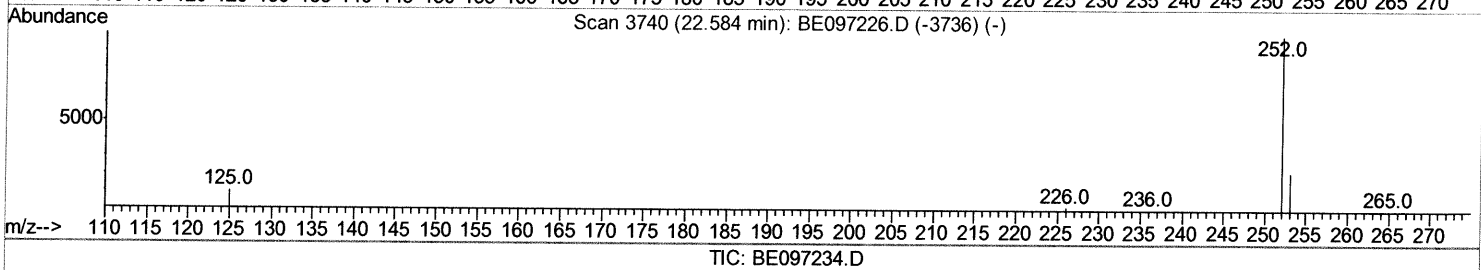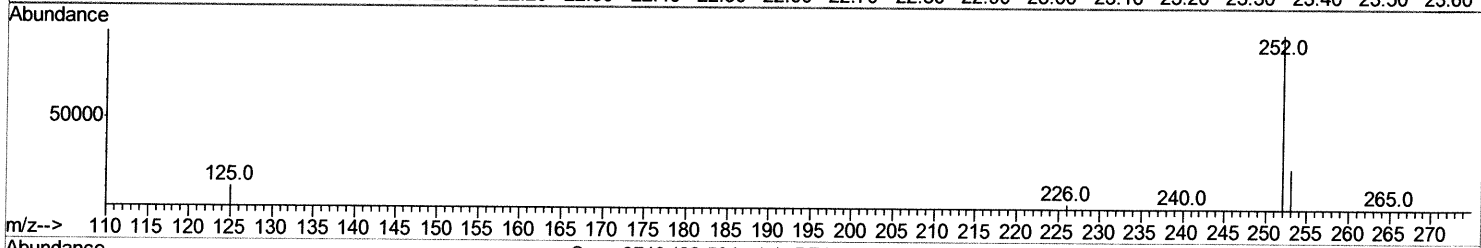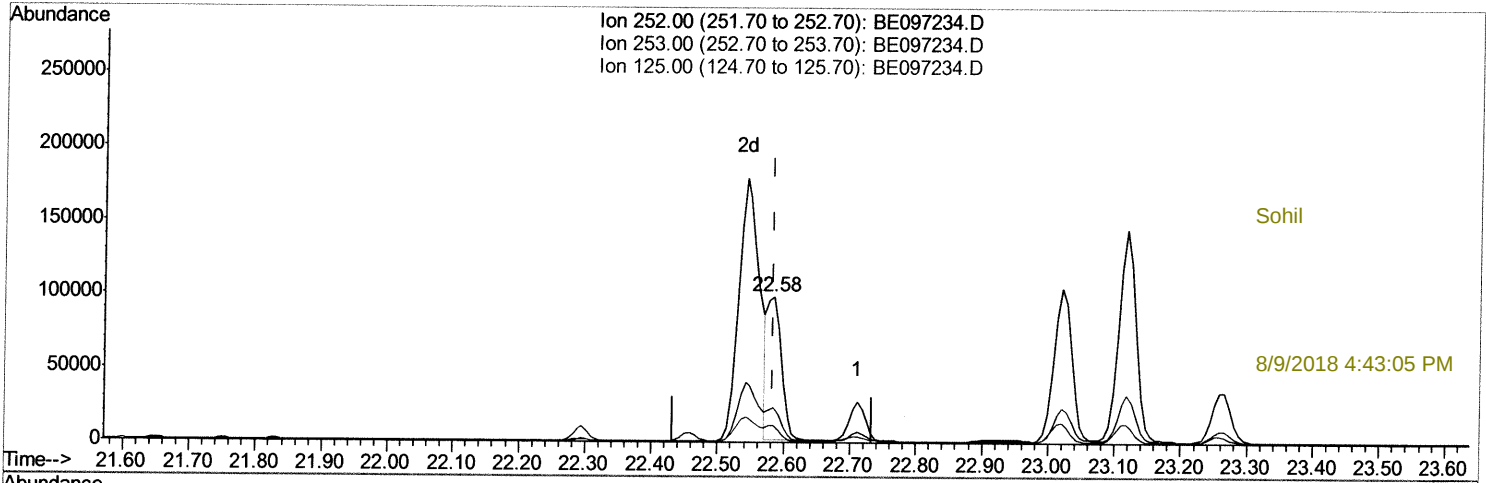

(22) Benzo(k)fluoranthene

22.584min (+0.000) 4.79ng/ul m> 52 8/10/18

response 136763

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	23.78#
125.00	17.10	11.51#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097234.D
Acq On : 8 Aug 2018 14:26
Operator : SJ/JU
Sample : J4268-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AC6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:33:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

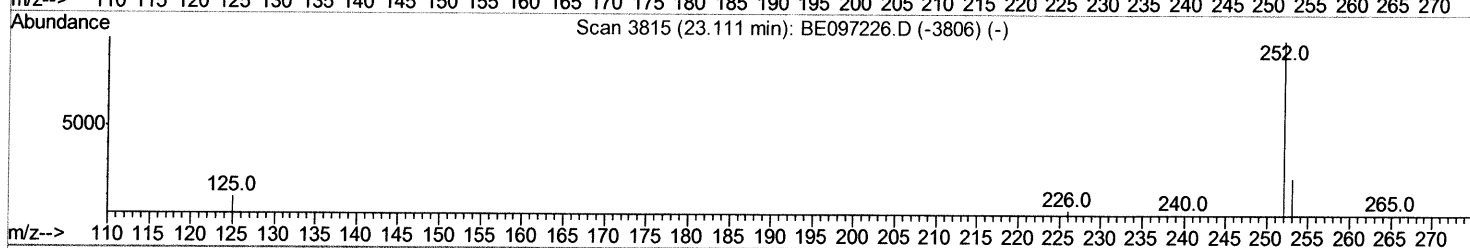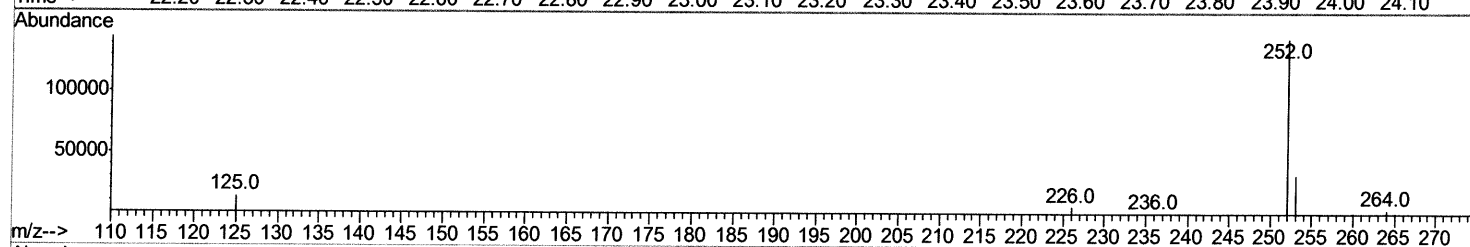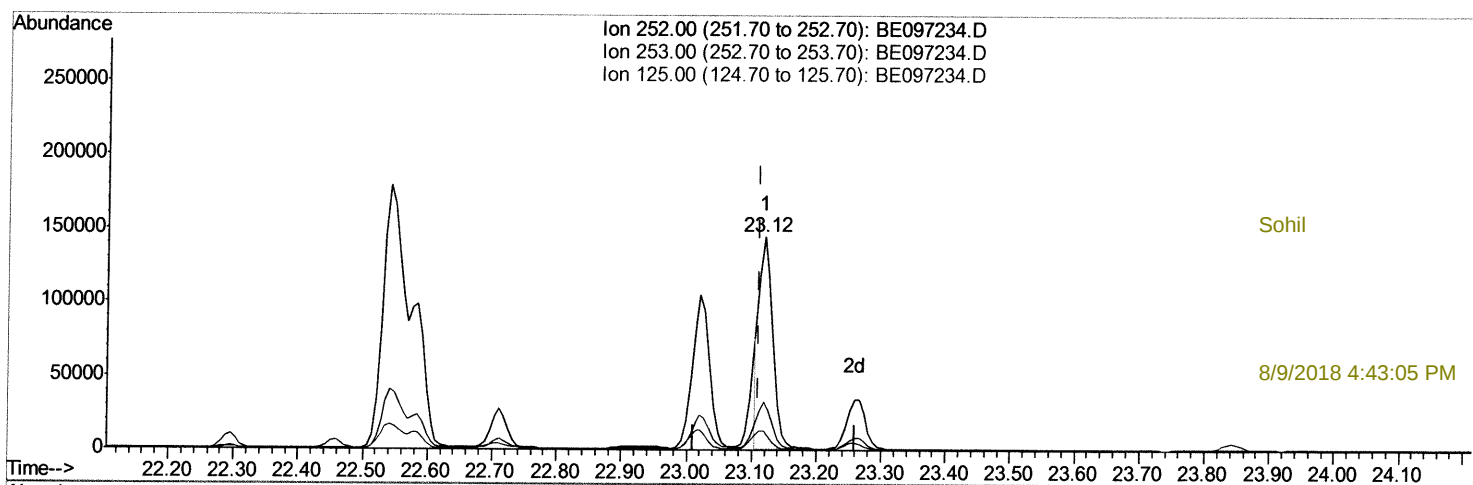

TIC: BE097234.D

(23) Benzo(a)pyrene (C)

23.118min (+0.007) 7.96ng/ul

response 210796

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	22.35#
125.00	22.60	9.18#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097234.D
 Acq On : 8 Aug 2018 14:26
 Operator : SJ/JU
 Sample : J4268-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AC6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:33:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

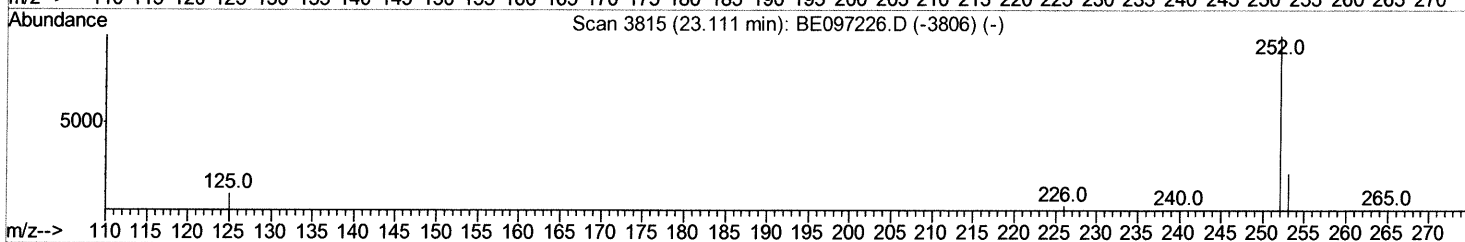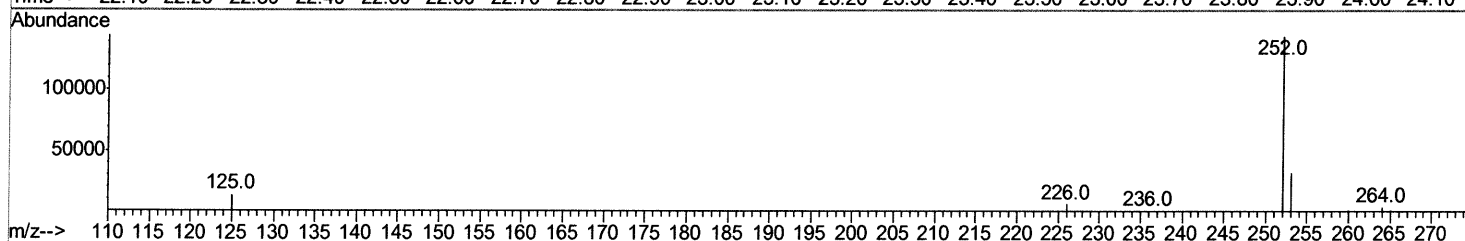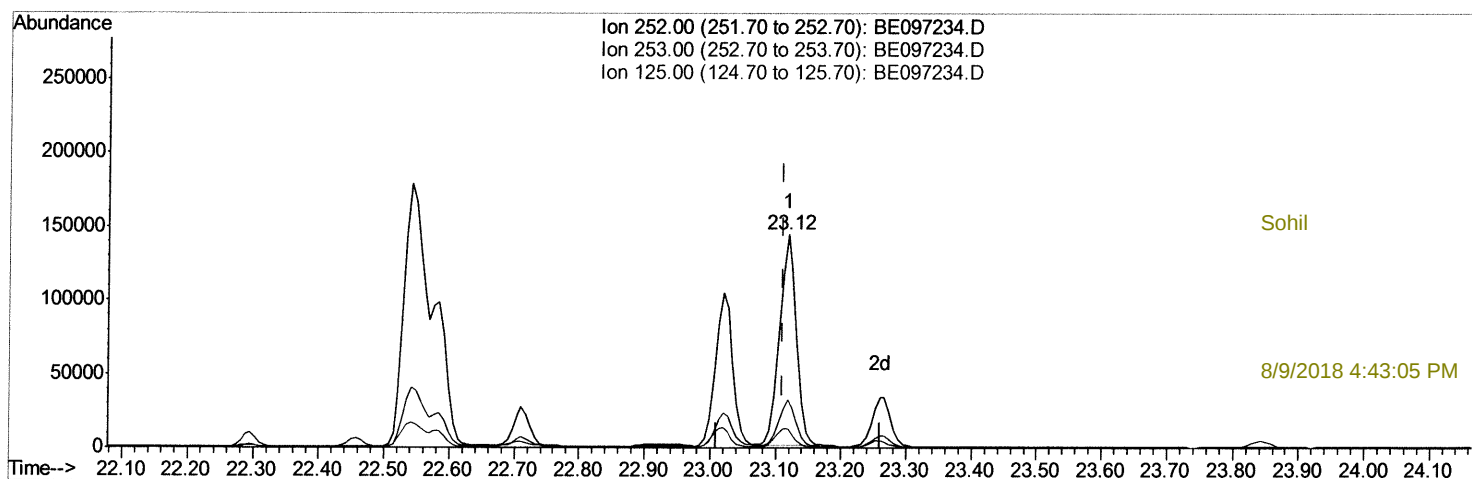

TIC: BE097234.D

(23) Benzo(a)pyrene (C)

23.118min (+0.007) 9.65ng/ul m> SJ 8/10/18

response 255654

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	22.35#
125.00	22.60	9.18#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097234.D
Acq On : 8 Aug 2018 14:26
Operator : SJ/JU
Sample : J4268-14
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AC6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:33:07 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

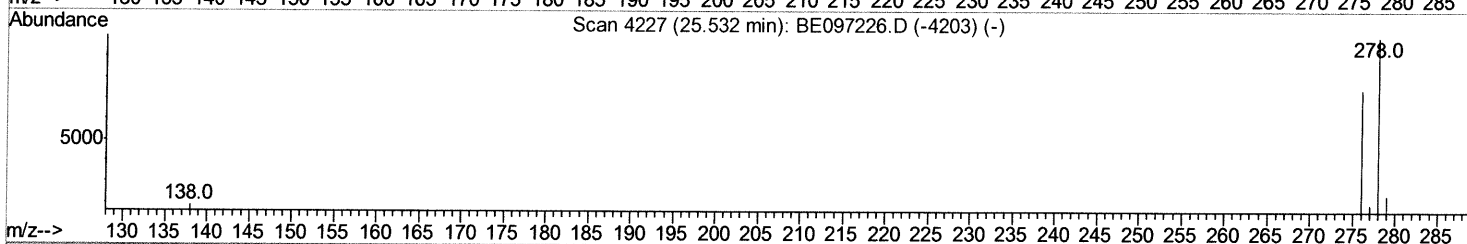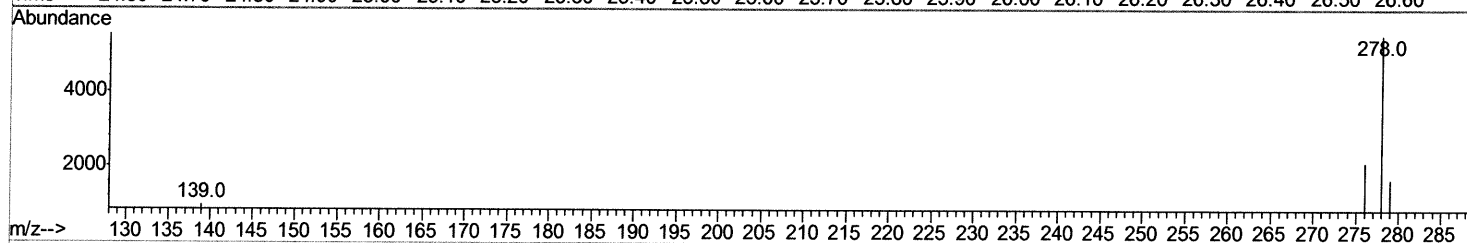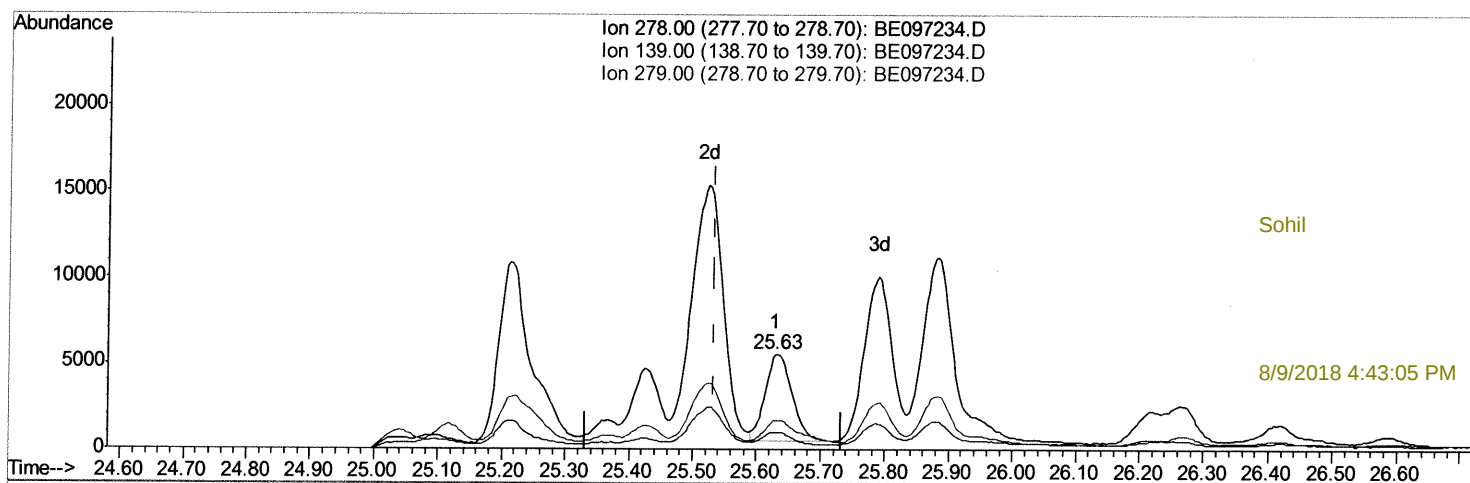

TIC: BE097234.D

(25) Dibenzo(a,h)anthracene

25.629min (+0.097) 0.55ng/ul

response 14848

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	18.12
279.00	32.40	30.49
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097234.D
 Acq On : 8 Aug 2018 14:26
 Operator : SJ/JU
 Sample : J4268-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:33:07 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

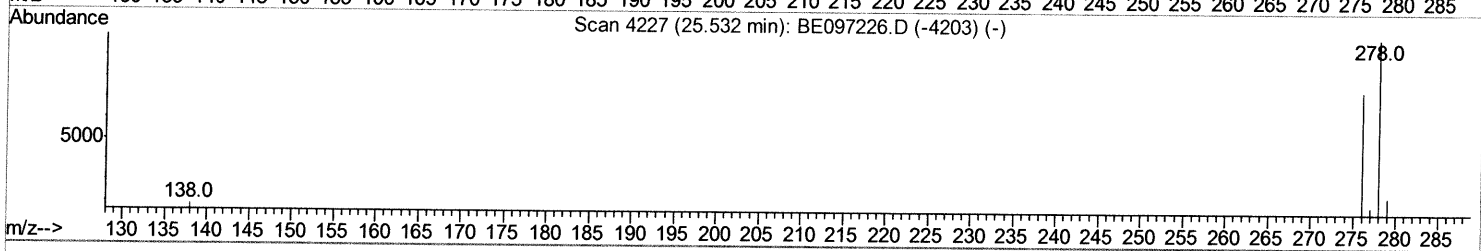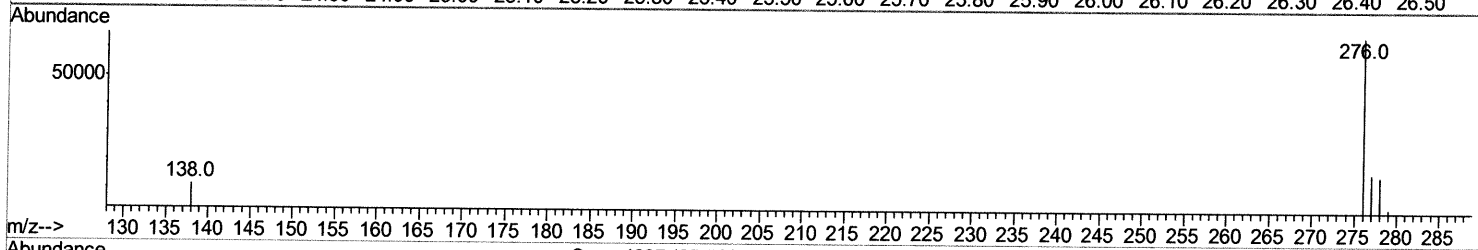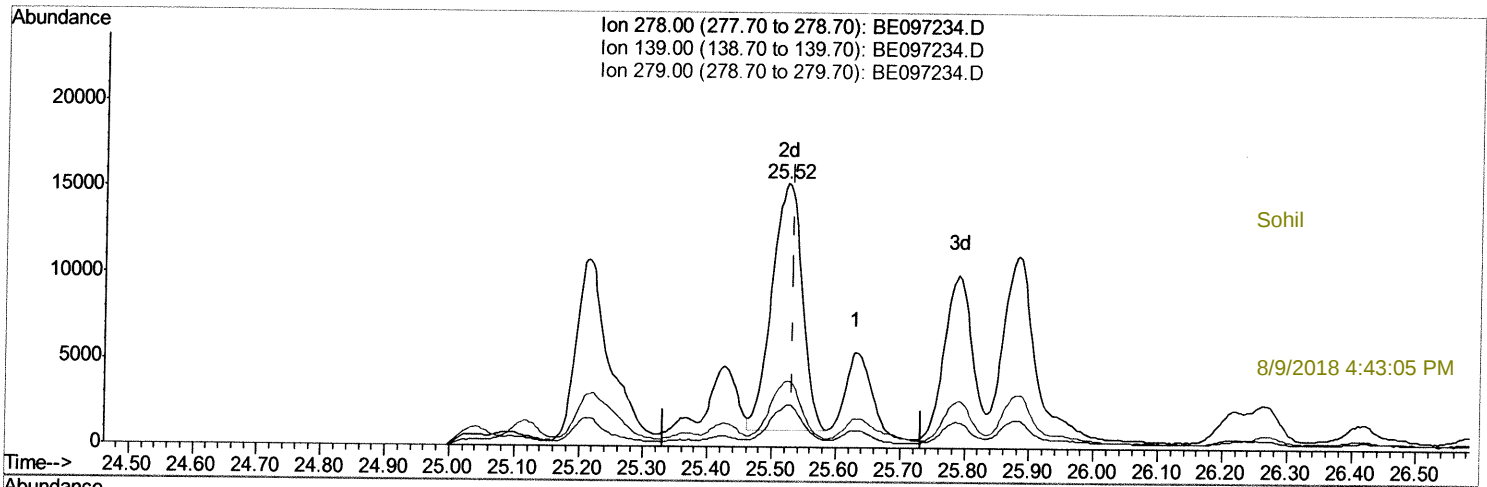

(25) Dibenzo(a,h)anthracene

25.522min (-0.010) 1.75ng/ul m> SJ 8/10/18

response 47414

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	15.99#
279.00	32.40	24.93#
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097234.D
 Acq On : 8 Aug 2018 14:26
 Operator : SJ/JU
 Sample : J4268-14
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:05 PM

Quant Time: Aug 09 00:39:13 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1245	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6483	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	3962	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.77	188	9545m	0.40	ng/ul	0.00
16) Chrysene-d12	20.97	240	10026m	0.40	ng/ul	0.00
20) Perylene-d12	23.22	264	9711m	0.40	ng/ul	0.00

SJ 8/10/18
 Sohil

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.73	152	1758	0.17	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	5371m	0.16	ng/ul	0.00

SJ 8/10/18

8/9/2018 4:43:05 PM

Target Compounds

					Ovalue	
3) Naphthalene	10.18	128	24968	1.590	ng/ul#	91
5) 2-Methylnaphthalene	11.80	142	4423	0.426	ng/ul	98
7) Acenaphthylene	13.73	152	10806	0.631	ng/ul	97
8) Acenaphthene	14.08	153	2018	0.163	ng/ul#	93
9) Fluorene	15.08	166	5117	0.359	ng/ul	93
12) Phenanthrene	16.81	178	163384m	6.715	ng/ul	
13) Anthracene	16.90	178	24192m	1.066	ng/ul	
15) Fluoranthene	18.84	202	510986m	15.887	ng/ul	
17) Pyrene	19.21	202	430266	16.016	ng/ul#	80
18) Benzo(a)anthracene	20.96	228	219888m	7.675	ng/ul	
19) Chrysene	21.01	228	269923	9.143	ng/ul	97
21) Benzo(b)fluoranthene	22.54	252	397762m	15.028	ng/ul	
22) Benzo(k)fluoranthene	22.58	252	136763m	4.792	ng/ul	
23) Benzo(a)pyrene	23.12	252	255654m	9.653	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.51	276	218653	6.597	ng/ul#	70
25) Dibenzo(a,h)anthracene	25.52	278	47414m	1.748	ng/ul	
26) Benzo(a,h,i)perylene	26.22	276	215276	7.515	ng/ul#	89

SJ 8/10/18

(#) = qualifier out of range (m) = manual integration (+) = signals summed