


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097238.D
Acq On : 8 Aug 2018 16:55
Operator : SJ/JU
Sample : J4268-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA1

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:16 PM

Quant Time: Aug 09 01:12:37 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

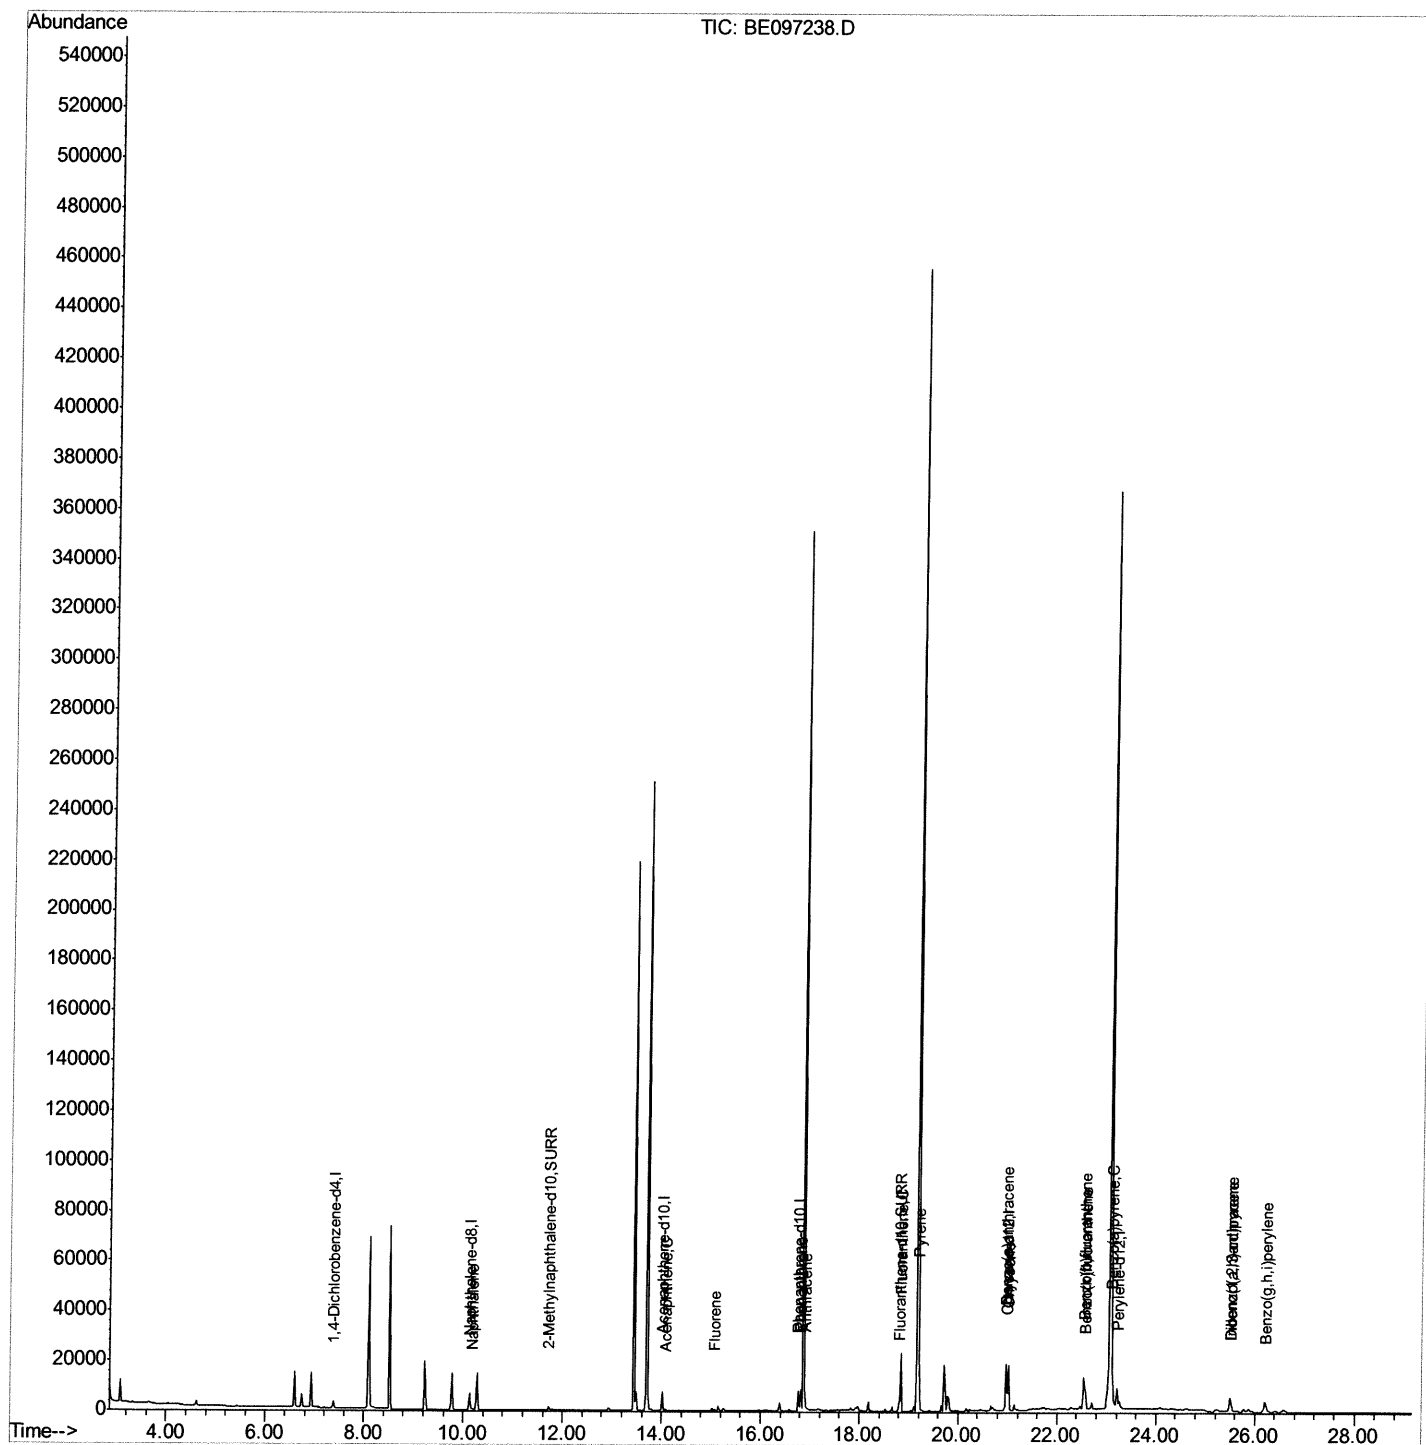

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097238.D
 Acq On : 8 Aug 2018 16:55
 Operator : SJ/JU
 Sample : J4268-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:16 PM

Quant Time: Aug 08 23:27:19 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

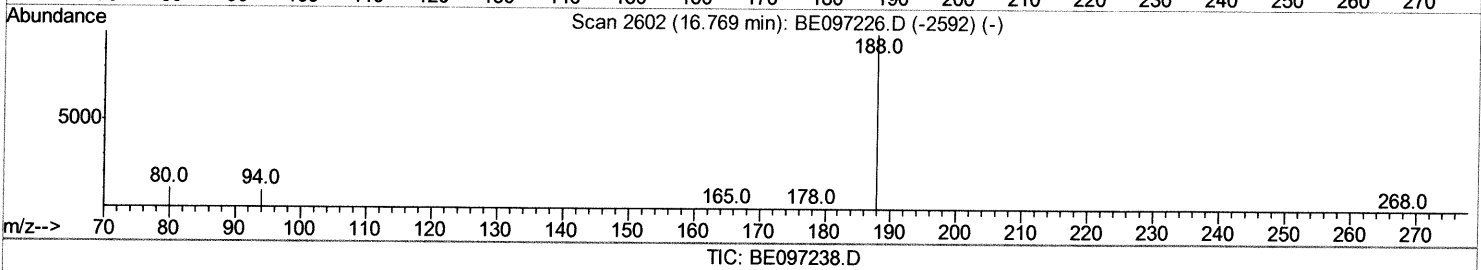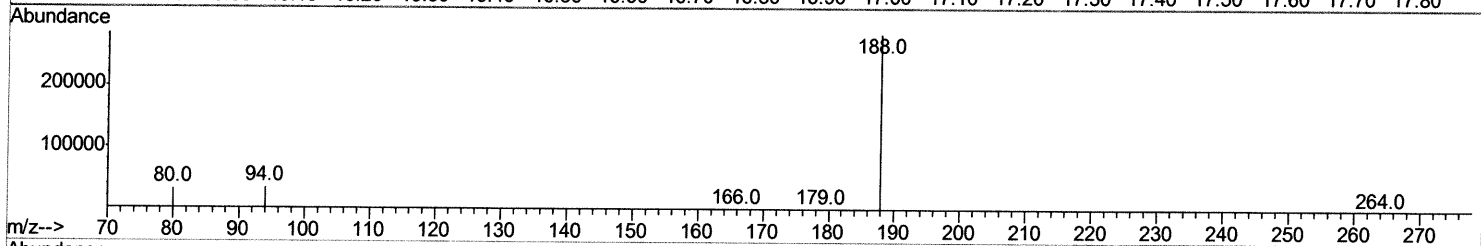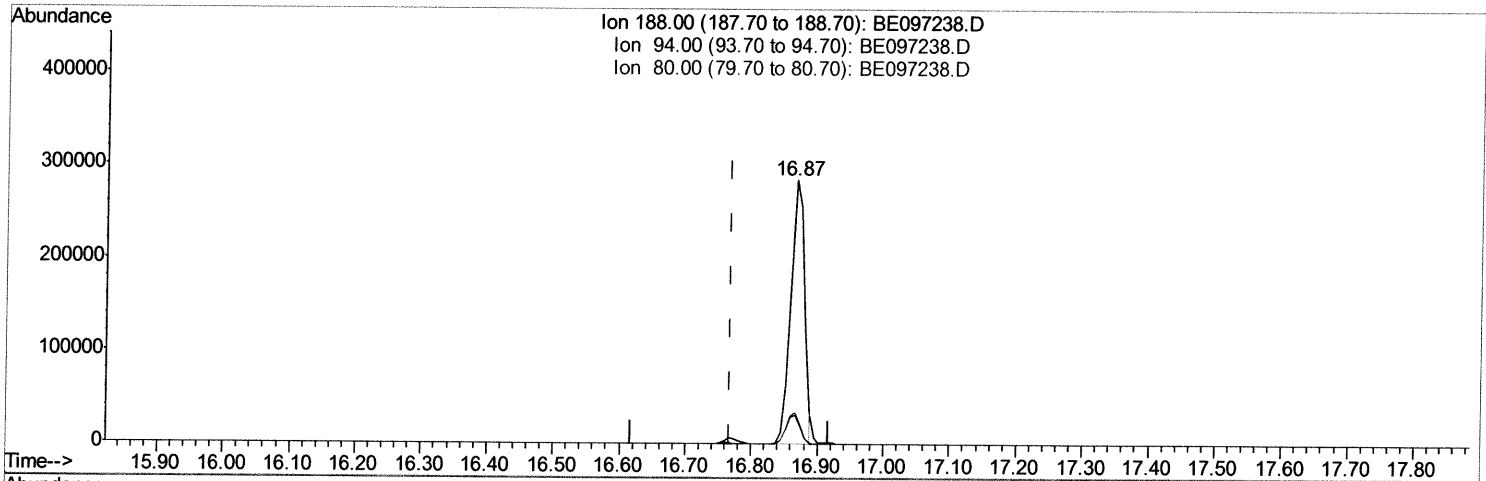

(10) Phenanthrene-d10 (I)
 16.866min (+0.098) 0.40ng/ul
 response 400091

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.99
80.00	11.80	11.15
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097238.D
Acq On : 8 Aug 2018 16:55
Operator : SJ/JU
Sample : J4268-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA1

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:16 PM

Quant Time: Aug 08 23:27:19 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

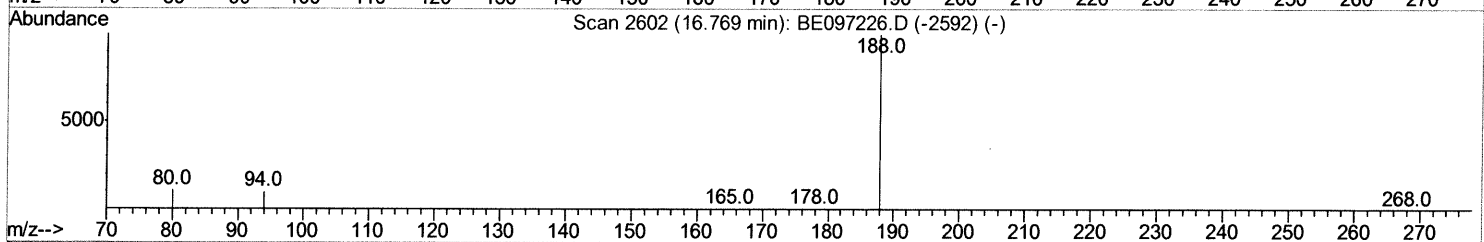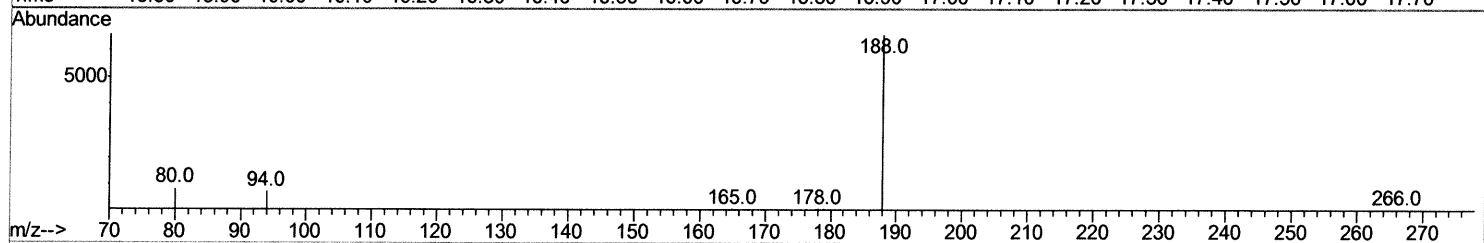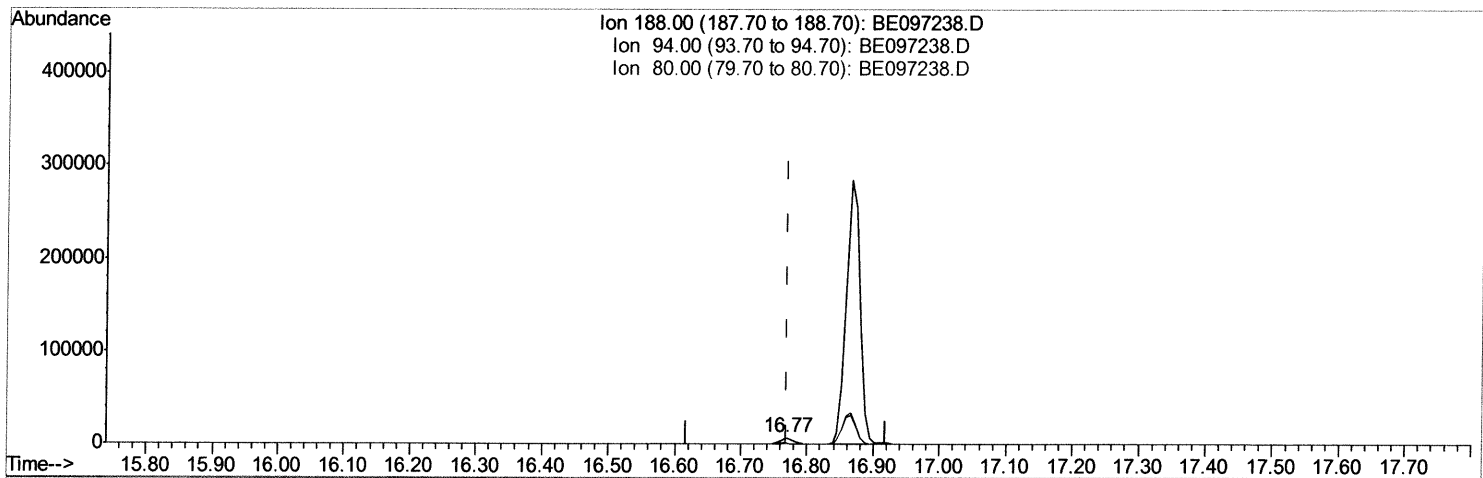

TIC: BE097238.D

(10) Phenanthrene-d10 (I)

16.768min (-0.001) 0.40ng/ul m> SJ 8/10/18

response 9269

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.84
80.00	11.80	12.43
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097238.D
 Acq On : 8 Aug 2018 16:55
 Operator : SJ/JU
 Sample : J4268-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:16 PM

Quant Time: Aug 09 01:07:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

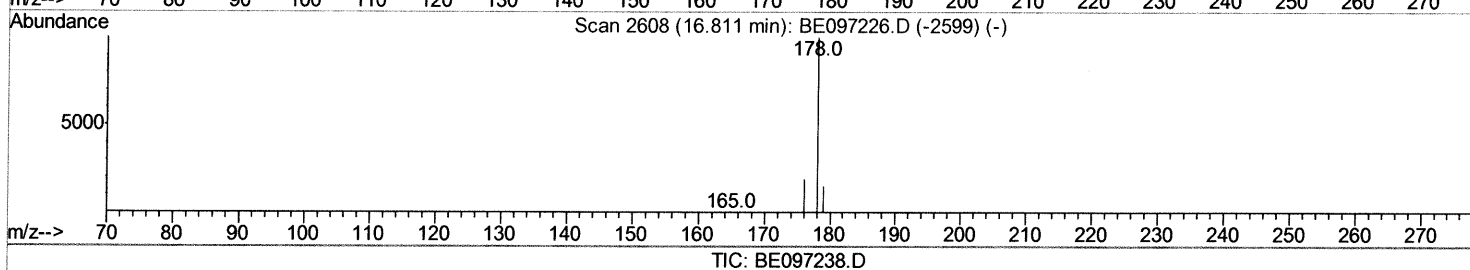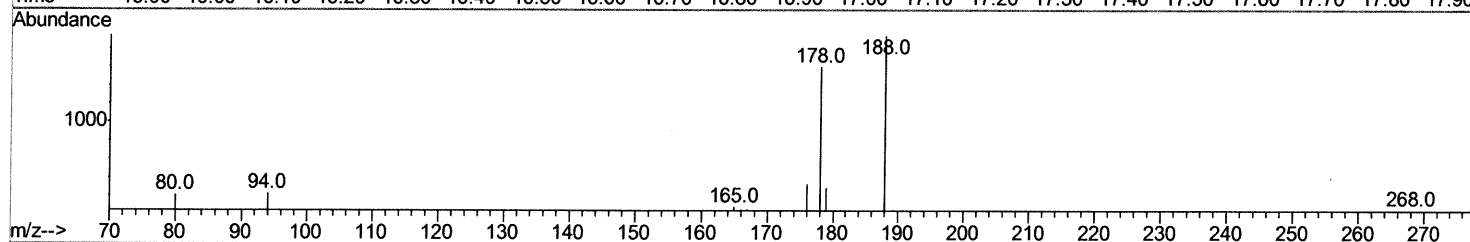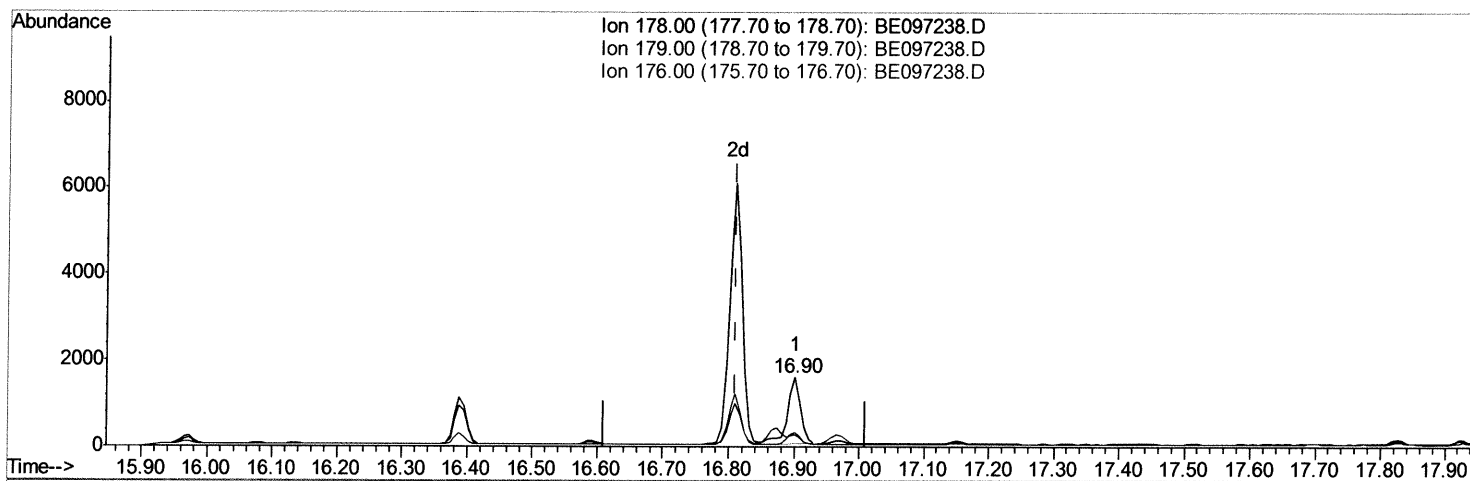

(12) Phenanthrene

16.902min (+0.091) 0.09ng/ul

response 2163

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	17.99#
176.00	17.00	20.36
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097238.D
 Acq On : 8 Aug 2018 16:55
 Operator : SJ/JU
 Sample : J4268-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:16 PM

Quant Time: Aug 09 01:07:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

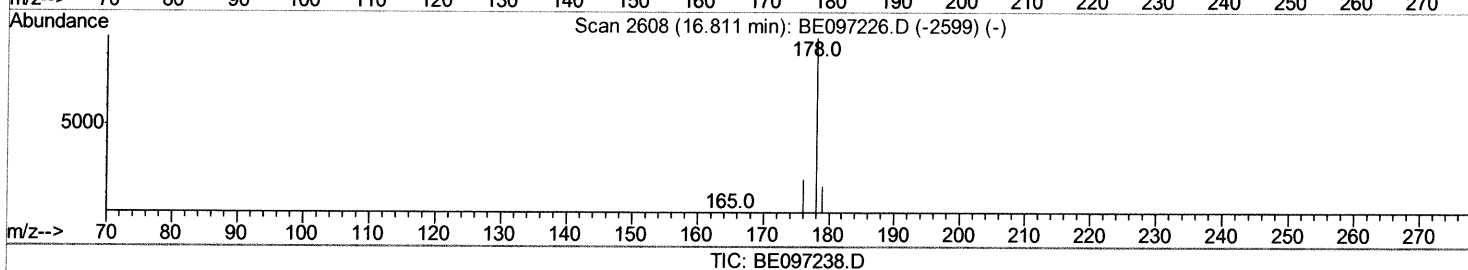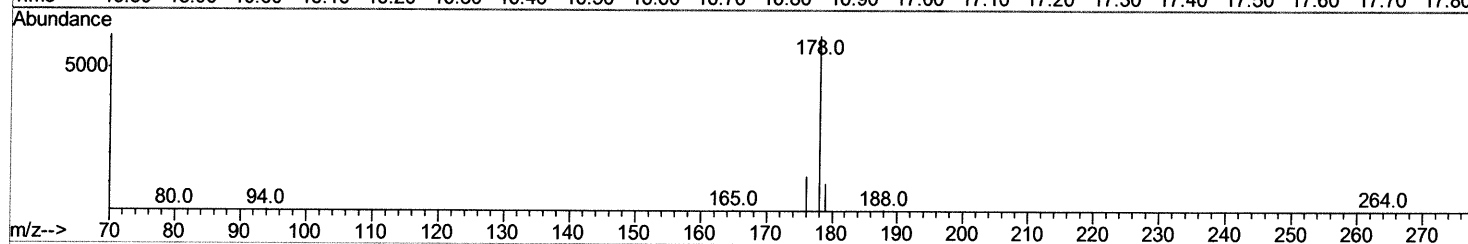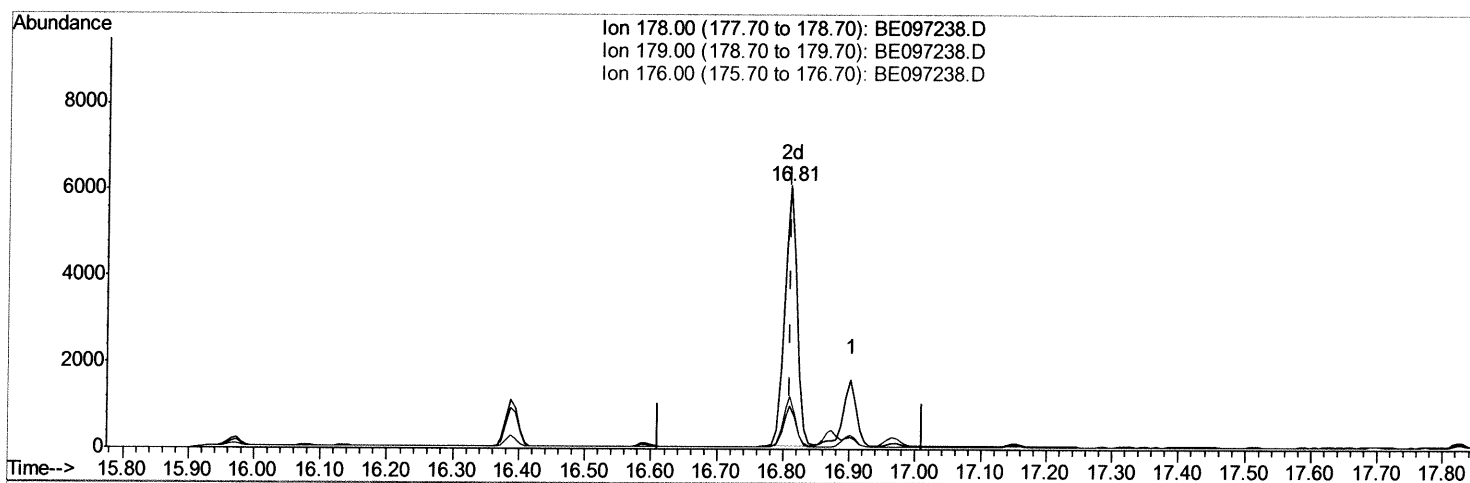

(12) Phenanthrene

16.810min (-0.001) 0.34ng/ul m > SJ 8/10/18

response 8139

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	16.45#
176.00	17.00	20.18
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097238.D
Acq On : 8 Aug 2018 16:55
Operator : SJ/JU
Sample : J4268-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA1

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:16 PM

Quant Time: Aug 09 01:07:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

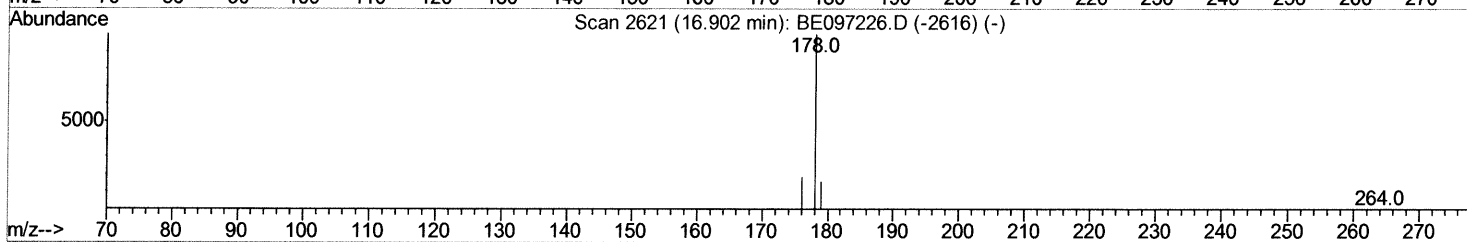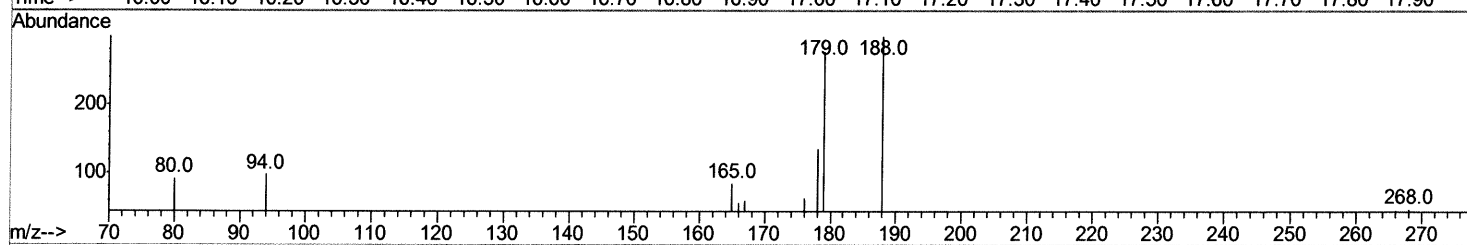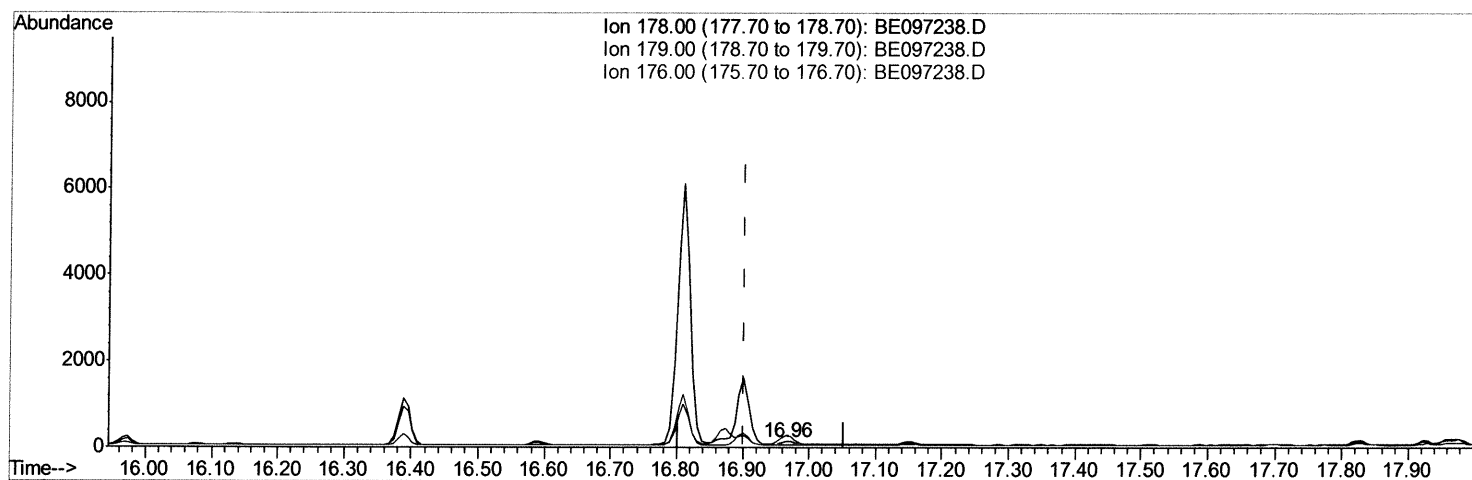

TIC: BE097238.D

(13) Anthracene

16.965min (+0.062) 0.00ng/ul

response 98

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	204.44#
176.00	18.40	47.41#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097238.D
 Acq On : 8 Aug 2018 16:55
 Operator : SJ/JU
 Sample : J4268-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:16 PM

Quant Time: Aug 09 01:07:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

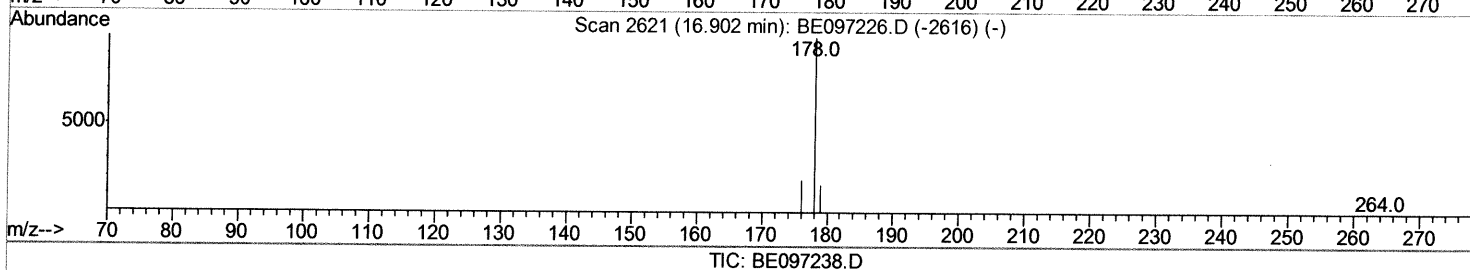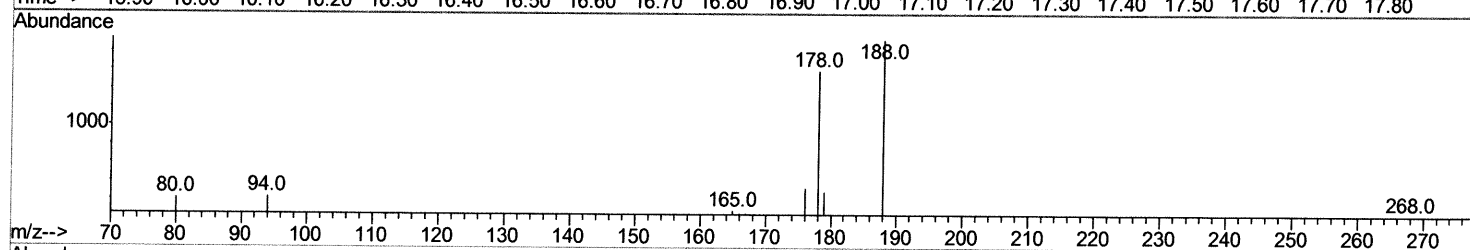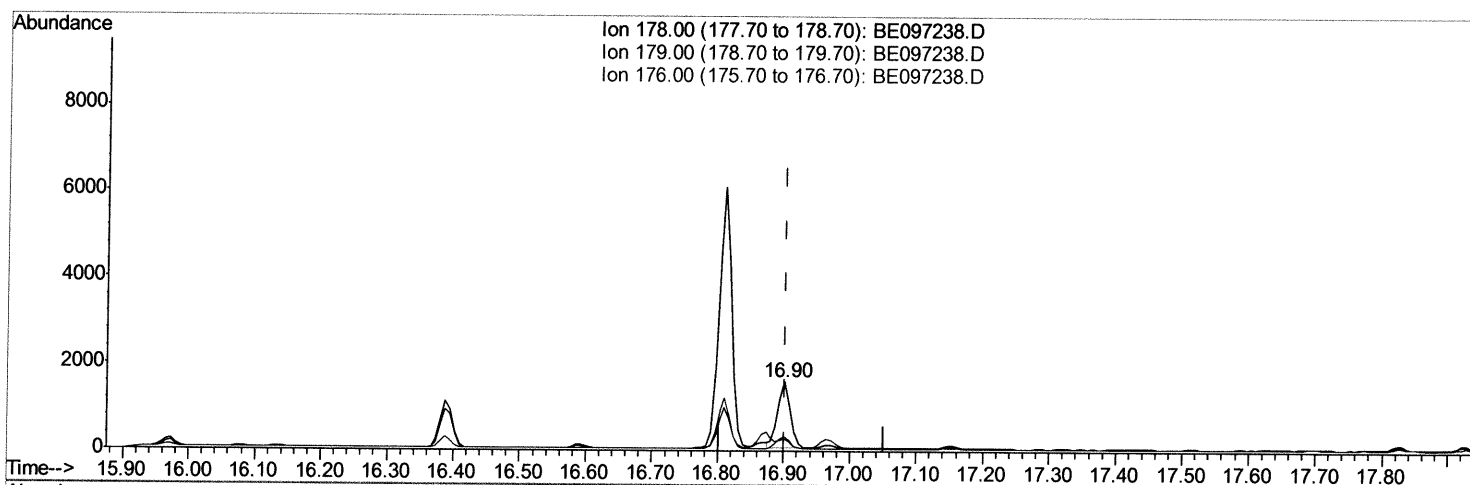

(13) Anthracene

16.902min (-0.001) 0.09ng/ul m > SJ 8/10/18

response 1984

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	17.99#
176.00	18.40	20.36
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097238.D
 Acq On : 8 Aug 2018 16:55
 Operator : SJ/JU
 Sample : J4268-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:16 PM

Quant Time: Aug 09 01:07:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

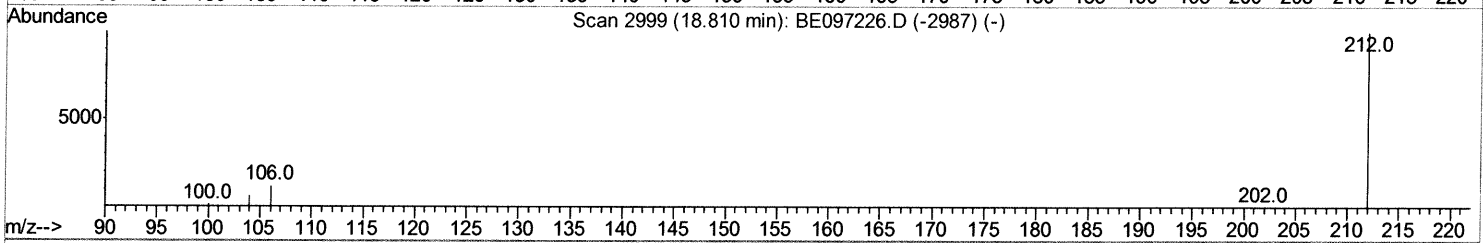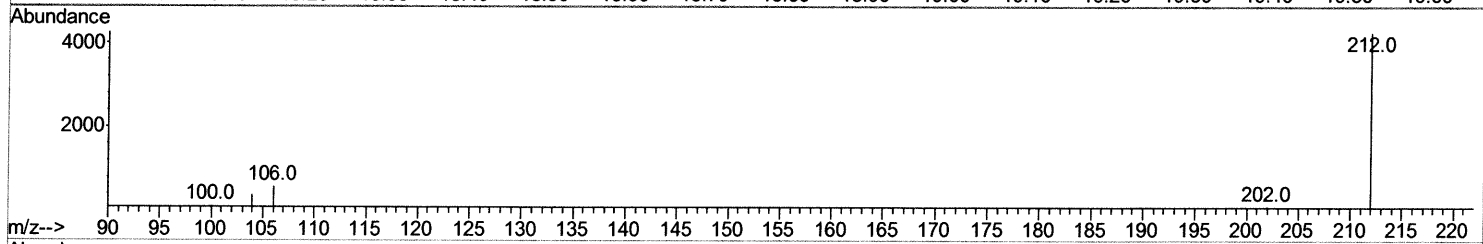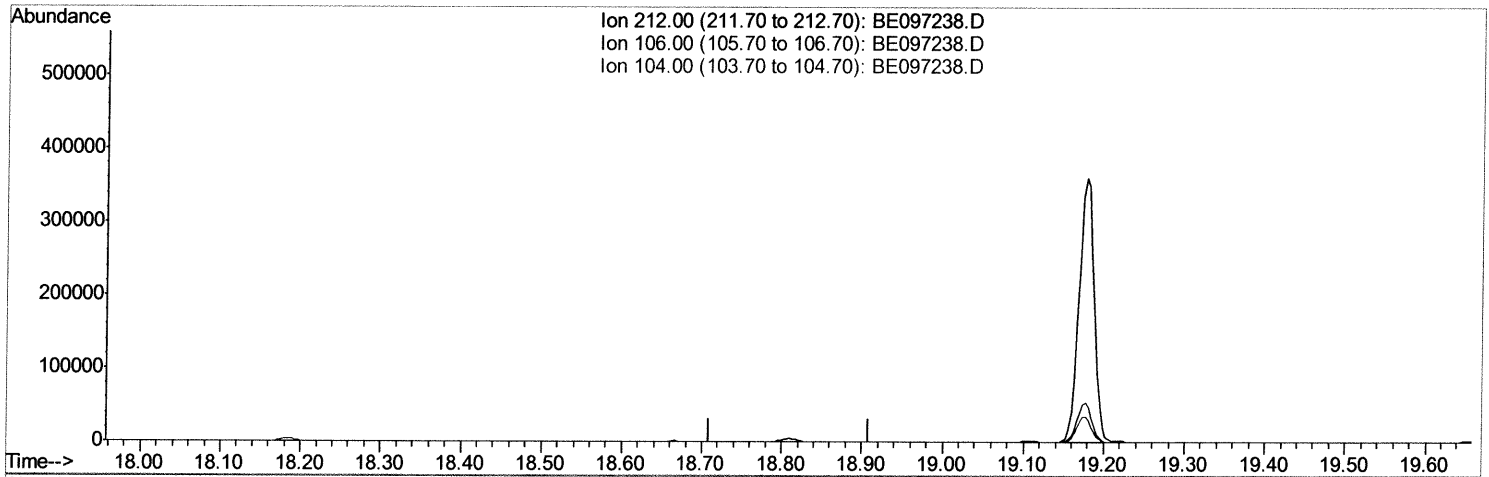

TIC: BE097238.D

(14) Fluoranthene-d10 (SURR)

18.810min (-18.810) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097238.D
 Acq On : 8 Aug 2018 16:55
 Operator : SJ/JU
 Sample : J4268-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:16 PM

Quant Time: Aug 09 01:07:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

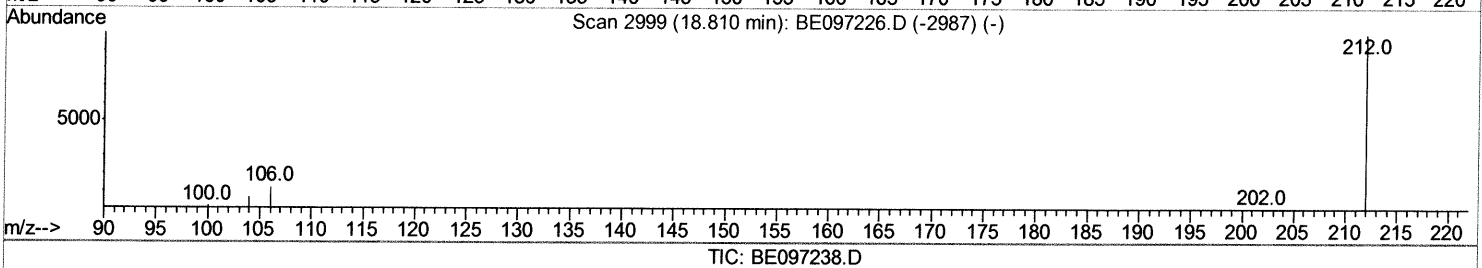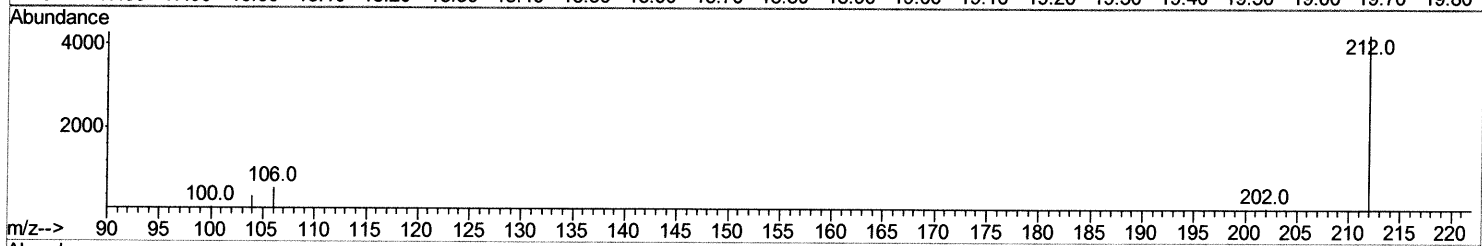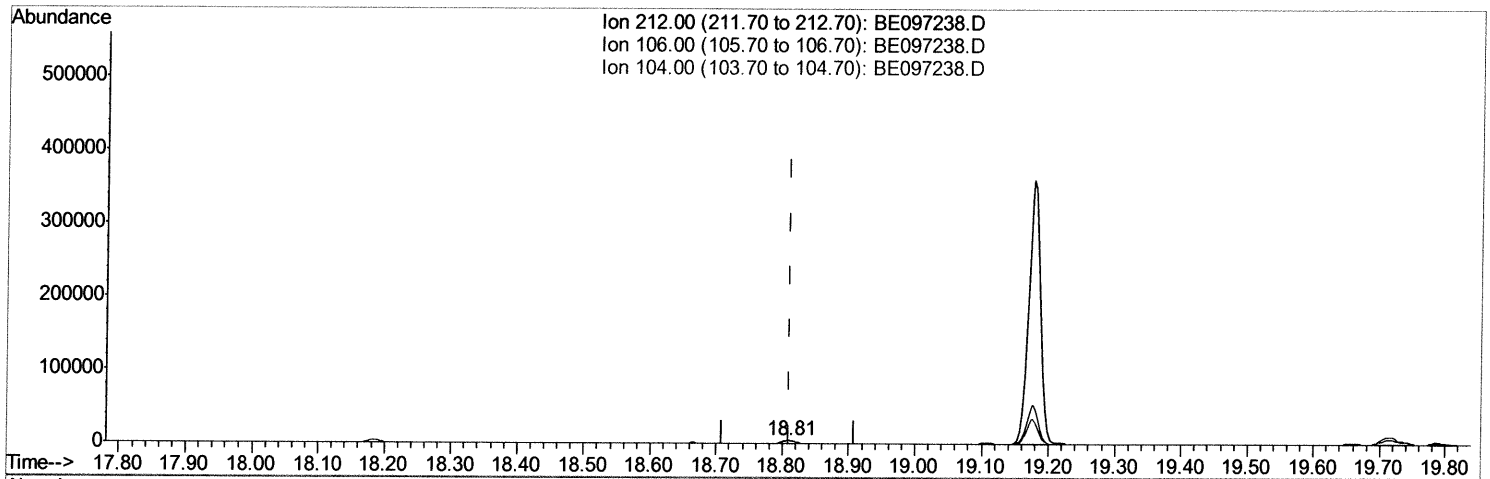

(14) Fluoranthene-d10 (SURR)

18.810min (+0.000) 0.17ng/ul m> SJ 8/10/18

response 5575

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097238.D
Acq On : 8 Aug 2018 16:55
Operator : SJ/JU
Sample : J4268-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA1

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:16 PM

Quant Time: Aug 09 01:07:02 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

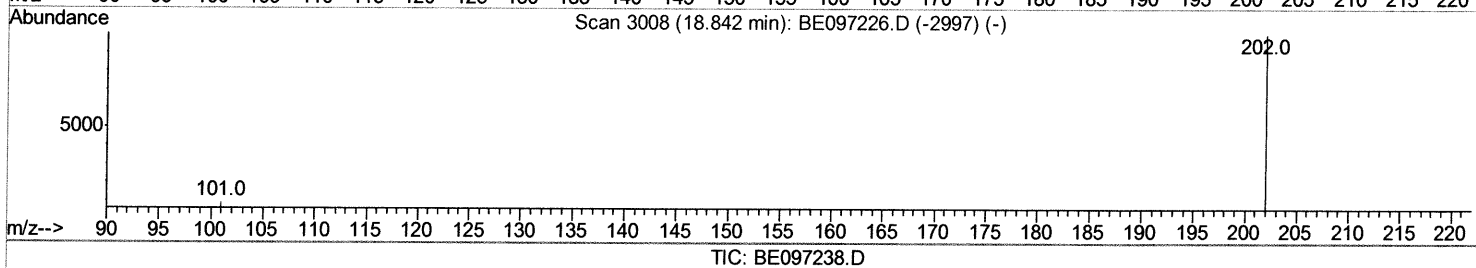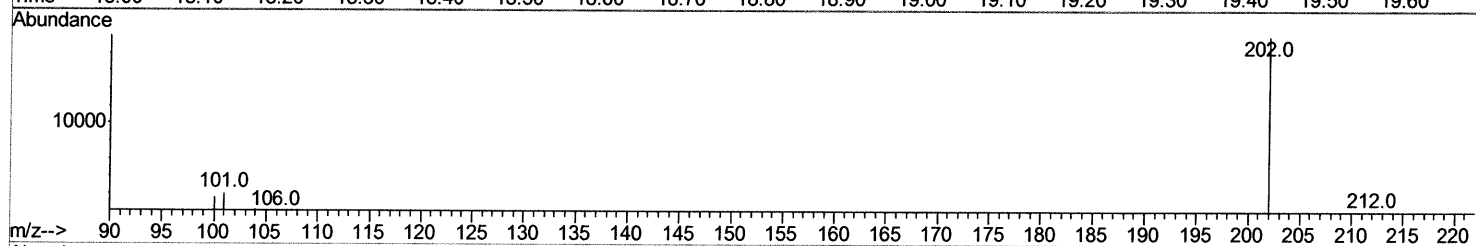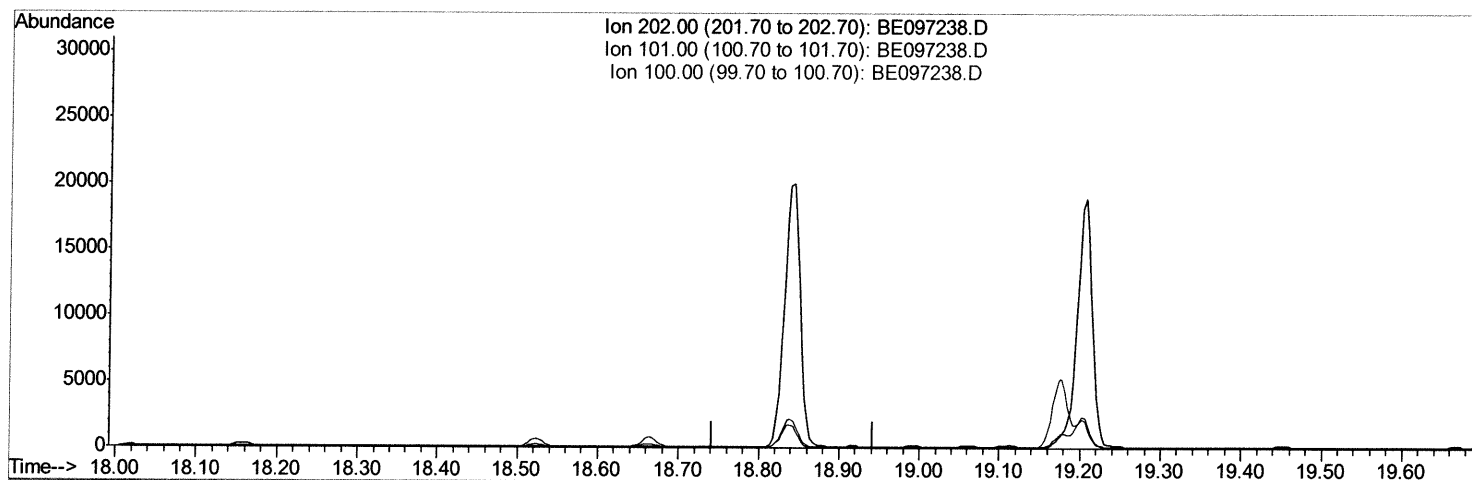

(15) Fluoranthene (C)

18.842min (-18.842) 0.00ng/ul

response 0

Ion	Exp%	Act%
202.00	100	0.00
101.00	10.30	0.00
100.00	19.50	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097238.D
 Acq On : 8 Aug 2018 16:55
 Operator : SJ/JU
 Sample : J4268-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:16 PM

Quant Time: Aug 09 01:07:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

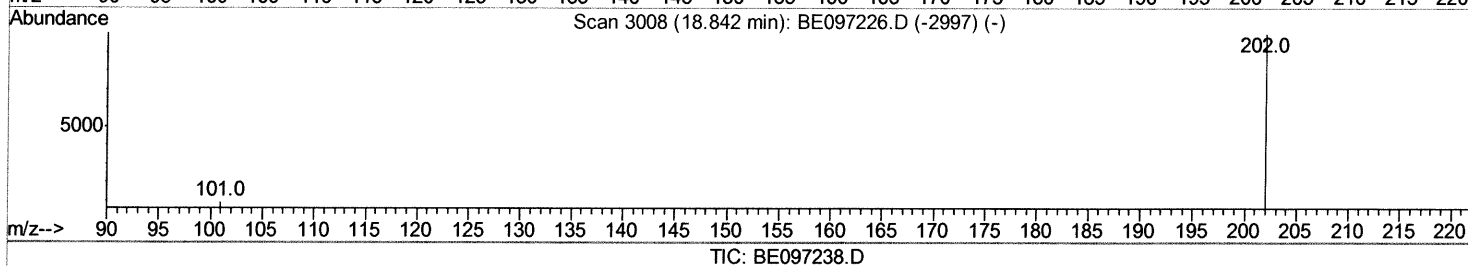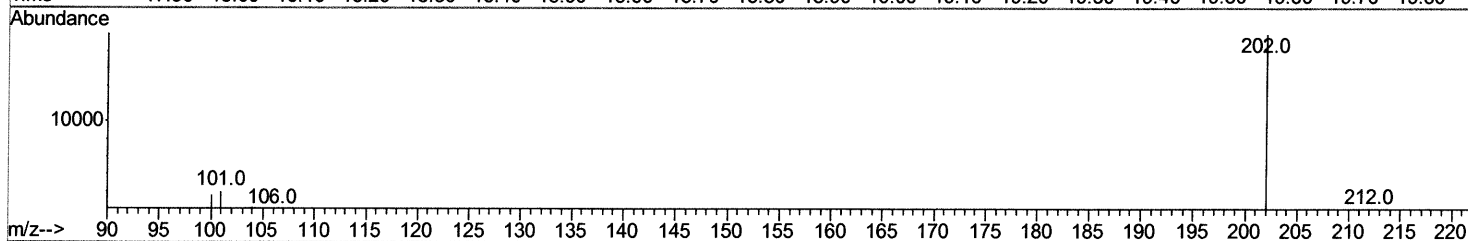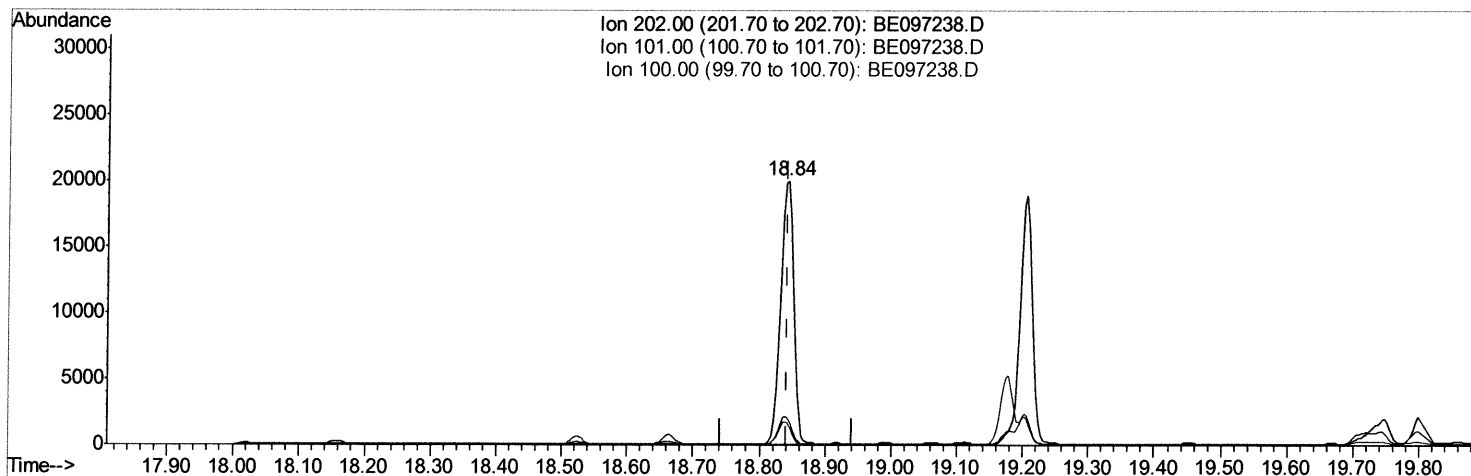

(15) Fluoranthene (C)

18.842min (+0.000) 0.87ng/ul m> SJ 8/10/18

response 27057

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	9.96
100.00	19.50	8.03
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097238.D
 Acq On : 8 Aug 2018 16:55
 Operator : SJ/JU
 Sample : J4268-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:16 PM

Quant Time: Aug 09 01:07:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

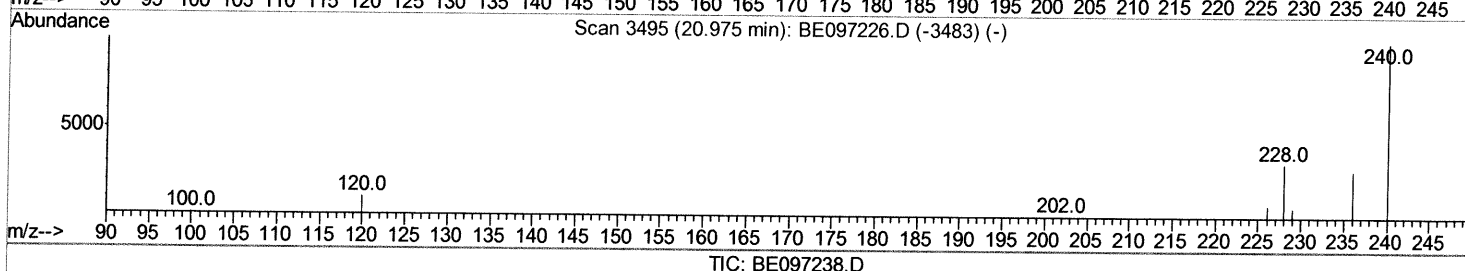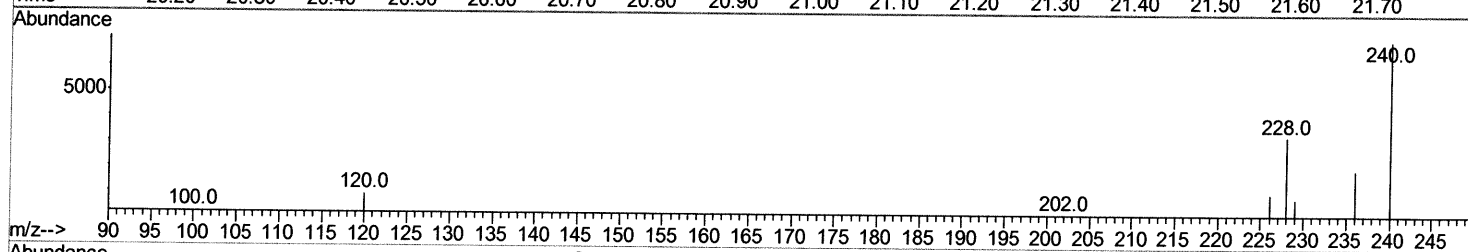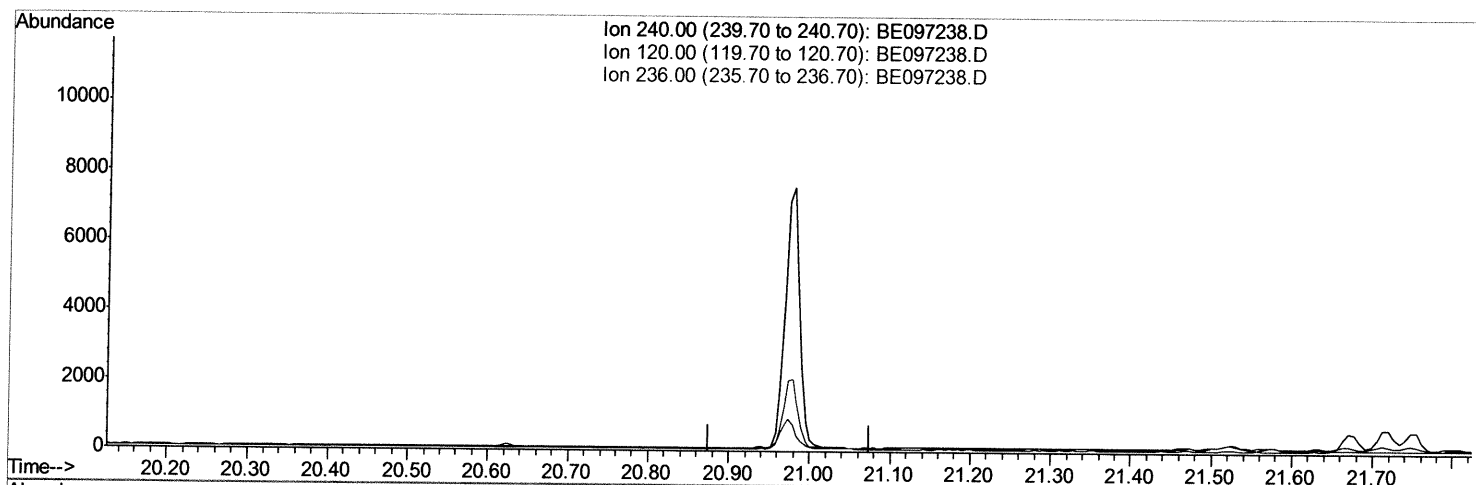

(16) Chrysene-d12 (I)

20.975min (-20.975) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.60	0.00#
236.00	34.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097238.D
 Acq On : 8 Aug 2018 16:55
 Operator : SJ/JU
 Sample : J4268-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:16 PM

Quant Time: Aug 09 01:07:02 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

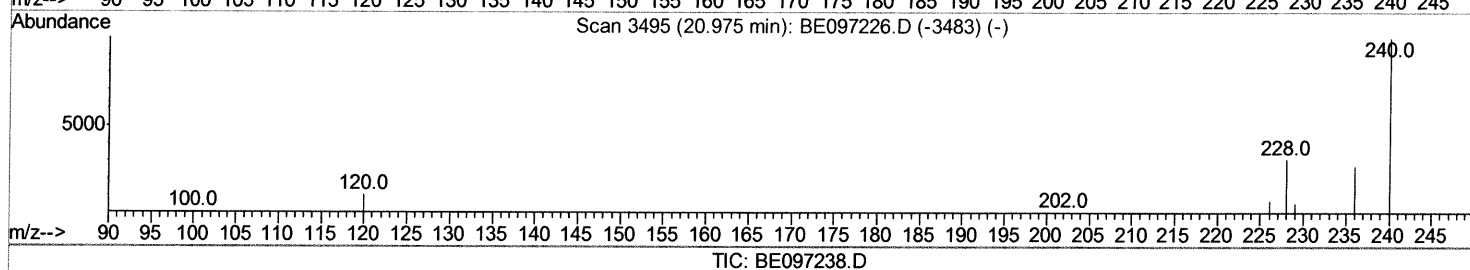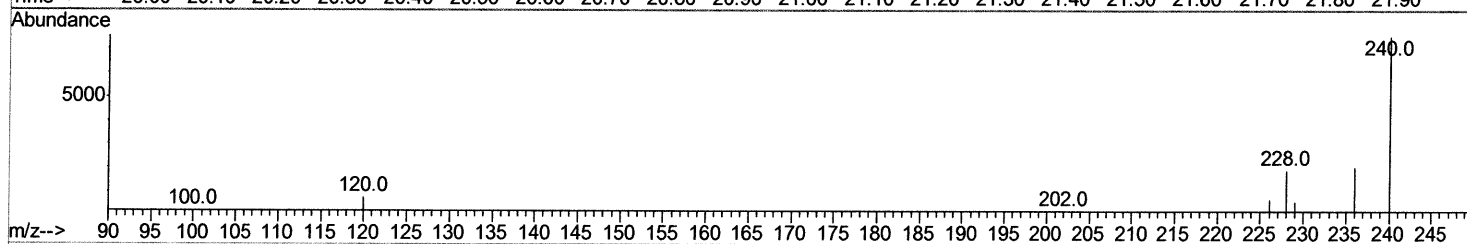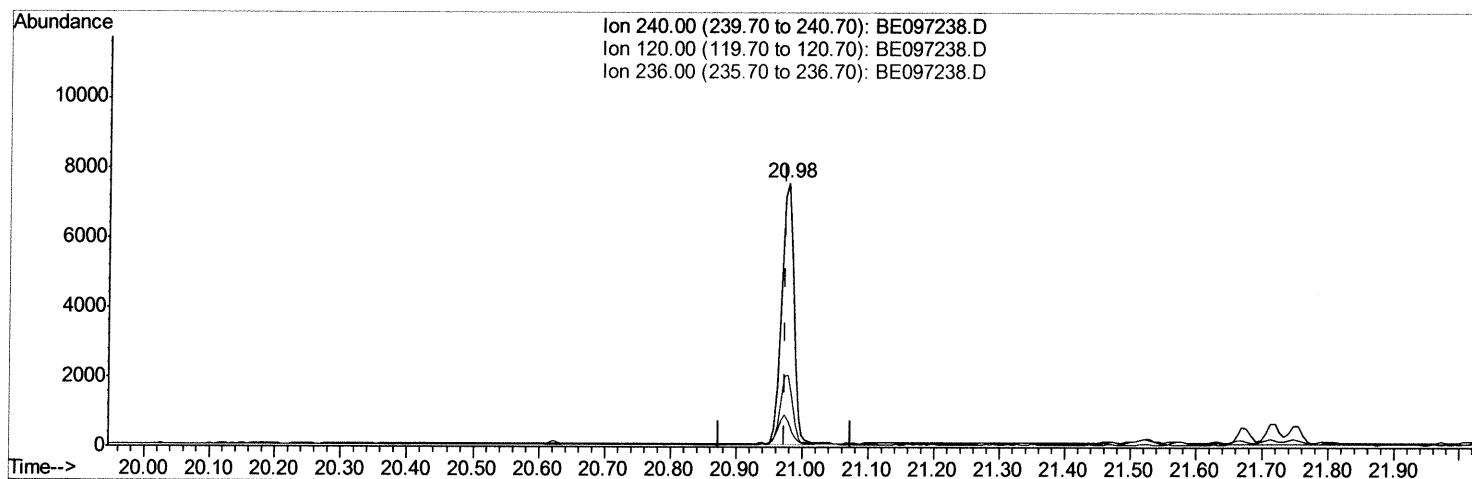

(16) Chrysene-d12 (I)

20.978min (+0.004) 0.40ng/ul m > SJ 8/10/18

response 9511

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	10.05#
236.00	34.90	27.22#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097238.D
Acq On : 8 Aug 2018 16:55
Operator : SJ/JU
Sample : J4268-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AA1

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:16 PM

Quant Time: Aug 09 01:09:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

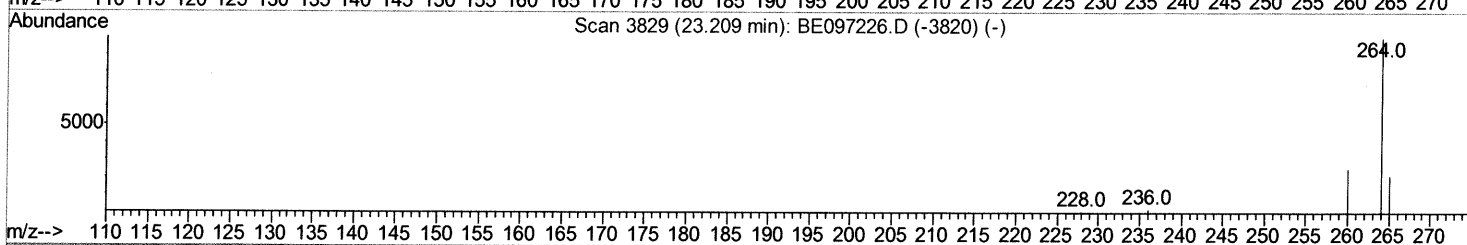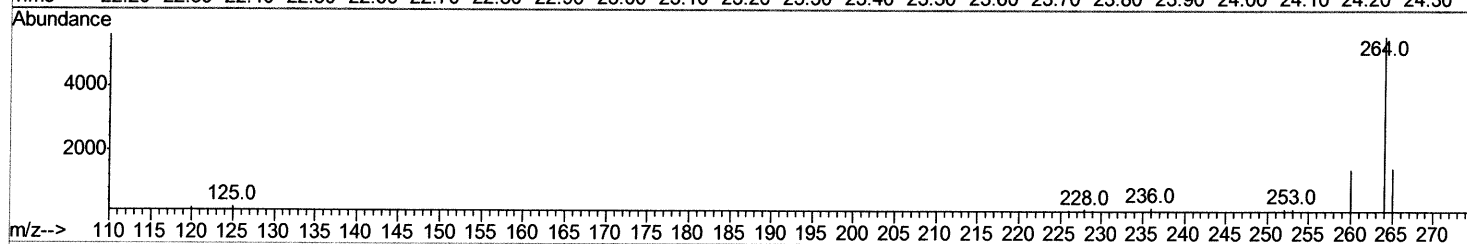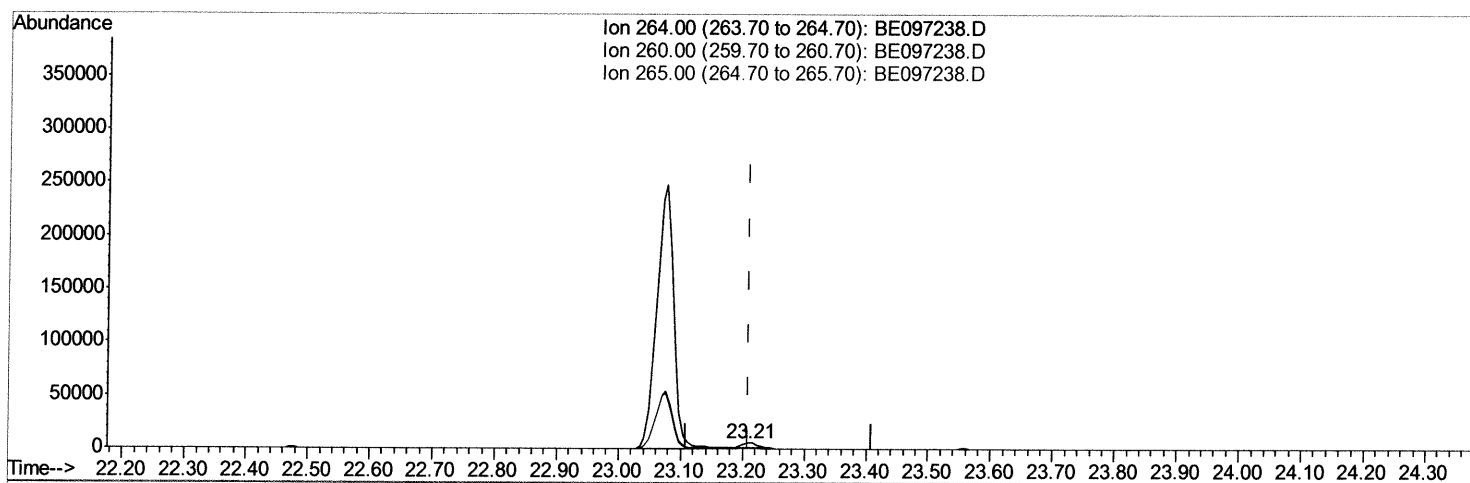

TIC: BE097238.D

(20) Perylene-d12 (I)

23.210min (+0.000) 0.40ng/ul

response 12019

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.34
265.00	103.50	26.17#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097238.D
Acq On : 8 Aug 2018 16:55
Operator : SJ/JU
Sample : J4268-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA1

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:16 PM

Quant Time: Aug 09 01:09:22 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

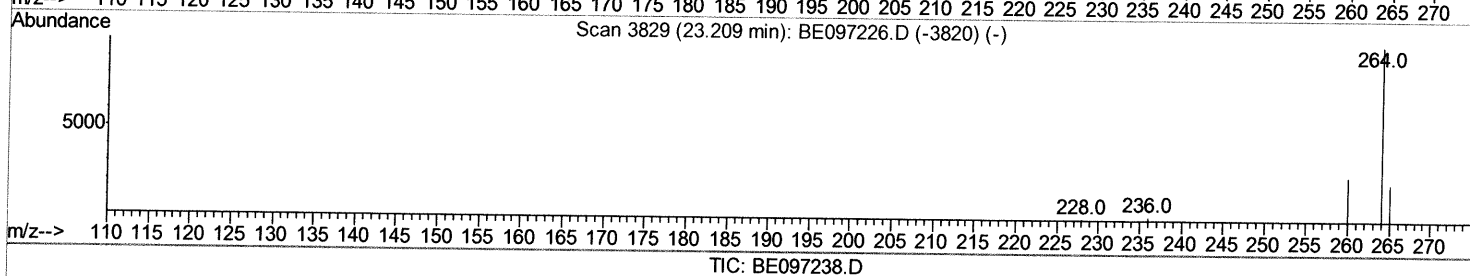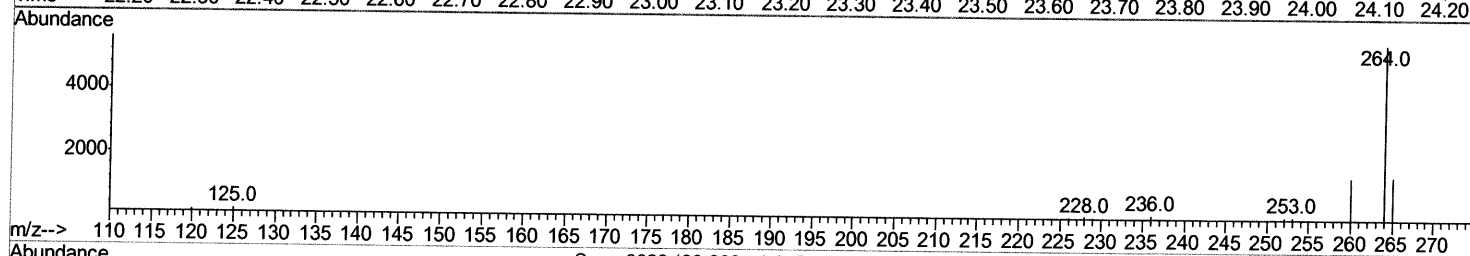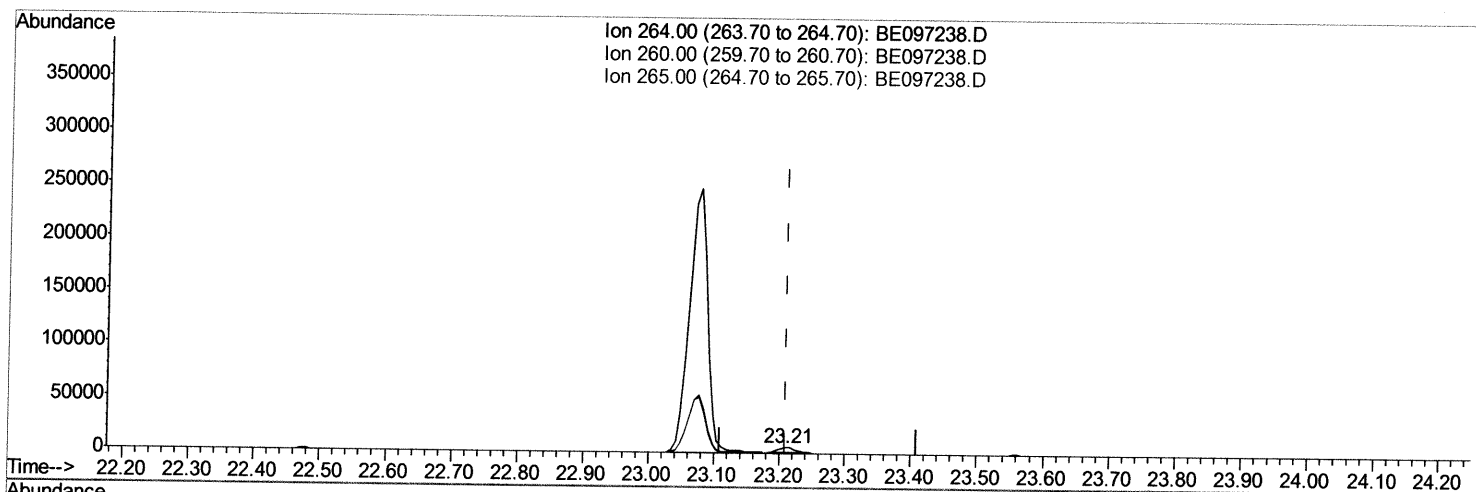

(20) Perylene-d12 (I)

23.210min (+0.000) 0.40ng/ul m > SJ 8/10/18

response 8979

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.34
265.00	103.50	26.17#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097238.D
 Acq On : 8 Aug 2018 16:55
 Operator : SJ/JU
 Sample : J4268-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:16 PM

Quant Time: Aug 09 01:09:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

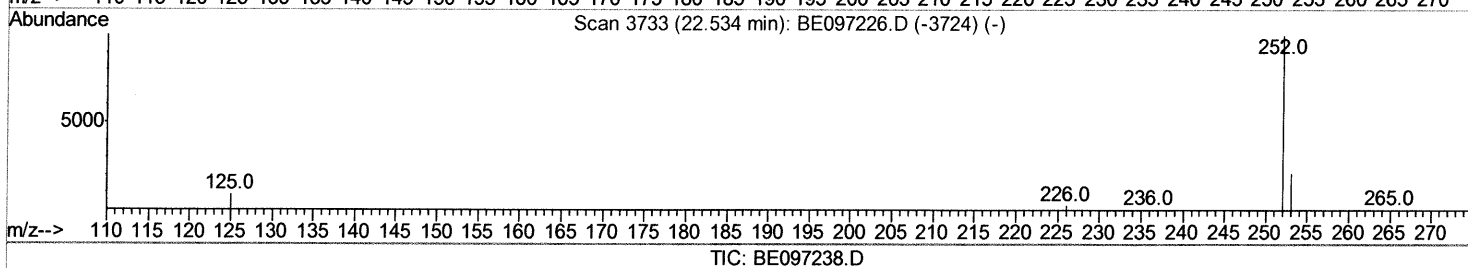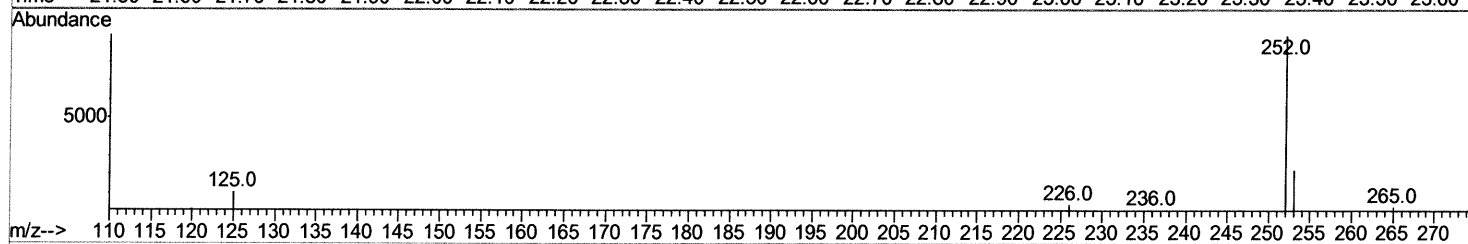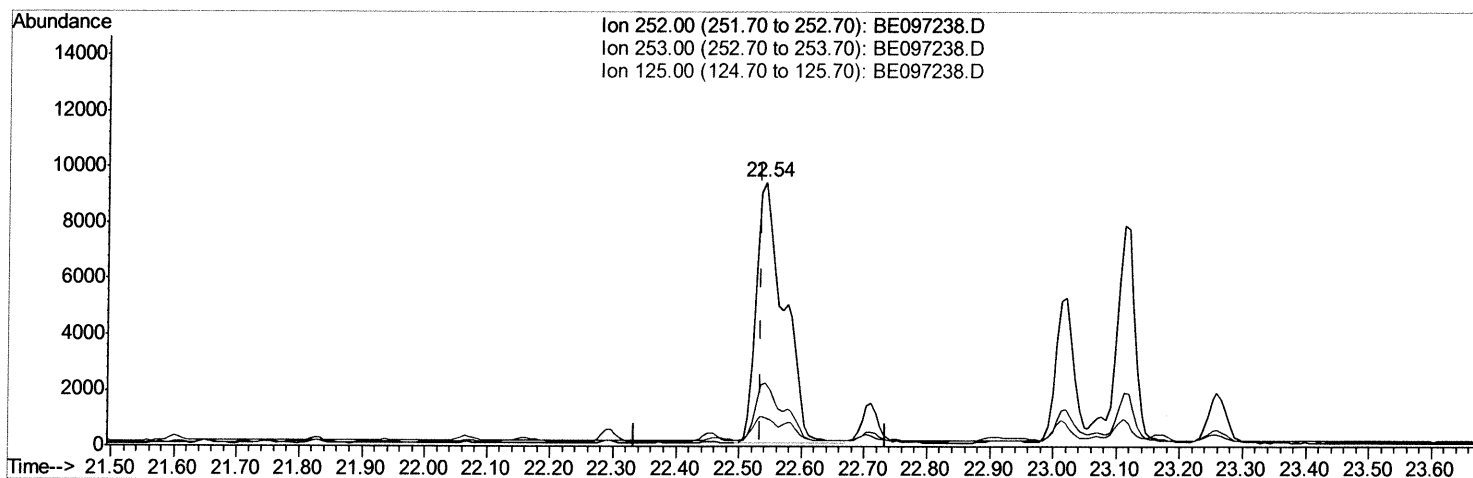

(21) Benzo(b)fluoranthene
 22.542min (+0.008) 1.17ng/ul
 response 28670

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	24.13
125.00	17.50	11.06
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097238.D
Acq On : 8 Aug 2018 16:55
Operator : SJ/JU
Sample : J4268-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AA1

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:16 PM

Quant Time: Aug 09 01:09:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

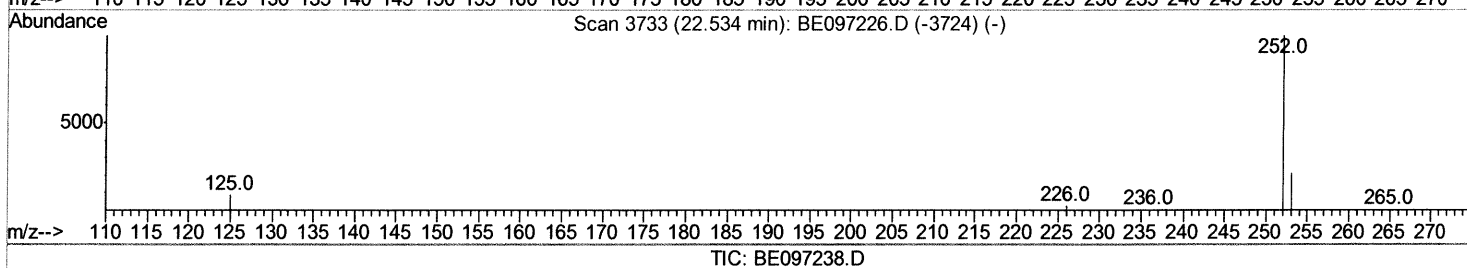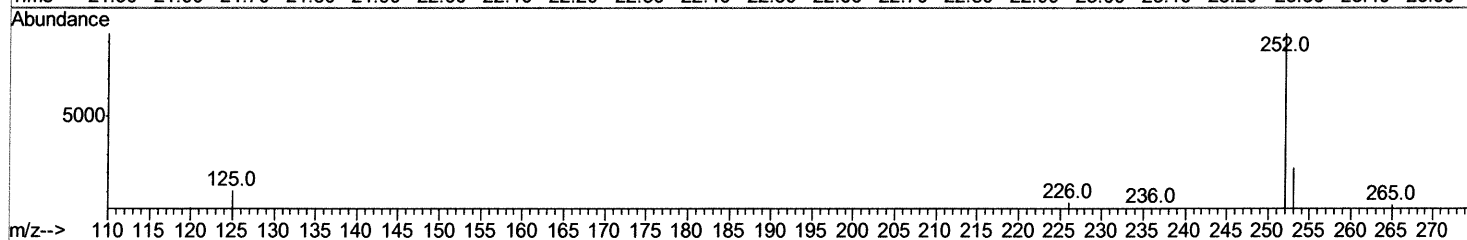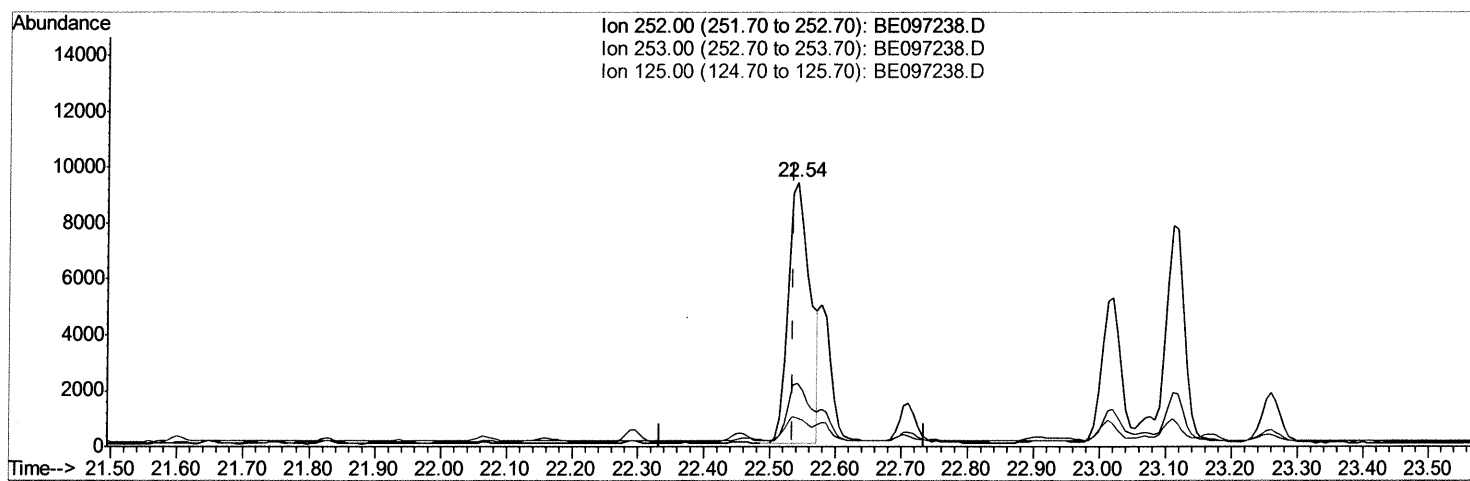

(21) Benzo(b)fluoranthene

22.542min (+0.008) 0.90ng/ul m> SJ 8/10/18

response 22018

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	24.13
125.00	17.50	11.06
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097238.D
 Acq On : 8 Aug 2018 16:55
 Operator : SJ/JU
 Sample : J4268-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:16 PM

Quant Time: Aug 09 01:09:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

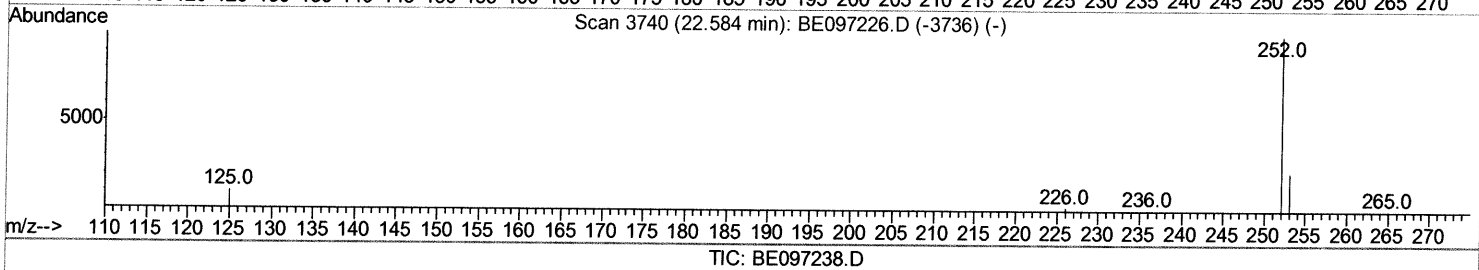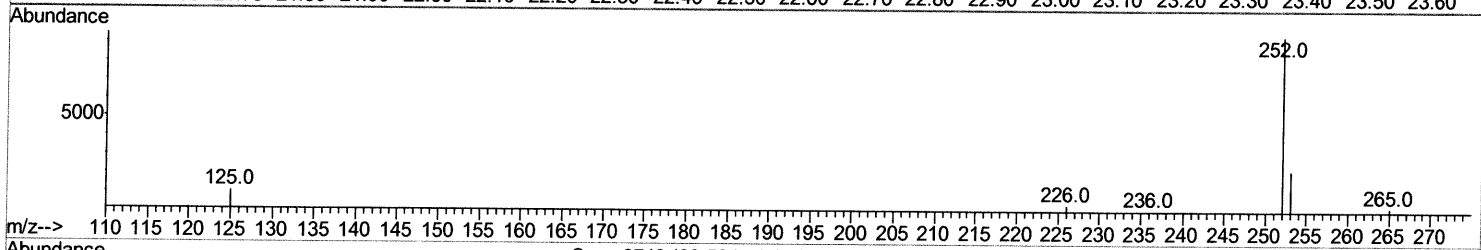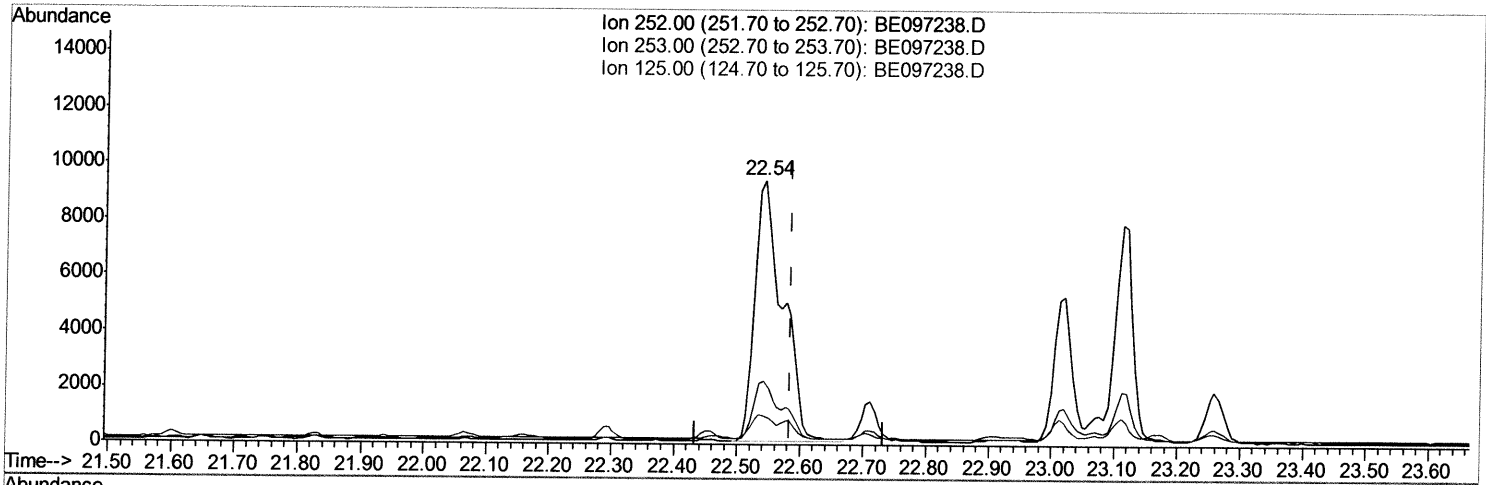

(22) Benzo(k)fluoranthene
 22.542min (-0.042) 1.09ng/ul
 response 28670

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	24.13#
125.00	17.10	11.06#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097238.D
 Acq On : 8 Aug 2018 16:55
 Operator : SJ/JU
 Sample : J4268-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:16 PM

Quant Time: Aug 09 01:09:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

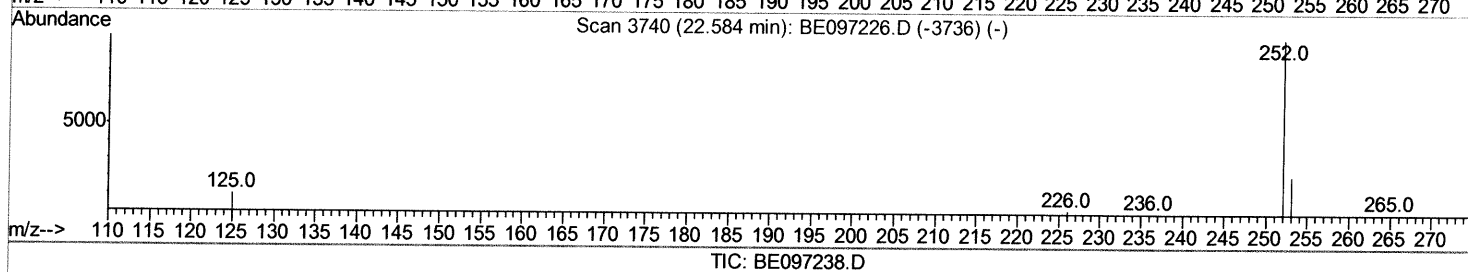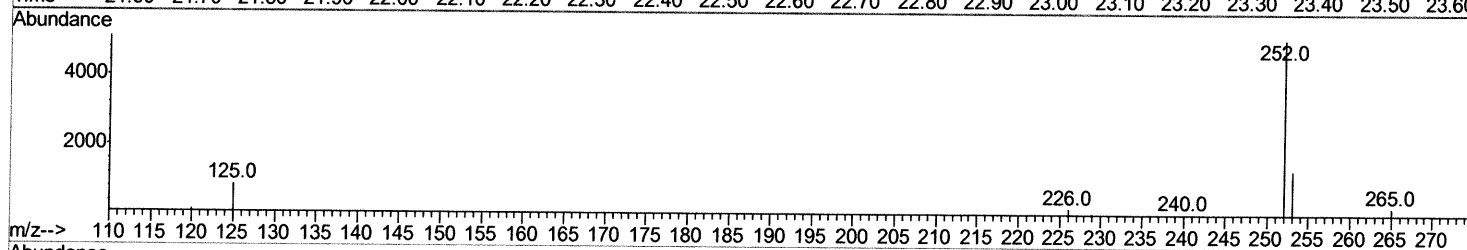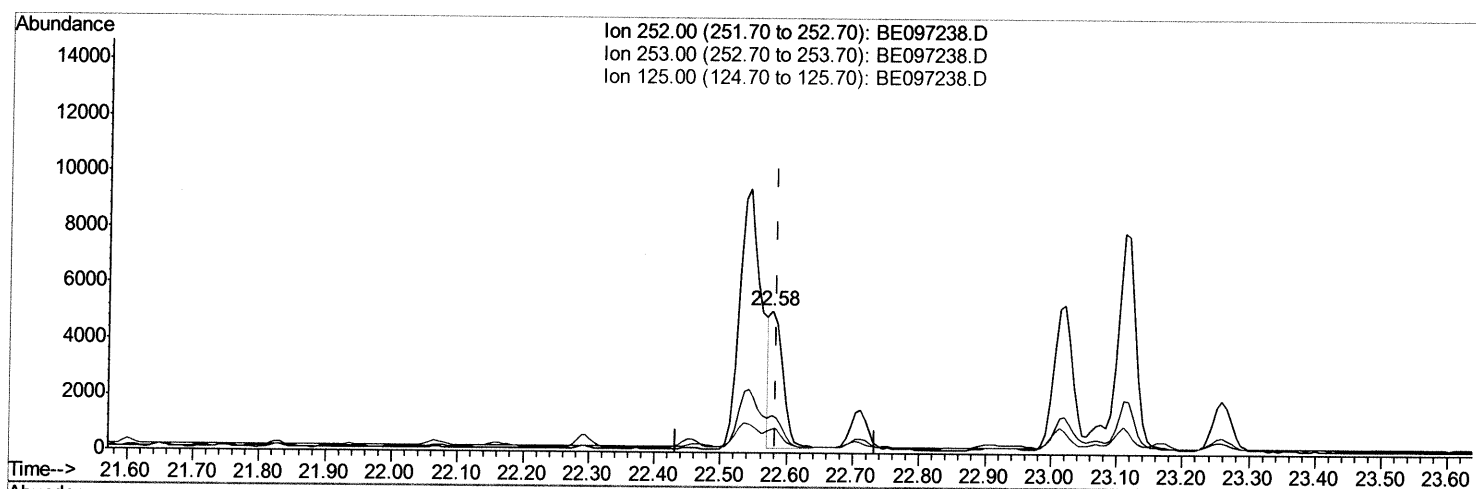

(22) Benzo(k)fluoranthene

22.577min (-0.007) 0.24ng/ul m> 51 8/10/18

response 6287

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	26.38
125.00	17.10	16.92
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097238.D
 Acq On : 8 Aug 2018 16:55
 Operator : SJ/JU
 Sample : J4268-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA1

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:16 PM

Quant Time: Aug 09 01:12:37 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1235	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6613	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	3990	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.77	188	9269m	0.40	ng/ul	0.00
16) Chrysene-d12	20.98	240	9511m	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	8979m	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.72	152	2005	0.19	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	5575m	0.17	ng/ul	0.00

Target Compounds

					Ovalue	
3) Naphthalene	10.18	128	866	0.054	ng/ul#	85
8) Acenaphthene	14.08	153	259	0.021	ng/ul#	88
9) Fluorene	15.08	166	320	0.022	ng/ul#	90
12) Phenanthrene	16.81	178	8139m	0.344	ng/ul	
13) Anthracene	16.90	178	1984m	0.090	ng/ul	
15) Fluoranthene	18.84	202	27057m	0.866	ng/ul	
17) Pyrene	19.21	202	24953	0.979	ng/ul#	79
18) Benzo(a)anthracene	20.96	228	13823	0.509	ng/ul#	86
19) Chrysene	21.01	228	16147	0.577	ng/ul	98
21) Benzo(b)fluoranthene	22.54	252	22018m	0.900	ng/ul	
22) Benzo(k)fluoranthene	22.58	252	6287m	0.238	ng/ul	
23) Benzo(a)pyrene	23.11	252	15865	0.648	ng/ul#	80
24) Indeno(1,2,3-cd)pyrene	25.50	276	10362	0.338	ng/ul#	72
25) Dibenzo(a,h)anthracene	25.52	278	2503	0.100	ng/ul#	92
26) Benzo(a,h,i)perylene	26.21	276	9755	0.368	ng/ul#	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed