

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097240.D
 Acq On : 8 Aug 2018 18:13
 Operator : SJ/JU
 Sample : J4268-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:34:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

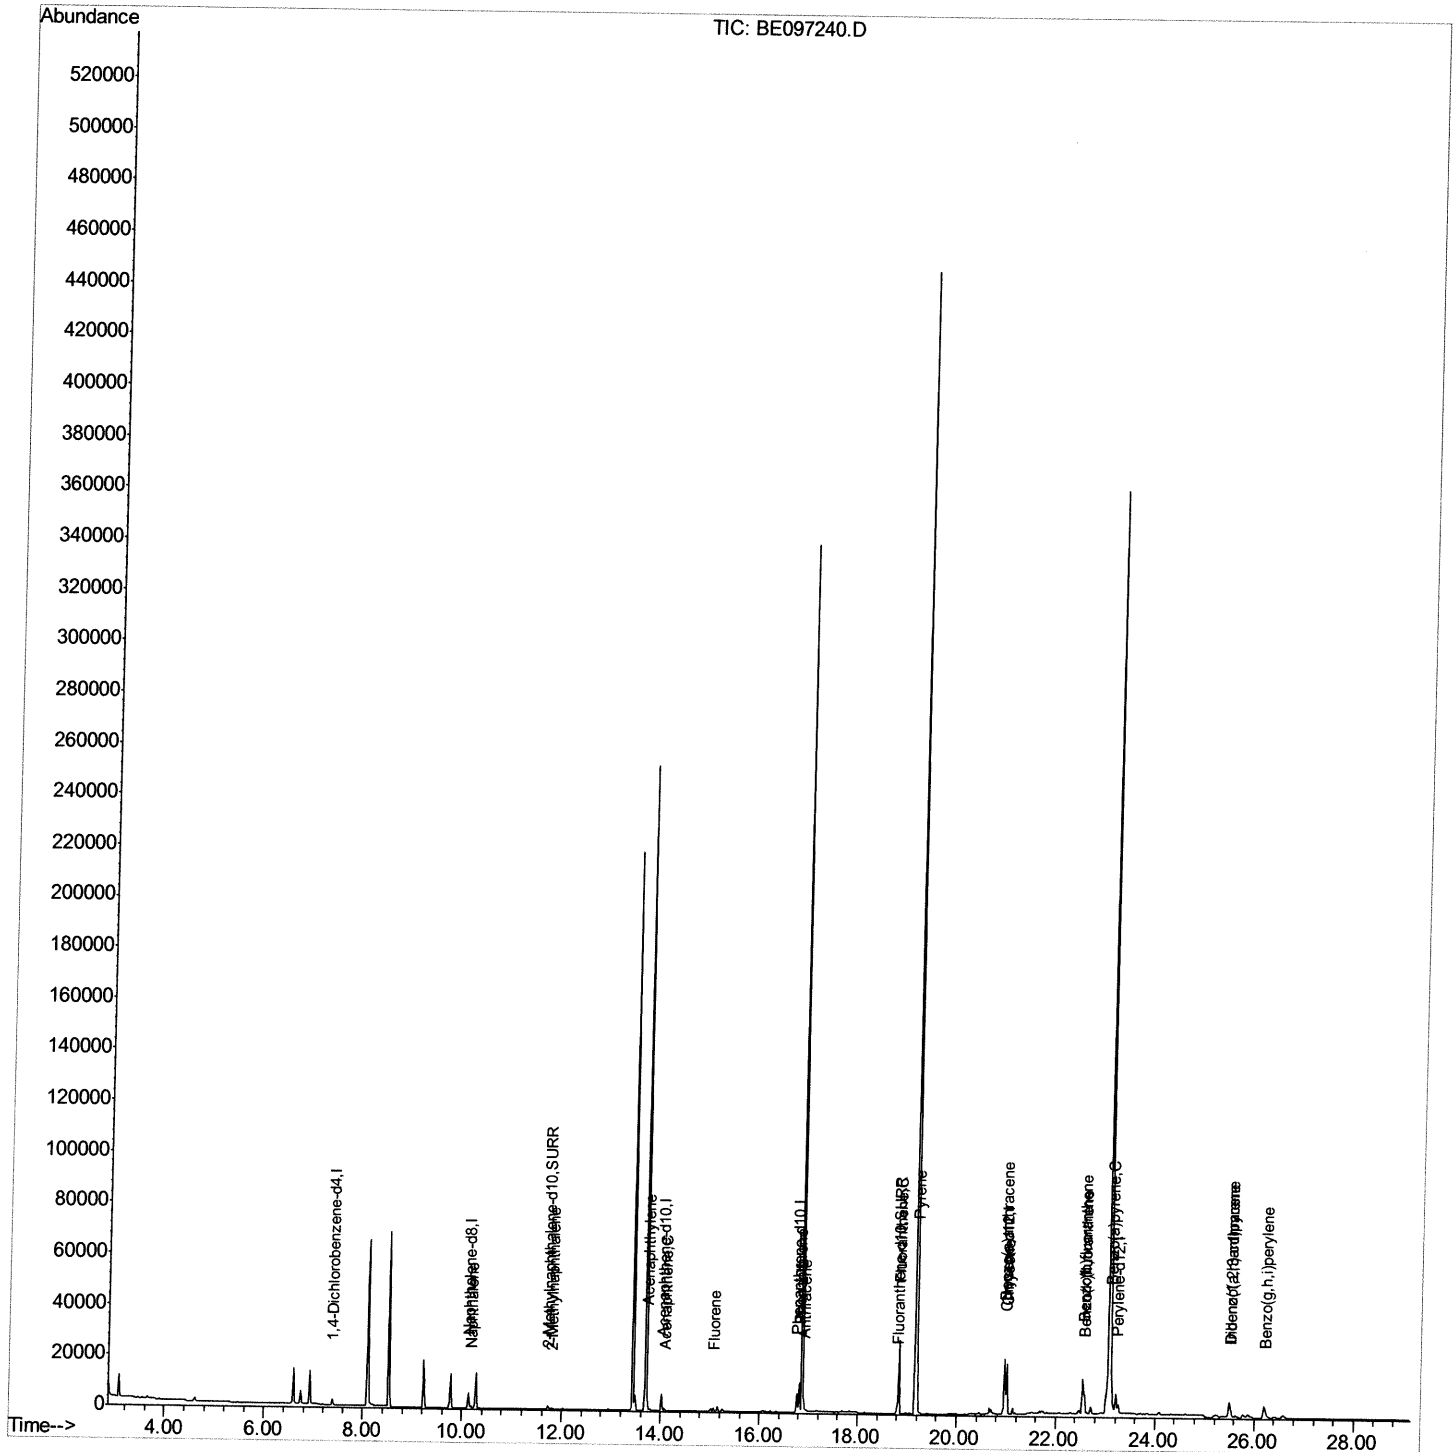

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097240.D
Acq On : 8 Aug 2018 18:13
Operator : SJ/JU
Sample : J4268-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:21 PM

Quant Time: Aug 08 23:27:30 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

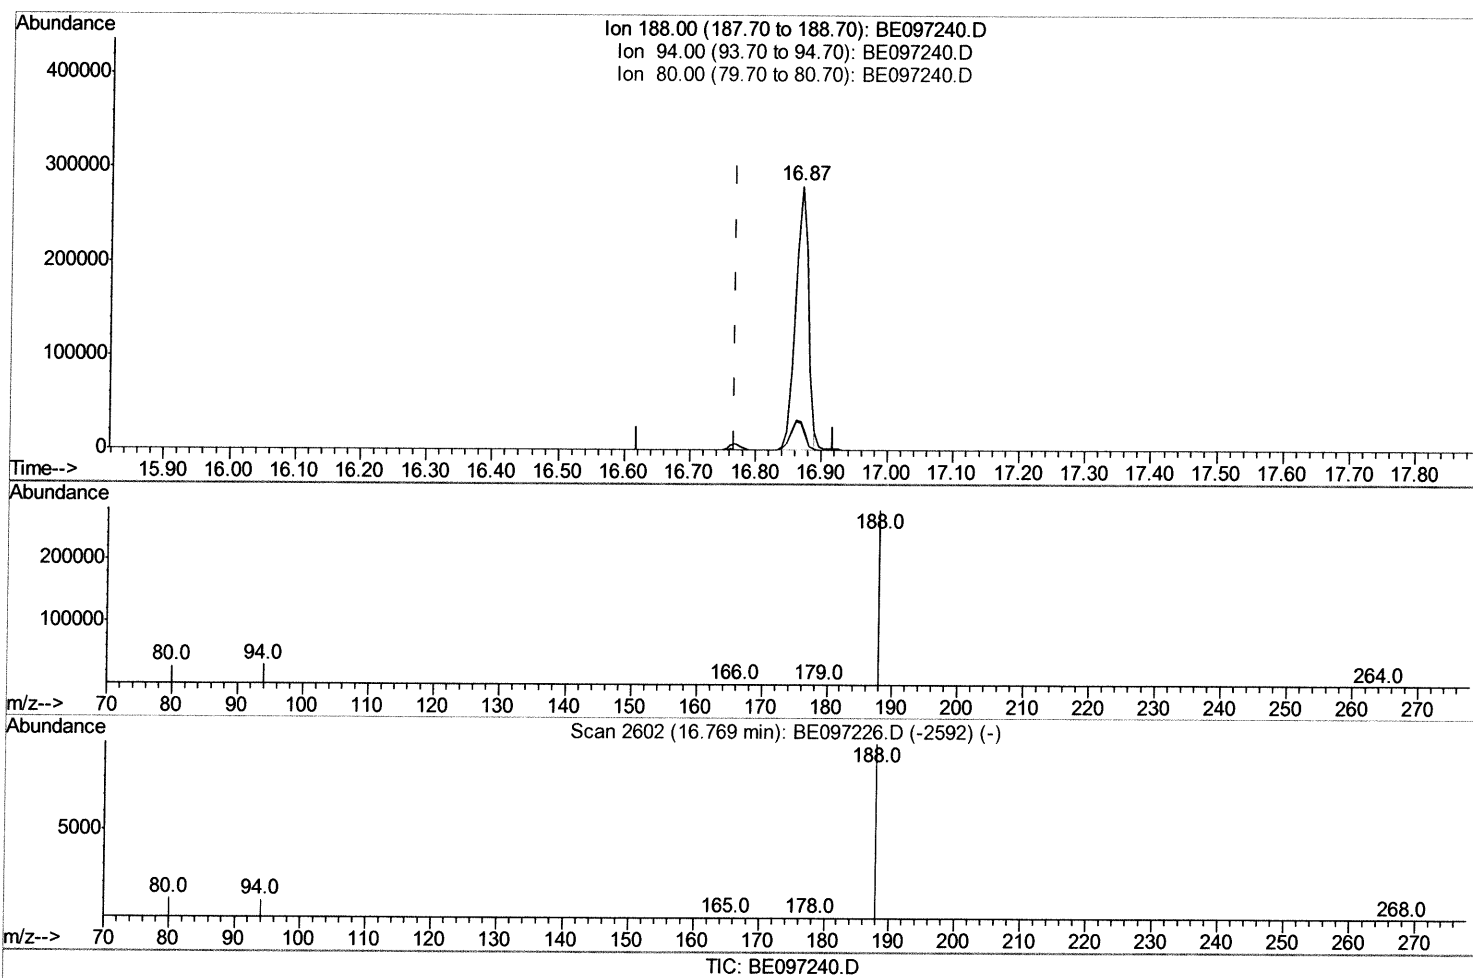

(10) Phenanthrene-d10 (I)

16.868min (+0.099) 0.40ng/ul

response 385347

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.75
80.00	11.80	9.90
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097240.D
 Acq On : 8 Aug 2018 18:13
 Operator : SJ/JU
 Sample : J4268-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:21 PM

Quant Time: Aug 08 23:27:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

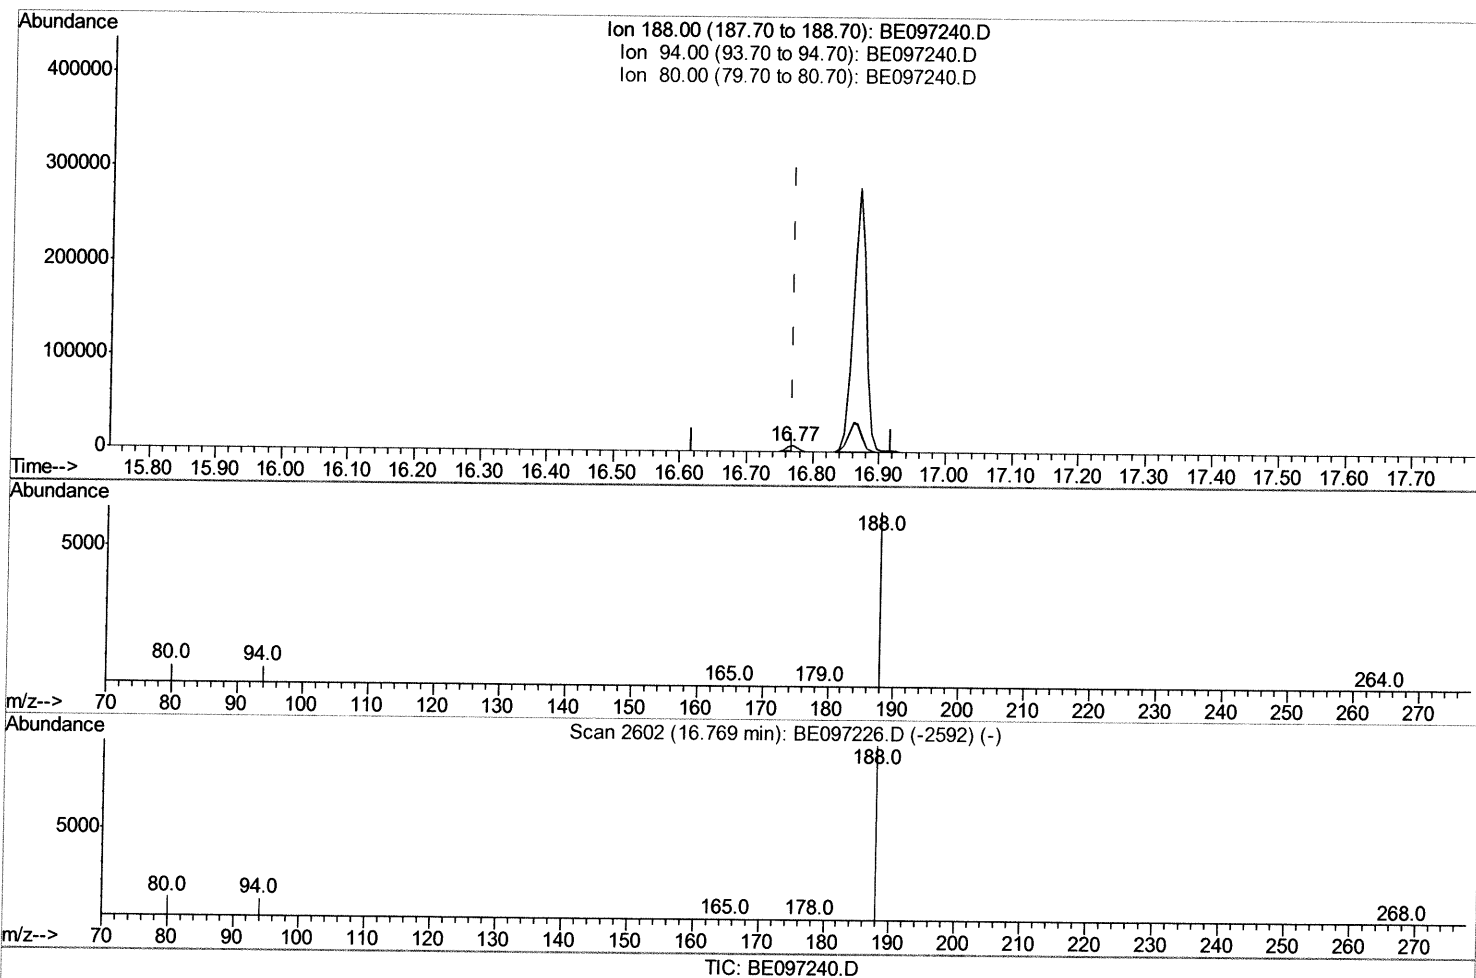

(10) Phenanthrene-d10 (I)

16.769min (+0.001) 0.40ng/ul m

response 8579

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	9.81
80.00	11.80	10.58
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097240.D
Acq On : 8 Aug 2018 18:13
Operator : SJ/JU
Sample : J4268-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:27:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

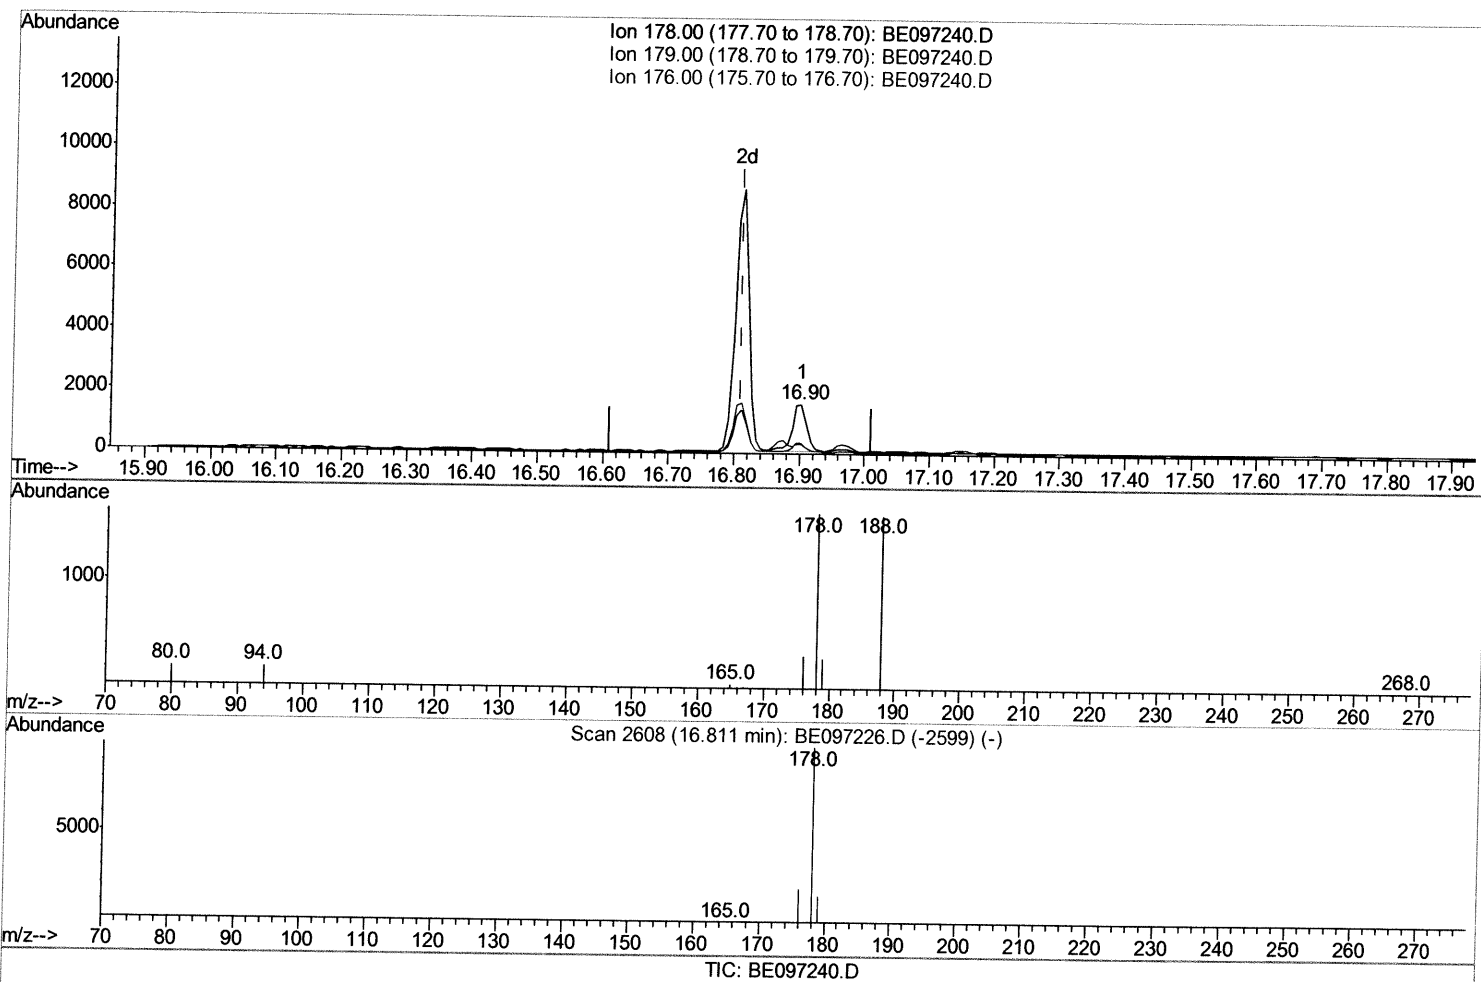

(12) Phenanthrene

16.903min (+0.092) 0.11ng/ul

response 2421

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	19.21
176.00	17.00	21.12#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097240.D
Acq On : 8 Aug 2018 18:13
Operator : SJ/JU
Sample : J4268-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:27:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

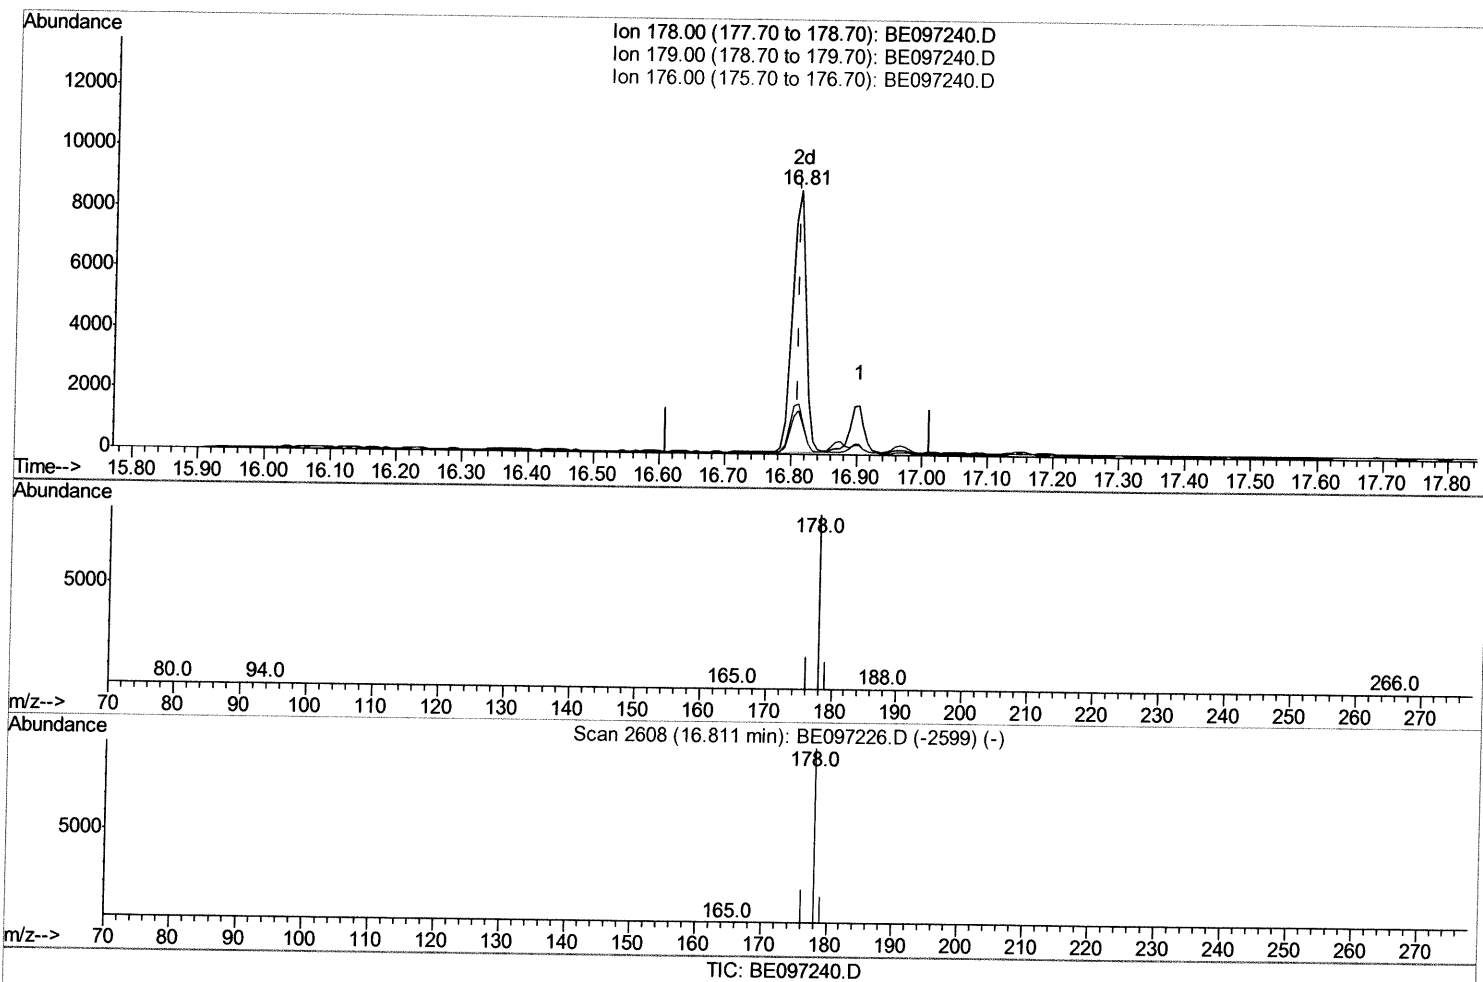

(12) Phenanthrene

16.812min (+0.001) 0.55ng/ul m

SJ 8/10/18

response 12112

Ion	Exp%	Act%
178.00	100	100
179.00	23.00	16.35#
176.00	17.00	19.22
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097240.D
Acq On : 8 Aug 2018 18:13
Operator : SJ/JU
Sample : J4268-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:27:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

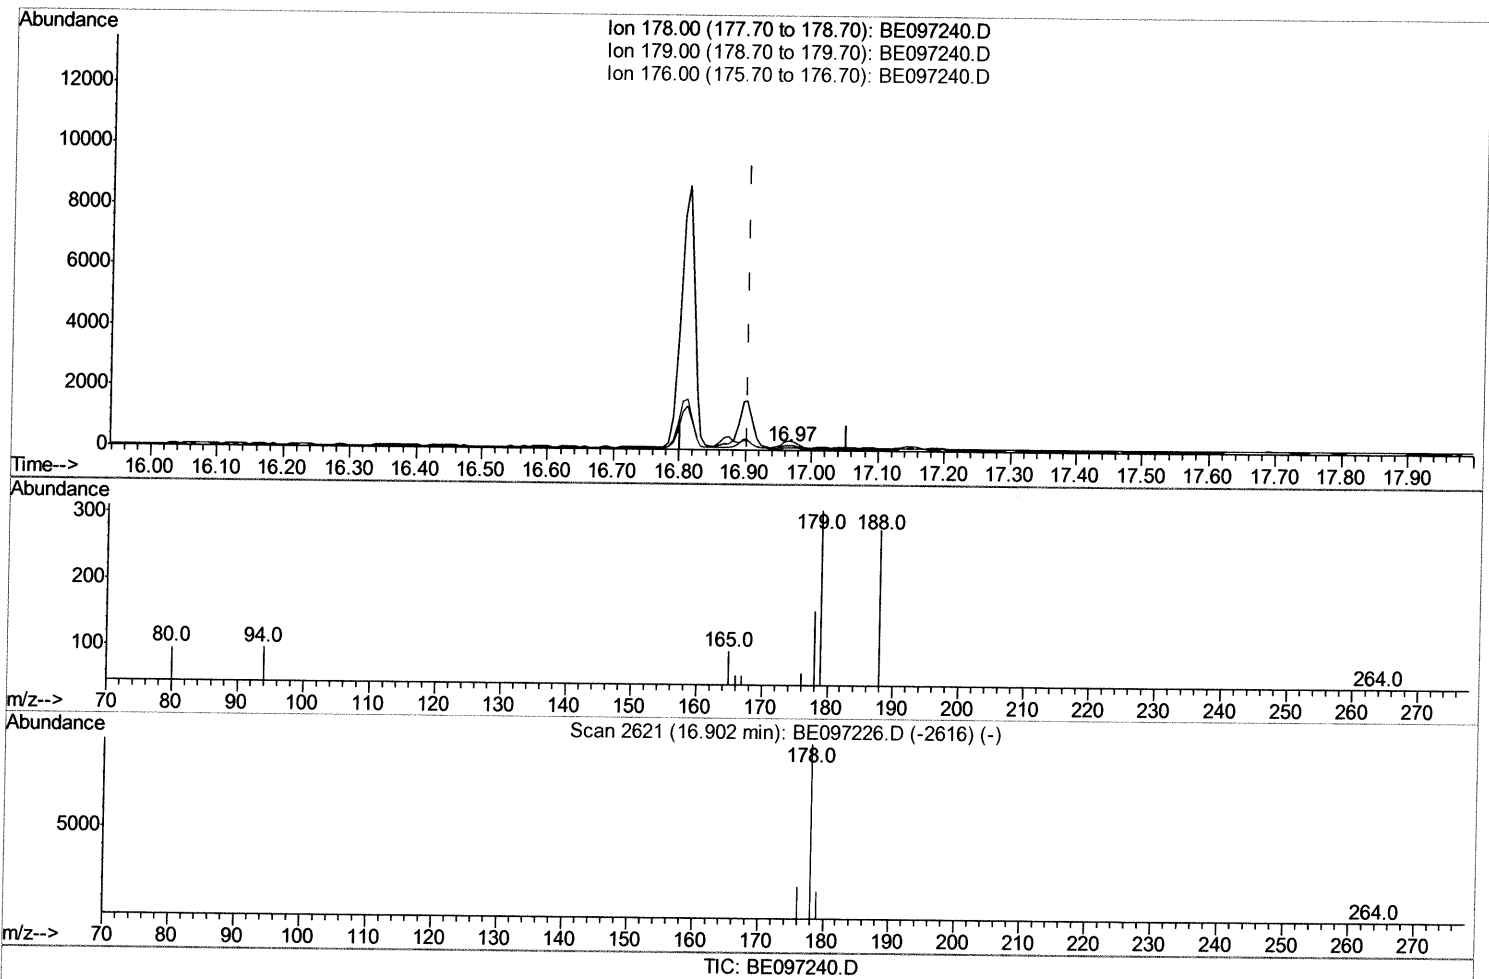

(13) Anthracene

16.966min (+0.064) 0.01ng/ul

response 130

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	195.57#
176.00	18.40	40.51#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097240.D
Acq On : 8 Aug 2018 18:13
Operator : SJ/JU
Sample : J4268-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:27:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

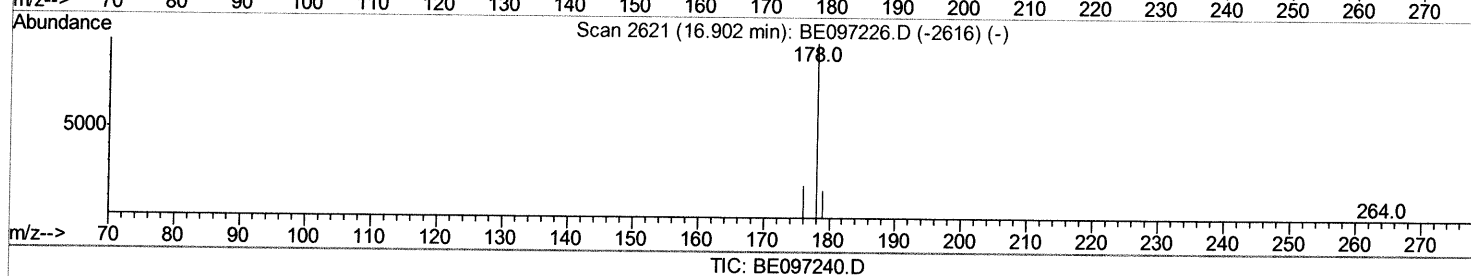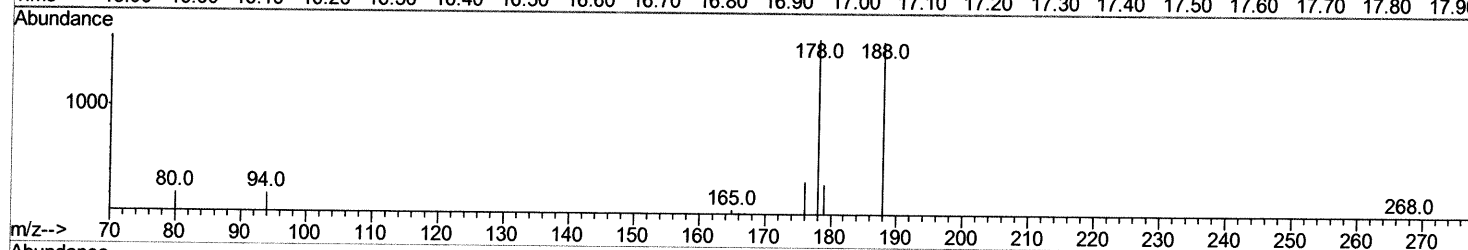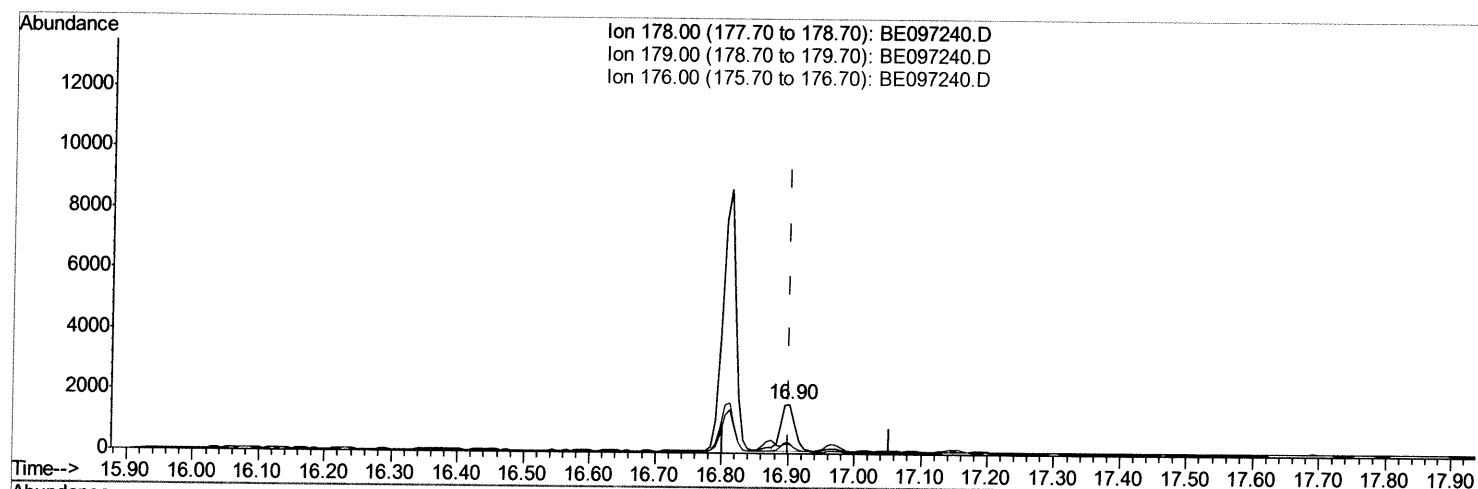

(13) Anthracene

16.903min (+0.001) 0.11ng/ul m > SJ 8/10/18

response 2239

Ion	Exp%	Act%
178.00	100	100
179.00	22.60	19.21
176.00	18.40	21.12
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097240.D
Acq On : 8 Aug 2018 18:13
Operator : SJ/JU
Sample : J4268-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:27:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

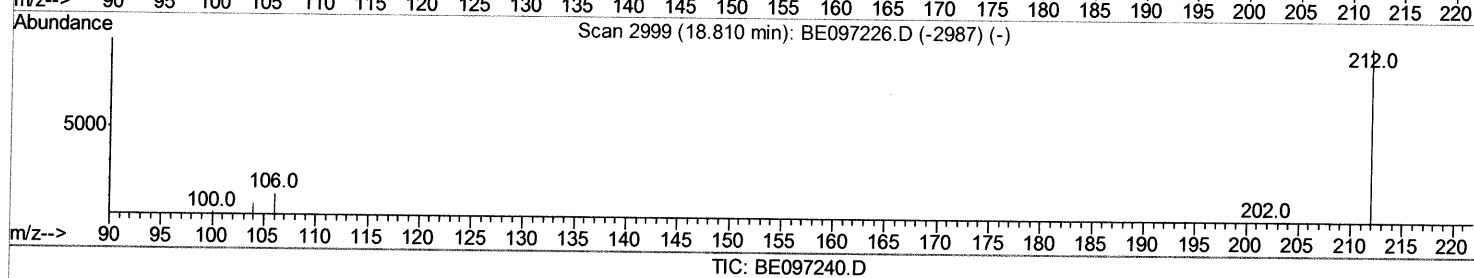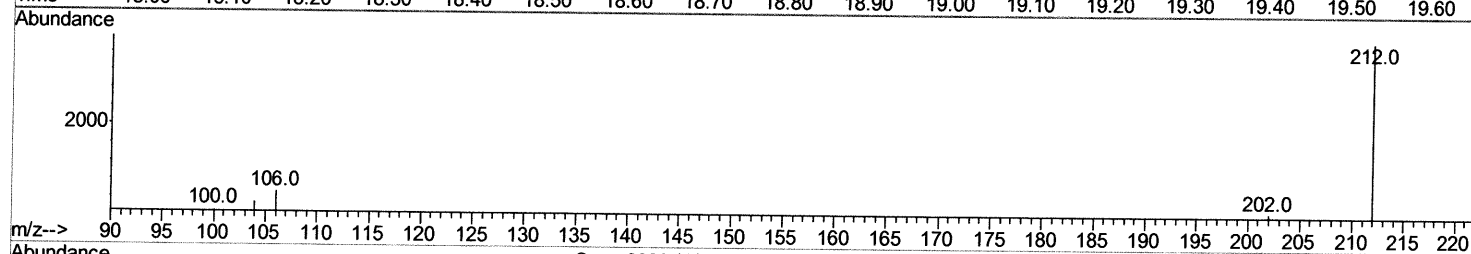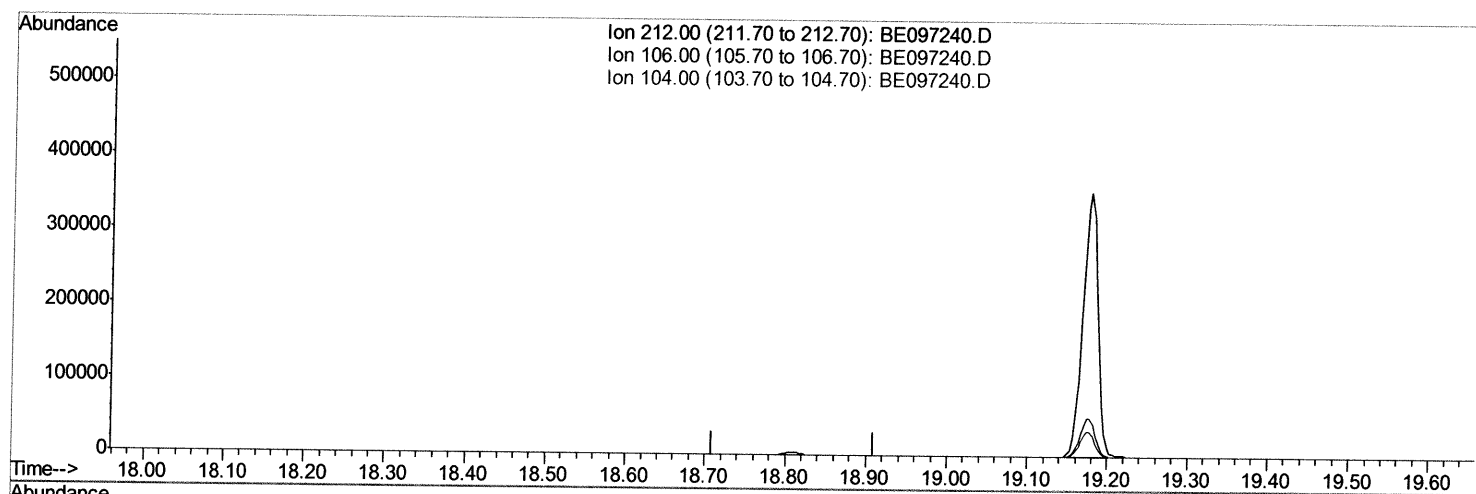

(14) Fluoranthene-d10 (SURR)

18.810min (-18.810) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097240.D
 Acq On : 8 Aug 2018 18:13
 Operator : SJ/JU
 Sample : J4268-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AA6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:27:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

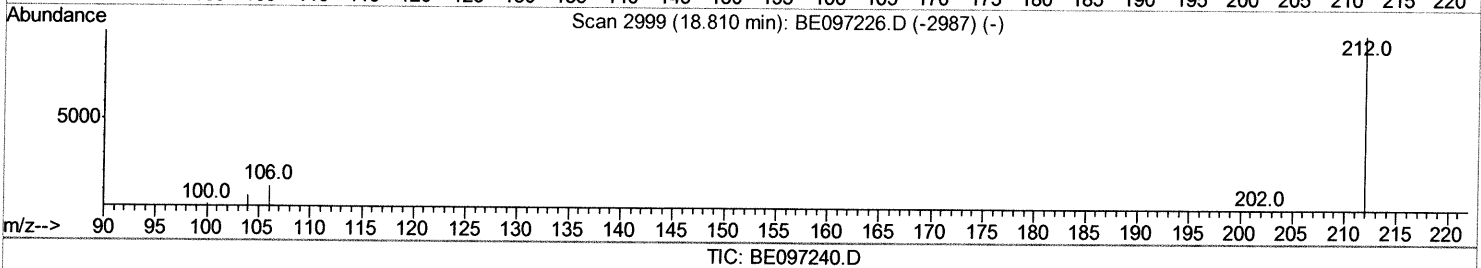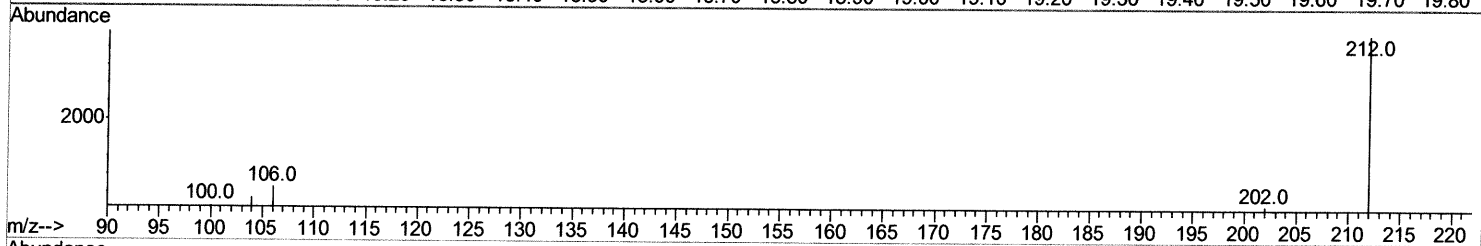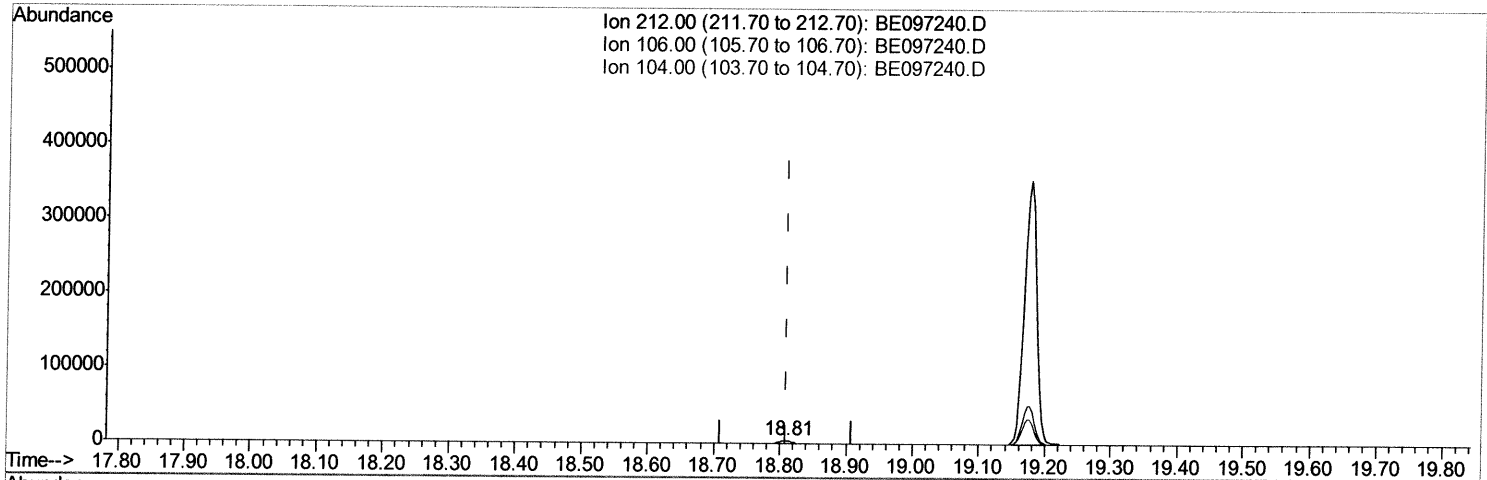

(14) Fluoranthene-d10 (SURR)

18.810min (+0.000) 0.18ng/ul m

response 5430

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097240.D
 Acq On : 8 Aug 2018 18:13
 Operator : SJ/JU
 Sample : J4268-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:27:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

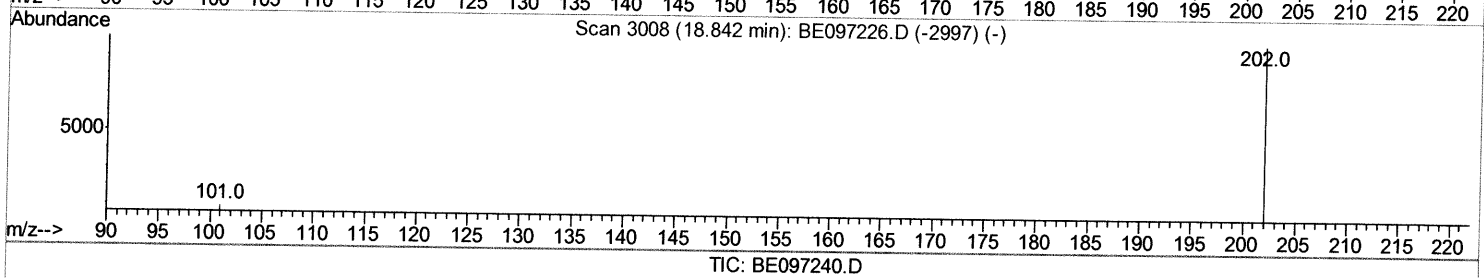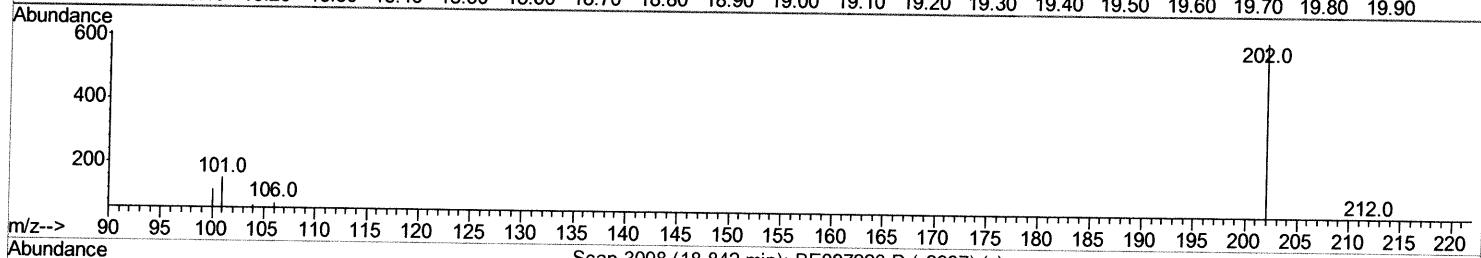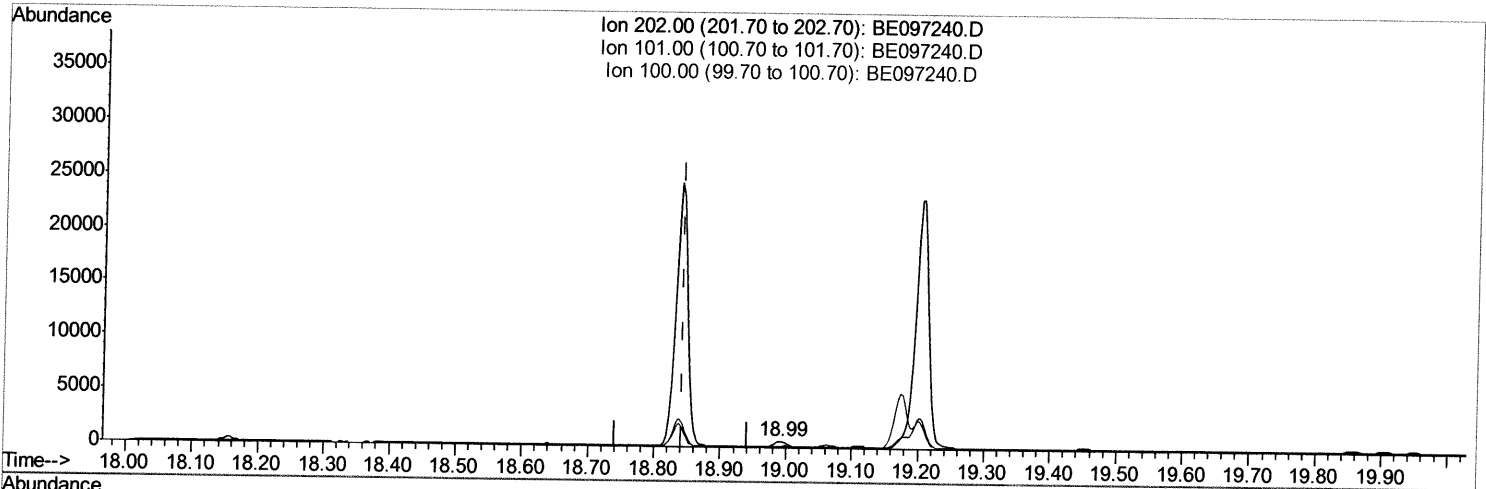

(15) Fluoranthene (C)

18.992min (+0.150) 0.02ng/ul

response 641

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	25.08
100.00	19.50	19.14
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097240.D
 Acq On : 8 Aug 2018 18:13
 Operator : SJ/JU
 Sample : J4268-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:27:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

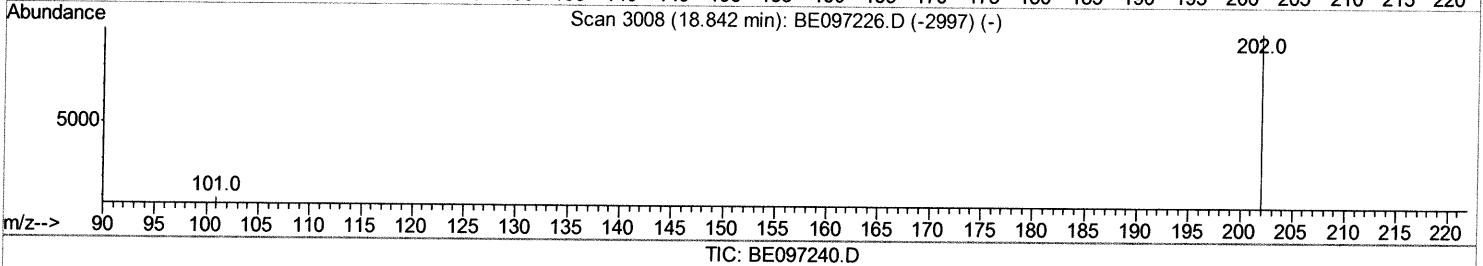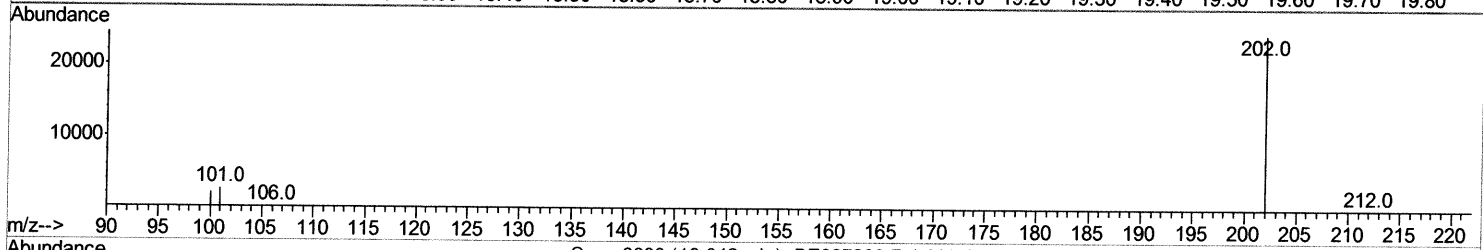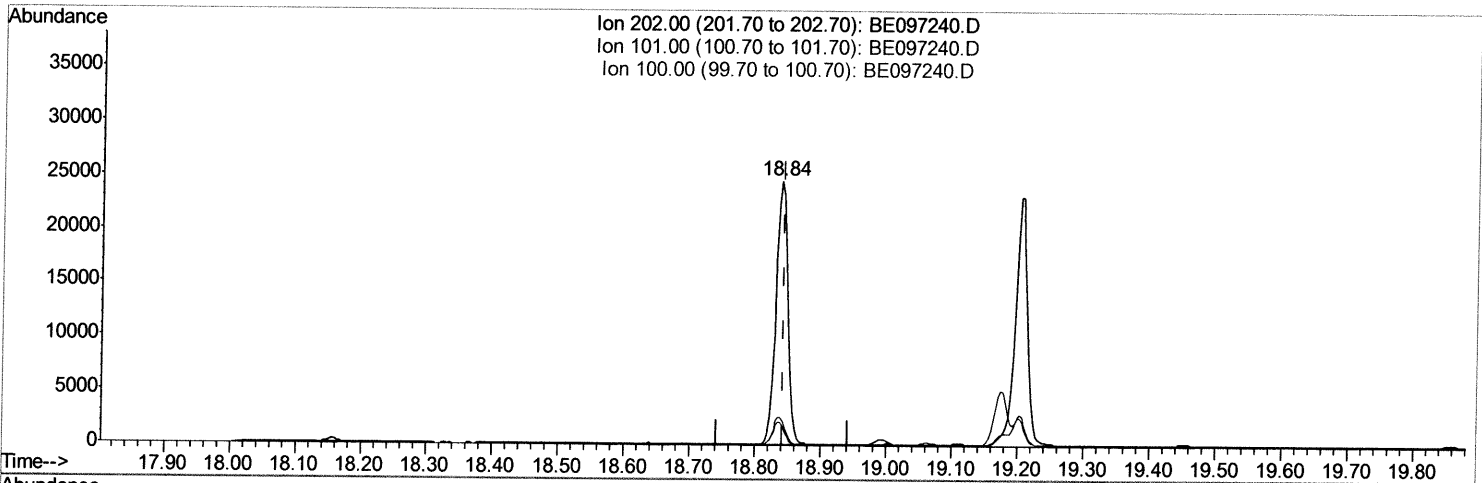

(15) Fluoranthene (C)

18.839min (-0.003) 1.10ng/ul m > SJ 8/10/18

response 31772

Ion	Exp%	Act%
202.00	100	100
101.00	10.30	10.61
100.00	19.50	8.57
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097240.D
Acq On : 8 Aug 2018 18:13
Operator : SJ/JU
Sample : J4268-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AA6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:27:18 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

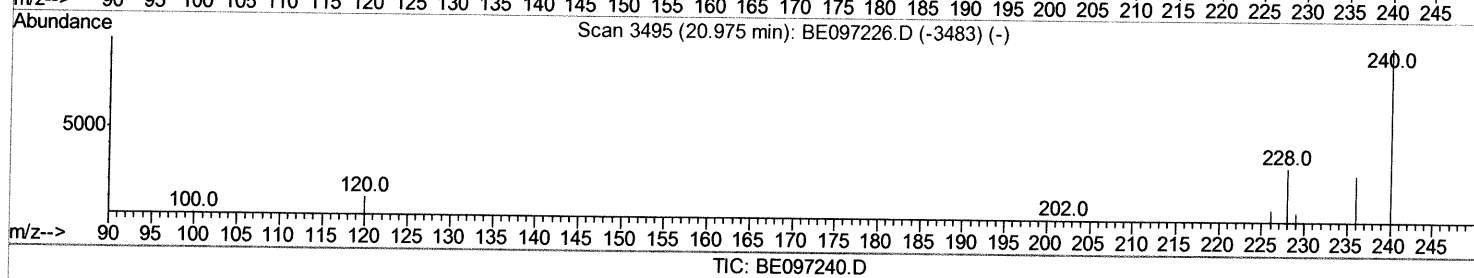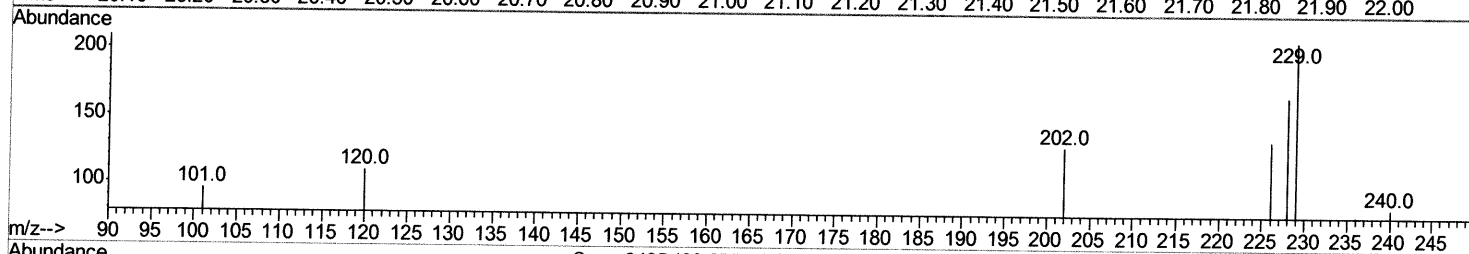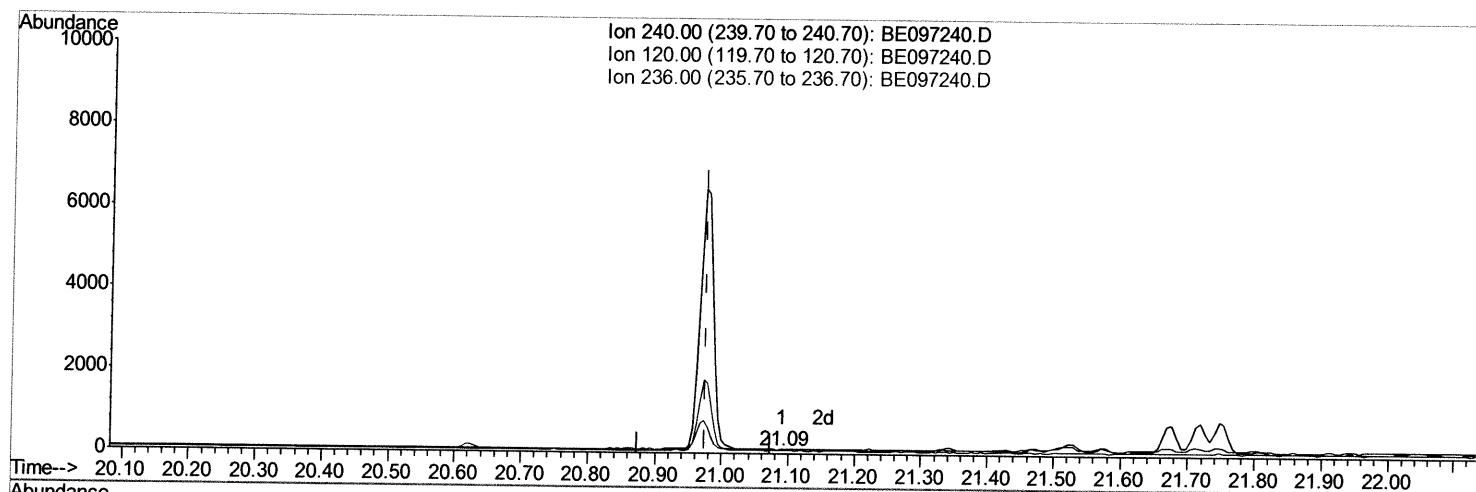

(16) Chrysene-d12 (I)

21.090min (+0.115) 0.40ng/ul

response 14

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	129.76#
236.00	34.90	94.05#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097240.D
 Acq On : 8 Aug 2018 18:13
 Operator : SJ/JU
 Sample : J4268-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AA6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:27:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

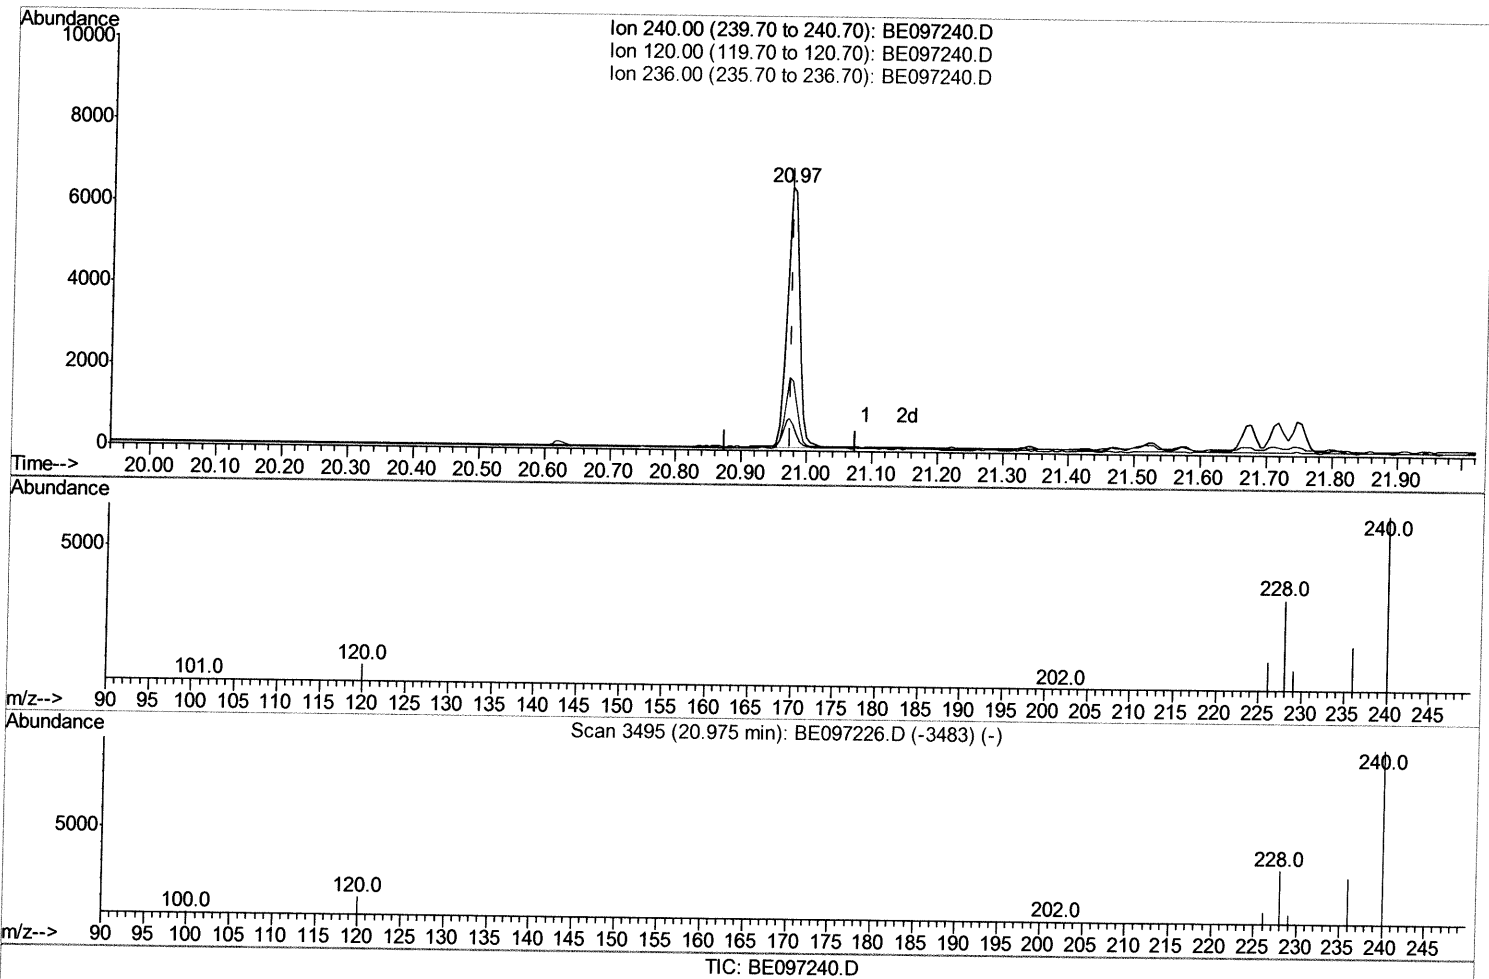

(16) Chrysene-d12 (I)

20.973min (-0.002) 0.40ng/ul m> SJ 8/10/18

response 8752

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	12.34#
236.00	34.90	27.79#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097240.D
 Acq On : 8 Aug 2018 18:13
 Operator : SJ/JU
 Sample : J4268-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:29:39 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

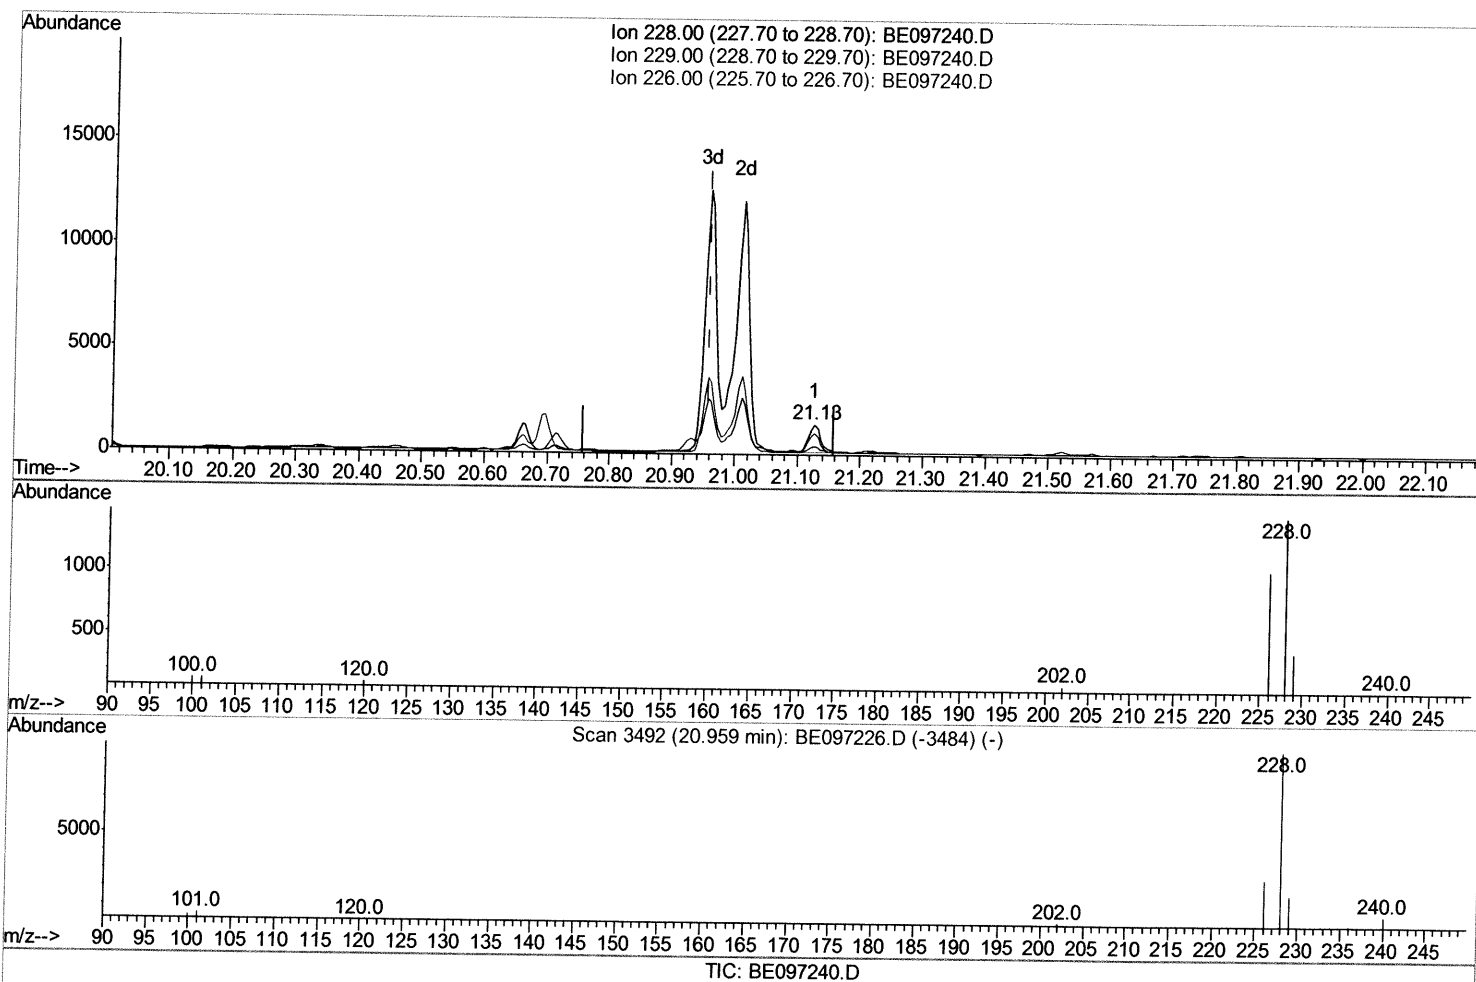

(18) Benzo(a)anthracene
 21.127min (+0.168) 0.07ng/ul
 response 1833

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	26.27
226.00	21.30	70.67#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097240.D
 Acq On : 8 Aug 2018 18:13
 Operator : SJ/JU
 Sample : J4268-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:29:39 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

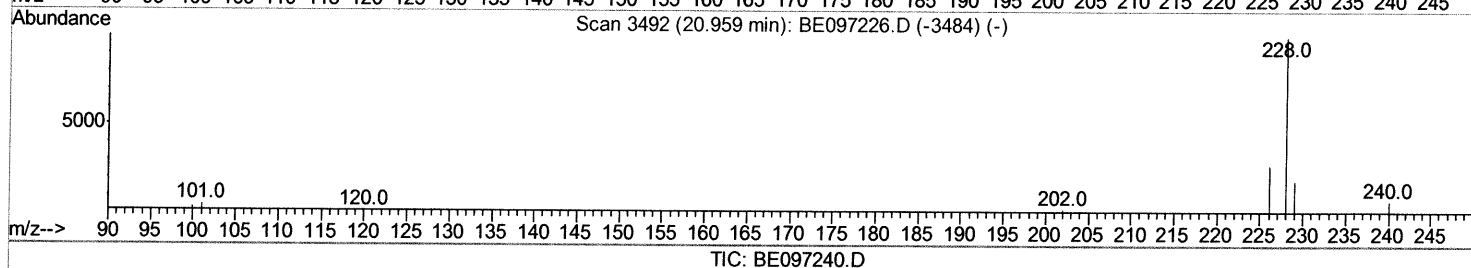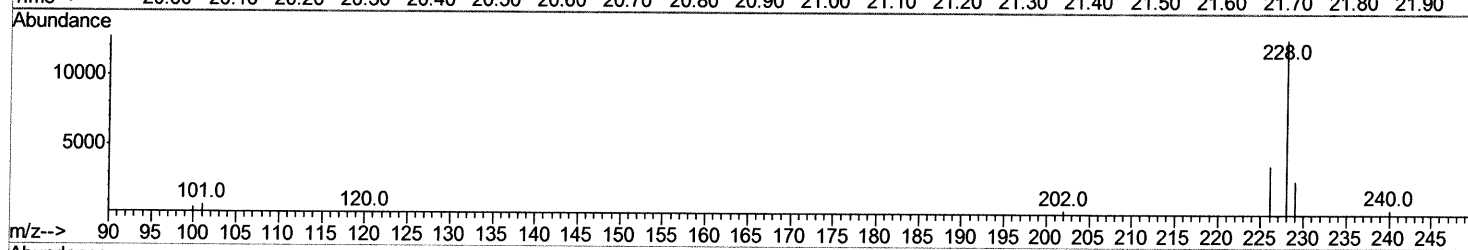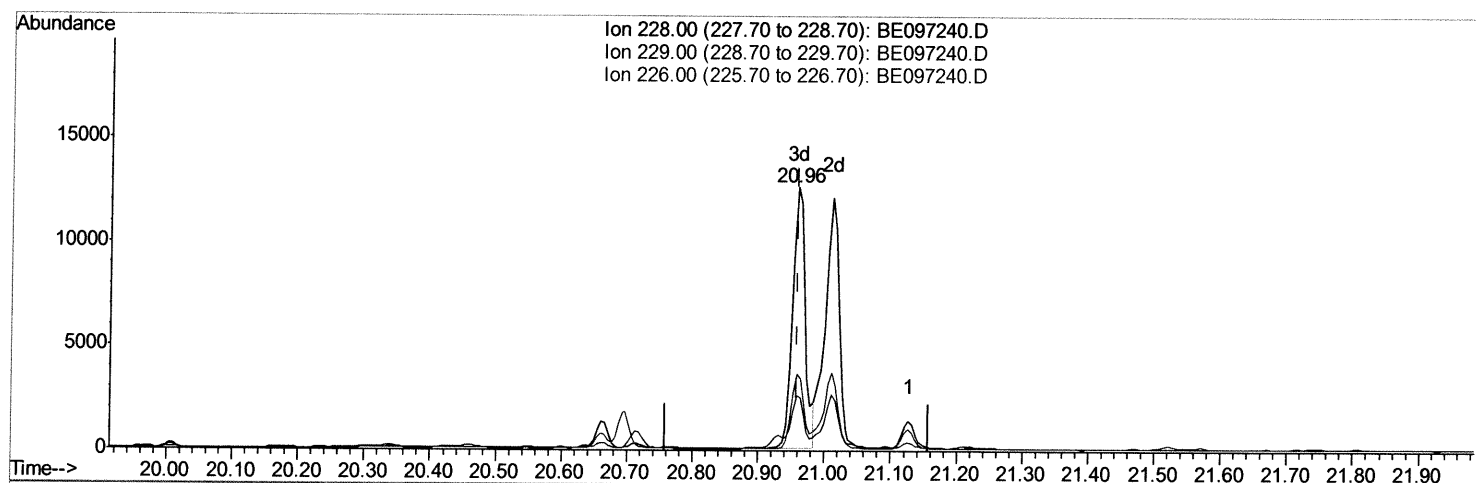

(18) Benzo(a)anthracene

20.957min (-0.002) 0.68ng/ul m) 52 8/10/18

response 17002

Ion	Exp%	Act%
228.00	100	100
229.00	28.50	20.98#
226.00	21.30	29.13#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097240.D
 Acq On : 8 Aug 2018 18:13
 Operator : SJ/JU
 Sample : J4268-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AA6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:29:39 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

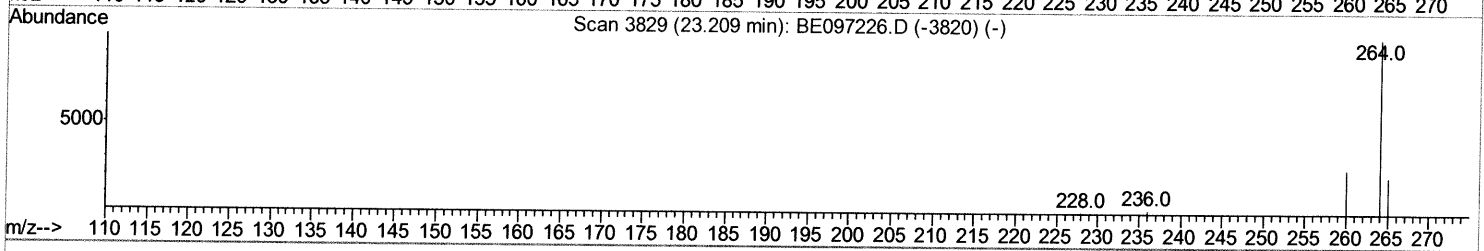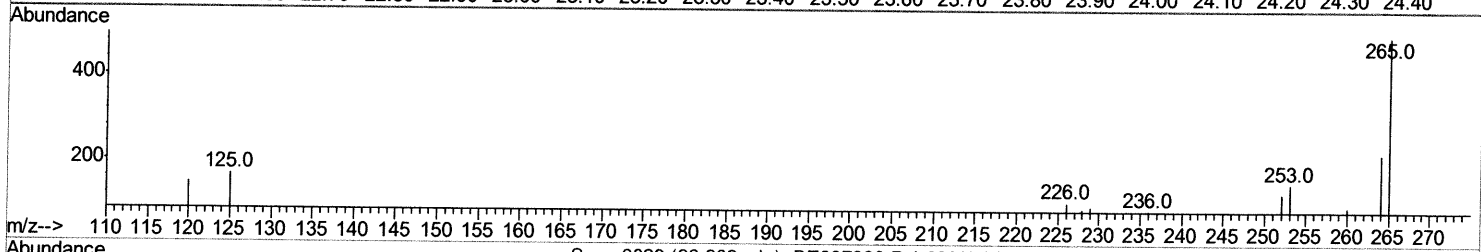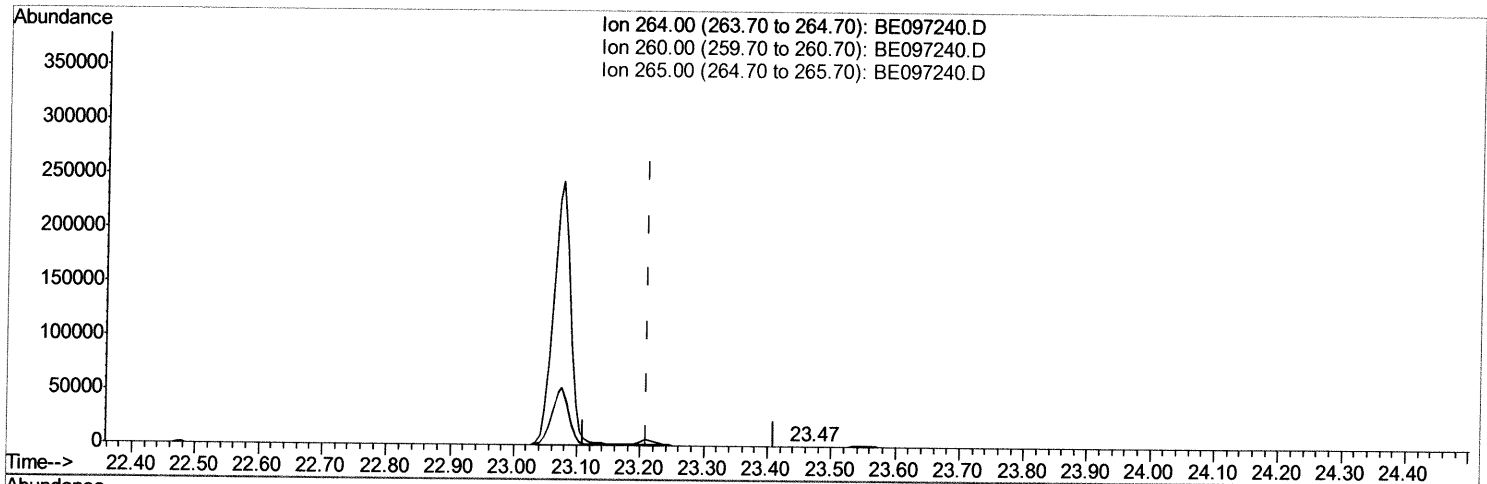

(20) Perylene-d12 (I)
 23.470min (+0.260) 0.40ng/ul
 response 56

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	43.18#
265.00	103.50	225.91#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097240.D
 Acq On : 8 Aug 2018 18:13
 Operator : SJ/JU
 Sample : J4268-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:29:39 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

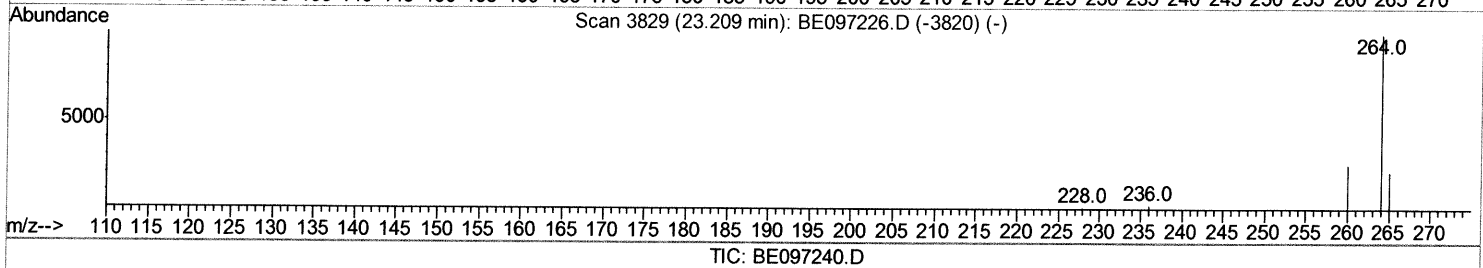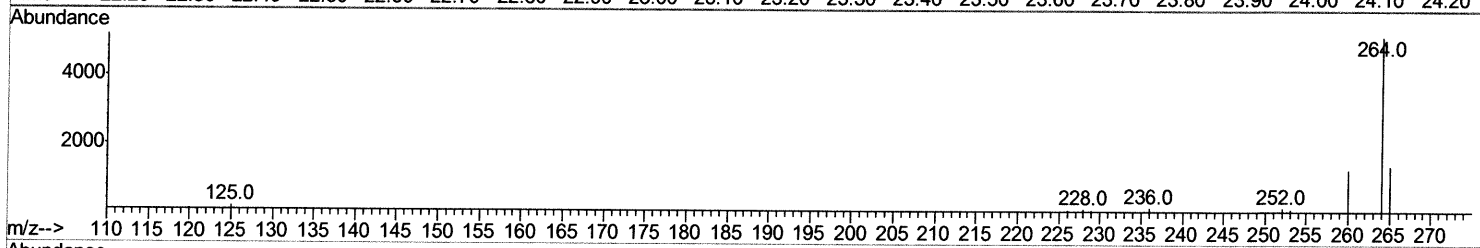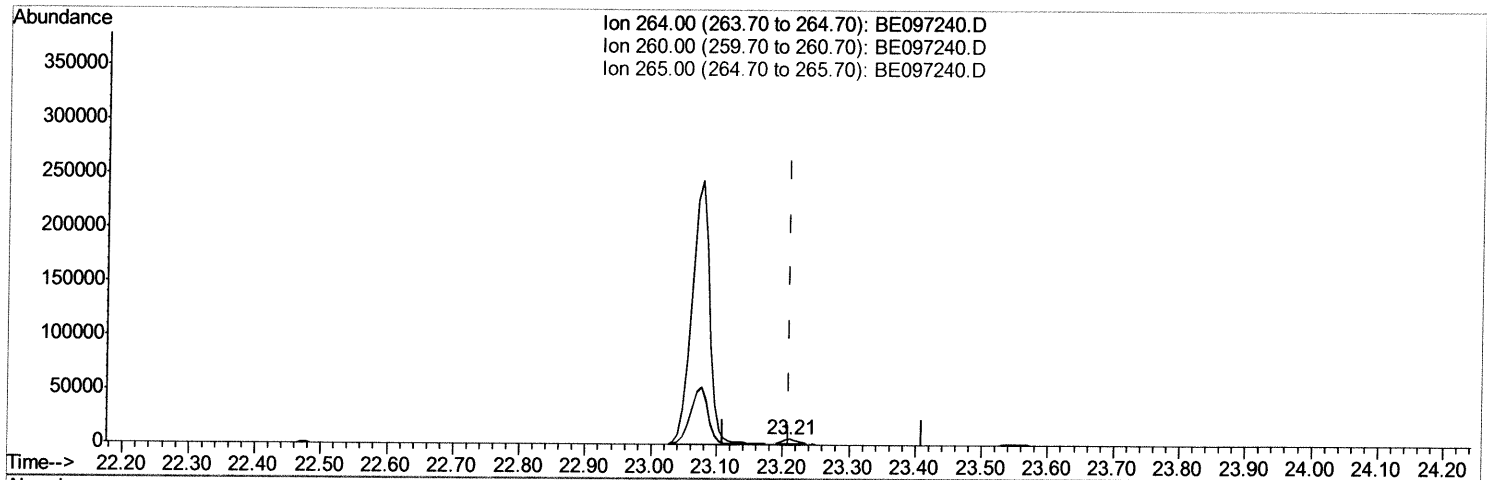

(20) Perylene-d12 (I)

23.209min (+0.000) 0.40ng/ul m> SJ 8/10/18

response 7996

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	25.29
265.00	103.50	27.25#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097240.D
Acq On : 8 Aug 2018 18:13
Operator : SJ/JU
Sample : J4268-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AA6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:31:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

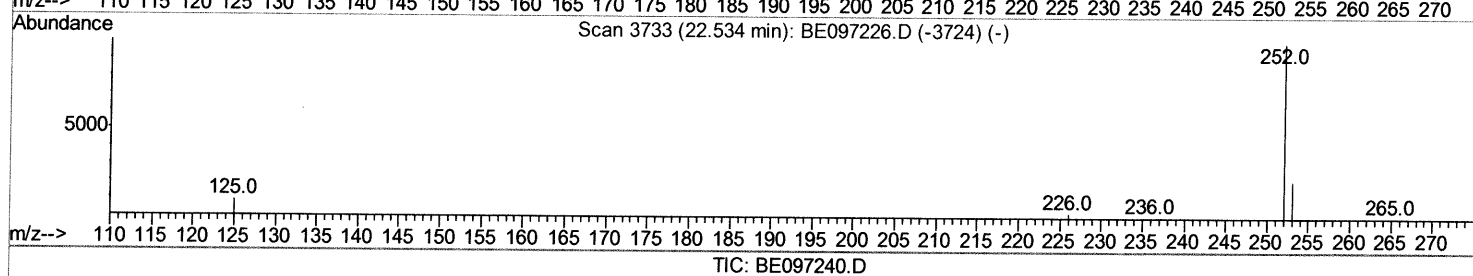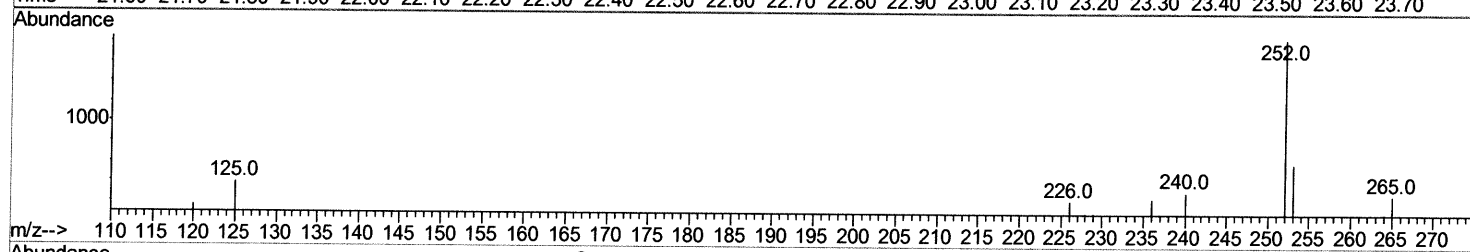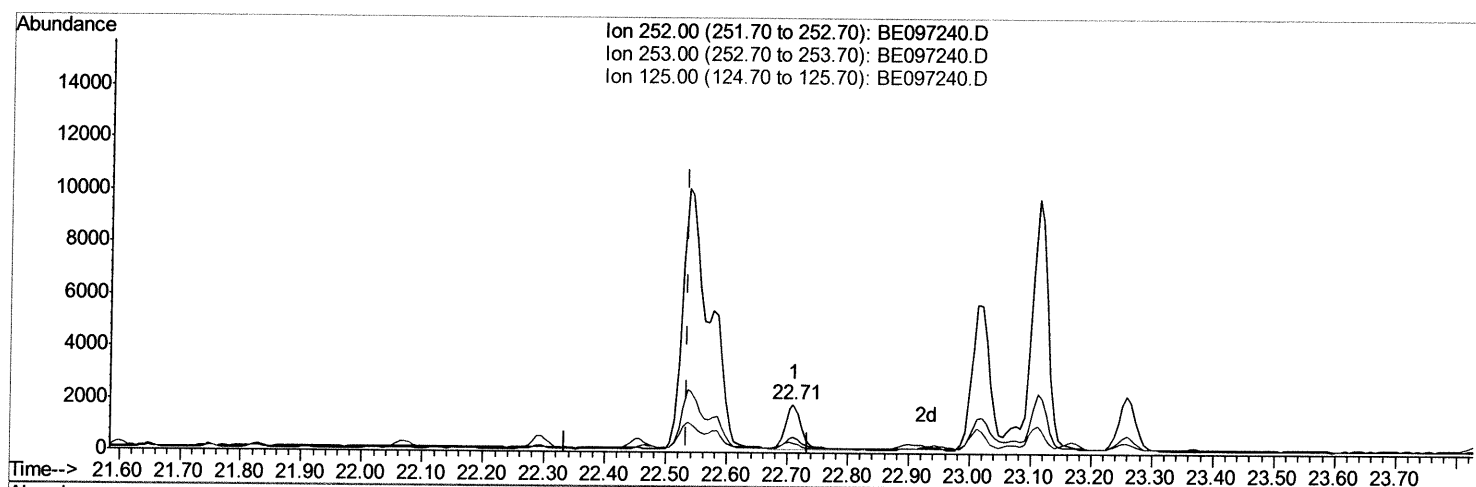

(21) Benzo(b)fluoranthene

22.710min (+0.176) 0.15ng/ul

response 3247

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	32.00
125.00	17.50	21.06
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097240.D
Acq On : 8 Aug 2018 18:13
Operator : SJ/JU
Sample : J4268-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:31:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

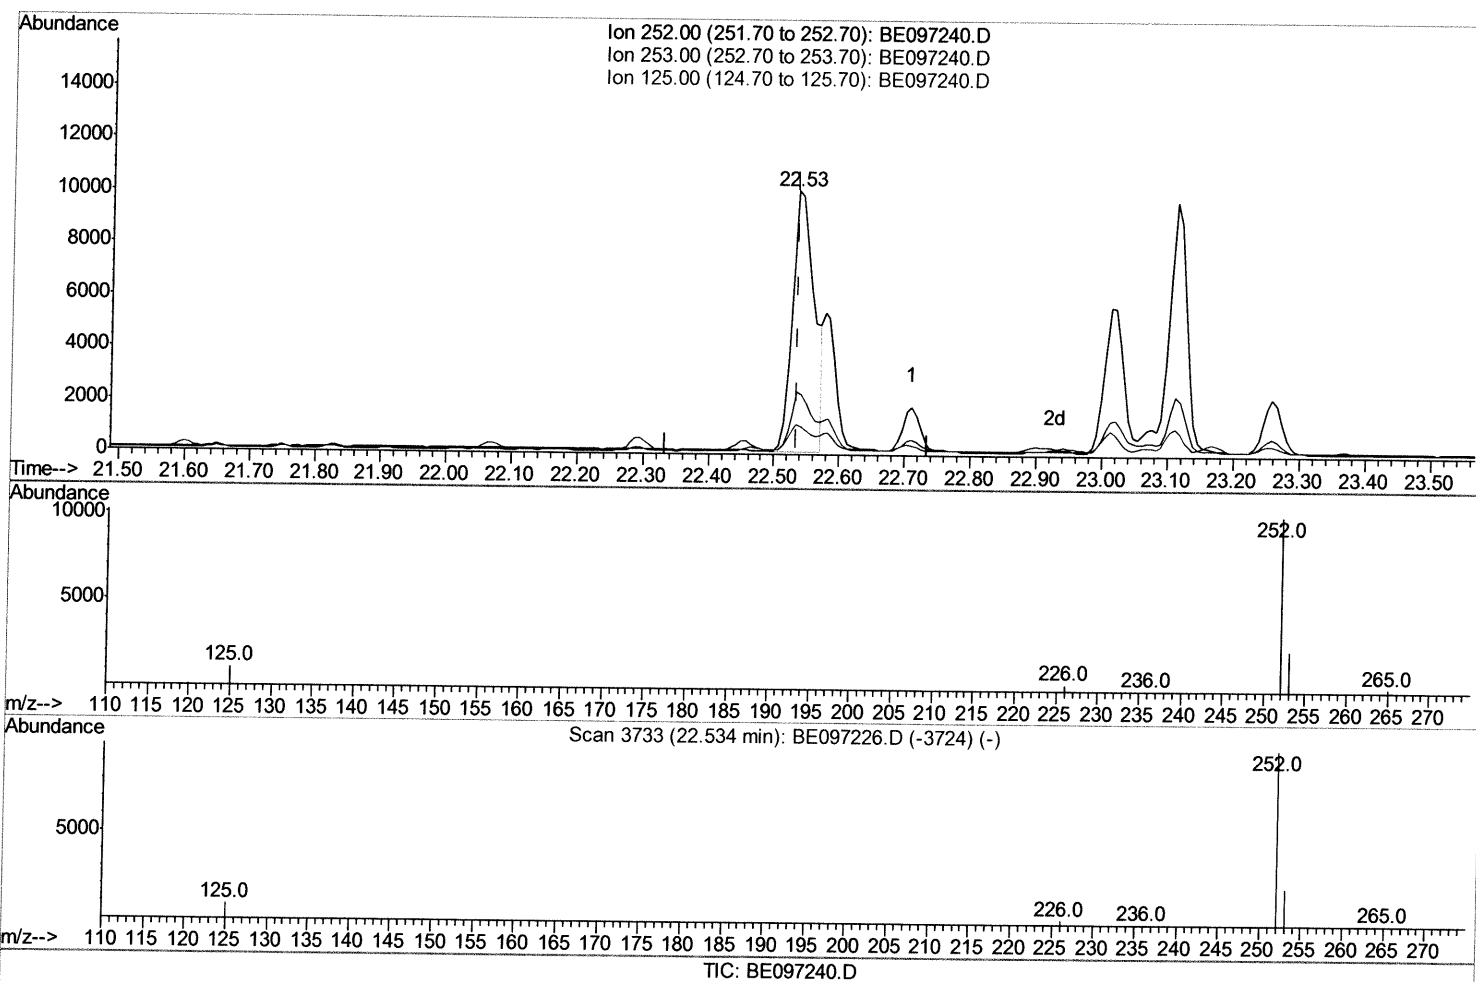

(21) Benzo(b)fluoranthene

22.534min (+0.000) 1.08ng/ul m> SJ 8/10/18

response 23462

Ion	Exp%	Act%
252.00	100	100
253.00	32.10	23.65
125.00	17.50	11.19
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097240.D
 Acq On : 8 Aug 2018 18:13
 Operator : SJ/JU
 Sample : J4268-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AA6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:31:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

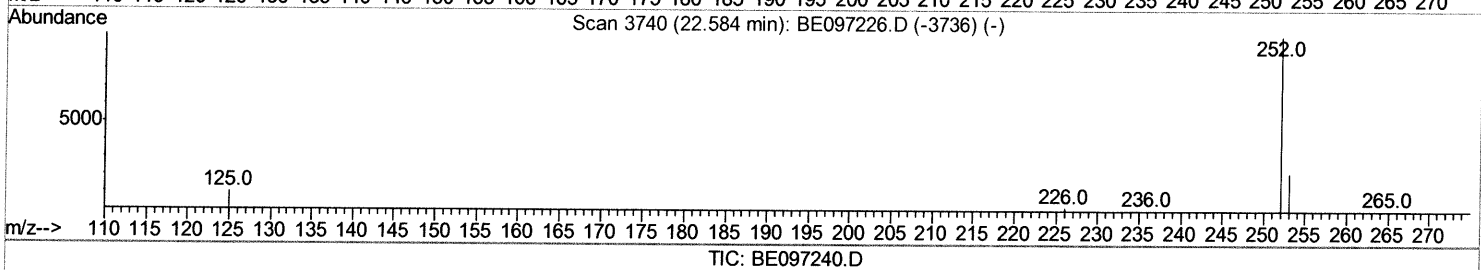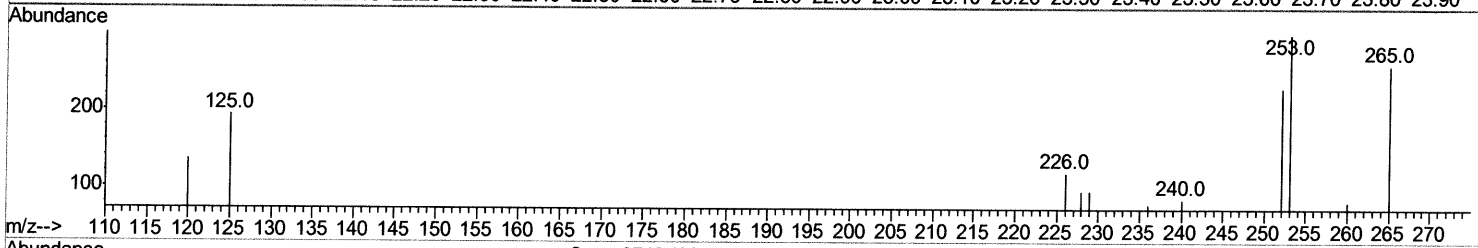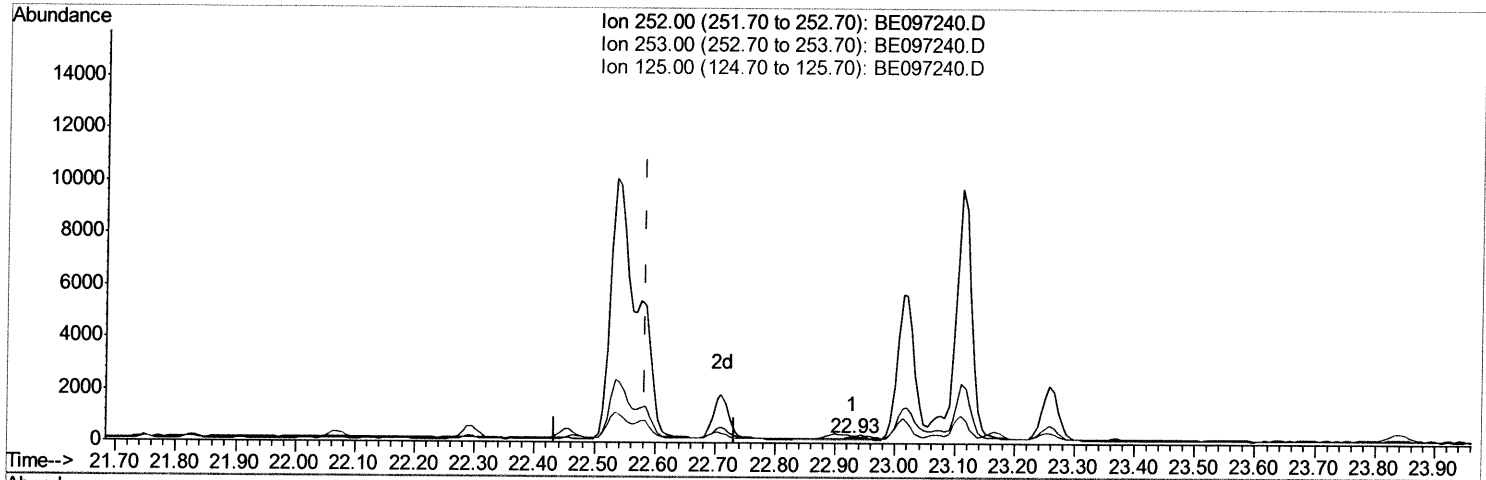

(22) Benzo(k)fluoranthene
 22.928min (+0.345) 0.02ng/ul
 response 378

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	130.57#
125.00	17.10	84.28#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097240.D
Acq On : 8 Aug 2018 18:13
Operator : SJ/JU
Sample : J4268-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:31:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

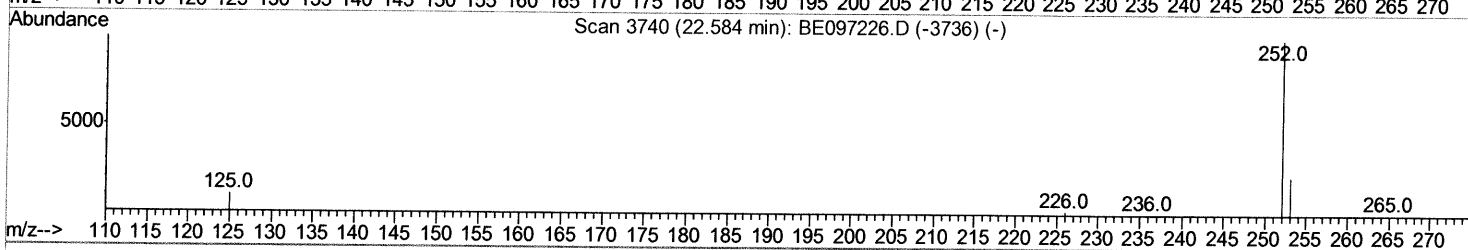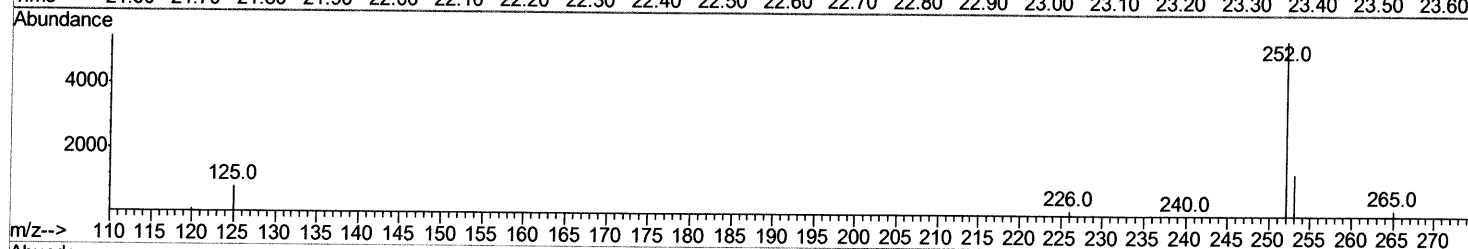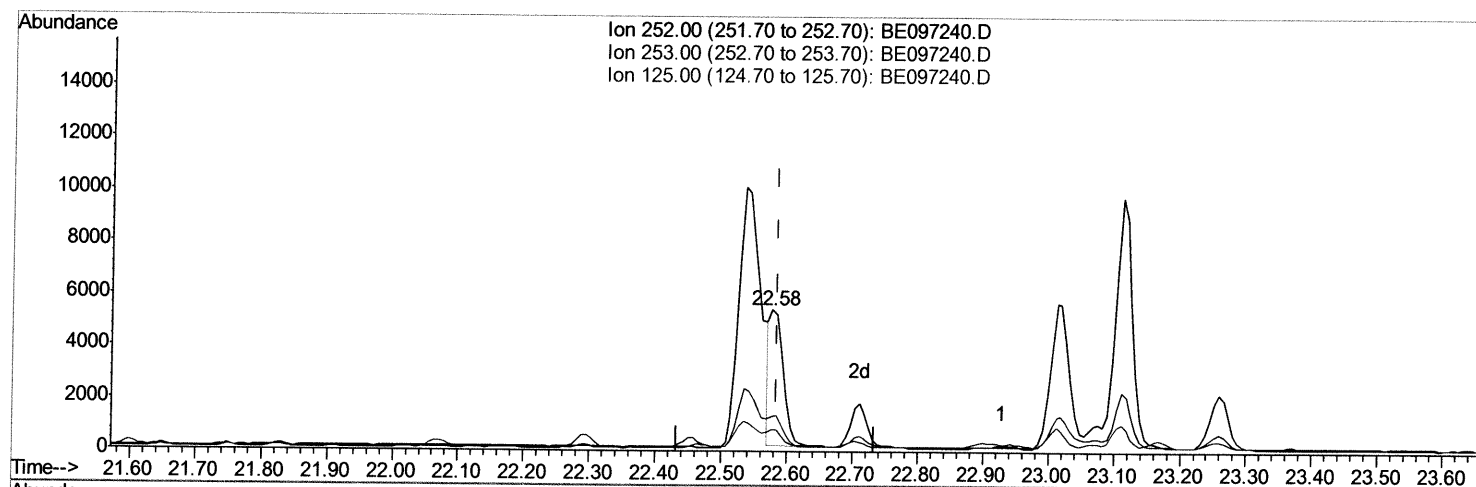

TIC: BE097240.D

(22) Benzo(k)fluoranthene

22.577min (-0.007) 0.30ng/ul m > SJ 8/10/18

response 7005

Ion	Exp%	Act%
252.00	100	100
253.00	30.60	25.02
125.00	17.10	15.65
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097240.D
Acq On : 8 Aug 2018 18:13
Operator : SJ/JU
Sample : J4268-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AA6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:31:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

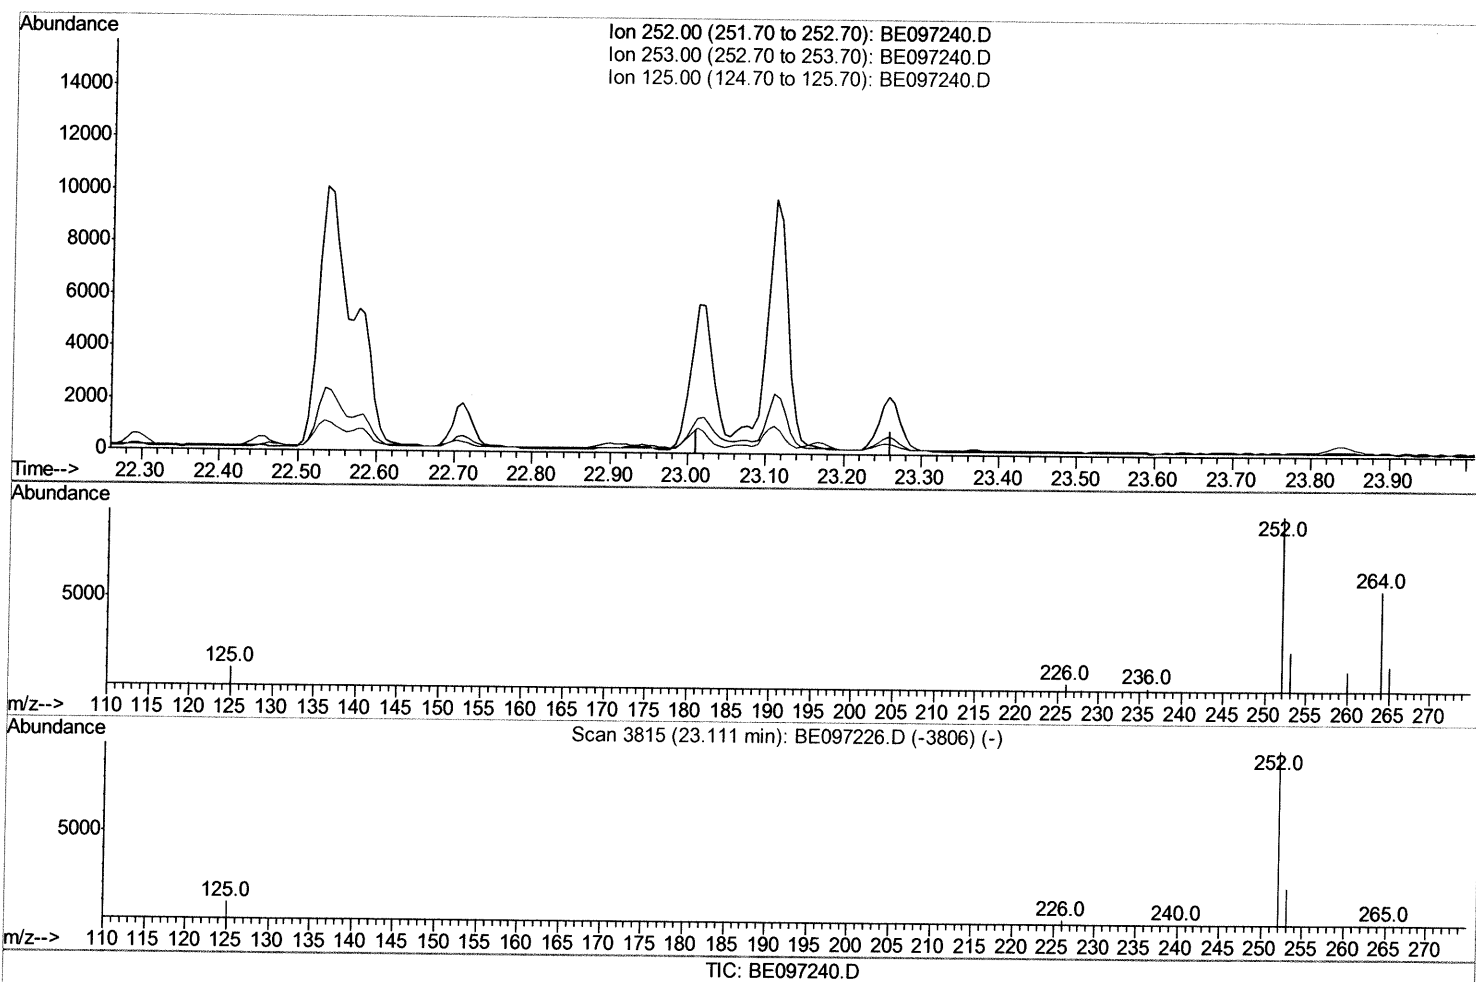

(23) Benzo(a)pyrene (C)

23.111min (-23.111) 0.00ng/ul

response 0

Ion	Exp%	Act%
252.00	100	0.00
253.00	35.60	0.00#
125.00	22.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097240.D
 Acq On : 8 Aug 2018 18:13
 Operator : SJ/JU
 Sample : J4268-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:31:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

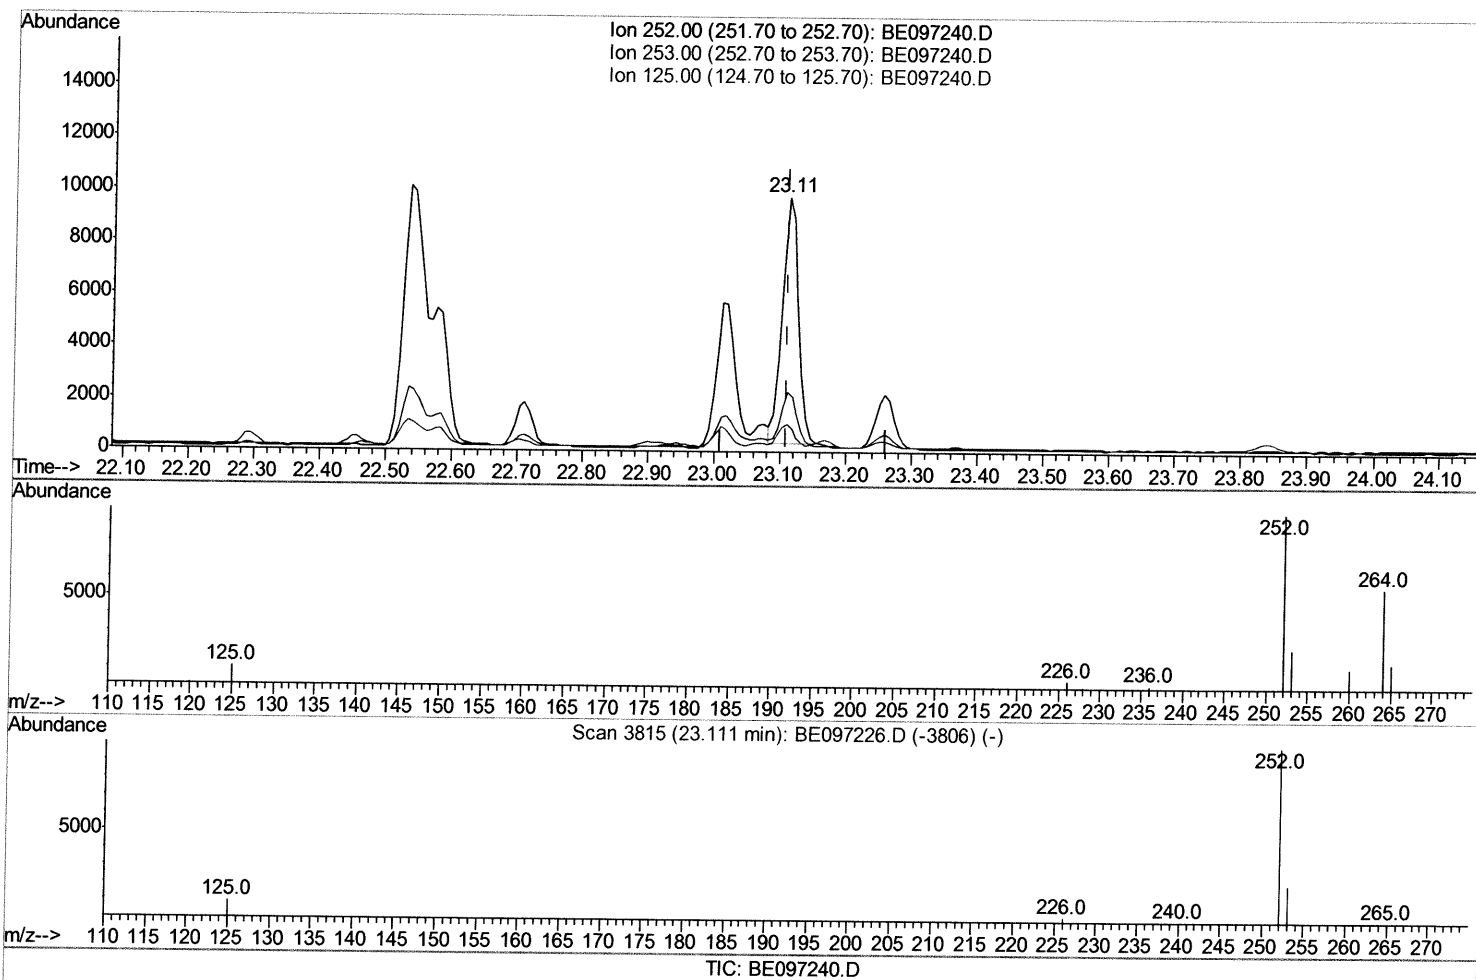

(23) Benzo(a)pyrene (C)

23.111min (+0.000) 0.75ng/ul m> SJ 8/10/18

response 16265

Ion	Exp%	Act%
252.00	100	100
253.00	35.60	23.49#
125.00	22.60	11.01#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097240.D
Acq On : 8 Aug 2018 18:13
Operator : SJ/JU
Sample : J4268-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:31:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

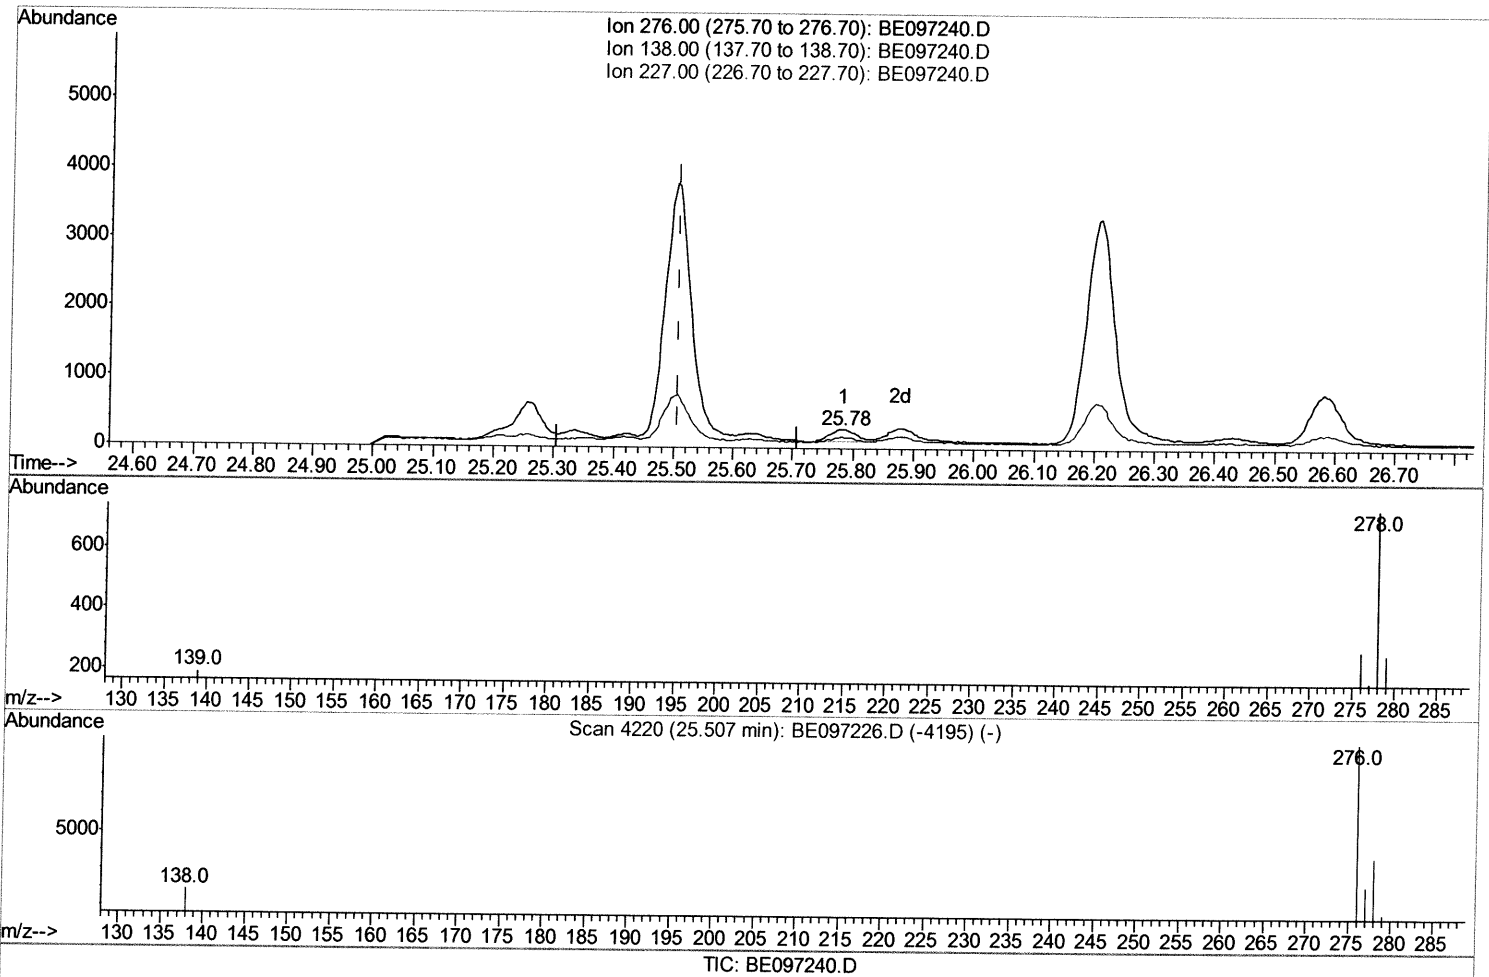

(24) Indeno(1,2,3-cd)pyrene

25.784min (+0.277) 0.02ng/ul

response 514

Ion	Exp%	Act%
276.00	100	100
138.00	35.00	42.02#
227.00	10.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097240.D
Acq On : 8 Aug 2018 18:13
Operator : SJ/JU
Sample : J4268-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
C0AA6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:31:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

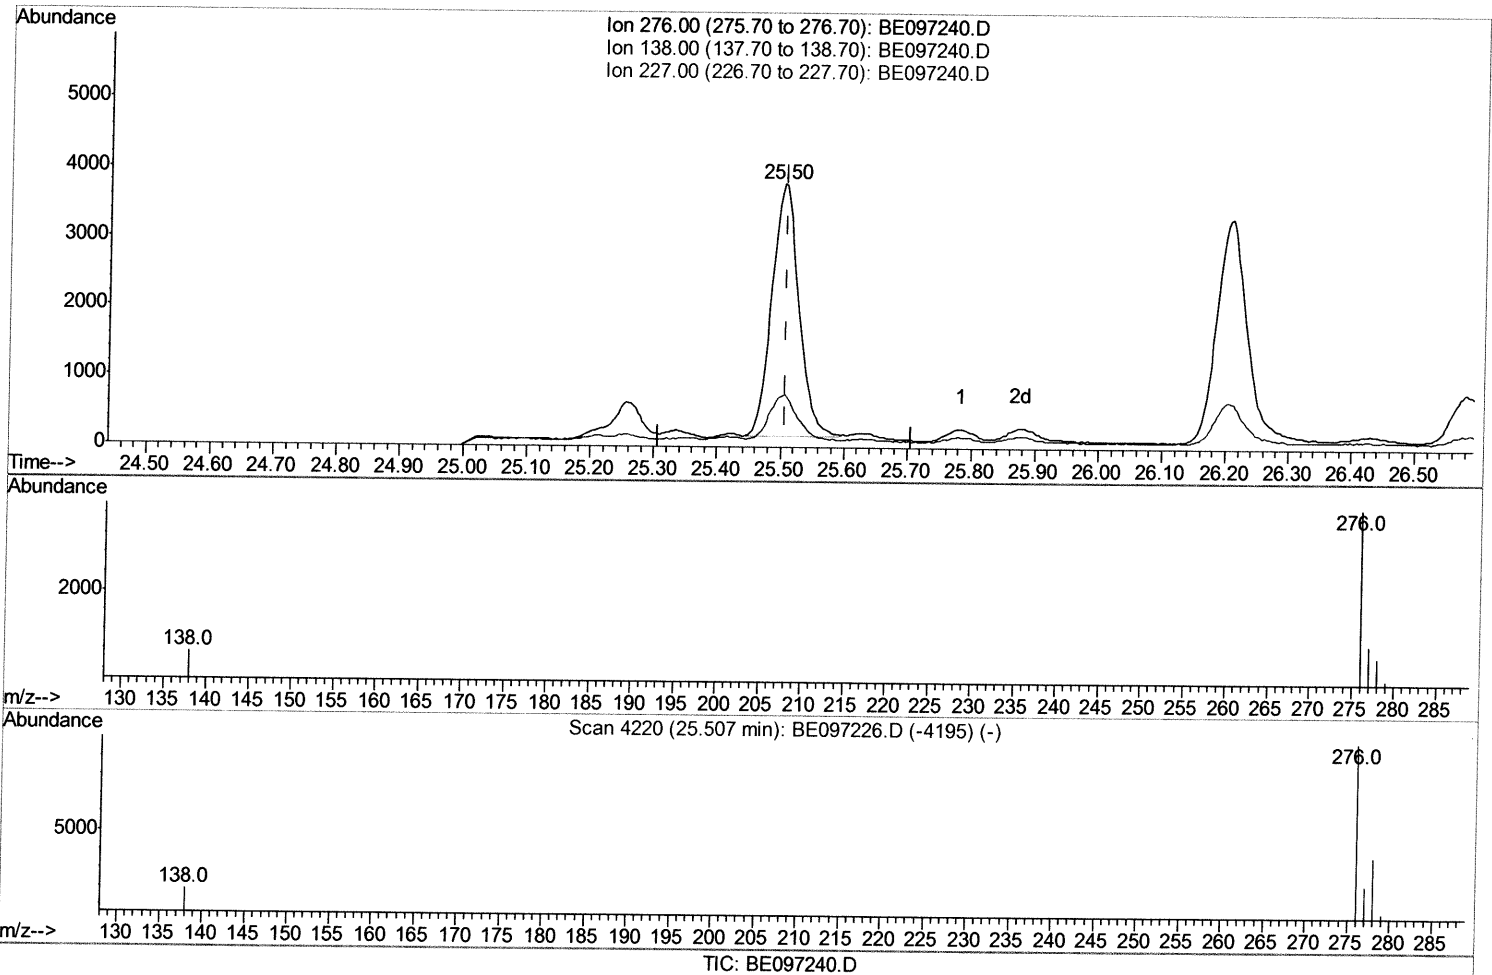

(24) Indeno(1,2,3-cd)pyrene

25.502min (-0.005) 0.40ng/ul m> SJ 8/10/18

response 10792

Ion	Exp%	Act%
276.00	100	100
138.00	35.00	2.00#
227.00	10.00	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097240.D
 Acq On : 8 Aug 2018 18:13
 Operator : SJ/JU
 Sample : J4268-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AA6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:31:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

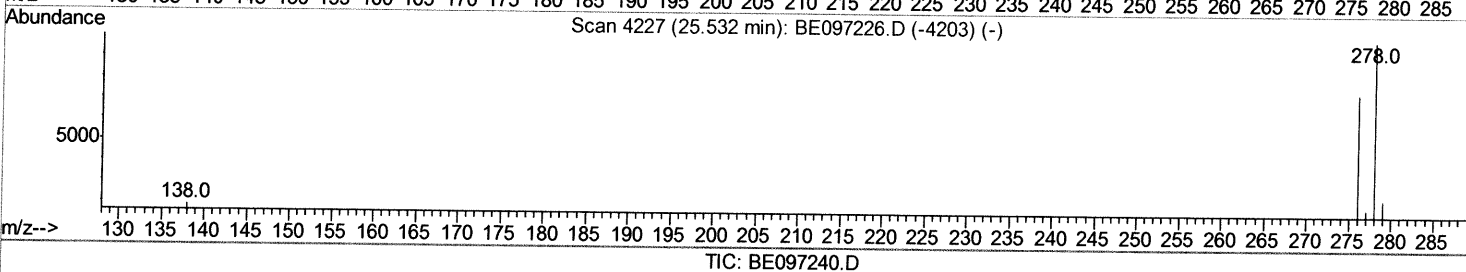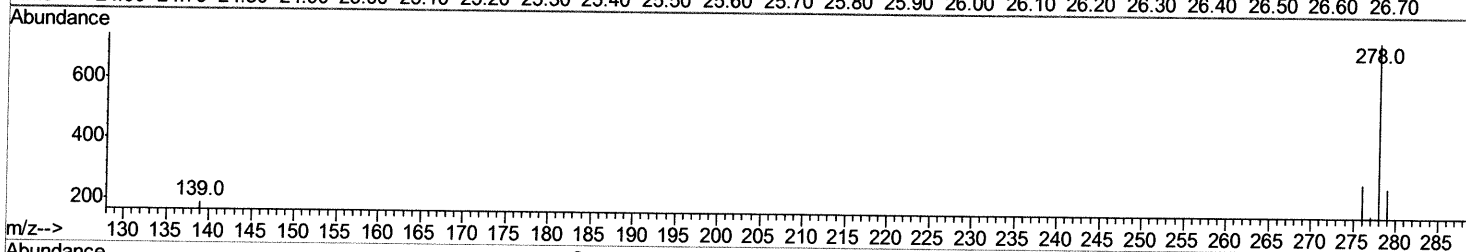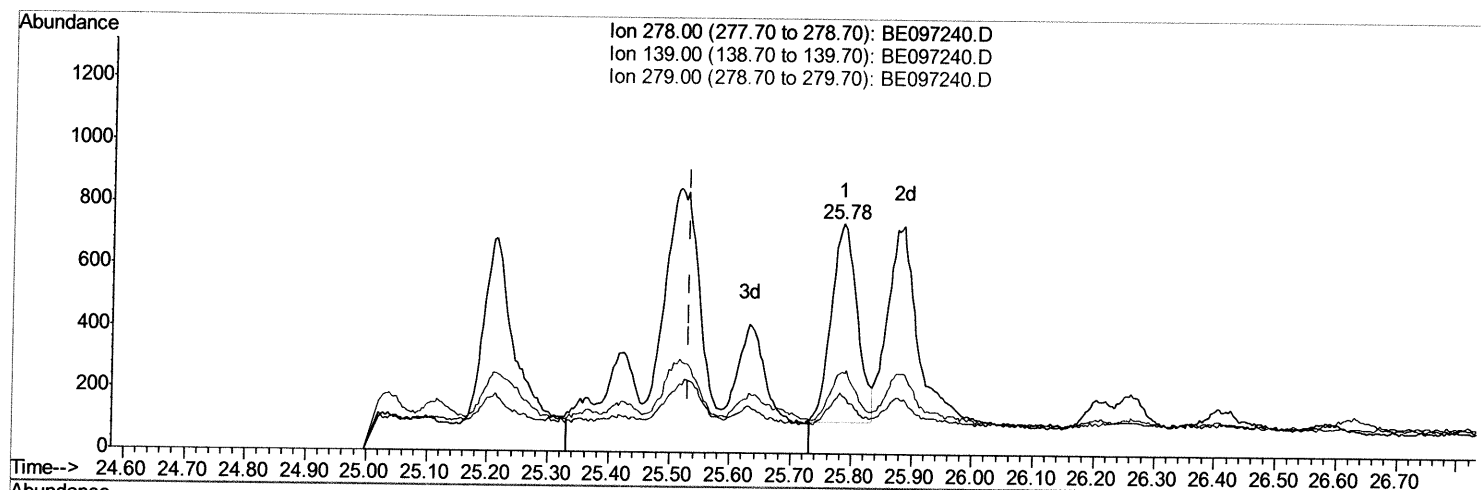

(25) Dibenzo(a,h)anthracene

25.784min (+0.252) 0.09ng/ul

response 1941

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	25.30
279.00	32.40	35.40
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
Data File : BE097240.D
Acq On : 8 Aug 2018 18:13
Operator : SJ/JU
Sample : J4268-04
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampled :
C0AA6

Manual Integrations
APPROVED

Sohil
8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:31:08 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 23:25:58 2018
Response via : Initial Calibration

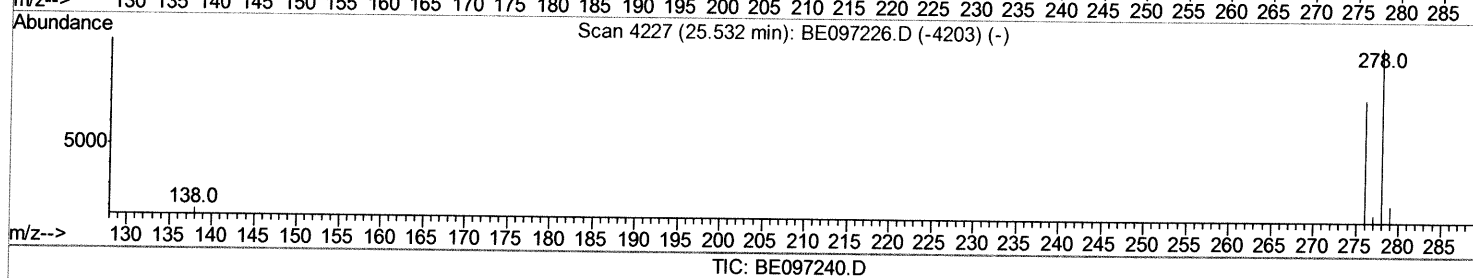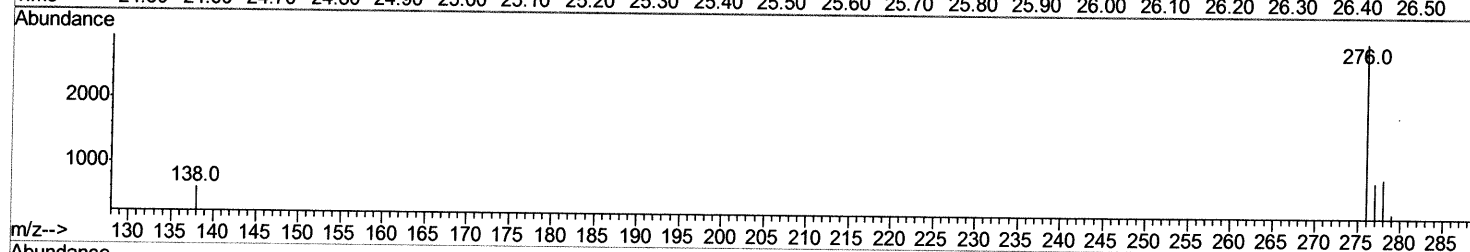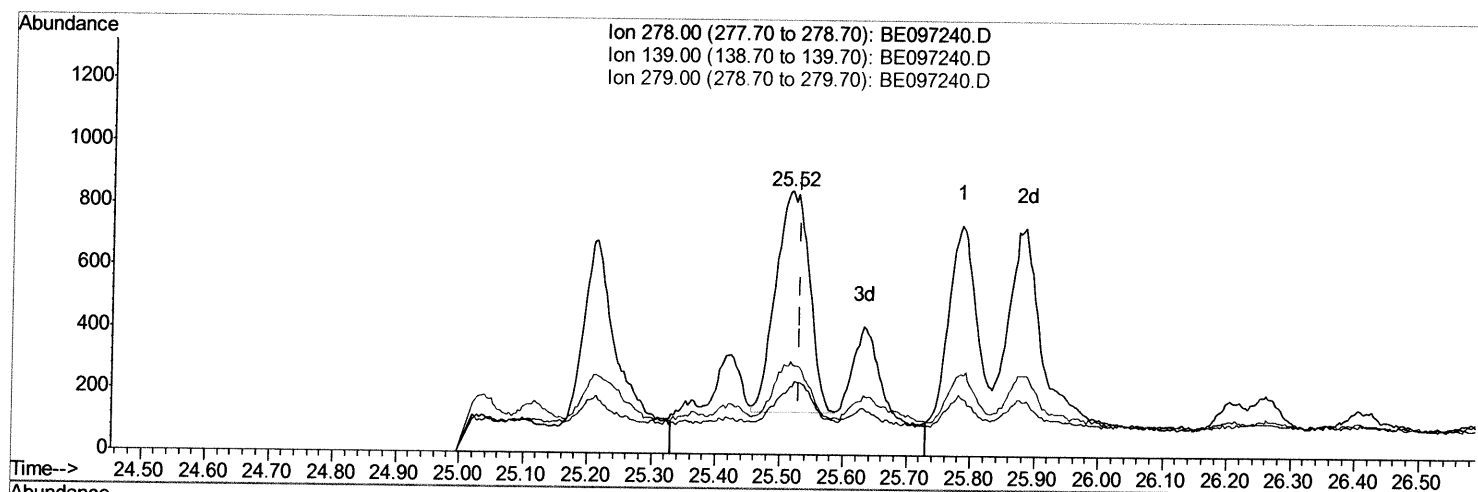

(25) Dibenzo(a,h)anthracene

25.517min (-0.016) 0.12ng/ul m> SJ 8/10/18

response 2595

Ion	Exp%	Act%
278.00	100	100
139.00	21.70	26.06#
279.00	32.40	35.33
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097240.D
 Acq On : 8 Aug 2018 18:13
 Operator : SJ/JU
 Sample : J4268-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:31:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

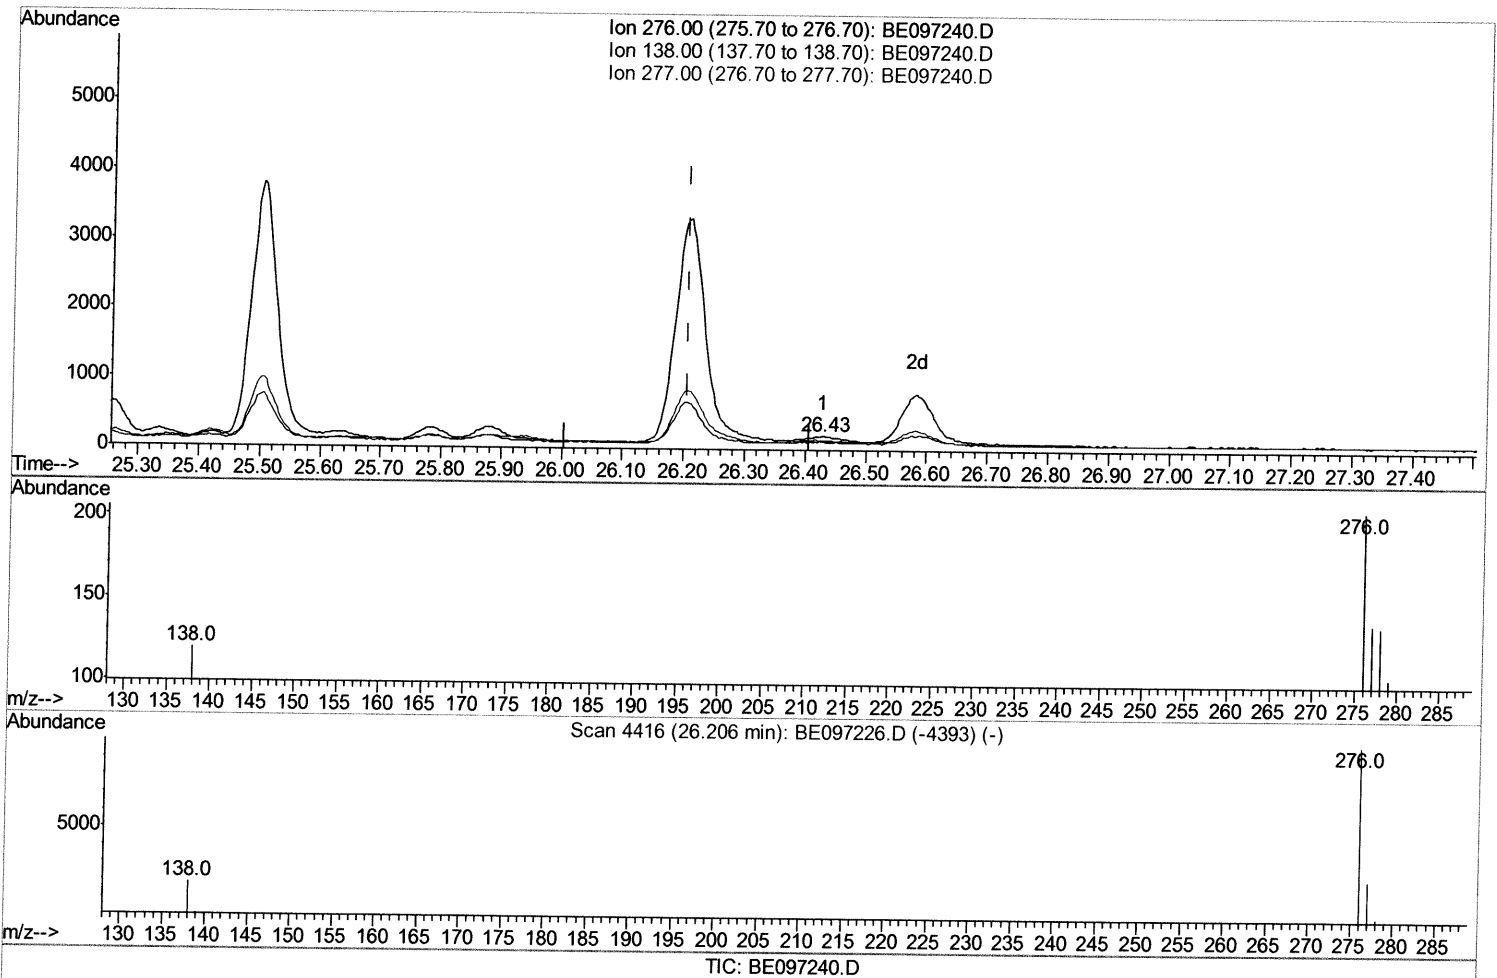

(26) Benzo(g,h,i)perylene
 26.430min (+0.223) 0.01ng/ul
 response 298

Ion	Exp%	Act%
276.00	100	100
138.00	27.30	58.05#
277.00	25.60	66.83#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097240.D
 Acq On : 8 Aug 2018 18:13
 Operator : SJ/JU
 Sample : J4268-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AA6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:31:08 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

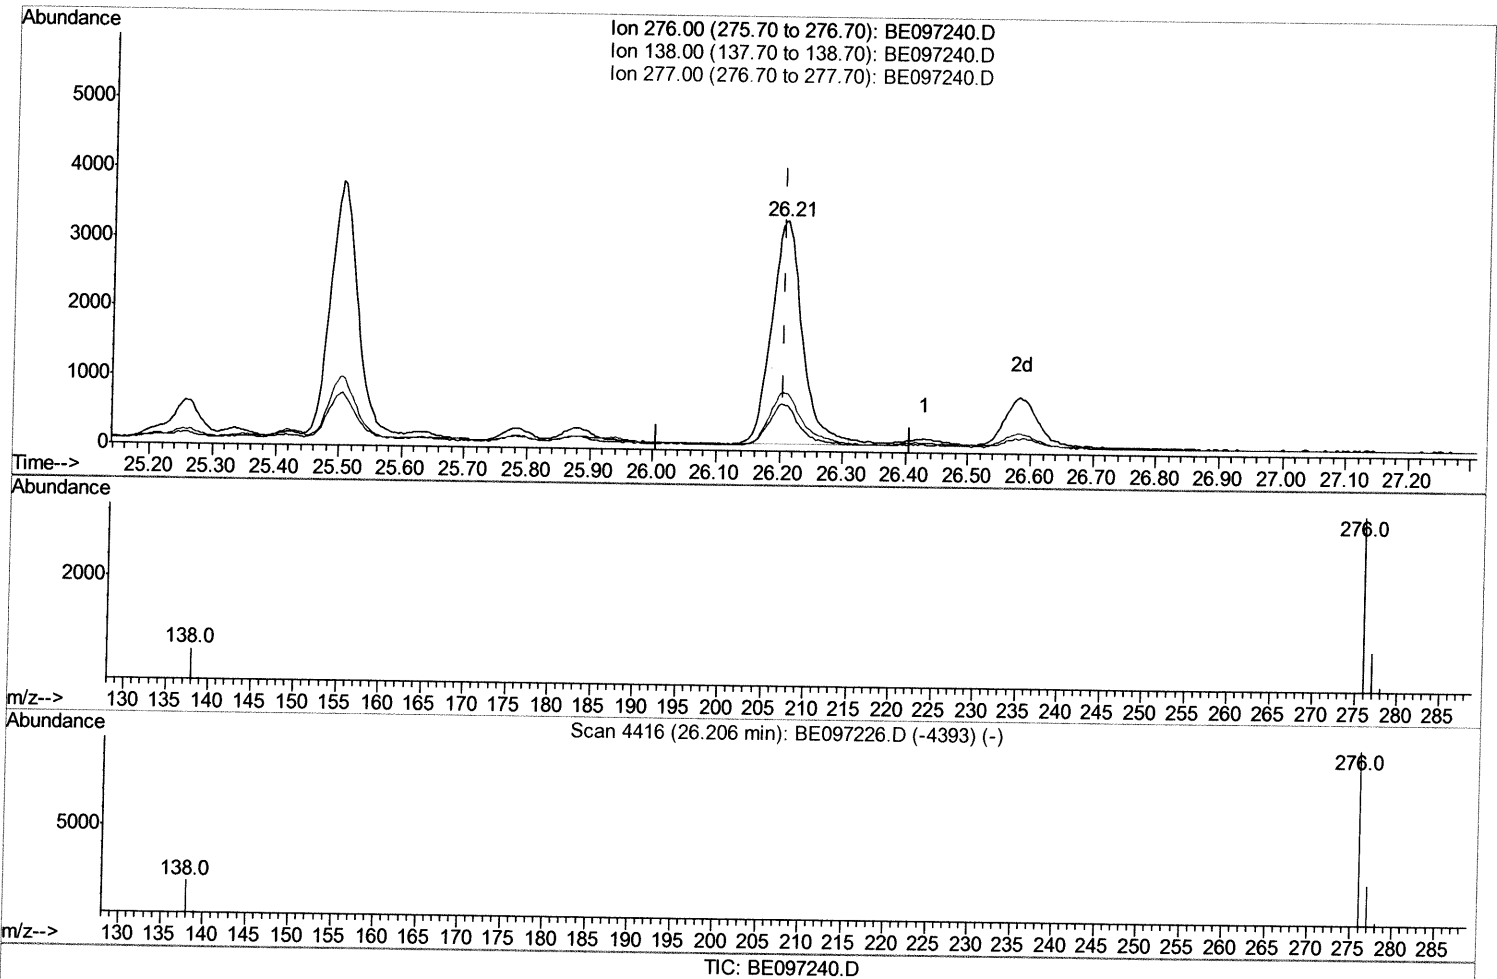

(26) Benzo(g,h,i)perylene

26.209min (+0.002) 0.46ng/ul m> SJ 8/10/18

response 10838

Ion	Exp%	Act%
276.00	100	100
138.00	27.30	19.84#
277.00	25.60	25.11
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE080818\
 Data File : BE097240.D
 Acq On : 8 Aug 2018 18:13
 Operator : SJ/JU
 Sample : J4268-04
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AA6

Manual Integrations
 APPROVED

Sohil
 8/9/2018 4:43:21 PM

Quant Time: Aug 09 01:34:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE080118.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 23:25:58 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.39	152	1147	0.40	ng/ul	0.00
2) Naphthalene-d8	10.13	136	6064	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.02	164	3674	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.77	188	8579m	0.40	ng/ul	0.00
16) Chrysene-d12	20.97	240	8752m	0.40	ng/ul	0.00
20) Perylene-d12	23.21	264	7996m	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.72	152	1878	0.19	ng/ul	0.00
14) Fluoranthene-d10	18.81	212	5430m	0.18	ng/ul	0.00

Target Compounds

					Ovalue	
3) Naphthalene	10.18	128	1120	0.076	ng/ul#	89
5) 2-Methylnaphthalene	11.80	142	256	0.026	ng/ul	97
7) Acenaphthylene	13.73	152	602	0.038	ng/ul#	77
8) Acenaphthene	14.08	153	601	0.052	ng/ul#	92
9) Fluorene	15.08	166	793	0.060	ng/ul#	93
12) Phenanthrene	16.81	178	12112m	0.554	ng/ul	
13) Anthracene	16.90	178	2239m	0.110	ng/ul	
15) Fluoranthene	18.84	202	31772m	1.099	ng/ul	
17) Pyrene	19.20	202	31446	1.341	ng/ul#	80
18) Benzo(a)anthracene	20.96	228	17002m	0.680	ng/ul	
19) Chrysene	21.01	228	17418	0.676	ng/ul	98
21) Benzo(b)fluoranthene	22.53	252	23462m	1.077	ng/ul	
22) Benzo(k)fluoranthene	22.58	252	7005m	0.298	ng/ul	
23) Benzo(a)pyrene	23.11	252	16265m	0.746	ng/ul	
24) Indeno(1,2,3-cd)pyrene	25.50	276	10792m	0.395	ng/ul	
25) Dibenzo(a,h)anthracene	25.52	278	2595m	0.116	ng/ul	
26) Benzo(a,h,i)perylene	26.21	276	10838m	0.460	ng/ul	

(#) = qualifier out of range (m) = manual integration (+) = signals summed