

Data Path : \\74.0.250.170\terastorage\svoasrv\HPCHEM1\BNA\_E\Data\BE080818\  
 Data File : BE097229.D  
 Acq On : 8 Aug 2018 11:18  
 Operator : SJ/JU  
 Sample : J4265-16  
 Misc :  
 ALS Vial : 5 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 C0AB6

Manual Integrations  
 APPROVED

Sohil  
 8/9/2018 4:42:51 PM

Quant Time: Aug 16 06:52:44 2018  
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\SOM-EPA-SIM-BE080118.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Aug 08 23:25:58 2018  
 Response via : Initial Calibration

| Internal Standards          | R.T.  | QIon | Response | Conc  | Units  | Dev(Min)     |
|-----------------------------|-------|------|----------|-------|--------|--------------|
| 1) 1,4-Dichlorobenzene-d4   | 7.39  | 152  | 1074     | 0.40  | ng/ul  | 0.00         |
| 2) Naphthalene-d8           | 10.13 | 136  | 5805     | 0.40  | ng/ul  | 0.00         |
| 6) Acenaphthene-d10         | 14.02 | 164  | 3676     | 0.40  | ng/ul  | 0.00         |
| 10) Phenanthrene-d10        | 16.77 | 188  | 8355m    | 0.40  | ng/ul  | 0.00         |
| 16) Chrysene-d12            | 20.98 | 240  | 7986m    | 0.40  | ng/ul  | 0.00         |
| 20) Perylene-d12            | 23.21 | 264  | 7221m    | 0.40  | ng/ul  | 0.00         |
| System Monitoring Compounds |       |      |          |       |        |              |
| 4) 2-Methylnaphthalene-d10  | 11.73 | 152  | 3302     | 0.35  | ng/ul  | 0.00         |
| 14) Fluoranthene-d10        | 18.81 | 212  | 9613m    | 0.33  | ng/ul  | 0.00         |
| Target Compounds            |       |      |          |       |        |              |
| 3) Naphthalene              | 10.18 | 128  | 482      | 0.034 | ng/ul# | Qvalue<br>77 |

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\terastorage\svoasrv\HPCHEM1\BNA\_E\Data\BE080818\  
Data File : BE097229.D  
Acq On : 8 Aug 2018 11:18  
Operator : SJ/JU  
Sample : J4265-16  
Misc :  
ALS Vial : 5 Sample Multiplier: 1




Instrument :  
BNA\_E  
ClientSampleId :  
C0AB6

Manual Integrations  
APPROVED

Sohil  
8/9/2018 4:42:51 PM

Quant Time: Aug 16 06:52:44 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\SOM-EPA-SIM-BE080118.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Aug 08 23:25:58 2018  
Response via : Initial Calibration

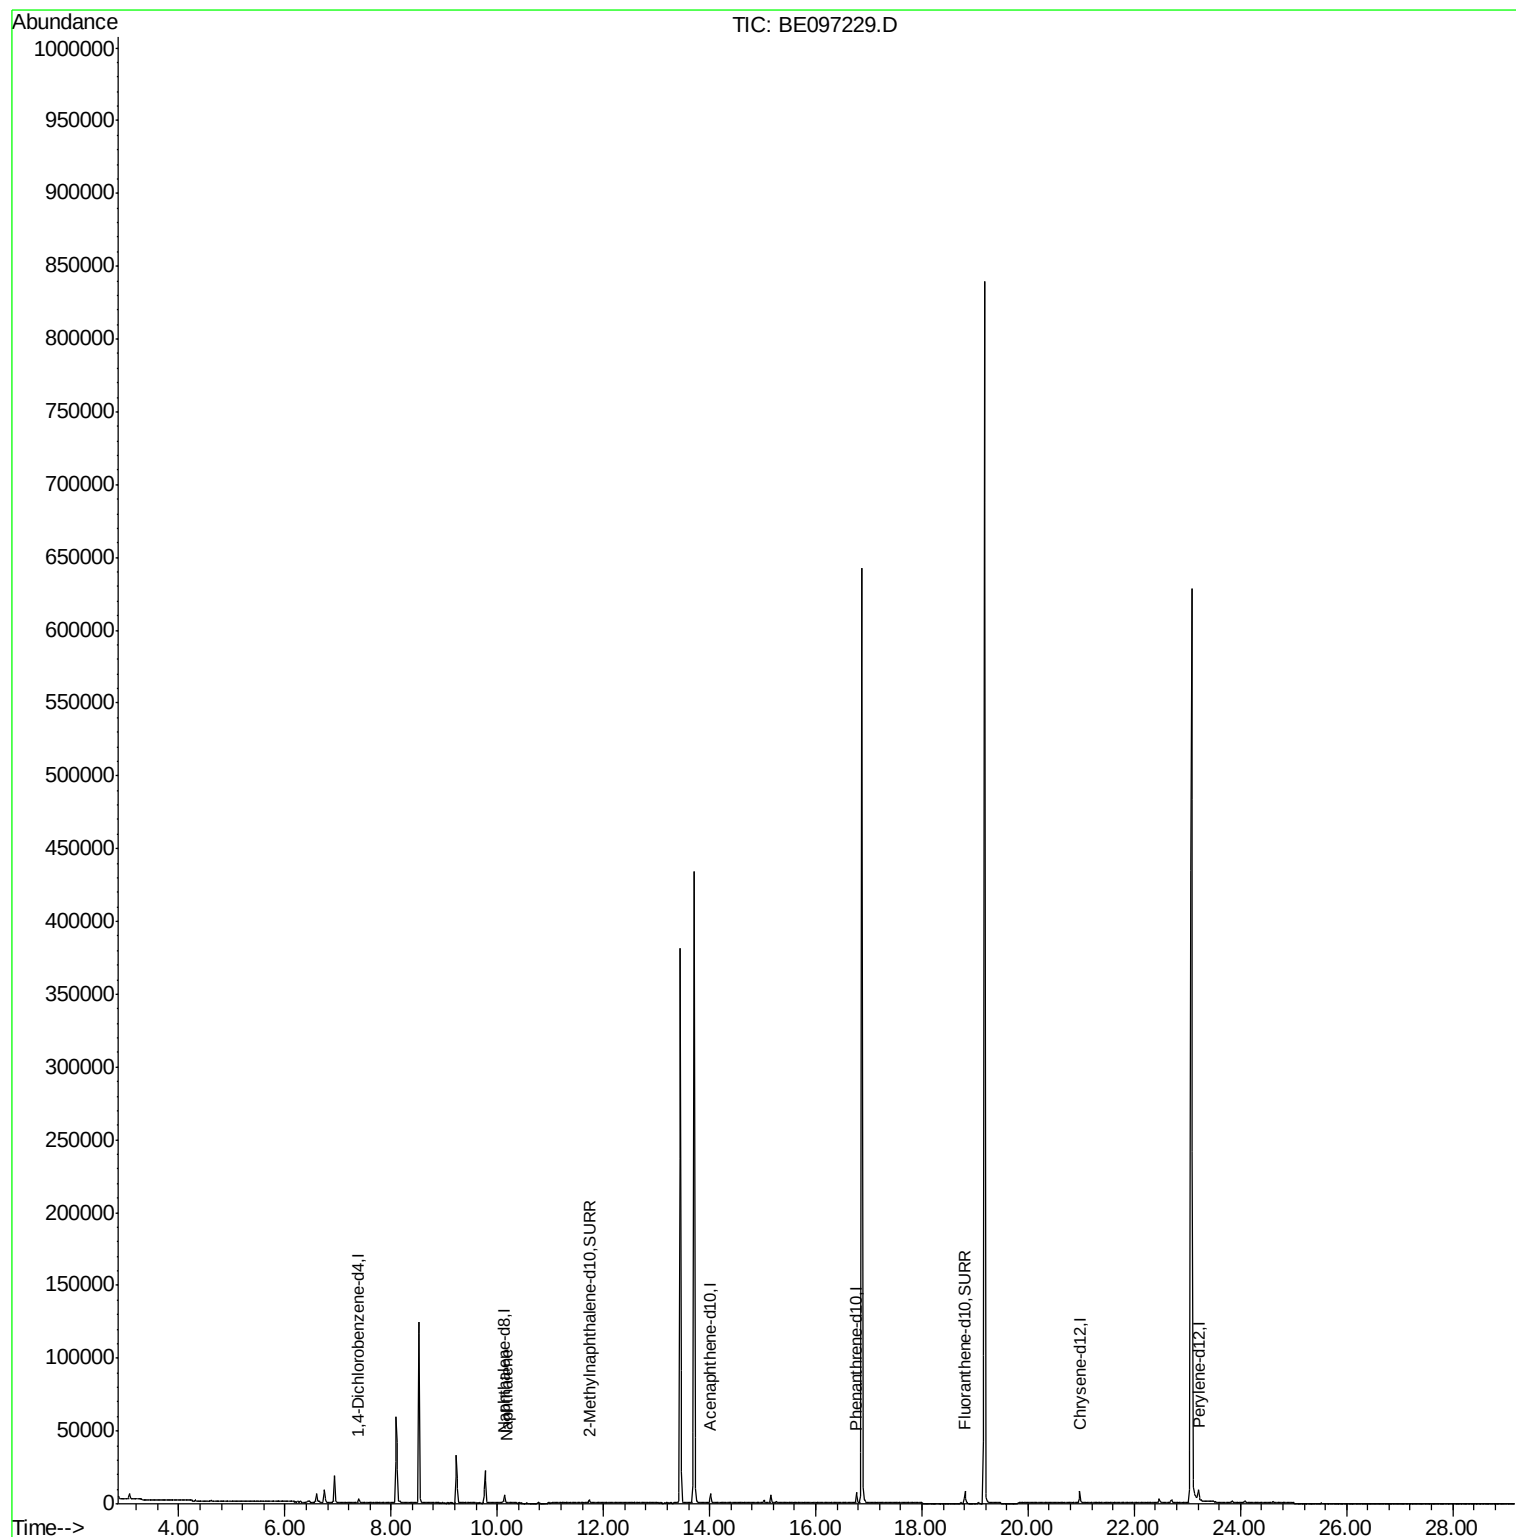

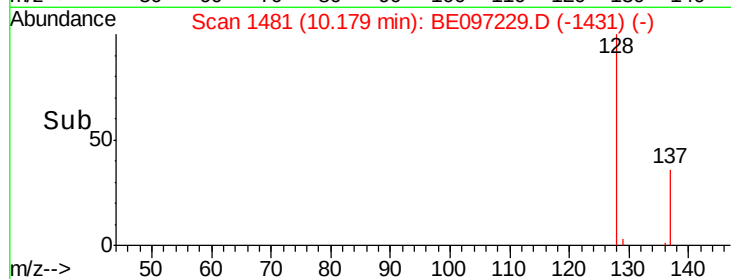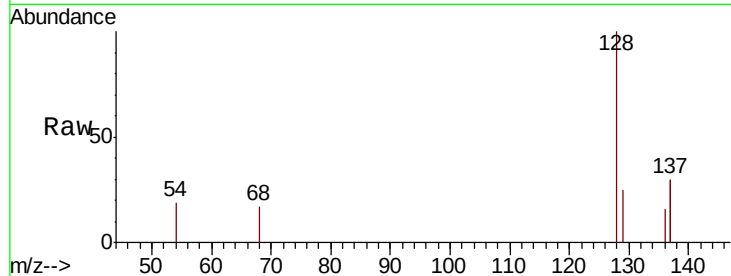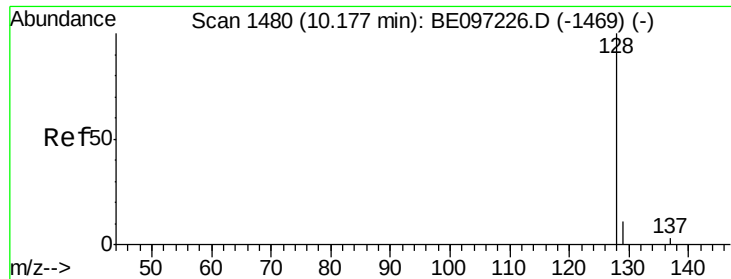

#3

Naphthalene

Concen: 0.034 ng/ul

RT: 10.18 min Scan# 1481

Delta R.T. 0.00 min

Lab File: BE097229.D

Acq: 8 Aug 2018 11:18

Instrument :

BNA\_E

ClientSampleId :

C0AB6

|           |       |       |       |
|-----------|-------|-------|-------|
| Tgt Ion:  | 128   | Resp: | 482   |
| Ion Ratio | Lower | Upper |       |
| 128       | 100   |       |       |
| 129       | 24.8  | 11.3  | 16.9# |
| 127       | 0.0   | 4.0   | 6.0#  |

Manual Integrations  
APPROVED

Sohil  
8/9/2018 4:42:51 PM

