
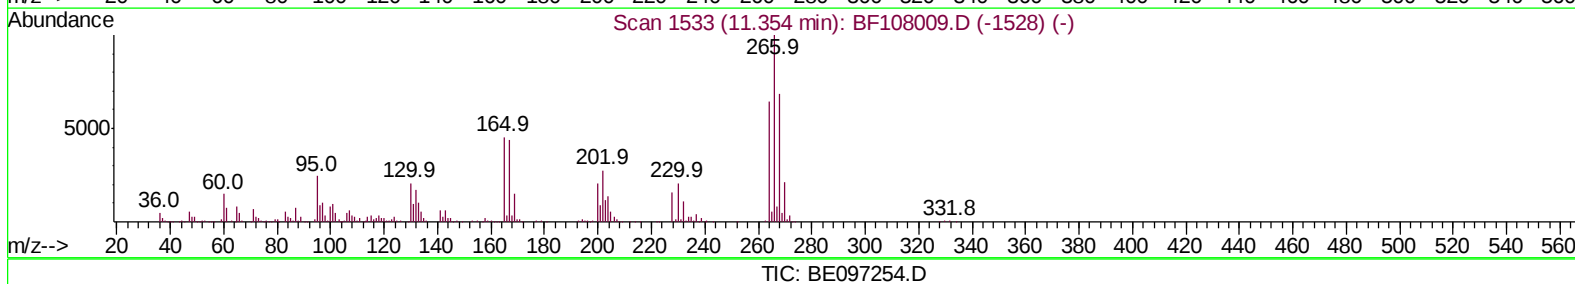
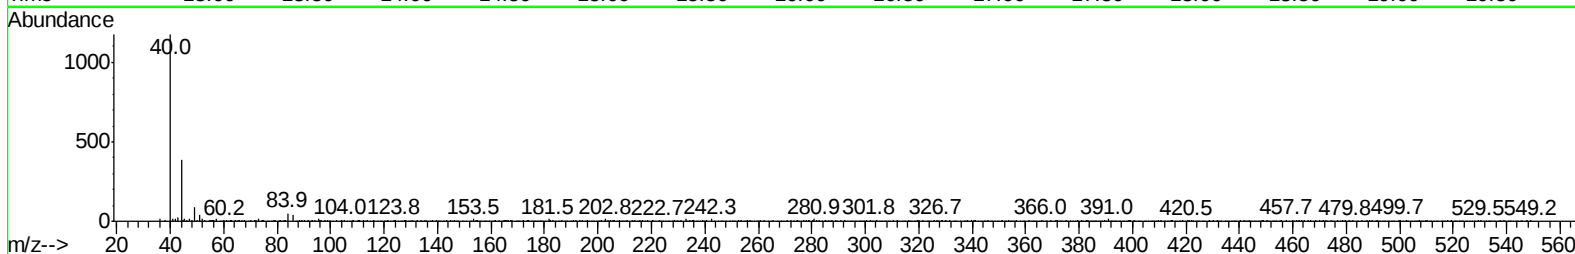


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE081018\
Data File : BE097254.D
Acq On : 10 Aug 2018 8:24
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 10:11:20 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Aug 08 12:24:24 2018
Response via : Initial Calibration

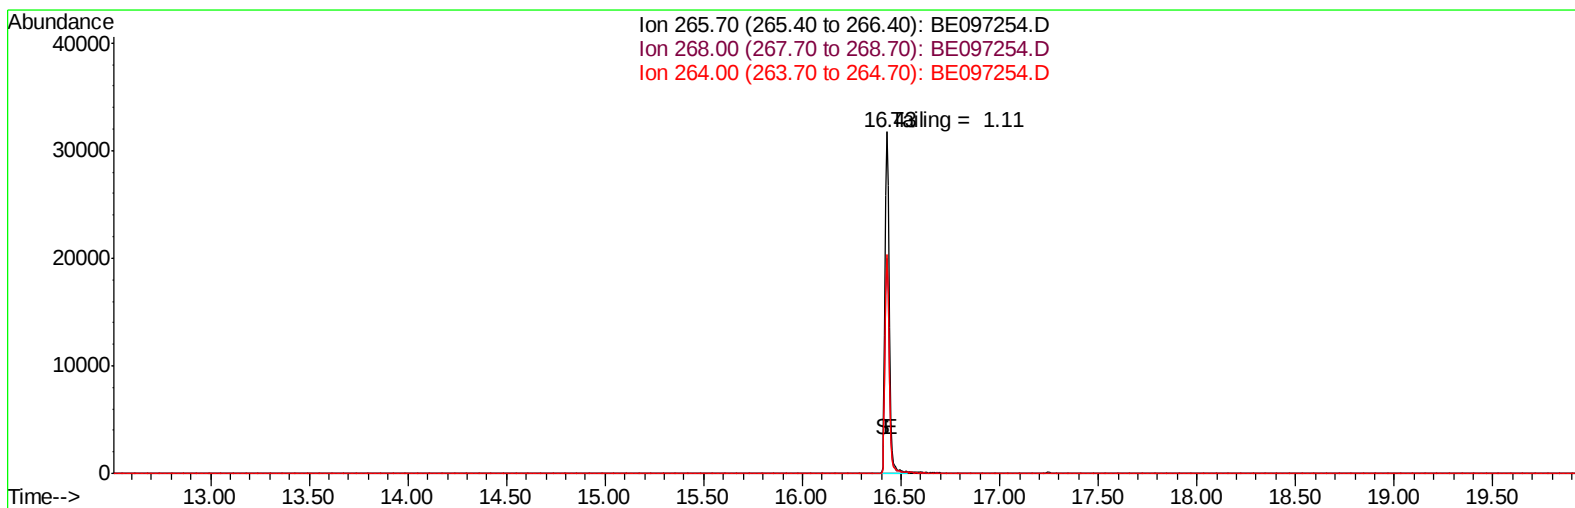

TIC: BE097254.D

(69) Pentachlorophenol (C)




11.201min (-0.153) 251.24ng

response 11

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	88.89#
264.00	61.90	55.56
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE081018\
 Data File : BE097254.D
 Acq On : 10 Aug 2018 8:24
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 14 10:11:20 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF080818.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Aug 08 12:24:24 2018
 Response via : Initial Calibration

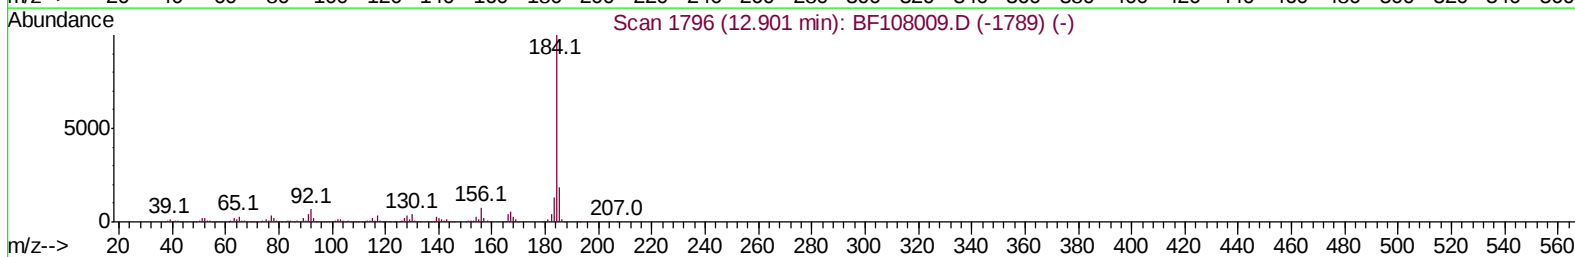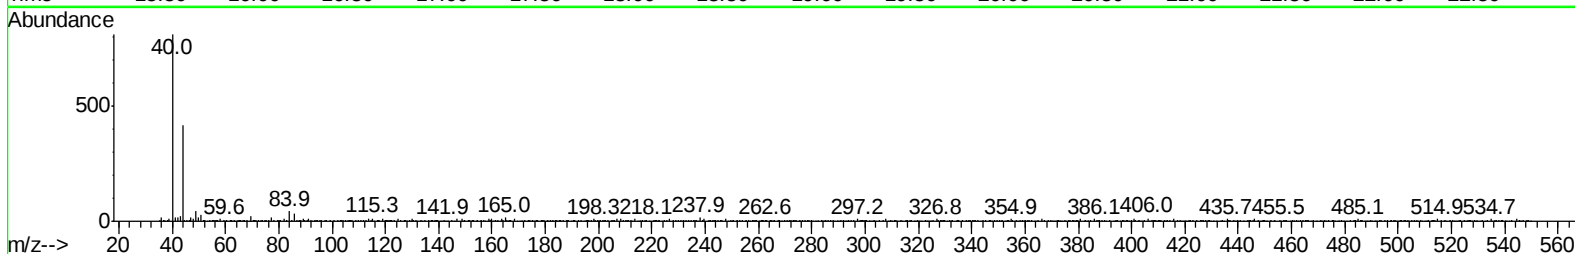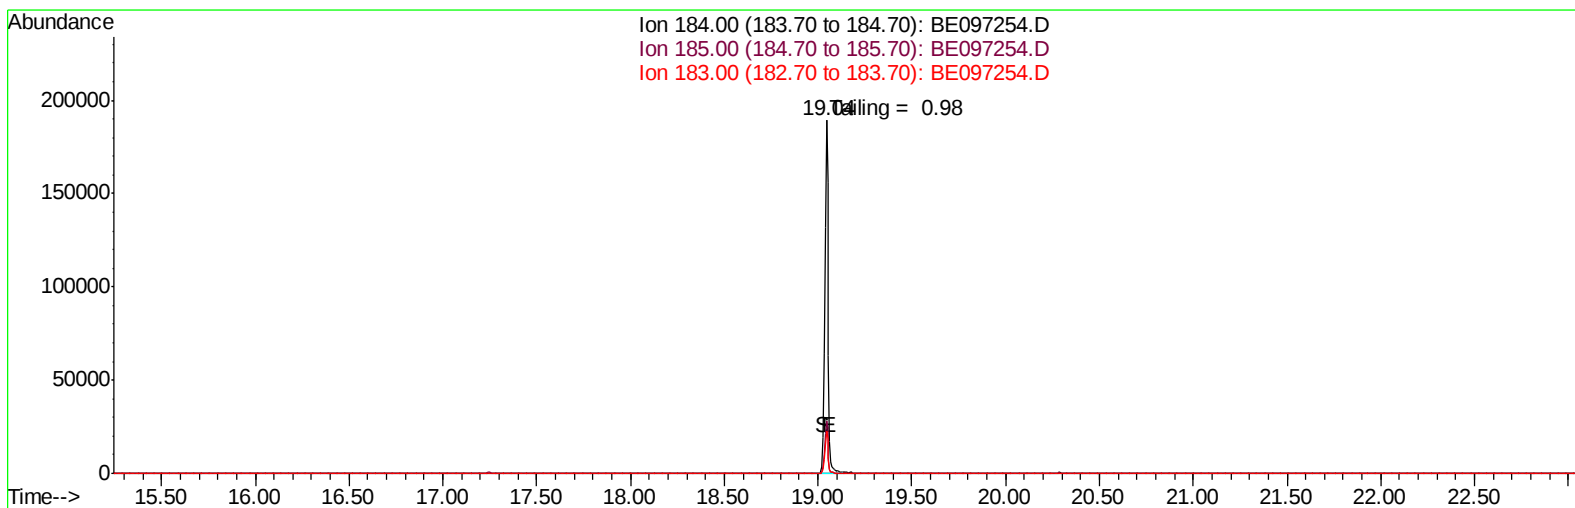

TIC: BE097254.D

(76) Benzidine

12.722min (-0.178) 5.35ng

response 3

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	42.86#
183.00	11.60	142.86#
0.00	0.00	0.00