


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE081018\
Data File : BE097254.D
Acq On : 10 Aug 2018 8:24
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE072418.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 31 10:49:28 2018

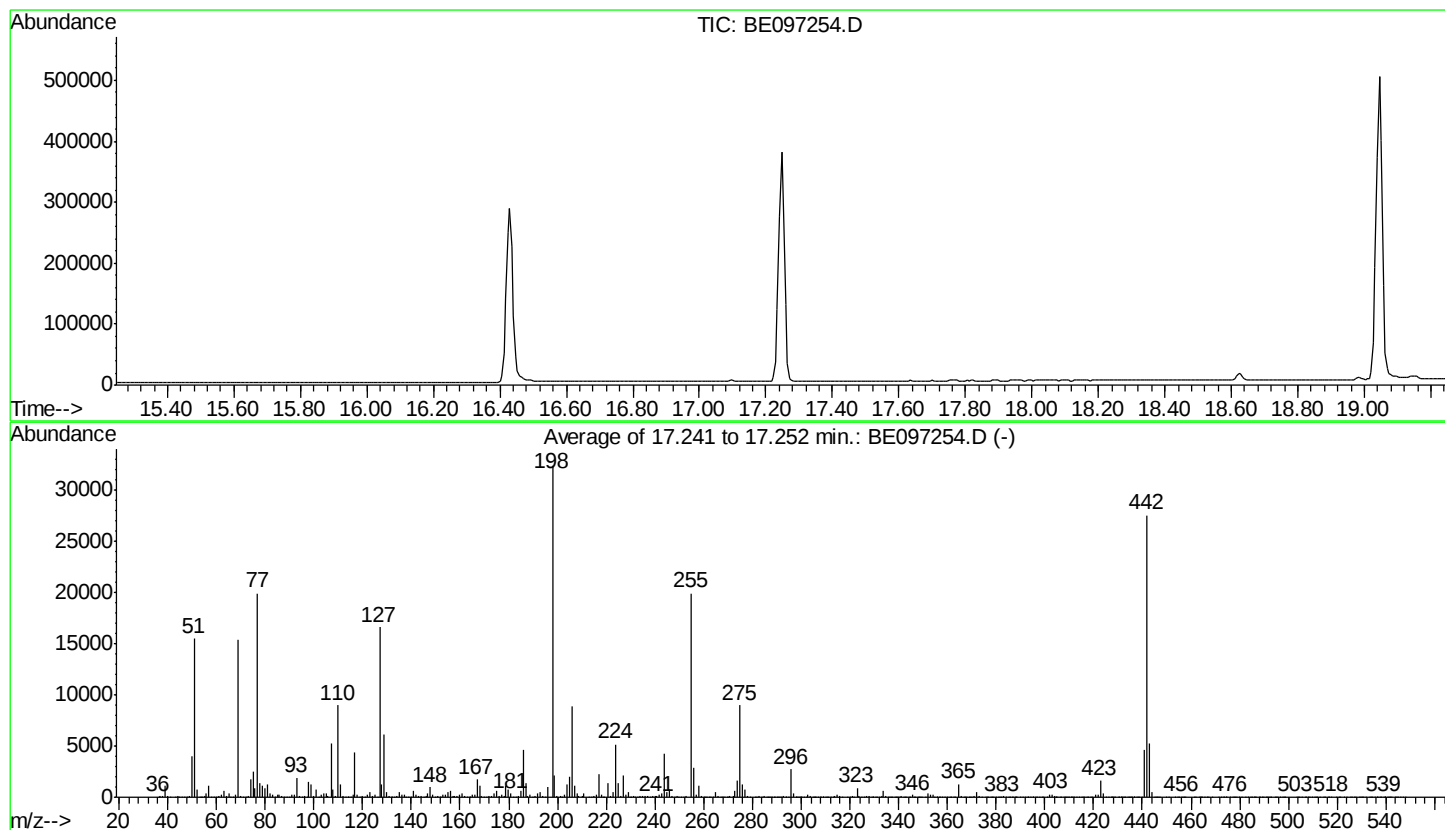

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2482

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.8	15468	PASS
68	69	0.00	2	1.9	284	PASS
69	198	0.00	100	47.4	15342	PASS
70	69	0.00	2	0.6	98	PASS
127	198	10	80	51.2	16572	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	32340	PASS
199	198	5	9	6.6	2142	PASS
275	198	10	60	27.8	8975	PASS
365	198	1	100	3.9	1251	PASS
441	198	0.01	100	14.3	4639	PASS
442	198	50	100	85.1	27531	PASS
443	442	15	24	19.2	5288	PASS