


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE081618\  
Data File : BE097285.D  
Acq On : 16 Aug 2018 10:42  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE081518.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Aug 15 14:23:39 2018

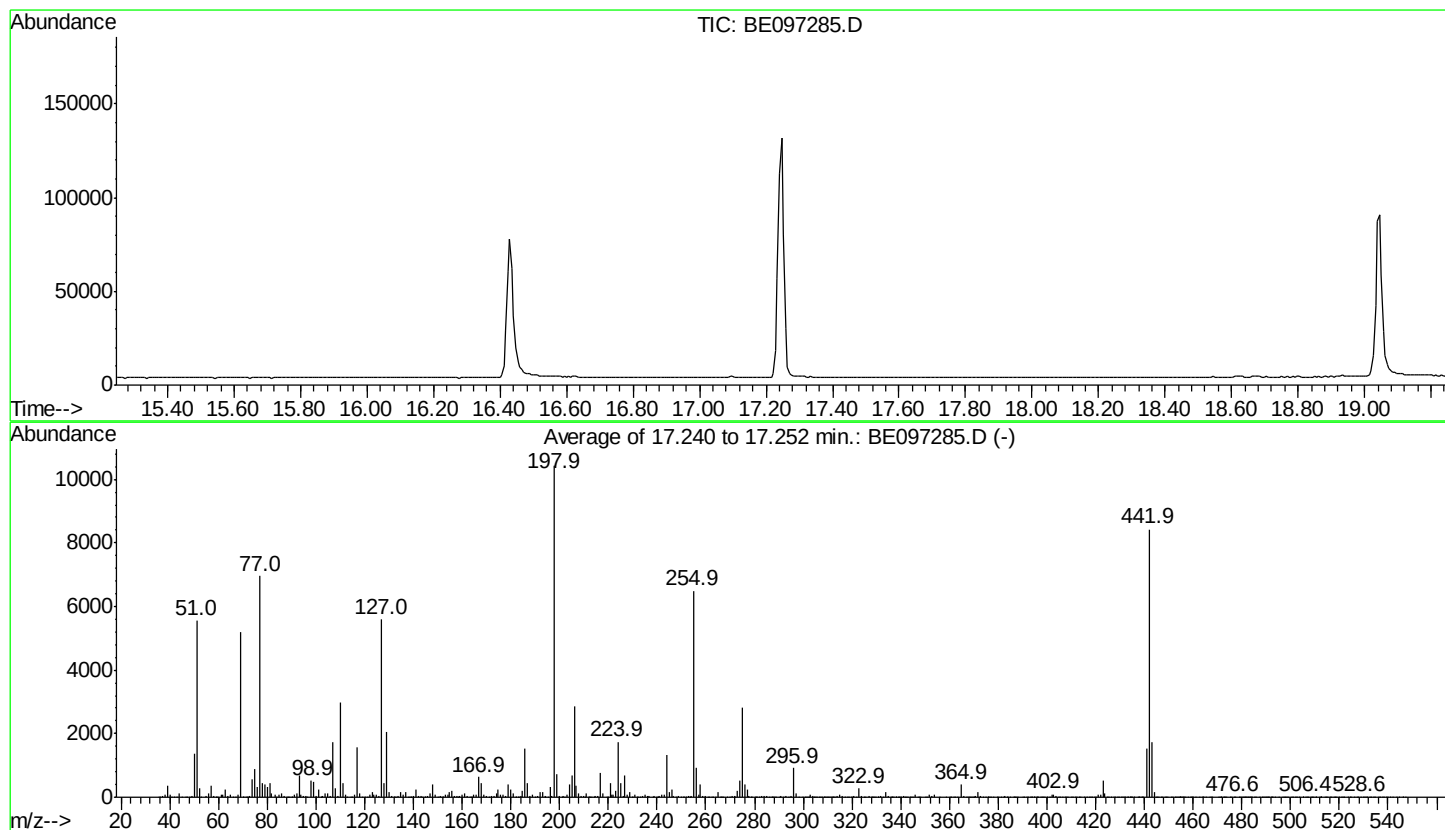

AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2488

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 53.3      | 5555    | PASS             |
| 68          | 69           | 0.00         | 2            | 1.8       | 93      | PASS             |
| 69          | 198          | 0.00         | 100          | 49.8      | 5194    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.2       | 9       | PASS             |
| 127         | 198          | 10           | 80           | 53.5      | 5583    | PASS             |
| 197         | 198          | 0.00         | 2            | 0.2       | 25      | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 10430   | PASS             |
| 199         | 198          | 5            | 9            | 6.9       | 721     | PASS             |
| 275         | 198          | 10           | 60           | 27.2      | 2835    | PASS             |
| 365         | 198          | 1            | 100          | 3.8       | 399     | PASS             |
| 441         | 198          | 0.01         | 100          | 14.6      | 1519    | PASS             |
| 442         | 198          | 50           | 100          | 80.8      | 8431    | PASS             |
| 443         | 442          | 15           | 24           | 20.6      | 1734    | PASS             |