


Data Path : Z:\svoasrv\HPCHEM1\BNA_E\Data\BE082018\
 Data File : BE097330.D
 Acq On : 20 Aug 2018 13:38
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE082018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Aug 20 18:32:10 2018

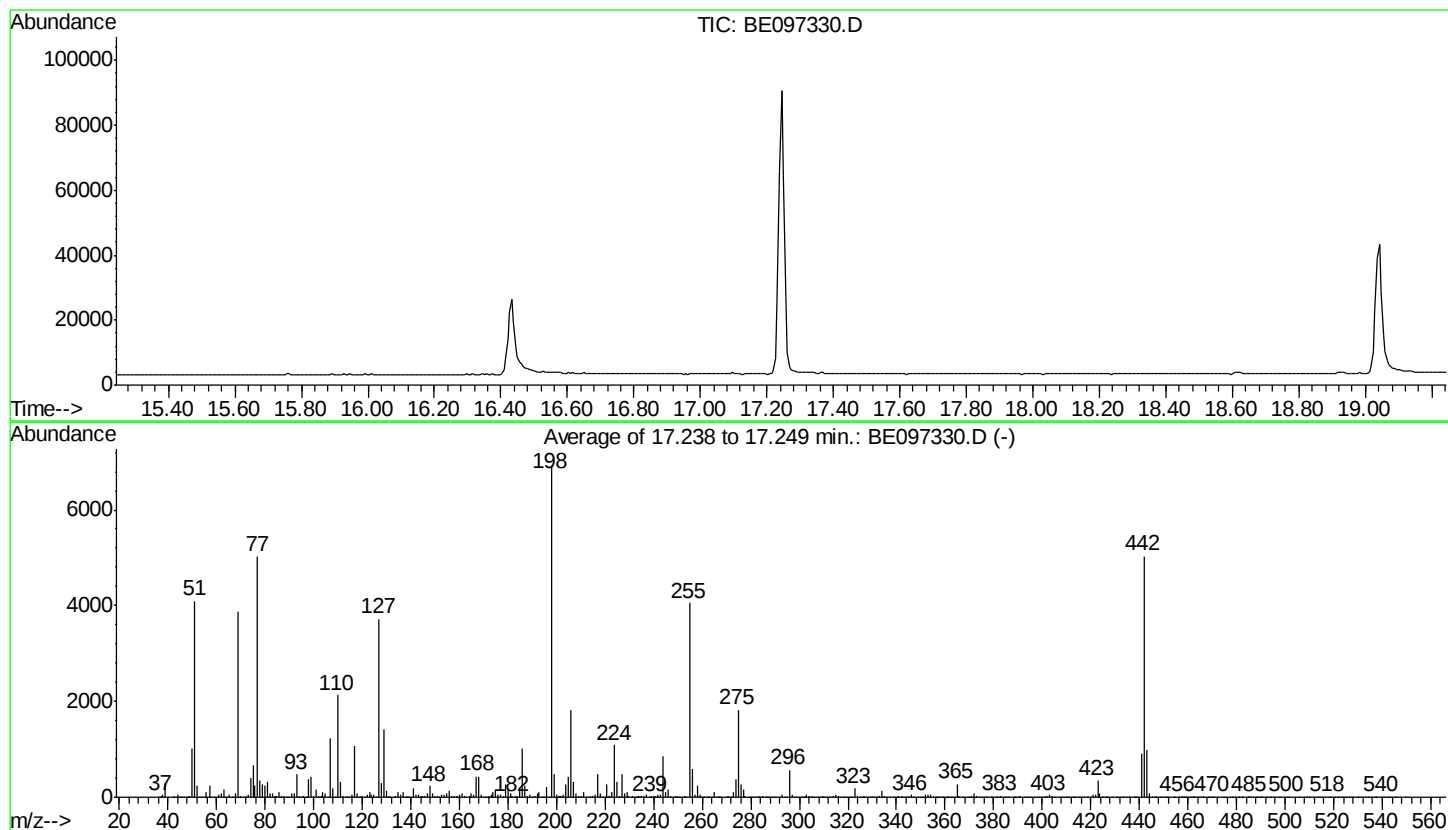

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.3	4103	PASS
68	69	0.00	2	1.8	71	PASS
69	198	0.00	100	55.9	3868	PASS
70	69	0.00	2	0.8	30	PASS
127	198	10	80	53.8	3728	PASS
197	198	0.00	2	0.1	8	PASS
198	198	100	100	100.0	6923	PASS
199	198	5	9	7.0	483	PASS
275	198	10	60	26.3	1820	PASS
365	198	1	100	3.9	270	PASS
441	443	0.01	100	92.1	915	PASS
442	198	50	100	72.7	5035	PASS
443	442	15	24	19.7	993	PASS