


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE082318\  
Data File : BE097353.D  
Acq On : 23 Aug 2018 9:56  
Operator : SJ/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_E  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE082218.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Wed Aug 22 18:07:26 2018

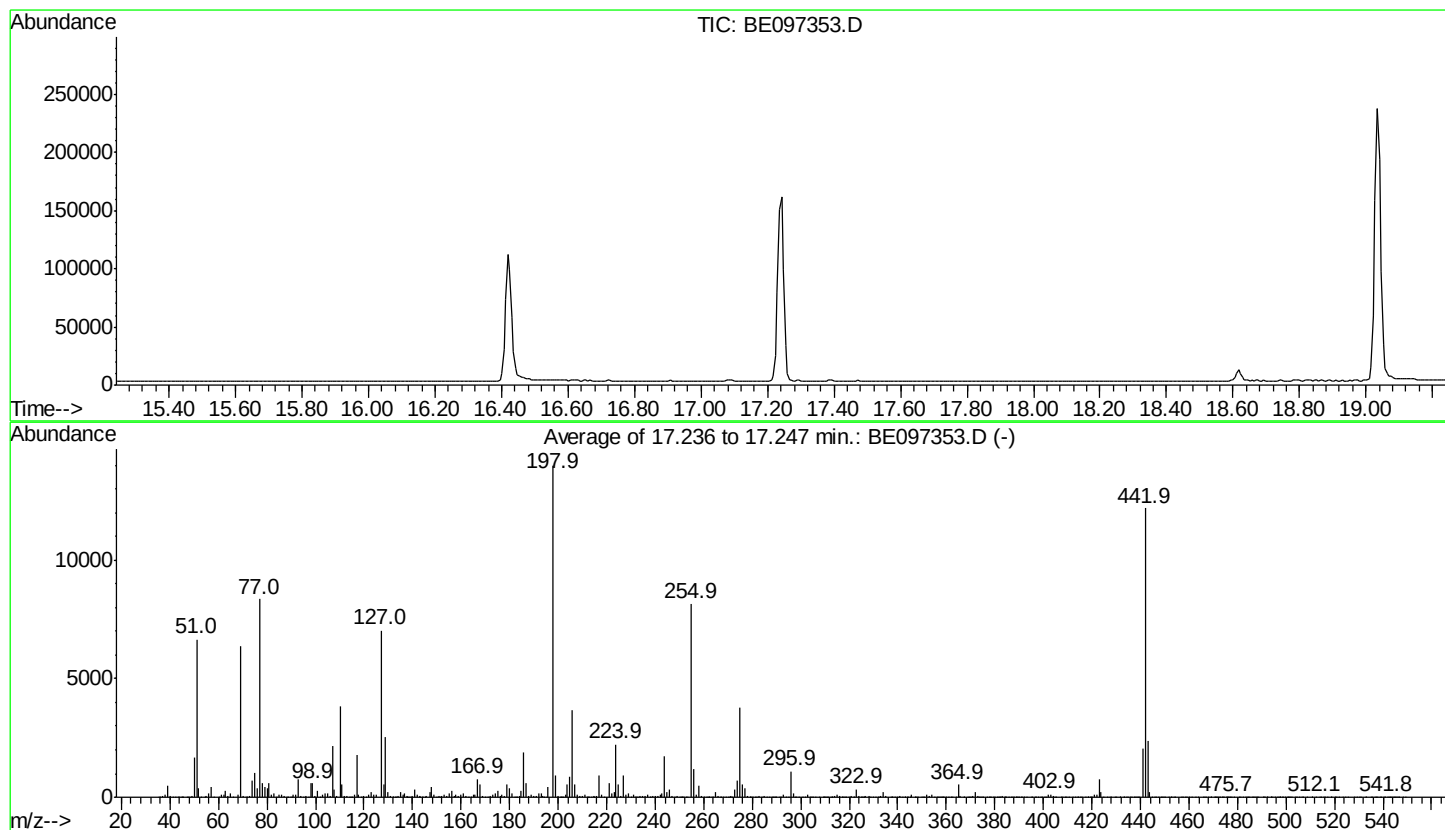

AutoFind: Scans 2493, 2494, 2495; Background Corrected with Scan 2481

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 47.5      | 6645    | PASS             |
| 68          | 69           | 0.00         | 2            | 2.0       | 125     | PASS             |
| 69          | 198          | 0.00         | 100          | 45.4      | 6353    | PASS             |
| 70          | 69           | 0.00         | 2            | 0.6       | 35      | PASS             |
| 127         | 198          | 10           | 80           | 50.2      | 7018    | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 13982   | PASS             |
| 199         | 198          | 5            | 9            | 6.4       | 900     | PASS             |
| 275         | 198          | 10           | 60           | 26.9      | 3768    | PASS             |
| 365         | 198          | 1            | 100          | 3.7       | 516     | PASS             |
| 441         | 198          | 0.01         | 100          | 14.5      | 2034    | PASS             |
| 442         | 198          | 50           | 100          | 87.1      | 12183   | PASS             |
| 443         | 442          | 15           | 24           | 19.5      | 2374    | PASS             |