

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097367.D
 Acq On : 24 Aug 2018 13:59
 Operator : SJ/JU
 Sample : J4422-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Aug 24 22:50:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	834	0.40	ng/ul	0.00
2) Naphthalene-d8	10.12	136	4326	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.01	164	2916	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.86	188	622249	0.40	ng/ul	0.10
16) Chrysene-d12	0.00	240	0	0.00	ng/ul	-20.97
20) Perylene-d12	23.20	264	13363	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.72	152	2347	0.34	ng/ul	0.00
14) Fluoranthene-d10	0.00	212	0	0.00	ng/ul	
Target Compounds						
9) Fluorene	15.01	166	860	0.083	ng/ul#	24
23) Benzo(a)pyrene	23.06	252	2685	0.080	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
Data File : BE097367.D
Acq On : 24 Aug 2018 13:59
Operator : SJ/JU
Sample : J4422-06
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Aug 24 22:50:57 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 24 22:49:42 2018
Response via : Initial Calibration

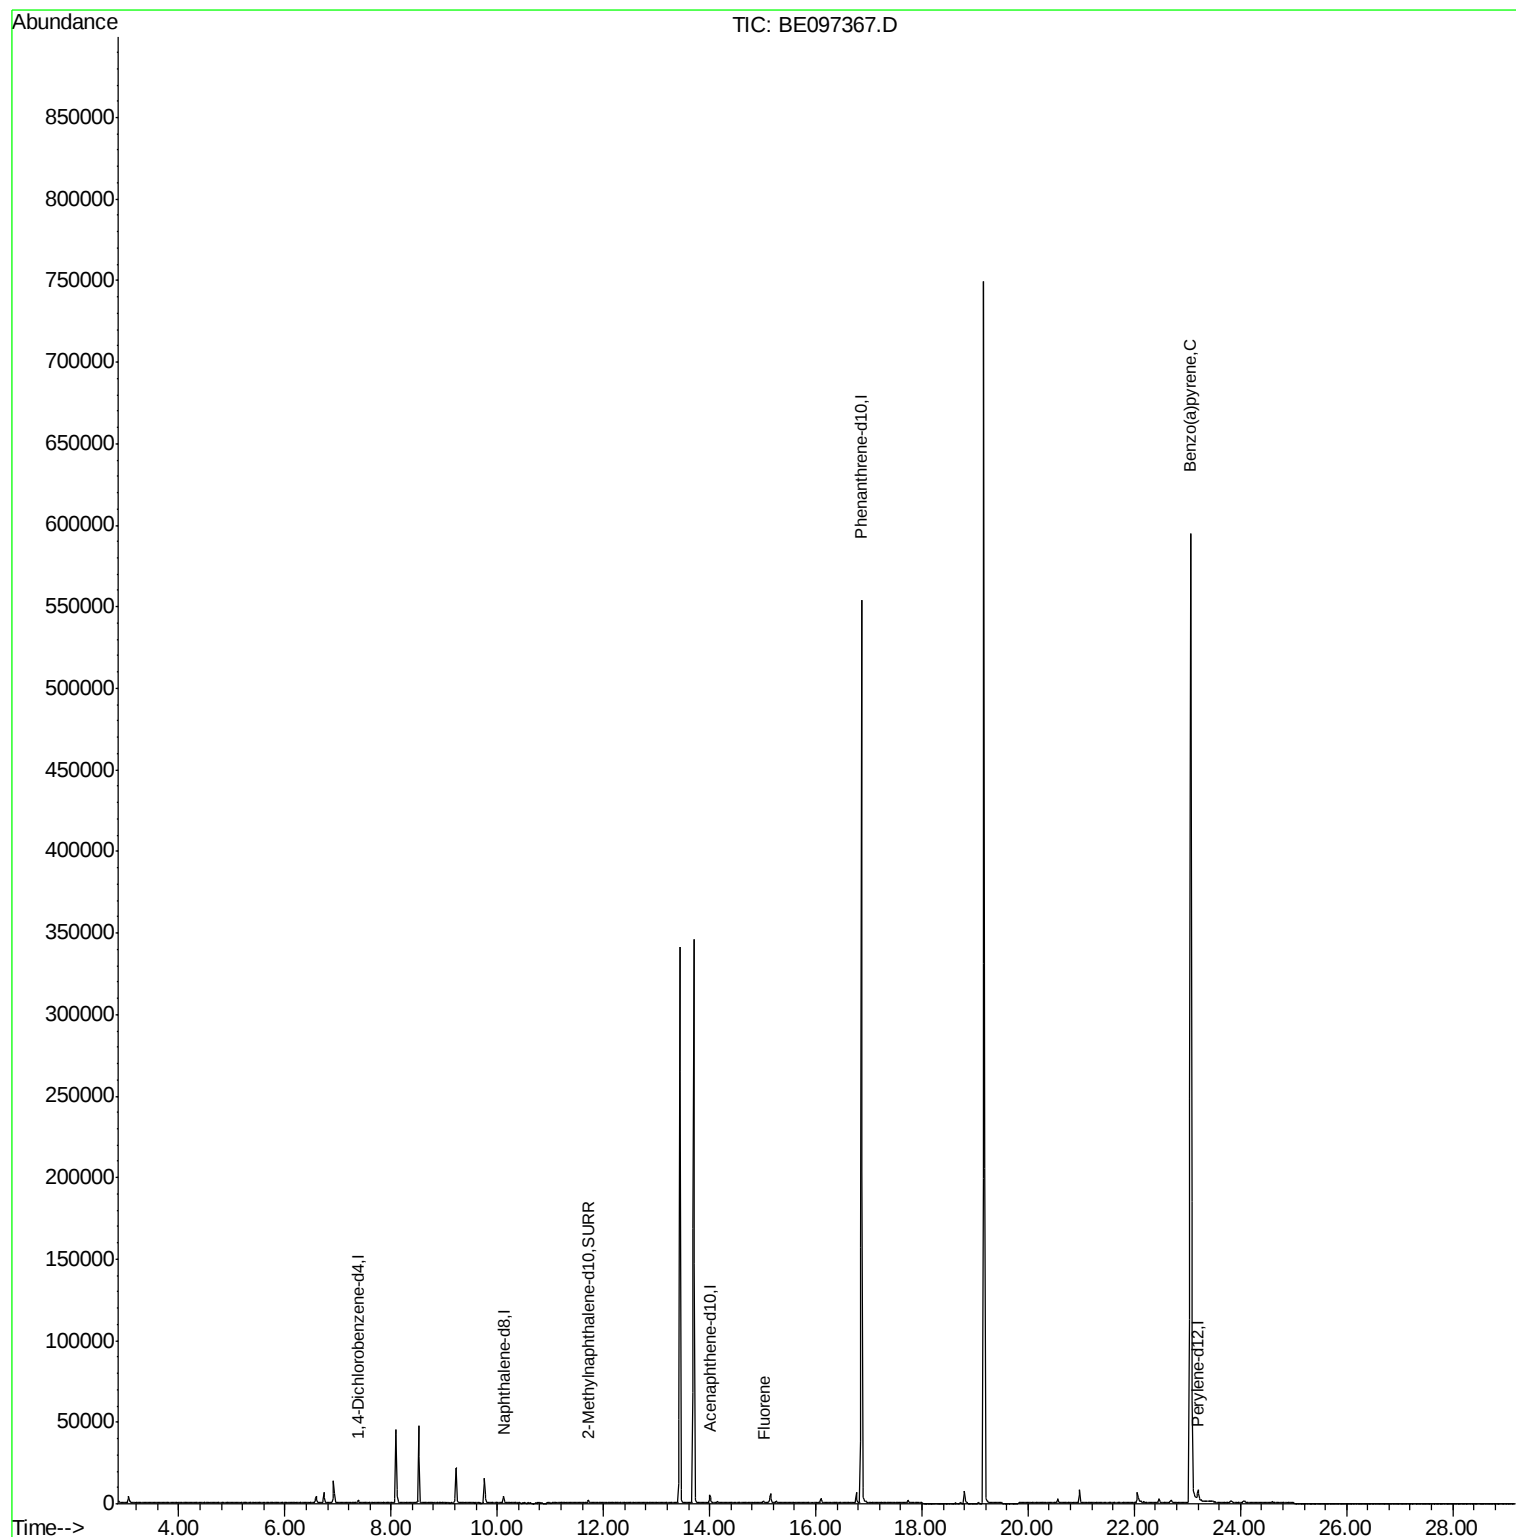

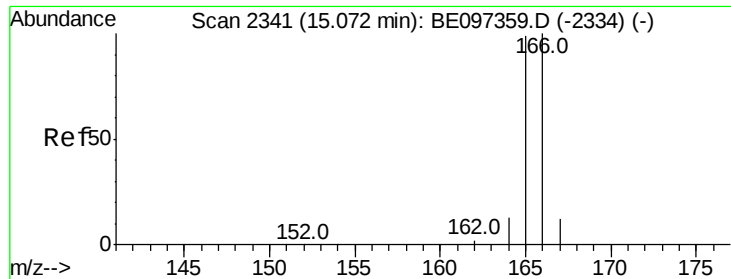

#9

Fluorene

Concen: 0.083 ng/ul

RT: 15.01 min Scan# 2331

Delta R.T. -0.06 min

Lab File: BE097367.D

Acq: 24 Aug 2018 13:59

Instrument :

BNA_E

ClientSampleId :





Tot Ion:166 Resp: 860

Ion Ratio Lower Upper

166 100

165 12.3 73.4 110.2#

167 35.9 14.6 22.0#

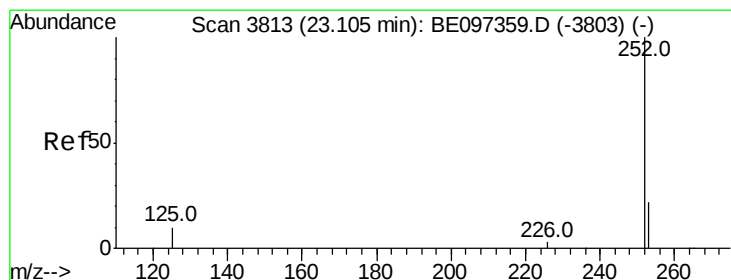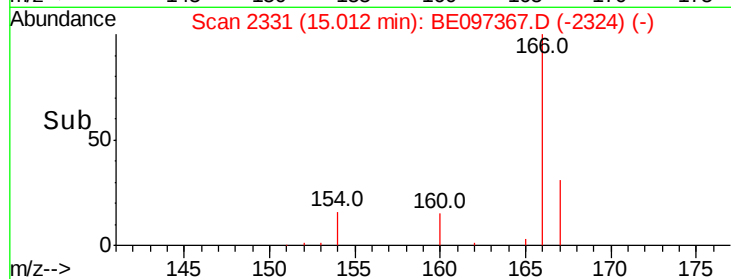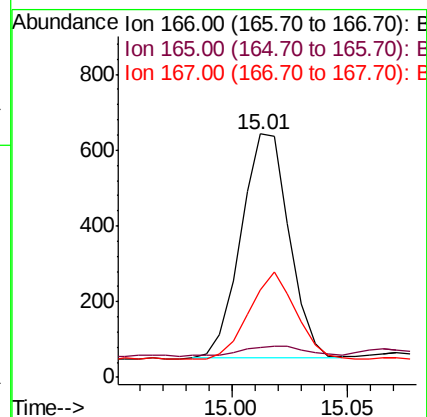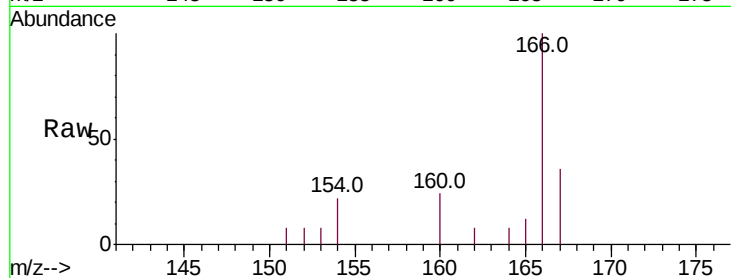

#23

Benzo(a)pyrene

Concen: 0.080 ng/ul

RT: 23.06 min Scan# 3807

Delta R.T. -0.04 min

Lab File: BE097367.D

Acq: 24 Aug 2018 13:59

Tgt Ion:252 Resp: 2685

Ion Ratio Lower Upper

252 100

253 35.8 28.5 42.7

125 22.9 18.1 27.1

