

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097361.D
 Acq On : 24 Aug 2018 10:15
 Operator : SJ/JU
 Sample : J4422-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB3

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:10:53 PM

Quant Time: Aug 24 23:09:24 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

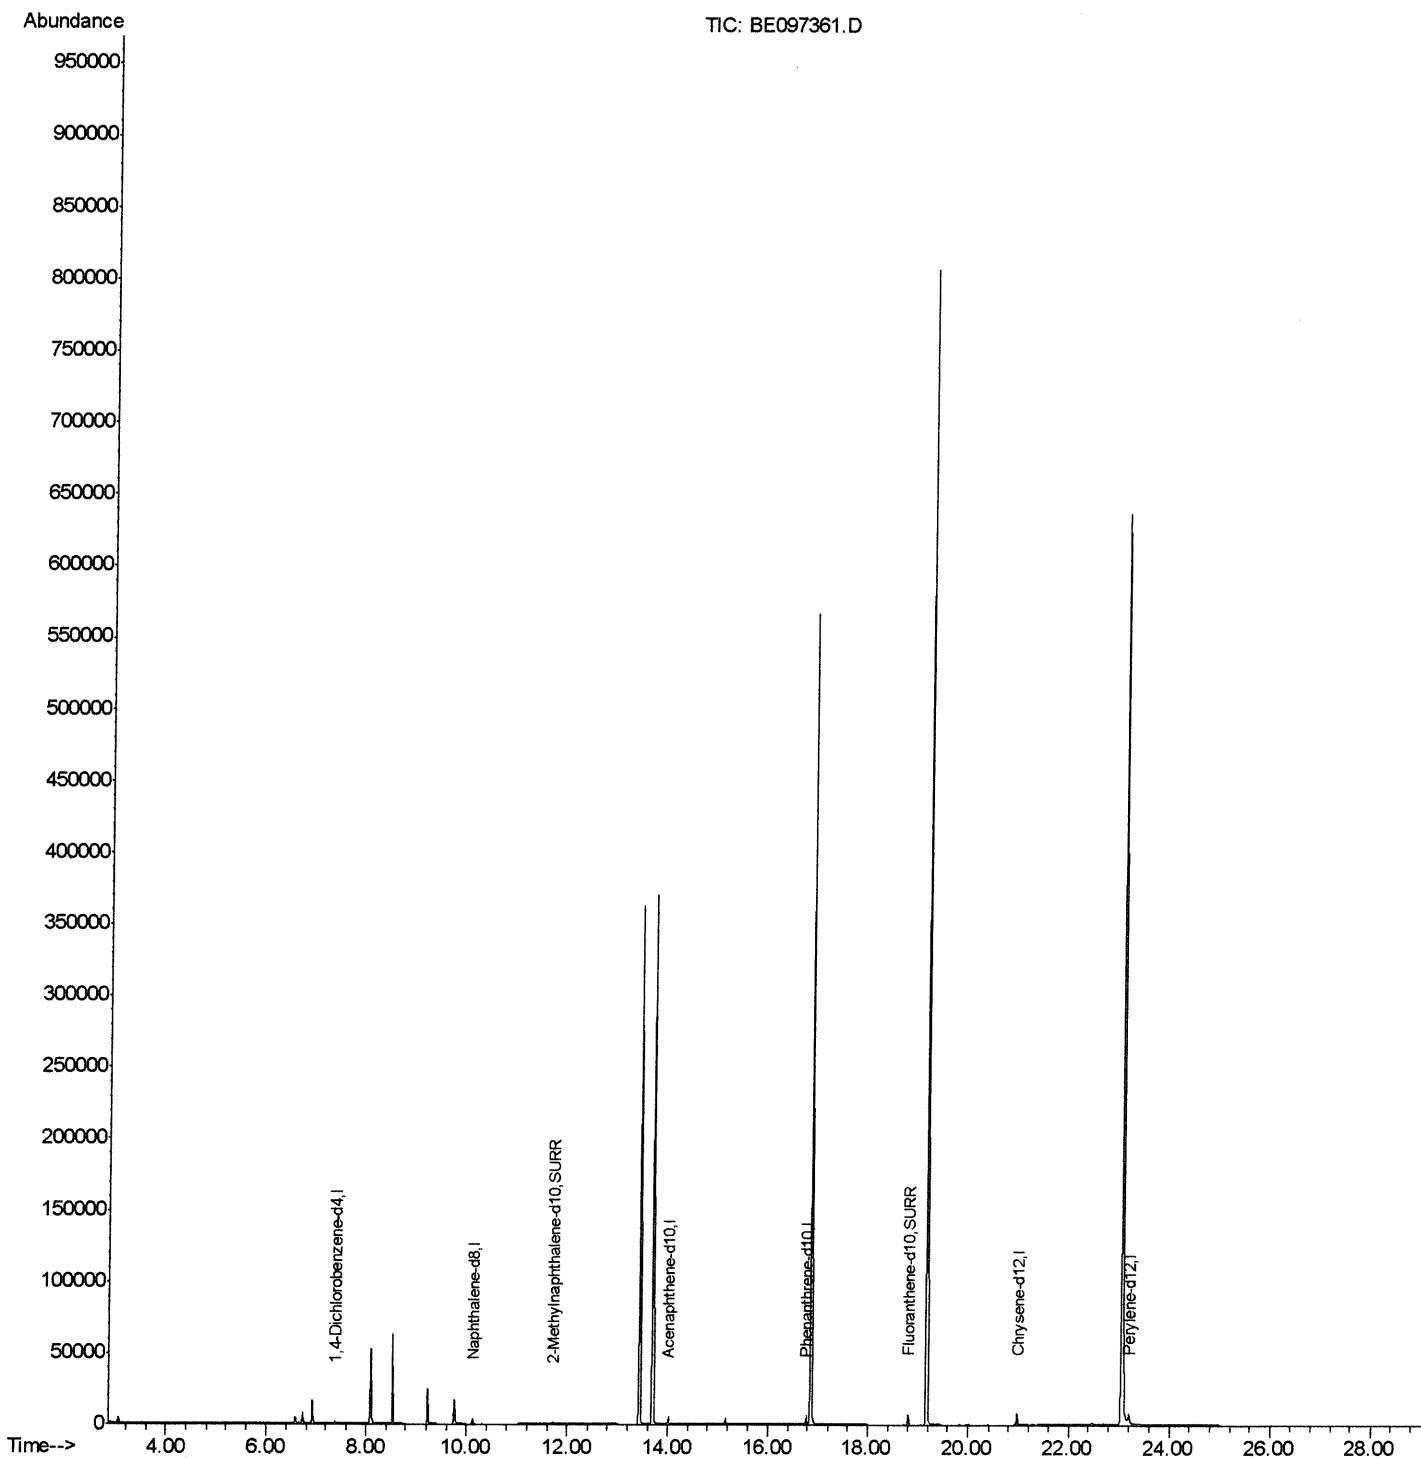

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097361.D
 Acq On : 24 Aug 2018 10:15
 Operator : SJ/JU
 Sample : J4422-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB3

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:10:53 PM

Quant Time: Aug 24 22:50:34 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

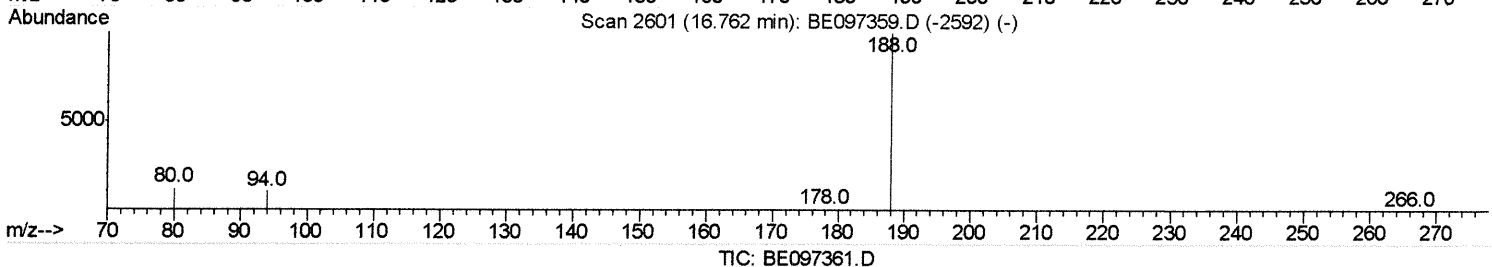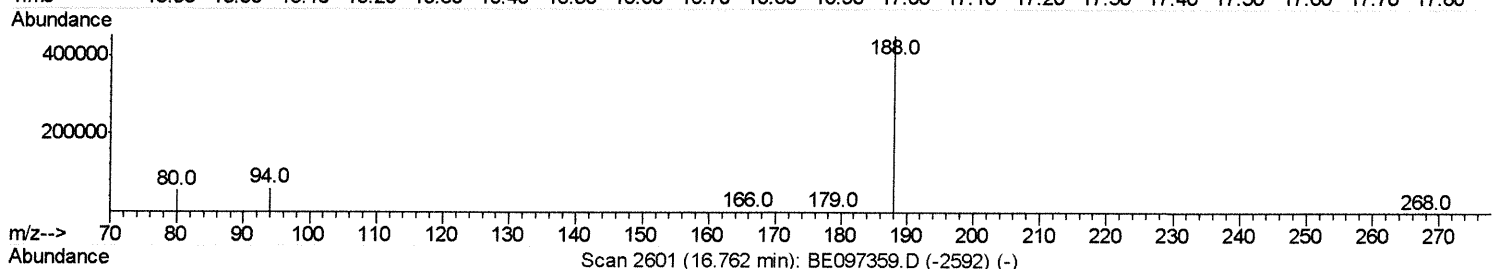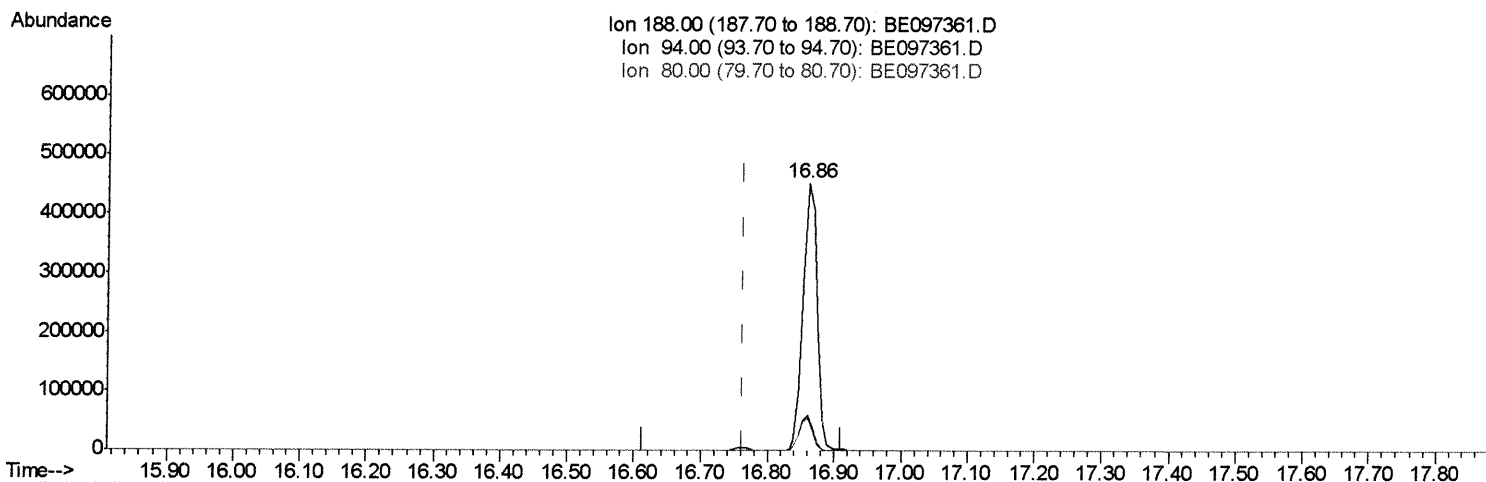

(10) Phenanthrene-d10 (I)

16.860min (+0.098) 0.40ng/ul

response 642210

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	13.21#
80.00	11.80	12.08
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097361.D
 Acq On : 24 Aug 2018 10:15
 Operator : SJ/JU
 Sample : J4422-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB3

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:10:53 PM

Quant Time: Aug 24 22:50:34 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

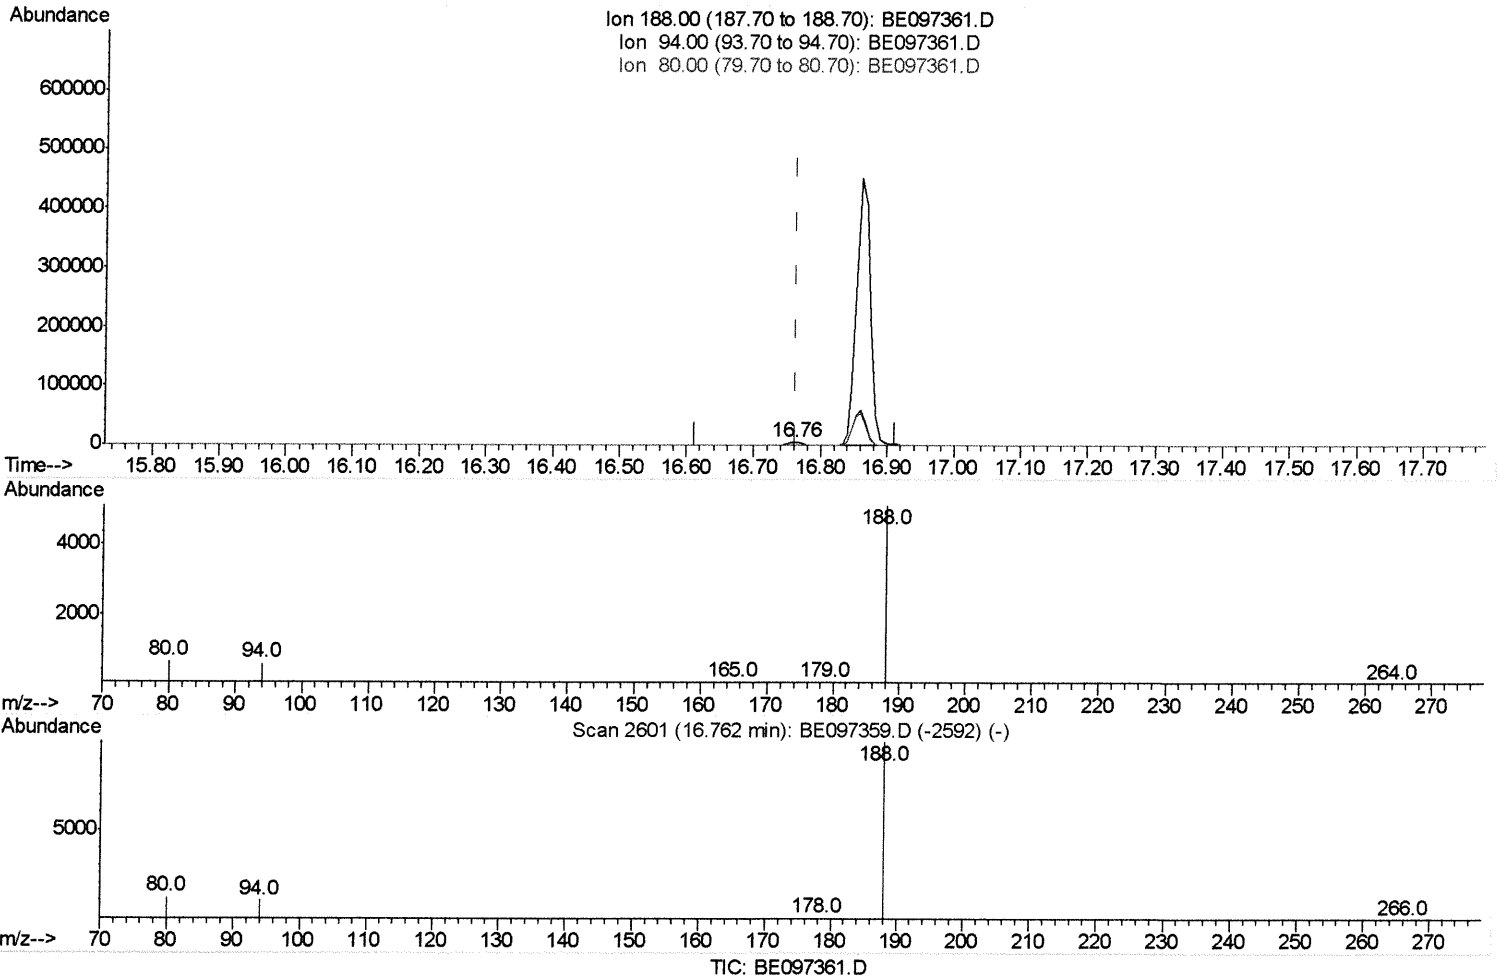

(10) Phenanthrene-d10 (I)

16.761min (-0.001) 0.40ng/ul m SJ 8/27/18

response 7277

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	11.31
80.00	11.80	12.52
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097361.D
 Acq On : 24 Aug 2018 10:15
 Operator : SJ/JU
 Sample : J4422-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB3

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:10:53 PM

Quant Time: Aug 24 23:07:15 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

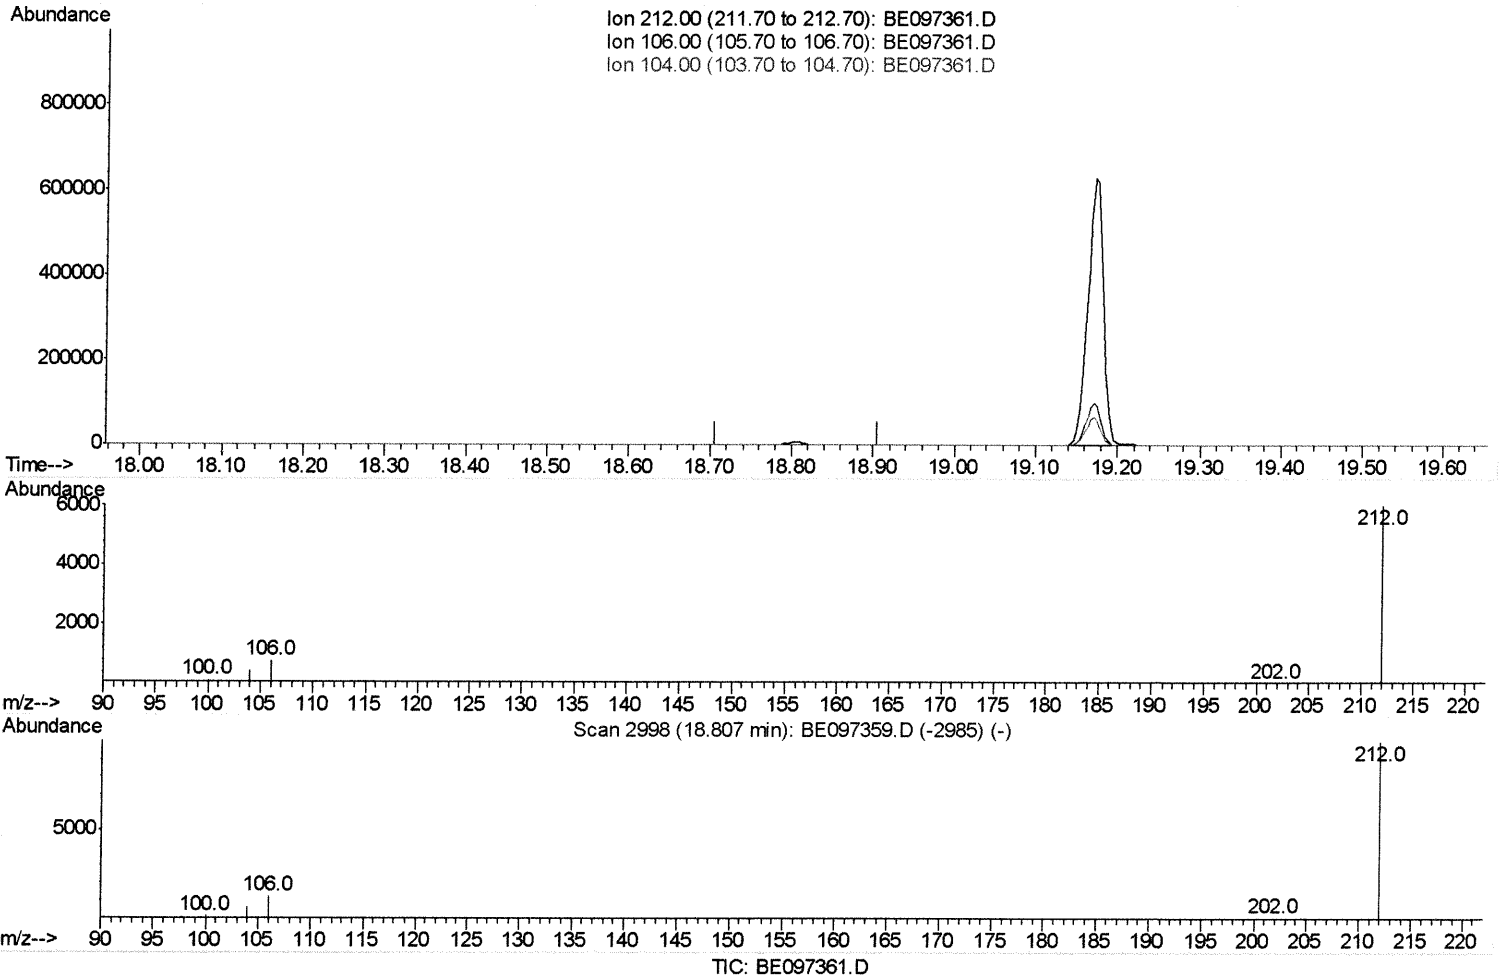

(14) Fluoranthene-d10 (SURR)

18.807min (-18.807) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097361.D
 Acq On : 24 Aug 2018 10:15
 Operator : SJ/JU
 Sample : J4422-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB3

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:10:53 PM

Quant Time: Aug 24 23:07:15 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

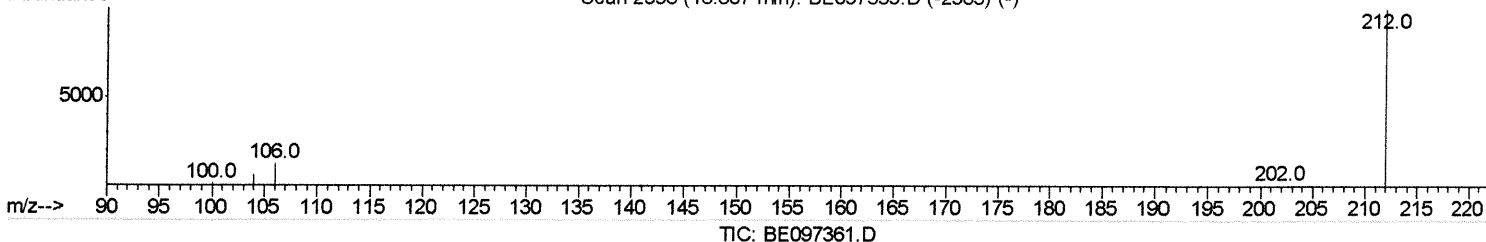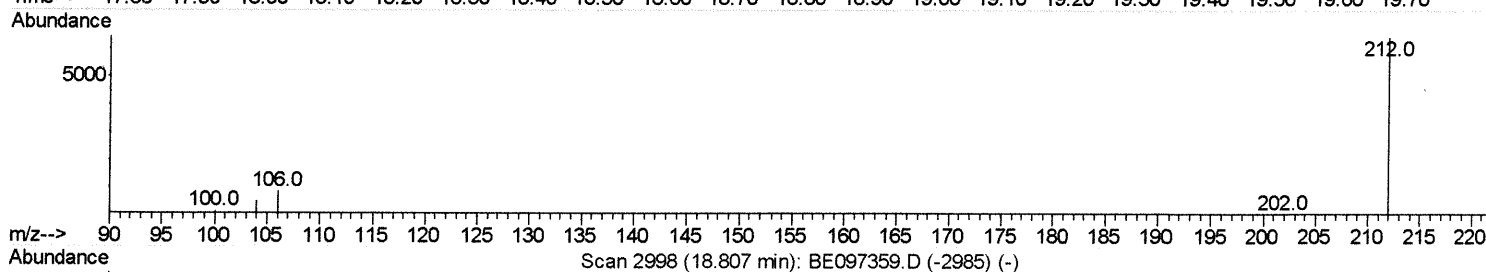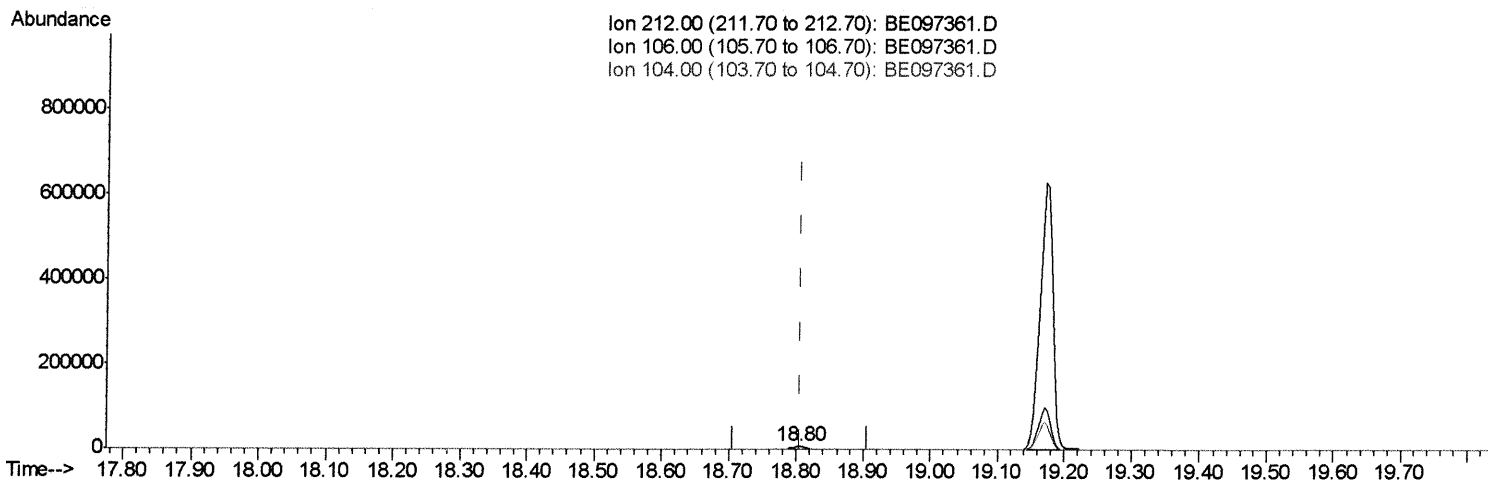

(14) Fluoranthene-d10 (SURR)

18.803min (-0.003) 0.45ng/ul m SJ 8/27/18

response 8760

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097361.D
 Acq On : 24 Aug 2018 10:15
 Operator : SJ/JU
 Sample : J4422-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB3

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:10:53 PM

Quant Time: Aug 24 23:07:15 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

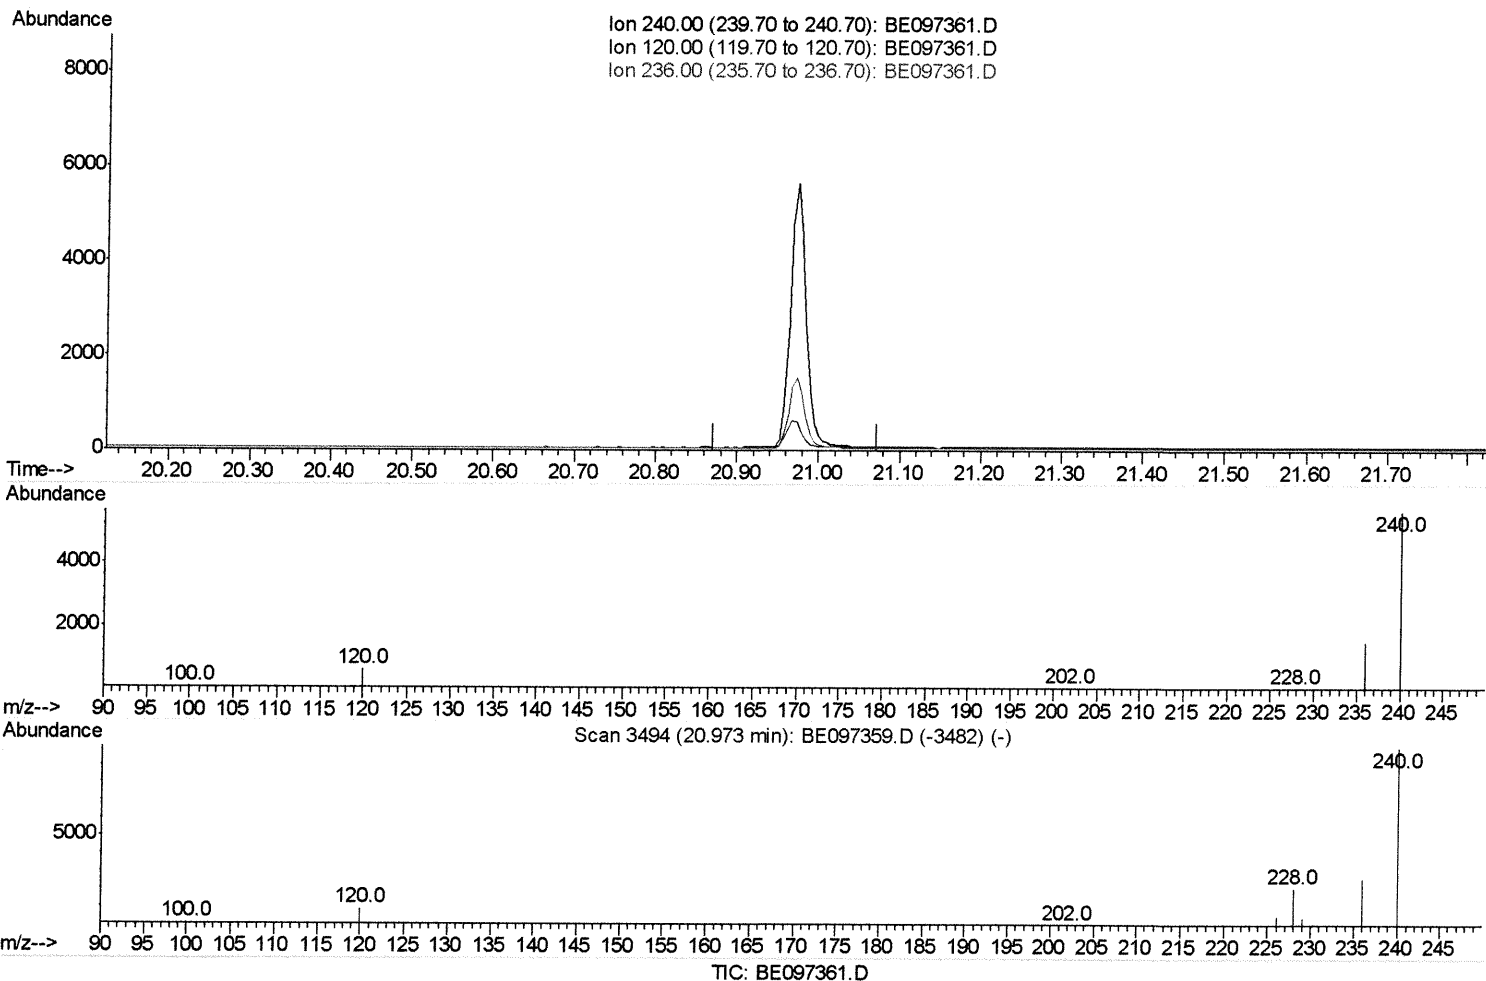

(16) Chrysene-d12 (I)

20.973min (-20.973) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.60	0.00#
236.00	34.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097361.D
 Acq On : 24 Aug 2018 10:15
 Operator : SJ/JU
 Sample : J4422-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampled :
 C0AB3

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:10:53 PM

Quant Time: Aug 24 23:07:15 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

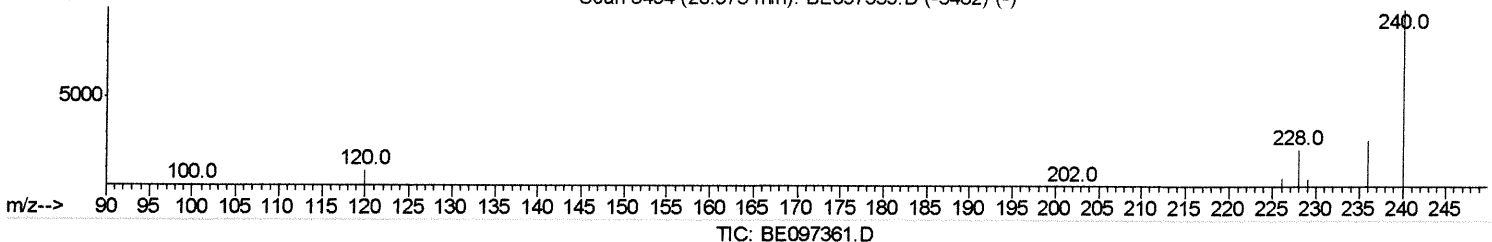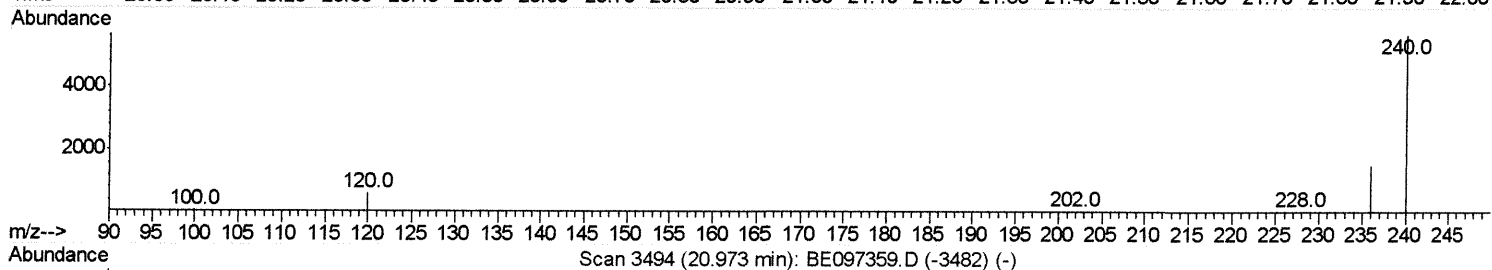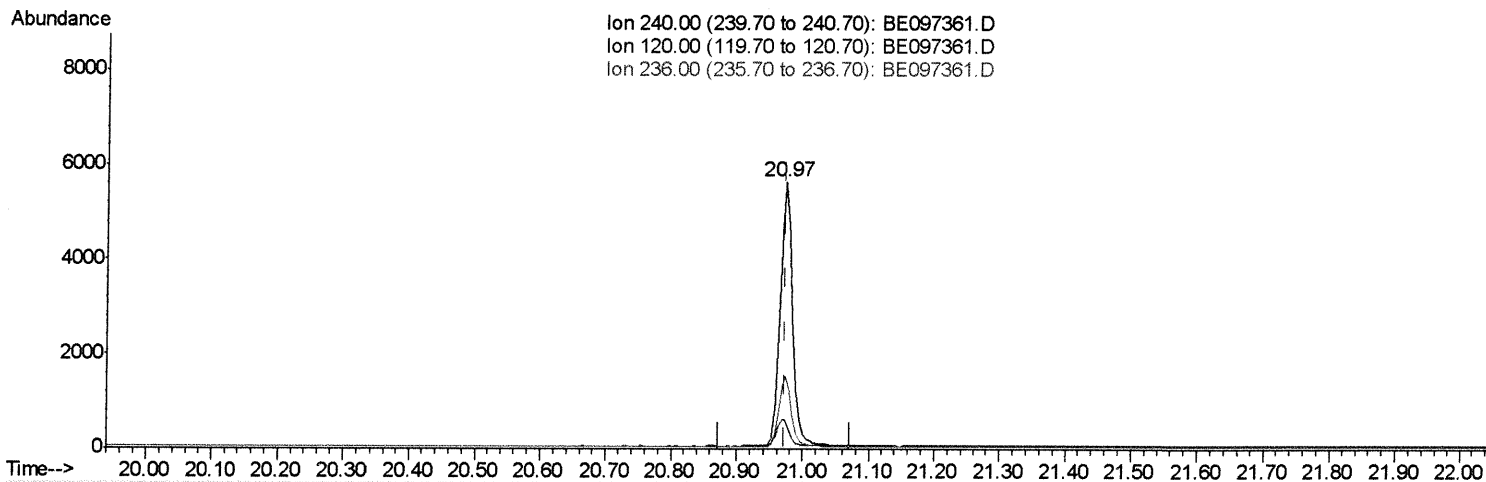

(16) Chrysene-d12 (I)

20.973min (-0.000) 0.40ng/ul m *SJ 8/27/18*

response 7489

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	10.81#
236.00	34.90	27.06#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097361.D
 Acq On : 24 Aug 2018 10:15
 Operator : SJ/JU
 Sample : J4422-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB3

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:10:53 PM

Quant Time: Aug 24 23:08:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

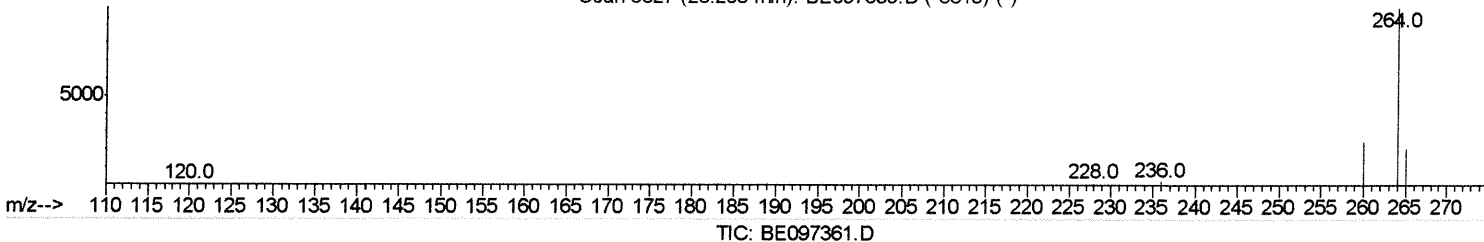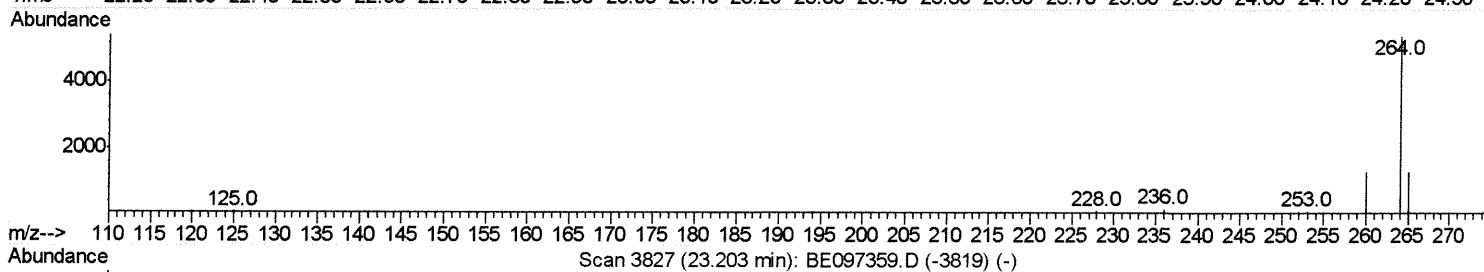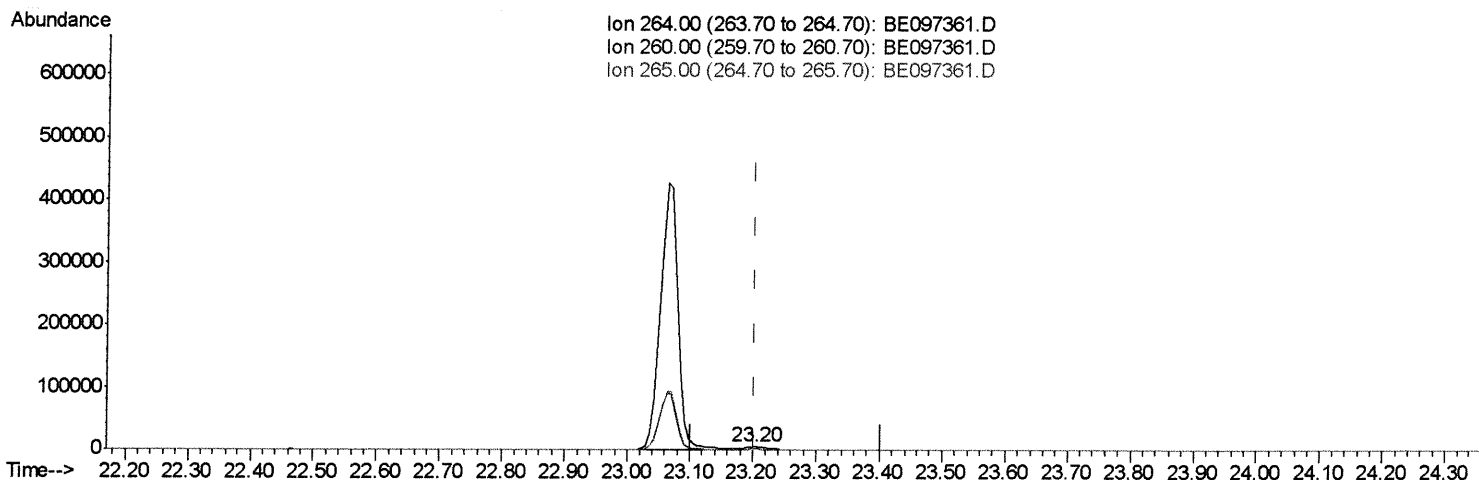

(20) Perylene-d12 (I)

23.204min (+0.001) 0.40ng/ul

response 13397

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.09
265.00	103.50	23.90#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097361.D
 Acq On : 24 Aug 2018 10:15
 Operator : SJ/JU
 Sample : J4422-02
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AB3

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:10:53 PM

Quant Time: Aug 24 23:08:26 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

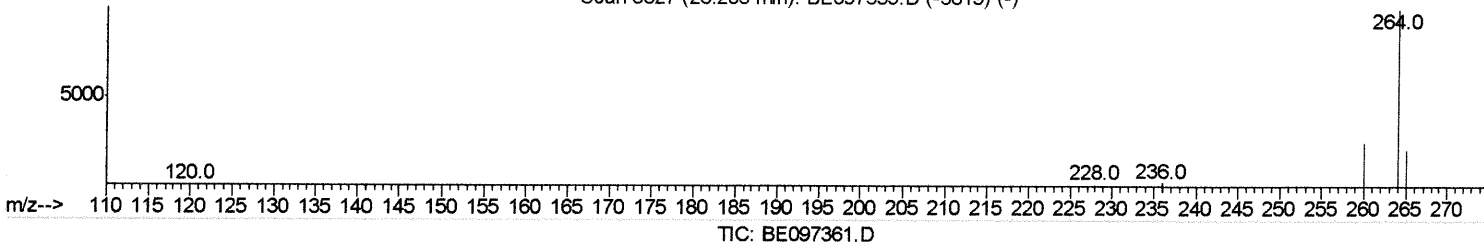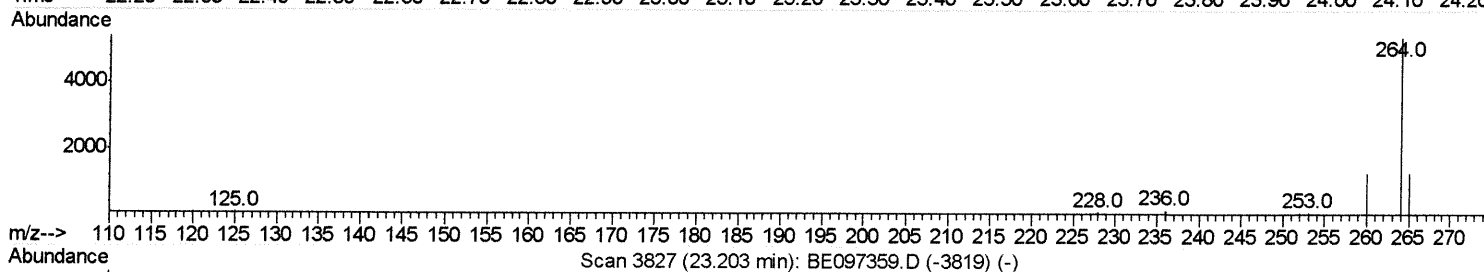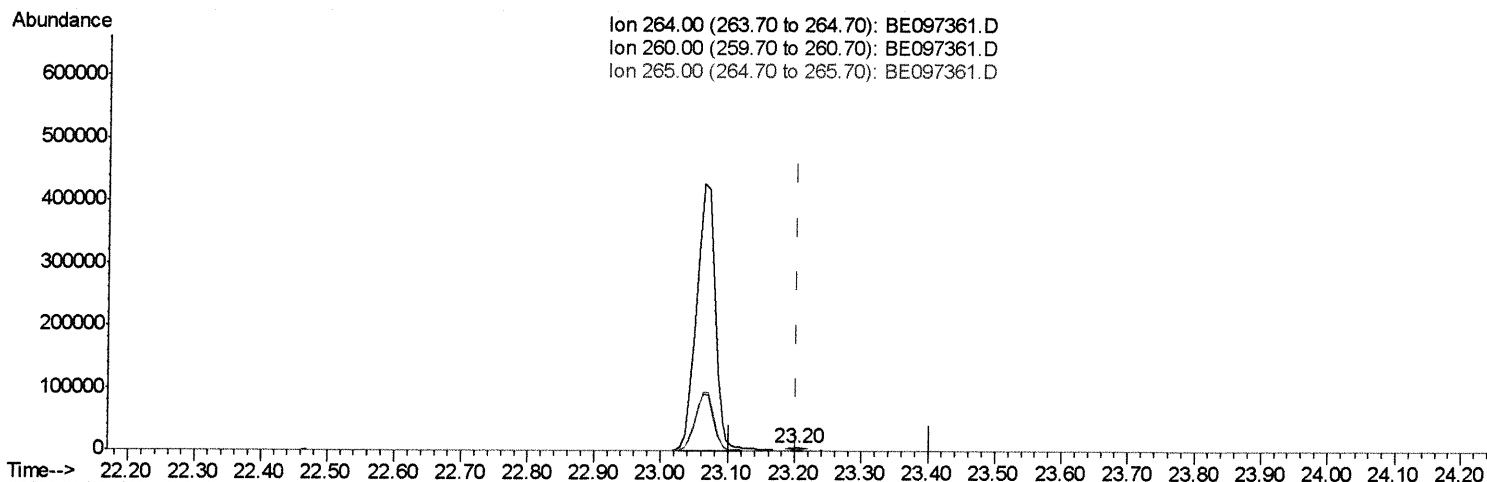

(20) Perylene-d12 (I)

23.204min (+0.001) 0.40ng/ul m SJ 8/27/18

response 6613

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.09
265.00	103.50	23.90#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Instrument :
BNA_E
ClientSampleId :
C0AB3

Manual Integrations
APPROVED

Sohil
8/27/2018 12:10:53 PM

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
Data File : BE097361.D
Acq On : 24 Aug 2018 10:15
Operator : SJ/JU
Sample : J4422-02
Misc :
ALS Vial : 4 Sample Multiplier: 1

Quant Time: Aug 24 23:09:24 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 24 22:49:42 2018
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	831	0.40	ng/ul	0.00
2) Naphthalene-d8	10.12	136	4311	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.01	164	2863	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.76	188	7277m	0.40	ng/ul	0.00
16) Chrysene-d12	20.97	240	7489m	0.40	ng/ul	0.00
20) Perylene-d12	23.20	264	6613m	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.72	152	2534	0.37	ng/ul	0.00
14) Fluoranthene-d10	18.80	212	8760m	0.45	ng/ul	0.00

Target Compounds

Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed