

Quantitation Report (QT Reviewed)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097367.D
 Acq On : 24 Aug 2018 13:59
 Operator : SJ/JU
 Sample : J4422-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC2

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:11:02 PM

Quant Time: Aug 24 23:59:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

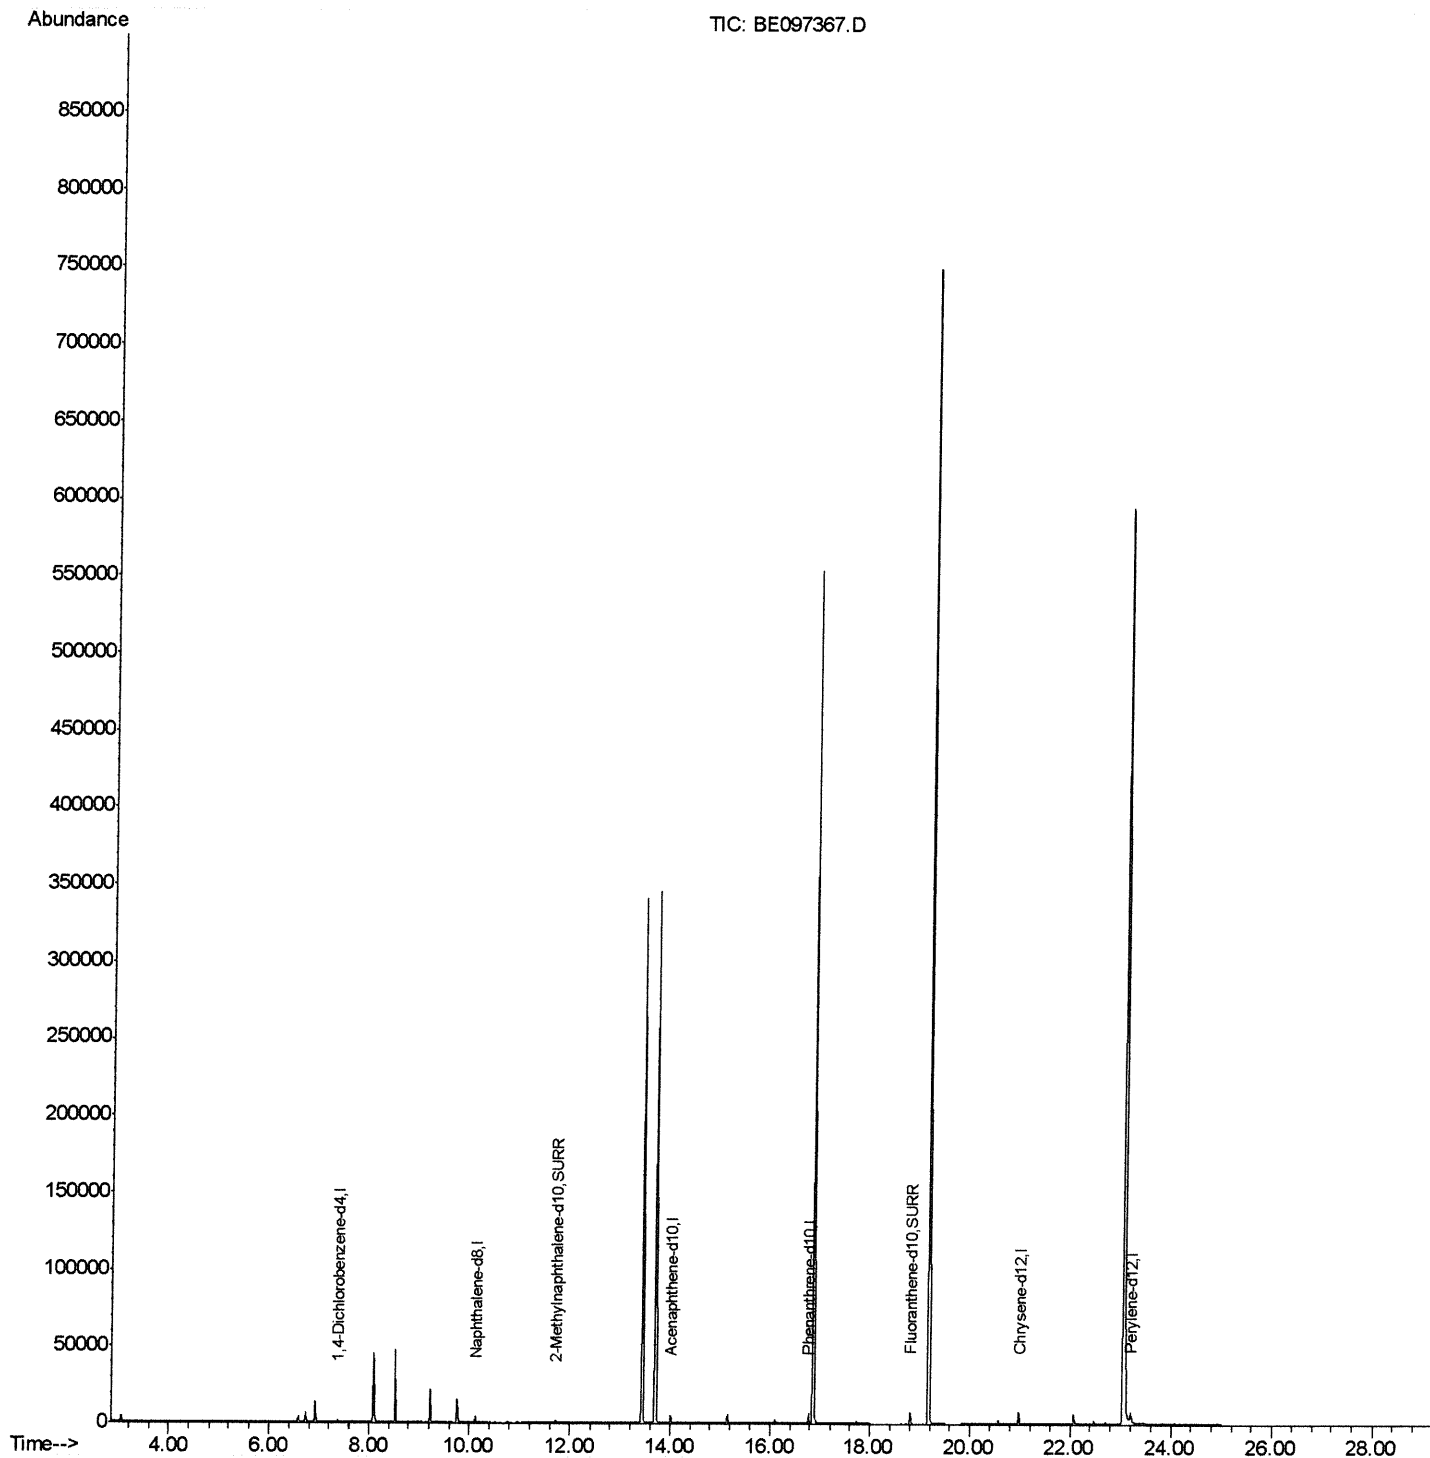

Quantitation Report (Qedit)


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097367.D
 Acq On : 24 Aug 2018 13:59
 Operator : SJ/JU
 Sample : J4422-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC2

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:11:02 PM

Quant Time: Aug 24 22:50:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

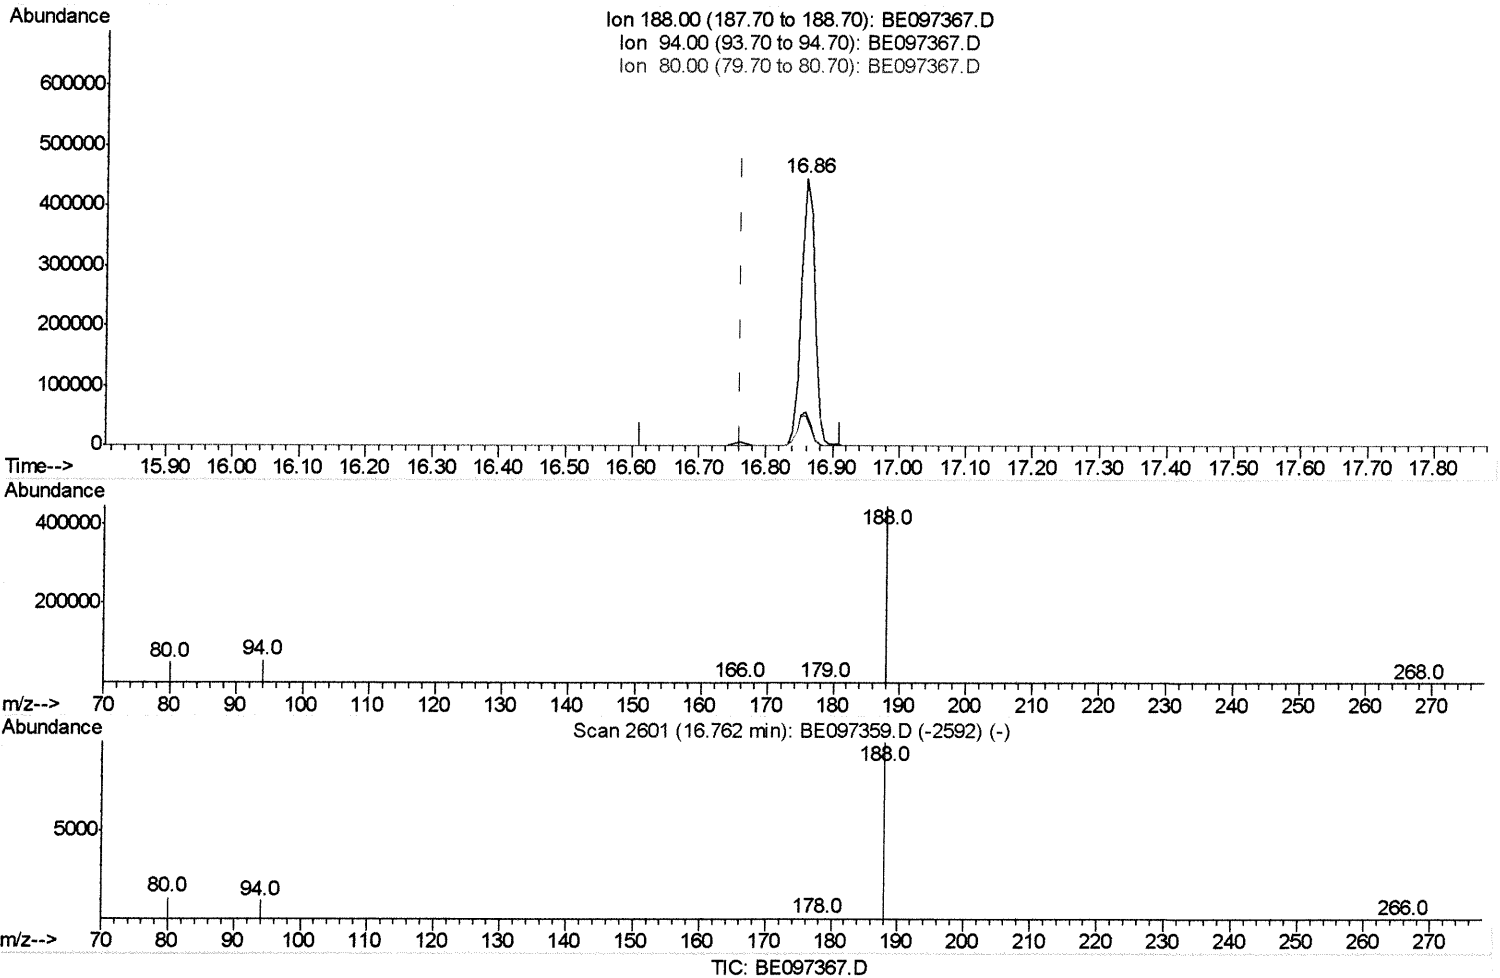

(10) Phenanthrene-d10 (I)

16.860min (+0.098) 0.40ng/ul

response 622249

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	12.67
80.00	11.80	11.53
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097367.D
 Acq On : 24 Aug 2018 13:59
 Operator : SJ/JU
 Sample : J4422-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC2

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:11:02 PM

Quant Time: Aug 24 22:50:57 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

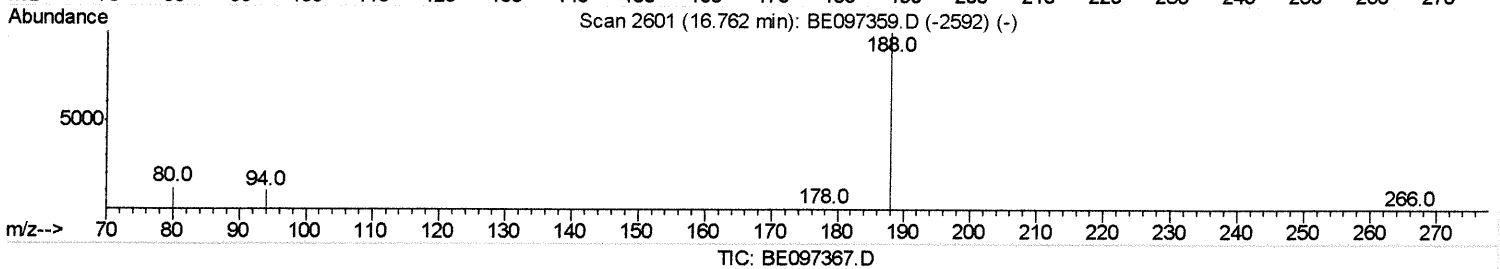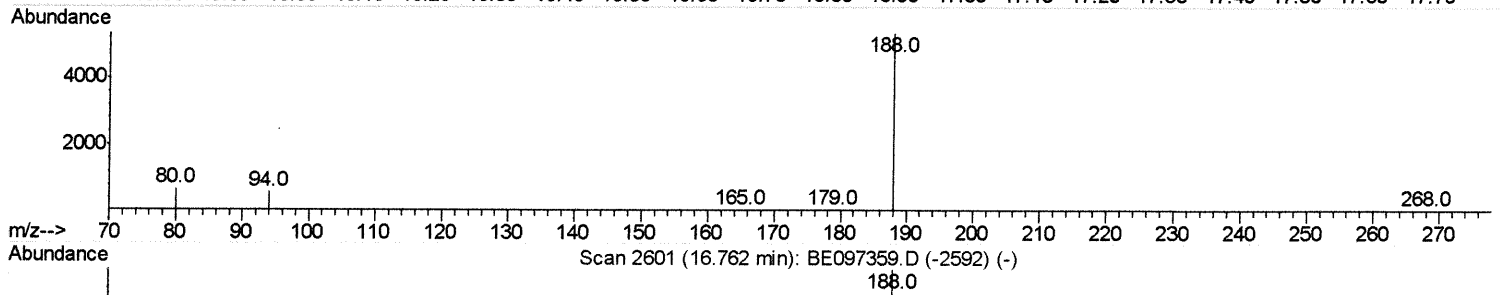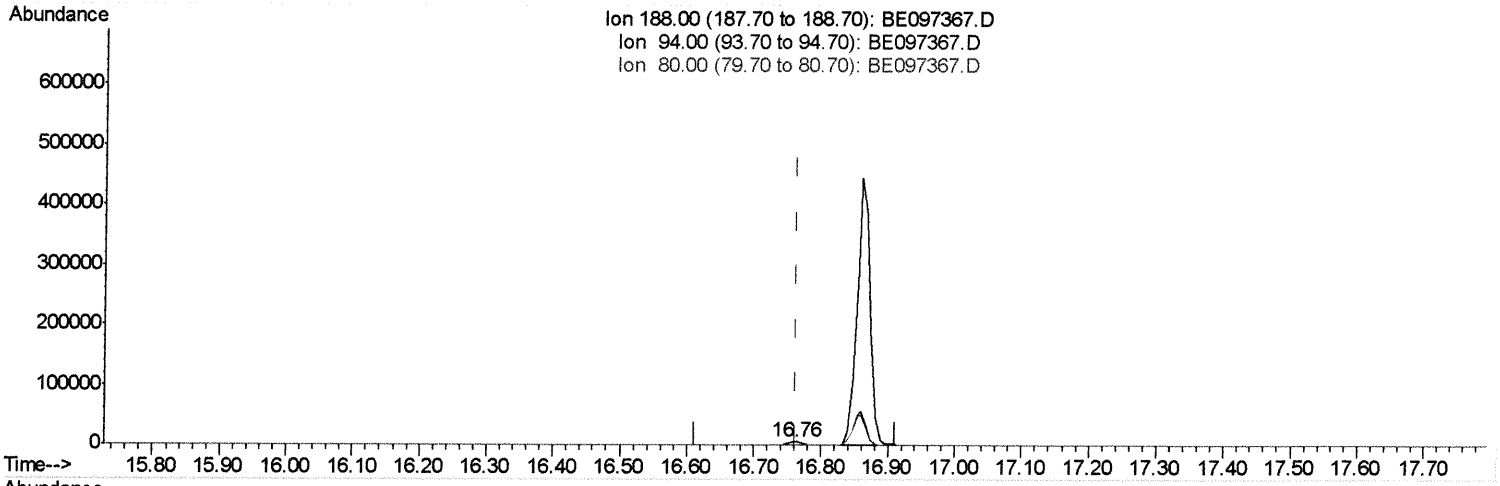

(10) Phenanthrene-d10 (I)

16.761min (-0.001) 0.40ng/ul m

SJ 8/27/18

response 7714

Ion	Exp%	Act%
188.00	100	100
94.00	11.00	10.75
80.00	11.80	12.43
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097367.D
 Acq On : 24 Aug 2018 13:59
 Operator : SJ/JU
 Sample : J4422-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC2

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:11:02 PM

Quant Time: Aug 24 23:55:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

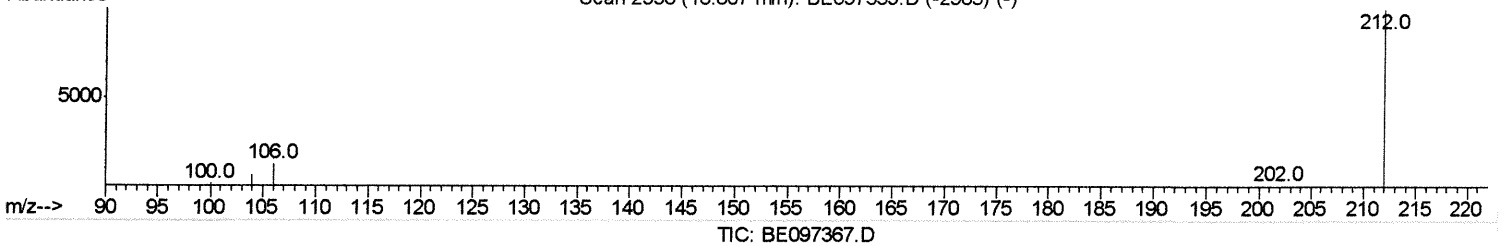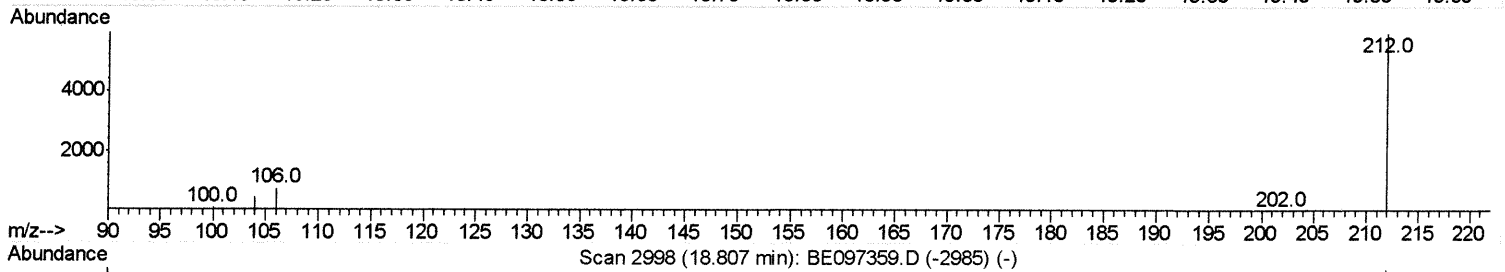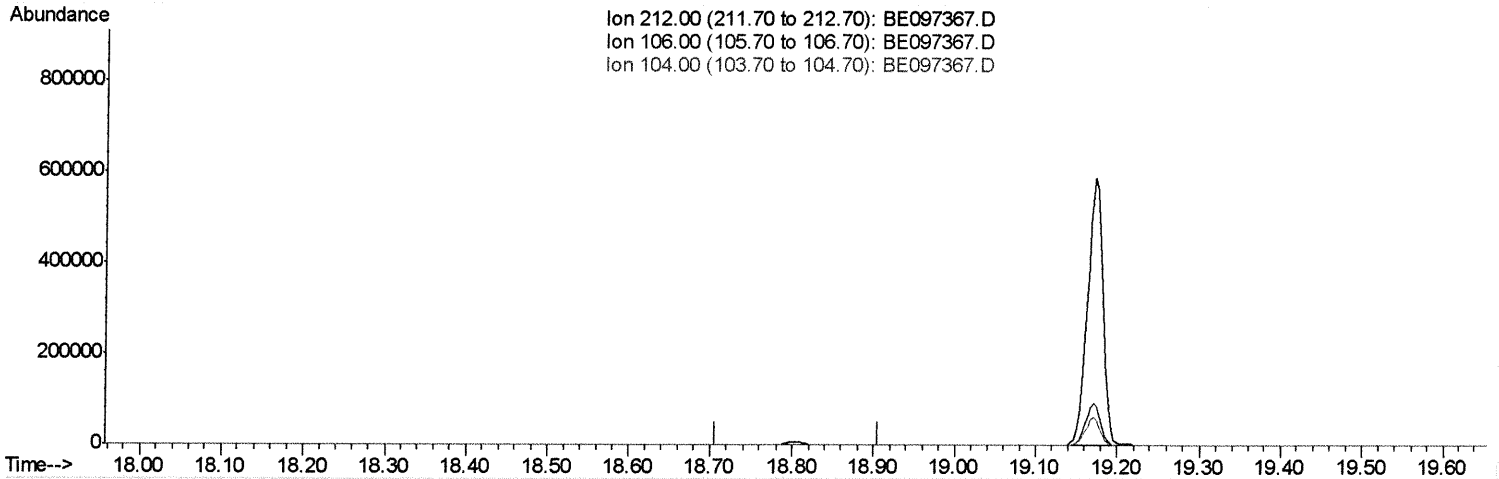

(14) Fluoranthene-d10 (SURR)

18.807min (-18.807) 0.00ng/ul

response 0

Ion	Exp%	Act%
212.00	100	0.00
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097367.D
 Acq On : 24 Aug 2018 13:59
 Operator : SJ/JU
 Sample : J4422-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC2

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:11:02 PM

Quant Time: Aug 24 23:55:30 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

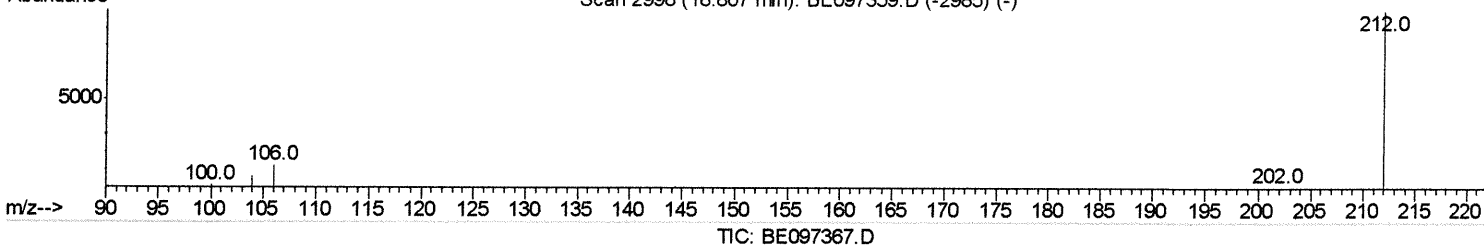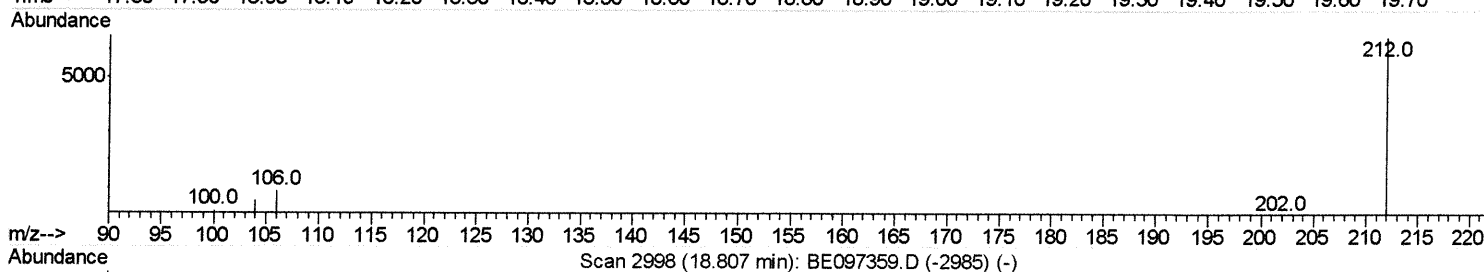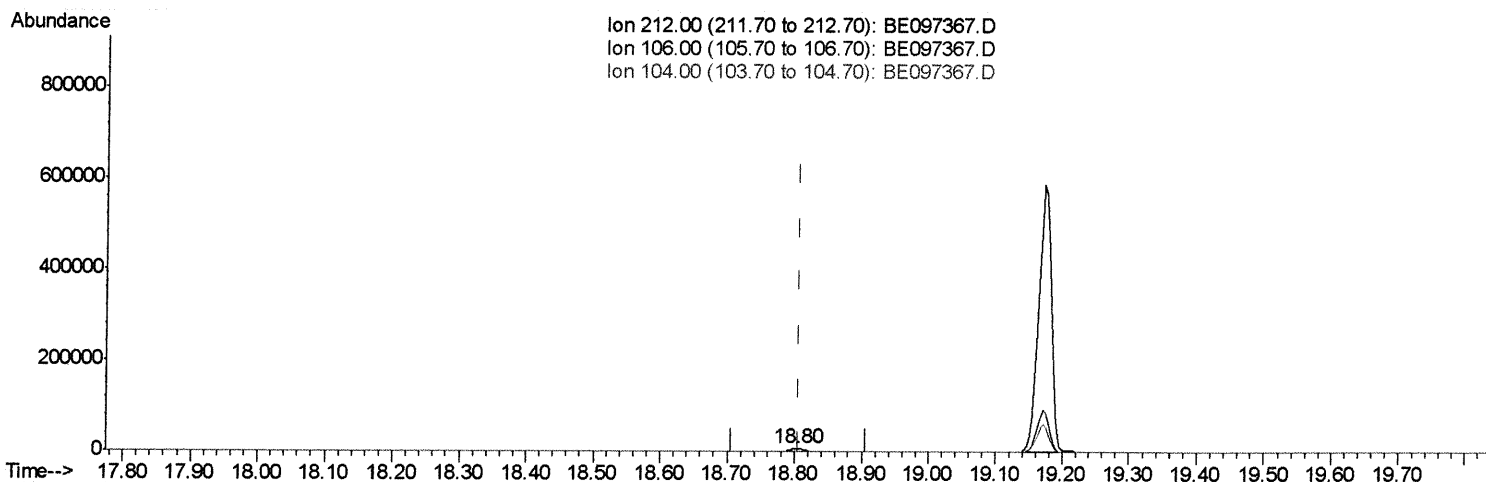

(14) Fluoranthene-d10 (SURR)

18.803min (-0.004) 0.43ng/ul m

SJ 8/27/18

response 8873

Ion	Exp%	Act%
212.00	100	100
106.00	18.30	0.00#
104.00	15.60	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097367.D
 Acq On : 24 Aug 2018 13:59
 Operator : SJ/JU
 Sample : J4422-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC2

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:11:02 PM

Quant Time: Aug 24 23:56:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

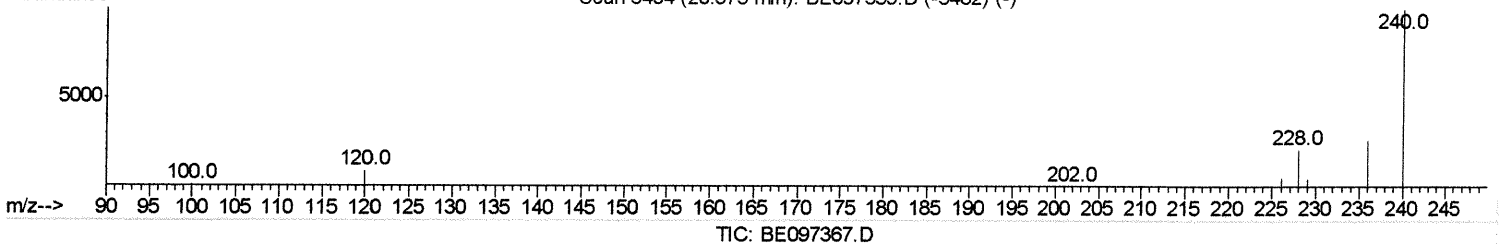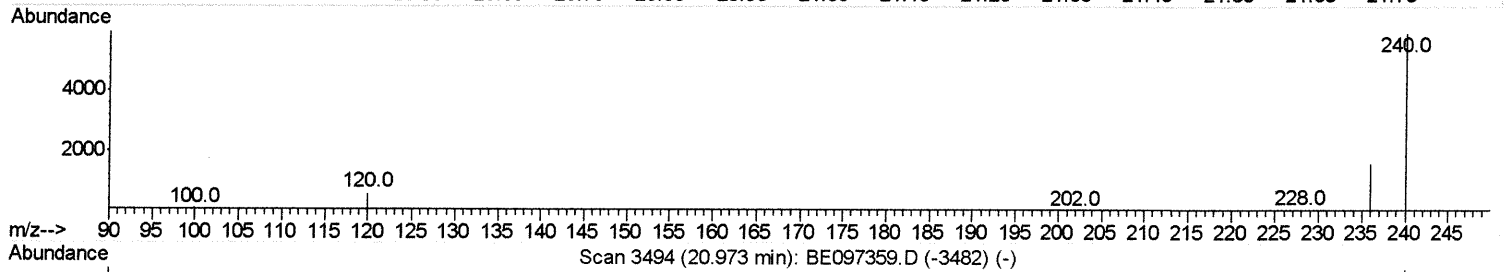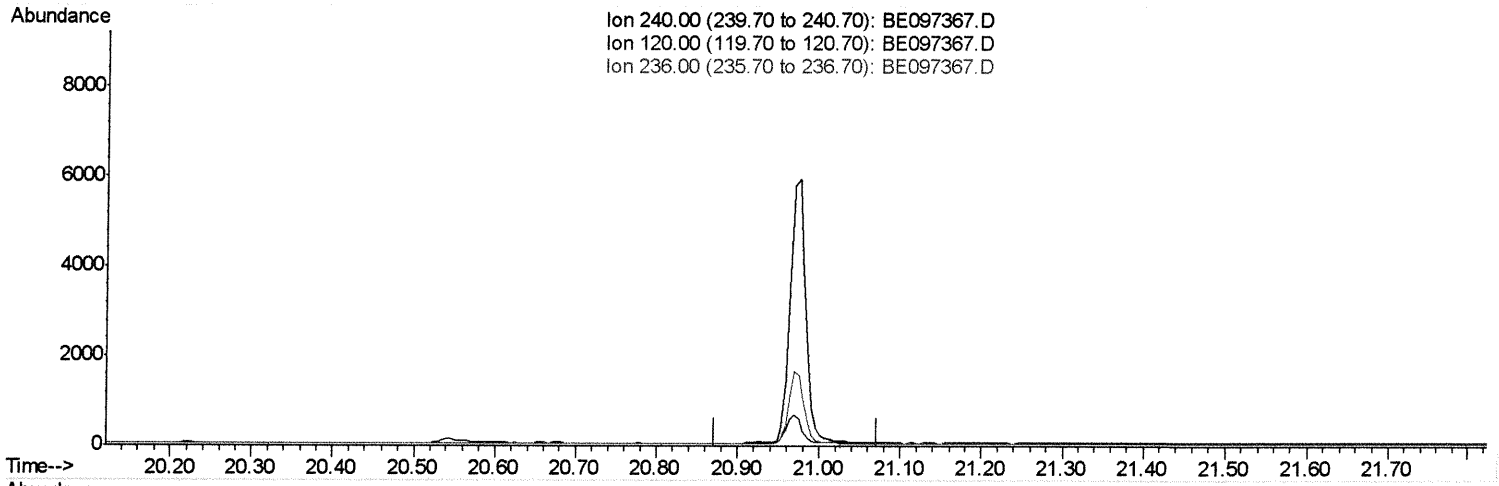

(16) Chrysene-d12 (I)

20.973min (-20.973) 0.00ng/ul

response 0

Ion	Exp%	Act%
240.00	100	0.00
120.00	20.60	0.00#
236.00	34.90	0.00#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097367.D
 Acq On : 24 Aug 2018 13:59
 Operator : SJ/JU
 Sample : J4422-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC2

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:11:02 PM

Quant Time: Aug 24 23:56:10 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

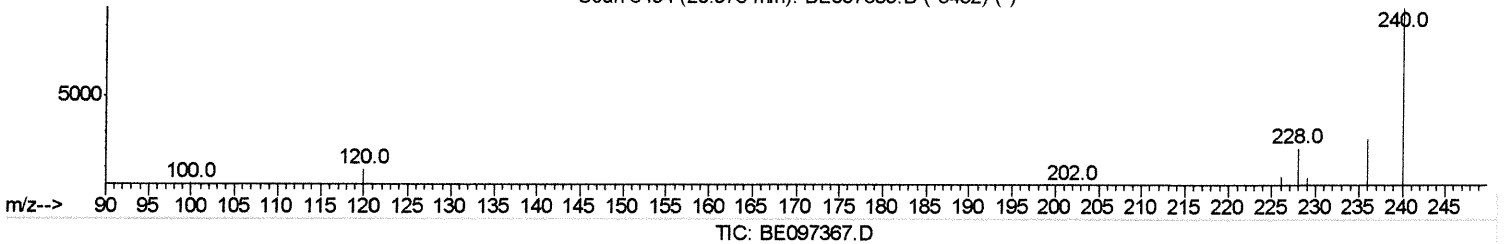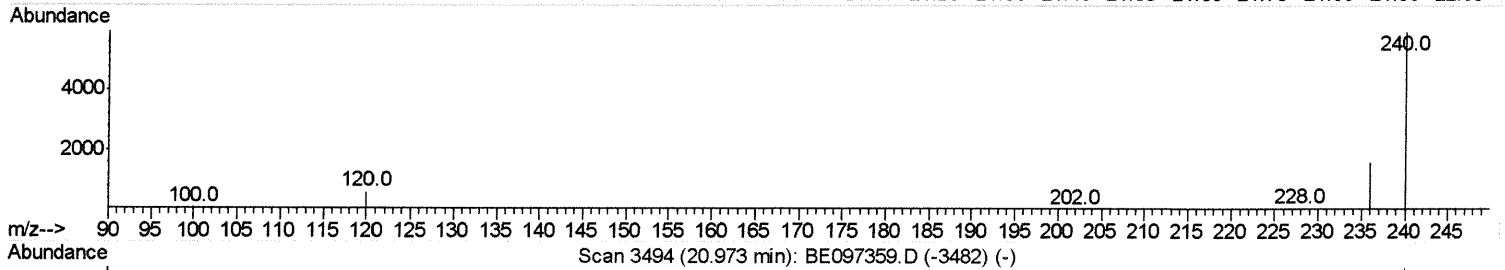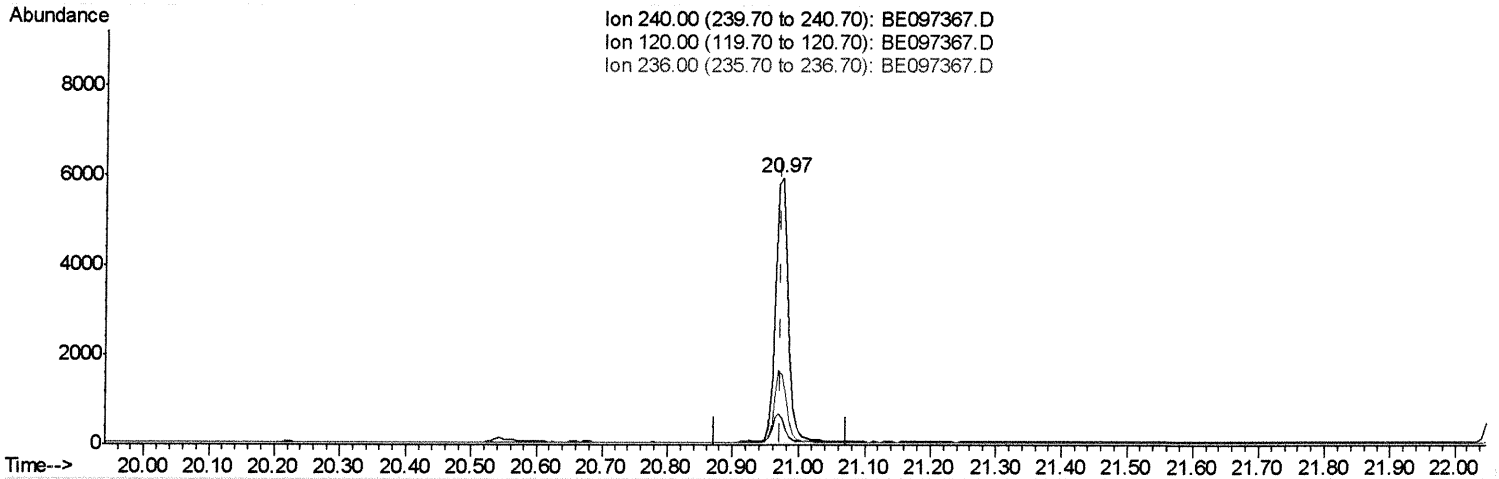

(16) Chrysene-d12 (I)

20.974min (+0.001) 0.40ng/ul m

SJ 8/27/18

response 7881

Ion	Exp%	Act%
240.00	100	100
120.00	20.60	9.80#
236.00	34.90	26.48#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097367.D
 Acq On : 24 Aug 2018 13:59
 Operator : SJ/JU
 Sample : J4422-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC2

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:11:02 PM

Quant Time: Aug 24 23:57:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

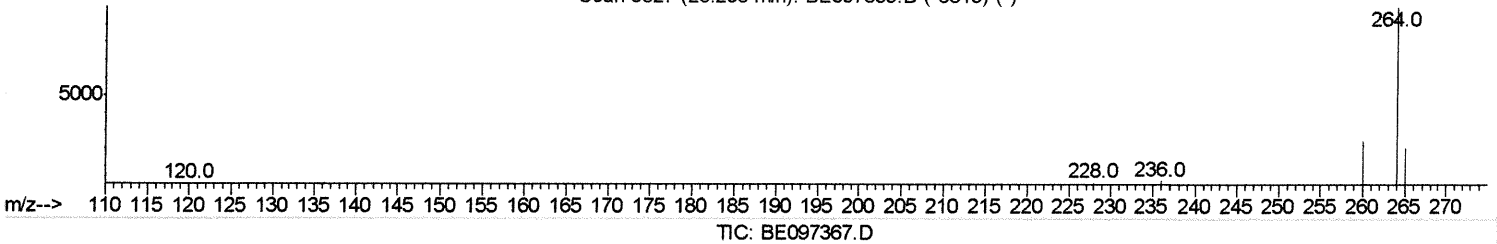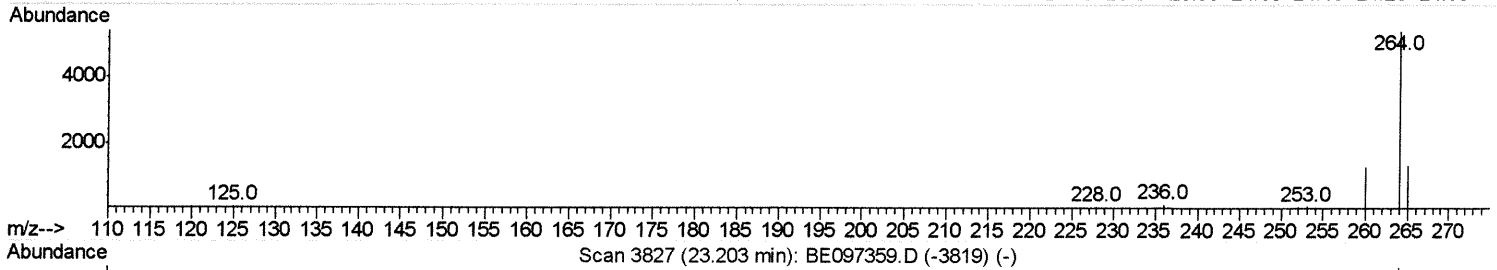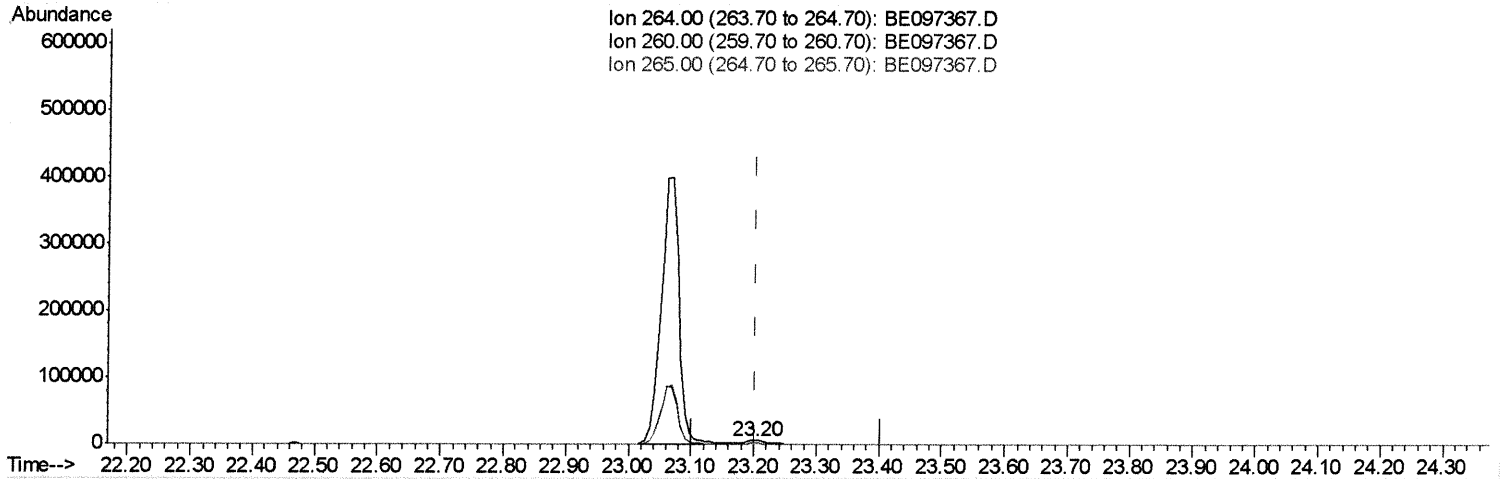

(20) Perylene-d12 (I)

23.202min (-0.001) 0.40ng/ul

response 13363

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.31
265.00	103.50	24.63#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097367.D
 Acq On : 24 Aug 2018 13:59
 Operator : SJ/JU
 Sample : J4422-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC2

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:11:02 PM

Quant Time: Aug 24 23:57:18 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

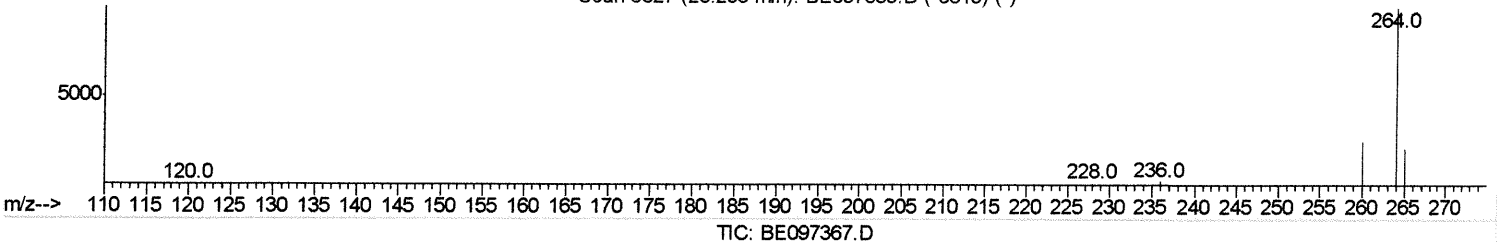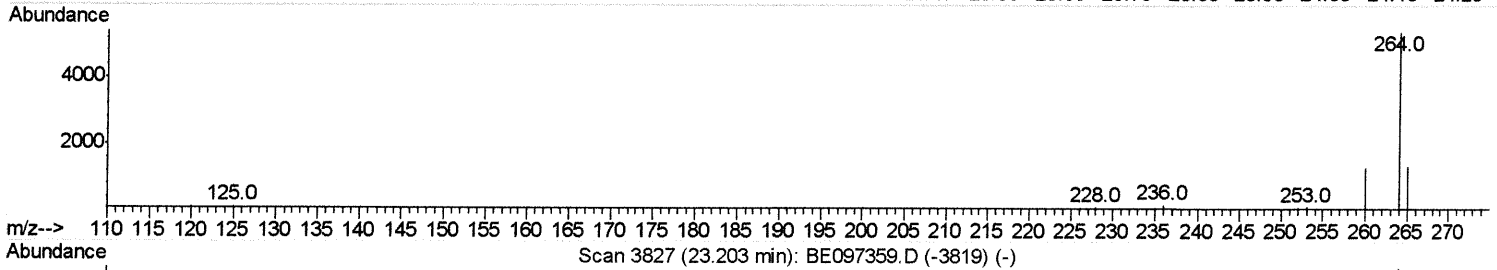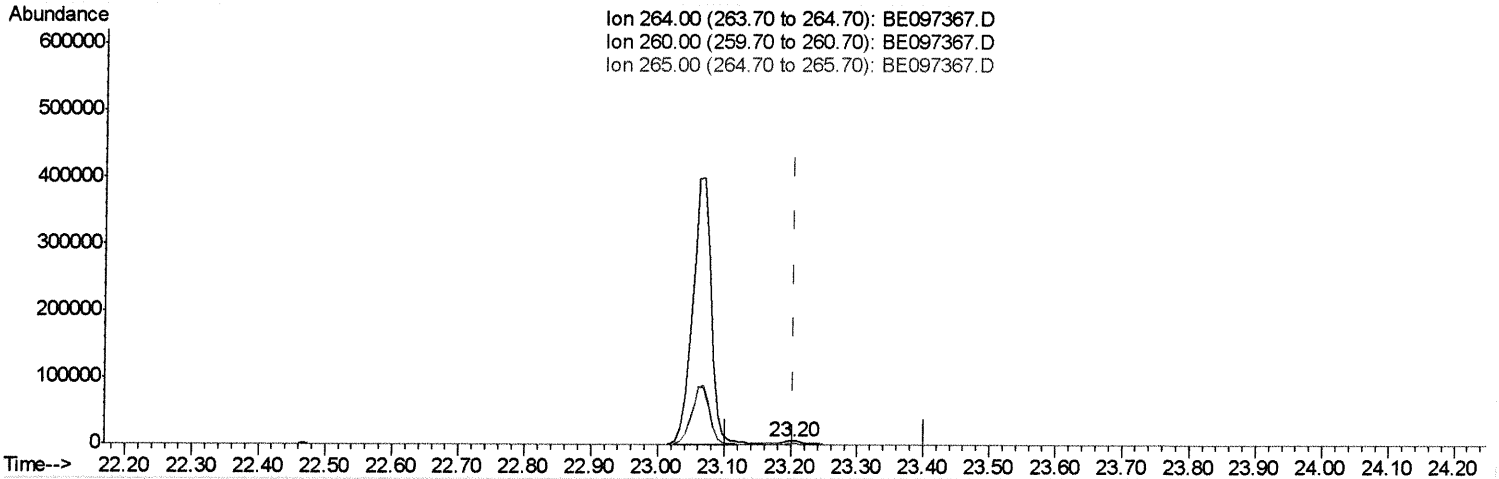

(20) Perylene-d12 (I)

23.202min (-0.001) 0.40ng/ul m

318/27/18

response 7341

Ion	Exp%	Act%
264.00	100	100
260.00	30.10	24.31
265.00	103.50	24.63#
0.00	0.00	0.00

Quantitation Report (QT Reviewed)

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097367.D
 Acq On : 24 Aug 2018 13:59
 Operator : SJ/JU
 Sample : J4422-06
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AC2

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:11:02 PM

Quant Time: Aug 24 23:59:50 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	834	0.40	ng/ul	0.00
2) Naphthalene-d8	10.12	136	4326	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.01	164	2916	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.76	188	7714m	0.40	ng/ul	0.00
16) Chrysene-d12	20.97	240	7881m	0.40	ng/ul	0.00
20) Perylene-d12	23.20	264	7341m	0.40	ng/ul	0.00

System Monitoring Compounds

4) 2-Methylnaphthalene-d10	11.72	152	2347	0.34	ng/ul	0.00
14) Fluoranthene-d10	18.80	212	8873m	0.43	ng/ul	0.00

Target Compounds Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed