

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
 Data File : BE097365.D
 Acq On : 24 Aug 2018 12:44
 Operator : SJ/JU
 Sample : J4422-12
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 C0AD4

Manual Integrations
 APPROVED

Sohil
 8/27/2018 12:10:59 PM

Quant Time: Aug 24 23:46:54 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Aug 24 22:49:42 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.38	152	849	0.40	ng/ul	0.00
2) Naphthalene-d8	10.12	136	4290	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.01	164	2863	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.76	188	7368m	0.40	ng/ul	0.00
16) Chrysene-d12	20.97	240	7395m	0.40	ng/ul	0.00
20) Perylene-d12	23.20	264	7325m	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.72	152	2344	0.34	ng/ul	0.00
14) Fluoranthene-d10	18.80	212	8173m	0.41	ng/ul	0.00
Target Compounds						
3) Naphthalene	10.17	128	467	0.045	ng/ul#	Ovalue 76

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE082418\
Data File : BE097365.D
Acq On : 24 Aug 2018 12:44
Operator : SJ/JU
Sample : J4422-12
Misc :
ALS Vial : 8 Sample Multiplier: 1




Instrument :
BNA_E
ClientSampleId :
C0AD4

Manual Integrations
APPROVED

Sohil
8/27/2018 12:10:59 PM

Quant Time: Aug 24 23:46:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\SOM-EPA-SIM-BE081718.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Aug 24 22:49:42 2018
Response via : Initial Calibration

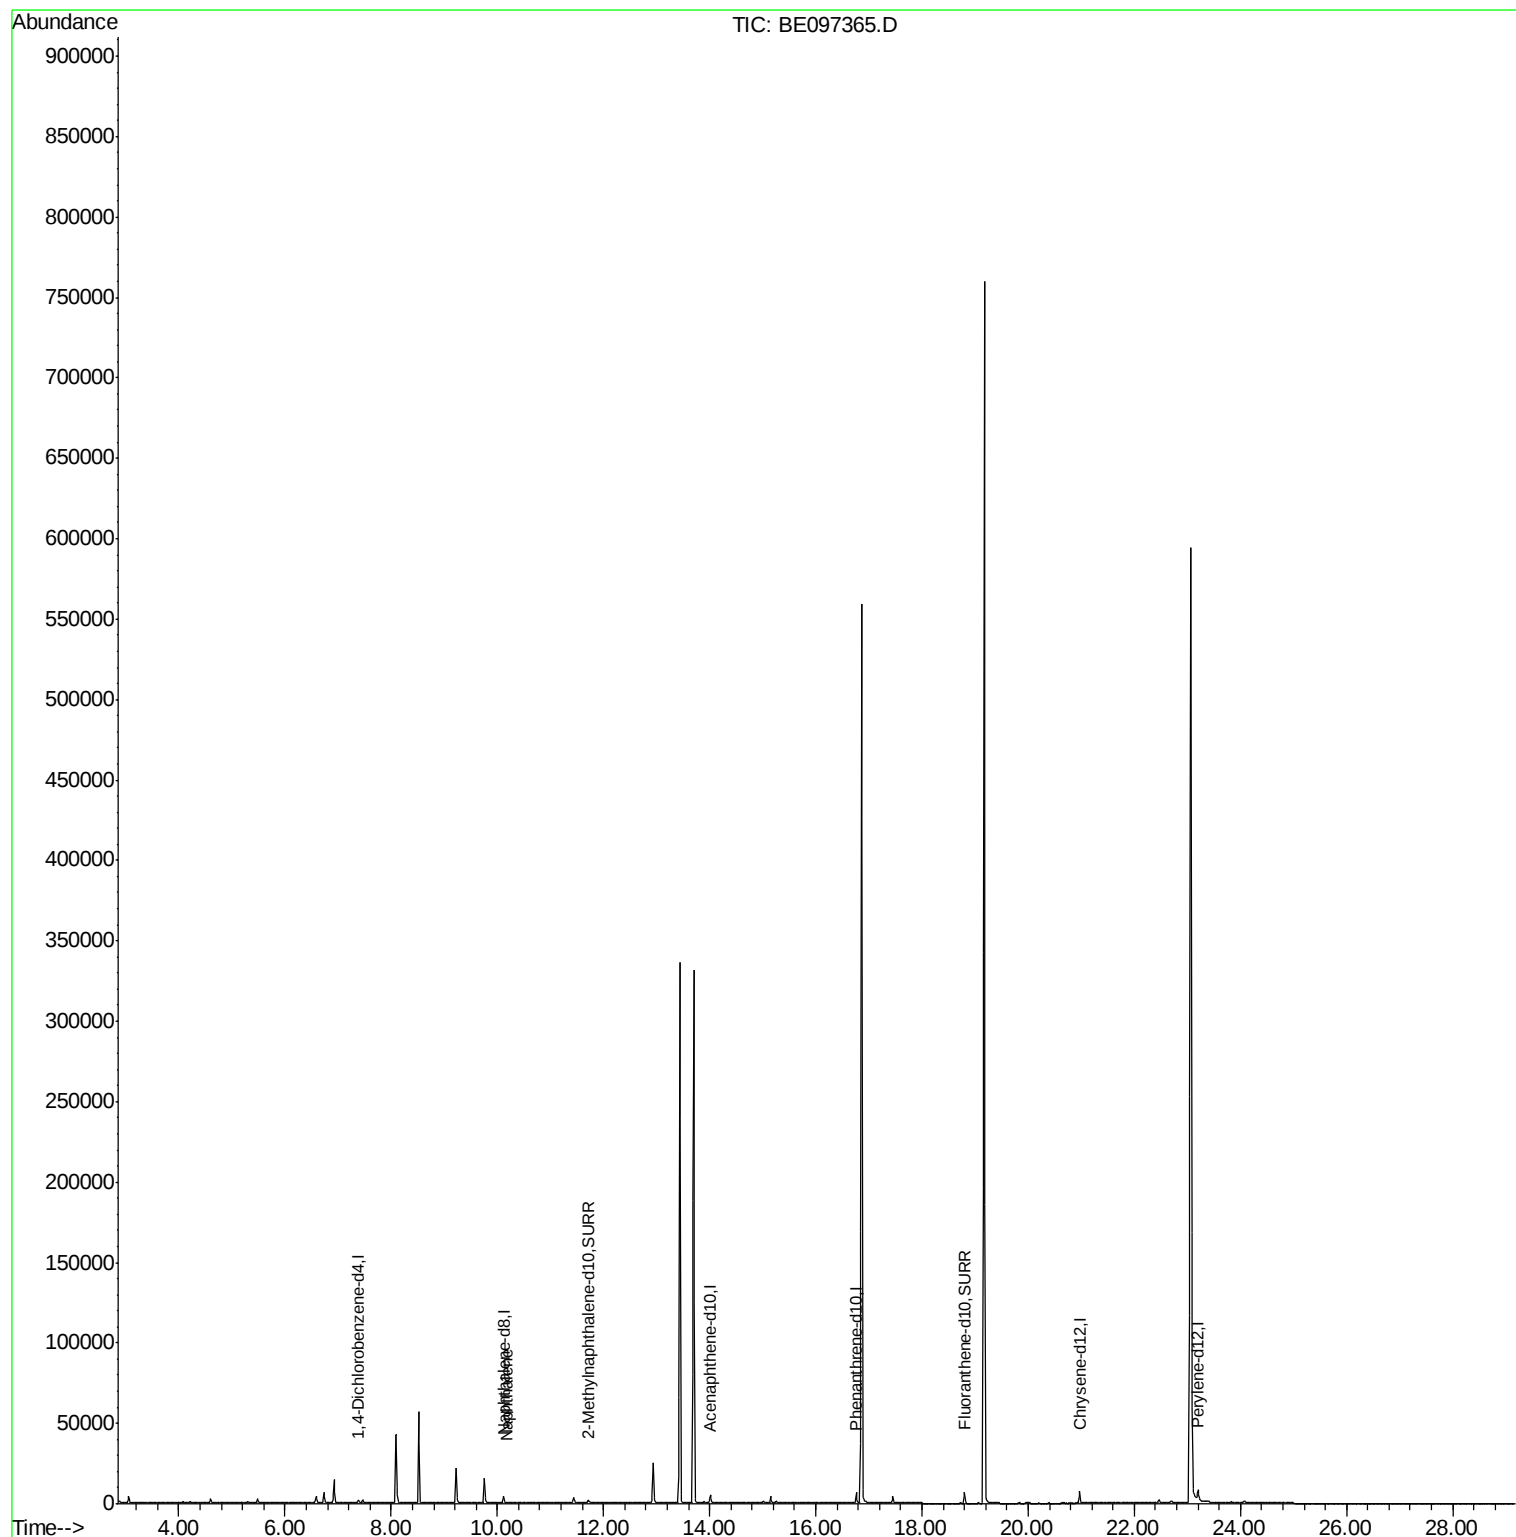

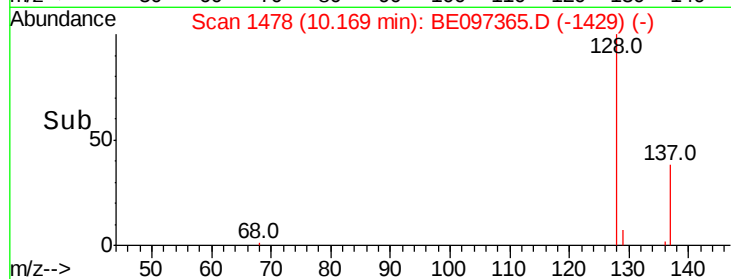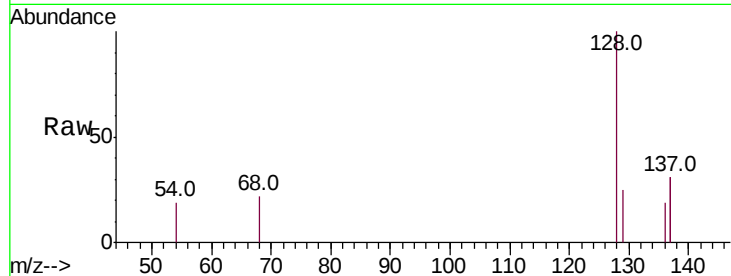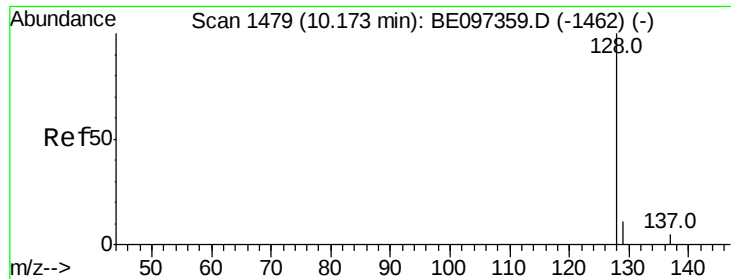

#3

Naphthalene

Concen: 0.045 ng/ul

RT: 10.17 min Scan# 1478

Delta R.T. -0.00 min

Lab File: BE097365.D

Acq: 24 Aug 2018 12:44

Instrument :

BNA_E

ClientSampleId :

C0AD4

Tot Ion:	128	Resp:	467
Ion Ratio	Lower	Upper	
128	100		
129	25.4	11.3	16.9#
127	0.0	4.0	6.0#

Manual Integrations
APPROVED

Sohil
8/27/2018 12:10:59 PM

